



FCC Part 1 Subpart I
FCC Part 2 Subpart J

TEST REPORT

FOR

AMBULATORY ELECTROCARDIOGRAM CHARGING BASE & GATEWAY

MODEL NO: MOME ARC CHARGER, MOME ARC GATEWAY

FCC ID: 2AHLC01858 (Charger), 2AHLC01856 (Gateway)

REPORT NUMBER: R14275554-E10

ISSUE DATE: 2023-11-21

Prepared for
INFOBIONIC, INC
400 TOTTEN POND RD STE 315
WALTHAM, MA 02451, U.S.A.

Prepared by
UL LLC
12 LABORATORY DR.
RESEARCH TRIANGLE PARK, NC 27709 USA
TEL: (919) 549-1400



Revision History

<u>Rev.</u>	<u>Issue Date</u>	<u>Revisions</u>	<u>Revised By</u>
V1	2023-10-03	Initial Issue	Niklas Haydon
V2	2023-10-13	Added E-Field measurements for configuration 4 to §8.3.	Richard Jankovics
V3	2023-11-21	Removed setup photos Added setup photos exhibit reference.	Brian Kiewra

TABLE OF CONTENTS

1. ATTESTATION OF TEST RESULTS	4
2. TEST METHODOLOGY	5
3. FACILITIES AND ACCREDITATION	5
4. DECISION RULES AND MEASUREMENT UNCERTAINTY	6
4.1. METROLOGICAL TRACEABILITY	6
4.2. DECISION RULES.....	6
4.3. MEASUREMENT UNCERTAINTY.....	6
5. EQUIPMENT UNDER TEST	7
5.1. DESCRIPTION OF EUT	7
5.2. DESCRIPTION OF TEST SETUP.....	7
6. TEST AND MEASUREMENT EQUIPMENT	10
7. DUTY CYCLE.....	11
8. MAXIMUM PERMISSIBLE RF EXPOSURE TEST RESULTS.....	14
8.1. FCC LIMITS.....	14
8.2. SUMMARY OF TEST RESULTS	14
8.3. DETAILED TEST RESULTS.....	16
9. SETUP PHOTO	20
END OF REPORT	20

1. ATTESTATION OF TEST RESULTS

COMPANY NAME: InfoBionic, Inc
400 Totten Pond Rd STE 315
Waltham, MA 02451, U.S.A

EUT DESCRIPTION: Ambulatory Electrocardiogram Charging Base & Gateway

MODEL NUMBER: MoMe ARC Charger, MoMe ARC Gateway

SERIAL NUMBER: Charger (MIB2007), Gateway(MIB2008)

DATE TESTED: 2022-11-14 to 2022-11-30, 2023-06-06

APPLICABLE STANDARDS	
STANDARD	TEST RESULTS
FCC PART 1 SUBPART I & PART 2 SUBPART J	Complies

UL LLC tested the above equipment in accordance with the requirements set forth in the above standards. The test results show that the equipment tested is capable of demonstrating compliance with the requirements as documented in this report.

The results documented in this report apply only to the tested sample, under the conditions and modes of operation as described herein. It is the manufacturer's responsibility to assure that additional production units of this model are manufactured with identical electrical and mechanical components. All samples tested were in good operating condition throughout the entire test program. Measurement Uncertainties are published for informational purposes only and were not taken into account unless noted otherwise.


This document may not be altered or revised in any way unless done so by UL LLC and all revisions are duly noted in the revisions section. Any alteration of this document not carried out by UL LLC will constitute fraud and shall nullify the document.

Approved & Released For
UL LLC By:



Francisco de Anda
Staff Engineer
Consumer Technology Division
UL LLC

Prepared By:



Niklas Haydon
Operations Leader
Consumer Technology Division
UL LLC

2. TEST METHODOLOGY

All testing / calculations were made in accordance with FCC KDB 447498 D01, KDB 447498 D03, KDB 680106 D01 v03 and FCC OET Bulletin 65 Edition 97-01.

3. FACILITIES AND ACCREDITATION

UL LLC is accredited by A2LA, Certificate Number 0751.06, for all testing performed within the scope of this report. Testing was performed at the locations noted below.

	Address	ISED CABID	ISED Company Number	FCC Registration
<input type="checkbox"/>	Building 12 Laboratory Dr RTP, NC 27709, U.S.A	US0067	2180C	825374
<input checked="" type="checkbox"/>	Building 2800 Suite Perimeter Park Dr. Suite B Morrisville, NC 27560, U.S.A	US0067	27265	825374

4. DECISION RULES AND MEASUREMENT UNCERTAINTY

4.1. METROLOGICAL TRACEABILITY

The measuring equipment utilized to perform the tests documented in this report has been calibrated in accordance with the manufacturer's recommendations, and is traceable to recognized national standards.

4.2. DECISION RULES

For all tests where the applicable $U_{LAB} \leq U_{MAX}$ the Decision Rule is based on Simple Acceptance in accordance with ISO Guide 98-4: 2012 Clause 8.2, where $U_{MAX} = 30\%$ (0.3) for RF Exposure evaluations. (Measurement uncertainty is not taken into account when stating conformity with a specified requirement.)

For all tests where the applicable $U_{LAB} > U_{MAX}$ the Decision Rule is based on Guarded Acceptance in accordance with ISO Guide 98-4: 2012 Clause 8.3.2, with a guard band equal to $(U_{LAB} - U_{MAX})$, where $U_{MAX} = 30\%$ (0.3) for RF Exposure evaluations. (Test results are adjusted by the value of the guard band to determine conformity with a specified requirement.)

4.3. MEASUREMENT UNCERTAINTY

Where relevant, the following measurement uncertainty levels have been estimated for tests performed on the apparatus:

PARAMETER	U_{Lab}
Magnetic Field using Exposure Level Meter	+/- 0.80 dB
Electric Field using Exposure Level Meter	+/- 0.91 dB
Time	3.39%

Uncertainty figures are valid to a confidence level of 95%, $k = 2$.

5. EQUIPMENT UNDER TEST

5.1. DESCRIPTION OF EUT

The EUT is made up of three devices. The base charges the gateway and the gateway charges the sensor. The operating frequencies for the sources and loads are as follows:

- Base is a source at 110kHz-200kHz
- Gateway is a load at 110kHz-200kHz
- Gateway is a source at 1MHz
- Sensor is a load at 1MHz

5.2. DESCRIPTION OF TEST SETUP

SUPPORT EQUIPMENT

Support Equipment List				
Description	Manufacturer	Model	Serial Number	FCC ID
AC Adapter	HDP	HDP12-MD05024U	N/A	N/A
Terminated Lead Set	Infobionic	N/A	N/A	N/A
Sensor	Infobionic	MoMe ARC Sensor	IB1033	2AHL01857

I/O CABLES

I/O Cable List						
Cable No.	Port	# of Identical Ports	Connector Type	Cable Type	Cable Length (m)	Remarks
1	USB	1	USB	Shielded	<3m	Power Cable
2	N/A	3	Leads	Shielded	<3m	Lead Cables

TEST SETUP

The following two configurations are tested:

Configuration	Mode	Descriptions
1	Standby Note: < 10% Power Detecting	Charger alone powered by AC/DC adapter in desktop configuration
2	Operating (Charger) Note: Measurements were made when the battery level of the load was at a state of <10%, 50%, >90% and 100%. Standby (Gateway) Note: < 10% Power Detecting	Charger powered by AC/DC adapter charging Gateway in desktop configuration
3	Operating Note: Measurements were made when the battery level of the load was at a state of <10%, 50%, >90% and 100%.	Charger powered by AC/DC adapter charging Gateway power by battery charging Sensor in desktop configuration
4	Operating Note: Measurements were made when the battery level of the load was at worst-case found in Config 3 (>90%).	Gateway powered by battery charging Sensor in portable configuration

MEASUREMENT SETUP

For desktop configuration, the measurement was taken using a probe placed 15cm surrounding the device and 20cm above the top surface of the EUT.

For portable configuration, the measurement was taken using a probe placed 0cm surrounding the device including front and back of the EUT.


Measurements were taken from the top and all sides of the EUT per KDB 680106 D01 v03.

For Portable configuration, measurements were made from the back surface with the worst-case battery charge state from configuration 3 (>90%). Measurement sensor could not be placed at 0 cm separation distance for all axis. Pursuant to FCC guidance in the TCBC Workshop April 2022 WPT Updates presentation, measurements were made as close to device as possible (probe radius = 4.6 cm), and out at 2 cm steps from device. The field is determined through numerical calculation based on the distance from the transmitting coil, which is 1.2 cm within the device. The calculated field is then validated to be within 30% of the measured values for the two closed points measured. Once validated, the numerical calculation can be used to report the field at the actual use.

Please note: the Gateway's belt clip provide 1.3 cm of separation distance to the surface of the Gateway. Testing was performed with the clip removed to allow probe placement as close as possible to the surface of the Gateway. The total distance between the transmitting coil and the user would be 1.2 cm (coil to surface) + 1.3 (surface to user) = 2.5 cm. This value is used in the numerical calculation of the field strength.

Note: Duty cycle for portable use is reduced to 50%. Testing was performed at 100% and corrected down.

CONFIGURATIONS 1-3

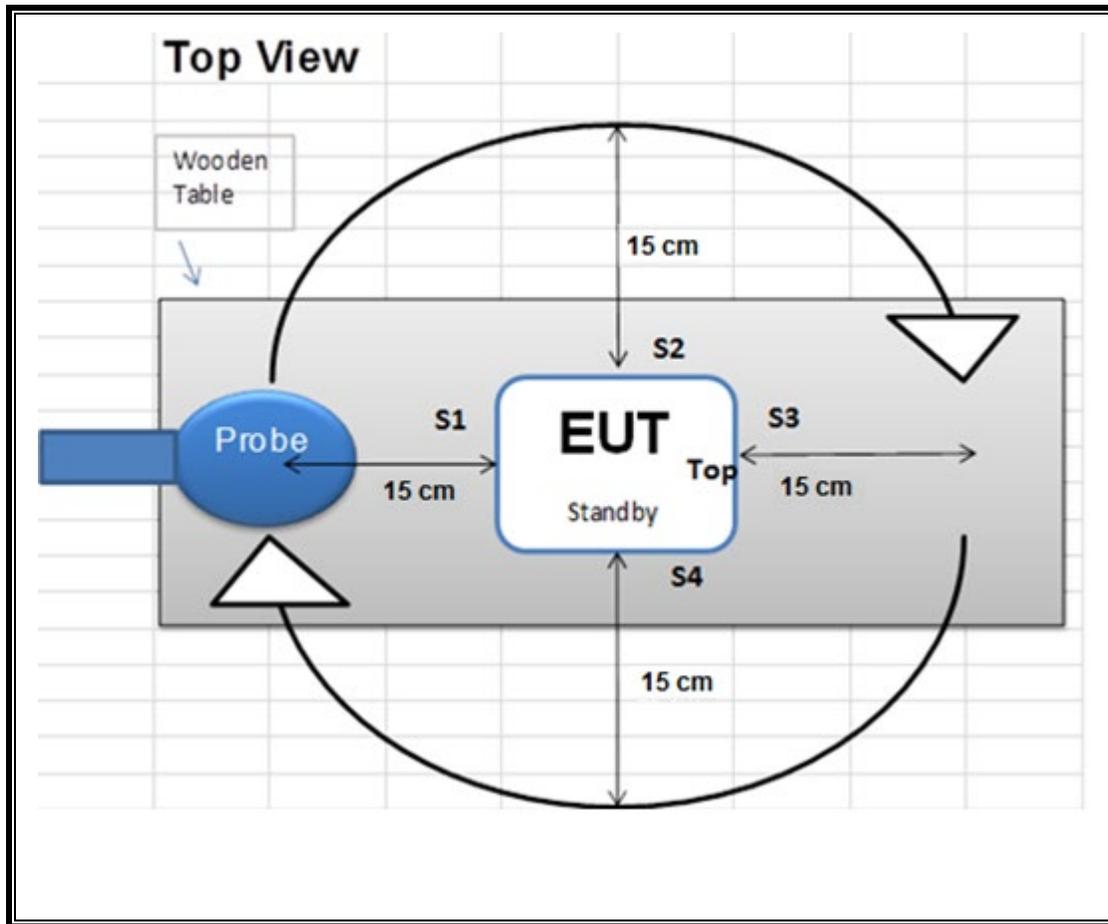

6. TEST AND MEASUREMENT EQUIPMENT

The following test and measurement equipment were used for the tests documented in this report:

Test Equipment List					
Description	Manufacturer	Model	Equip. ID	Cal Date	Cal Due
Exposure Level Meter	Narda	EHP-200AC	170WX80318	2022-07-20	2023-07-20
Exposure Level Meter	Narda	EHP-200AC	170WX80318	2023-07-31	2024-07-31
Spectrum Analyzer	Agilent	N9030A	MY54410168	2022-05-02	2023-05-02

Note: Test equipment was only used within calibration dates.

7. DUTY CYCLE

LIMITS

None; for reporting purposes only.

PROCEDURE



Zero-Span Spectrum Analyzer Method.



ON TIME AND DUTY CYCLE RESULTS

Mode	ON Time B (msec)	Period (msec)	Duty Cycle x (linear)	Duty Cycle (%)
Charger Standby (Config 1)	171.00	903.00	0.1894	18.94%
Charger Operating (Config 2 & 3)	100.00	100.00	1.00	100.00%
Gateway Standby (Config 2)	44.00	620.00	0.0710	7.10%
Gateway Operating (Config 3 & 4)	100.00	100.00	1.00	100.00%

Note: Duty cycle for charger standby is worst

Note: Duty cycle for portable use is reduced to 50%. Measurements taken at 100%.

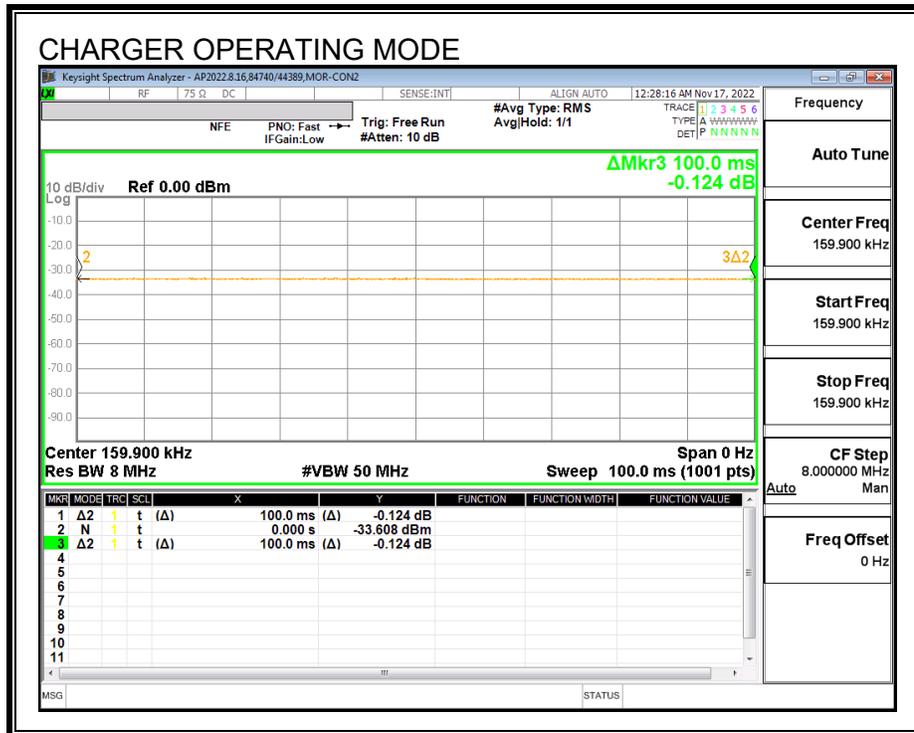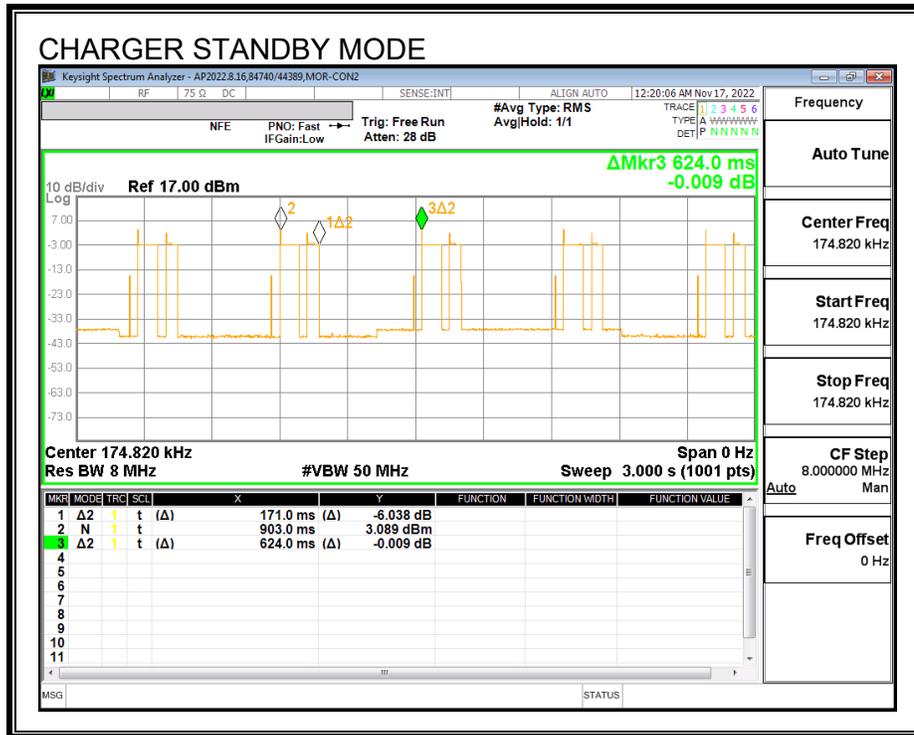

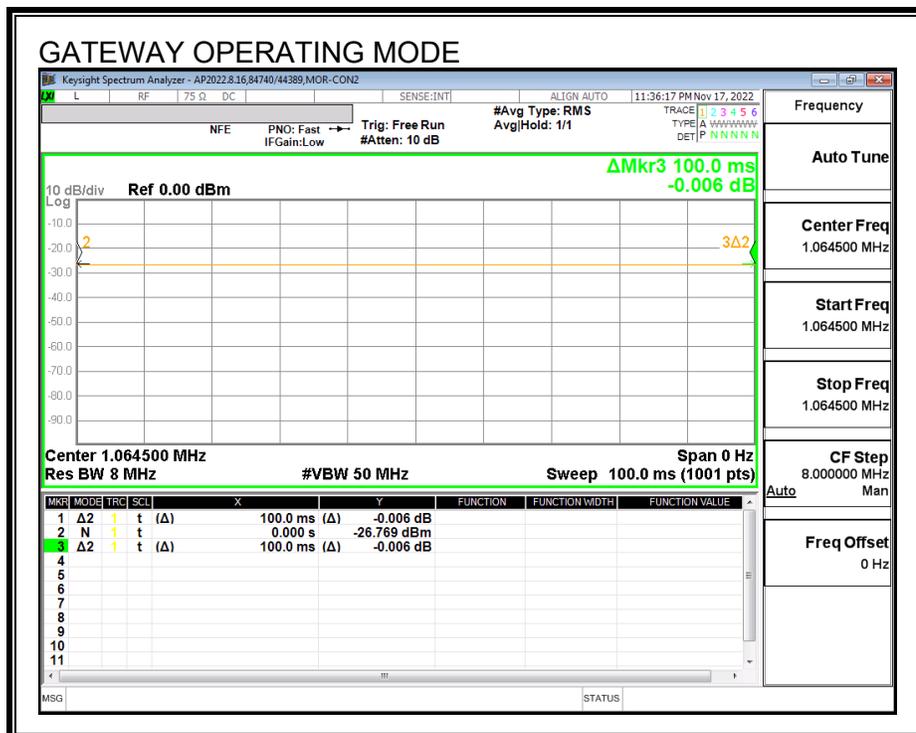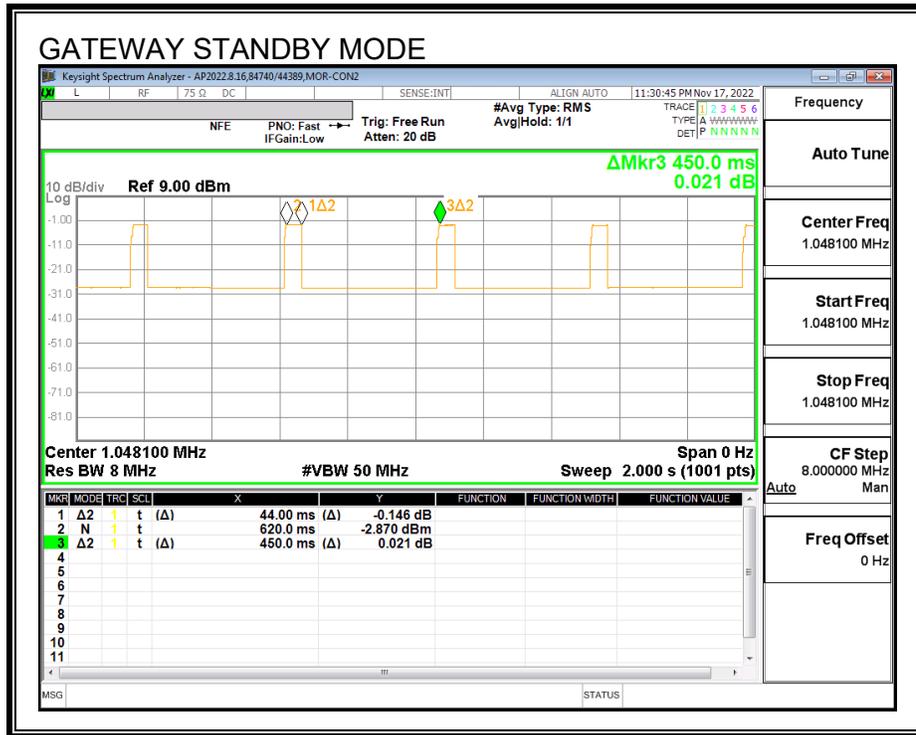

8. MAXIMUM PERMISSIBLE RF EXPOSURE TEST RESULTS

8.1. FCC LIMITS

Per KDB 680106 D01 v03r01, 3. a) (2) Evaluation of RF Exposure test data for determining compliance of wireless power transfer (WPT) systems (both portable and not) operating at frequencies below 100 kHz is provided on a case-by-case basis. In these situations, a WPT system will not require additional RF exposure testing when supporting data from measurements and/or numerical simulations show that, for all the positions of space relevant for the body exposure, the external (unperturbed) temporal peak field strengths do not exceed the following reference levels:

- 83 V/m for the electric field
- and
- 90 A/m for the magnetic field.

8.2. SUMMARY OF TEST RESULTS

This report contains data provided by the customer which can impact the validity of results. UL LLC is only responsible for the validity of results after the integration of the data provided by the customer.

RESULTS

ID:	84740/21193	Date:	2022-11-14 to 2022-11-30, 2023-06-06
------------	-------------	--------------	---

Note:

Both magnetic and electric field strengths have been investigated from 9 kHz to 30 MHz.

For desktop configuration, the measurement was taken using a probe placed 15cm surrounding the device and 20cm above the top surface of the EUT.

For portable configuration, the measurement was taken using a probe placed 0cm from the back of the EUT, moving out in 2 cm steps.

The inductive wireless power transfer device meets all of the following requirements:

- Power transfer frequency is less than 1 MHz
- Output power from each primary coil is less than or equal to 15 watts.
- The transfer system includes only single primary and secondary coils. This includes charging systems that may have multiple primary coils and clients that are able to detect and allow coupling only between individual pairs of coils.
- Client device is placed directly in contact with the transmitter.
- Mobile exposure conditions only (portable exposure conditions are not covered by this exclusion).
- The aggregate H-field strengths at 15 cm surrounding the device and 20 cm above the top surface from all simultaneous transmitting coils are demonstrated to be less than 50% of the MPE limit.

FCC RF Exposure Summary of Results

Desktop Application

Electric Field			Magnetic Field		
FCC Limit (V/m)	Maximum Average Reading (V/m)	Percentage (%)	FCC Limit (A/m)	Maximum Average Reading (A/m)	Percentage (%)
83	2.032	2.45%	90	0.489	0.54%

Portable Application

At 2.5 cm from the coil, the field is calculated at 2.23 A/m. Given a 50% duty cycle, the time-averaged field would be **1.115 A/m**. The limit is 1.63 A/m, there the EUT is found to meet the RF Exposure guidelines.

8.3. DETAILED TEST RESULTS

E- FIELD AND H- FIELD MEASUREMENTS

Note: Peak measurements were performed. RMS values were calculated from the peak measurement. Please refer to the formula for calculating the RMS values: [Field Strength x √Duty Cycle].

Config	Test Mode	Meas Dist (cm)	E field Limit	Electric Field Reading				Magnetic Field Limit	Magnetic Field Reading			
			(V/m)	(V/m)				(A/m)	(A/m)			
			FCC	Location	Value	Duty Cycle %	FCC Average	FCC	Location	Value		
1	Standby	15 cm from edges and 20 cm from top surface	83	1	0.760	18.2	0.324	90	1	0.031	18.2	0.013
				2	0.785		0.335		2	0.031		0.013
				3	0.822		0.351		3	0.031		0.013
				4	0.732		0.312		4	0.022		0.009
				Top	0.395		0.169		Top	0.055		0.023
				Max	0.822		0.351		Max	0.055		0.023

Config	Test Mode	Meas Dist (cm)	E field Limit	Electric Field Reading				Magnetic Field Limit	Magnetic Field Reading				
			(V/m)	(V/m)				(A/m)	(A/m)				
			FCC	Location	Value	Duty Cycle %	FCC Average	FCC	Location	Value			Duty Cycle %
2	Operating Power ~0% Charging	15 cm from edges and 20 cm from top surface	83	1	0.782	100.0	0.782	90	1	0.028	100.0	0.028	
				2	0.794		0.794		2	0.020		0.020	
				3	0.944		0.944		3	0.050		0.050	
				4	0.674		0.674		4	0.022		0.022	
				Top	0.783		0.783		Top	0.023		0.023	
				Max	0.944		0.944		Max	0.050		0.050	
	Operating Power 50% Charging			1	0.815	100.0	0.815		100.0	1	0.025	100.0	0.025
				2	0.819		0.819			2	0.023		0.023
				3	0.921		0.921			3	0.047		0.047
				4	0.743		0.743			4	0.019		0.019
				Top	0.711		0.711			Top	0.022		0.022
				Max	0.921		0.921			Max	0.047		0.047
	Operating Power >90% Charging			S1	0.720	100.0	0.720		100.0	S1	0.022	100.0	0.022
				S2	0.835		0.835			S2	0.020		0.020
				S3	0.842		0.842			S3	0.046		0.046
				S4	0.631		0.631			S4	0.021		0.021
				Top	0.700		0.700			Top	0.447		0.447
				Max	0.842		0.842			Max	0.447		0.447
	Operating Power 100% Charged			S1	0.626	100.0	0.626		100.0	S1	0.019	100.0	0.019
				S2	0.761		0.761			S2	0.023		0.023
S3		0.997	0.997	S3	0.045		0.045						
S4		0.609	0.609	S4	0.021		0.021						
Top		0.587	0.587	Top	0.020		0.020						
Max		0.997	0.997	Max	0.045		0.045						


Note for Configuration 2: Span of the meter was set to capture both charging sources

Config	Test Mode	Meas Dist (cm)	E field Limit	Electric Field Reading				Magnetic Field Limit	Magnetic Field Reading				
			(V/m)	(V/m)				(A/m)	(A/m)				
			FCC	Location	Value	Duty Cycle %	FCC Average	FCC	Location	Value	Duty Cycle %	FCC Average	
3	Operating Power ~0% Charging	15 cm from edges and 20 cm from top surface	83	1	1.192	100.0	1.192	90	1	0.024	100.0	0.024	
				2	1.225		1.225		2	0.024		0.024	
				3	1.724		1.724		3	0.054		0.054	
				4	2.032		2.032		4	0.022		0.022	
				Top	0.920		0.920		Top	0.023		0.023	
				Max	2.032		2.032		Max	0.054		0.054	
	Operating Power 50% Charging			1	1.976	100.0	1.976		90	1	0.026	100.0	0.026
				2	1.013		1.013			2	0.019		0.019
				3	1.132		1.132			3	0.045		0.045
				4	1.093		1.093			4	0.018		0.018
				Top	0.904		0.904			Top	0.022		0.022
				Max	1.976		1.976			Max	0.045		0.045
	Operating Power >90% Charging	S1	1.303	100.0	1.303	90	S1	0.023		100.0	0.023		
		S2	1.161		1.161		S2	0.022			0.022		
		S3	1.113		1.113		S3	0.050			0.050		
		S4	0.791		0.791		S4	0.019			0.019		
		Top	0.835		0.835		Top	0.489			0.489		
		Max	1.303		1.303		Max	0.489			0.489		
	Operating Power 100 % Charged	S1	1.303	100.0	1.303		90	S1	0.023	100.0	0.023		
		S2	1.055		1.055			S2	0.020		0.020		
S3		1.320	1.320		S3			0.045	0.045				
S4		0.825	0.825		S4			0.017	0.017				
Top		0.829	0.829		Top			0.022	0.022				
Max		1.320	1.320		Max			0.045	0.045				

Note: for Configuration 3: Span of the meter was set to capture both charging sources

Configuration 4 – Portable use RF exposure
 H-Field Data

Probe coil distance from EUT surface (cm)	EUT Tx coil distance to EUT surface (cm)	Total Field Distance (cm)	Estimated Field		Measured	Limit (A/m)	Deviation
			Tesla	Calculated Field (A/m)	Measured Field (A/m)		
0	1.2	1.2	1.18E-05	9.36		1.63	
0.6	1.2	1.8	5.81E-06	4.63		1.63	
1.3	1.2	2.5	2.80E-06	2.23		1.63	
2.6	1.2	3.8	9.56E-07	0.76		1.63	
4.6	1.2	5.8	2.93E-07	0.23	0.21	1.63	-8%
6.6	1.2	7.8	1.24E-07	0.10	0.10	1.63	3%
8.6	1.2	9.8	6.34E-08	0.05	0.07	1.63	
10.6	1.2	11.8	3.66E-08	0.03	0.06	1.63	
12.6	1.2	13.8	2.30E-08	0.02	0.05	1.63	
14.6	1.2	15.8	1.54E-08	0.01	0.04	1.63	
16.6	1.2	17.8	1.08E-08	0.01	0.04	1.63	
18.6	1.2	19.8	7.83E-09	0.01	0.03	1.63	
20.6	1.2	21.8	5.88E-09	0.00	0.03	1.63	

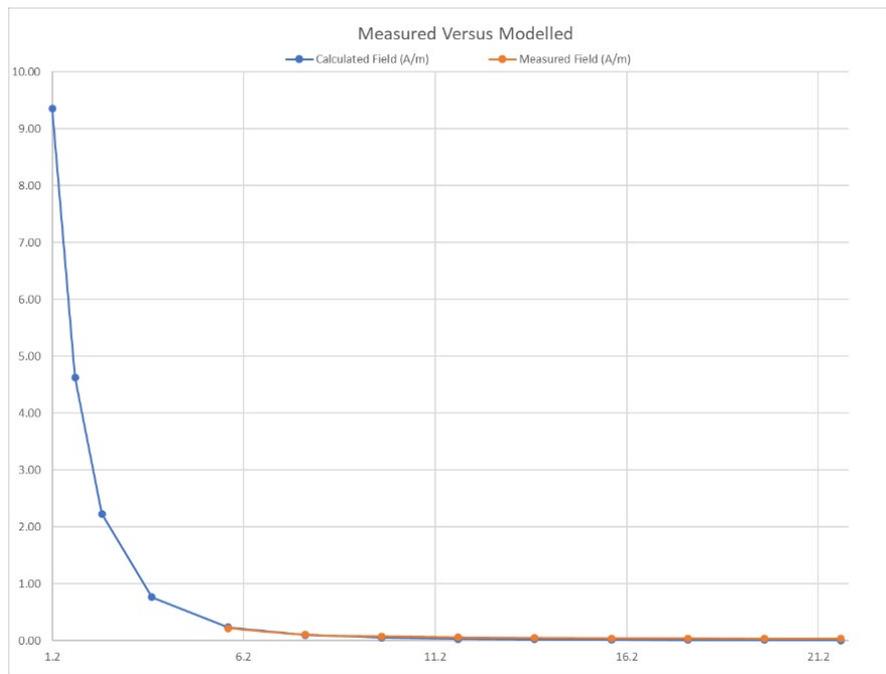

Calculated field based on the following (source: [Magnetic Field of a Current Loop \(gsu.edu\)](https://www.gsu.edu/~physics/faculty/whalen/pages/11%20Magnetic%20Field%20of%20a%20Current%20Loop.pdf))

$$B_z = \frac{\mu_0}{4\pi} \frac{2\pi R^2 I}{(z^2 + R^2)^{3/2}} \quad \mu_0 = 4\pi \times 10^{-7} T \cdot m / A$$

I = Current in amperes
 R = radius of loop in meters
 z = distance in meters along centerline of loop

E-Field Data

Config	Test Mode	Meas Dist (cm)	E field Limit (V/m)	Electric Field Reading			
				(V/m)			
				FCC	Location	Value	Duty Cycle %
4	Operating Power ~ 0% Charging	0cm	614	1	20.812	100.0	20.812
				2	21.488		21.488
				3	16.342		16.342
				4	28.539		28.539
				Back	23.505		23.505
				Front	31.433		31.433
				Max	31.433		31.433
	Operating Power 50% Charging			1	22.942	100.0	22.942
				2	21.494		21.494
				3	15.891		15.891
				4	26.079		26.079
				Back	34.495		34.495
				Front	30.132		30.132
				Max	34.495		34.495
	Operating Power >90% Charging			S1	18.033	100.0	18.033
				S2	22.938		22.938
				S3	13.519		13.519
				S4	22.818		22.818
				Back	28.125		28.125
				Front	27.012		27.012
Max		28.125	28.125				
Operating Power 100 % Charged	S1	19.015	100.0	19.015			
	S2	25.352		25.352			
	S3	16.005		16.005			
	S4	24.120		24.120			
	Back	24.100		24.100			
	Front	29.007		29.007			
	Max	29.007		29.007			

9. SETUP PHOTO

Refer to R1427554-EP6 for setup photos.

END OF REPORT