

APPENDIX B EUT TEST POSITION PHOTOS

Liquid depth $\geq 15\text{cm}$


Phantom: SAM (30deg probe tilt) with CRP v5.0_20150321; Type: QD000P40CD; Serial: TP:1874




Vertical-Front Setup Photo (5mm)

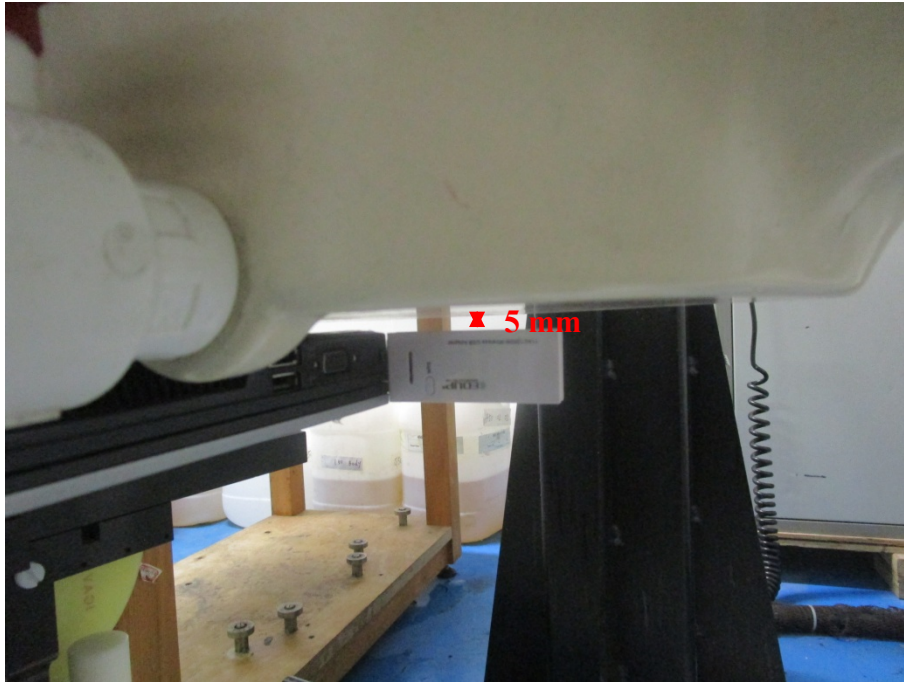

Horizontal-Down Setup Photo (5mm)

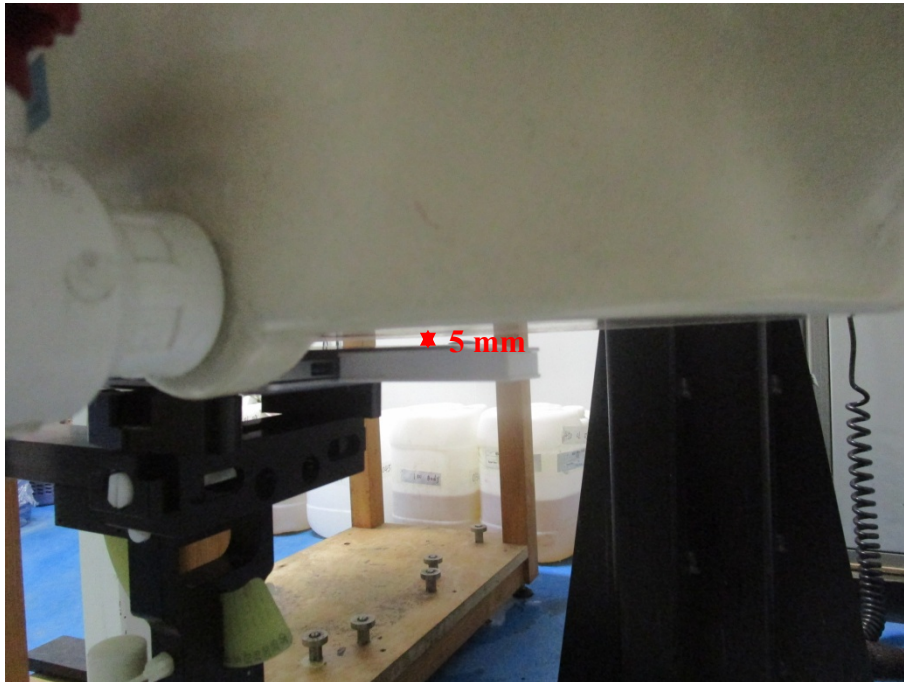

Body Top Setup Photo (5mm)

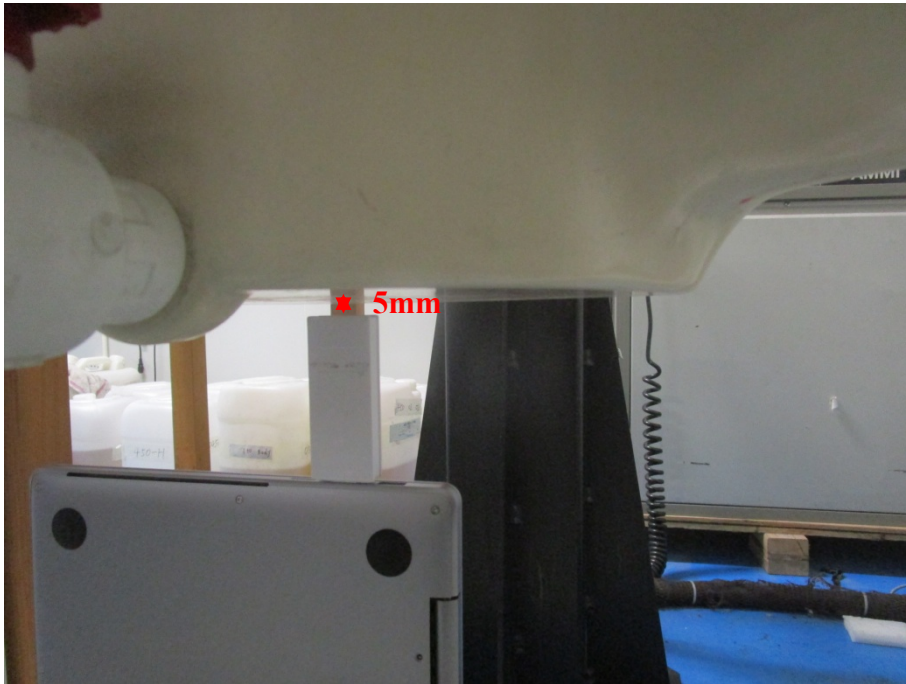

Horizontal-Up(Adding USB extension cable) Setup Photo (5mm)



Vertical-Back (Adding USB extension cable) Setup Photo (5mm)

