


The Tenuto 2 device has a silicon outer sheath which is fitted onto the inner skeleton and glued in position. This sheath cannot be marked and it is not possible to add a label on the outside due to the use case which involves the product being used with body parts.

It will be inappropriate and unsafe to add any engraving or markings on the outside of the unit itself as these would collect dirt and impact the ability to clean the device for use which would make the unit unhygienic.

The FCC ID is on the OCB and also on the packaging and visible at the time of purchase.

The attached KDB was submitted for a previous application and supports this approach.

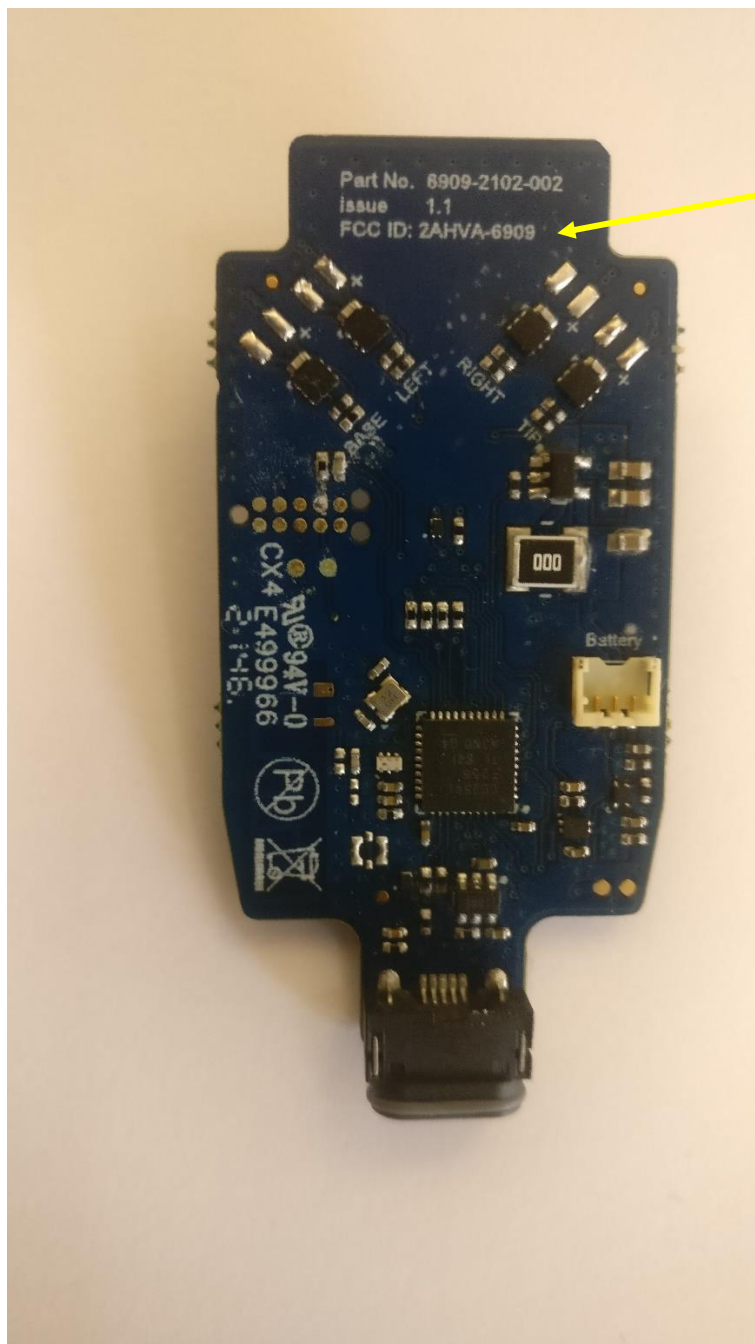

FCC ID on PCB

The FCC ID is also on the packaging and visible at the time of purchase

