


Impedance Plot for SN 46/11 DIP 2G450-189; 2450Head

Calibrated impedance: $49.8\Omega + 3.3j\Omega$; Measurement impedance: $51.9\Omega - 4.5j\Omega$ (within 5Ω)



Calibrated return loss: -29.54dB; Measurement return loss: -29.55dB(within 20%)

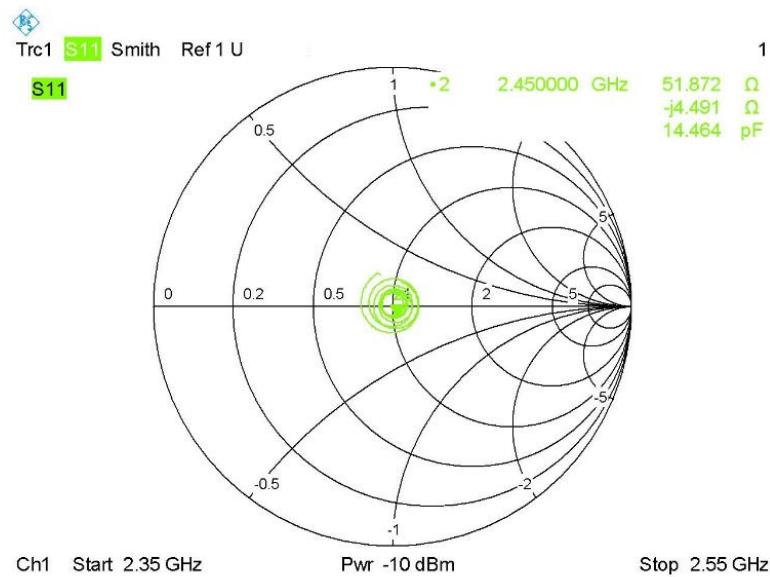