

System Check_Head_750MHz

DUT: D750V3 - SN1107


Communication System: CW; Frequency: 750.0 MHz; Duty Cycle: 1:1
Medium: HSL_750_230203 Medium parameters used: $f=750.0$ MHz; $\sigma=0.898$ S/m; $\epsilon_r=42.0$
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(10.51, 10.51, 10.51); Calibrated: 2022-10-31
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2022-12-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 0.457 W/kg; SAR (10g) = 0.307 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.03 dB
SAR (1g) = 0.427 W/kg; SAR (8g) = 0.296 W/kg; SAR (10g) = 0.281 W/kg

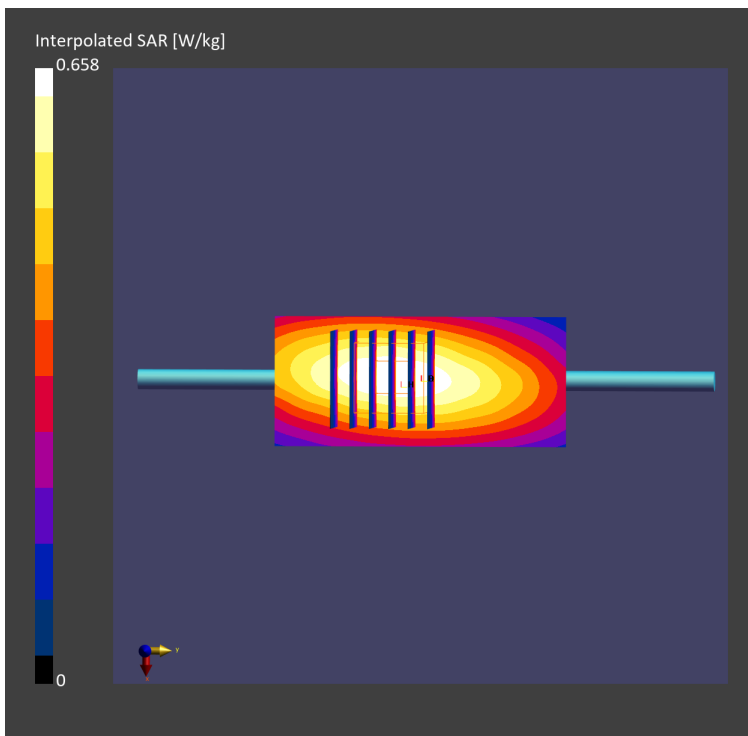

System Check_Head_850MHz


DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.0 MHz; Duty Cycle: 1:1
Medium: HSL_850_230203 Medium parameters used: $f= 835.0$ MHz; $\sigma= 0.933$ S/m; $\epsilon_r = 41.7$
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

- DASY6 Configuration:
- Probe: EX3DV4 - SN3931; ConvF(9.85, 9.85, 9.85); Calibrated: 2022-10-31
 - Sensor-Surface: 1.4 mm
 - Electronics: DAE4 Sn1707; Calibrated: 2022-12-15
 - Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
 - Measurement Software: 16.2.2.1588
 - UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 0.571 W/kg; SAR (10g) = 0.378 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.02 dB
SAR (1g) = 0.533 W/kg; SAR (8g) = 0.367 W/kg; SAR (10g) = 0.347 W/kg

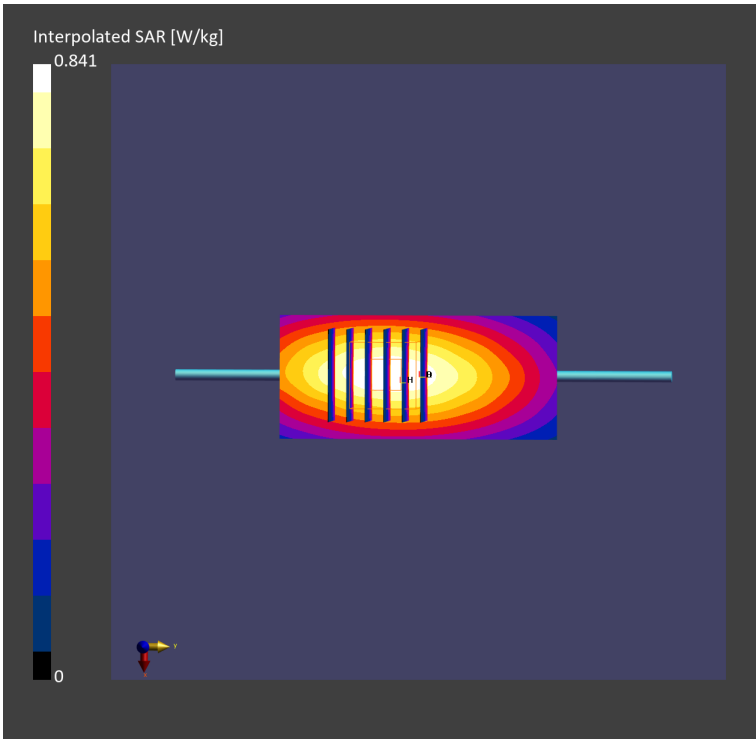

System Check_Head_1750MHz


DUT: D1750V2-1112

Communication System: CW; Frequency: 1750.0 MHz; Duty Cycle: 1:1
Medium: HSL_1750_230202 Medium parameters used: $f=1750.0$ MHz; $\sigma=1.36$ S/m; $\epsilon_r=41.0$
Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

- DASY6 Configuration:
- Probe: EX3DV4 - SN3931; ConvF(8.66, 8.66, 8.66); Calibrated: 2022-10-31
 - Sensor-Surface: 1.4 mm
 - Electronics: DAE4 Sn1707; Calibrated: 2022-12-15
 - Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
 - Measurement Software: 16.2.2.1588
 - UID: CW

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.67 W/kg; SAR (10g) = 0.915 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 1.73 W/kg; SAR (8g) = 1.00 W/kg; SAR (10g) = 0.924 W/kg

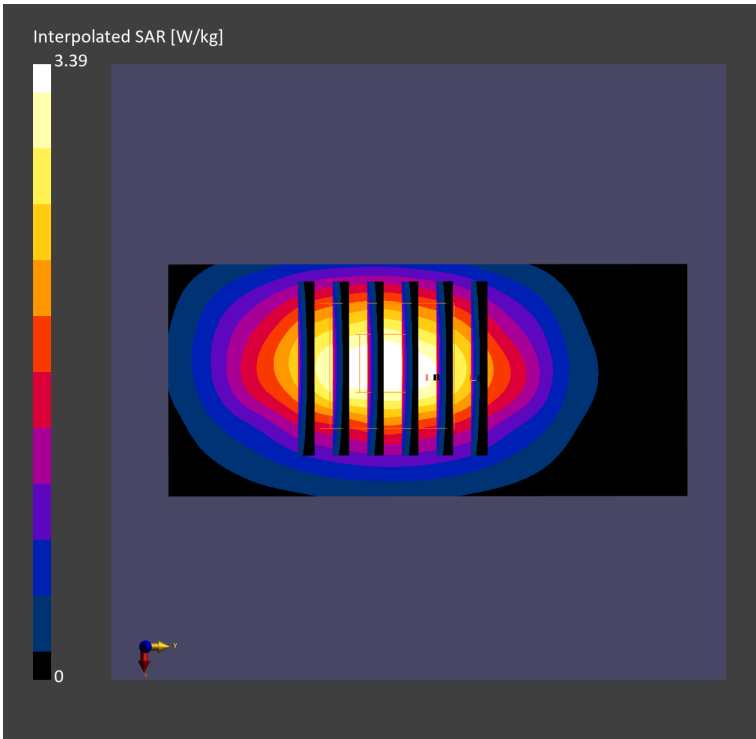

System Check_Head_1900MHz

DUT: D1900V2-5d185


Communication System: CW; Frequency: 1900.0 MHz; Duty Cycle: 1:1
Medium: HSL_1900_230202 Medium parameters used: $f=1900.0$ MHz; $\sigma=1.44$ S/m; $\epsilon_r=39.4$
Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(8.36, 8.36, 8.36); Calibrated: 2022-10-31
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2022-12-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.86 W/kg; SAR (10g) = 0.990 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 1.92 W/kg; SAR (8g) = 1.09 W/kg; SAR (10g) = 0.999 W/kg

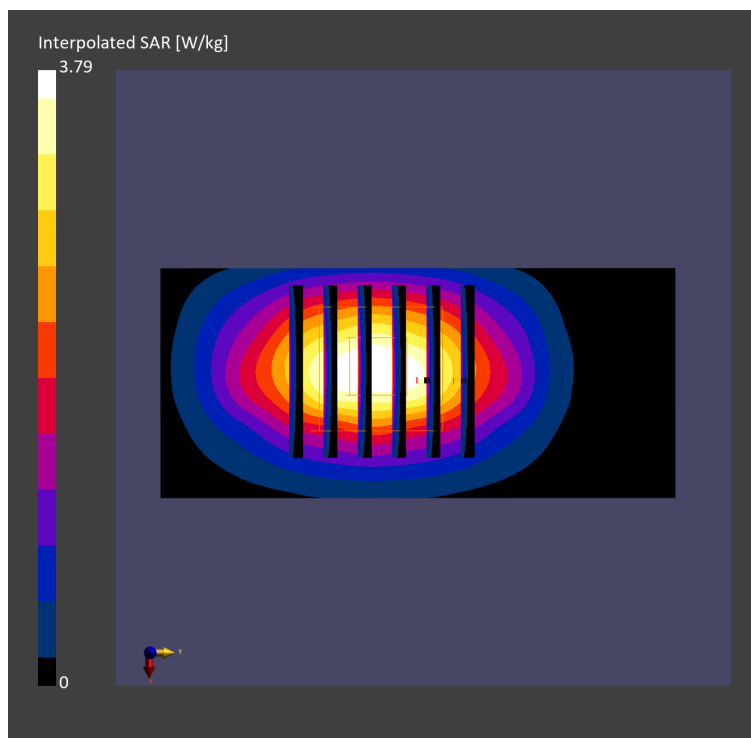

System Check_Head_2300MHz


DUT: D2300V2-1006

Communication System: CW; Frequency: 2300.0 MHz; Duty Cycle: 1:1
Medium: HSL_2300_230202 Medium parameters used: $f=2300.0$ MHz; $\sigma=1.66$ S/m; $\epsilon_r=39.0$
Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

- DASY6 Configuration:
- Probe: EX3DV4 - SN3931; ConvF(7.93, 7.93, 7.93); Calibrated: 2022-10-31
 - Sensor-Surface: 1.4 mm
 - Electronics: DAE4 Sn1707; Calibrated: 2022-12-15
 - Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
 - Measurement Software: 16.2.2.1588
 - UID: CW

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.32 W/kg; SAR (10g) = 1.13 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 2.40 W/kg; SAR (8g) = 1.26 W/kg; SAR (10g) = 1.14 W/kg

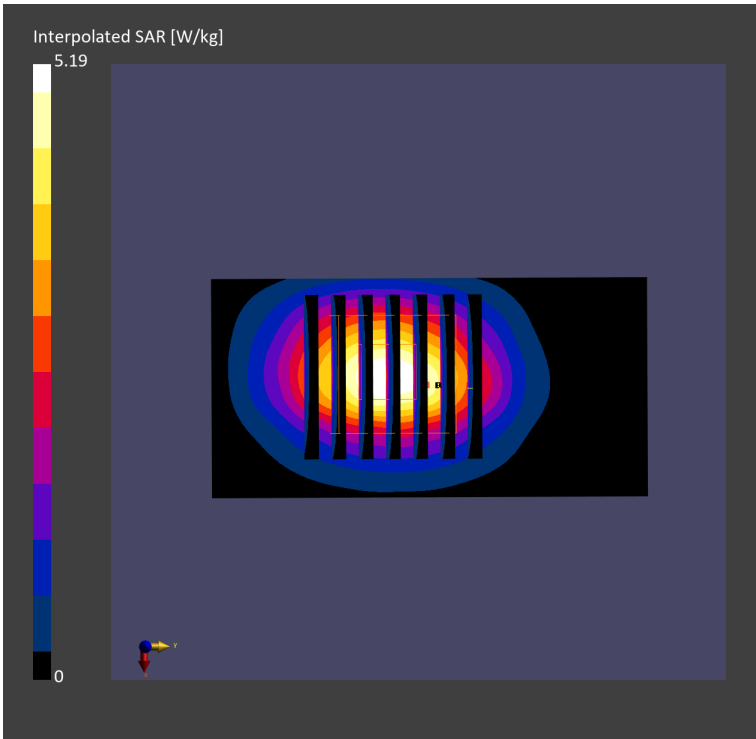

System Check_Head_2600MHz

DUT: D2600V2-1078


Communication System: CW; Frequency: 2600.0 MHz; Duty Cycle: 1:1
Medium: HSL_2600_230202 Medium parameters used: $f=2600.0$ MHz; $\sigma=1.99$ S/m; $\epsilon_r=37.8$
Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(7.4, 7.4, 7.4); Calibrated: 2022-10-31
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2022-12-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.78 W/kg; SAR (10g) = 1.28 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 2.90 W/kg; SAR (8g) = 1.44 W/kg; SAR (10g) = 1.30 W/kg

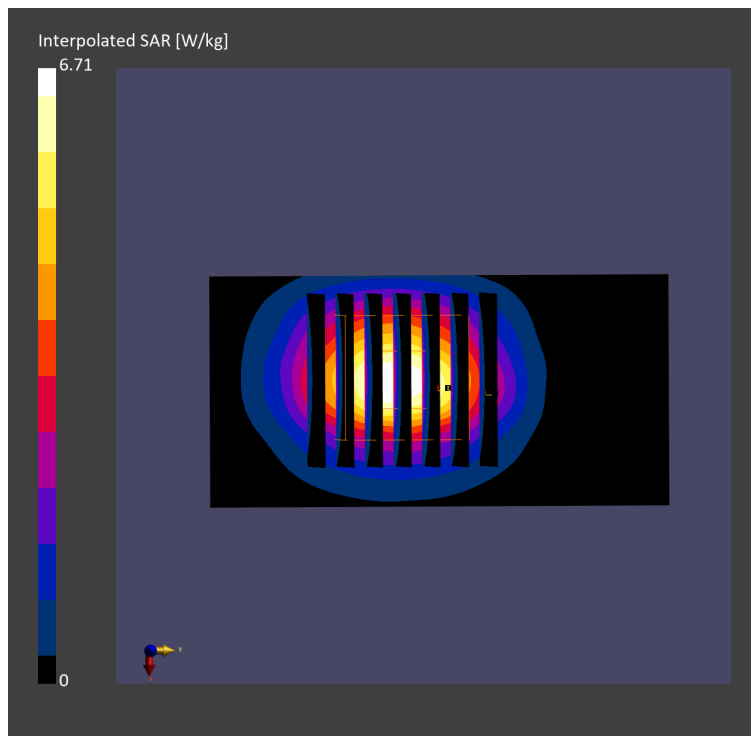

System Check_Head_3500MHz


DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.0 MHz; Duty Cycle: 1:1
Medium: HSL_3500_230203 Medium parameters used: $f=3500.0$ MHz; $\sigma=3.00$ S/m; $\epsilon_r=38.2$
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

- DASY6 Configuration:
- Probe: EX3DV4 - SN3931; ConvF(7.19, 7.19, 7.19); Calibrated: 2022-10-31
 - Sensor-Surface: 1.4 mm
 - Electronics: DAE4 Sn1707; Calibrated: 2022-12-15
 - Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
 - Measurement Software: 16.2.2.1588
 - UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.34 W/kg; SAR (10g) = 1.30 W/kg;

Pin=50mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.12 dB
SAR (1g) = 3.28 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.27 W/kg

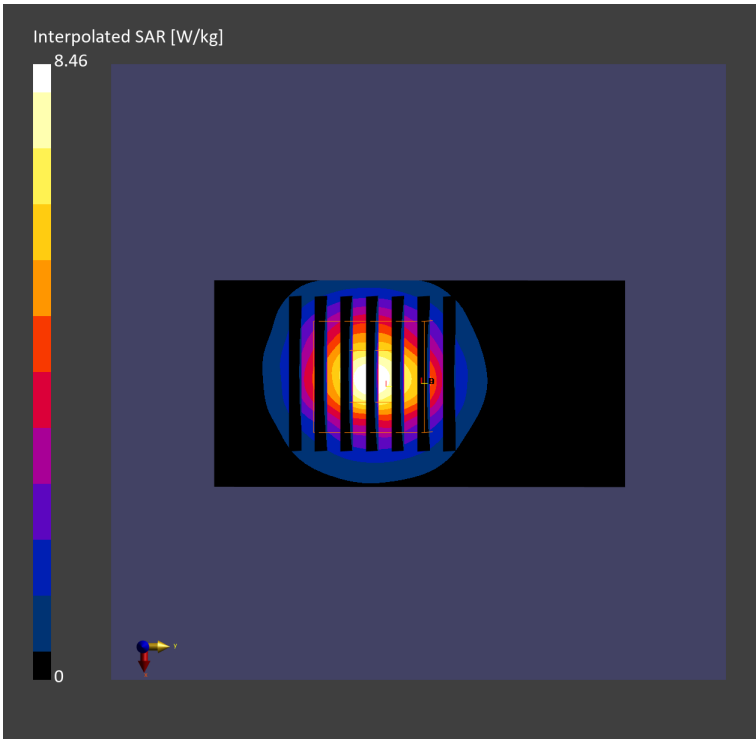

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.0 MHz; Duty Cycle: 1:1
Medium: HSL_3700_230203 Medium parameters used: $f=3700.0$ MHz; $\sigma=3.16$ S/m; $\epsilon_r=37.9$
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(7.06, 7.06, 7.06); Calibrated: 2022-10-31
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2022-12-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.31 W/kg; SAR (10g) = 1.24 W/kg;

Pin=50mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.09 dB
SAR (1g) = 3.11 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.16 W/kg

