
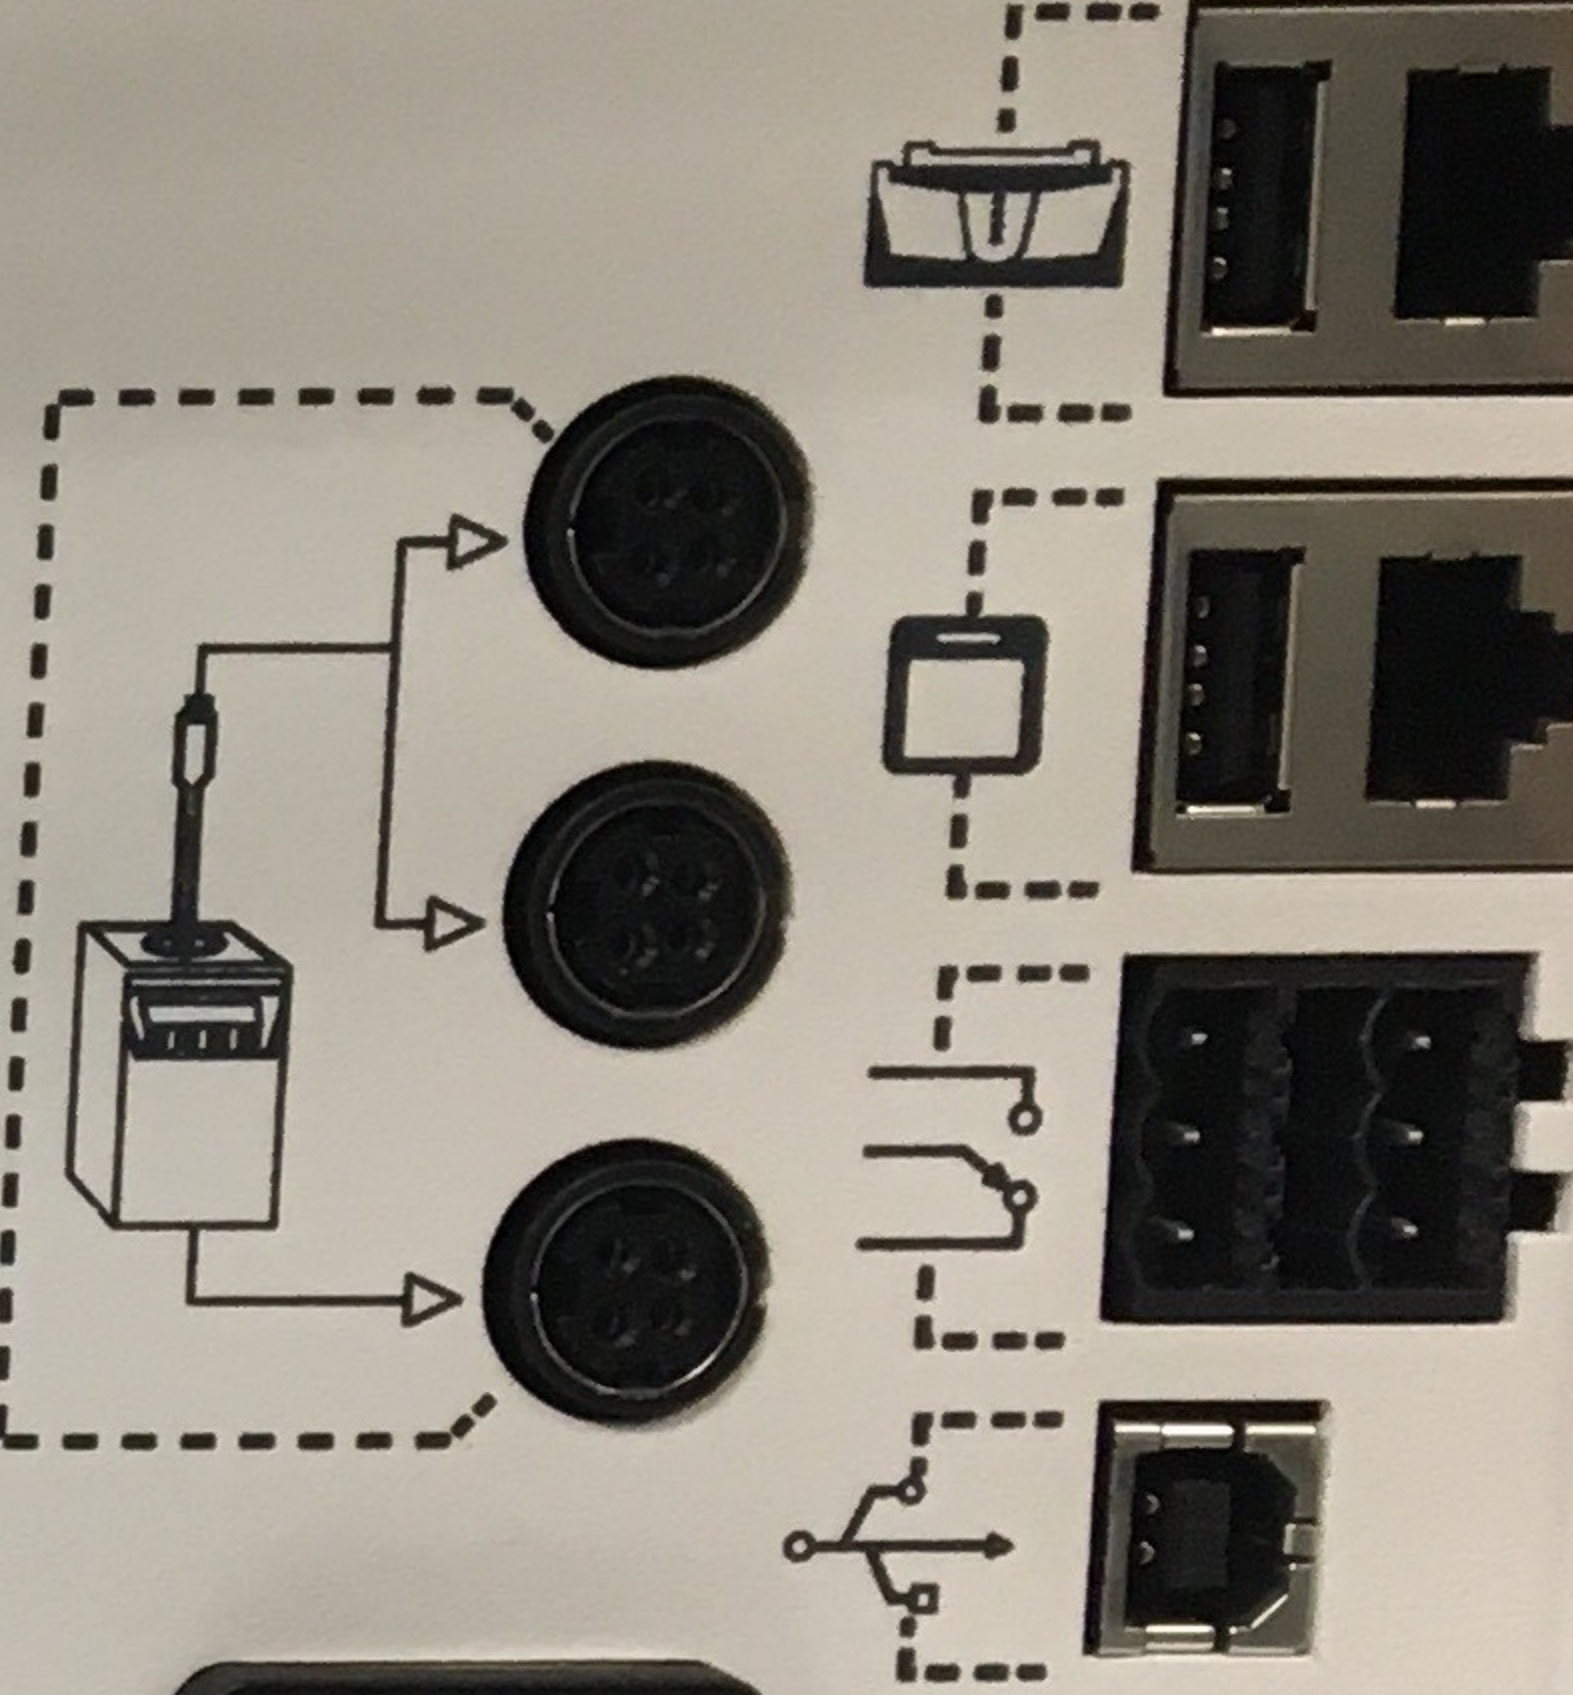
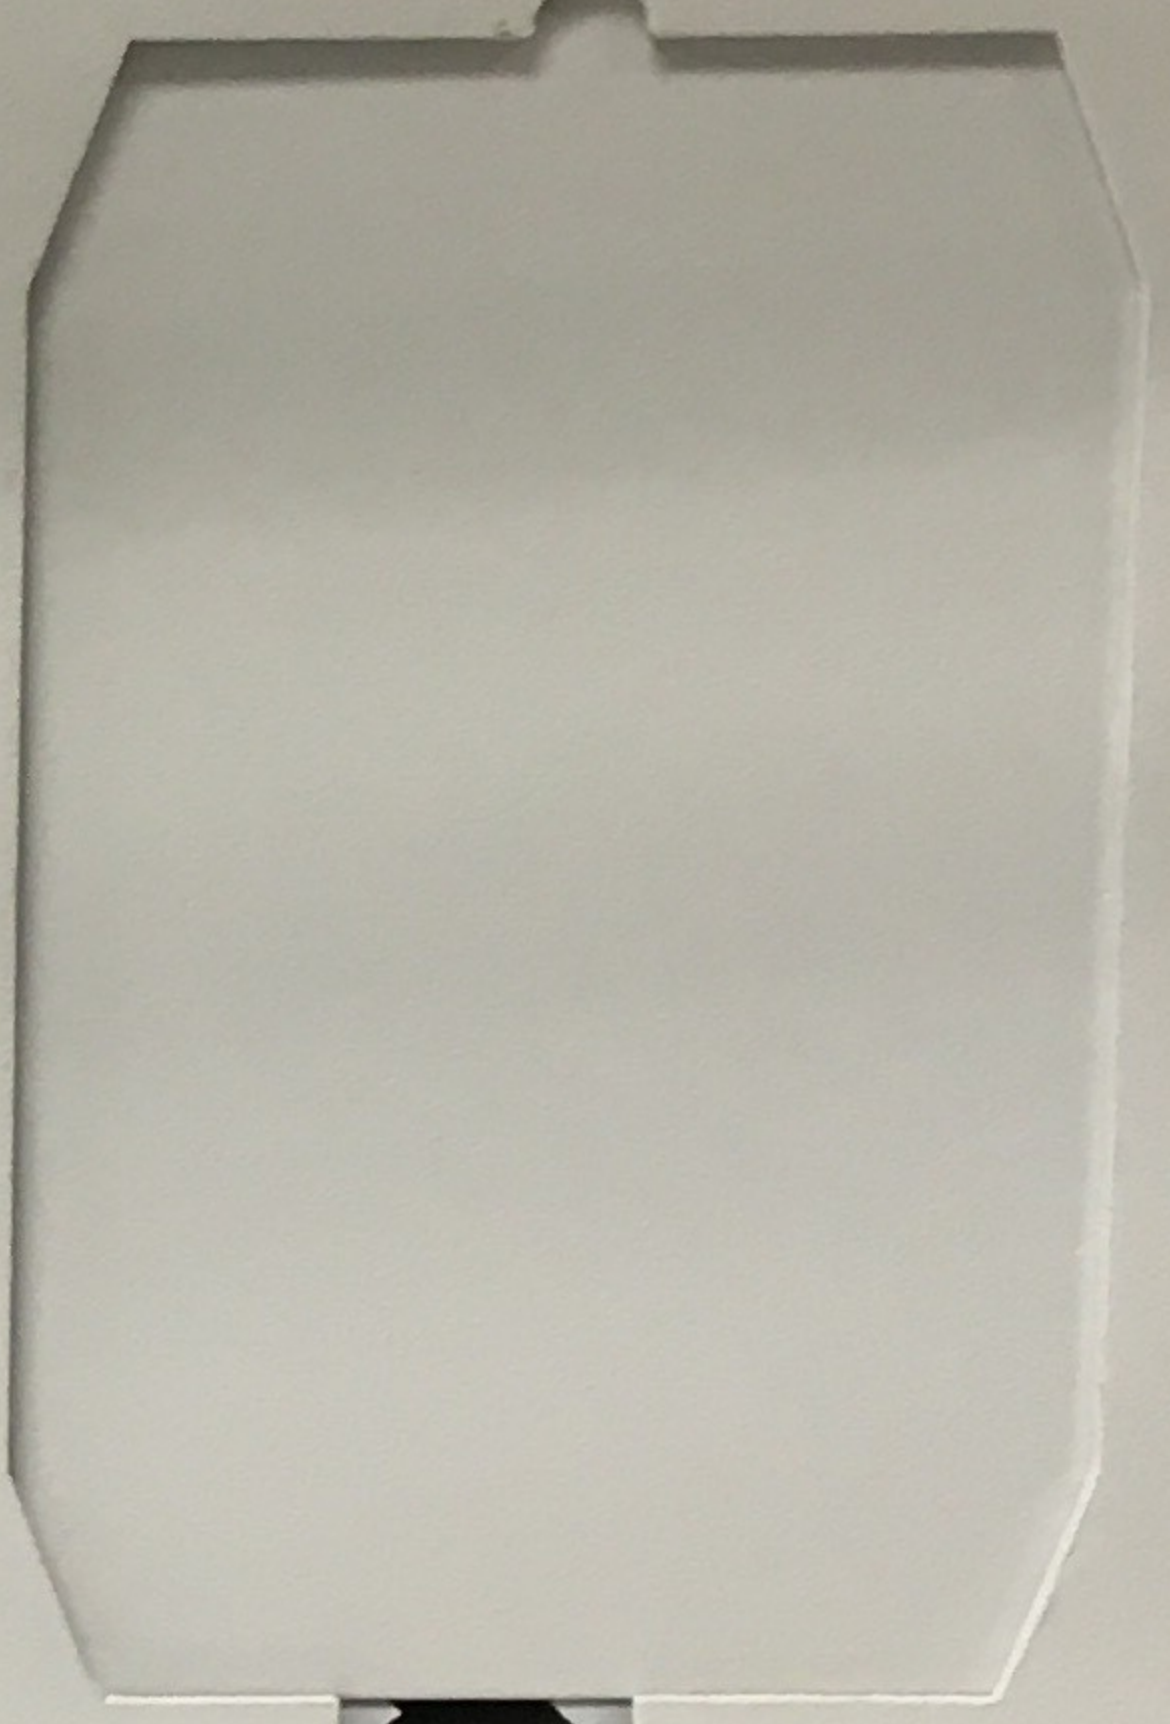
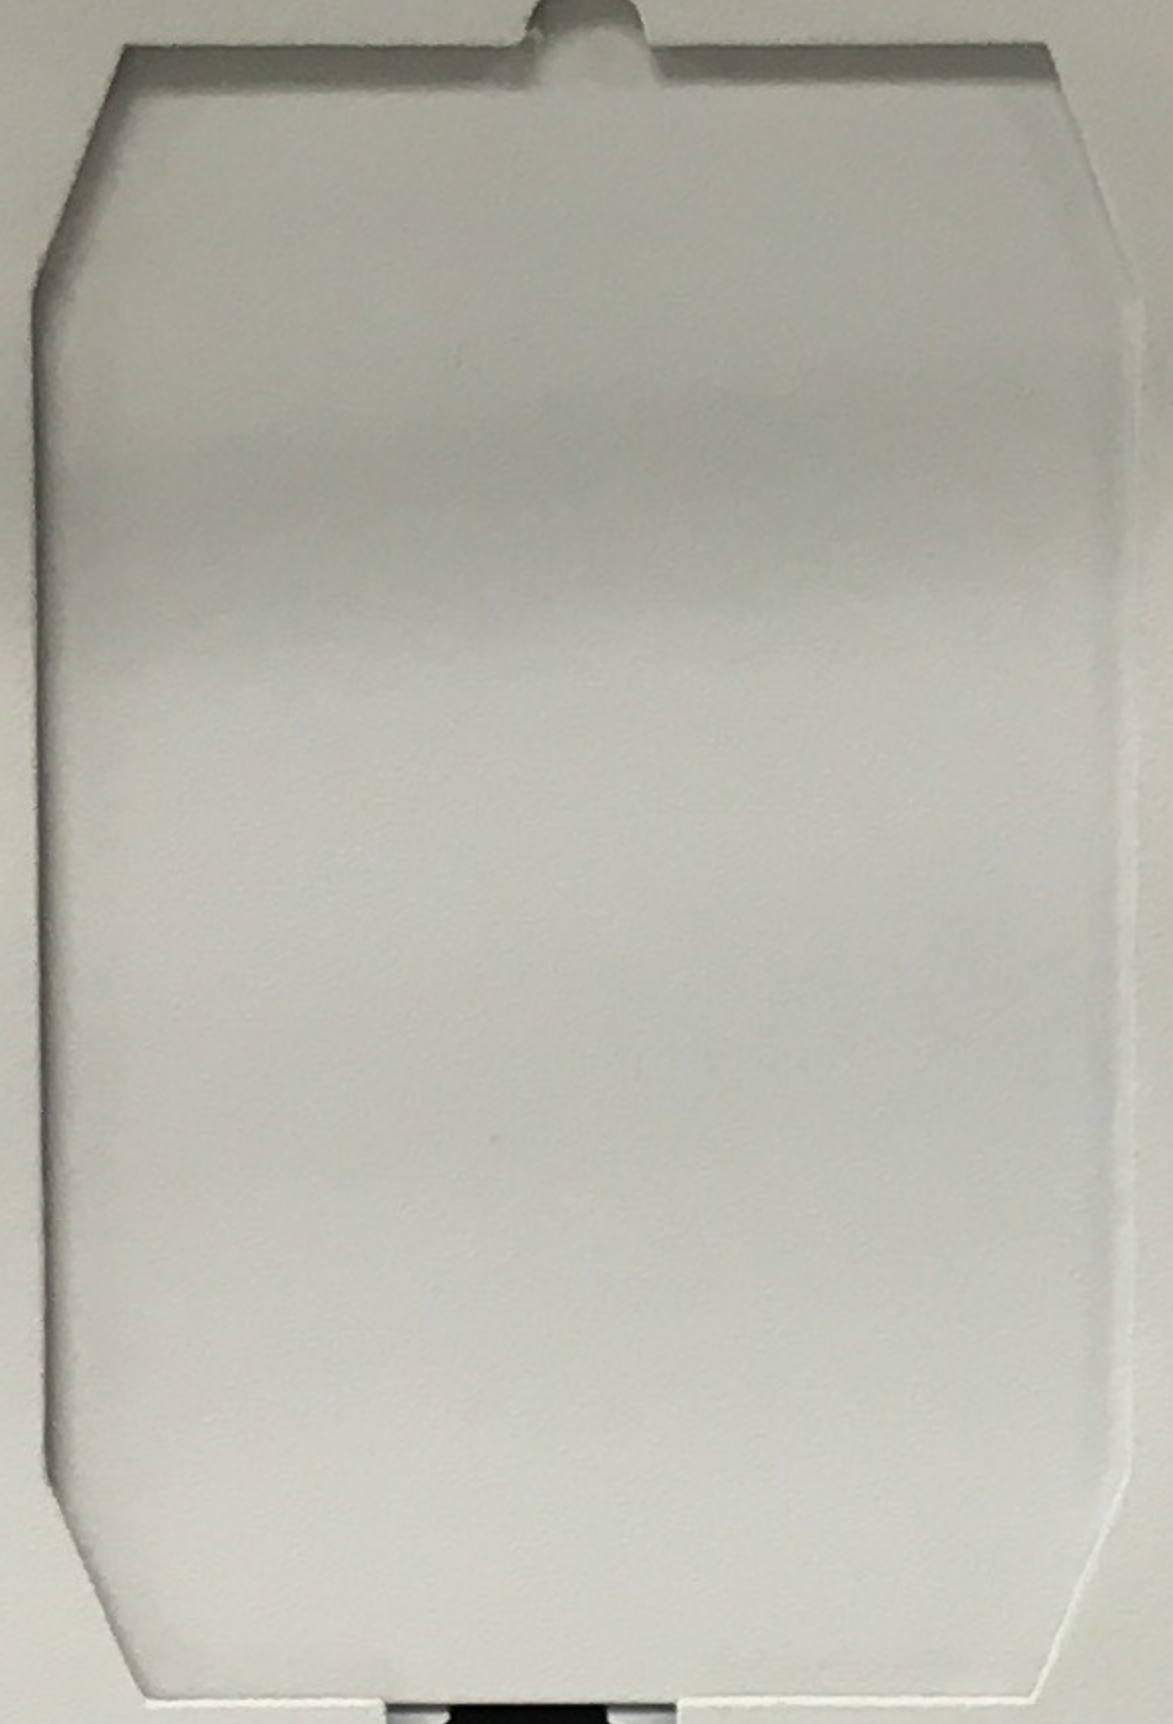
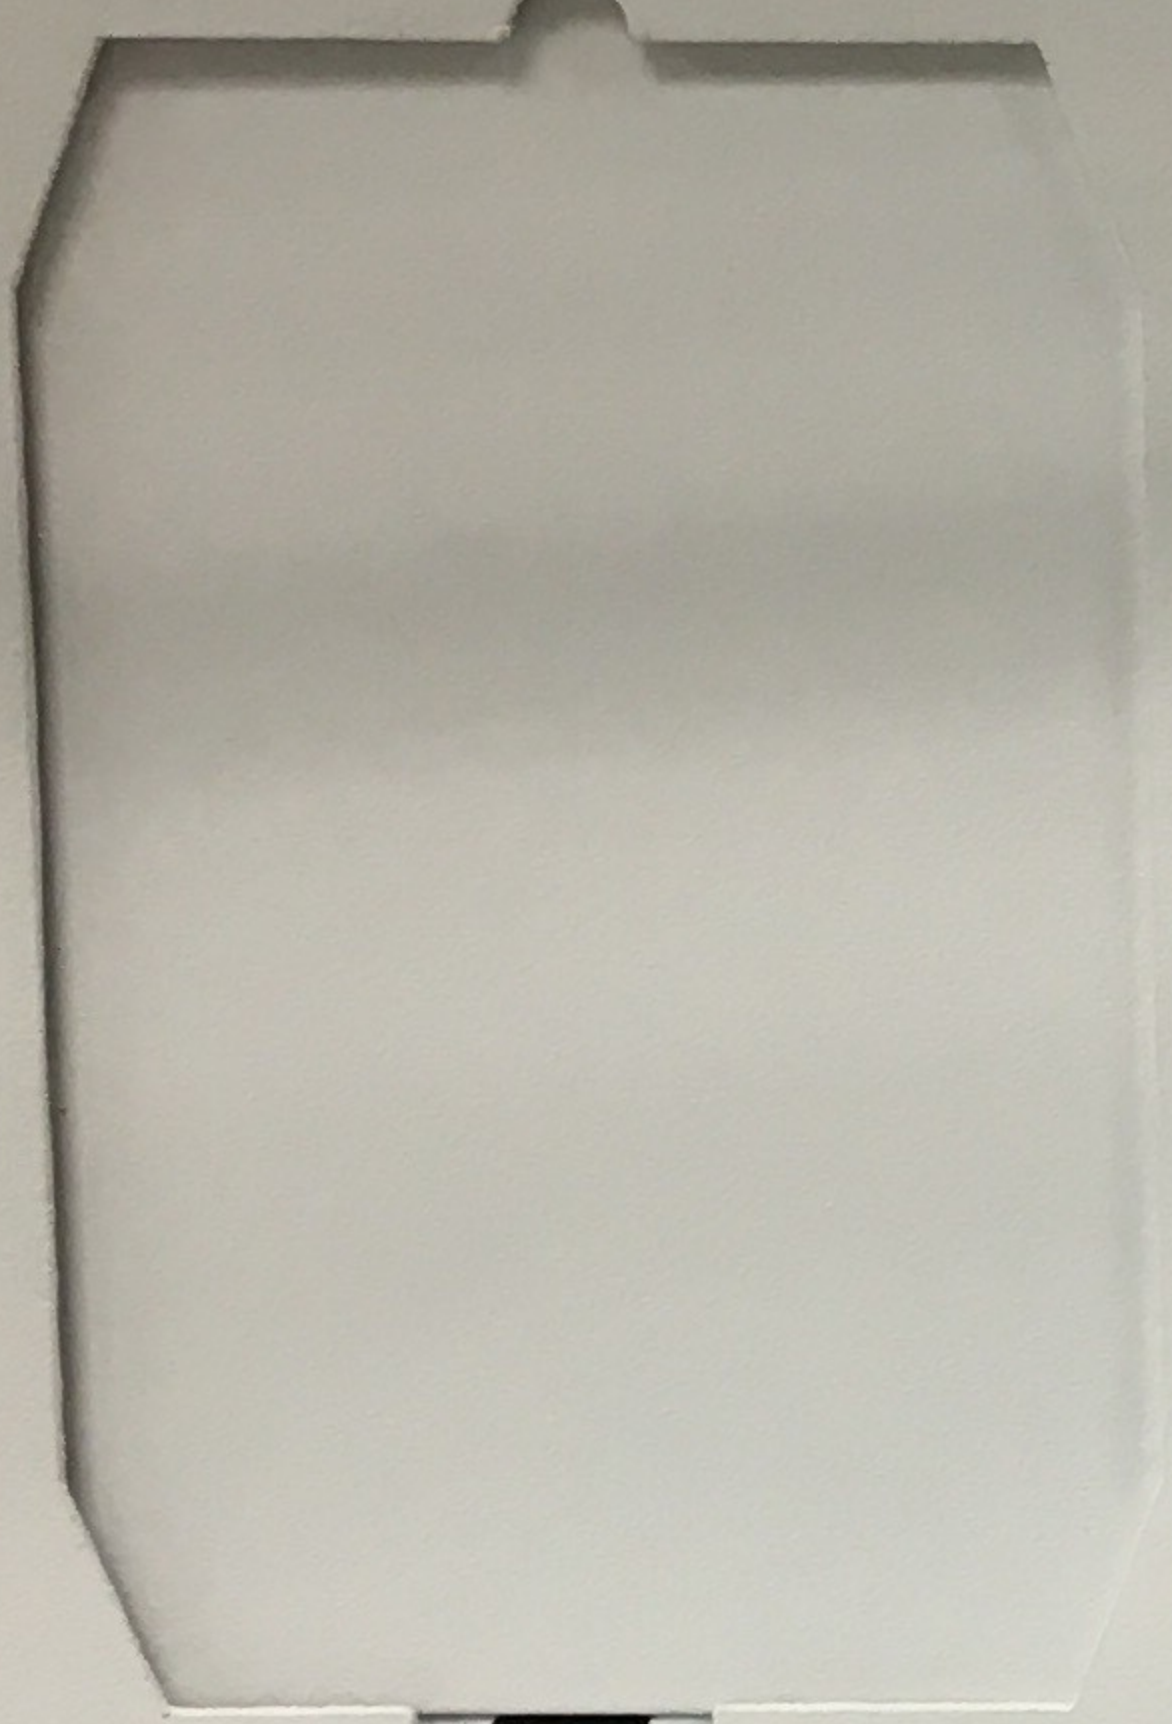


4


3

2

1

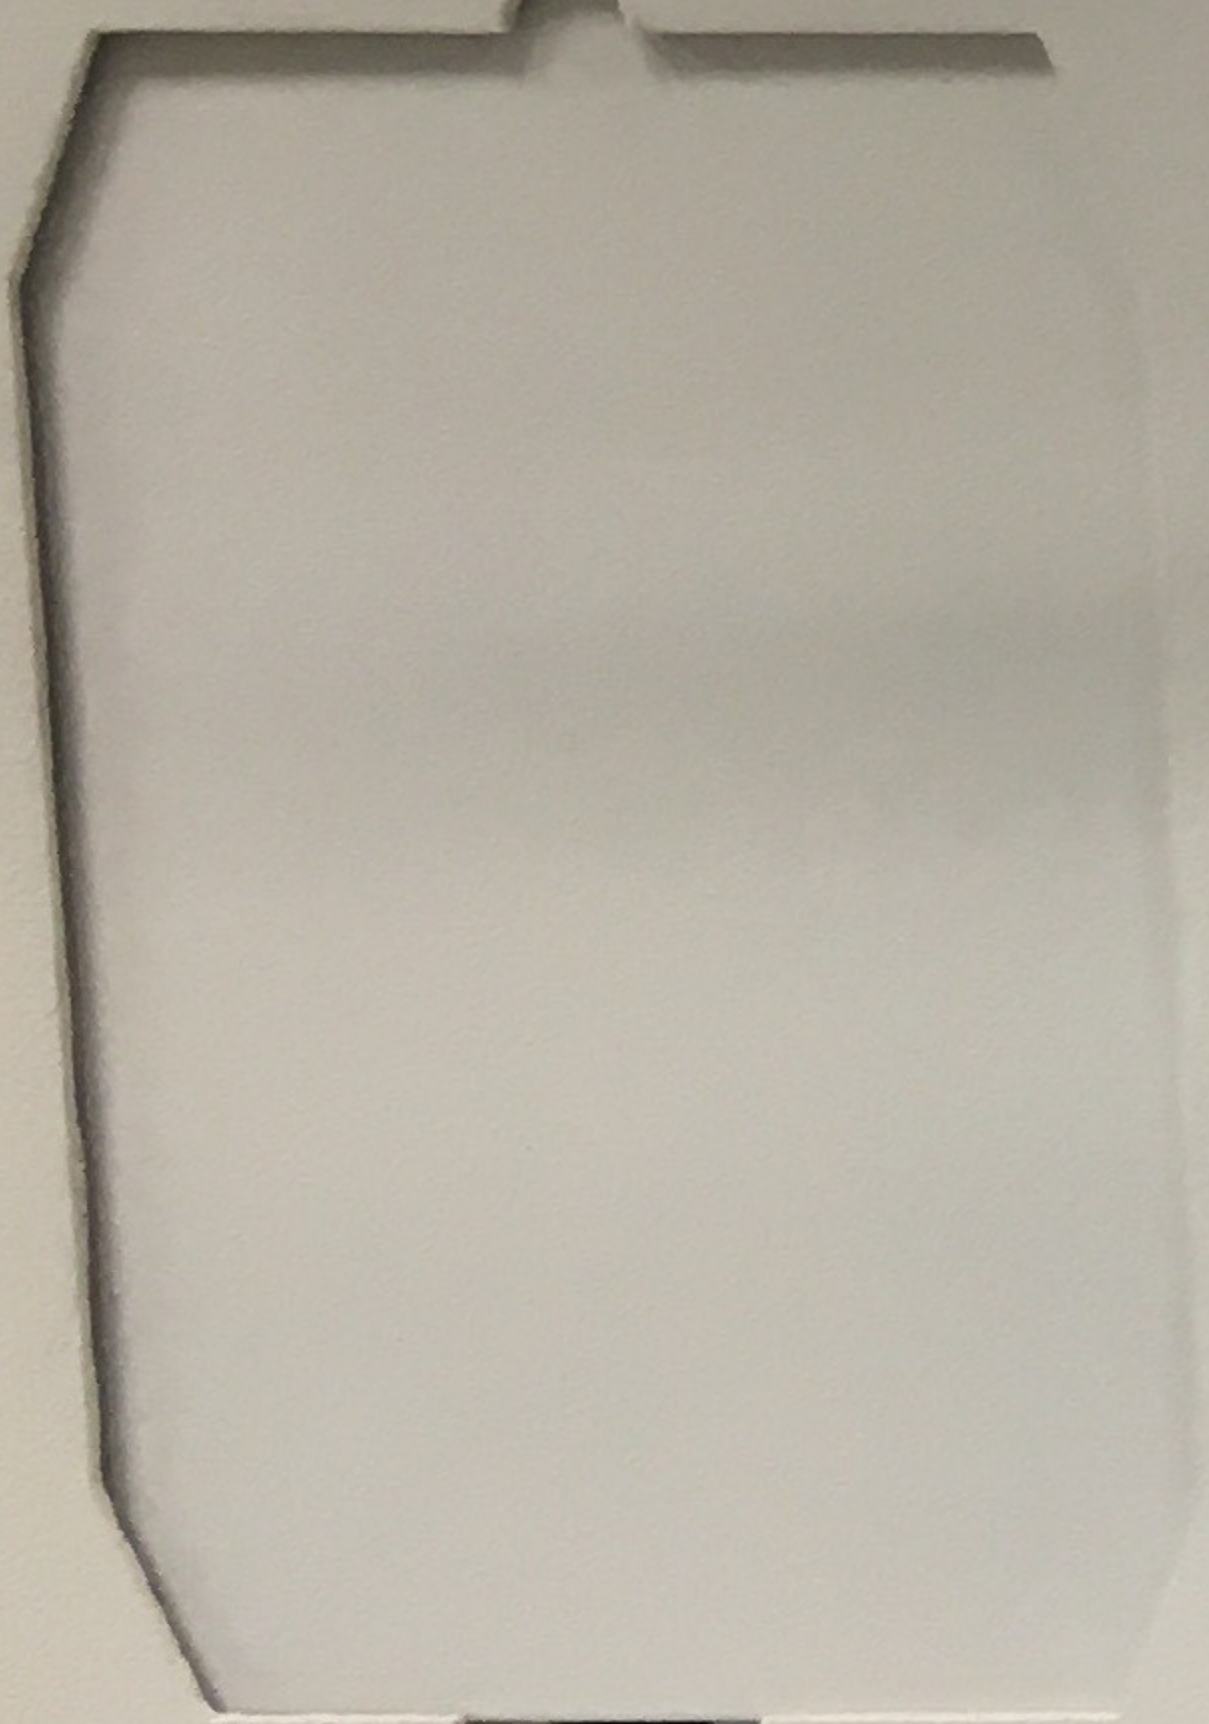

SERVICE PORT


AMPHENOL THERMOMETRICS, INC.  
 KAYE VALIDATOR X2015  
 SERIAL NO.   
 ASSEMBLED IN USA 16090009

**Amphenol Thermometrics, Inc.**  
 Calibration & Services Contact:  
 USA - Tel.: 814-834-9140  
 Europe/Asiapac - Tel.: +49(0) 7231-143350  
 Web: www.amphenol-sensors.com

FCC ID: 2AJQZ-AVS-X2015  
 IC: 7738A-WB11NDF1  
 CMIT ID: XXXXXXXXXXXX  
 Model No.: X2015

CONFORMS TO  
 UL 61010-1  
 CERTIFIED TO  
 CSA C22.2 NO. 1010-1



 T, 4.0 A  
 RATINGS:  
 100-240 ~  
 1.8 A RMS MAX  
 50/60 Hz

