	Issue Department: Bedding Division	Date:	2021-12-08
	System Instruction	Author:	
User Manual of RF405B		Edition:	1.0
		Page 1 of 4	

User Manual of RF405B

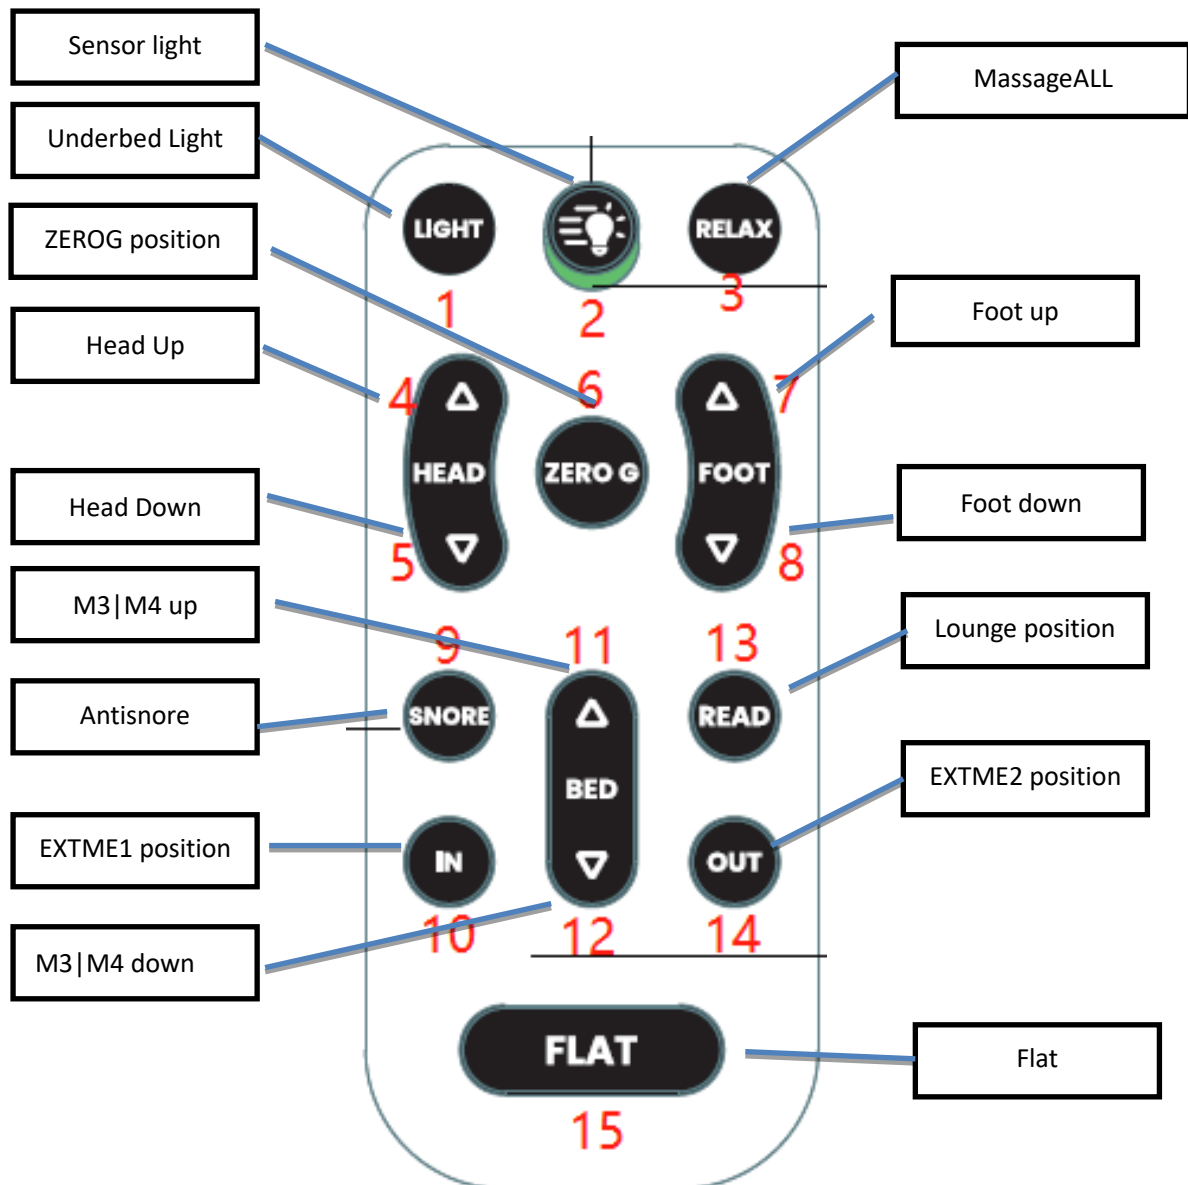


Figure 1 button of remote

Item

1.1 ZG button 6

Click the ZG button, the actuator moves to ZG position, stop when click any button during the movement;

Press and hold the ZG button for 5s, timer LED of remote flashes, the control box records current position as ZG position;

When in the process of moving to memory positions, the head and foot actuators move first, then the tilt and lumbar actuators move;

1.2 AntiSnore button 9

Click AntiSnore button, actuators move to AntiSnore position, stop when click any button during movement;

Press and hold AntiSnore button for 5s, timer LED of remote flashes, the control box records current position as AntiSnore position;

When in the process of moving to memory positions, the head and foot actuators move first, then the tilt and lumbar actuators move;

1.3Head up button 4

Press and hold HEAD UP button of remote, head actuator moves out, stop when released;

1.4 Head down button 5

Press and hold HEAD DOWN button of remote, head actuator moves in, stop when released;

1.5 Foot up button 7

Pressa and hold FOOT UP button of remote, foot actuator moves out, stop when released;

1.6 Foot down button 8

Press and hold Foot DOWN button of remote, Foot actuator moves in, stop when released;

1.7 Flat button 15

Click FLAT button, the bed goes flat, stop when click any button during the process of going flat;

1.8 Massage all 3

Click Massage all button, all massage motor switches massage intensity, massage intensity switches among 0-1-2-3;

1.9 M3/M4 motor up button 11

Press and hold M3/M4 UP button of remote, M3/M4 actuator moves out, stop when released;

1.10 M3/M4 motor down button 12

Press and hold M3/M4 down button of remote, M3/M4 actuator moves in, stop when released;

1.11 Memory position button 10 and 13 14

Click memory position to move the actuator to the memory position.

Press and hold the button for 5s, timer LED of remote flashes, the control box records current position as the memory position;

1.12 Under bed light button 1

Click the under bed light button, the under bed light switch its on/off state; After the under bed light opens, if do not manually close, it will automatically turn off after 5 minutes;

1.12 Sensor light switch 2

Turn up the switch , open the Sensor function of the bed light , the turn down the switch to close sensor function.

FCC:

Any Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

ISED RSS Warning:

This device complies with Innovation, Science and Economic Development Canada licence exempt RSS standard(s). Operation is subject to the following two conditions: (1) this device may not cause interference, and (2) this device must accept any interference, including interference that may cause undesired operation of the device.

Le présent appareil est conforme aux CNR d'ISED applicables aux appareils radio exempts de licence.

L'exploitation est autorisée aux deux conditions suivantes:

- (1) l'appareil ne doit pas produire de brouillage, et
- (2) l'utilisateur de l'appareil doit accepter tout brouillage radioélectrique subi, même si le brouillage est susceptible d'en compromettre le fonctionnement.

ISED RF exposure statement:

This equipment complies with ISED radiation exposure limits set forth for an uncontrolled environment. The device has been evaluated to meet general RF exposure requirement.

Le matériel est conforme aux limites de dose d'exposition aux rayonnements énoncés pour un autre environnement. Ce dispositif a été évalué à satisfaire l'exigence générale de l'exposition aux rf.