

Test Report No.50121721 001

Appendix D: Radiated and Mains Spurious Emission Data

(File: 50121721AppendixD)



Contents

Spurious Emissions, Band Edges, 2.35-2.5G	2
Spurious Emissions, TX Mode, 1-18G.....	6
Spurious Emissions, TX Mode, 18-26G.....	12
Spurious Emissions, TX Mode, 30M-1G	18
Spurious Emissions, TX Mode, 9k-30M	20
Spurious Emissions, RX Mode, 1-18G	22
Spurious Emissions, RX Mode, 18-26G	24
Spurious Emissions, RX Mode, 30M-1G.....	26
Spurious Emissions, RX Mode, 9K-30M.....	28

Spurious Emissions, Band Edges, 2.35-2.5G



Radiated Bandedge (GFSK)

Low Channel (Hor)

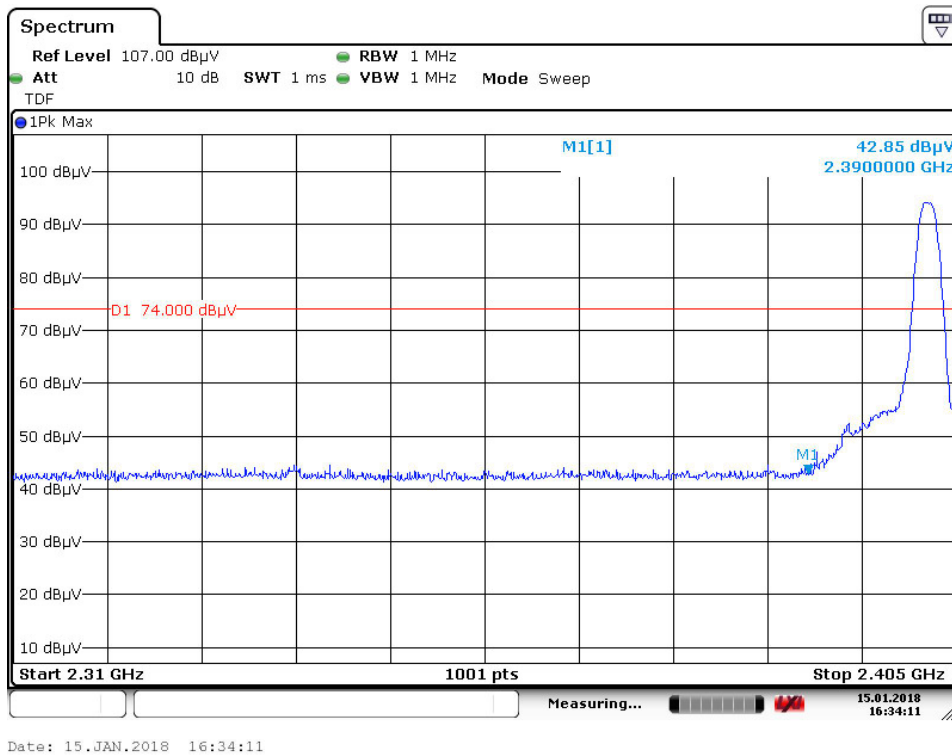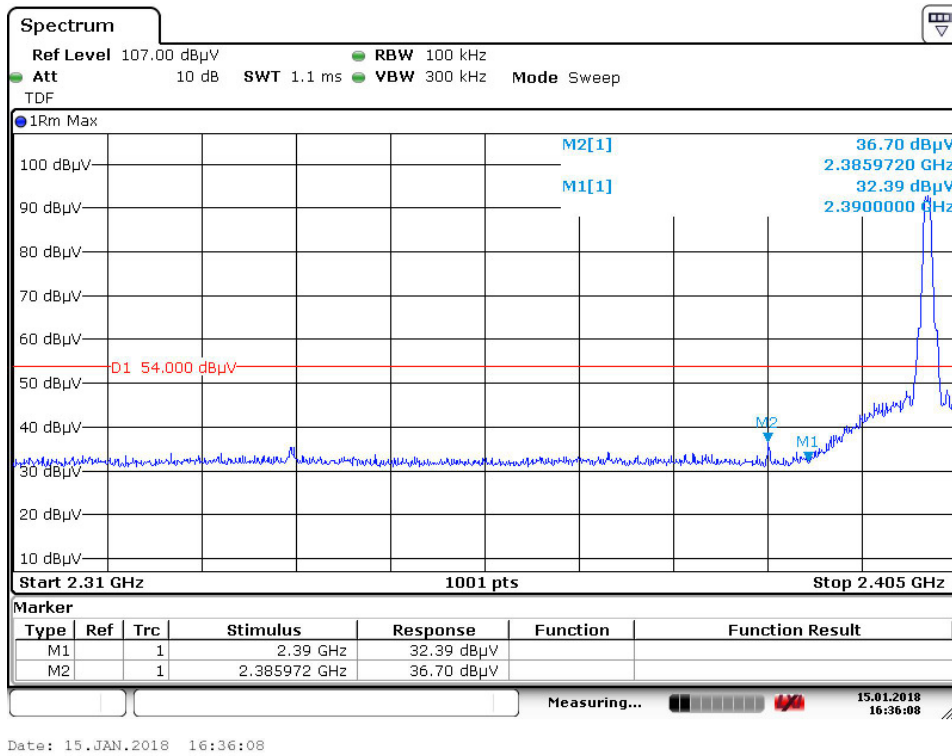

Spurious Emissions, Band Edge, 2.35-2.5G


Low Channel (Ver)

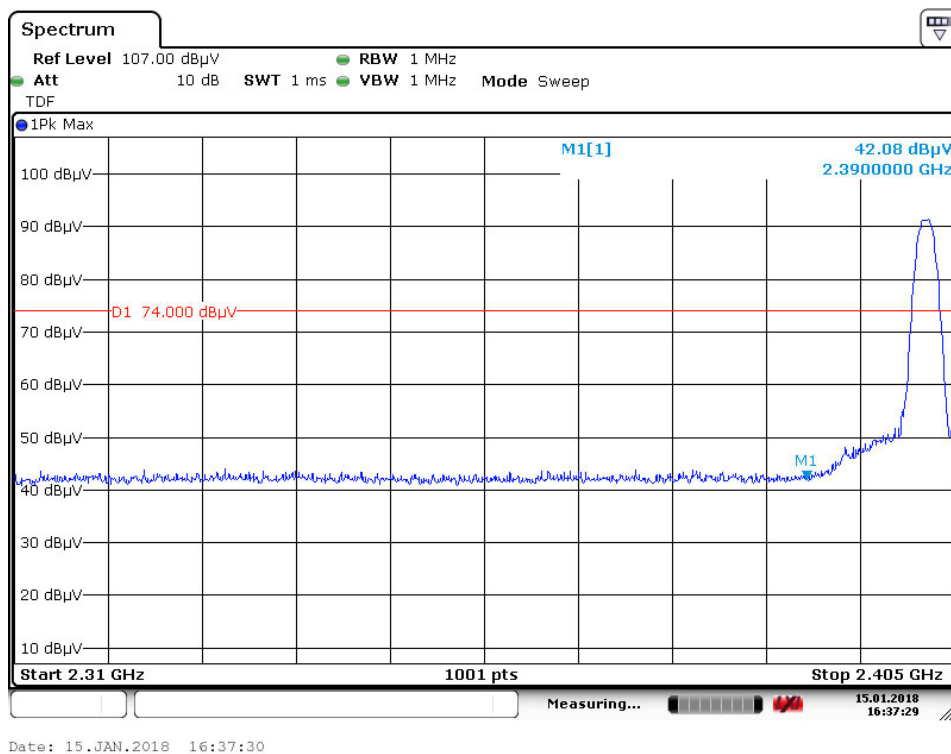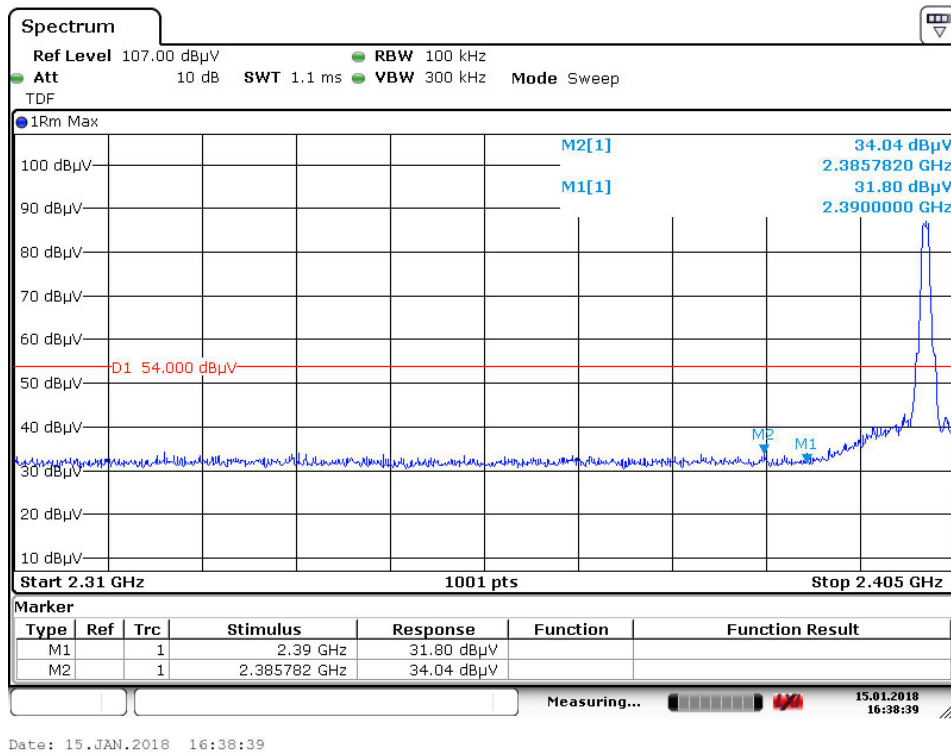


Spurious Emissions, Band Edge, 2.35-2.5G

Radiated Bandedge (GFSK)

High Channel (Hor)

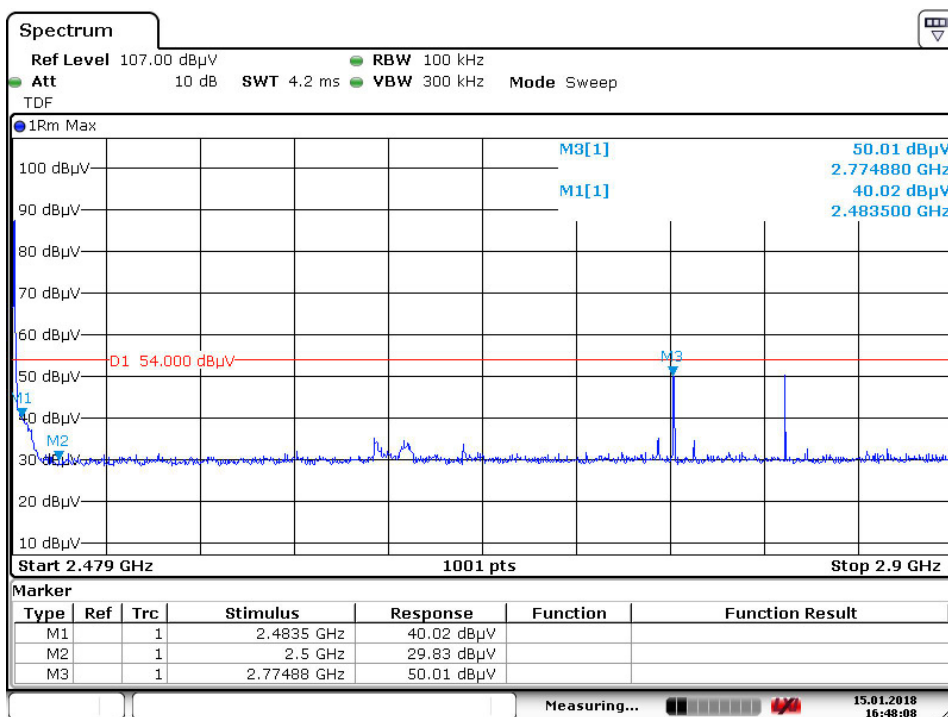



Date: 15.JAN.2018 16:48:08

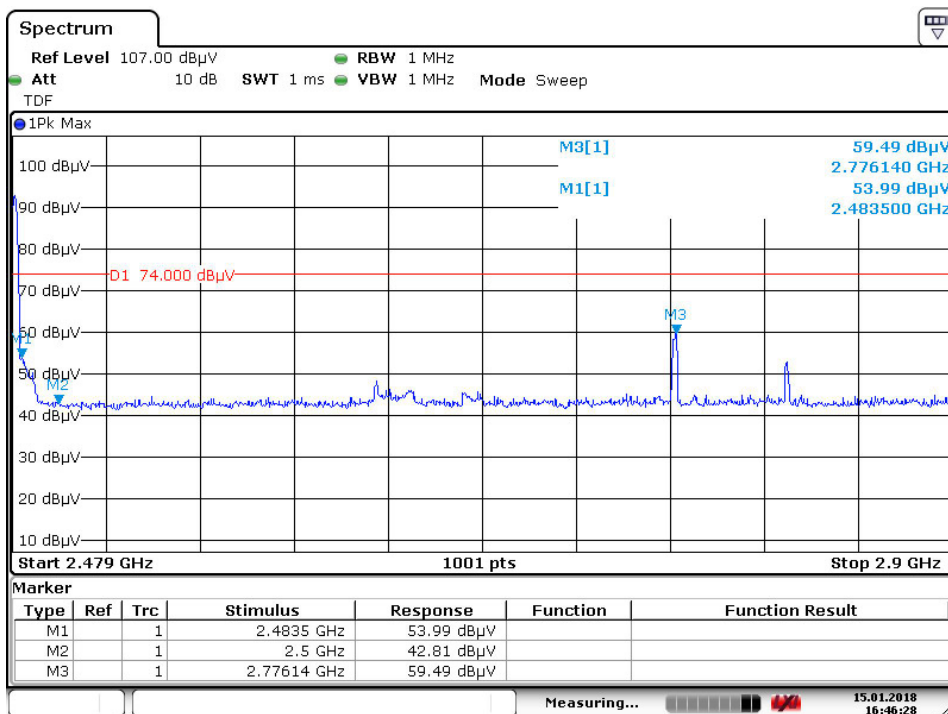

Date: 15.JAN.2018 16:46:28

Spurious Emissions, Band Edge, 2.35-2.5G

High Channel (Ver)

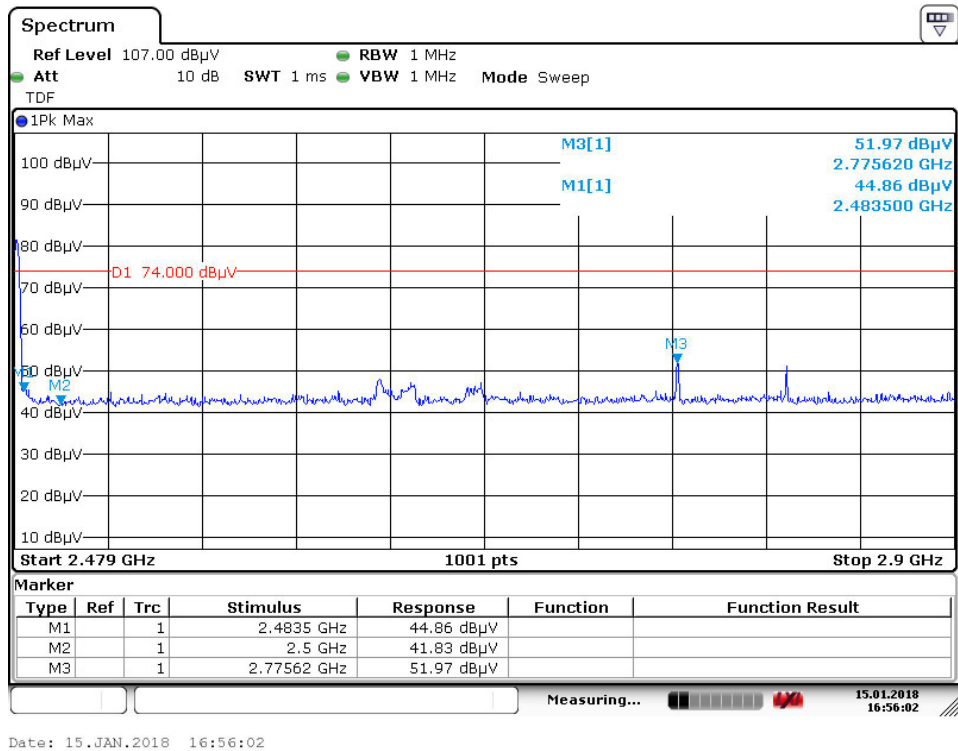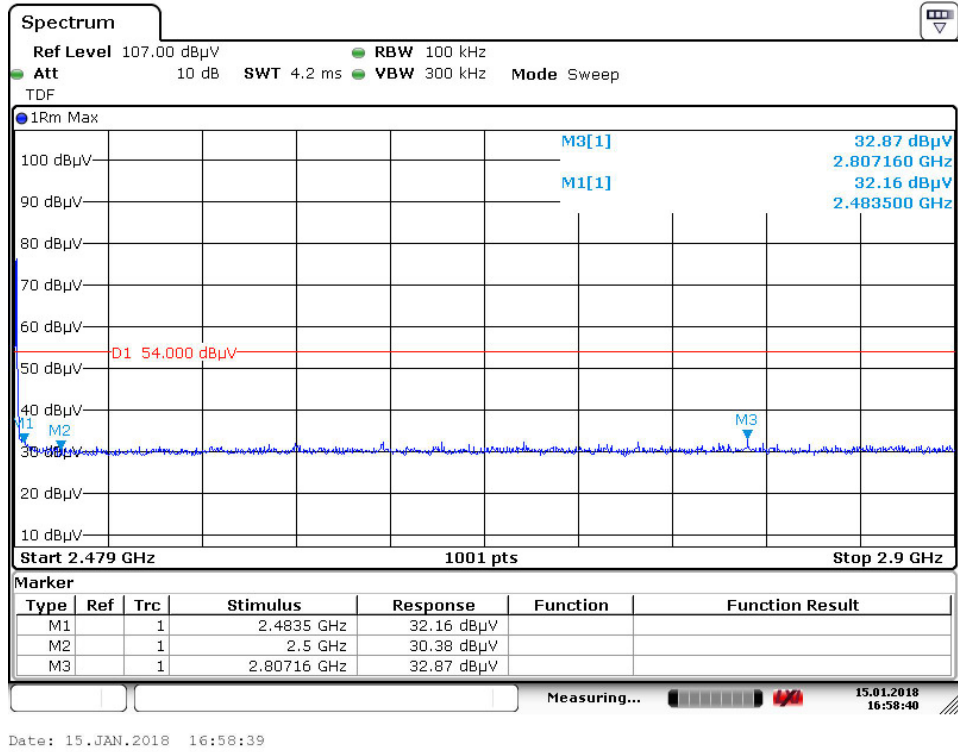

Spurious Emissions, Band Edge, 2.35-2.5G


Spurious Emissions, TX Mode, 1-18G



TUV Rheinland Taiwan Ltd.


11F., No.758, Sec.4 Bade Road. Songshan Dist, Taipei City 105

Tel:+886-2172-7000 fax:+886-2528-0018

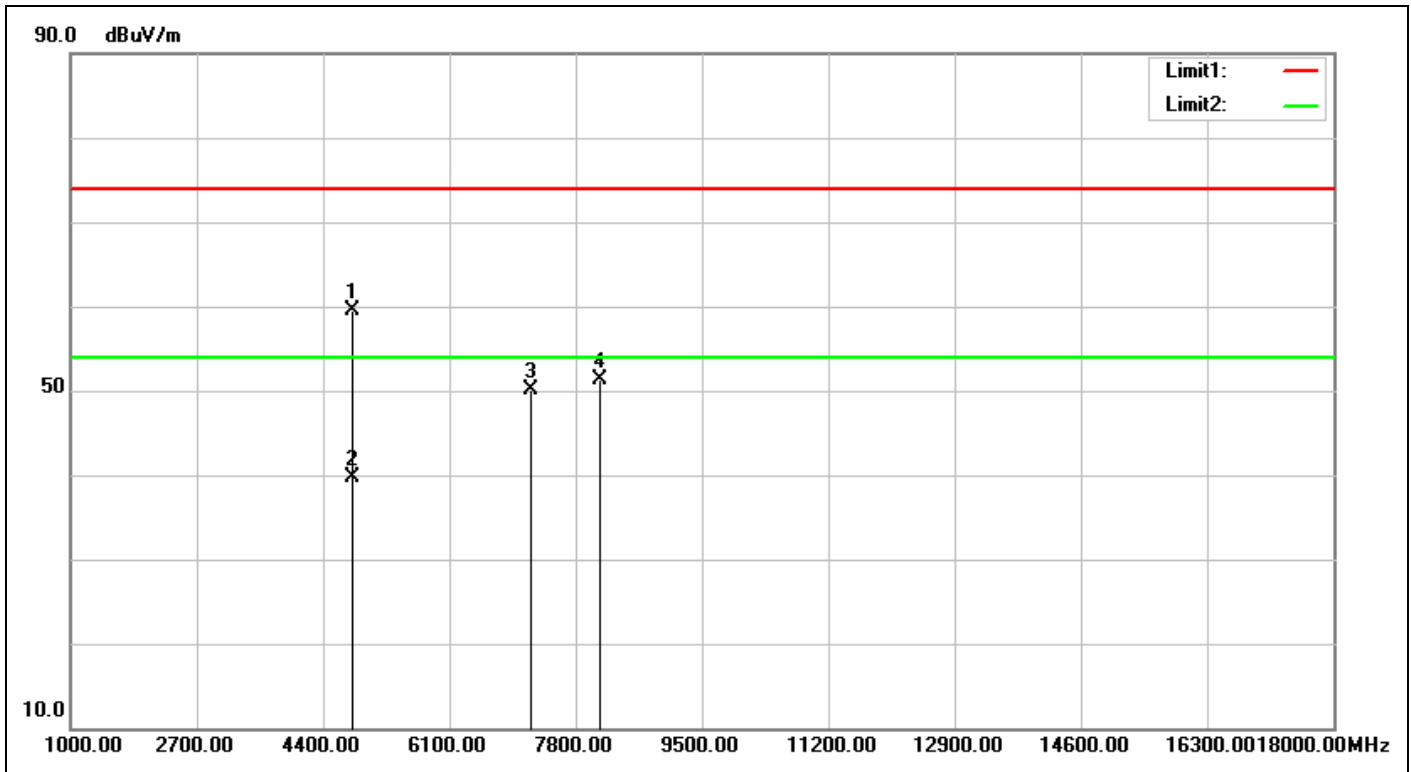


Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC Above 1G PEAK	Ant. Polarization:	Horizontal
Test item:	Radiation Emission	Test Time:	2018/1/15 17:01:35
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2402-TX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	4804.000	-2.72	62.17	59.45	74.00	-14.55	peak	100	178	
2	4804.000	-2.72	42.38	39.66	54.00	-14.34	AVG	100	178	
3	7206.000	5.25	44.88	50.13	74.00	-23.87	peak		0	
4	8123.000	5.96	45.28	51.24	74.00	-22.76	peak	100	78	

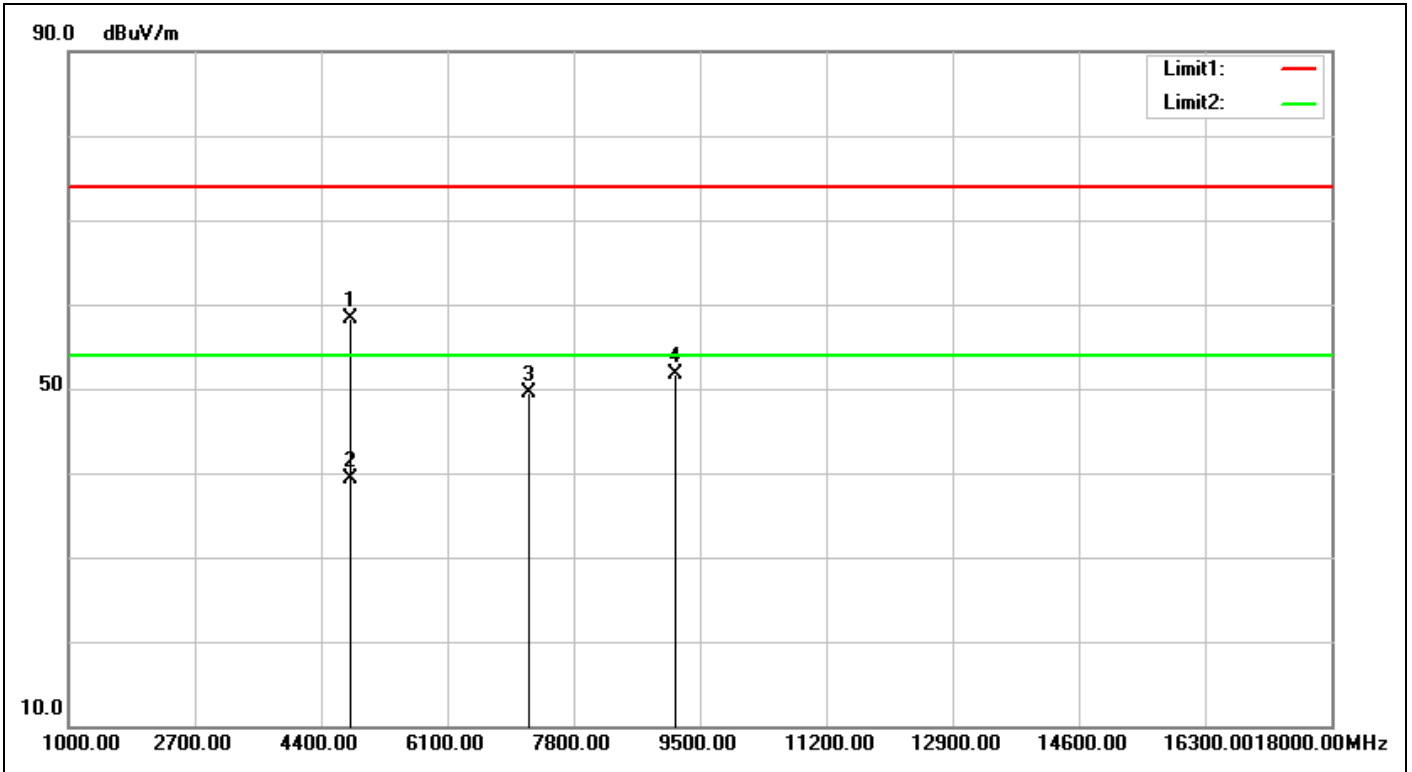


Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC Above 1G PEAK	Ant. Polarization:	Vertical
Test item:	Radiation Emission	Test Time:	2018/1/15 17:02:38
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2402-TX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	4804.000	-2.72	61.01	58.29	74.00	-15.71	peak	100	229	
2	4804.000	-2.72	42.06	39.34	54.00	-14.66	AVG	100	229	
3	7206.000	5.25	44.28	49.53	74.00	-24.47	peak			
4	9160.000	6.48	45.17	51.65	74.00	-22.35	peak	100	213	

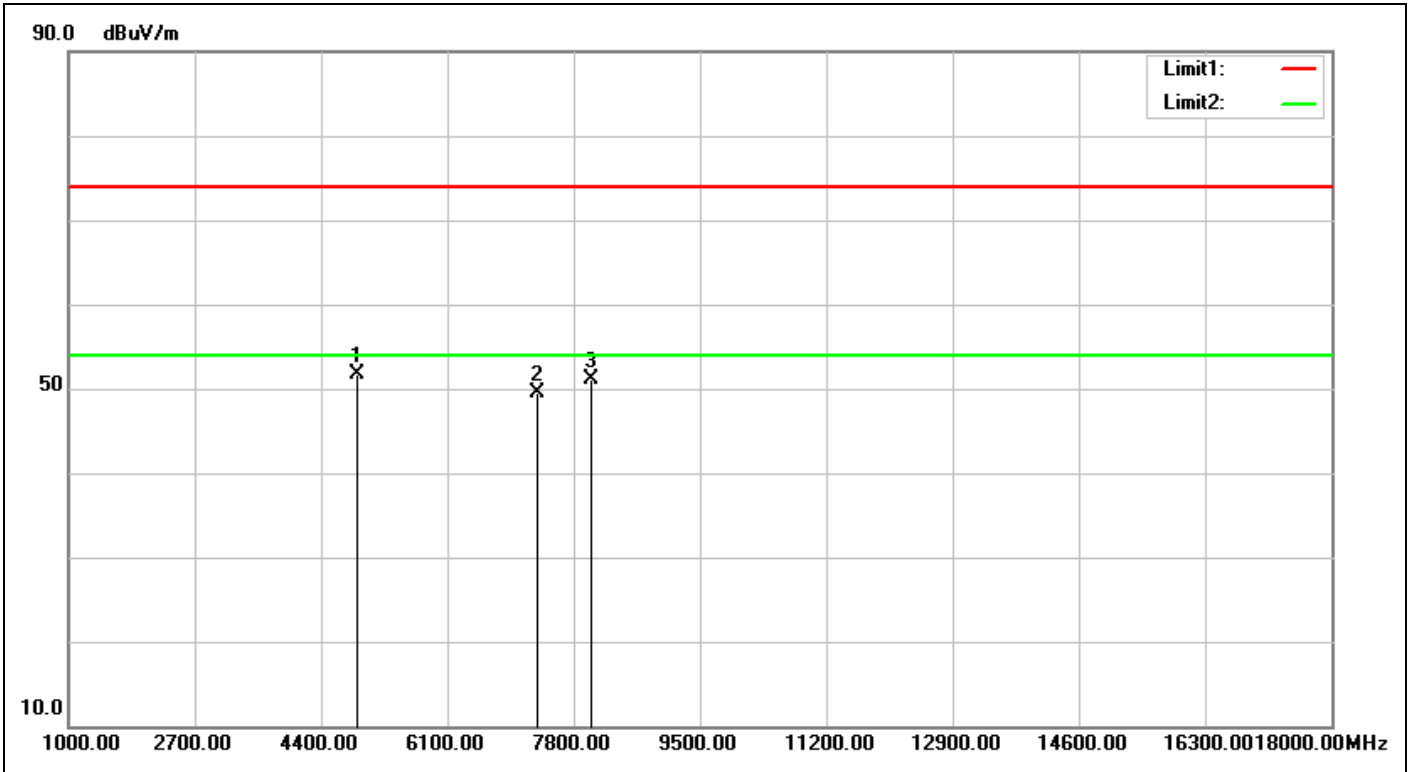


Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC Above 1G PEAK	Ant. Polarization:	Horizontal
Test item:	Radiation Emission	Test Time:	2018/1/15 17:11:11
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2440-TX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	4880.000	-2.50	54.25	51.75	74.00	-22.25	peak	100	167	
2	7320.000	5.54	44.02	49.56	74.00	-24.44	peak			
3	8038.000	5.86	45.27	51.13	74.00	-22.87	peak	100	114	

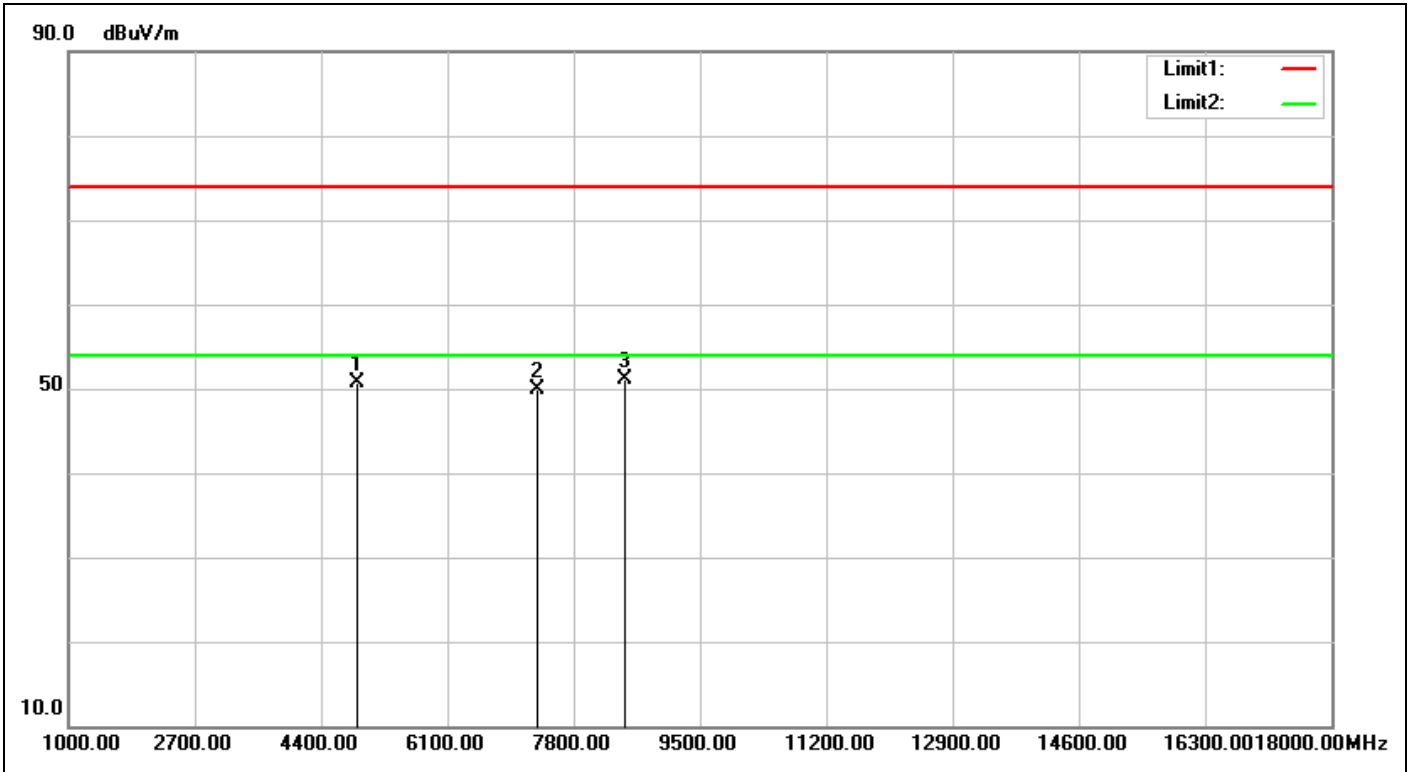


Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC Above 1G PEAK	Ant. Polarization:	Vertical
Test item:	Radiation Emission	Test Time:	2018/1/15 17:12:14
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2440-TX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	4880.000	-2.50	53.12	50.62	74.00	-23.38	peak	100	3	
2	7320.000	5.54	44.38	49.92	74.00	-24.08	peak			
3	8480.000	6.35	44.75	51.10	74.00	-22.90	peak	100	146	

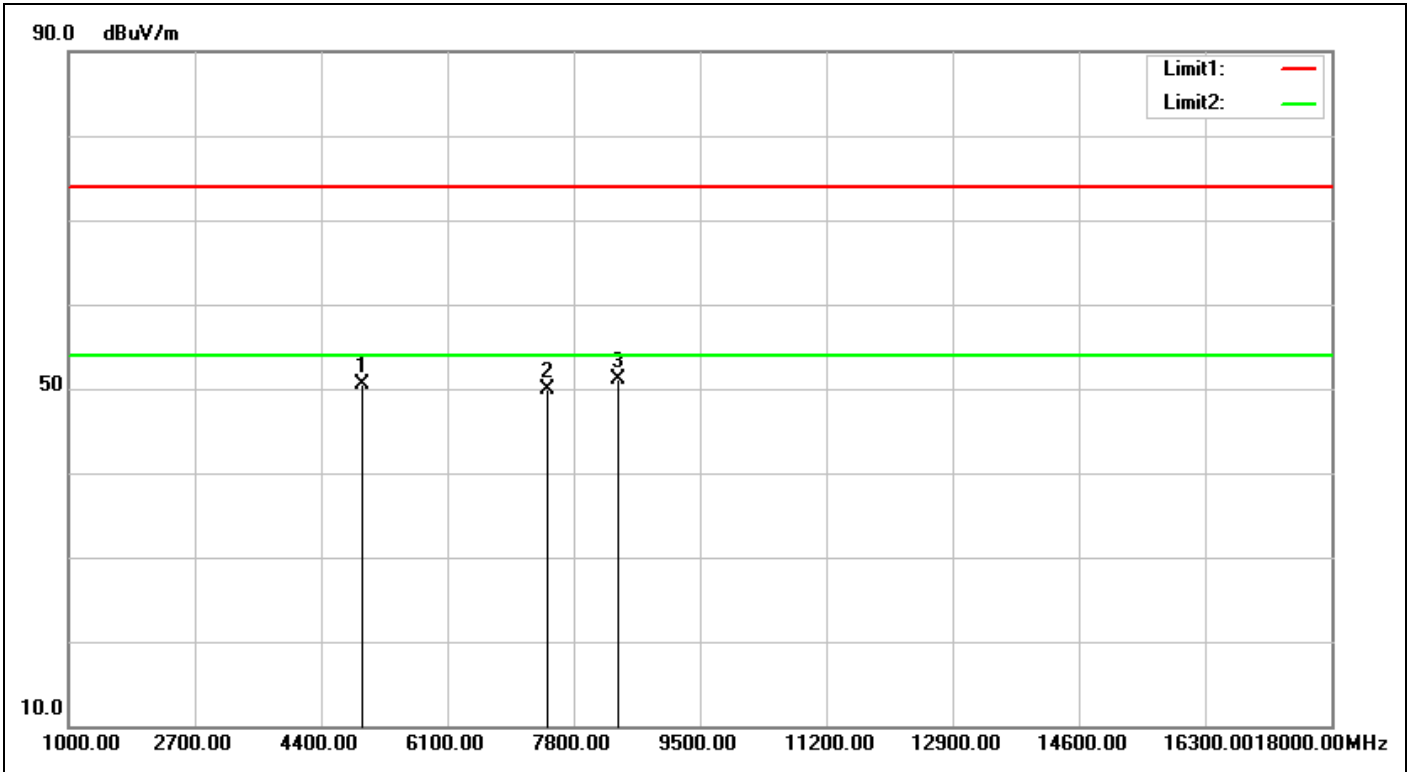

Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC Above 1G PEAK	Ant. Polarization:	Horizontal
Test item:	Radiation Emission	Test Time:	2018/1/15 17:16:12
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2480-TX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	4960.000	-2.28	52.70	50.42	74.00	-23.58	peak	100	78	
2	7440.000	5.84	44.09	49.93	74.00	-24.07	peak			
3	8395.000	6.26	44.93	51.19	74.00	-22.81	peak	100	0	

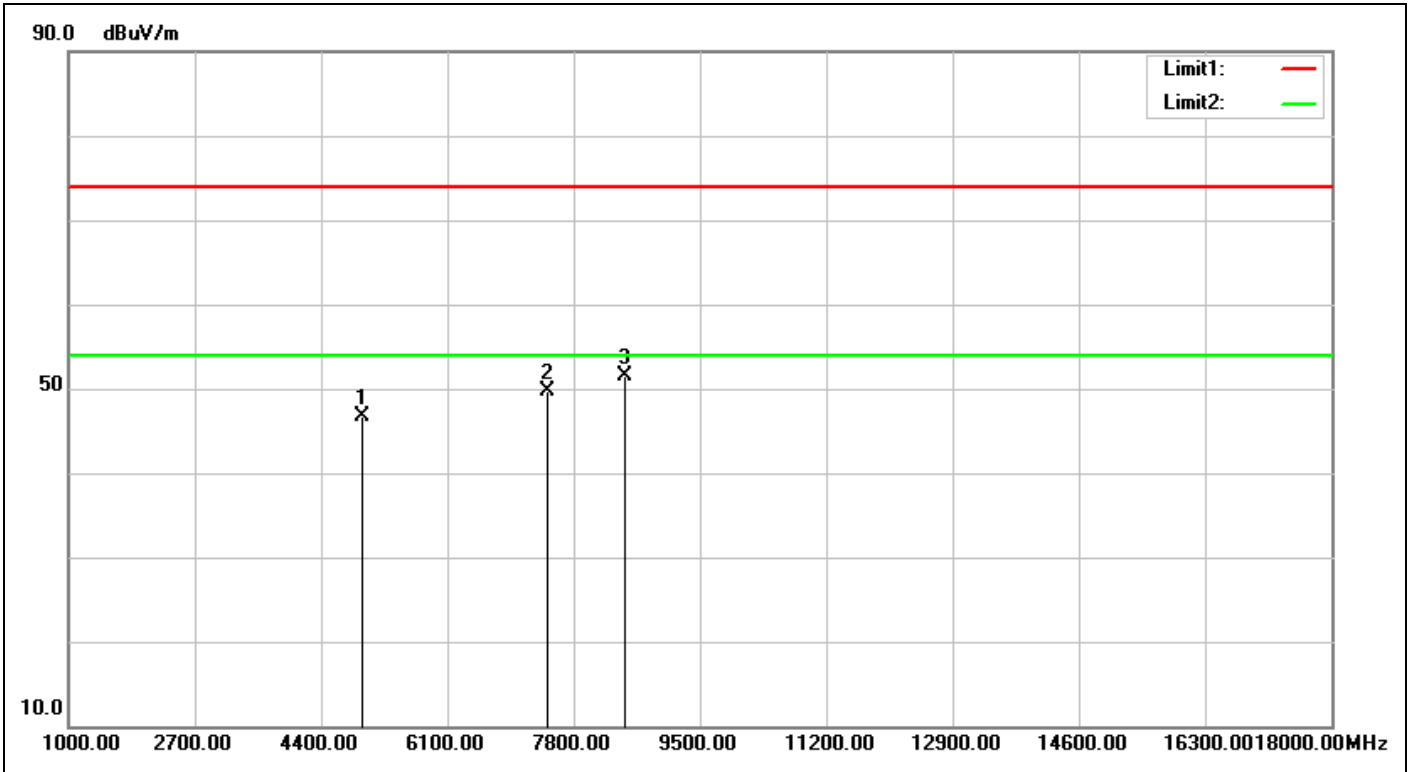


Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC Above 1G PEAK	Ant. Polarization:	Vertical
Test item:	Radiation Emission	Test Time:	2018/1/15 17:17:15
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2480-TX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	4960.000	-2.28	48.98	46.70	74.00	-27.30	peak			
2	7440.000	5.84	43.91	49.75	74.00	-24.25	peak			
3	8480.000	6.35	45.19	51.54	74.00	-22.46	peak	100	265	

Spurious Emissions, TX Mode, 18-26G




TUV Rheinland Taiwan Ltd.
 11F., No.758, Sec.4 Bade Road. Songshan Dist, Taipei City 105
 Tel:+886-2172-7000 fax:+886-2528-0018

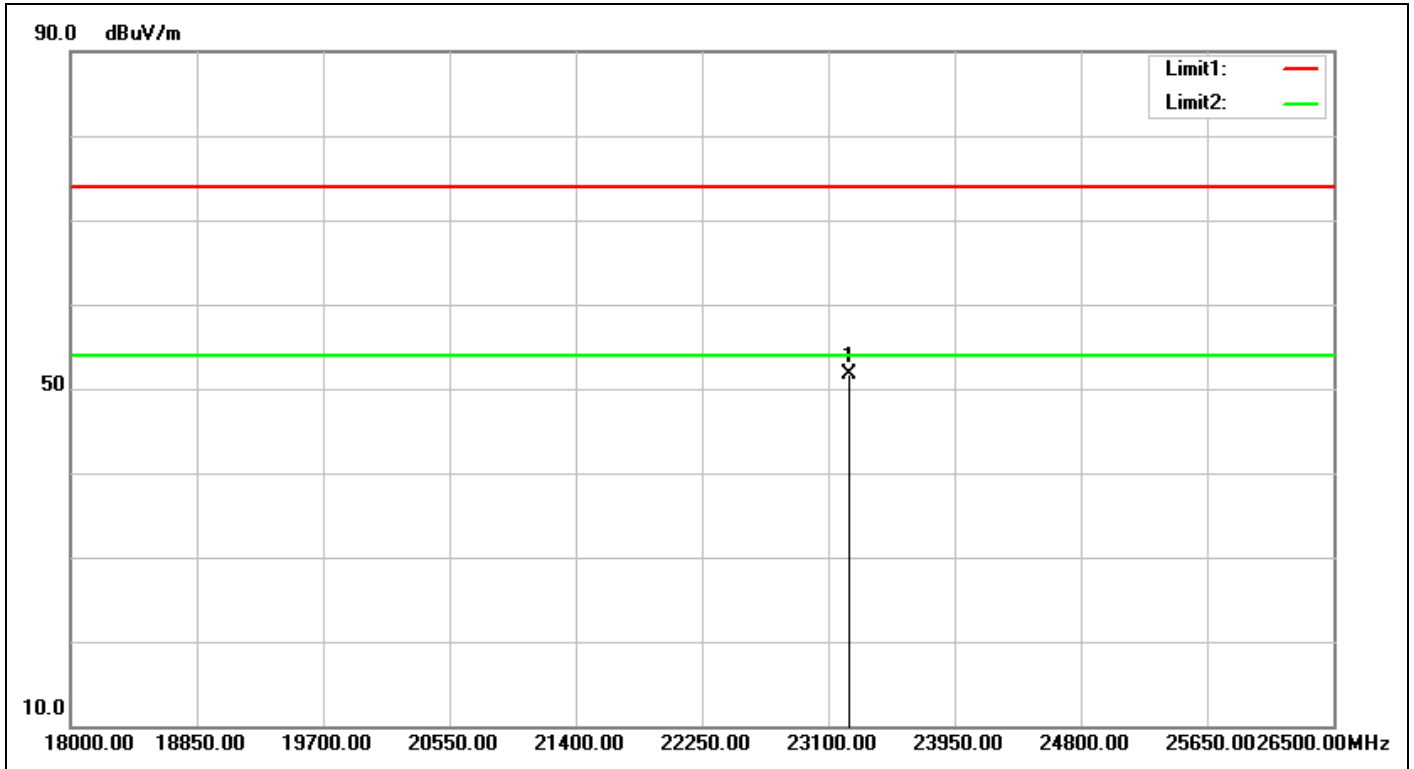


Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC Above 1G PEAK	Ant. Polarization:	Horizontal
Test item:	Radiation Emission	Test Time:	2018/1/15 18:55:16
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2402-TX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	23244.500	33.61	18.05	51.66	74.00	-22.34	peak		0	

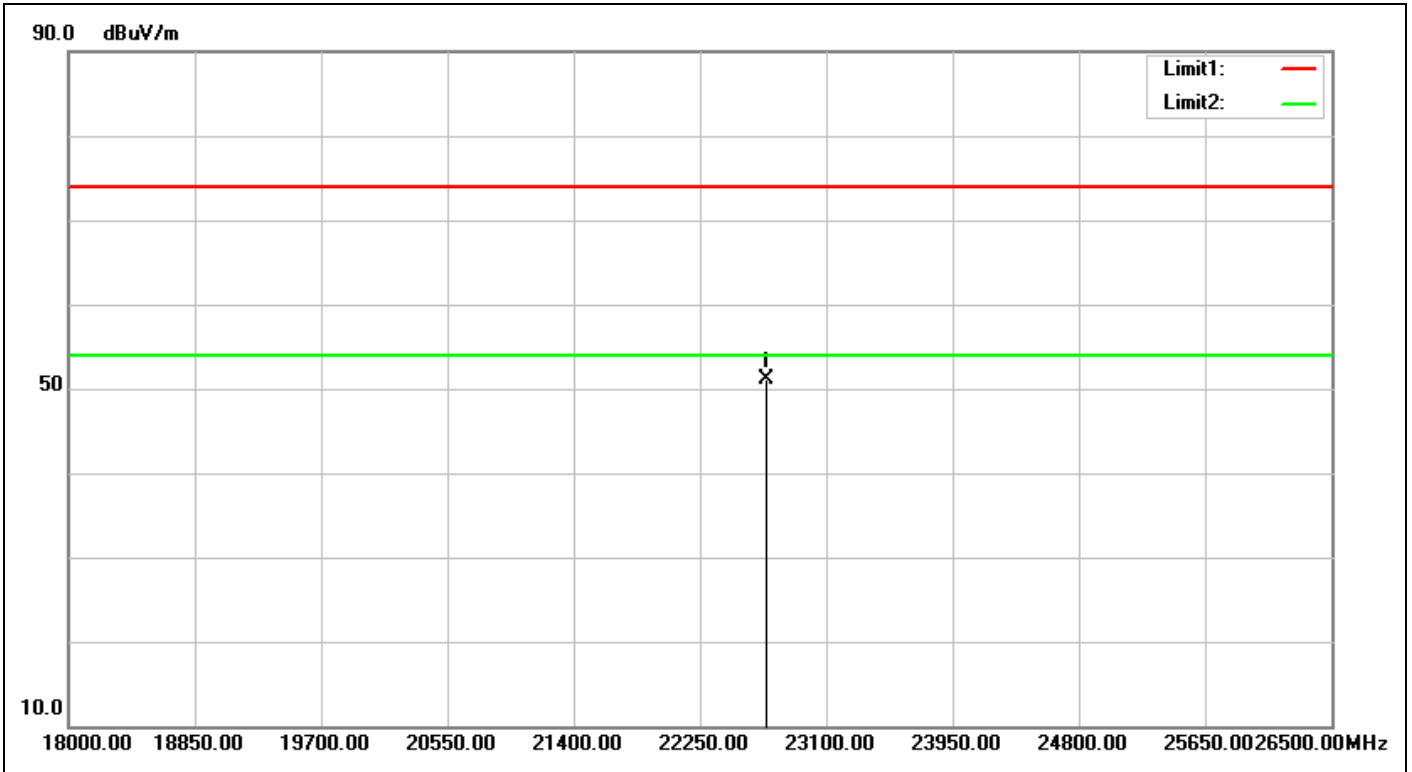


Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC Above 1G PEAK	Ant. Polarization:	Vertical
Test item:	Radiation Emission	Test Time:	2018/1/15 18:56:26
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2402-TX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	22692.000	33.26	17.90	51.16	74.00	-22.84	peak			

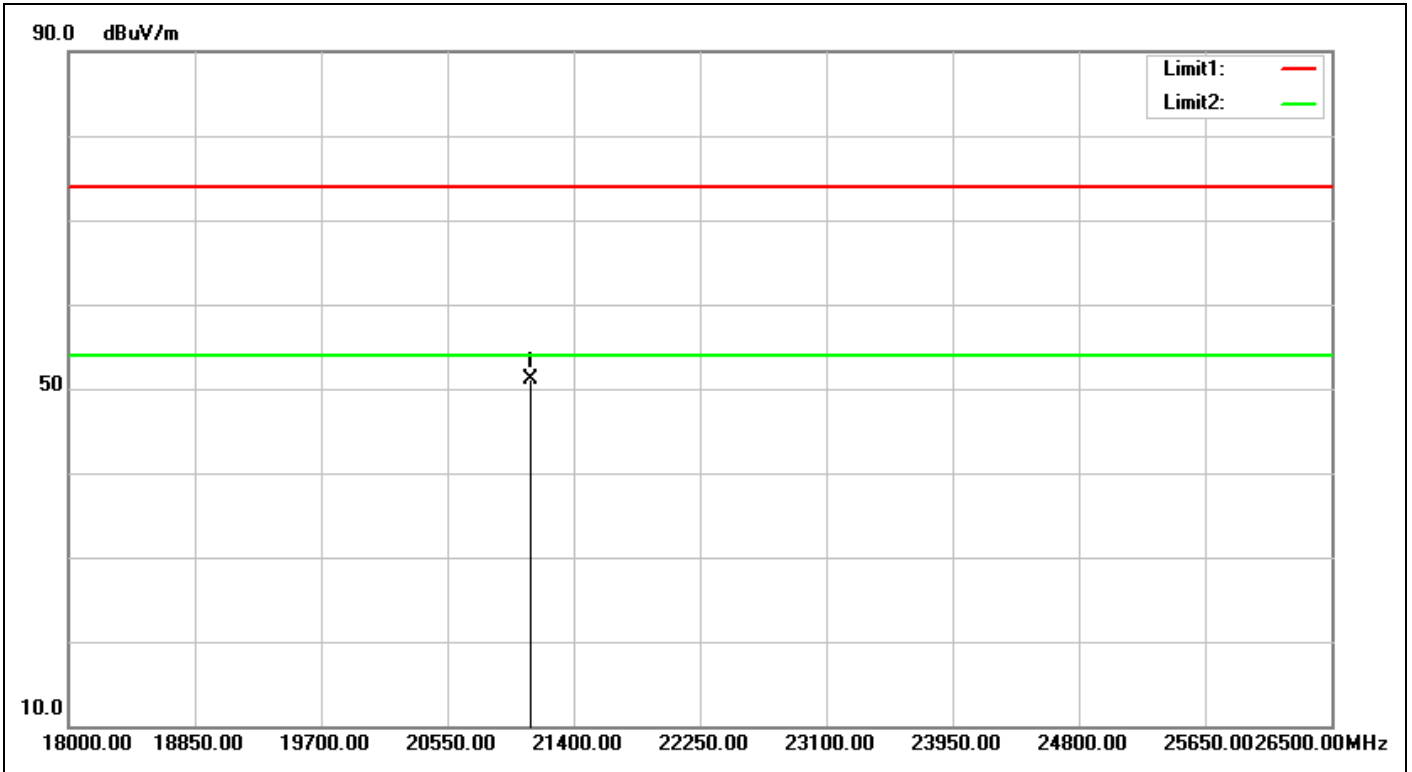


Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC Above 1G PEAK	Ant. Polarization:	Horizontal
Test item:	Radiation Emission	Test Time:	2018/1/15 18:56:55
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2440-TX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	21111.000	33.08	18.12	51.20	74.00	-22.80	peak			

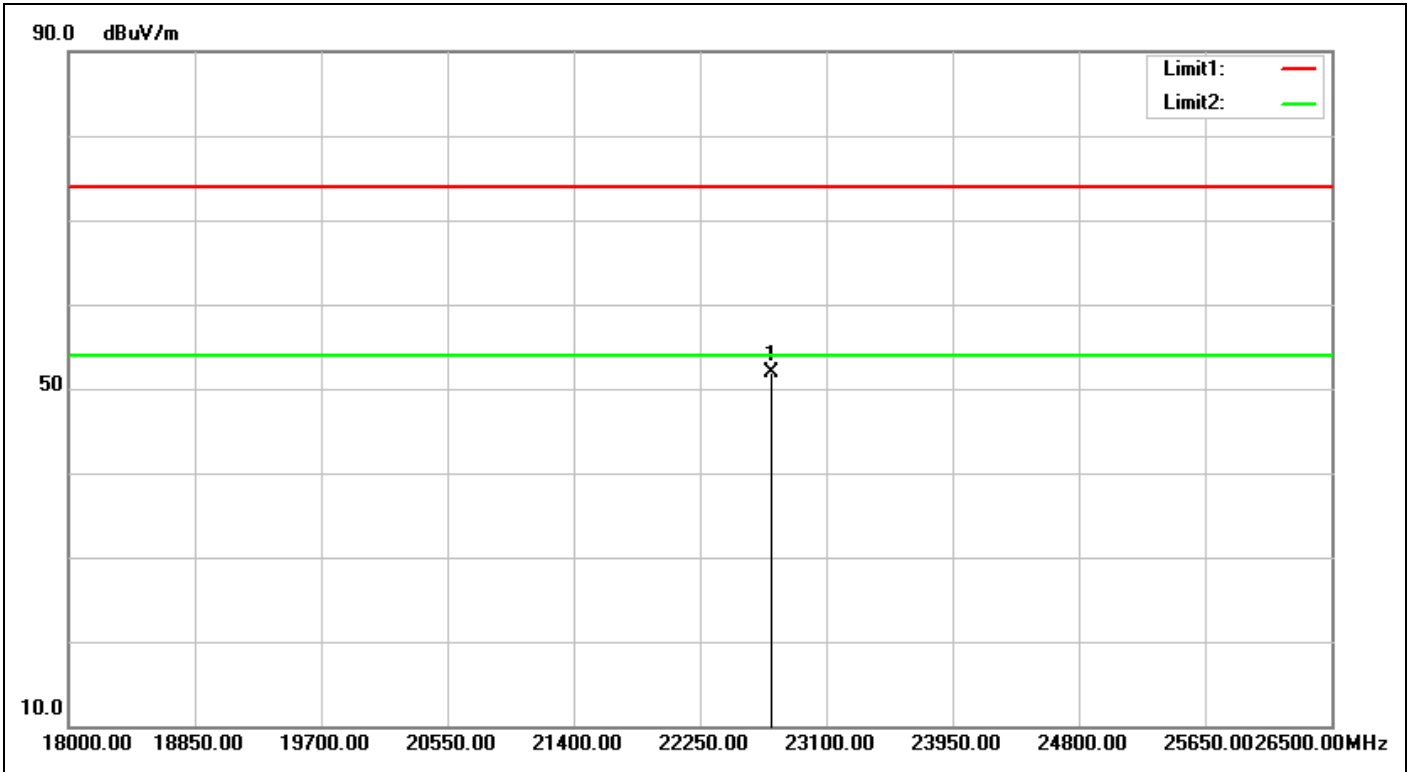


Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC Above 1G PEAK	Ant. Polarization:	Vertical
Test item:	Radiation Emission	Test Time:	2018/1/15 18:57:15
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2440-TX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	22734.500	33.27	18.56	51.83	74.00	-22.17	peak			

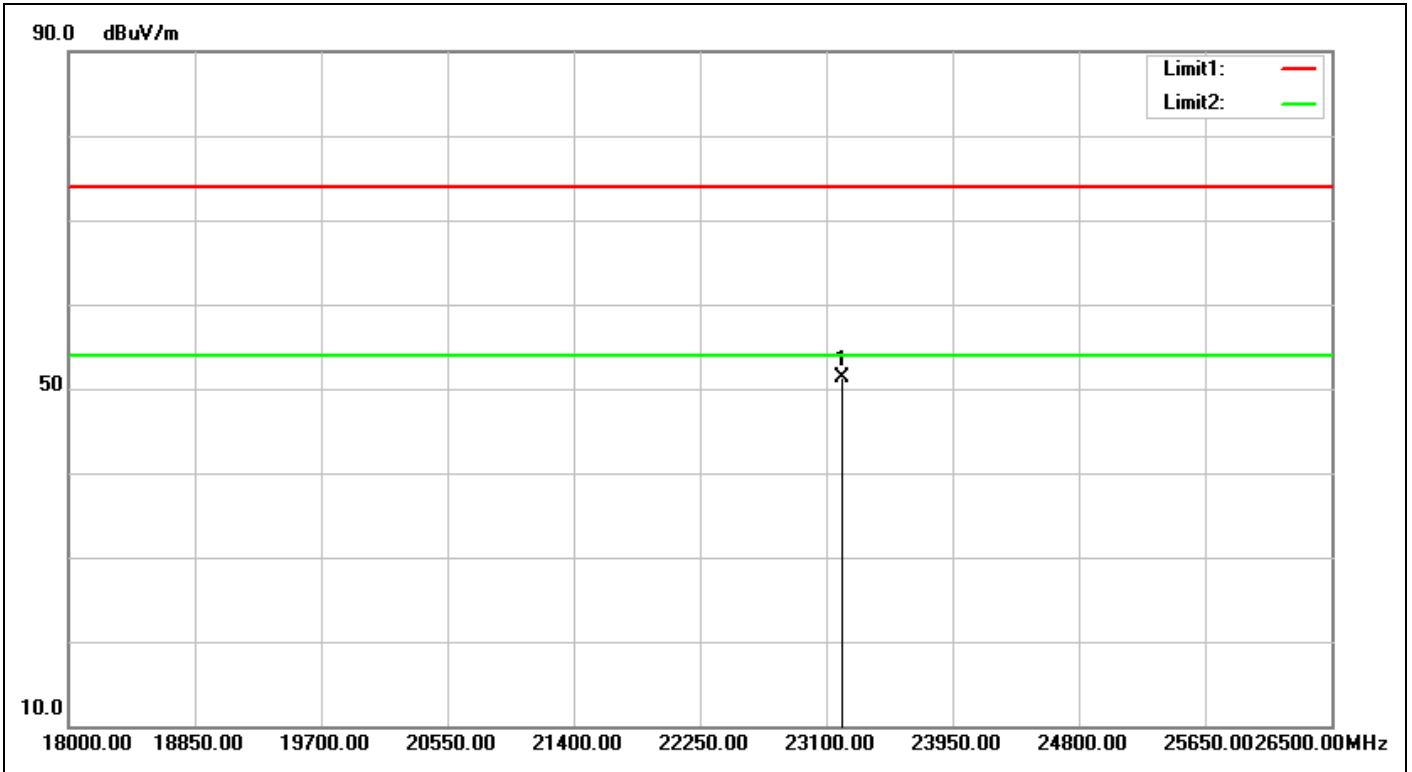

Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC Above 1G PEAK	Ant. Polarization:	Horizontal
Test item:	Radiation Emission	Test Time:	2018/1/15 18:57:40
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2480-TX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	23202.000	33.57	17.66	51.23	74.00	-22.77	peak			

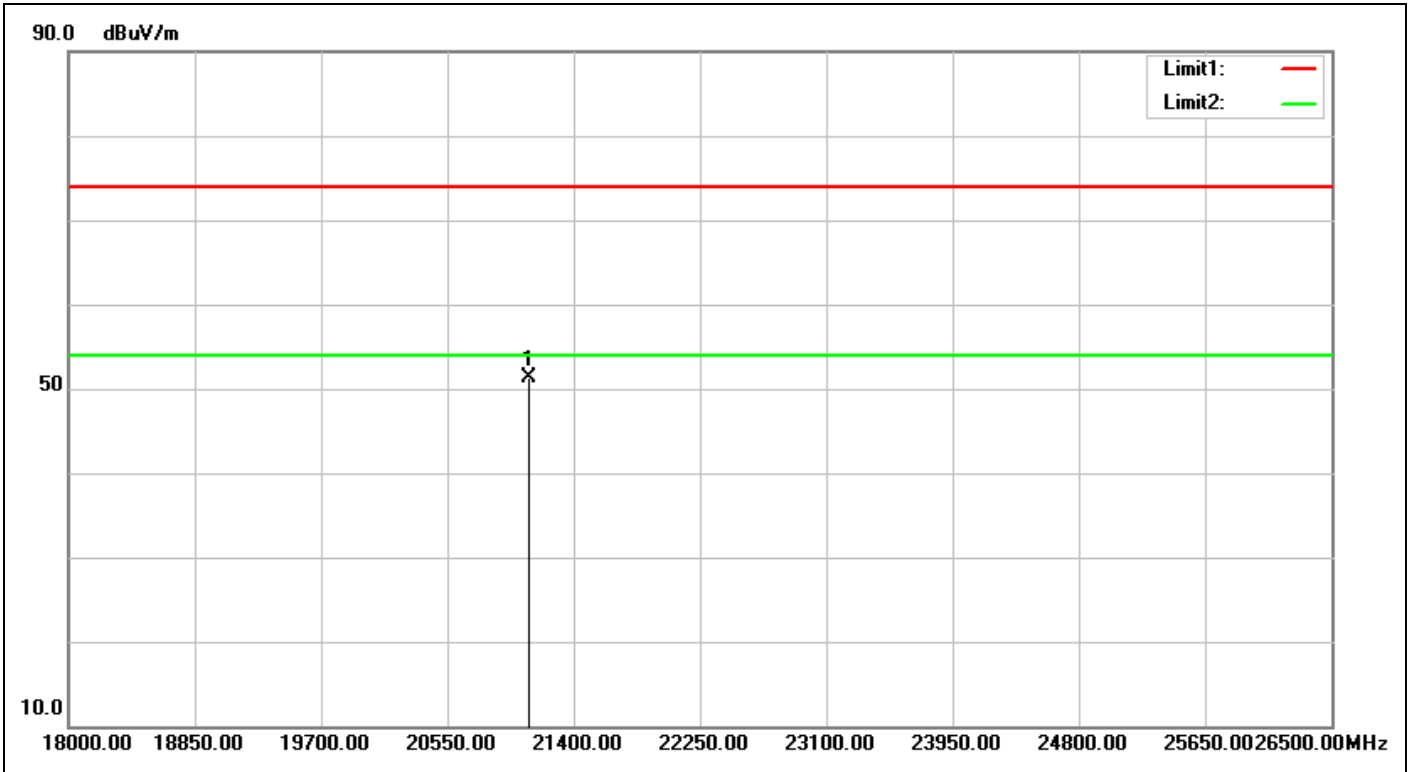

Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC Above 1G PEAK	Ant. Polarization:	Vertical
Test item:	Radiation Emission	Test Time:	2018/1/15 18:58:03
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2480-TX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	21102.500	33.07	18.27	51.34	74.00	-22.66	peak			


Spurious Emissions, TX Mode, 30M-1G



TUV Rheinland Taiwan Ltd.


11F., No.758, Sec.4 Bade Road. Songshan Dist, Taipei City 105

Tel:+886-2172-7000 fax:+886-2528-0018

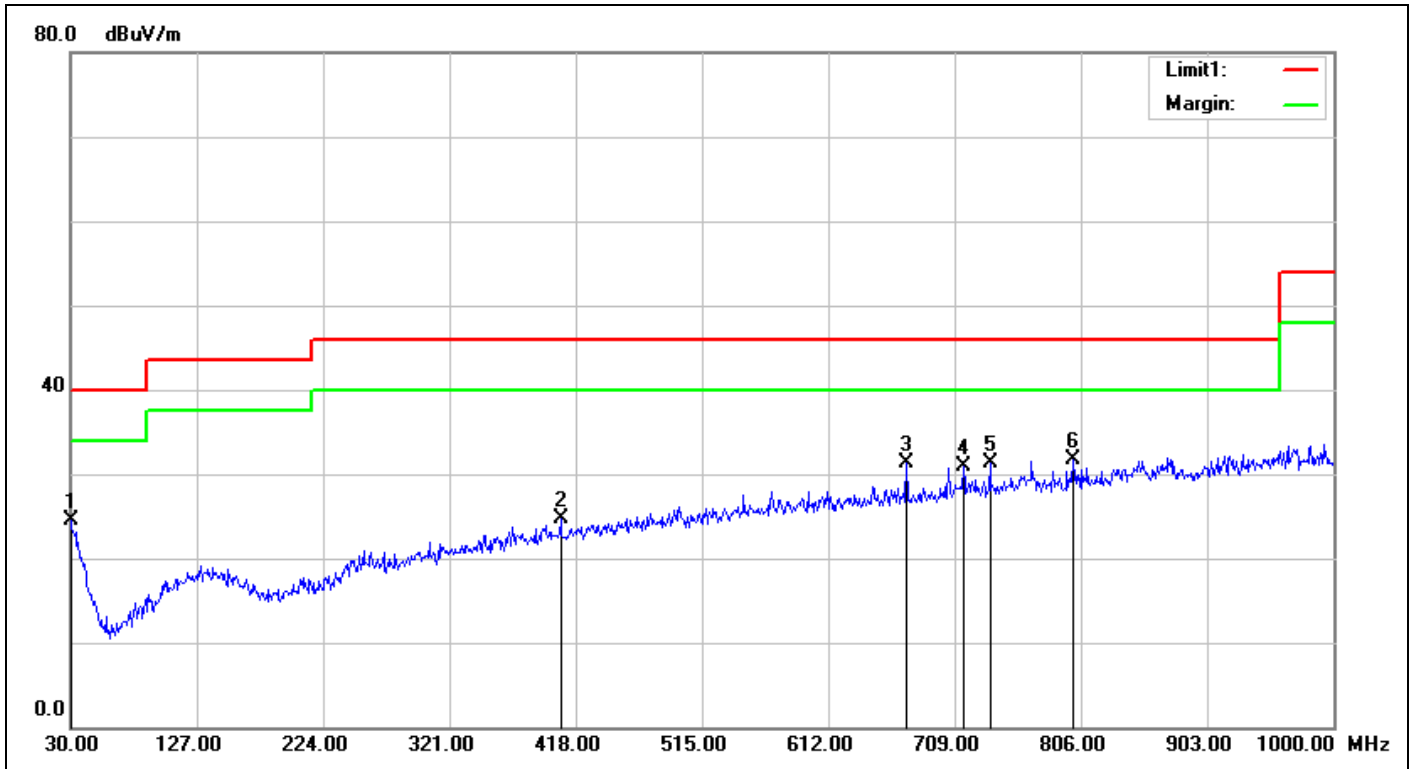

Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC Class B 3M Radiation	Ant. Polarization:	Horizontal
Test item:	Radiation Emission	Test Time:	2018/1/15 20:19:58
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2440-TX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	30.0000	-0.25	24.82	24.57	40.00	-15.43	QP	100	155	
2	406.3600	-2.37	27.06	24.69	46.00	-21.31	QP	100	309	
3	672.1400	0.85	30.46	31.31	46.00	-14.69	QP	100	75	
4	715.7900	1.62	29.27	30.89	46.00	-15.11	QP	100	158	
5	736.1600	2.06	29.30	31.36	46.00	-14.64	QP	100	248	
6	800.1799	2.77	28.89	31.66	46.00	-14.34	QP	100	272	

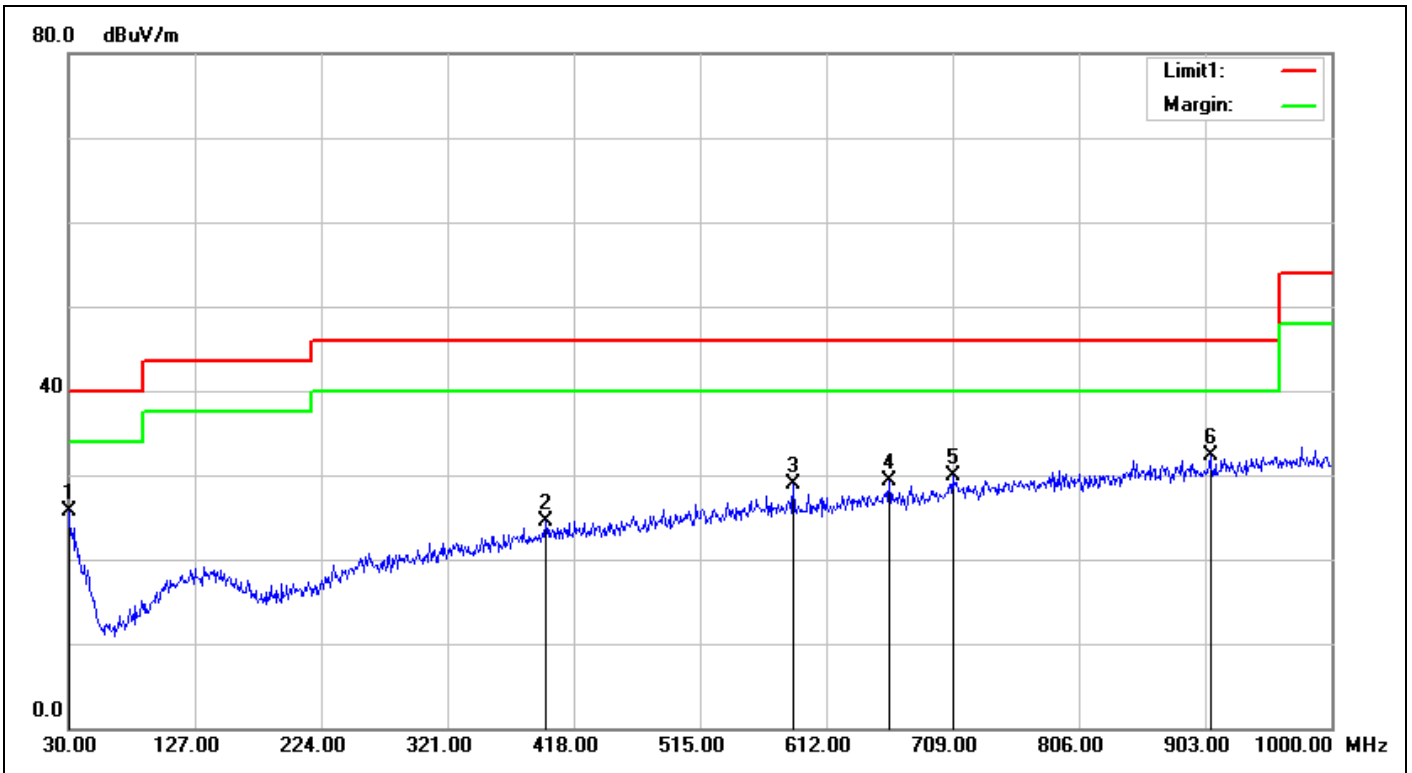

Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC Class B 3M Radiation	Ant. Polarization:	Vertical
Test item:	Radiation Emission	Test Time:	2018/1/15 20:21:02
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2440-TX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	30.0000	-0.25	25.93	25.68	40.00	-14.32	QP	100	274	
2	396.6600	-2.49	26.94	24.45	46.00	-21.55	QP	100	317	
3	586.7800	-0.06	28.92	28.86	46.00	-17.14	QP	100	346	
4	660.5000	0.69	28.52	29.21	46.00	-16.79	QP	100	131	
5	709.0000	1.47	28.49	29.96	46.00	-16.04	QP	100	11	
6	906.8800	4.26	27.99	32.25	46.00	-13.75	QP	100	0	


Spurious Emissions, TX Mode, 9k-30M



TUV Rheinland Taiwan Ltd.

11F., No.758, Sec.4 Bade Road, Songshan Dist, Taipei City 105


Tel:+886-2172-7000 fax:+886-2528-0018

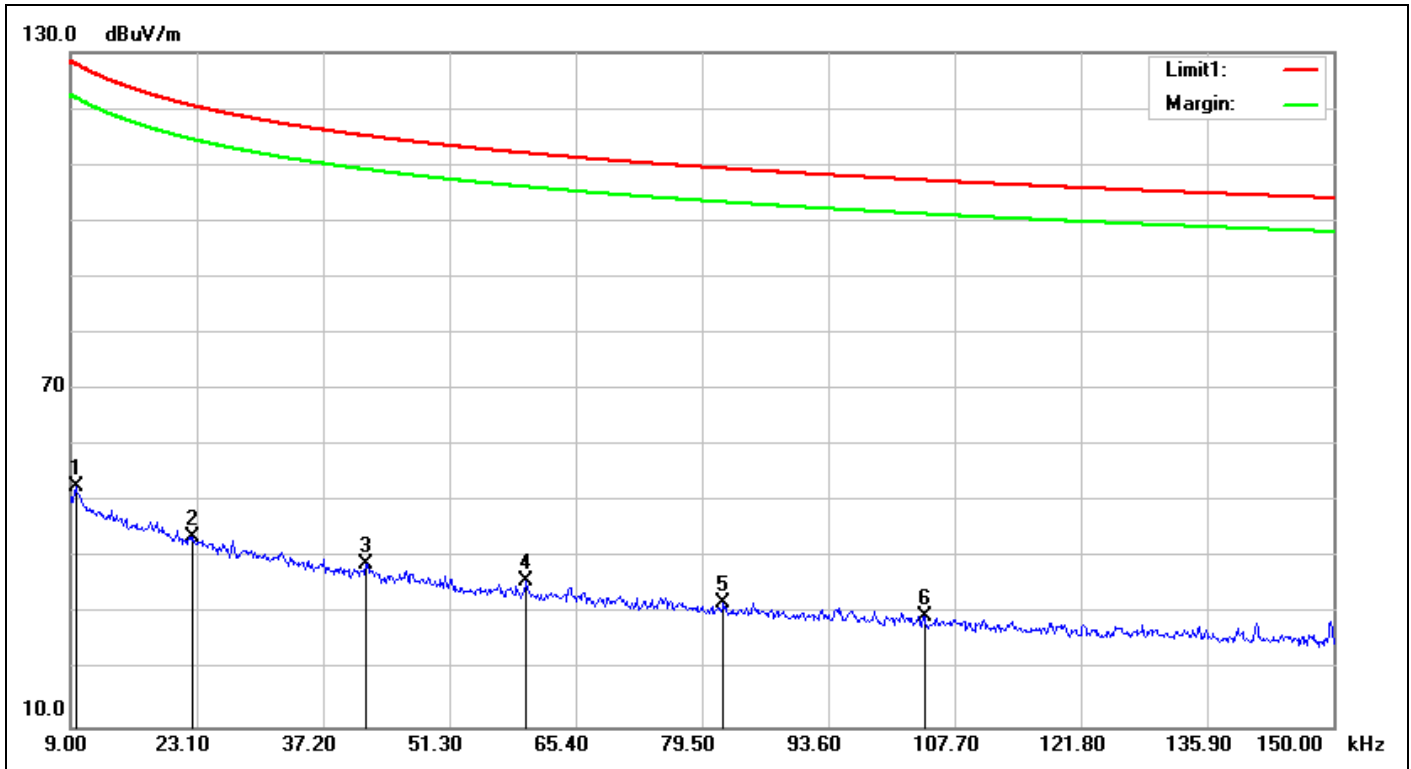

Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC2.8_9k-1G_3m	Ant. Polarization:	
Test item:	Radiation Emission	Test Time:	2018/1/15 20:43:27
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2440-TX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	0.0095	19.73	32.88	52.61	128.03	-75.42	QP	100	272	
2	0.0226	20.06	23.67	43.73	120.51	-76.78	QP	100	352	
3	0.0419	19.71	19.22	38.93	115.15	-76.22	QP	100	27	
4	0.0599	19.37	16.64	36.01	112.05	-76.04	QP	100	163	
5	0.0818	19.24	12.83	32.07	109.34	-77.27	QP	100	189	
6	0.1043	19.13	10.60	29.73	107.23	-77.50	QP	100	128	

Spurious Emissions, TX Mode, 9k-30M

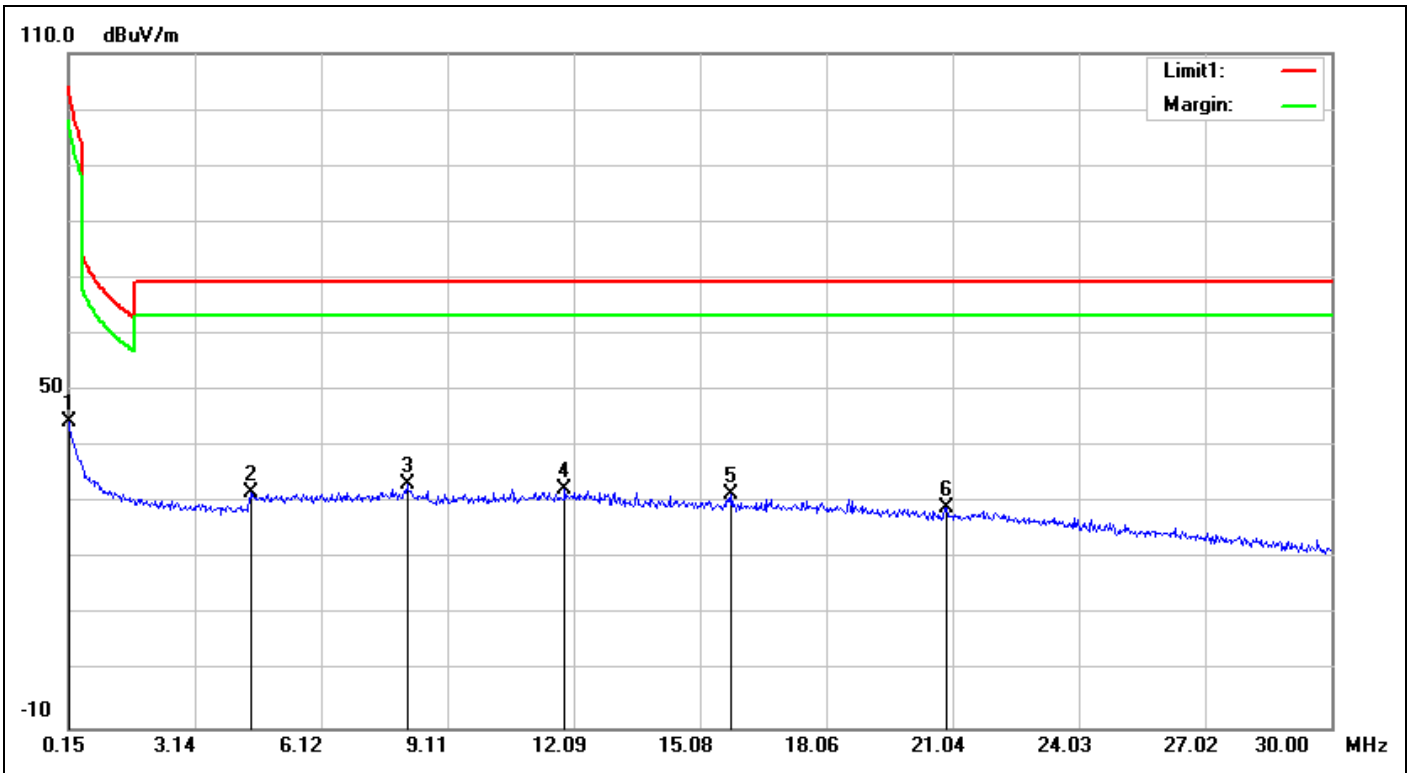


Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC2.8_9k-1G_3m	Ant. Polarization:	
Test item:	Radiation Emission	Test Time:	2018/1/15 20:49:17
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2440-TX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	0.1500	19.08	25.26	44.34	104.08	-59.74	QP	100	205	
2	4.4782	19.44	12.52	31.96	69.50	-37.54	QP	100	197	
3	8.1498	20.05	13.18	33.23	69.50	-36.27	QP	100	69	
4	11.8810	20.55	11.85	32.40	69.50	-37.10	QP	100	261	
5	15.8212	21.25	10.45	31.70	69.50	-37.80	QP	100	144	
6	20.8957	22.04	7.02	29.06	69.50	-40.44	QP	100	174	

Spurious Emissions, RX Mode, 1-18G




TUV Rheinland Taiwan Ltd.
 11F., No.758, Sec.4 Bade Road, Songshan Dist, Taipei City 105
 Tel:+886-2172-7000 fax:+886-2528-0018

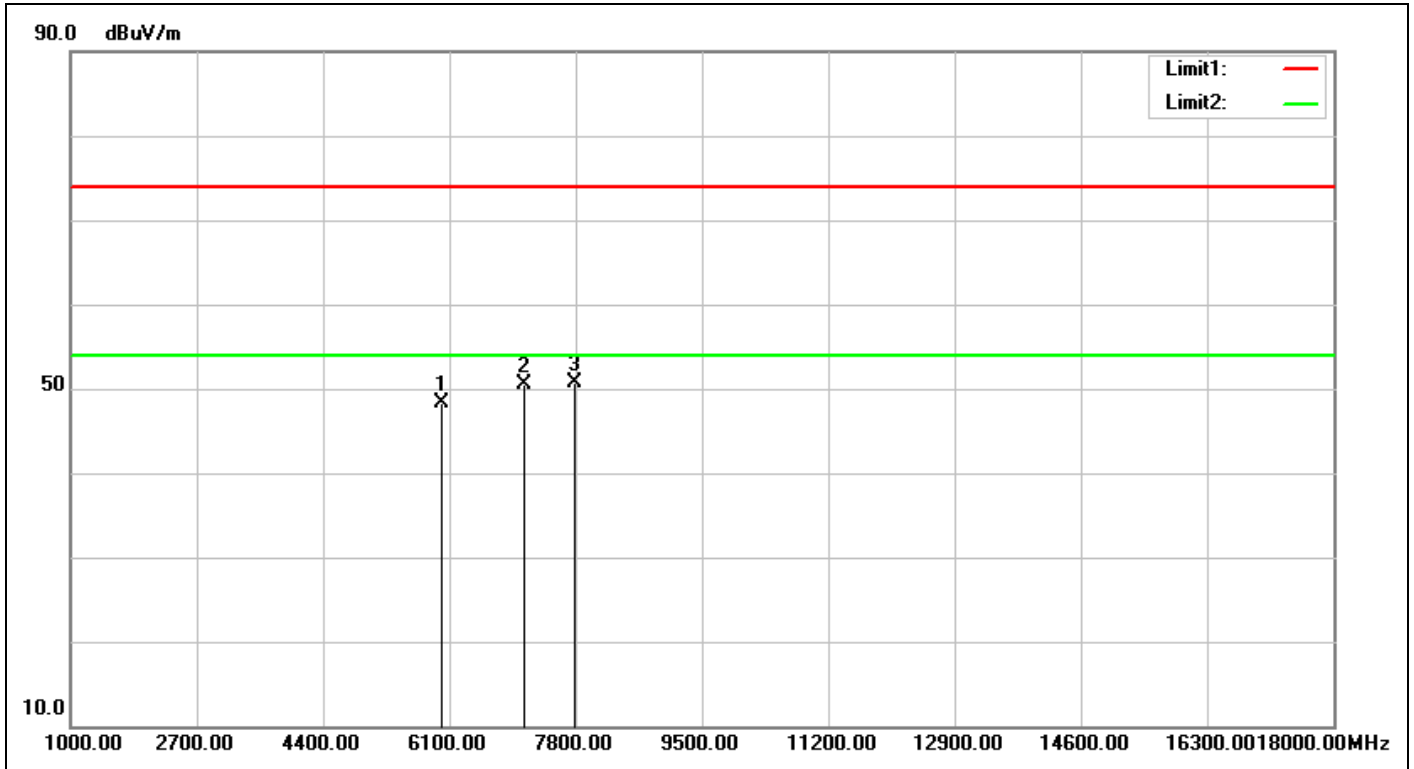

Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC Above 1G PEAK	Ant. Polarization:	Horizontal
Test item:	Radiation Emission	Test Time:	2018/1/15 17:24:05
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2440-RX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	5998.000	2.34	46.06	48.40	74.00	-25.60	peak	100	20	
2	7103.000	3.95	46.50	50.45	74.00	-23.55	peak	100	355	
3	7783.000	4.86	45.93	50.79	74.00	-23.21	peak	100	180	

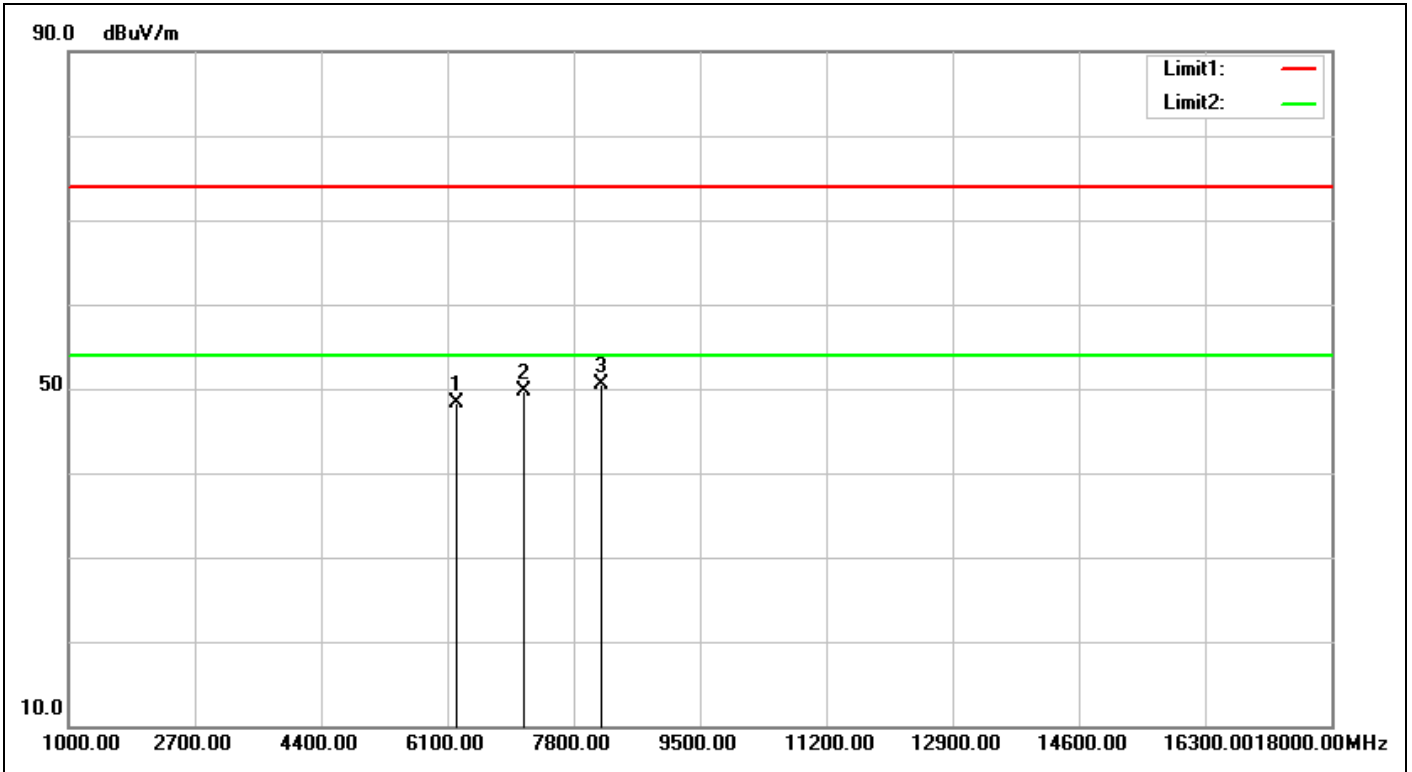


Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC Above 1G PEAK	Ant. Polarization:	Vertical
Test item:	Radiation Emission	Test Time:	2018/1/15 17:25:08
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2440-RX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	6219.000	3.22	45.13	48.35	74.00	-25.65	peak	100	5	
2	7120.000	3.99	45.81	49.80	74.00	-24.20	peak	100	307	
3	8174.000	4.98	45.48	50.46	74.00	-23.54	peak	100	360	

Spurious Emissions, RX Mode, 18-26G




TUV Rheinland Taiwan Ltd.
 11F., No.758, Sec.4 Bade Road. Songshan Dist, Taipei City 105
 Tel:+886-2172-7000 fax:+886-2528-0018

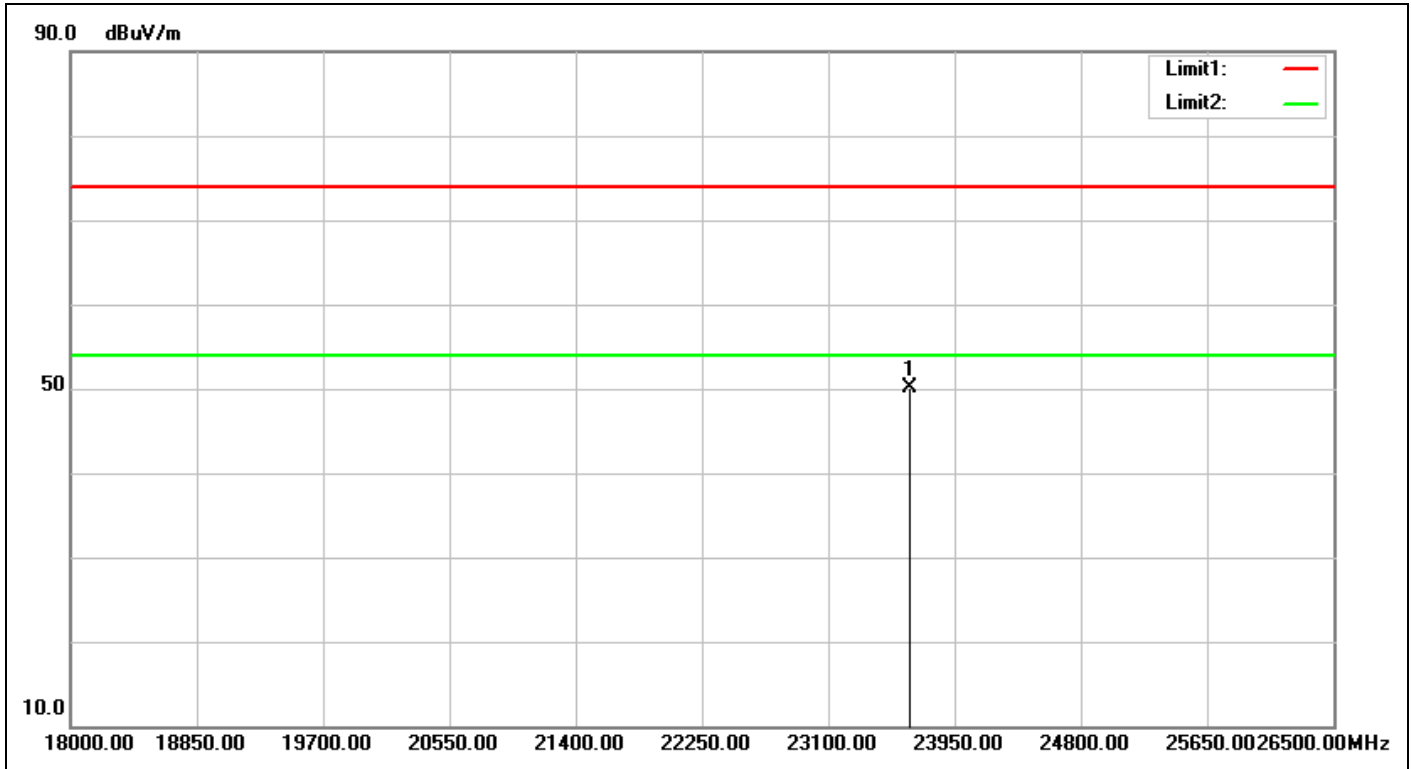

Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC Above 1G PEAK	Ant. Polarization:	Horizontal
Test item:	Radiation Emission	Test Time:	2018/1/15 19:01:07
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2440-RX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	23652.500	32.71	17.42	50.13	74.00	-23.87	peak		0	

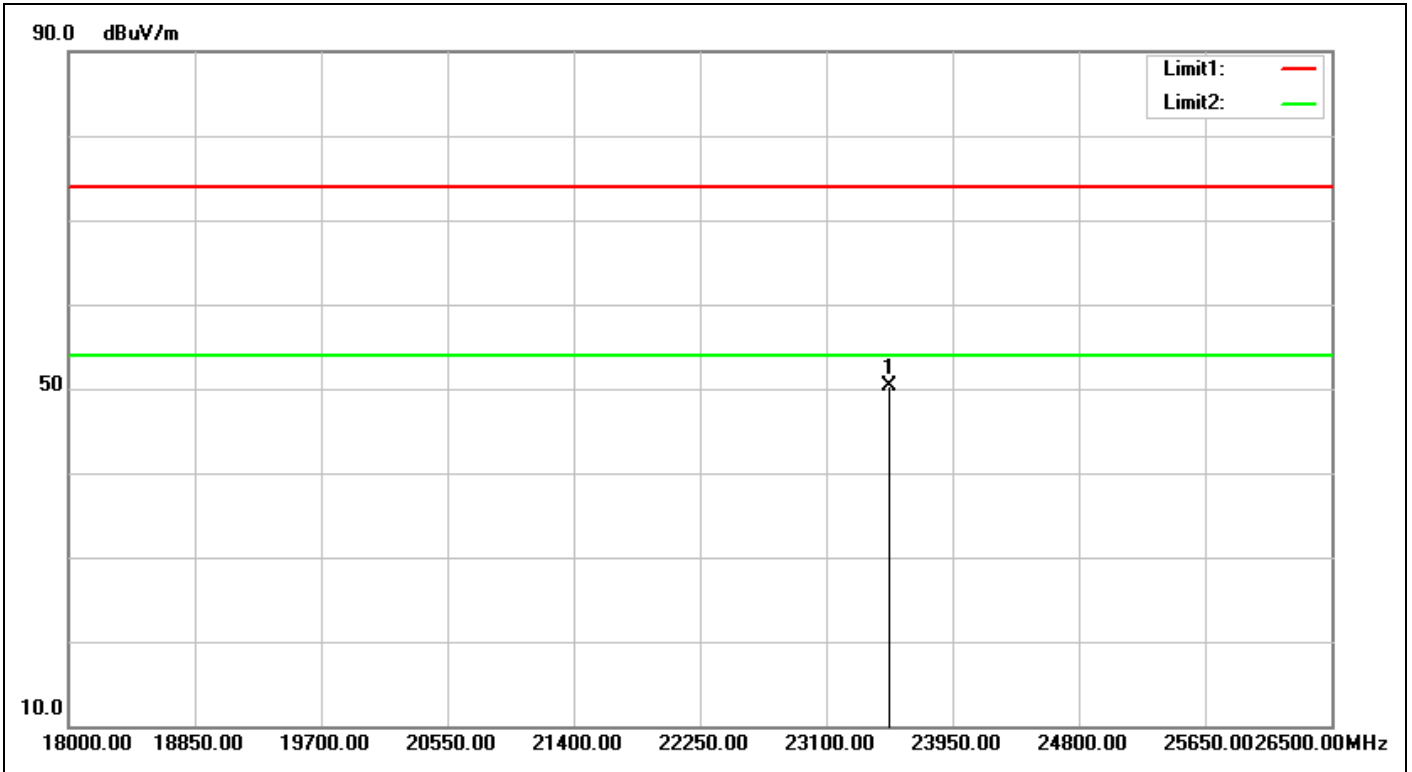

Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC Above 1G PEAK	Ant. Polarization:	Vertical
Test item:	Radiation Emission	Test Time:	2018/1/15 19:01:29
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2440-RX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	23525.000	32.81	17.56	50.37	74.00	-23.63	peak			


Spurious Emissions, RX Mode, 30M-1G



TUV Rheinland Taiwan Ltd.


11F., No.758, Sec.4 Bade Road, Songshan Dist, Taipei City 105

Tel:+886-2172-7000 fax:+886-2528-0018

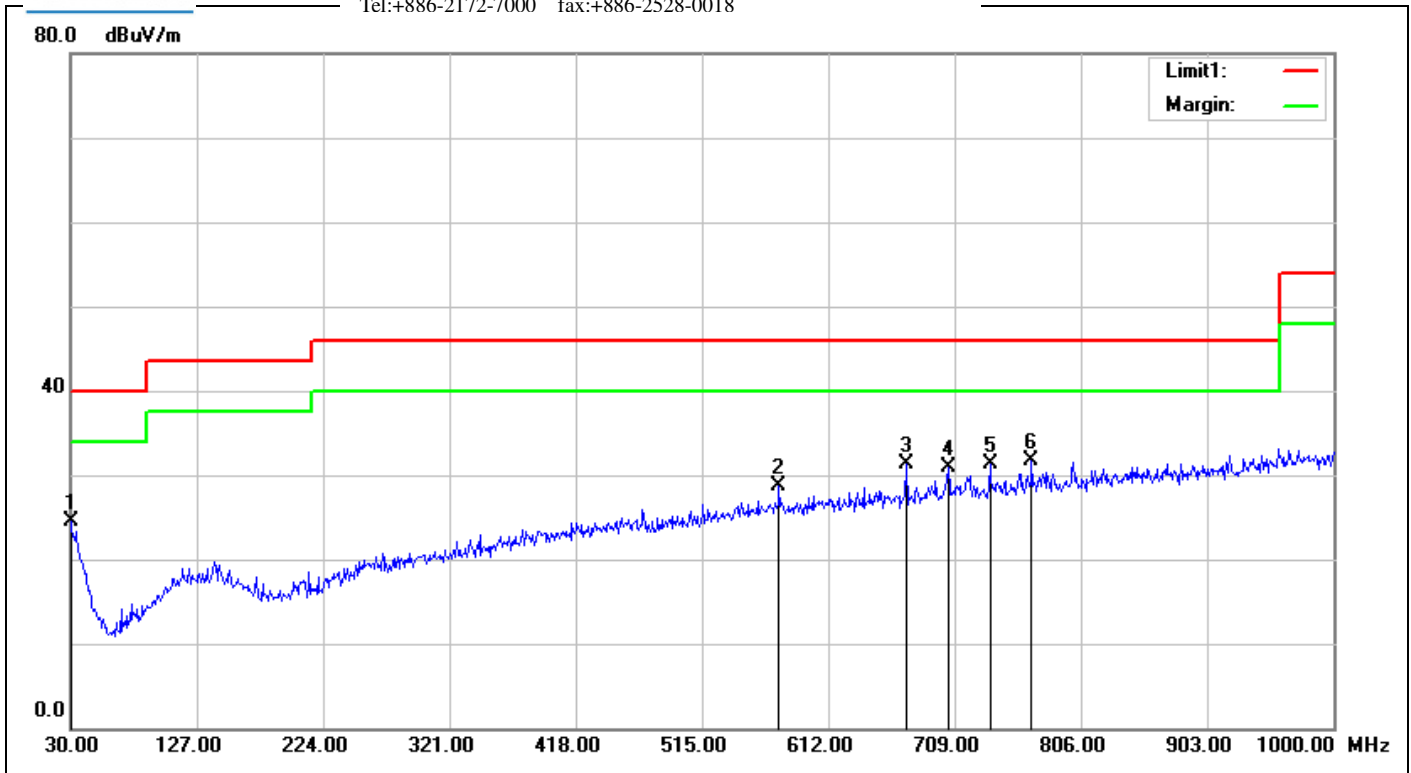

Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC Class B 3M Radiation	Ant. Polarization:	Horizontal
Test item:	Radiation Emission	Test Time:	2018/1/15 20:24:29
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2440-RX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	30.0000	-0.25	24.80	24.55	40.00	-15.45	QP	100	313	
2	574.1700	-0.20	28.85	28.65	46.00	-17.35	QP	100	276	
3	672.1400	0.85	30.50	31.35	46.00	-14.65	QP	100	219	
4	704.1500	1.35	29.46	30.81	46.00	-15.19	QP	100	59	
5	736.1600	2.06	29.29	31.35	46.00	-14.65	QP	100	53	
6	768.1700	2.51	29.24	31.75	46.00	-14.25	QP	100	240	

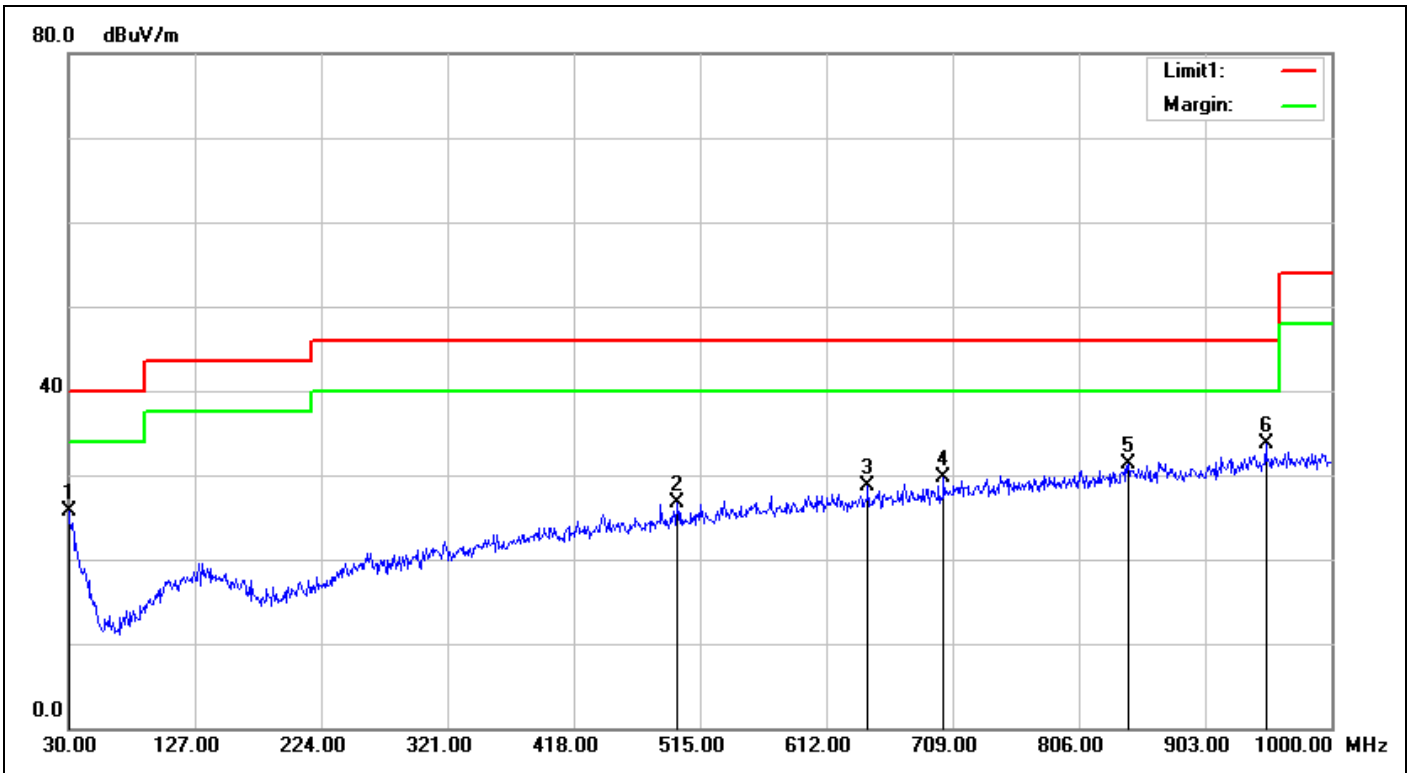

Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC Class B 3M Radiation	Ant. Polarization:	Vertical
Test item:	Radiation Emission	Test Time:	2018/1/15 20:25:32
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2440-RX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	30.0000	-0.25	25.95	25.70	40.00	-14.30	QP	100	157	
2	497.5400	-1.21	27.94	26.73	46.00	-19.27	QP	100	99	
3	644.0100	0.47	28.21	28.68	46.00	-17.32	QP	100	184	
4	702.2100	1.31	28.43	29.74	46.00	-16.26	QP	100	216	
5	843.8300	3.60	27.65	31.25	46.00	-14.75	QP	100	115	
6	949.5600	5.48	28.30	33.78	46.00	-12.22	QP	100	266	


Spurious Emissions, RX Mode, 9K-30M



TUV Rheinland Taiwan Ltd.


11F., No.758, Sec.4 Bade Road. Songshan Dist, Taipei City 105

Tel:+886-2172-000 fax:+886-2528-0018

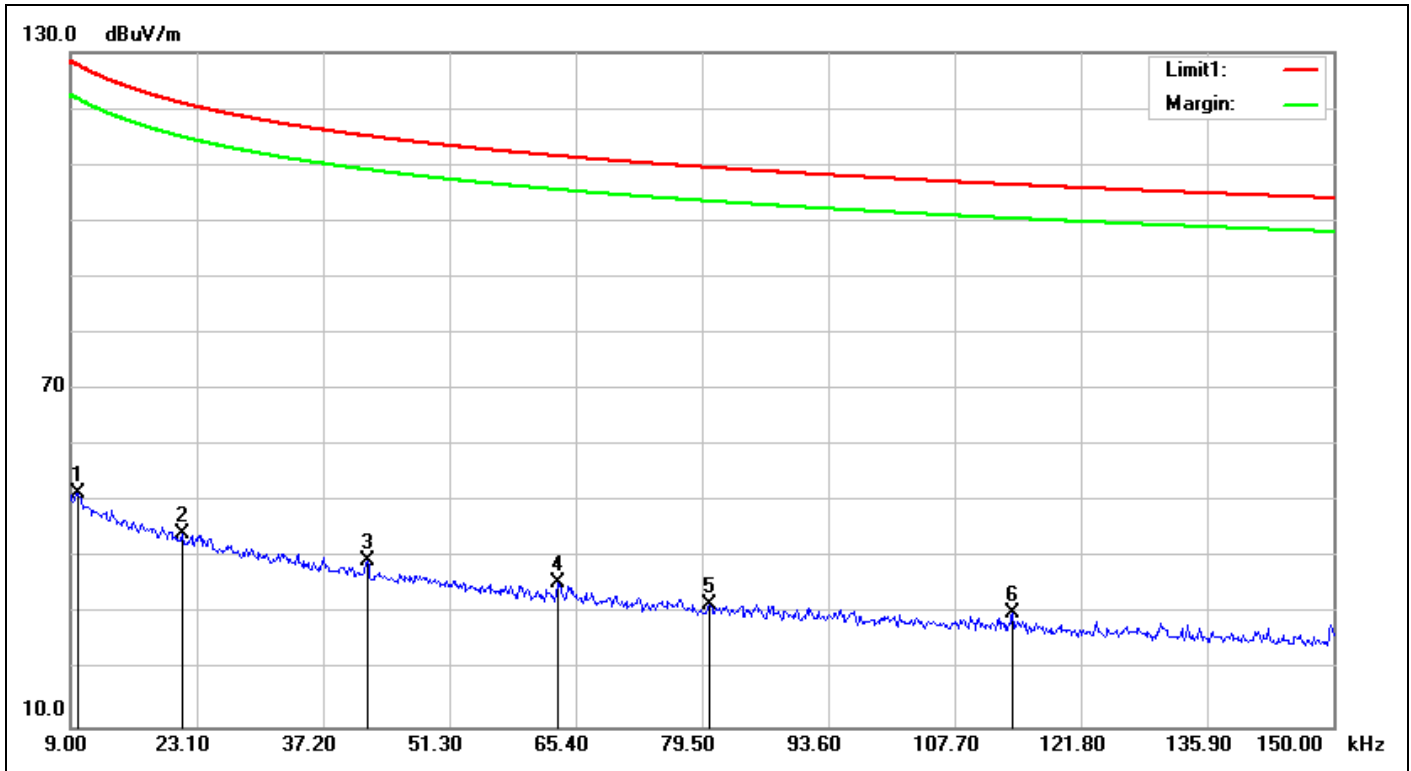

Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC2.8_9k-1G_3m	Ant. Polarization:	
Test item:	Radiation Emission	Test Time:	2018/1/15 20:44:30
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2440-RX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	0.0098	19.85	31.85	51.70	127.76	-76.06	QP	100	200	
2	0.0215	20.05	24.24	44.29	120.94	-76.65	QP	100	258	
3	0.0421	19.71	19.93	39.64	115.11	-75.47	QP	100	260	
4	0.0634	19.35	16.33	35.68	111.55	-75.87	QP	100	189	
5	0.0803	19.25	12.54	31.79	109.50	-77.71	QP	100	136	
6	0.1142	19.12	11.01	30.13	106.44	-76.31	QP	100	356	

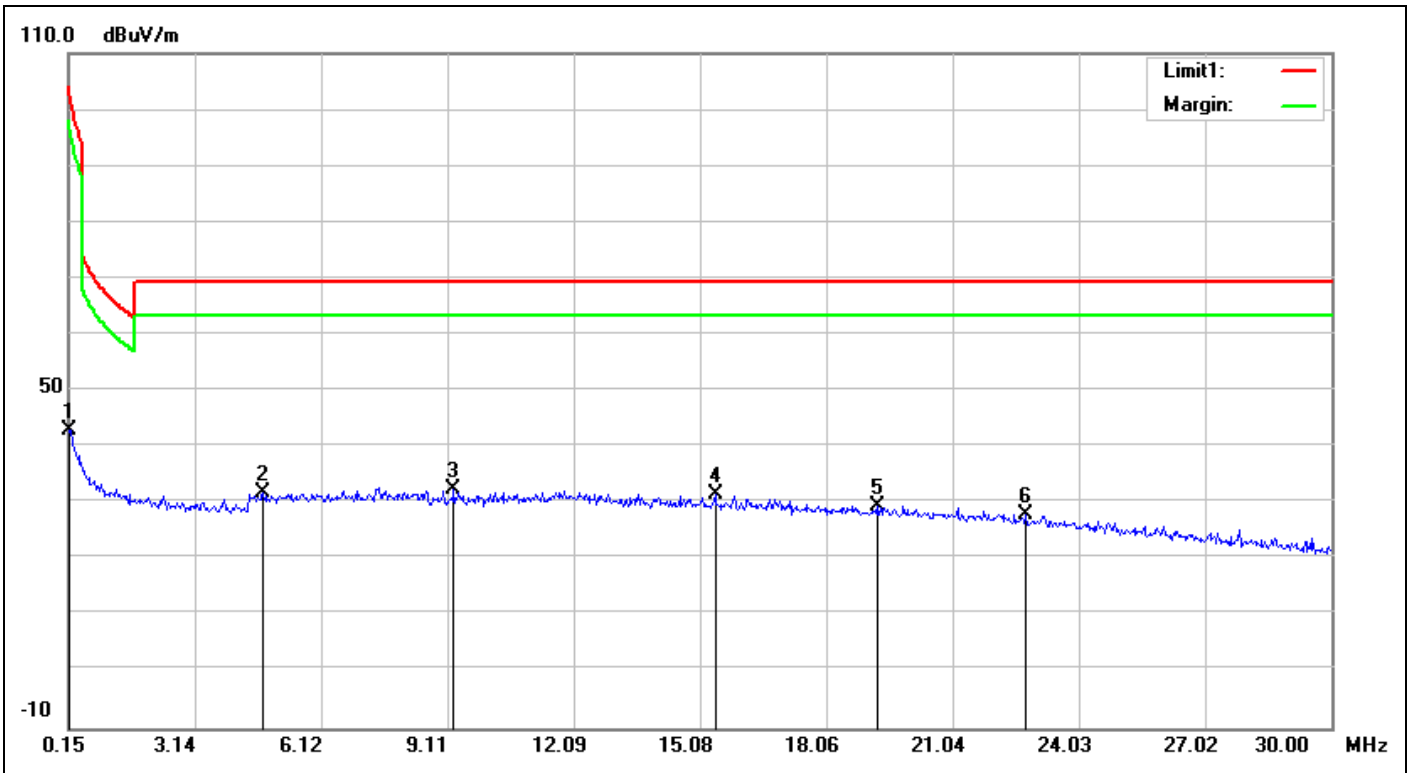

Service No.:	114072368	Test Distance:	3m
Test Standard:	NCC2.8_9k-1G_3m	Ant. Polarization:	
Test item:	Radiation Emission	Test Time:	2018/1/15 20:50:21
Applicant:	General Life Biotechnology Co., Ltd.	Test Rating:	DC 3V
Product:	BeneCheck Supreme Multi-Monitoring System	Temp.(°C)/Hum.(%):	22(°C)/65%
Model No.:	SEE REPORT NO: 50121721 APPENDIX I	Test Engineer:	Curry Chen
Test Mode:	2440-RX		
Remark:			

No.	Frequency (MHz)	Factor (dB/m)	Reading (dBuV)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Det.	Height (cm)	Azimuth (°)	Remark
1	0.1500	19.08	23.95	43.03	104.08	-61.05	QP	100	104	
2	4.7469	19.60	12.19	31.79	69.50	-37.71	QP	100	115	
3	9.2543	20.15	12.24	32.39	69.50	-37.11	QP	100	194	
4	15.4332	21.18	10.48	31.66	69.50	-37.84	QP	100	97	
5	19.2540	21.85	7.72	29.57	69.50	-39.93	QP	100	192	
6	22.7763	22.17	5.73	27.90	69.50	-41.60	QP	100	91	