

Appendix D

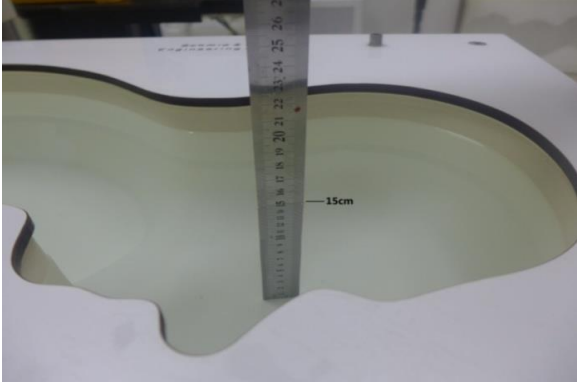
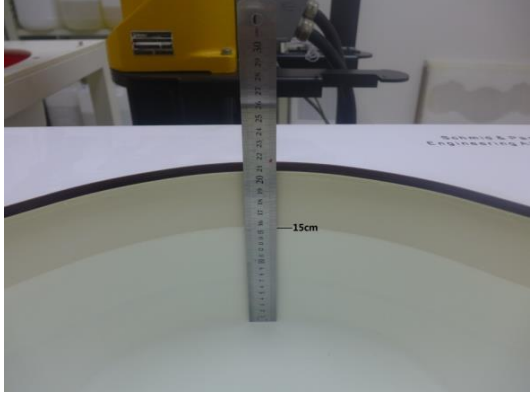
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

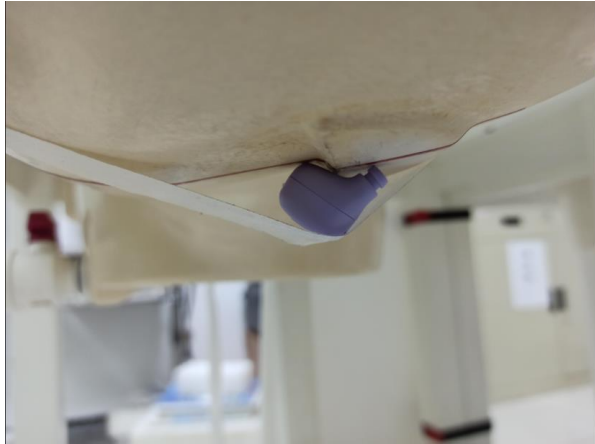
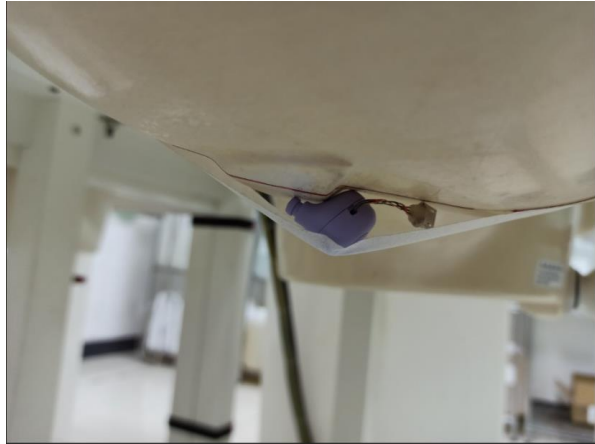
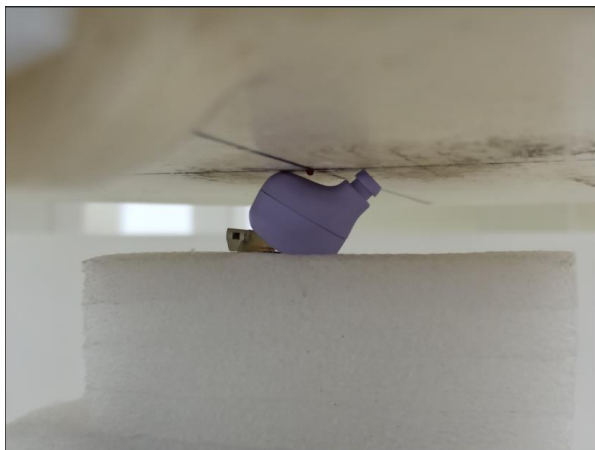



1. SAR measurement System



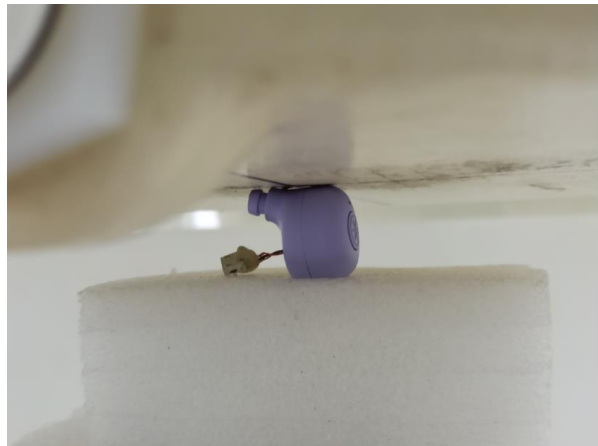
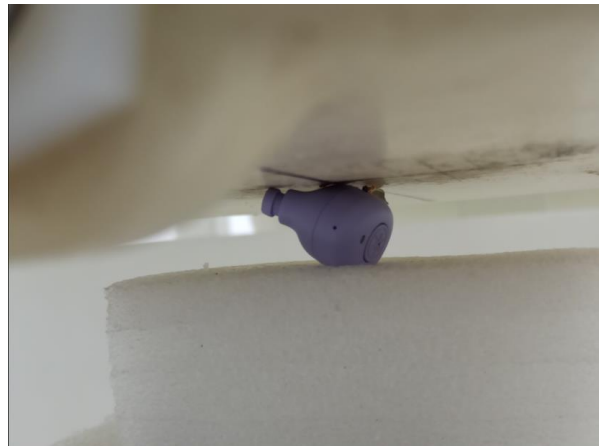


2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 2450	Photo 2: Tissue Simulant Liquid for Head 2450
	

3. Photographs of EUT test position

<p>Photo 3: Left cheek 0mm</p>	<p>Photo 4: Right cheek 0mm</p>
	
<p>Photo 5: Side 1 0mm</p>	<p>Photo 6: Side 2 0mm</p>
	
<p>Photo 7: Side 3 0mm</p>	<p>Photo 8: Side 4 0mm</p>
	

<p>Photo 9: Side 5 0mm</p>	<p>Photo 10: Side 6 0mm</p>
 A close-up photograph of a purple electronic component mounted on a white foam block. The component has a small yellow component attached to its side. The background is a light-colored surface.	 A close-up photograph of the same purple electronic component from a different angle. The yellow component is more visible, and the component is mounted on the same white foam block.
<p>Photo 11: Side 7 0mm</p>	<p>Photo 12: Side 8 0mm</p>
 A close-up photograph of the purple electronic component from another angle. The yellow component is clearly visible on the side of the component, which is mounted on the white foam block.	 A close-up photograph of the purple electronic component from a final angle. The component is mounted on the white foam block, and the yellow component is visible on its side.

4. EUT Constructional Details

