



849 NW State Road 45
Newberry, FL 32669 USA
Ph.: 888.472.2424 or
352.472.5500
Fax: 352.472.2030
Email: info@timcoengr.com
Website: www.timcoengr.com

FCC PART 15.249 & IC RSS-210 UNLICENSED INTENTIONAL RADIATOR TEST REPORT

Applicant	IRADIMED CORPORATION
Address	1025 WILLA SPRINGS DRIVE
	WINTER SPRINGS FL 32708
FCC ID	2AKRU-IRM01
IC	22312-IRM01
Model Number	3881
Product Description	MRI WIRELESS ECG ePOD
Date Sample Received	12/8/2016
Final Test Date	03/10/2017
Tested By	Tim Royer
Approved By	Cory Leverett

Report Number	Version Number	Description	Issue Date
2449AUT16TestReport_	Rev1	Initial Issue	01/16/2017
2449AUT16TestReport_	Rev1	Added Bandedge plots pg 11 - 13	03/10/2017

**THE ATTACHED REPORT SHALL NOT BE REPRODUCED EXCEPT IN FULL
WITHOUT THE WRITTEN APPROVAL OF TIMCO ENGINEERING, INC.**

TABLE OF CONTENTS

GENERAL INFORMATION	4
EUT Specification	4
Test Supporting Equipment	4
RESULTS SUMMARY	5
OCCUPIED BANDWIDTH	6
Test Data: Measurement Table.....	6
Test Data: Low end of Band Plot.....	7
Test Data: Middle of Band Plot	8
Test Data: High end of Band Plot	9
BANDEDGE	10
Test Data: Measurement Table.....	10
Test Data: Low end of Band Peak Plot	11
Test Data: Low end of Band Average Plot	12
Test Data: Upper end of Band Peak Plot	13
Test Data: Upper end of Band Average Plot	14
RADIATED SPURIOUS EMISSIONS	15
Test Data: Measurement Table.....	17
EMC EQUIPMENT LIST	18

GENERAL REMARKS

The attached report shall not be reproduced except in full without the written permission of Timco Engineering Inc.

Summary

The device under test does:

- ☒ Fulfill the general approval requirements as identified in this test report and was selected by the customer.
- ☐ Not fulfill the general approval requirements as identified in this test report

Attestations

This equipment has been tested in accordance with the standards identified in this test report. To the best of my knowledge and belief, these tests were performed using the measurement procedures described in this report.

All instrumentation and accessories used to test products for compliance to the indicated standards are calibrated regularly in accordance with ISO 17025 requirements.

I attest that the necessary measurements were made at:

Timco Engineering Inc.
849 NW State Road 45
Newberry, FL 32669



Tested by:

Name and Title: **Tim Royer**, Project Manager/Testing Engineer

Date: 03/ 10/ 2017



Reviewed and approved by:

Name and Title: Cory Leverett, Engineering Project Manager

Date: 03/ 10/ 2017

Applicant: IRADIMED CORPORATION
FCC ID: 2AKRU-IRM01
IC: 22312-IRM01
Report: 2449AUT16TestReport_Rev1

[Table of Contents](#)

GENERAL INFORMATION

EUT Specification

Regulatory Standards	FCC Title 47 CFR Part 15.249 IC RSS-210 Issue 8 A2.9 & RSS-GEN Issue 4		
FCC ID	2AKRU-IRM01		
IC	22312-IRM01		
Model	3881		
EUT Description	MRI WIRELESS ECG ePOD		
Modulation Type	GFSK		
Operating Frequency	TX: 2404 – 2434 MHz	RX: 2404 – 2434 MHz	
EUT Power Source	☐ 110–120Vac/50– 60Hz		
	☐ DC Power		
	☒ Battery Operated Exclusively 3.7 VDC		
Test Item	☐ Prototype	☐ Pre-Production	☒ Production
Type of Equipment	☐ Fixed	☐ Mobile	☒ Portable
Antenna Connector	None		
Antenna	Integral		
Test Conditions	Temperature: 24-26°C Relative humidity: 50-65%		
Measurement Standard	ANSI C63.10-2013 ANSI C63.4-2014 (Radiated Site Validation)		

Test Supporting Equipment

Device	Manufacturer	Model	S/ N	Supplied By	Used For
N/A					

RESULTS SUMMARY

FCC Rule Part No.	IC Standard Ref.	Requirement	Test Item	Result
2.1049	RSS-GEN 6.6	Occupied Bandwidth	99% Bandwidth	Pass
15.249(a)(c)	RSS-210 § A2.9(a)	Fundamental and Harmonics	Radiated Spurious Emissions	Pass
15.249(d)(e)	RSS-247 § 5.5	Spurious Emissions	Bandedge	Pass
			Radiated Spurious Emissions	Pass

Notes: none

OCCUPIED BANDWIDTH


Rules Part No.: FCC 2.1049, IC RSS GEN § 6.6

FCC Requirements: Reporting only

IC Requirements: Reporting Only

Test Method: THE TEST PROCEDURES USED ARE DETAILED IN THE STANDARD LISTED ABOVE.

Setup:

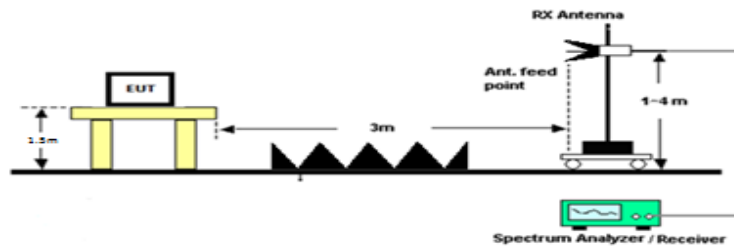


Test Data: Measurement Table

Tuned Frequency (MHz)	99% BW (KHz)
2404	861.4
2412	867.0
2434	867.0

RESULTS:

OCCUPIED BANDWIDTH

Test Data: Low end of Band Plot

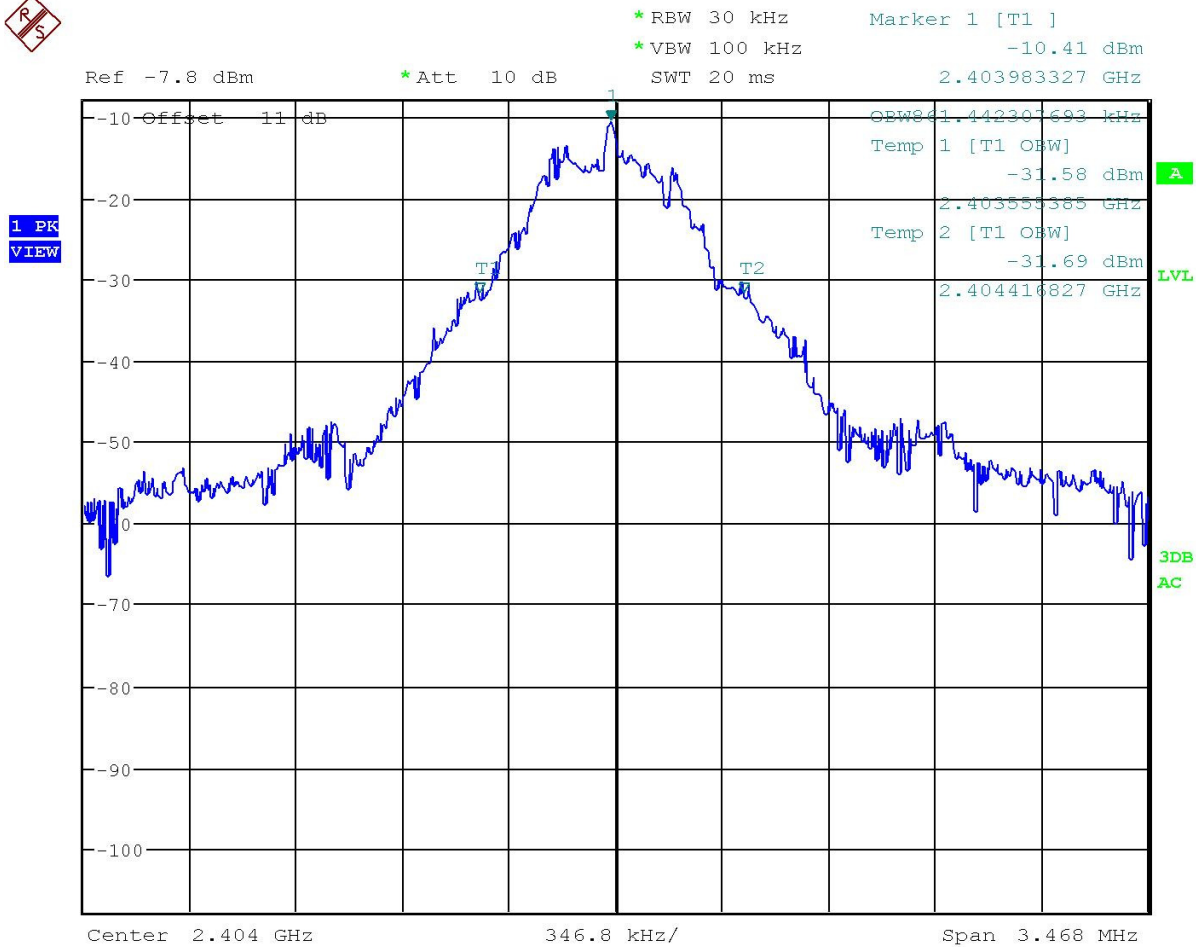

Date: 16.JAN.2017 11:36:10

RESULTS: Meets Requirements

Applicant: IRADIMED CORPORATION
 FCC ID: 2AKRU-IRM01
 IC: 22312-IRM01
 Report: 2449AUT16TestReport_Rev1

[Table of Contents](#)

OCCUPIED BANDWIDTH

Test Data: Middle of Band Plot



* RBW 30 kHz
* VBW 100 kHz
SWT 20 ms
Marker 1 [T1]
-18.70 dBm
2.411983327 GHz


Ref -7.8 dBm

* Att 10 dB

SWT 20 ms

2.411983327 GHz

1 PK
VIEW

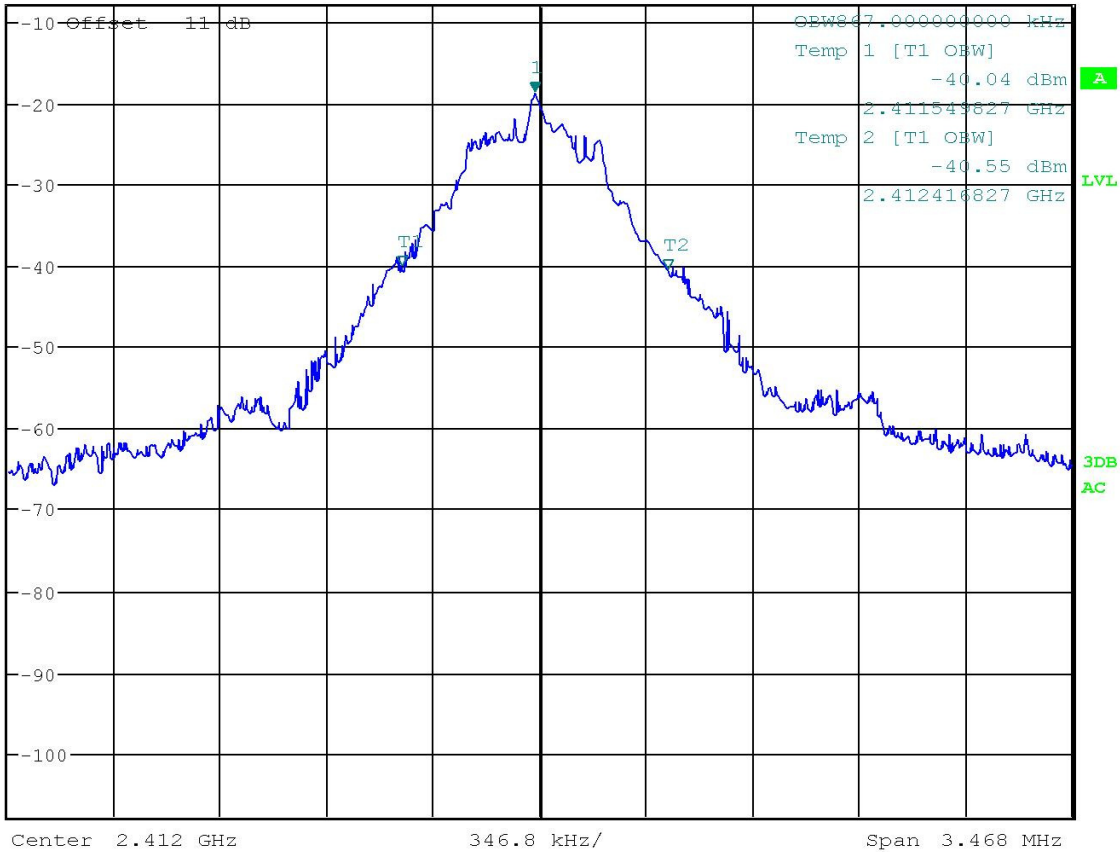

Date: 16.JAN.2017 14:14:01


RESULTS: Meets Requirements

Applicant: IRADIMED CORPORATION
FCC ID: 2AKRU-IRM01
IC: 22312-IRM01
Report: 2449AUT16TestReport_Rev1

[Table of Contents](#)

OCCUPIED BANDWIDTH

Test Data: High end of Band Plot

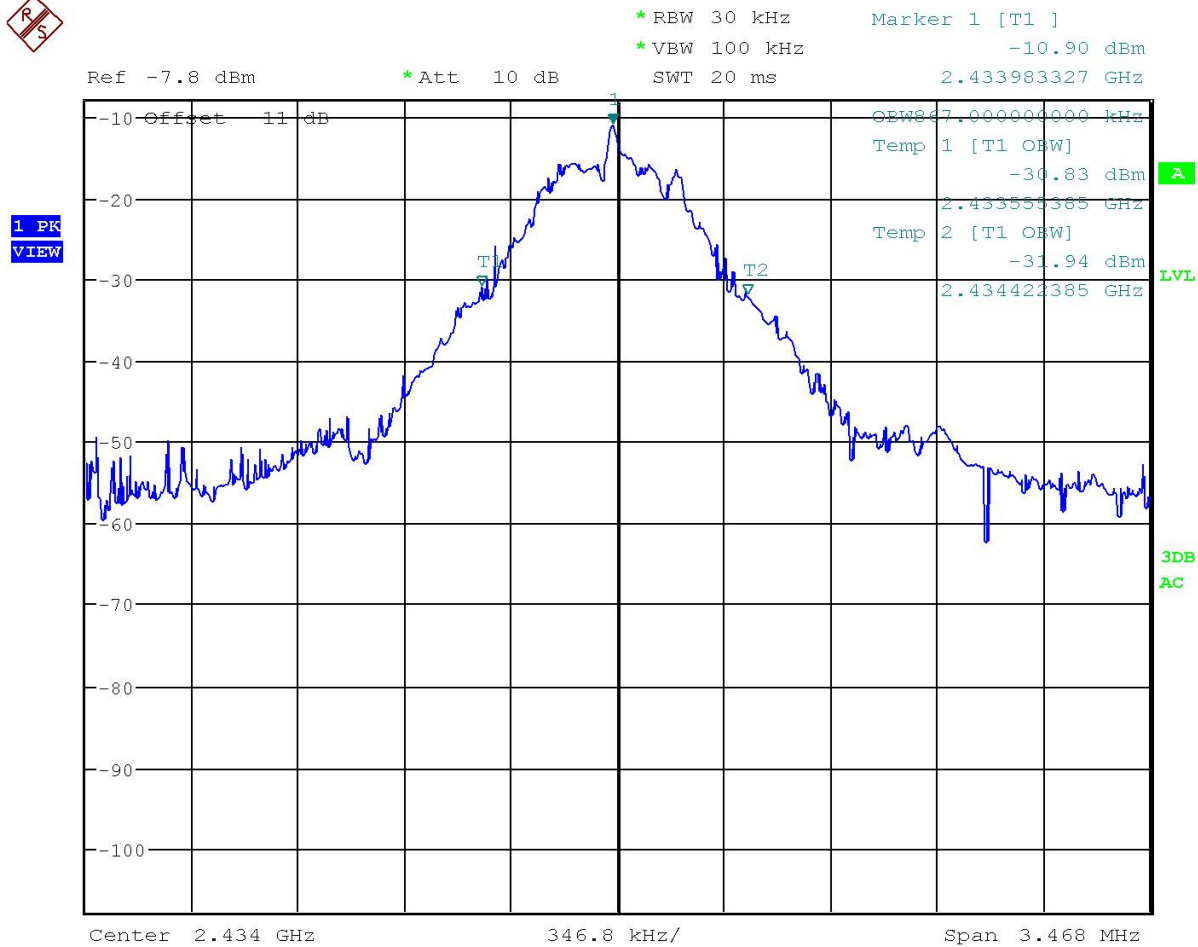

Date: 16.JAN.2017 11:33:48

RESULTS: Meets Requirements


BANDEDGE

Rule Part No.: FCC 15.249(d), IC RSS 210 § A2.9(b)

Requirements: Emissions must be at least 50 dB down from the highest emission level Within the authorized band as measured with a 100 kHz RBW, or to the limits of 15.209.

Test Method: THE TEST PROCEDURES USED ARE DETAILED IN THE STANDARD LISTED ABOVE.

Setup:

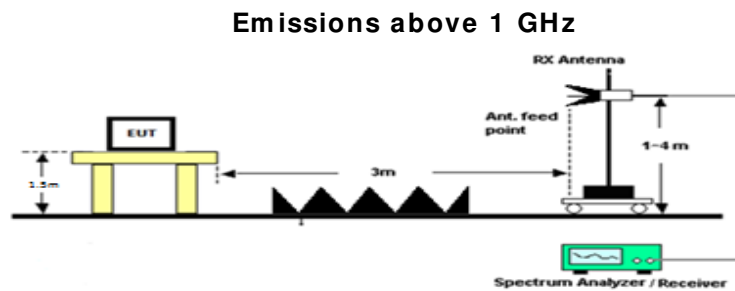

Test Data: Bandedge Measurement Table


Tuned Frequency (MHz)	Emission Frequency (MHz)	Detector (PK/AV)	Read Level (dBuV)	Polarity	Coax Loss (dB)	ACF (dB)	Field Strength (dBuV/M)	Limit (dBuV/M)	Margin (dB)
2404	2399.73	Peak	19.00	V	5.69	31.89	56.58	74	17.48
2404	2399.73	Average	1.75	V	5.69	31.89	39.33	54	14.67
2434	2484.30	Peak	14.69	V	5.78	32.67	53.14	74	20.86
2434	2484.30	Average	1.53	V	5.78	32.67	39.98	54	14.02

Results Meet Requirements

BANDEDGE

Test Data: Lower Bandedge Peak Plot


 Ref Lvl 72 dBμV
 Marker 1 [T1] 19.00 dBμV
 2.39973146 GHz
 RBW 1 MHz
 VBW 3 MHz
 SWT 5 ms
 RF Att 0 dB
 Unit dBμV

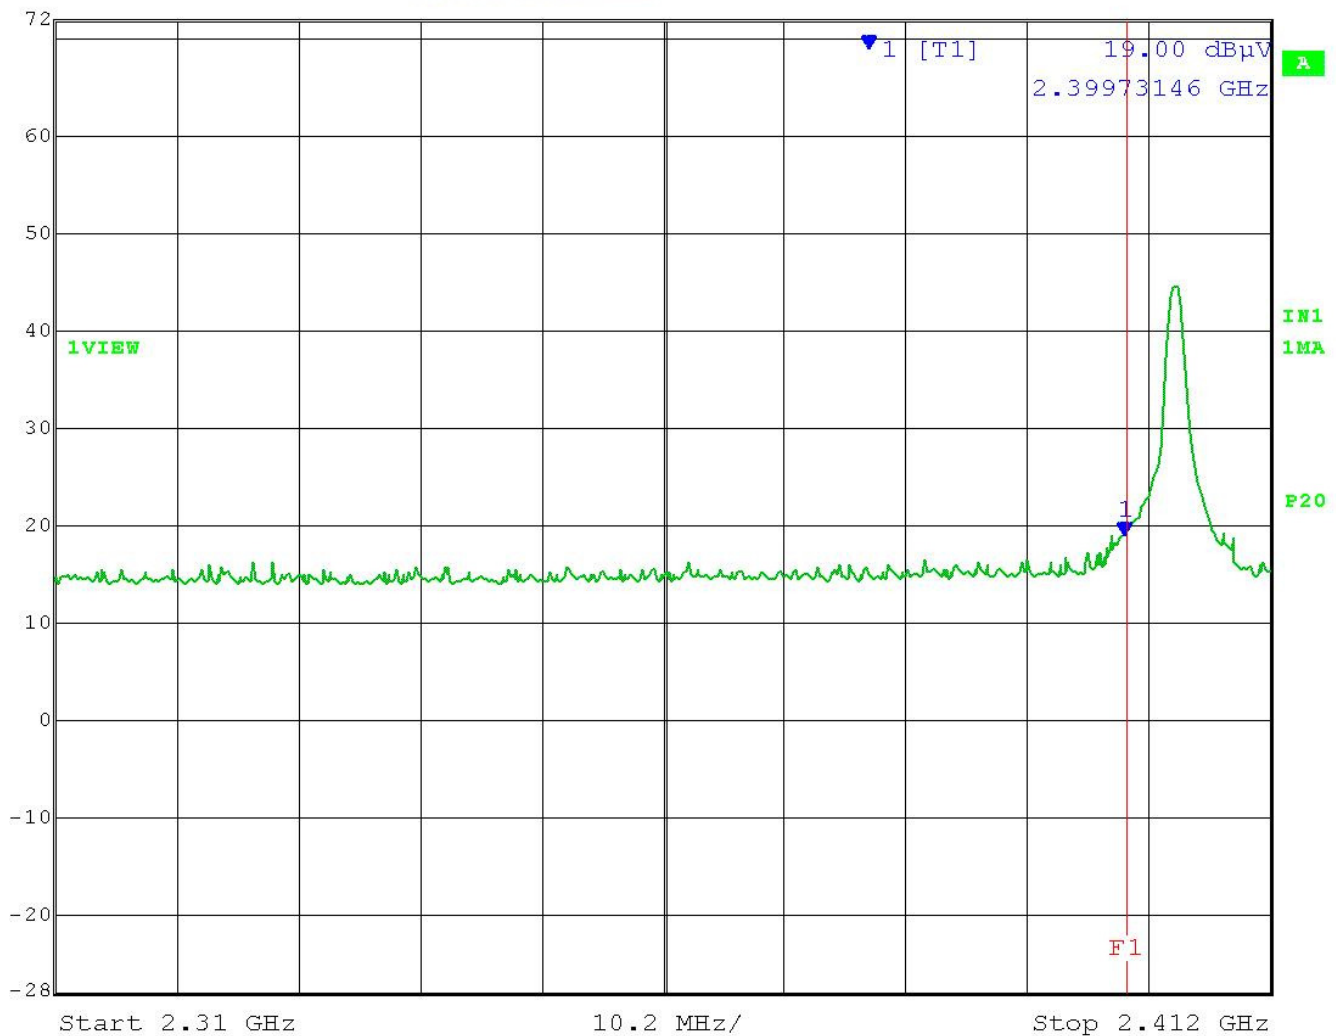

Date: 10.MAR.2017 10:24:38

RESULTS: Meets Requirements

Applicant: IRADIMED CORPORATION
 FCC ID: 2AKRU-IRM01
 IC: 22312-IRM01
 Report: 2449AUT16TestReport_Rev1


[Table of Contents](#)

BANDEDGE

Test Data: Lower Bandedge Average Plot



Ref Lvl	Marker 1 [T1]	RBW	1 MHz	RF Att	0 dB
72 dBμV	1.75 dBμV	VBW	10 Hz		
	2.39973146 GHz	SWT	5.6 s	Unit	dBμV

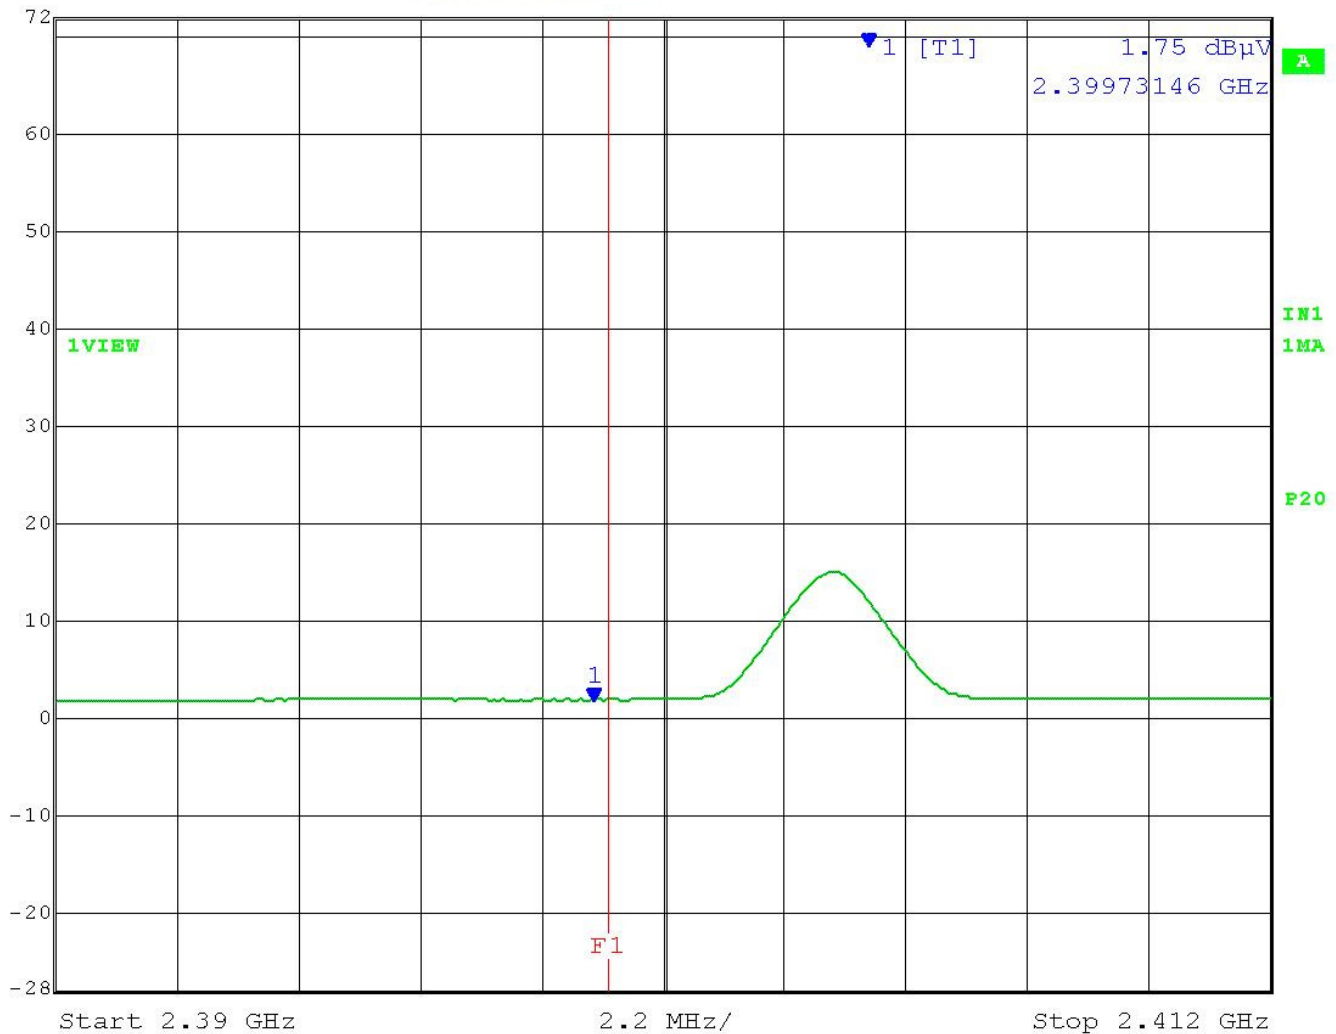

Date: 10.MAR.2017 10:26:11

RESULTS: Meets Requirements

Applicant: IRADIMED CORPORATION
 FCC ID: 2AKRU-IRM01
 IC: 22312-IRM01
 Report: 2449AUT16TestReport_Rev1


[Table of Contents](#)

BANDEDGE

Test Data: Upper Bandedge Peak Plot



Marker 1 [T1] RBW 1 MHz RF Att 0 dB
 Ref Lvl 14.69 dBμV VBW 3 MHz
 72 dBμV 2.48431810 GHz SWT 5 ms Unit dBμV

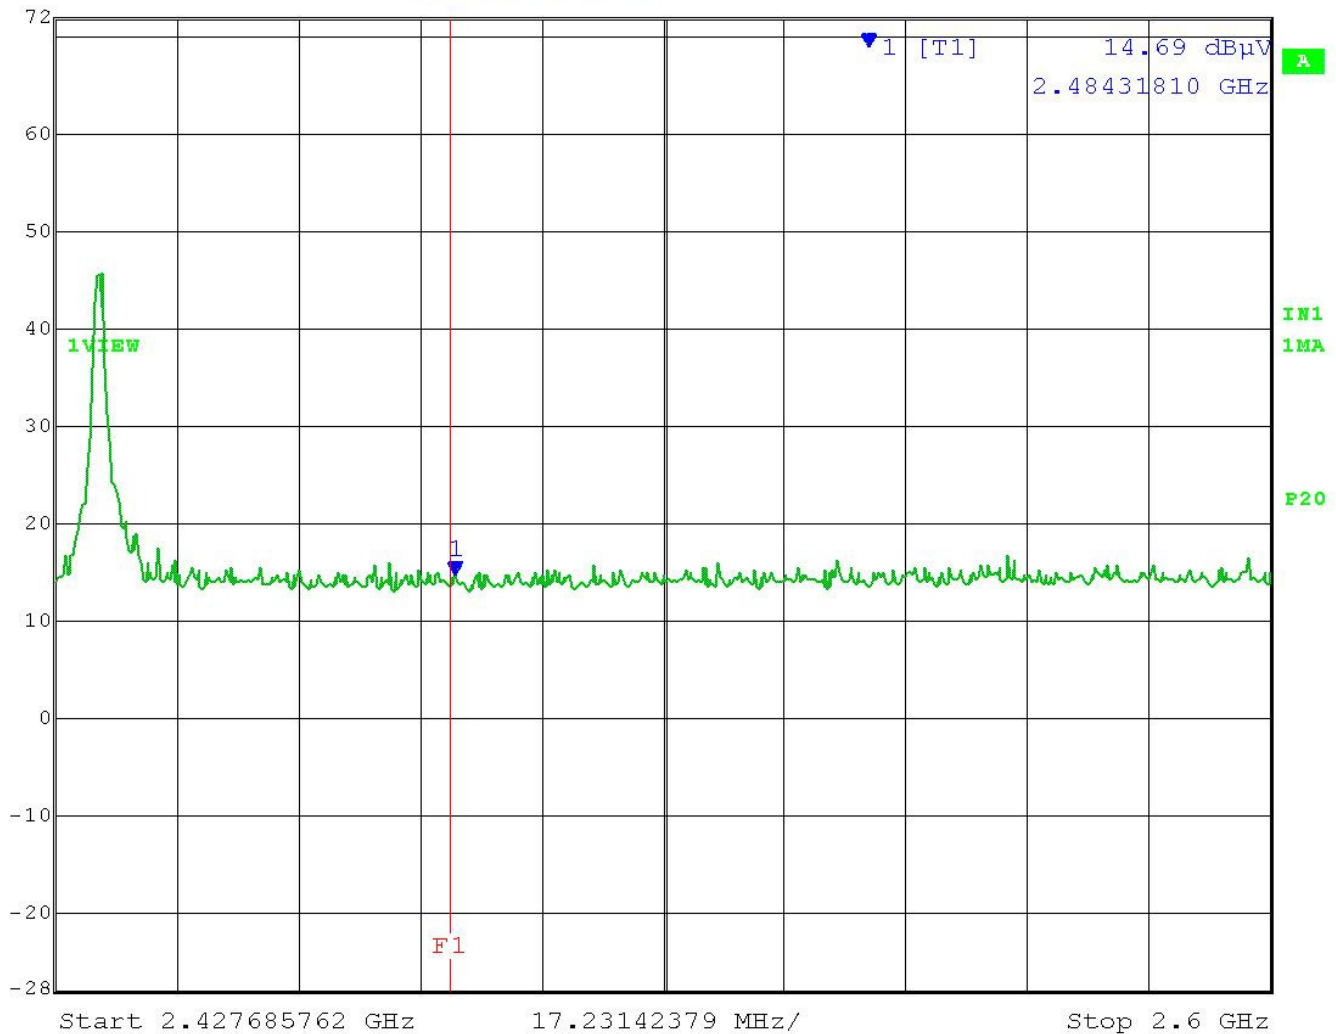

Date: 10.MAR.2017 10:32:36

RESULTS: Meets Requirements

Applicant: IRADIMED CORPORATION
 FCC ID: 2AKRU-IRM01
 IC: 22312-IRM01
 Report: 2449AUT16TestReport_Rev1


[Table of Contents](#)

BANDEDGE

Test Data: Upper Bandedge Average Plot



Ref Lvl	Marker 1 [T1]	RBW	1 MHz	RF Att	0 dB
72 dBμV	1.53 dBμV	VBW	10 Hz		
	2.48431810 GHz	SWT	18.5 s	Unit	dBμV

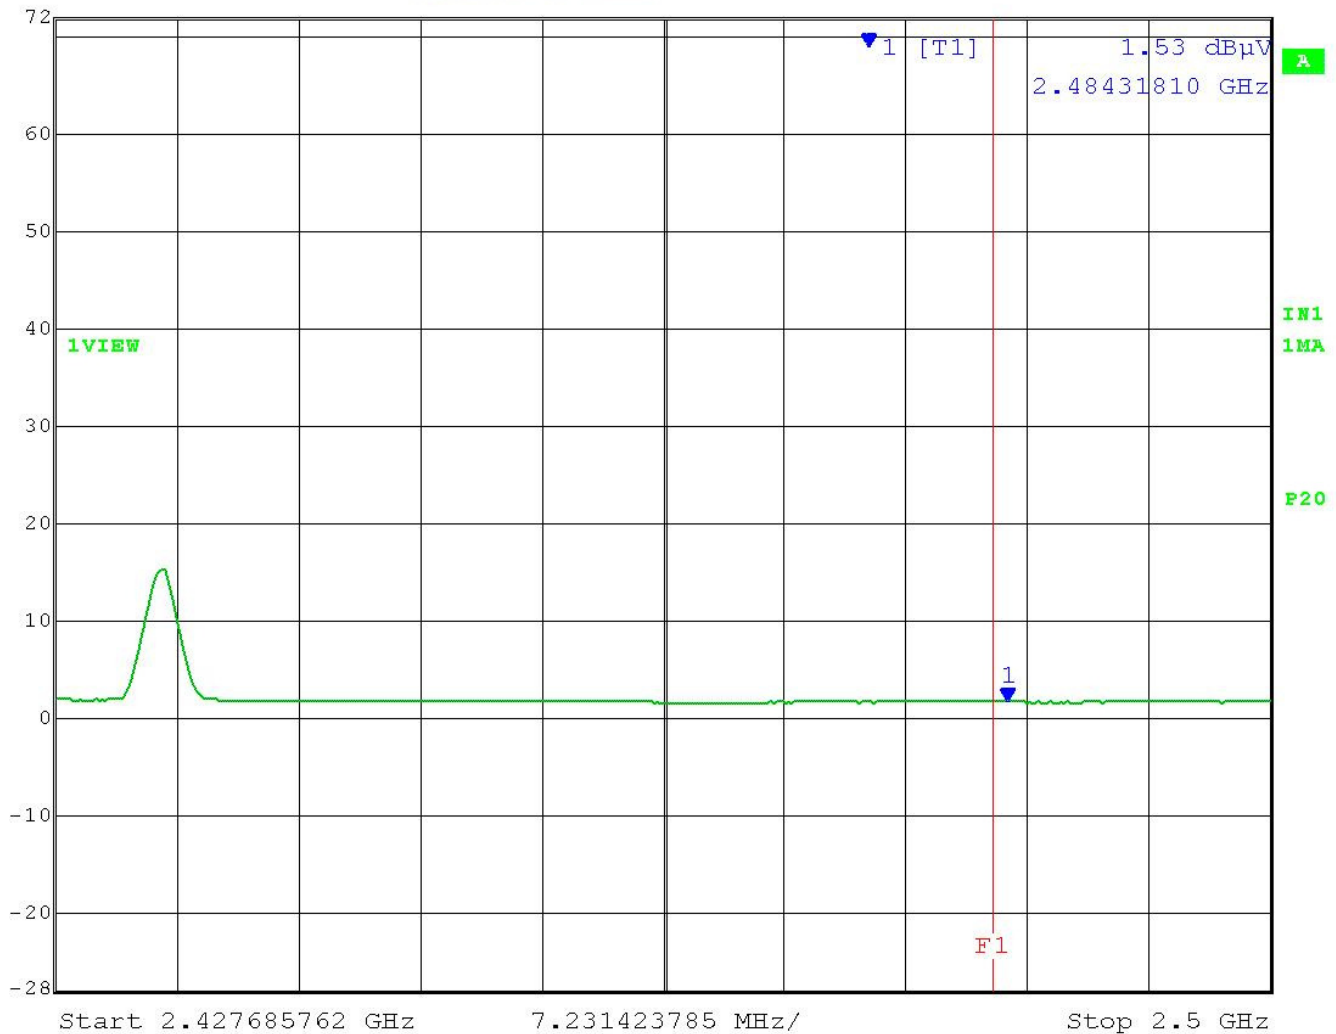

Date: 10.MAR.2017 10:35:27

RESULTS: Meets Requirements

RADIATED SPURIOUS EMISSIONS

Rules Part No.: FCC part 15.249 (a)(c)(d)(e)

Requirements: the field strength of emissions from intentional radiators operated within these frequency bands shall comply with the following:

As shown in §15.35(b), for frequencies above 1000 MHz, the field strength limits of this section are based on average limits. However, the peak field strength of any emission shall not exceed the maximum permitted average limits specified above by more than 20 dB under any condition of modulation

Field strength limits are specified at a distance of 3 meters

Emissions radiated outside of the specified frequency bands, except for harmonics, shall be attenuated by at least 50 dB below the level of the fundamental or to the general radiated emission limits in §15.209, whichever is the lesser attenuation.

Frequency	Limits
Part 15.209	
9 to 490 kHz	2400/F (kHz) μ V/m @ 300 meters
490 to 1705 kHz	24000/F (kHz) μ V/m @ 30 meters
1705 kHz to 30 MHz	29.54 dB μ V/m @ 30 meters
30 – 88	40.0 dB μ V/m @ 3 meters
80 – 216	43.5 dB μ V/m @ 3 meters
216 – 960	46.0 dB μ V/m @ 3 meters
Above 960	54.0 dB μ V/m @ 3 meters
Part 15.249	
Fundamental 902 – 928 MHz	94.0 dB μ V/m @ 3 meters
Fundamental 2.4 – 2.4835 GHz	94.0 dB μ V/m @ 3 meters
Harmonics	54.0 dB μ V/m @ 3 meters

Test Method: ANSI C63.4 § Annex D Validation of radiated emissions standard test sites
 ANSI C63.10 § 6.3 Common requirements radiated emissions
 ANSI C63.10 § 6.4 Emissions below 30 MHz
 ANSI C63.10 § 6.5 Emissions between 30 & 1000 MHz
 ANSI C63.10 § 6.6 Emissions above 1 GHz

Field Strength Calculation:

The field strength at 3m was established by adding the meter reading of the spectrum analyzer (which is set to read in units of dB μ V) to the antenna correction factor supplied by the antenna manufacturer plus the coax loss. The antenna correction factors are stated in terms of dB. The gain of the preselector was accounted for in the spectrum analyzer meter reading.

Example:

Freq (MHz)	Meter Reading	+ ACF	+ CL = FS
33	20 dB μ V	+ 10.36 dB	+ 0.5 = 30.86 dB μ V/m @ 3m

Applicant: IRADIMED CORPORATION

FCC ID: 2AKRU-IRM01

IC: 22312-IRM01


Report: 2449AUT16TestReport_Rev1

[Table of Contents](#)


RADIATED SPURIOUS EMISSIONS

Setup:


Emissions below 30 MHz

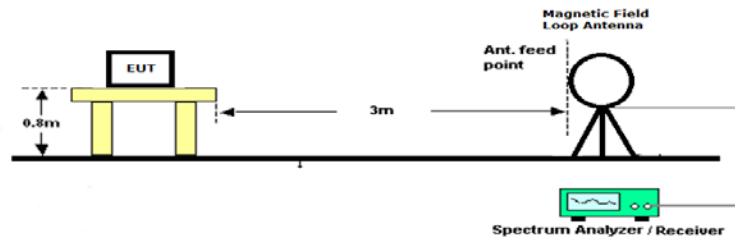

Emissions 30 – 1000 MHz

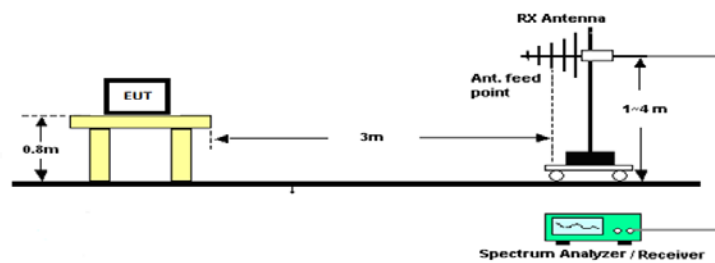

Emissions above 1 GHz

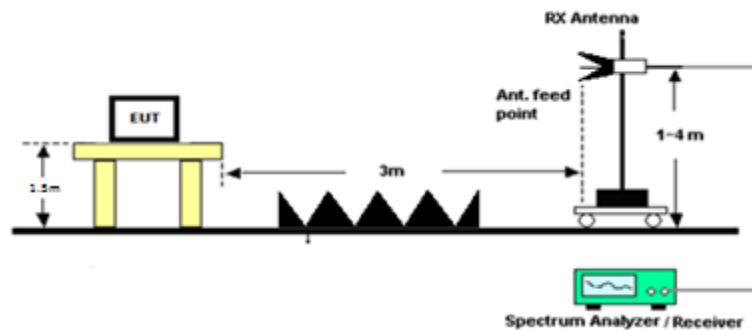

RADIATED SPURIOUS EMISSIONS

Notes: The EUT was checked in three orthogonal planes as required, a setup photo is provided to show the orientation of the worst case position.

Only emissions within 20dB of the limit are reported.

The spectrum was measured from 9 KHz to 25 GHz

Test Data: Measurement Table

Tuned Freq (MHz)	Emission Frequency (MHz)	Detector (QP/PK/AV)	Meter Reading (dBuV)	Antenna Polarity (H/V)	Coax Loss (dB)	Correction Factor (dB/M)	Field Strength (dBuV/M)	Limit (dBuV/M)	Margin (dB)
2404.00	271.79	PK	19.97	V	1.93	14.09	35.99	46.00	10.01
2404.00	332.05	PK	20.83	H	2.11	13.60	36.54	46.00	9.46
2404.00	580.76	PK	21.26	V	2.78	18.26	42.30	46.00	3.70
2404.00	733.33	PK	20.57	H	3.12	20.20	43.89	46.00	2.11
2404.00	2338.90	PK	13.65	H	5.61	32.09	51.35	54.00	2.65
2404.00	2397.00	PK	13.28	V	5.62	32.14	51.04	54.00	2.96
2404.00	2398.00	PK	12.77	H	5.66	32.29	50.72	54.00	3.28
2404.00	2404.00	PK	48.89	V	5.69	32.41	86.99	94.00	7.01
2404.00	4808.00	PK	0.29	V	8.07	33.99	42.35	54.00	11.65
2404.00	7212.00	PK	-0.82	V	9.92	35.42	44.52	54.00	9.48
2404.00	9616.00	PK	-1.46	V	11.43	36.83	46.80	54.00	7.20
2412.00	170.03	PK	0.01	V	1.49	15.79	17.29	43.50	26.21
2412.00	325.64	PK	23.23	H	2.09	13.60	38.92	46.00	7.08
2412.00	398.72	PK	23.23	V	2.28	15.35	40.86	46.00	5.14
2412.00	629.92	PK	22.06	H	2.89	18.90	43.85	46.00	2.15
2412.00	700.00	PK	21.68	V	3.06	20.60	45.34	46.00	0.66
2412.00	2412.00	PK	53.01	V	5.70	32.44	91.15	94.00	2.85
2412.00	4824.00	PK	0.56	H	8.09	33.98	42.63	54.00	11.37
2412.00	7236.00	PK	-0.39	V	9.94	35.47	45.02	54.00	8.98
2412.00	9648.00	PK	-1.22	H	11.45	36.90	47.13	54.00	6.87
2434.00	301.28	PK	23.36	V	2.03	13.27	38.66	46.00	7.34
2434.00	352.56	PK	24.02	H	2.16	14.71	40.89	46.00	5.11
2434.00	617.98	PK	22.70	V	2.86	18.76	44.32	46.00	1.68
2434.00	635.89	PK	21.17	H	2.91	19.25	43.33	46.00	2.67
2434.00	2434.00	PK	52.19	V	5.73	32.50	90.42	94.00	3.58
2434.00	2485.80	PK	13.98	V	5.78	32.66	52.42	54.00	1.58
2434.00	2488.90	PK	13.60	V	5.79	32.67	52.06	54.00	1.94

Results: Meets Requirements

Applicant: IRADIMED CORPORATION
FCC ID: 2AKRU-IRM01
IC: 22312-IRM01
Report: 2449AUT16TestReport_Rev1

[Table of Contents](#)

EMC EQUIPMENT LIST

Device	Manufacturer	Model	Serial Number	Cal/Char Date	Due Date
Antenna: Biconical 1096 Chamber	Eaton	94455-1	1096	07/14/15	07/14/17
Antenna: Log-Periodic 1122	Electro-Metrics	LPA-25	1122	07/14/15	07/14/17
Antenna: Standard Gain Horn 18.0-26.3 GHz	Systron Donner	DBE-520-20	Not Serialized	NA	NA
Antenna: Standard Gain Horn 12.4-18.0 GHz	ATM	62-442-6	D262108-01	NA	NA
CHAMBER	Panashield	3M	N/A	04/25/16	12/31/17
Antenna: Double-Ridged Horn/ETS Horn 1	ETS-Lindgren Chamber	3117	00035923	01/30/17	01/30/2017
Software: Field Strength Program	Timco	N/A	Version 4.0	NA	NA
Antenna: Active Loop	ETS-Lindgren	6502	00062529	11/18/15	11/18/17
EMI Test Receiver R & S ESU 40 Chamber	Rohde & Schwarz	ESU 40	100320	04/01/16	04/01/18
Coaxial Cable - Chamber 3 cable set (Primary)	Micro-Coax	Chamber 3 cable set (Primary)	KMKM-0244-01; KMKM-0670-00; KFKF-0198-01	08/08/16	08/08/18
Pre-amp	RF-LAMBDA	RNLA00M45GA	NA	01/04/16	01/04/18
Band Reject Filter 2.4 GHz	Micro-Tronics	BRM50702-02	-G042	9/27/16	9/27/18
High Pass Filter 18GHz	Micro-Tronics	HPS18771	-002	9/27/16	9/27/18
Bore-sight Antenna Positioning Tower	Sunol Sciences	TLT2	N/A	NA	NA

* EMI RECEIVER SOFTWARE VERSION

The receiver firmware used was version 4.43 Service Pack 3

END OF TEST REPORT