

## System Check\_H2450

**DUT: Dipole 2450 MHz; Type:D2450V2; SN:927**

Communication System: CW; Frequency: 2450 MHz;Duty Cycle: 1:1

Medium: H2450 Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.79$  S/m;  $\epsilon_r = 40.105$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature : 22.4 °C; Liquid Temperature : 22.2 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN3970;Calibrated: 2022/4/18;
- Electronics: DAE4 Sn1418; Calibrated: 2022/3/24
- Phantom: ELI v5.0; Type: QDOVA002AA; Serial: TP:1231
- Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

**Pin=250mW/Area Scan (41x51x1):** Interpolated grid: dx=2.000 mm, dy=2.000 mm

Maximum value of SAR (interpolated) = 25.4 W/kg


**Pin=250mW/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 114.7 V/m; Power Drift = 0.10 dB

Peak SAR (extrapolated) = 30.4 W/kg

**SAR(1 g) = 13.01 W/kg; SAR(10 g) = 6.09 W/kg**

Maximum value of SAR (measured) = 23.4 W/kg

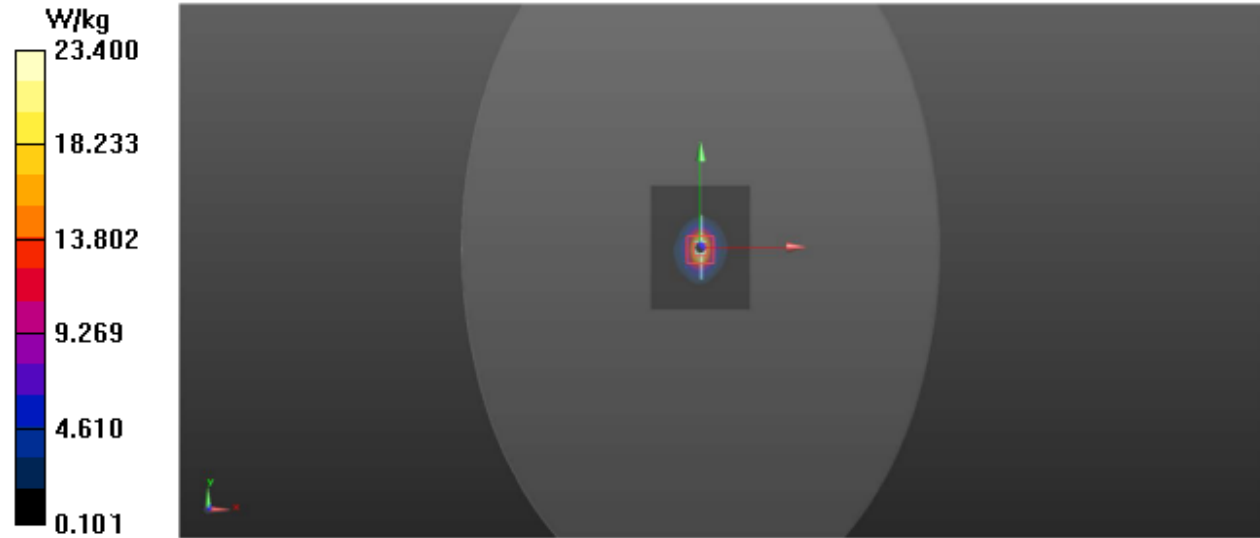

## System Check\_H5250

**DUT: Dipole 5GHzV2;Type:D5GHzV2; SN:1169**

Communication System: CW; Frequency: 5250 MHz;Duty Cycle: 1:1

Medium: H5G Medium parameters used:  $f = 5250$  MHz;  $\sigma = 4.74$  S/m;  $\epsilon_r = 36.82$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature : 22.1 °C; Liquid Temperature : 21.9 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN3970; Calibrated: 2023/5/17;
- Electronics: DAE4 Sn1418; Calibrated: 2023/4/25
- Phantom: ELI v5.0; Type: QDOVA002AA; Serial: TP:1231
- Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

**Pin=100mW/Area Scan (7x9x1):** Interpolated grid: dx=2.000 mm, dy=2.000 mm

Maximum value of SAR (interpolated) = 33.0 W/kg

**Pin=100mW/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=2mm

Reference Value = 58.461 V/m; Power Drift = 0.14 dB

Peak SAR (extrapolated) = 36.1 W/kg

**SAR(1 g) = 7.62 W/kg; SAR(10 g) = 2.13 W/kg**

Maximum value of SAR (measured) = 32.6 W/kg

