


Impedance Plot for SN 22/16 DIP 0G750-417


750 Head

Calibrated impedance: $55.4\Omega - 1.2j\Omega$; Measurement impedance: $52.4\Omega + 3.9j\Omega$ (within 5Ω)

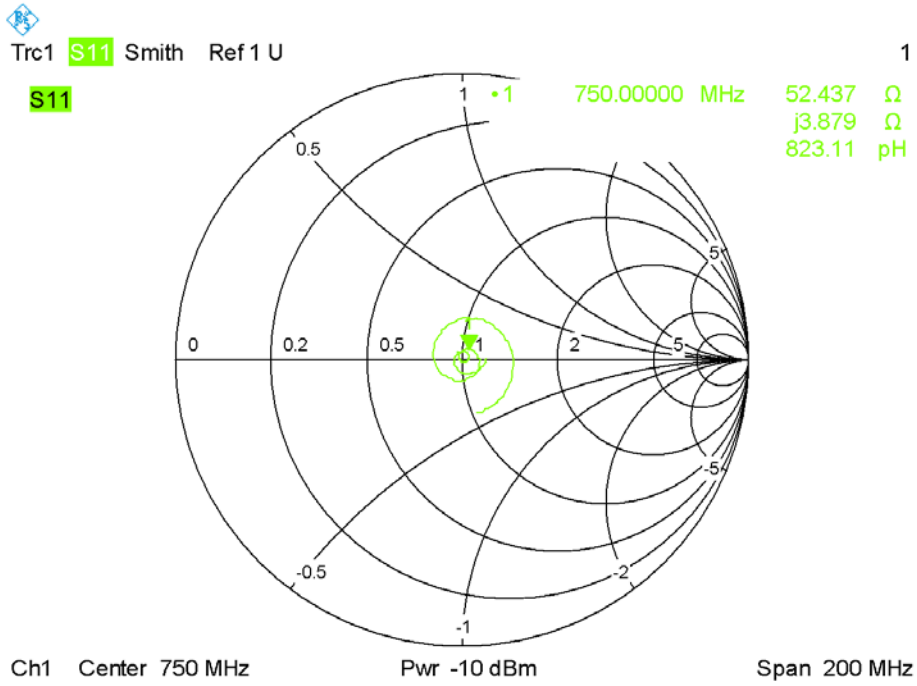

Date: 29.MAY.2023 10:29:42

Calibrated return loss: -25.16dB; Measurement return loss: -24.82dB (within 20%)

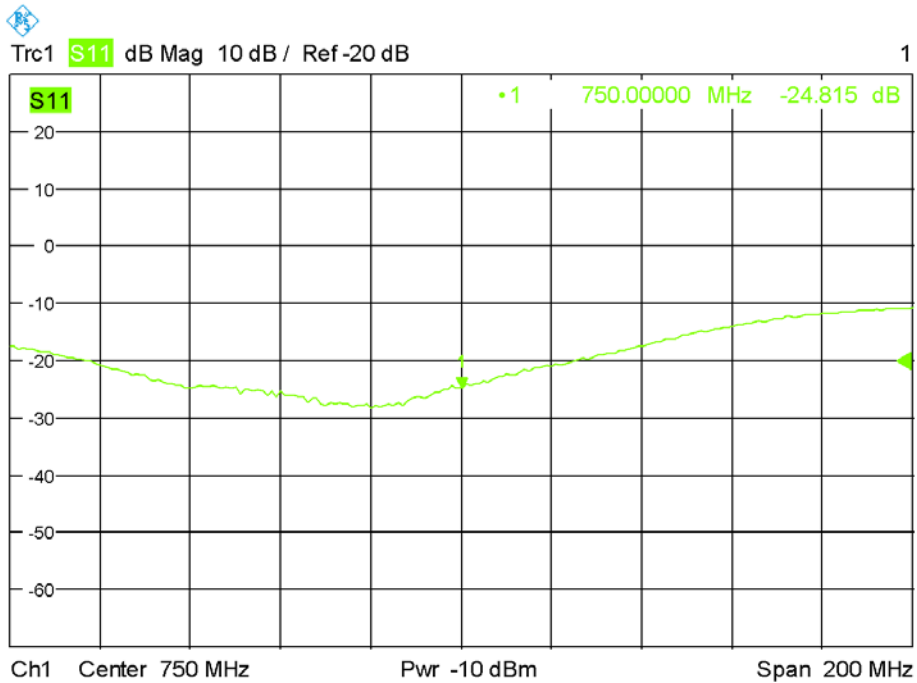


Date: 29.MAY.2023 10:30:54

Impedance Plot for SN 15/16 DIP 0G835-399


835 Head

Calibrated impedance: $59.4\Omega - 0.8j\Omega$; Measurement impedance: $62.7\Omega - 1.3j\Omega$ (within 5Ω)

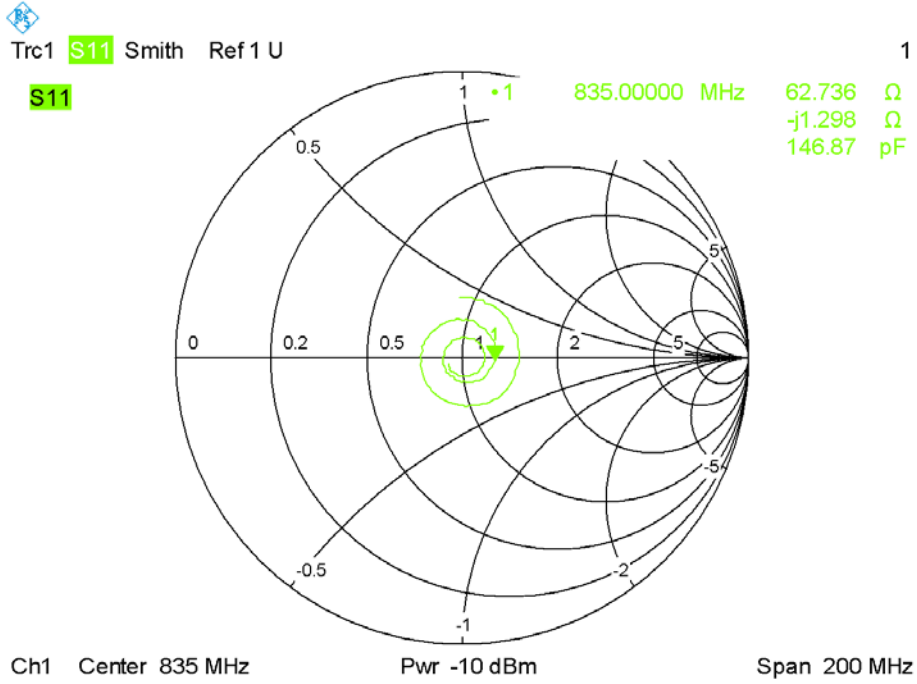

Date: 29.MAY.2023 10:36:07


Calibrated return loss: -20.99dB; Measurement return loss: -21.73dB (within 20%)

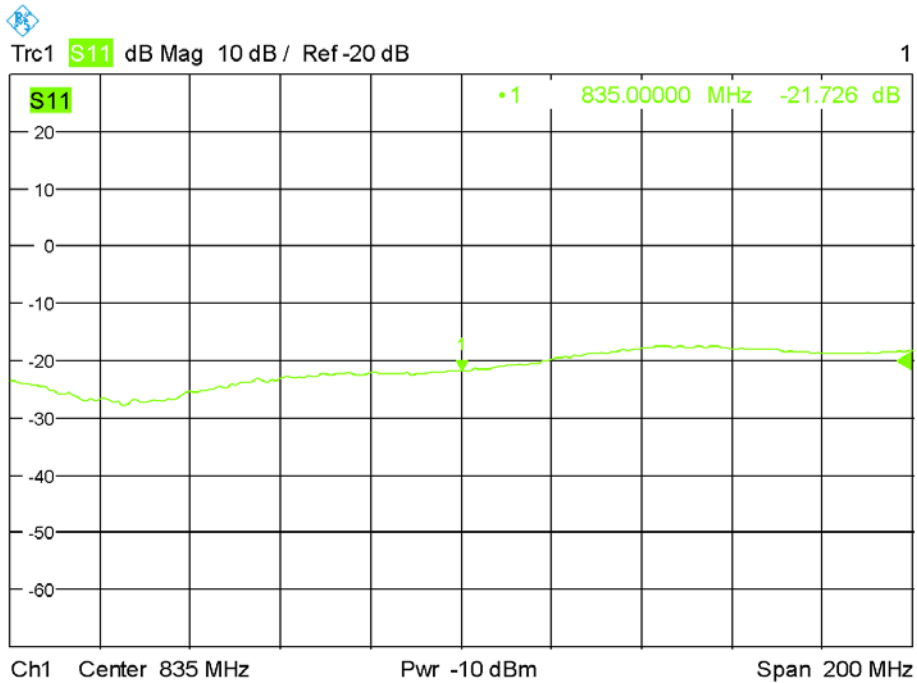

Date: 29.MAY.2023 10:38:24


Impedance Plot for SN 46/11 DIP 1G800-186
1800 Head

Calibrated impedance: $47.2\Omega + 4.6j\Omega$; Measurement impedance: $47.7\Omega + 1.5j\Omega$ (within 5Ω)

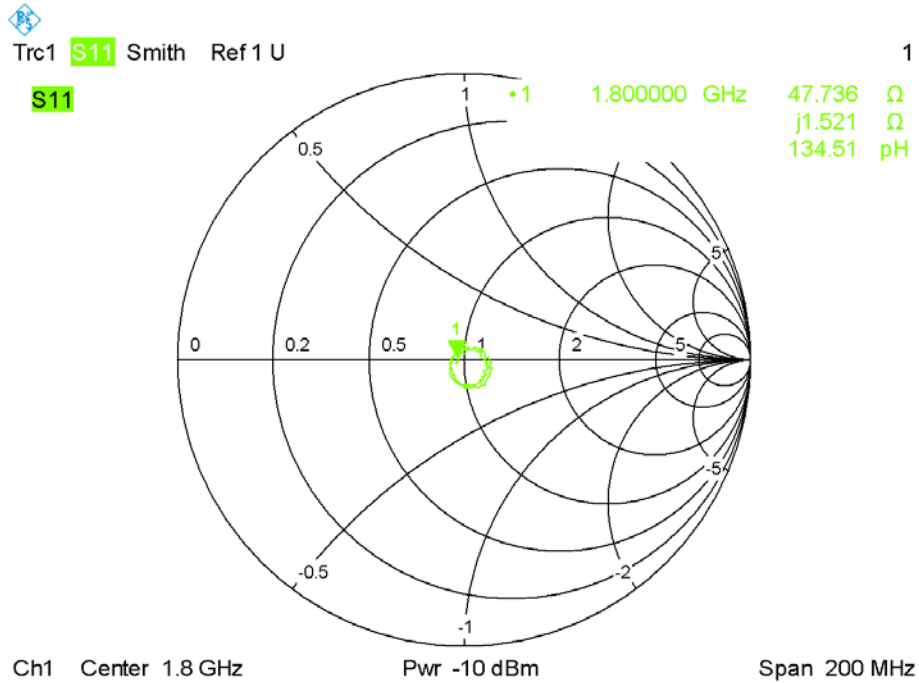

Date: 29.MAY.2023 10:20:15

Calibrated return loss: -25.33dB; Measurement return loss: -27.28dB (within 20%)

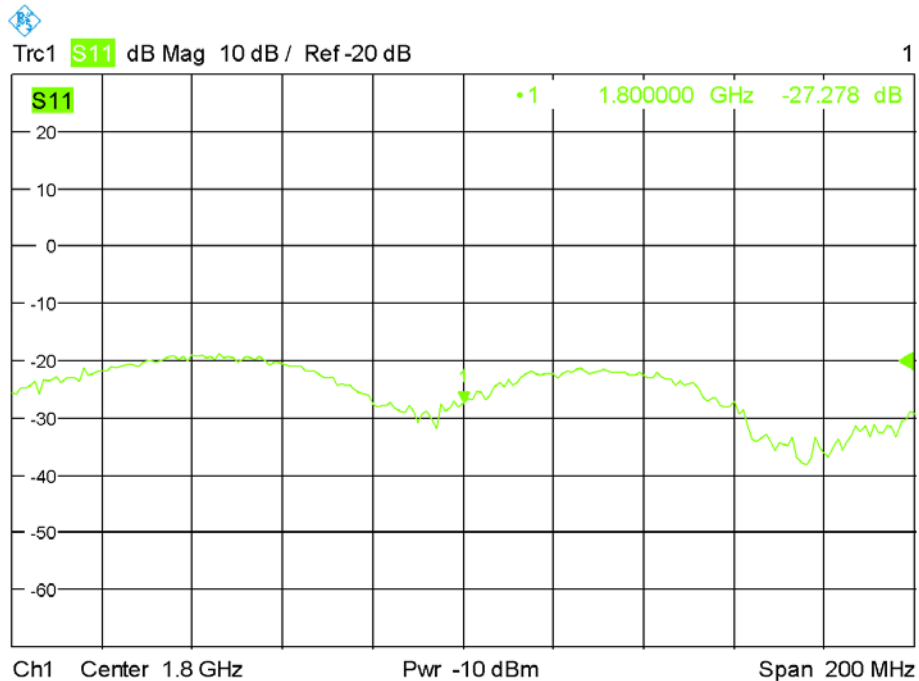


Date: 29.MAY.2023 10:21:25


Impedance Plot for SN 29/15 DIP 1G900-389

1900 Head

Calibrated impedance: $52.2\Omega + 6.1j\Omega$; Measurement impedance: $51.0\Omega + 3.2j\Omega$ (within 5Ω)

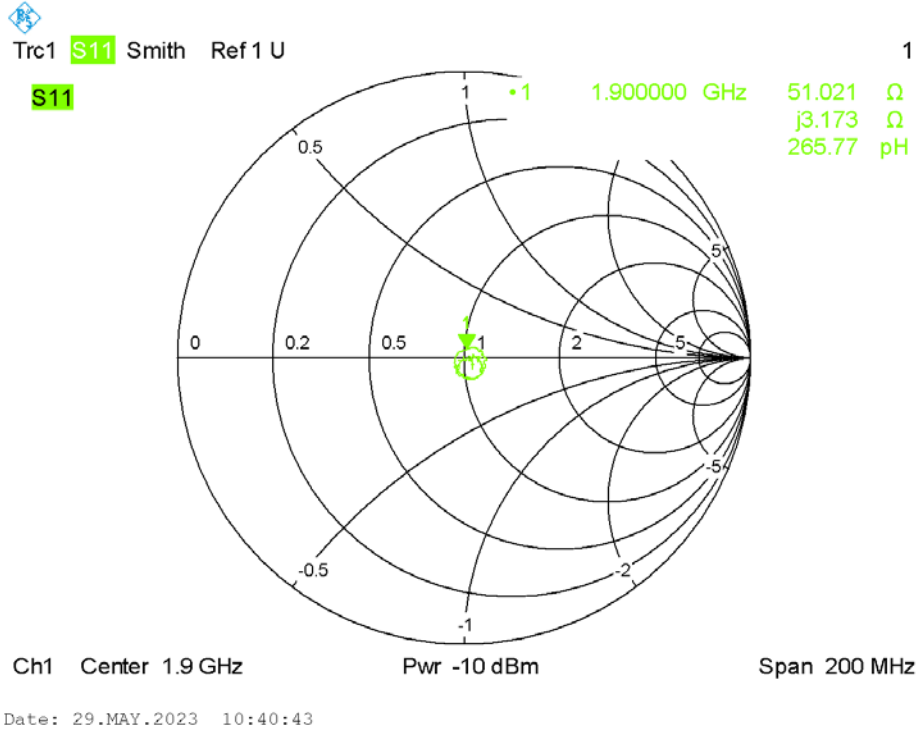


Calibrated return loss: -23.76dB; Measurement return loss: -21.07dB (within 20%)

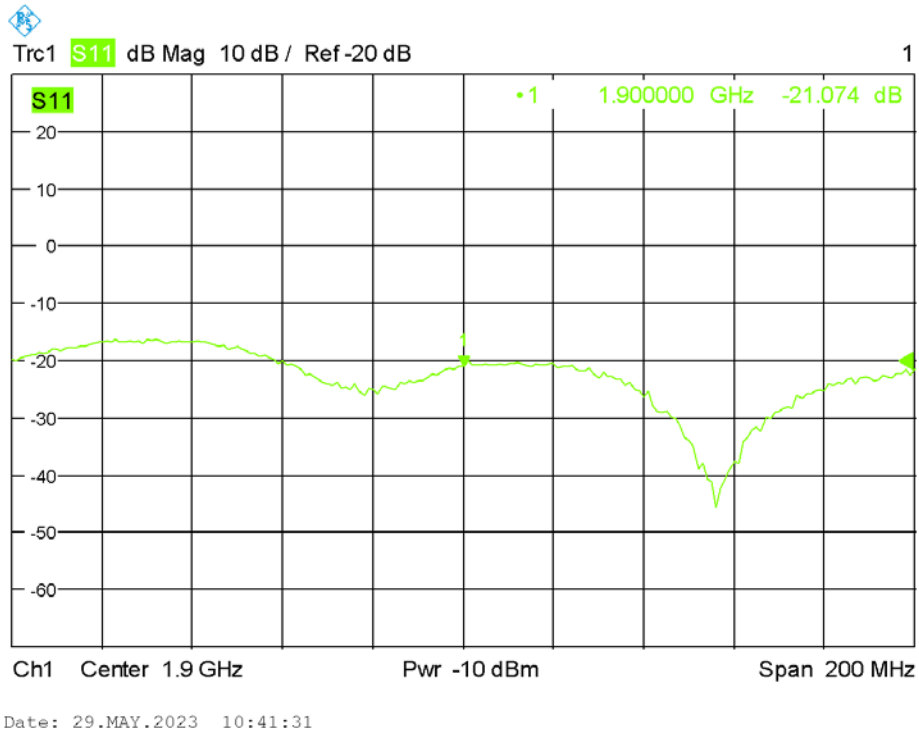

Impedance Plot for SN 29/15 DIP 2G450-393


2450 Head

Calibrated impedance: $52.3\Omega + 3.4j\Omega$; Measurement impedance: $55.8\Omega + 1.6j\Omega$ (within 5Ω)

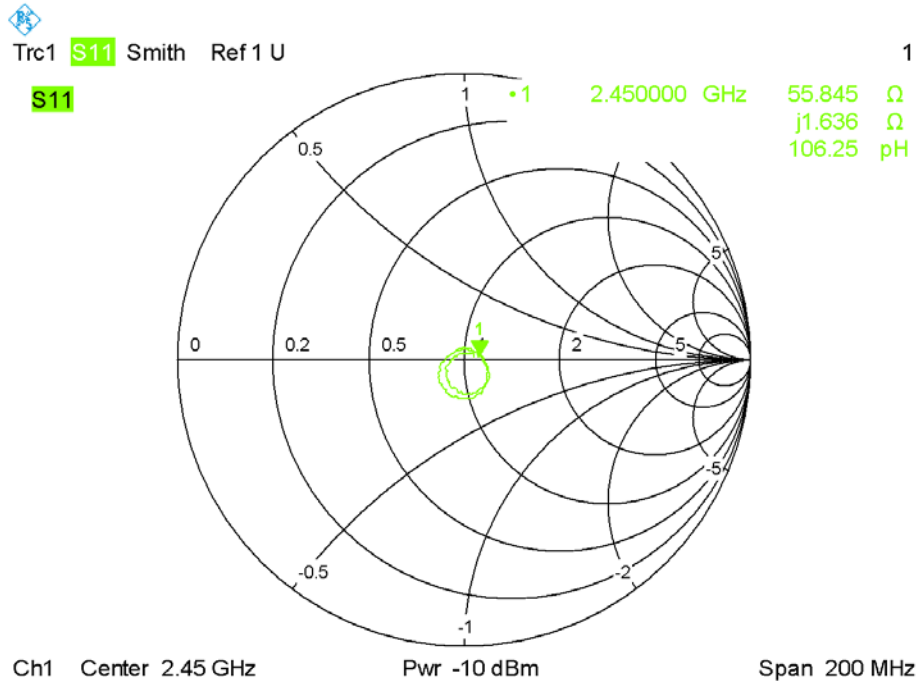

Date: 29.MAY.2023 10:49:23

Calibrated return loss: -27.80dB; Measurement return loss: -24.53dB (within 20%)

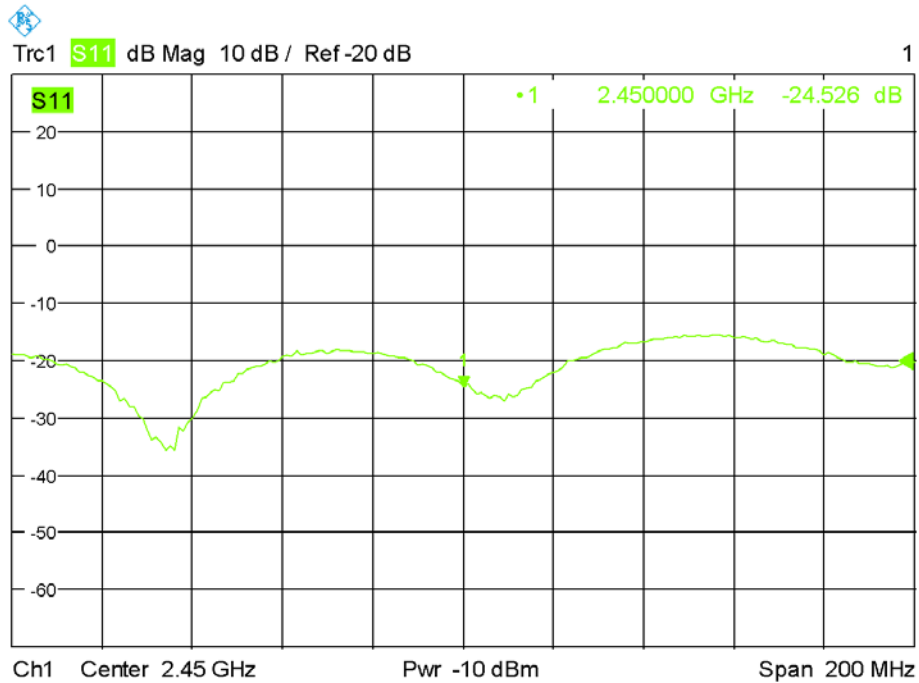


Date: 29.MAY.2023 10:50:11

Impedance Plot for SN17/22 DIP 5G000-671


5200 Head

Calibrated impedance: $54.06\Omega + 8.44j\Omega$; Measurement impedance: $55.03\Omega + 7.00j\Omega$ (within 5Ω)

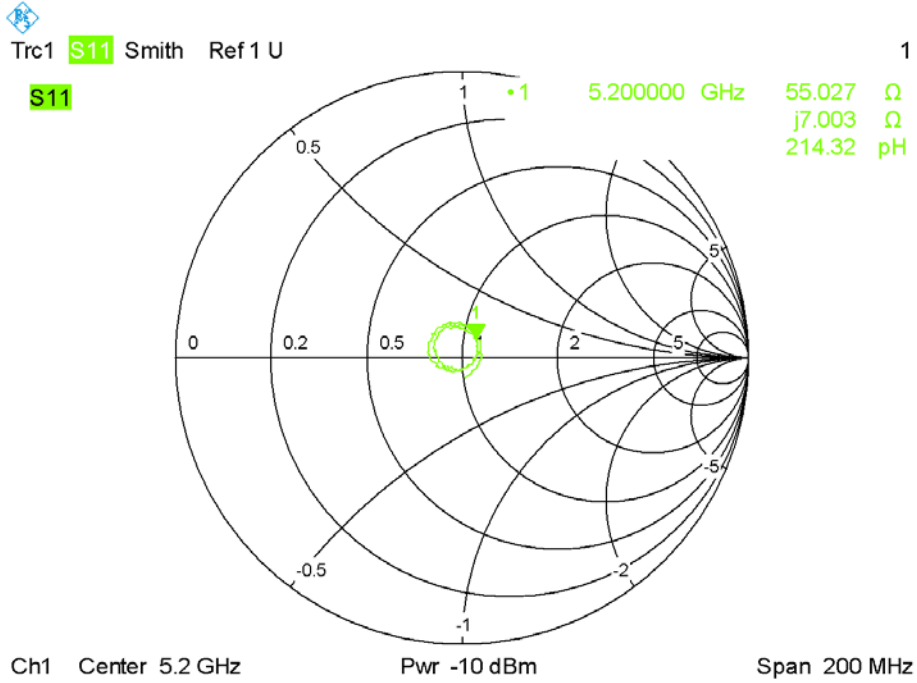

Date: 29.MAY.2023 11:06:34


Calibrated return loss: -20.52dB; Measurement return loss: -21.29dB (within 20%)

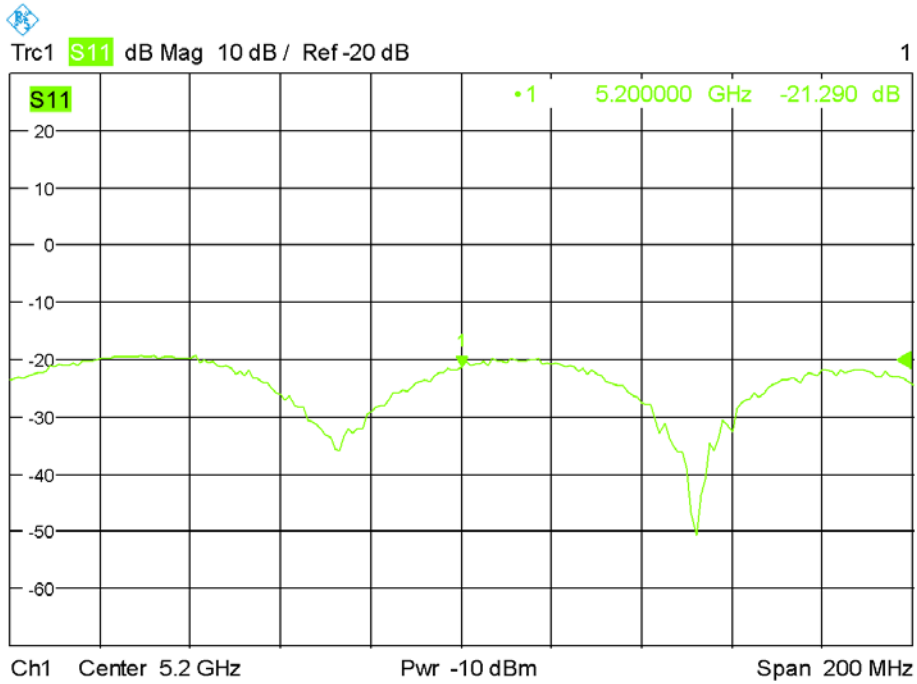


Date: 29.MAY.2023 11:08:53

5400 Head

Calibrated impedance: $47.05\Omega + 1.02j\Omega$; Measurement impedance: $46.79\Omega + 2.24j\Omega$ (within 5Ω)

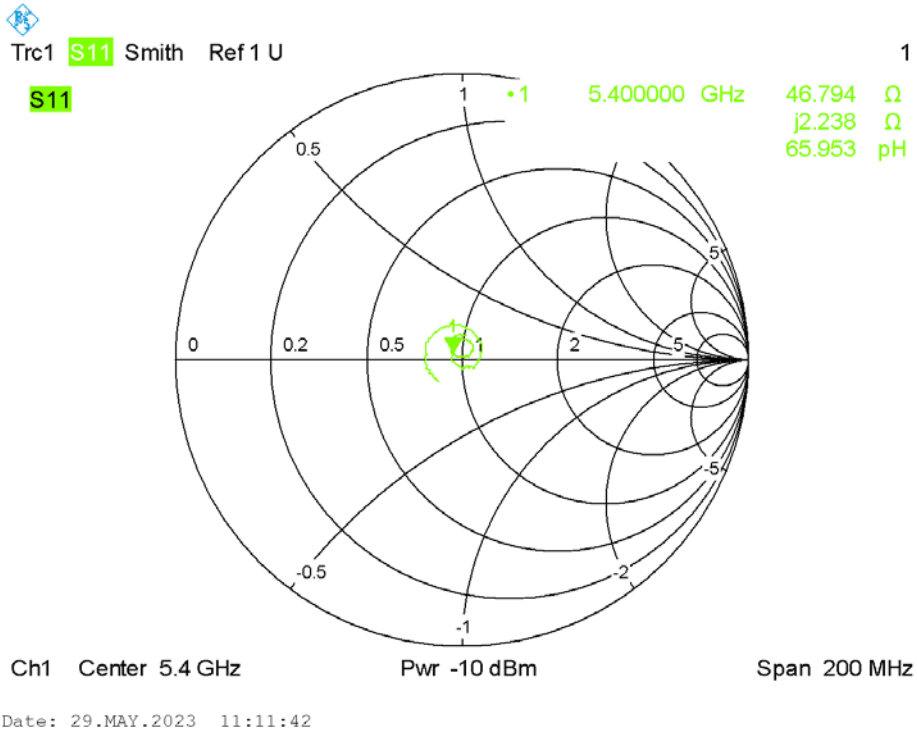


Calibrated return loss: -30.10dB; Measurement return loss: -29.33dB (within 20%)

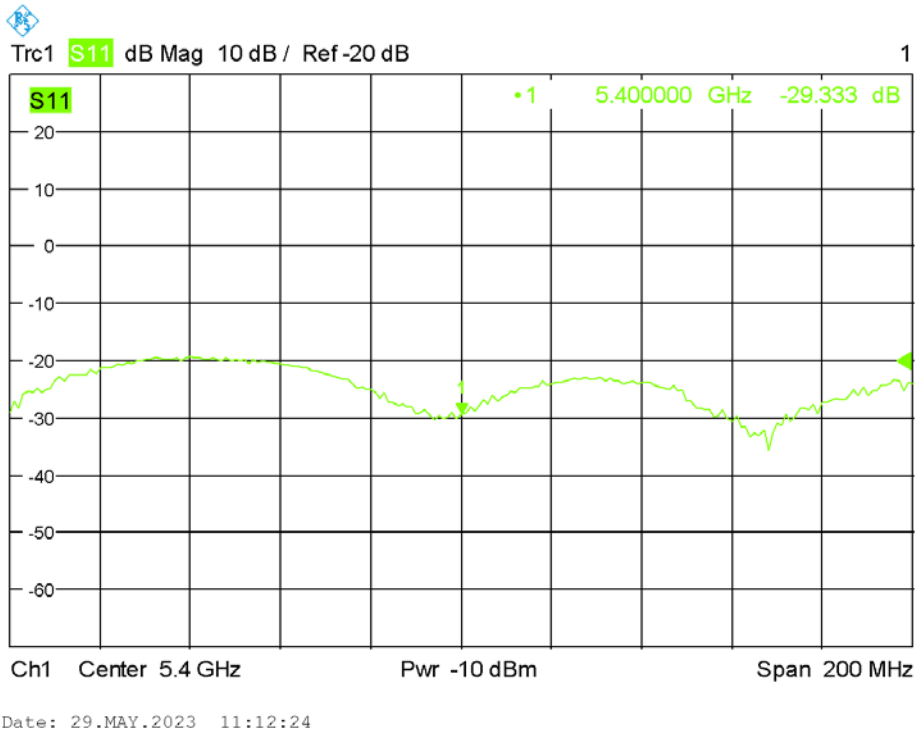


5600 Head

Calibrated impedance: $49.63\Omega + 8.57j\Omega$; Measurement impedance: $49.57\Omega + 4.70j\Omega$ (within 5Ω)

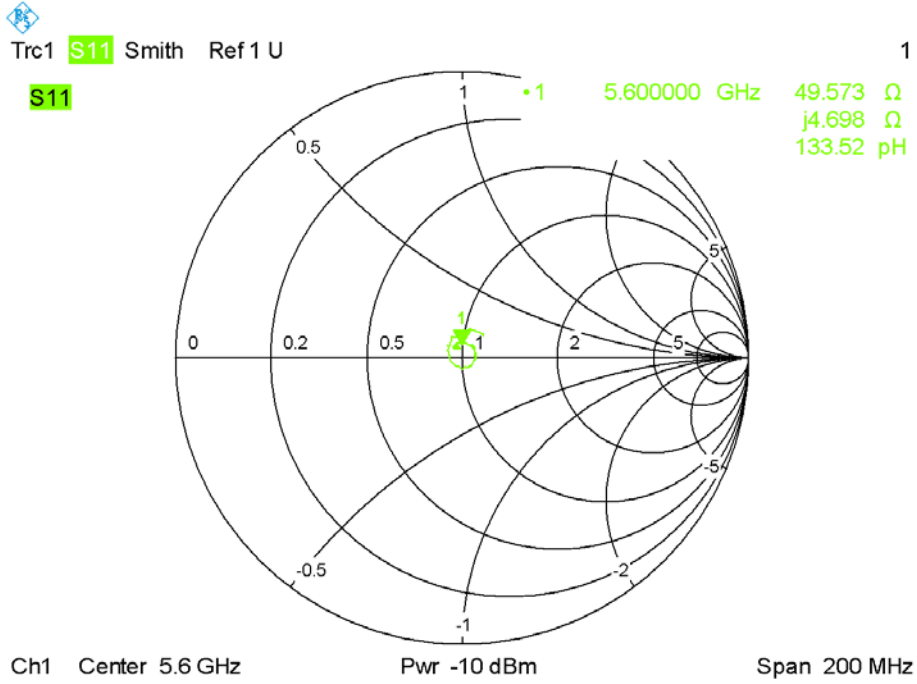

Date: 29.MAY.2023 11:13:27


Calibrated return loss: -21.30dB; Measurement return loss: -18.18dB (within 20%)

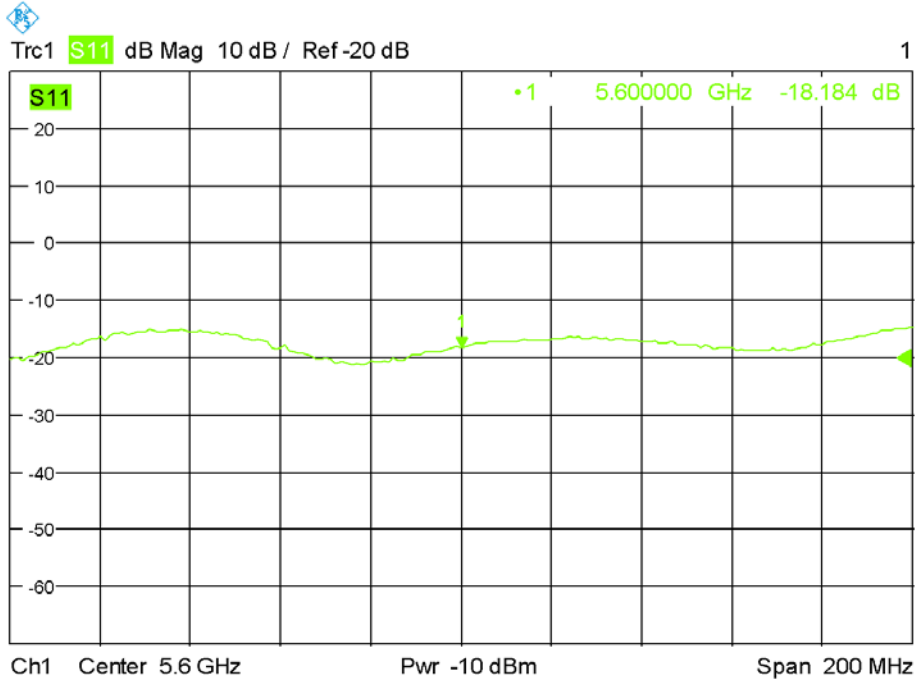

Date: 29.MAY.2023 11:14:18

5800 Head

Calibrated impedance: $47.44\Omega - 4.21j\Omega$; Measurement impedance: $48.59\Omega - 6.81j\Omega$ (within 5Ω)

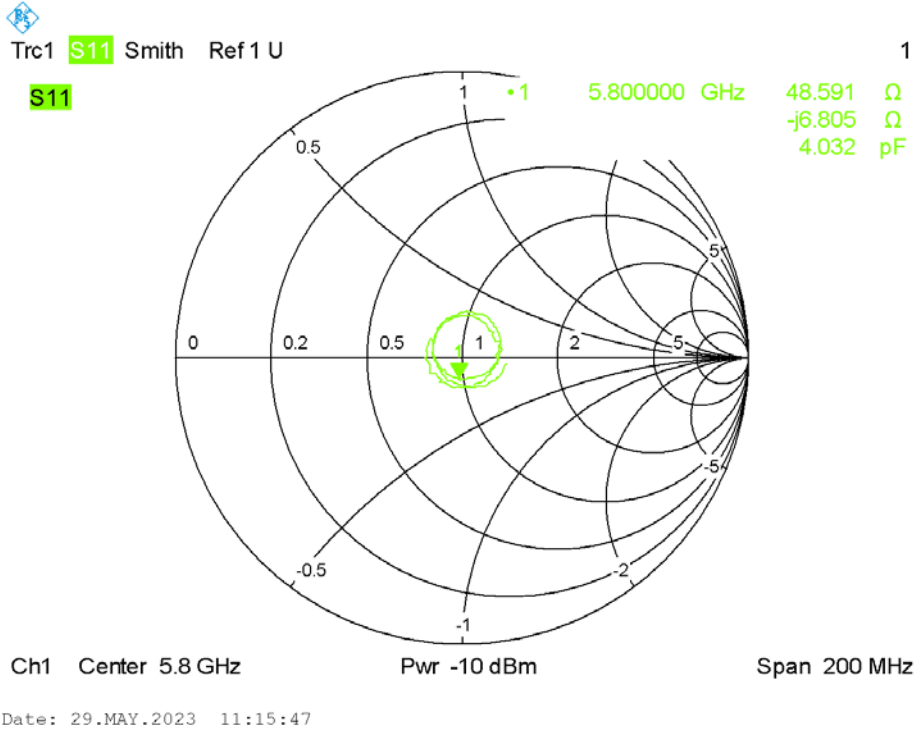

Calibrated return loss: -26.14dB; Measurement return loss: -22.57dB (within 20%)

