



Impedance Plot for

SN 47/14 DIP 0G750-340; 750Head

Calibrated impedance: $54.2\Omega + 3.9j\Omega$; Measurement impedance: $55.1\Omega - 2.2j\Omega$ (within 5Ω)

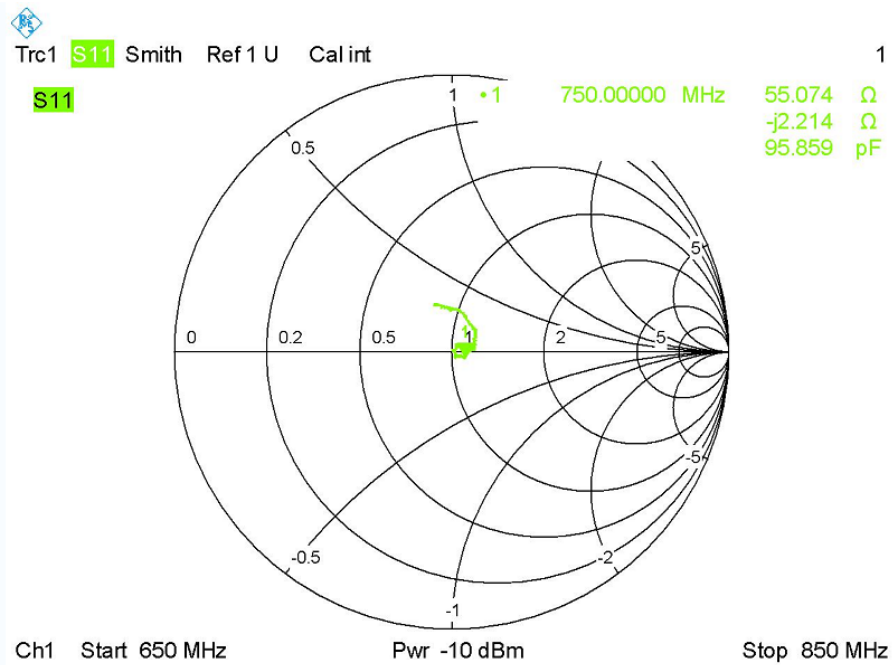


Calibrated return loss: -25.20dB; Measurement return loss: -23.05 dB (within 20%)

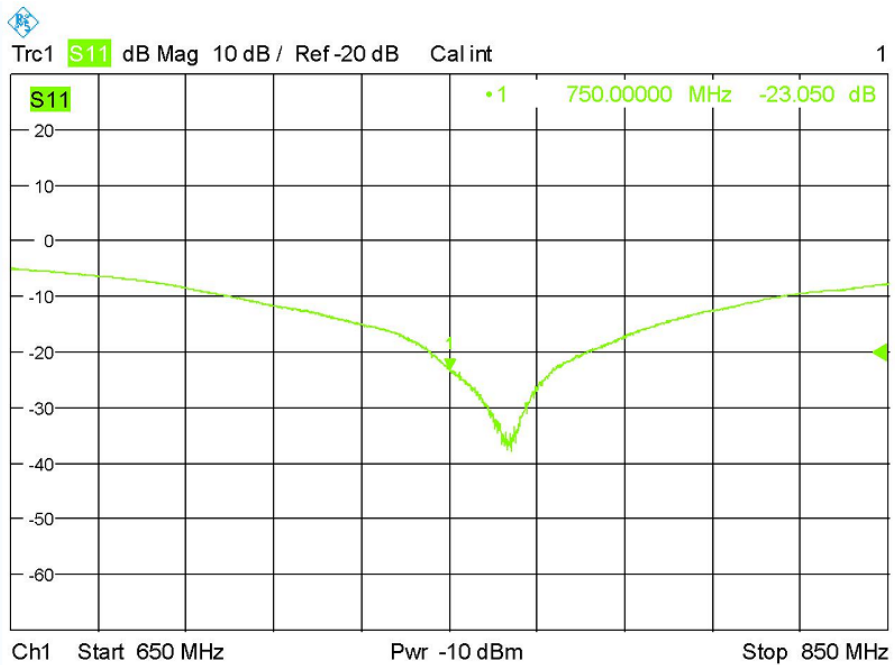


SN 29/15 DIP 0G835-383; 835Head

Calibrated impedance: $56.3\Omega + 0.8j\Omega$; Measurement impedance: $57.1\Omega - 5.0j\Omega$ (within 5Ω)

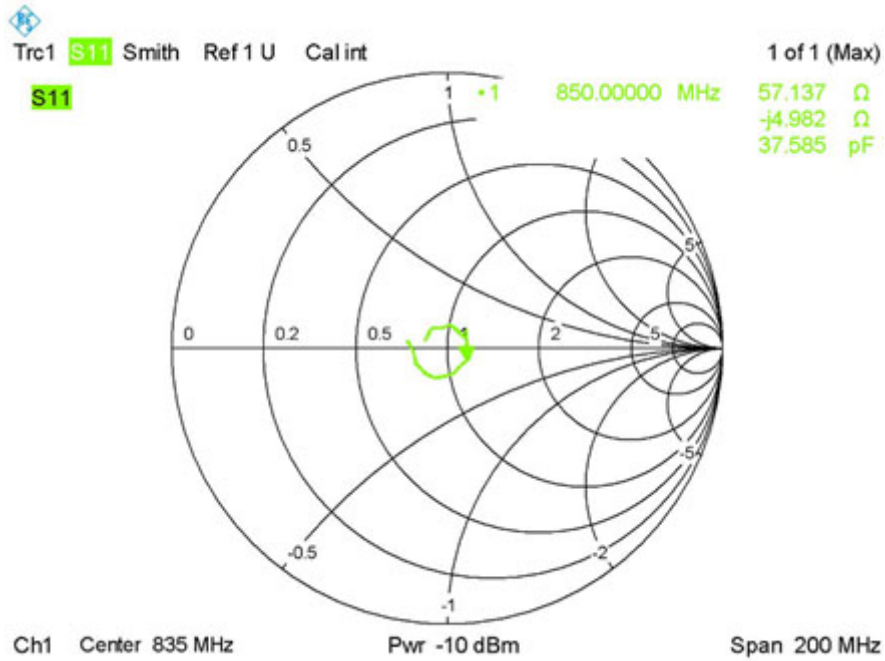


Calibrated return loss: -24.51 dB; Measurement return loss: -22.89 dB (within 20%)

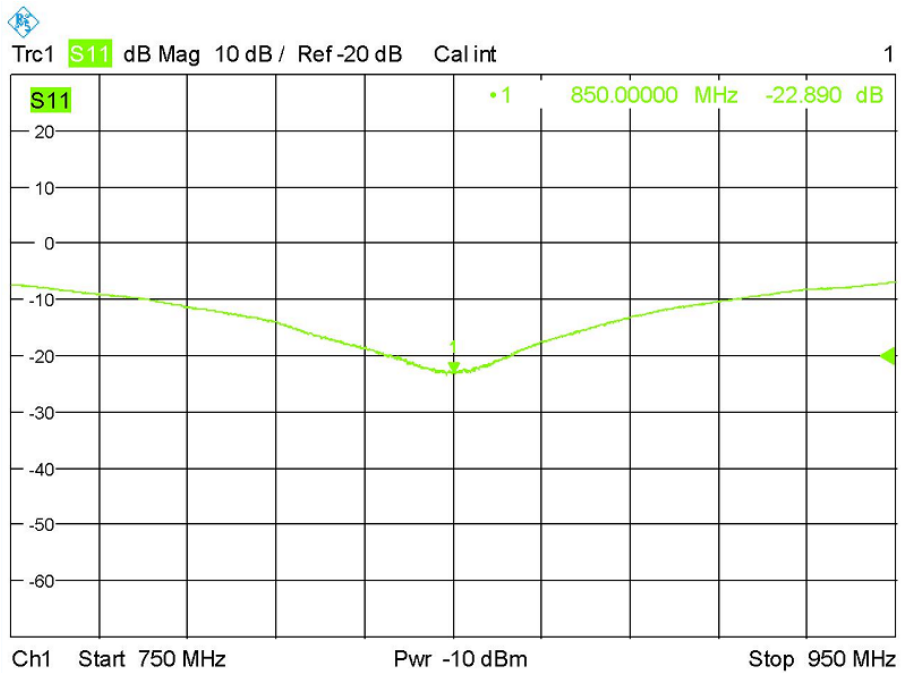


SN 46/11 DIP 1G800-186; 1800Head

Calibrated impedance: $46.7\Omega + 3.0j\Omega$; Measurement impedance: $48.5\Omega + 2.3j\Omega$ (within 5Ω)

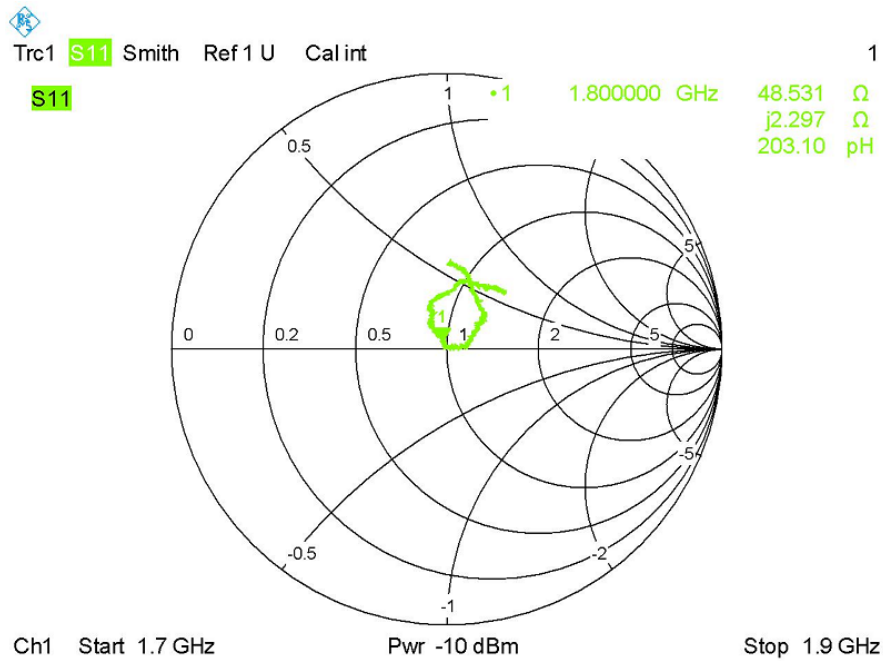


Calibrated return loss: -26.66dB; Measurement return loss: -27.3 dB (within 20%)

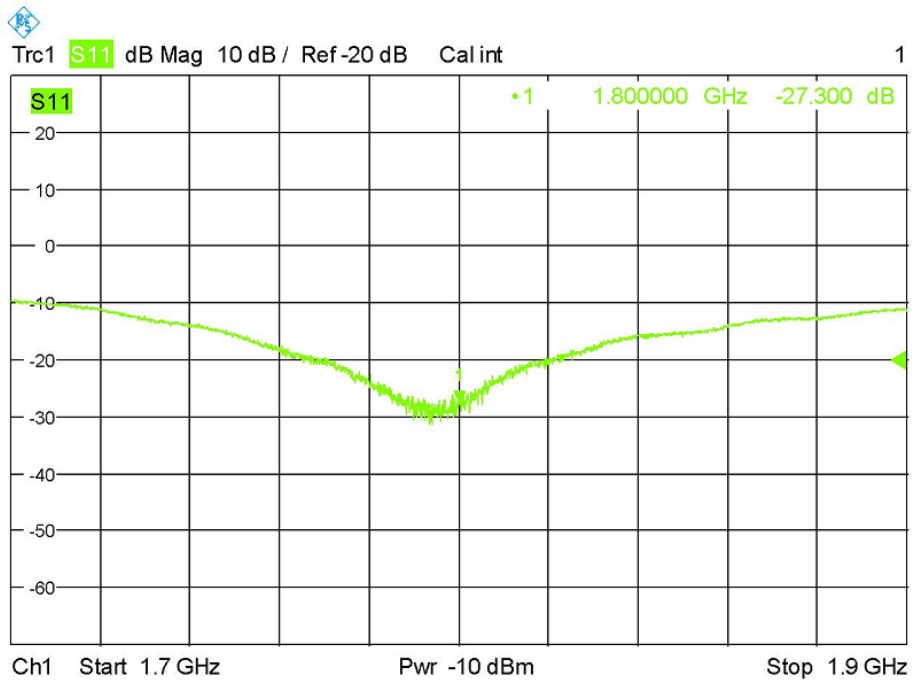


SN 46/11 DIP 1G900-187; 1900Head

Calibrated impedance: $50.7\Omega + 4.1j\Omega$; Measurement impedance: $48.6\Omega + 2.9j\Omega$ (within 5Ω)

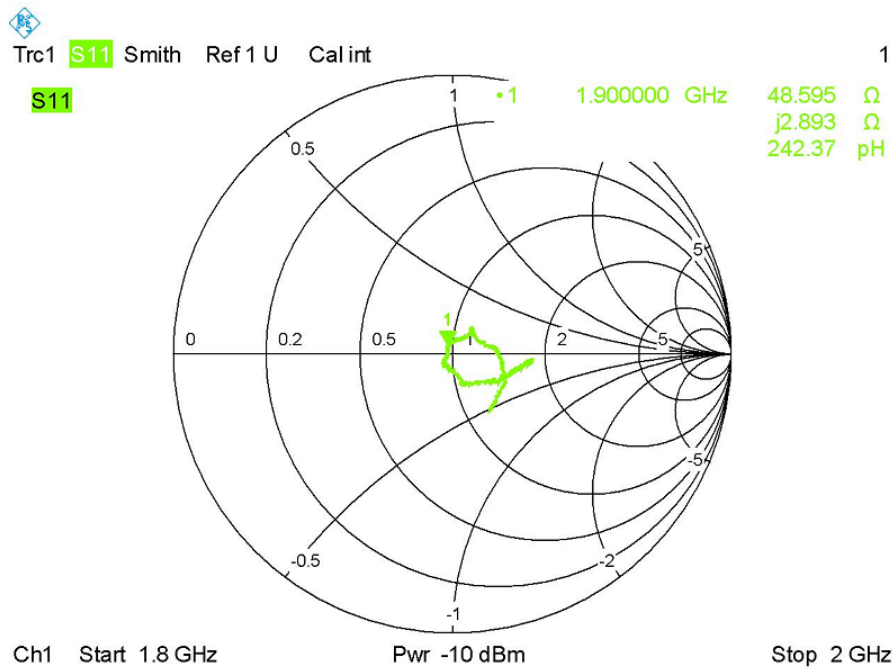


Calibrated return loss: -27.75dB; Measurement return loss: -28.54 dB (within 20%)

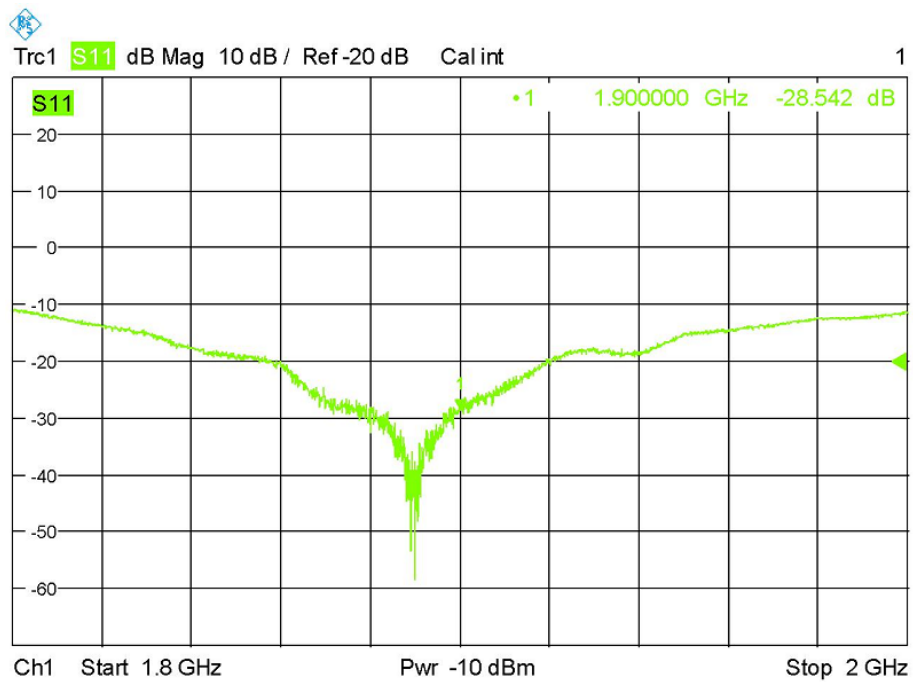


SN 46/11 DIP 2G450-189; 2450Head

Calibrated impedance: $49.8\Omega + 3.3j\Omega$; Measurement impedance: $50.9\Omega - 2.1j\Omega$ (within 5Ω)

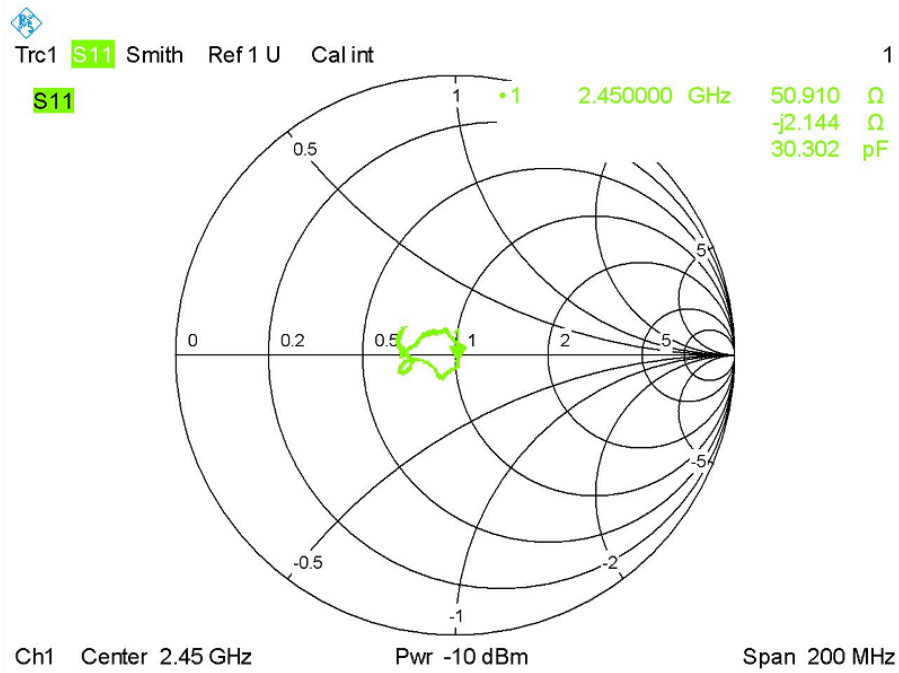


Calibrated return loss: -29.54dB; Measurement return loss: -31.08 dB (within 20%)

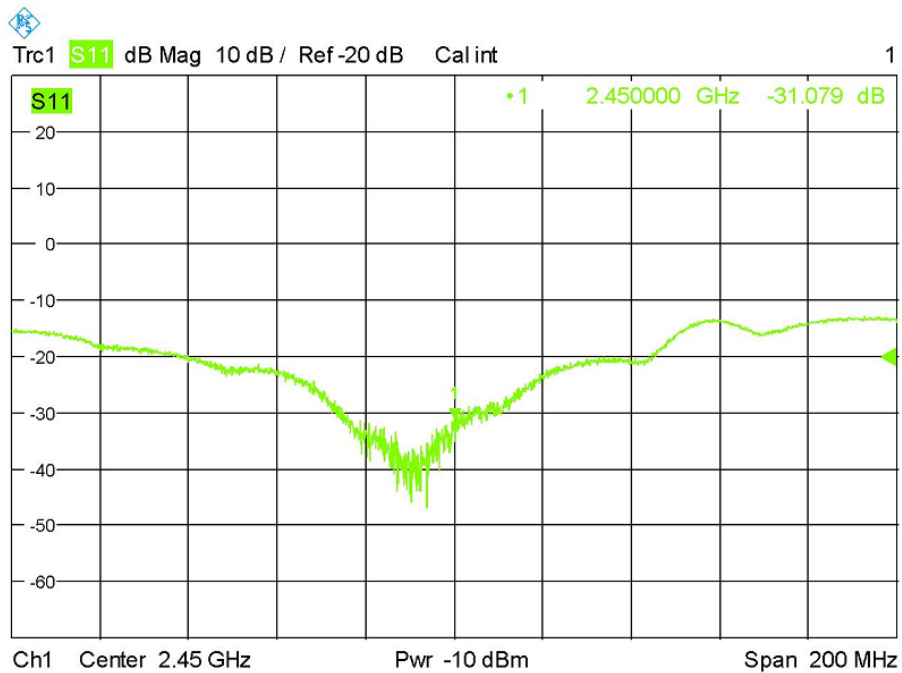

SN 47/14 DIP 2G600-342; 2600Head

Calibrated impedance: $55.5\Omega + 2.6j\Omega$; Measurement impedance: $57.2\Omega + 3.2j\Omega$ (within 5Ω)

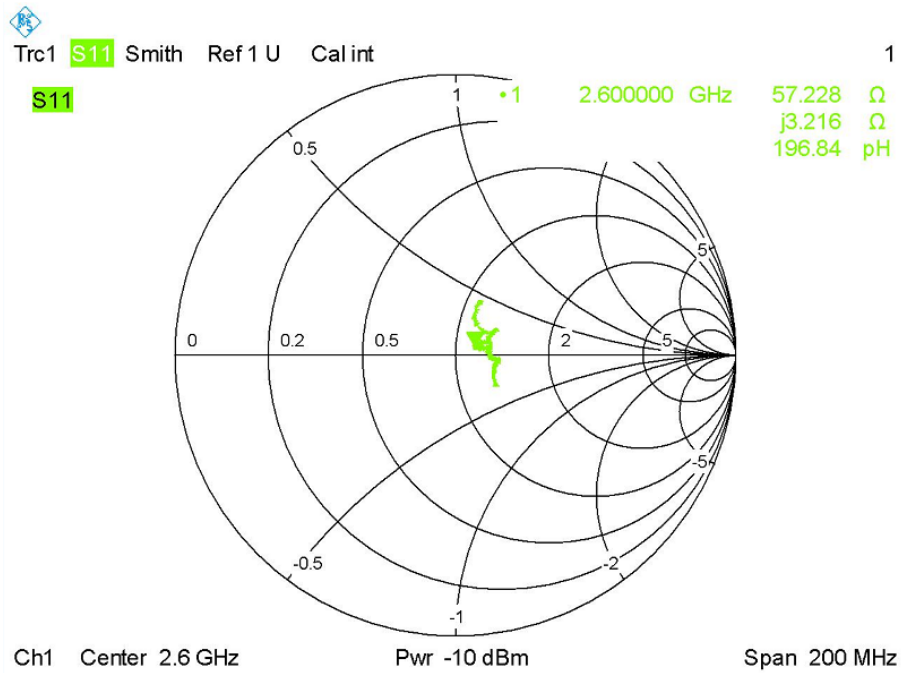

Calibrated return loss: -24.86dB; Measurement return loss: -23.1 dB (within 20%)

