


## APPENDIX

### 11. Photographs of Test Setup




**Fig.1 Photograph of the SAR measurement system**

**Photograph of the tissue simulant fluid liquid depth (Body)**

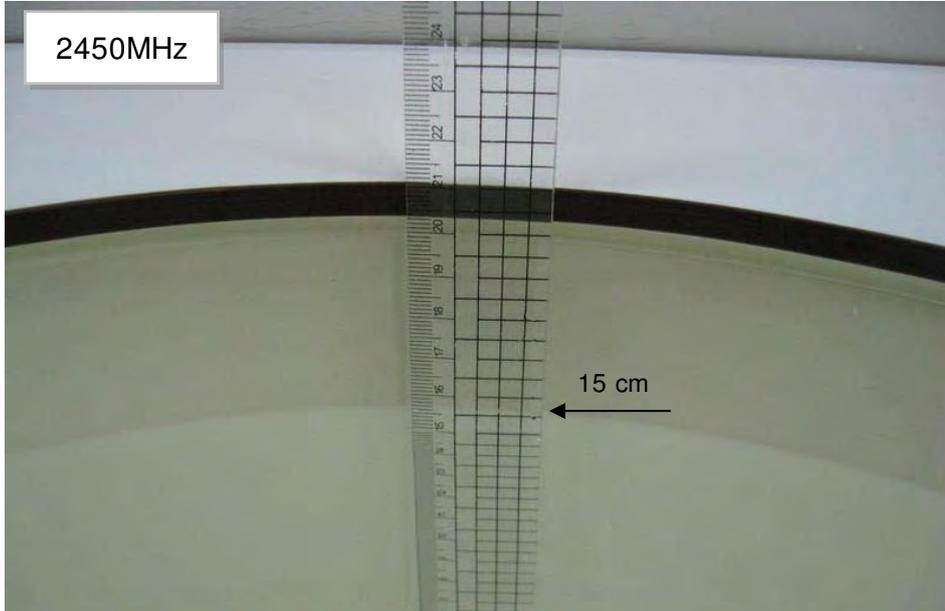


**Fig.2**


**Body - distance between flat phantom and EUT is 0 mm**

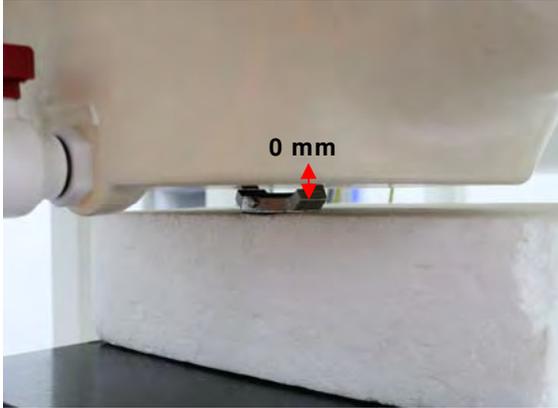

**Fig.3 Configuration 1: remove the watchband and make the watch's back touch against the flat phantom**

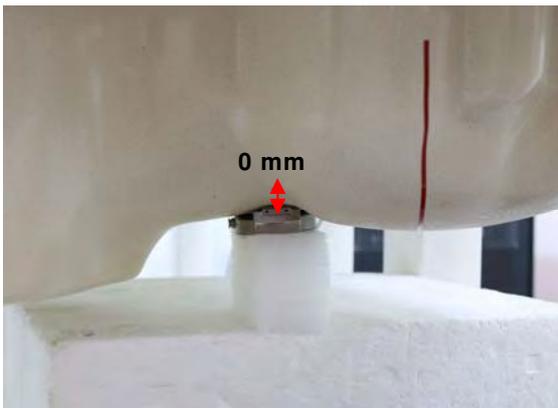

**Fig.4 Configuration 2: remove the watchband and make the watch's back touch against the neck phantom area**

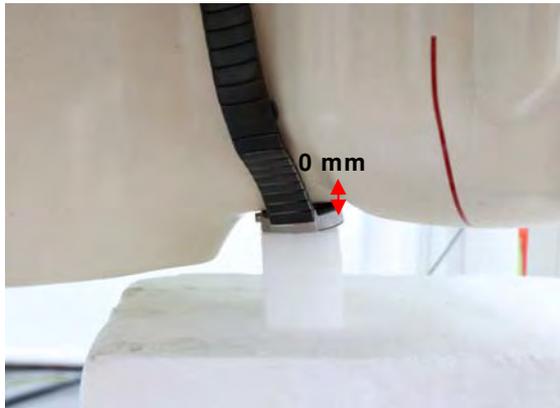

**Fig.5 Configuration 3: remove the one side's watchband and make the watch's back touch against the neck phantom area**

## 12. Photographs of the EUT


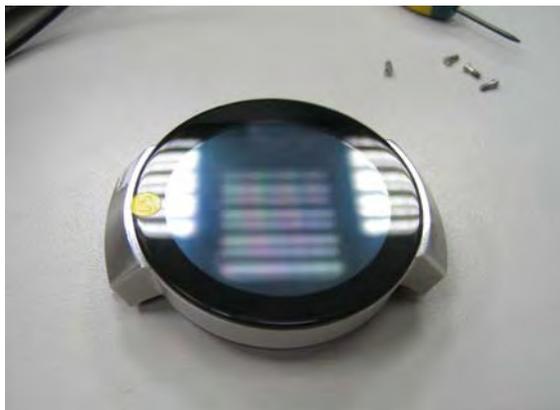


Fig.6 EUT

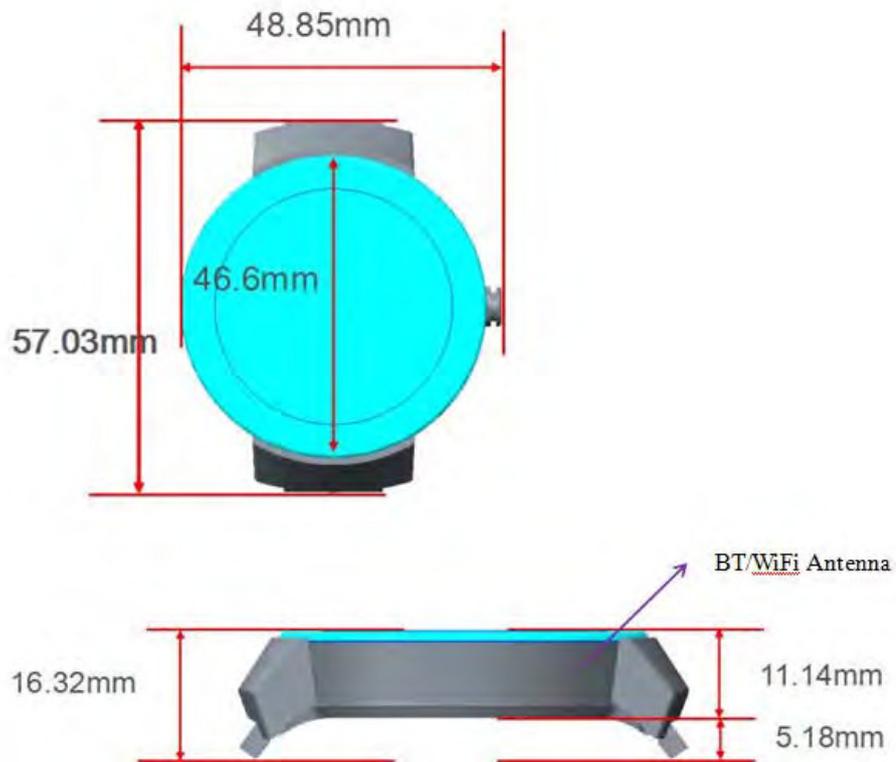

**Fig.7 Antenna location**

**- End of Report -**