

15. Test Plots

15.1 System Performance Check

System check at 750 MHz

Date of measurement: 29/11/2024


A. Experimental conditions.

Probe	SN 26/23 EPGO420
ConvF	0.87
Area Scan	surf_sam_plan.txt
Zoom Scan	5x5x7,dx=8mm dy=8mm dz=5mm
Phantom	Validation plane
Device Position	Dipole
Band	CW750
Signal	CW

B. Permittivity

Frequency (MHz)	750.000
Relative permittivity (real part)	40.272
Relative permittivity (imaginary part)	24.595
Conductivity (S/m)	0.859

C. SAR Surface and Volume

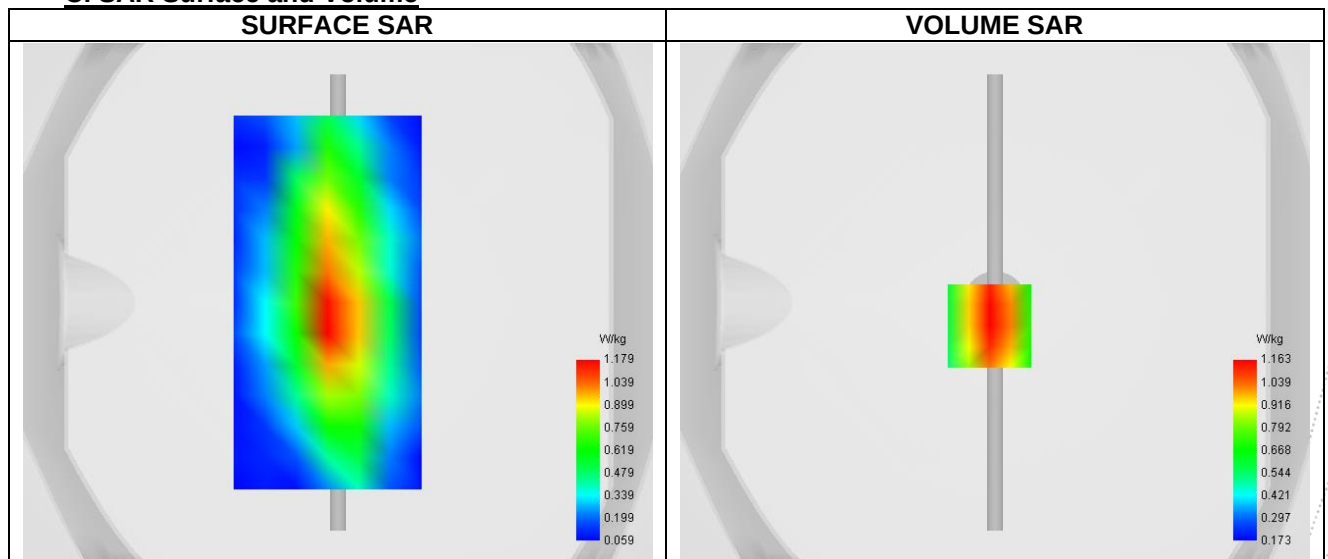

Maximum location: X=-2.00, Y=-9.00 ; SAR Peak: 1.61 W/kg


D. SAR 1g & 10g

SAR 10g (W/Kg)	1.376
SAR 1g (W/Kg)	2.119
Variation (%)	-1.115
Horizontal validation criteria: minimum distance (mm)	0.000000
Vertical validation criteria: SAR ratio M2/M1 (%)	0.000000


E. Z Axis Scan

Z (mm)	0.00	4.00	9.00	14.00	19.00
--------	------	------	------	-------	-------

SAR (W/Kg)	1.603	1.163	0.769	0.506	0.333
------------	-------	-------	-------	-------	-------

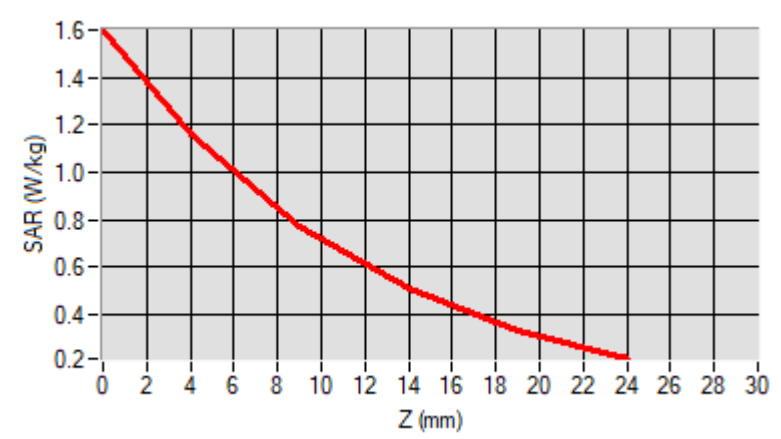

F. 3D Image

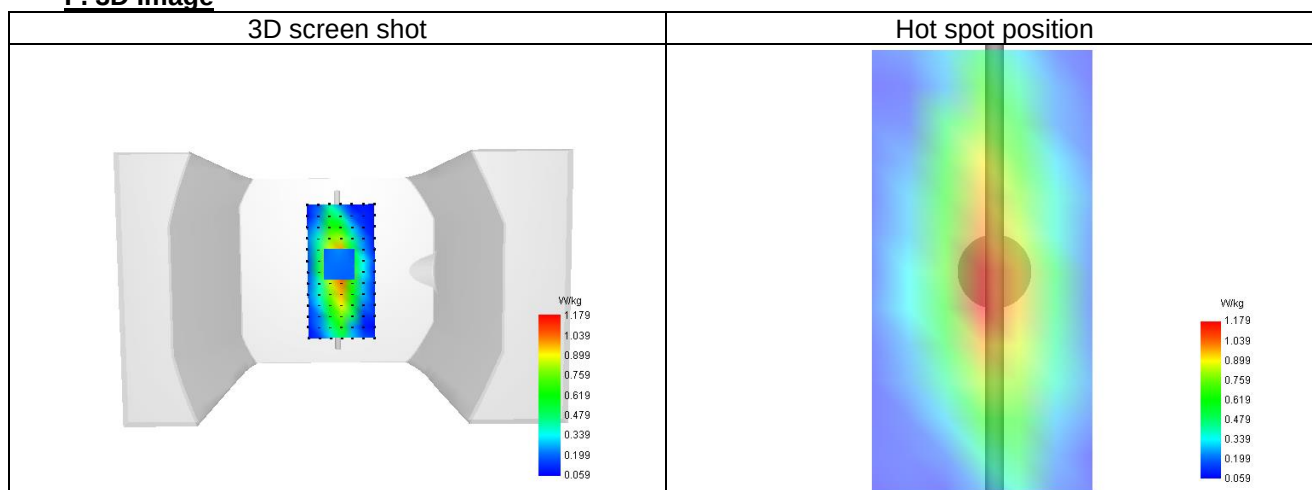

System check at 835 MHz


Date of measurement: 29/11/2024

A. Experimental conditions.

Probe	SN 26/23 EPG0420
ConvF	0.80
Area Scan	surf_sam_plan.txt
Zoom Scan	5x5x7,dx=8mm dy=8mm dz=5mm
Phantom	Validation plane
Device Position	Dipole
Band	CW835
Signal	CW

B. Permittivity

Frequency (MHz)	835.000
Relative permittivity (real part)	40.706
Relative permittivity (imaginary part)	20.910
Conductivity (S/m)	0.869

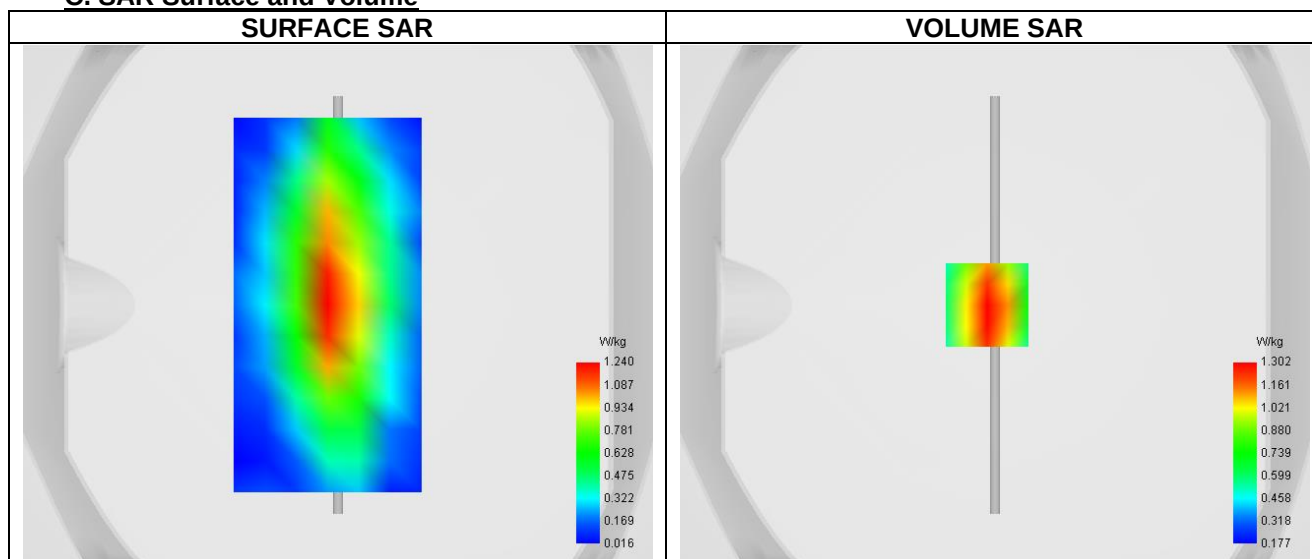C. SAR Surface and Volume


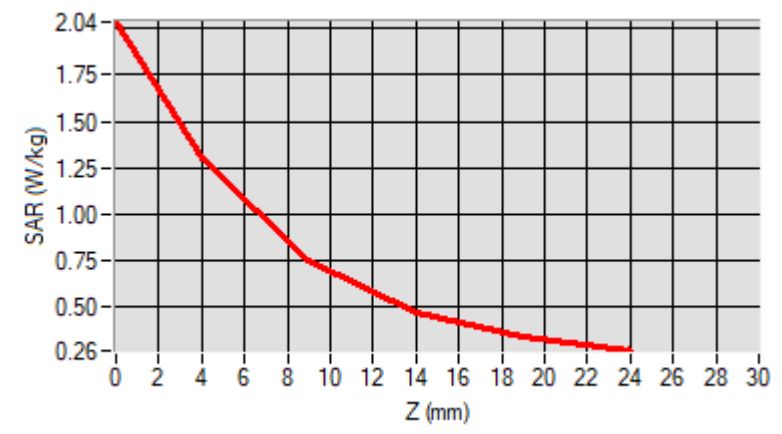
Maximum location: X=-3.00, Y=0.00 ; SAR Peak: 2.06 W/kg

D. SAR 1g & 10g


SAR 10g (W/Kg)	2.572
SAR 1g (W/Kg)	1.238
Variation (%)	-2.280
Horizontal validation criteria: minimum distance (mm)	0.000000
Vertical validation criteria: SAR ratio M2/M1 (%)	0.000000

E. Z Axis Scan

Z (mm)	0.00	4.00	9.00	14.00	19.00
SAR (W/Kg)	2.036	1.302	0.747	0.462	0.331



F. 3D Image

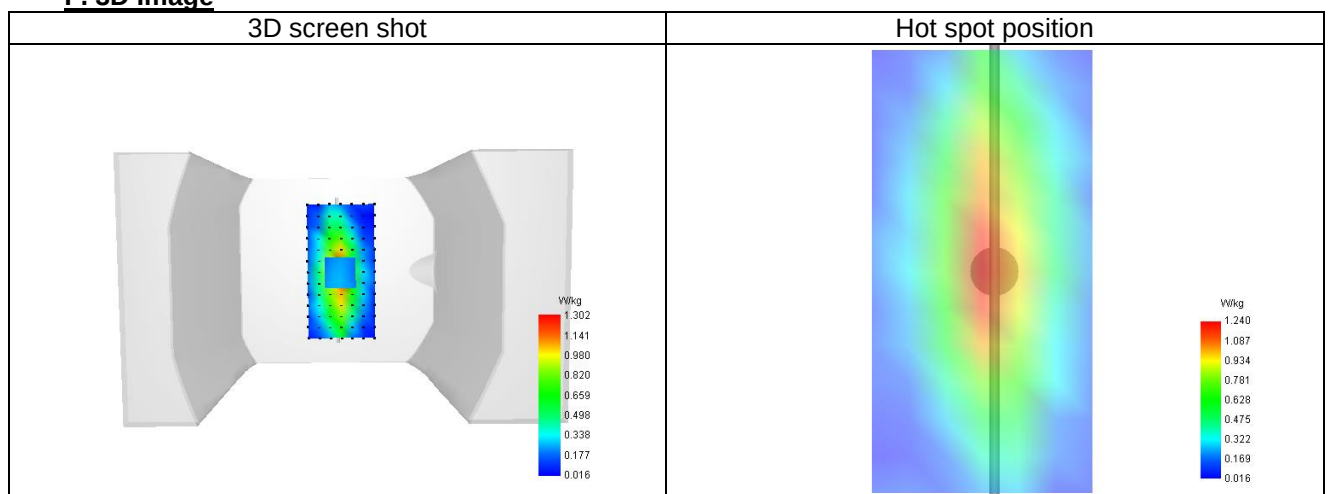

System check at 1800 MHz


Date of measurement: 10/12/2024

A. Experimental conditions.

Probe	SN 26/23 EPGO420
ConvF	1.01
Area Scan	surf_sam_plan.txt
Zoom Scan	5x5x7,dx=8mm dy=8mm dz=5mm
Phantom	Validation plane
Device Position	Dipole
Band	CW1800
Signal	CW

B. Permittivity


Frequency (MHz)	1800.000
Relative permittivity (real part)	39.520
Relative permittivity (imaginary part)	15.200
Conductivity (S/m)	1.369

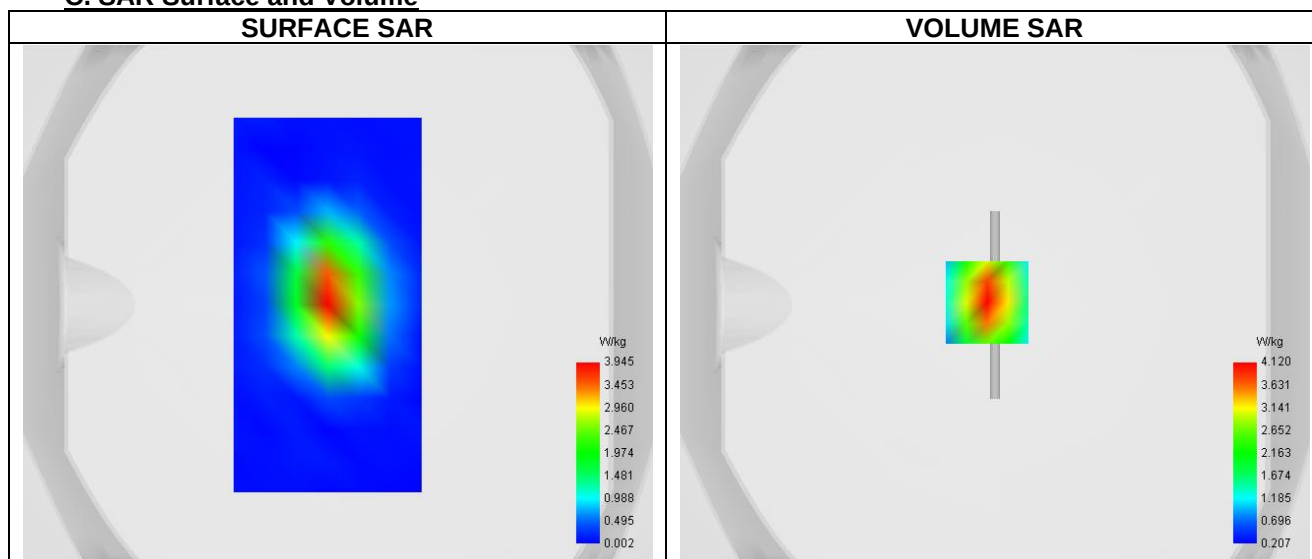C. SAR Surface and Volume

D. SAR 1g & 10g


SAR 10g (W/Kg)	5.368
SAR 1g (W/Kg)	9.830
Variation (%)	1.358
Horizontal validation criteria: minimum distance (mm)	0.000000
Vertical validation criteria: SAR ratio M2/M1 (%)	0.000000

E. Z Axis Scan

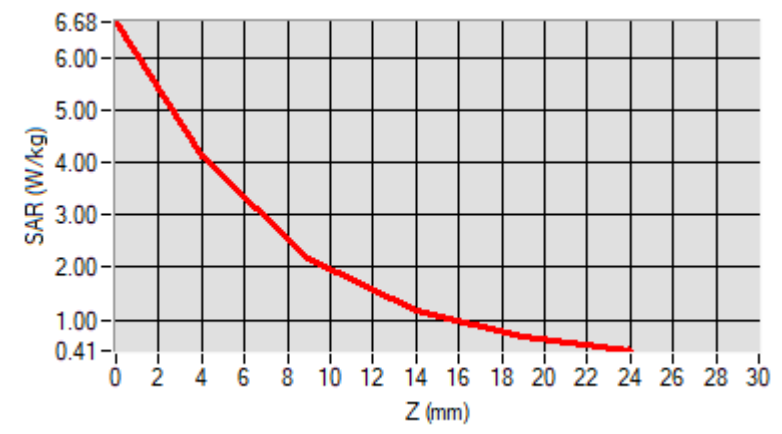Z (mm)	0.00	4.00	9.00	14.00	19.00
SAR (W/Kg)	6.684	4.120	2.184	1.177	0.685



F. 3D Image

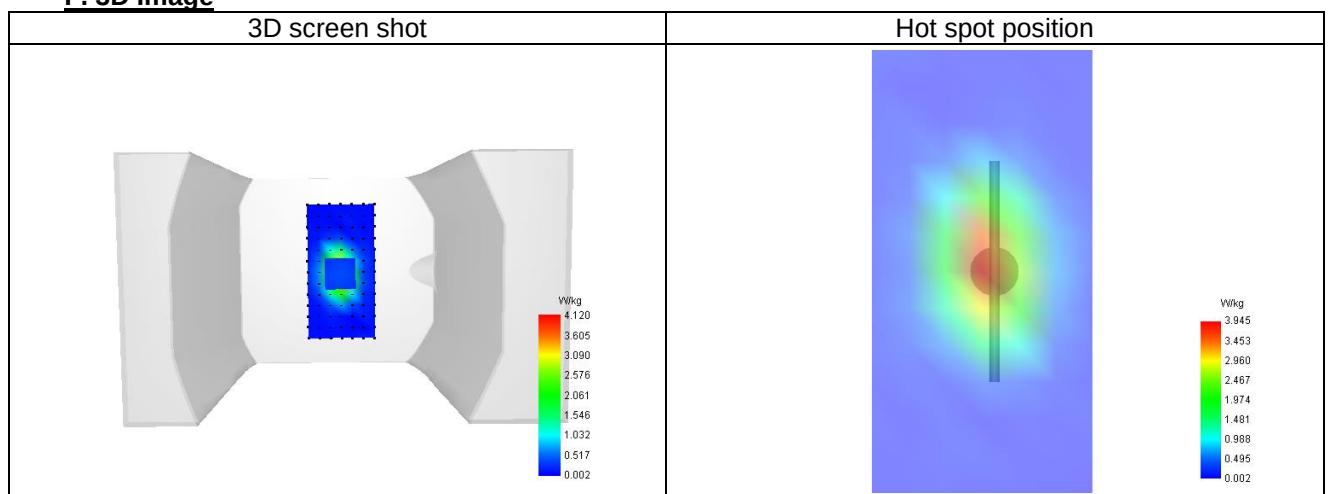

System check at 1900 MHz


Date of measurement: 10/12/2024

A. Experimental conditions.

Probe	SN 26/23 EPGO420
ConvF	1.11
Area Scan	surf_sam_plan.txt
Zoom Scan	5x5x7,dx=8mm dy=8mm dz=5mm
Phantom	Validation plane
Device Position	Dipole
Band	CW1900
Signal	CW

B. Permittivity

Frequency (MHz)	1900.000
Relative permittivity (real part)	38.494
Relative permittivity (imaginary part)	14.400
Conductivity (S/m)	1.412

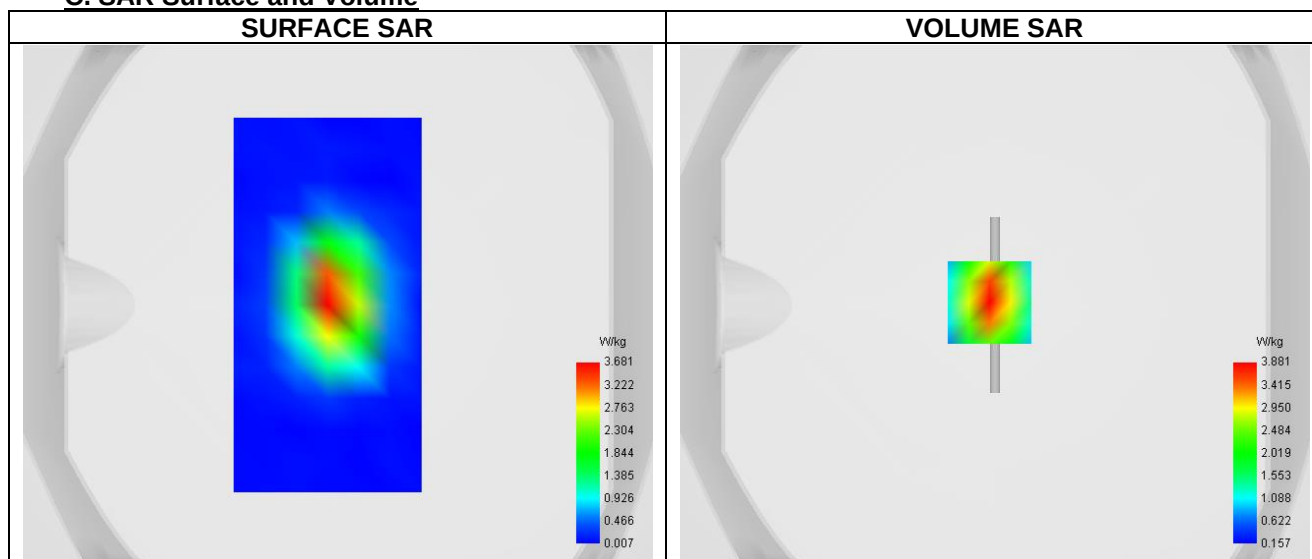C. SAR Surface and Volume


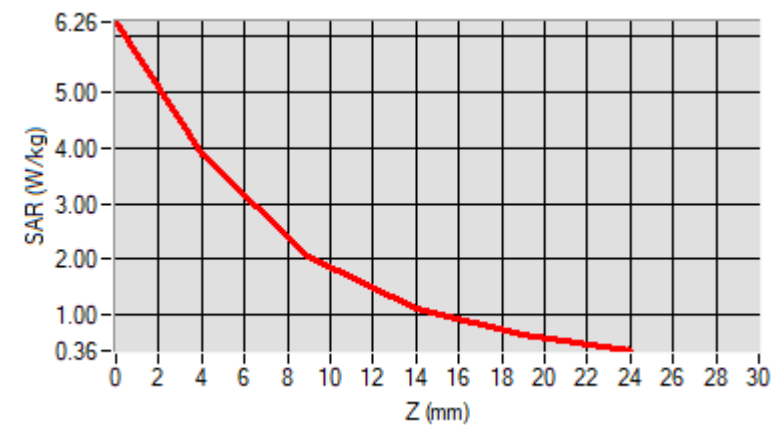
Maximum location: X=-2.00, Y=1.00 ; SAR Peak: 6.27 W/kg

D. SAR 1g & 10g


SAR 10g (W/Kg)	5.362
SAR 1g (W/Kg)	10.106
Variation (%)	1.233
Horizontal validation criteria: minimum distance (mm)	0.000000
Vertical validation criteria: SAR ratio M2/M1 (%)	0.000000

E. Z Axis Scan

Z (mm)	0.00	4.00	9.00	14.00	19.00
SAR (W/Kg)	6.259	3.881	2.069	1.111	0.634



F. 3D Image

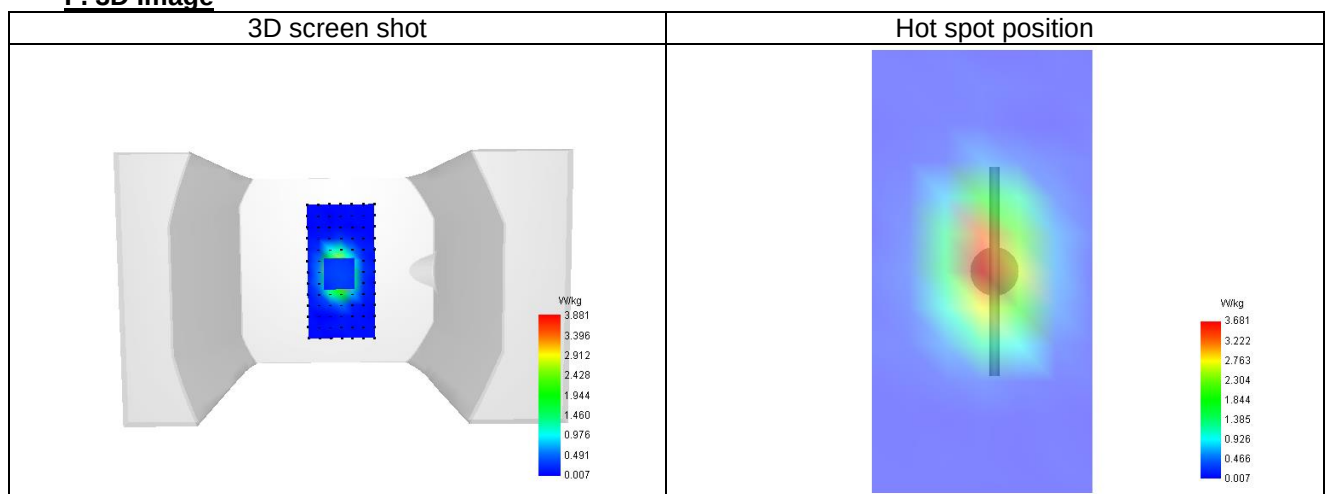

System check at 2100 MHz


Date of measurement: 19/12/2024

A. Experimental conditions.

Probe	SN 26/23 EPGO420
ConvF	1.16
Area Scan	surf_sam_plan.txt
Zoom Scan	5x5x7,dx=8mm dy=8mm dz=5mm
Phantom	Validation plane
Device Position	Dipole
Band	CW2100
Signal	CW

B. Permittivity

Frequency (MHz)	2100.000
Relative permittivity (real part)	38.221
Relative permittivity (imaginary part)	13.824
Conductivity (S/m)	1.526

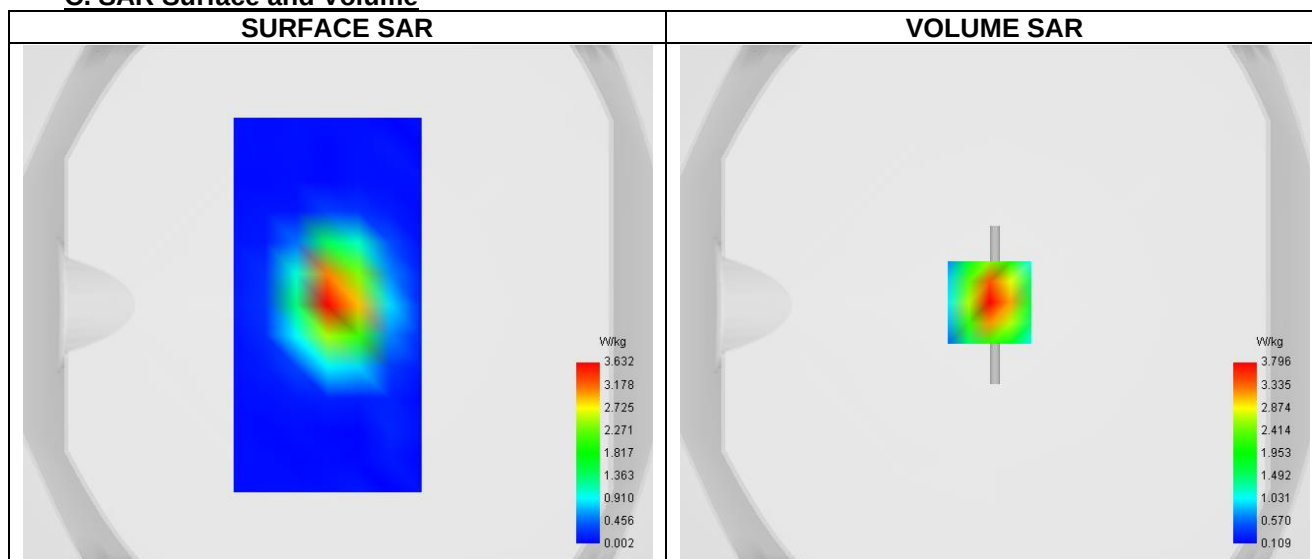C. SAR Surface and Volume


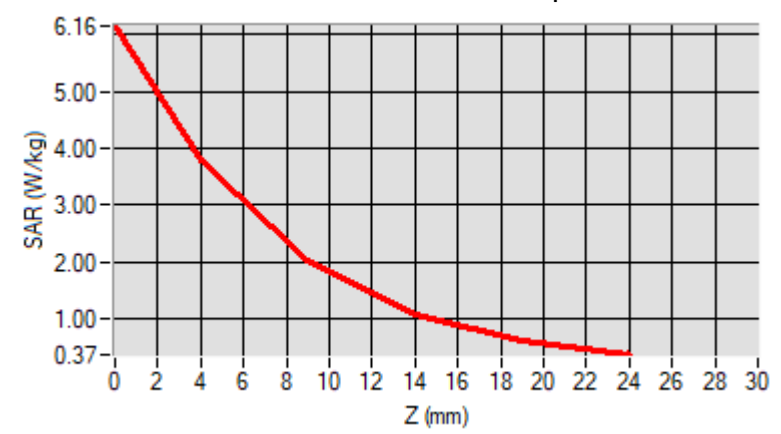
Maximum location: X=-2.00, Y=1.00 ; SAR Peak: 6.20 W/kg

D. SAR 1g & 10g


SAR 10g (W/Kg)	5.638
SAR 1g (W/Kg)	11.333
Variation (%)	3.679
Horizontal validation criteria: minimum distance (mm)	0.000000
Vertical validation criteria: SAR ratio M2/M1 (%)	0.000000

E. Z Axis Scan

Z (mm)	0.00	4.00	9.00	14.00	19.00
SAR (W/Kg)	6.156	3.796	2.013	1.083	0.627



F. 3D Image

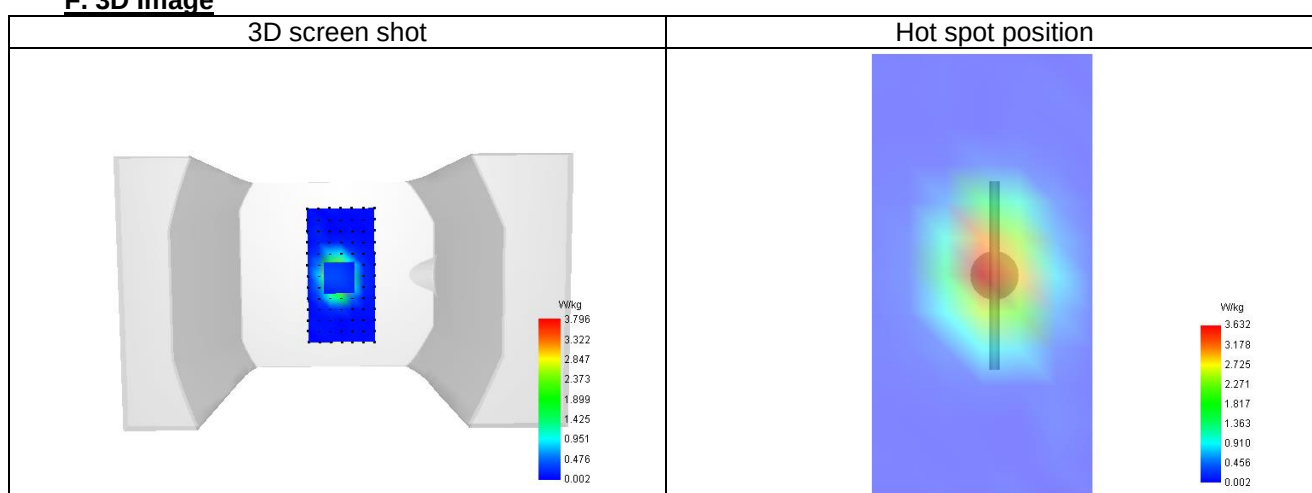

System check at 2450 MHz


Date of measurement: 19/12/2024

A. Experimental conditions.

Probe	SN 26/23 EPGO420
ConvF	1.32
Area Scan	surf_sam_plan.txt
Zoom Scan	7x7x12,dx=8mm dy=8mm dz=5mm
Phantom	Validation plane
Device Position	Dipole
Band	CW2450
Signal	CW

B. Permittivity

Frequency (MHz)	2450.000
Relative permittivity (real part)	40.339
Relative permittivity (imaginary part)	14.330
Conductivity (S/m)	1.796

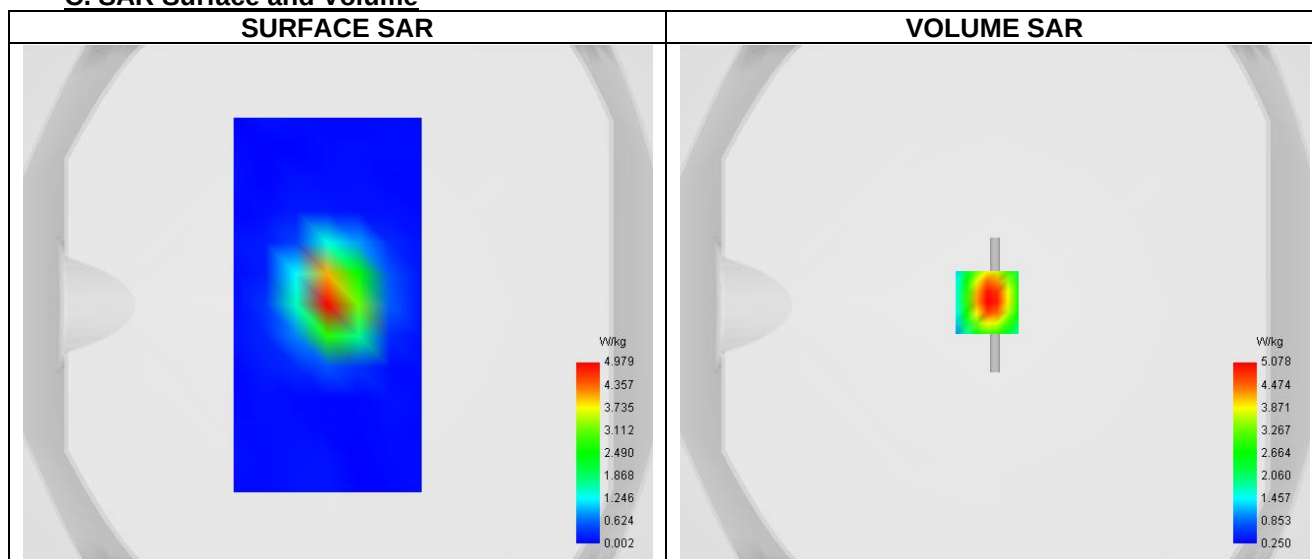C. SAR Surface and Volume


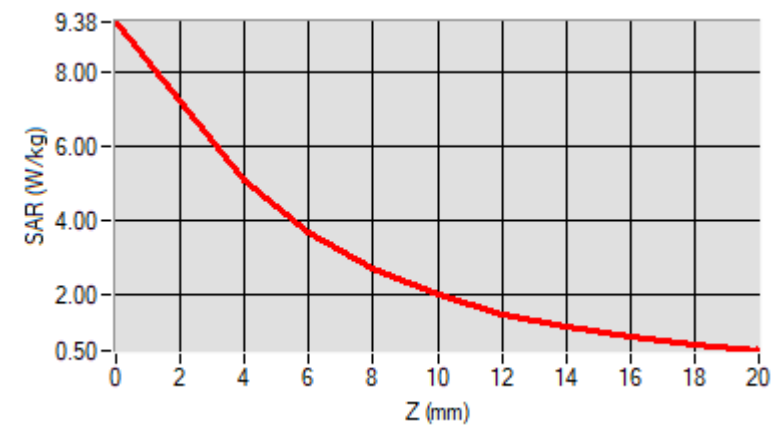
Maximum location: X=-3.00, Y=1.00 ; SAR Peak: 9.50 W/kg

D. SAR 1g & 10g


SAR 10g (W/Kg)	6.246
SAR 1g (W/Kg)	13.943
Variation (%)	-2.070
Horizontal validation criteria: minimum distance (mm)	0.000000
Vertical validation criteria: SAR ratio M2/M1 (%)	0.000000

E. Z Axis Scan

Z (mm)	0.00	4.00	6.00	8.00	10.00	12.00	14.00	16.00	18.00
SAR (W/Kg)	9.380	5.078	3.712	2.709	2.001	1.499	1.138	0.871	0.667



F. 3D Image

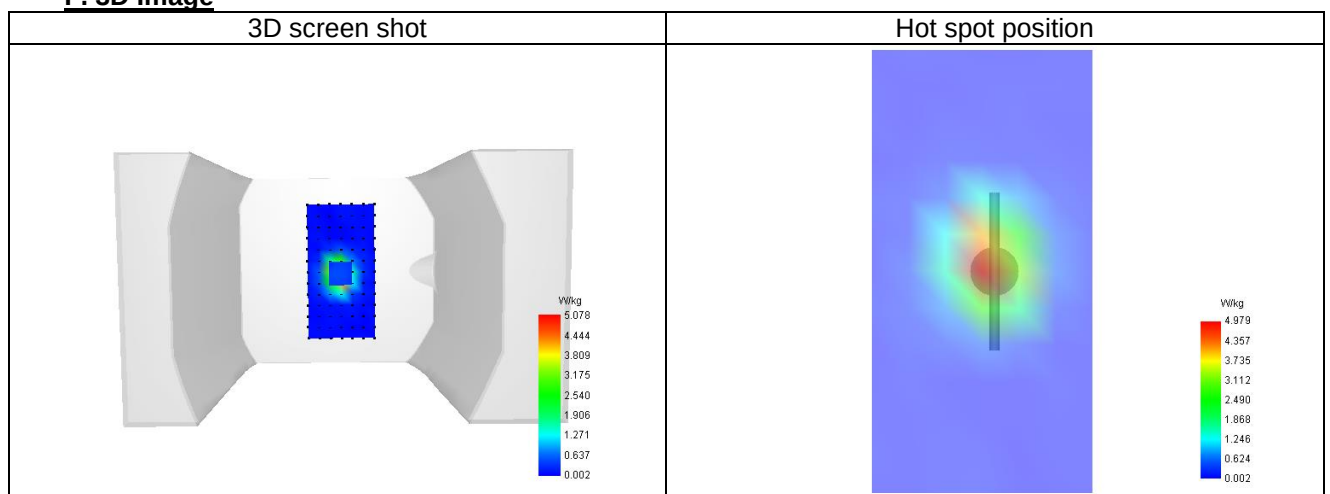

System check at 2600 MHz


Date of measurement: 19/12/2024

A. Experimental conditions.

Probe	SN 26/23 EPGO420
ConvF	1.19
Area Scan	surf_sam_plan.txt
Zoom Scan	5x5x7,dx=8mm dy=8mm dz=5mm
Phantom	Validation plane
Device Position	Dipole
Band	CW2600
Signal	CW

B. Permittivity

Frequency (MHz)	2600.000
Relative permittivity (real part)	39.432
Relative permittivity (imaginary part)	14.889
Conductivity (S/m)	2.014

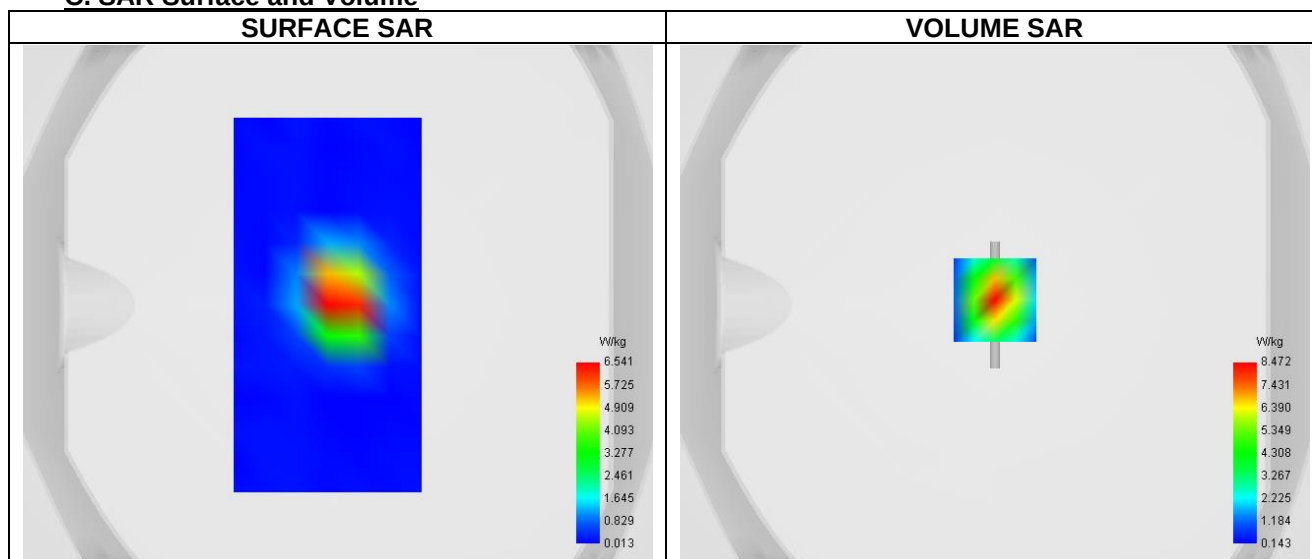C. SAR Surface and Volume


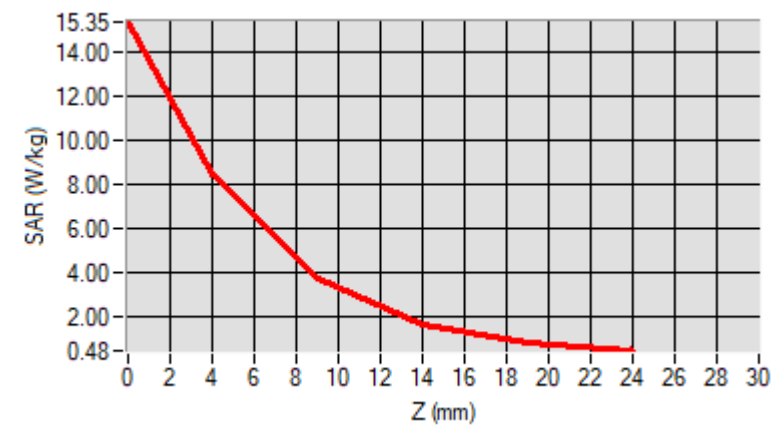
Maximum location: X=0.00, Y=2.00 ; SAR Peak: 15.35 W/kg

D. SAR 1g & 10g


SAR 10g (W/Kg)	6.234
SAR 1g (W/Kg)	13.429
Variation (%)	3.063
Horizontal validation criteria: minimum distance (mm)	0.000000
Vertical validation criteria: SAR ratio M2/M1 (%)	0.000000

E. Z Axis Scan

Z (mm)	0.00	4.00	9.00	14.00	19.00
SAR (W/Kg)	15.347	8.472	3.768	1.677	0.856



F. 3D Image

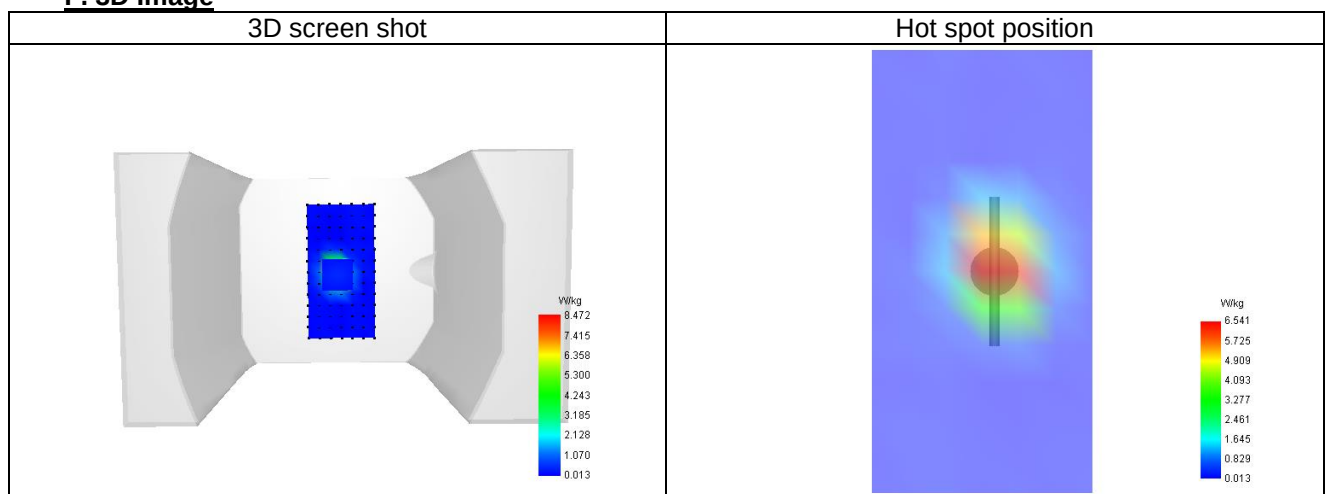

15.2 SAR Test Graph Results

Plot 1

Date of measurement: 19/12/2024


A. Experimental conditions.

Probe	SN 26/23 EPGO420
ConvF	1.11
Area Scan	surf_sam_plan.txt
Zoom Scan	5x5x7,dx=8mm dy=8mm dz=5.0mm
Phantom	Validation plane
Device Position	Body
Band	ISM
Signal	IEEE 802.11 b

B. Permittivity

Frequency (MHz)	2412.000
Relative permittivity (real part)	40.339
Relative permittivity (imaginary part)	13.182
Conductivity (S/m)	1.796

C. SAR Surface and Volume

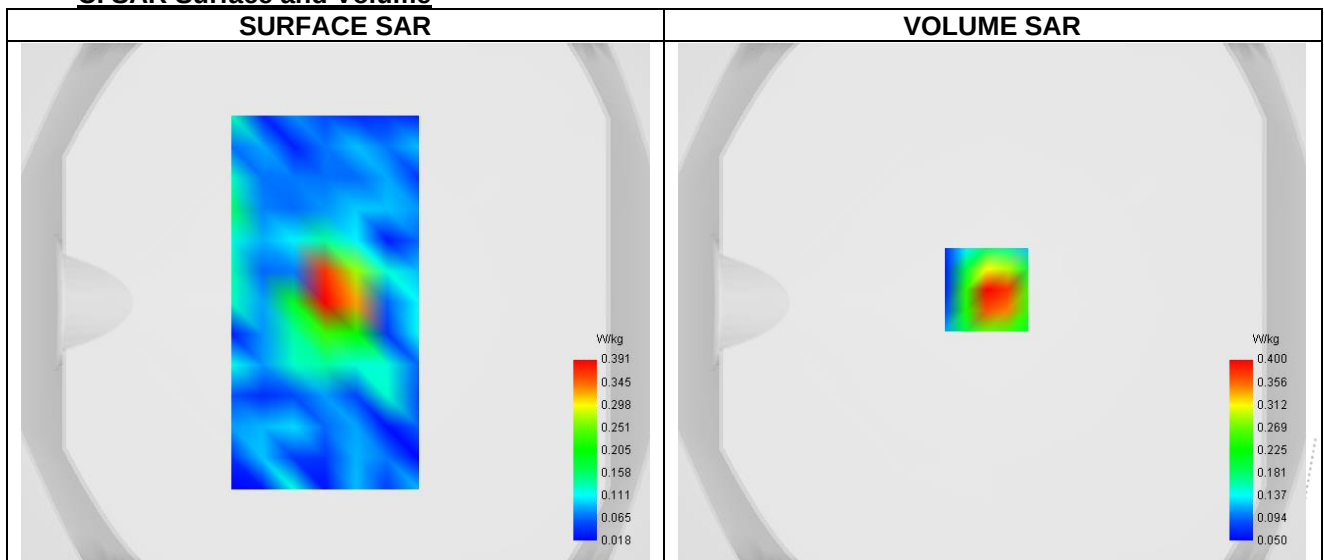


D. SAR 1g & 10g


SAR 10g (W/Kg)	0.108
SAR 1g (W/Kg)	0.287
Variation (%)	-1.820
Horizontal validation criteria: minimum distance (mm)	0.000000
Vertical validation criteria: SAR ratio M2/M1 (%)	0.000000

E. Z Axis Scan

Z (mm)	0.00	4.00	9.00	14.00	19.00
SAR (W/Kg)	0.632	0.400	0.229	0.145	0.110

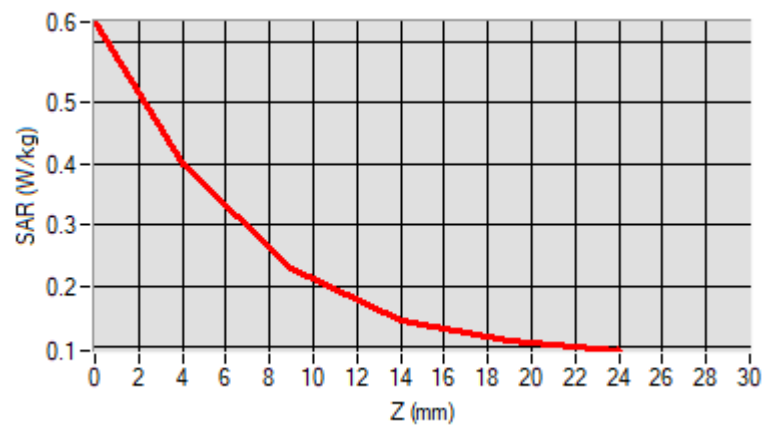

F. 3D Image

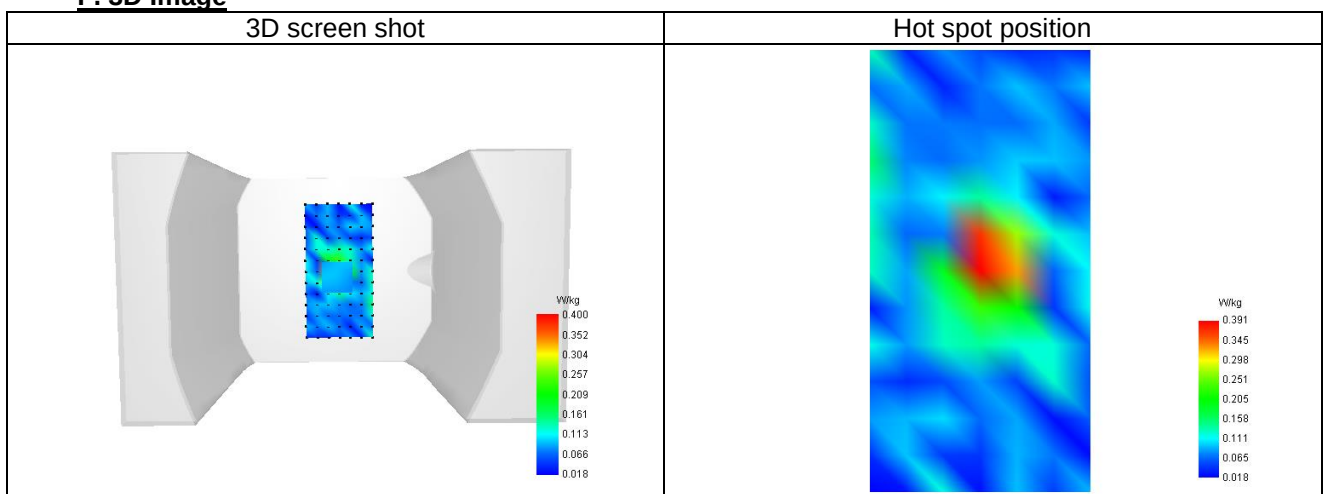

Plot 2


Date of measurement: 29/11/2024

A. Experimental conditions.

Probe	SN 26/23 EPGO420
ConvF	0.81
Area Scan	surf_sam_plan.txt
Zoom Scan	5x5x7,dx=8mm dy=8mm dz=5.0mm
Phantom	Validation plane
Device Position	Body
Band	GPRS850
Signal	TDMA (GPRS)

B. Permittivity

Frequency (MHz)	848.800
Relative permittivity (real part)	40.272
Relative permittivity (imaginary part)	19.400
Conductivity (S/m)	0.859

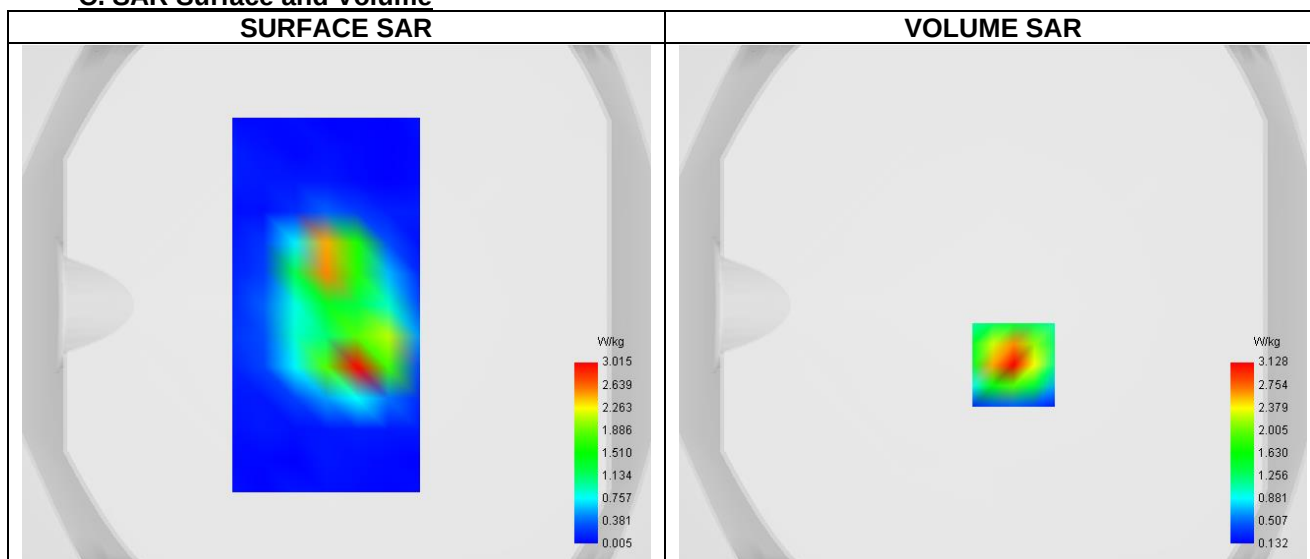C. SAR Surface and Volume


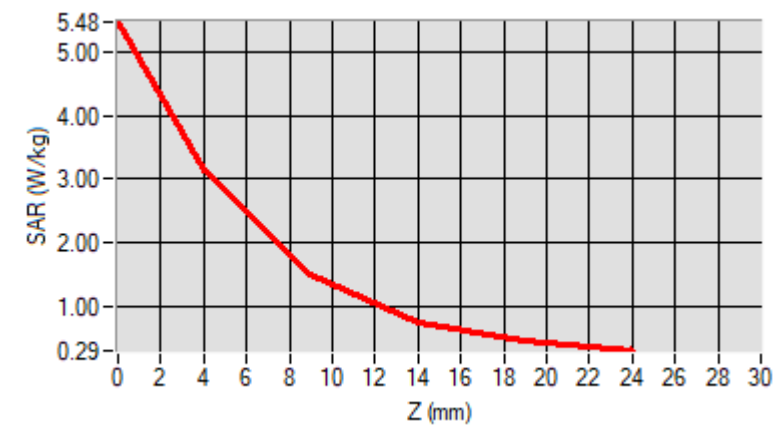
Maximum location: X=8.00, Y=-23.00 ; SAR Peak: 5.55 W/kg

D. SAR 1g & 10g


SAR 10g (W/Kg)	1.393
SAR 1g (W/Kg)	2.906
Variation (%)	3.690
Horizontal validation criteria: minimum distance (mm)	0.000000
Vertical validation criteria: SAR ratio M2/M1 (%)	0.000000

E. Z Axis Scan

Z (mm)	0.00	4.00	9.00	14.00	19.00
SAR (W/Kg)	5.476	3.128	1.490	0.740	0.437



F. 3D Image

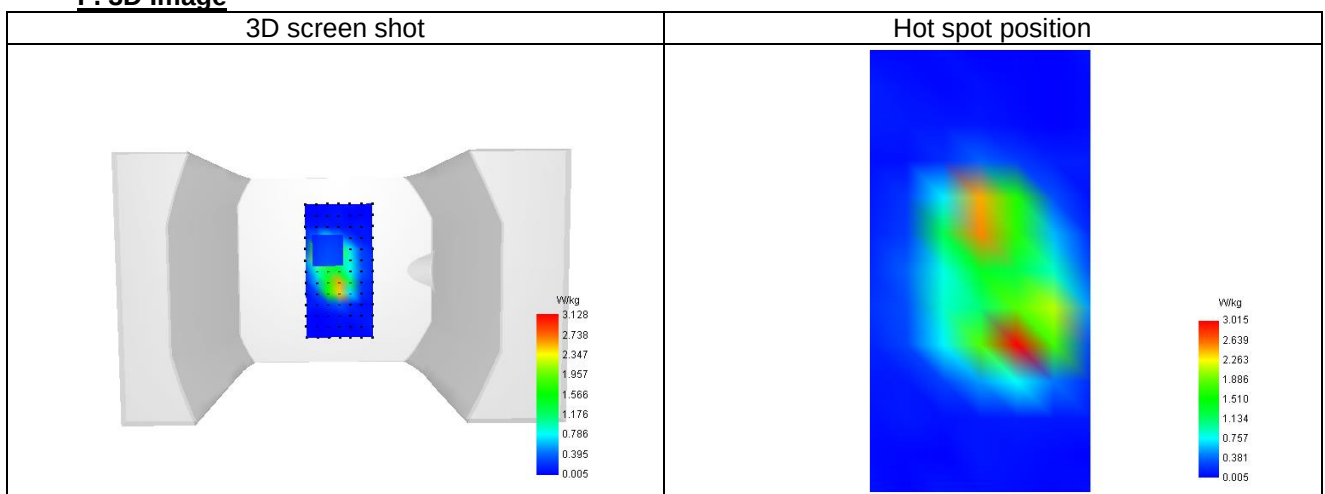

Plot 3


Date of measurement: 10/12/2024

A. Experimental conditions.

Probe	SN 26/23 EPGO420
ConvF	1.04
Area Scan	surf_sam_plan.txt
Zoom Scan	5x5x7,dx=8mm dy=8mm dz=5.0mm
Phantom	Validation plane
Device Position	Body
Band	GPRS1900
Signal	TDMA (GPRS)

B. Permittivity

Frequency (MHz)	1880.000
Relative permittivity (real part)	38.494
Relative permittivity (imaginary part)	13.408
Conductivity (S/m)	1.412

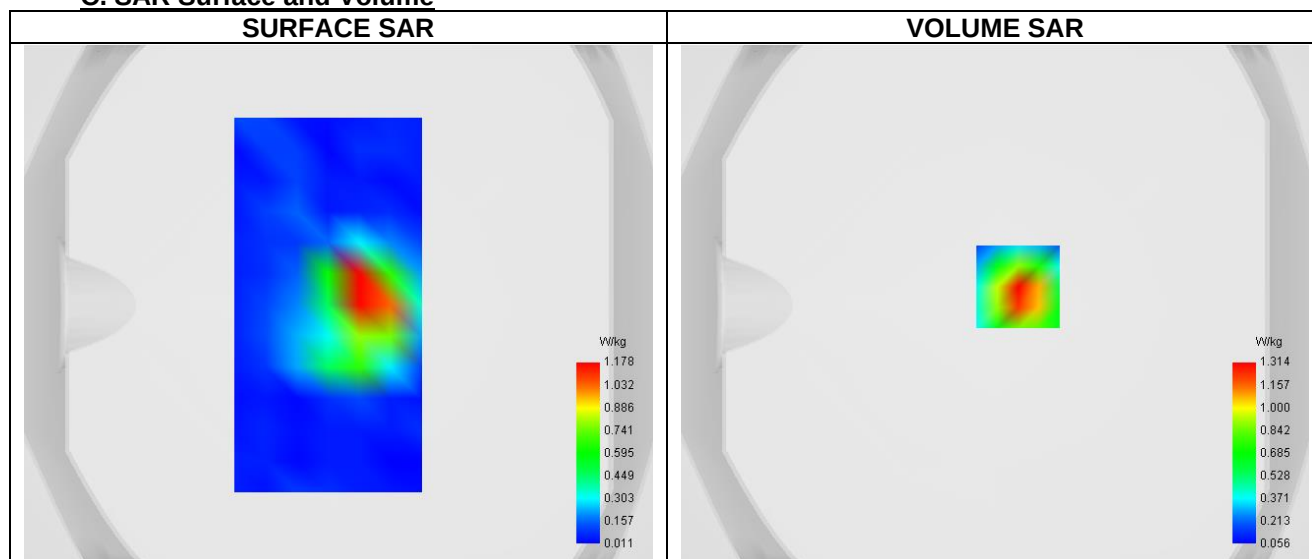C. SAR Surface and Volume


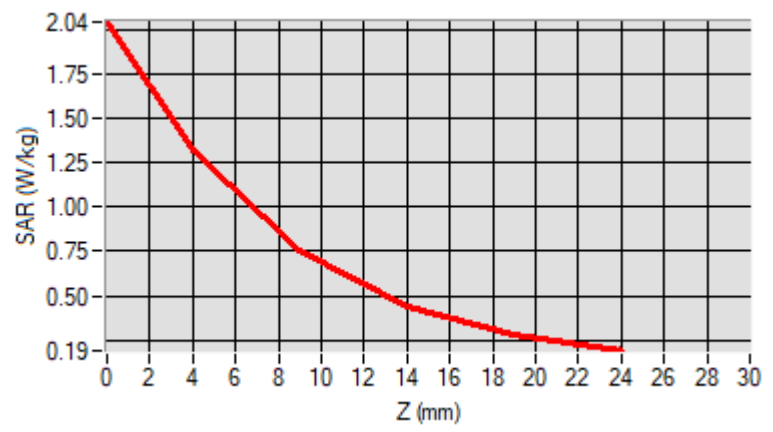
Maximum location: X=10.00, Y=7.00 ; SAR Peak: 2.22 W/kg

D. SAR 1g & 10g


SAR 10g (W/Kg)	0.671
SAR 1g (W/Kg)	1.266
Variation (%)	-0.150
Horizontal validation criteria: minimum distance (mm)	0.000000
Vertical validation criteria: SAR ratio M2/M1 (%)	0.000000

E. Z Axis Scan

Z (mm)	0.00	4.00	9.00	14.00	19.00
SAR (W/Kg)	2.140	1.336	0.739	0.440	0.305



F. 3D Image

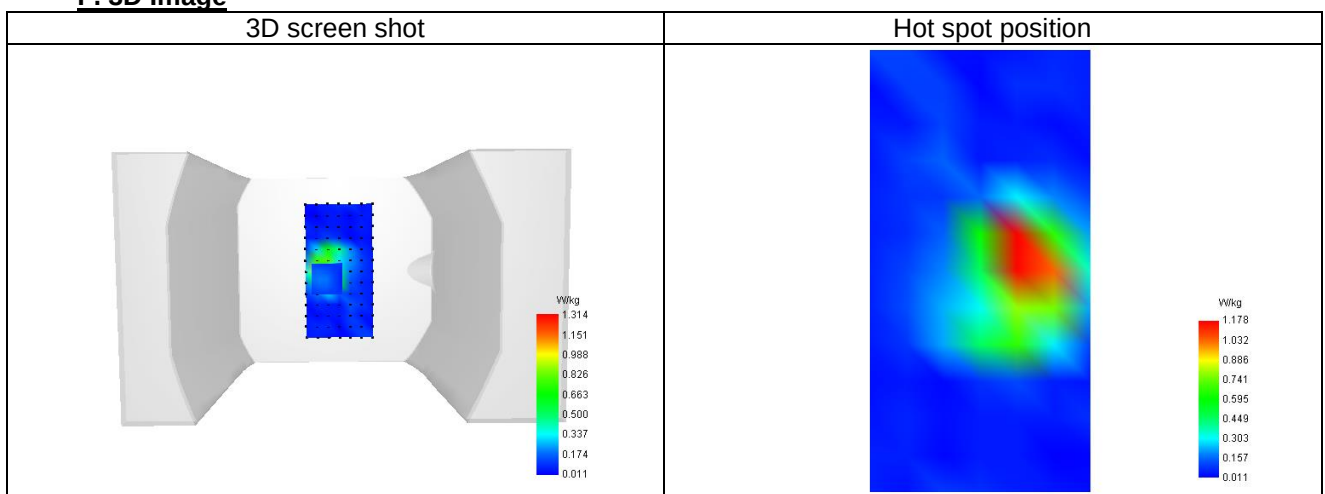

Plot 4


Date of measurement: 10/12/2024

A. Experimental conditions.

Probe	SN 26/23 EPGO420
ConvF	1.04
Area Scan	surf_sam_plan.txt
Zoom Scan	5x5x7,dx=8mm dy=8mm dz=5.0mm
Phantom	Validation plane
Device Position	Body
Band	Band 2 (1900)
Signal	WCDMA
Mode	Release 99
Connection Type	RMC, 12.2 kbps

B. Permittivity

Frequency (MHz)	1907.600
Relative permittivity (real part)	38.494
Relative permittivity (imaginary part)	13.210
Conductivity (S/m)	1.412

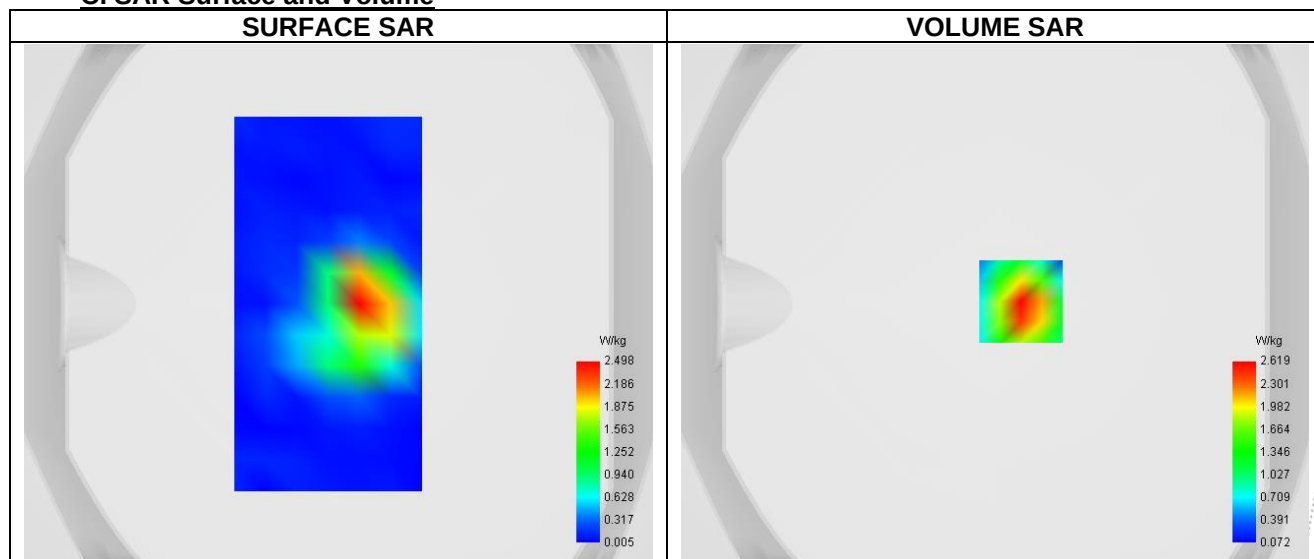C. SAR Surface and Volume


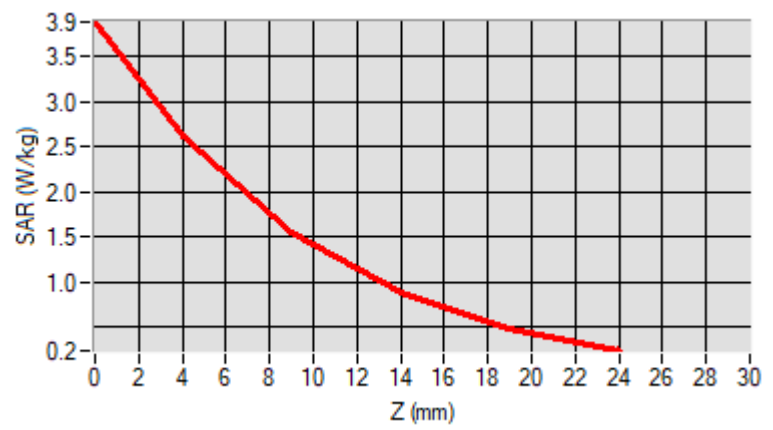
Maximum location: X=10.00, Y=1.00 ; SAR Peak: 3.98 W/kg

D. SAR 1g & 10g


SAR 10g (W/Kg)	1.281
SAR 1g (W/Kg)	2.441
Variation (%)	0.670
Horizontal validation criteria: minimum distance (mm)	0.000000
Vertical validation criteria: SAR ratio M2/M1 (%)	0.000000

E. Z Axis Scan

Z (mm)	0.00	4.00	9.00	14.00	19.00
SAR (W/Kg)	3.882	2.619	1.547	0.883	0.484



F. 3D Image

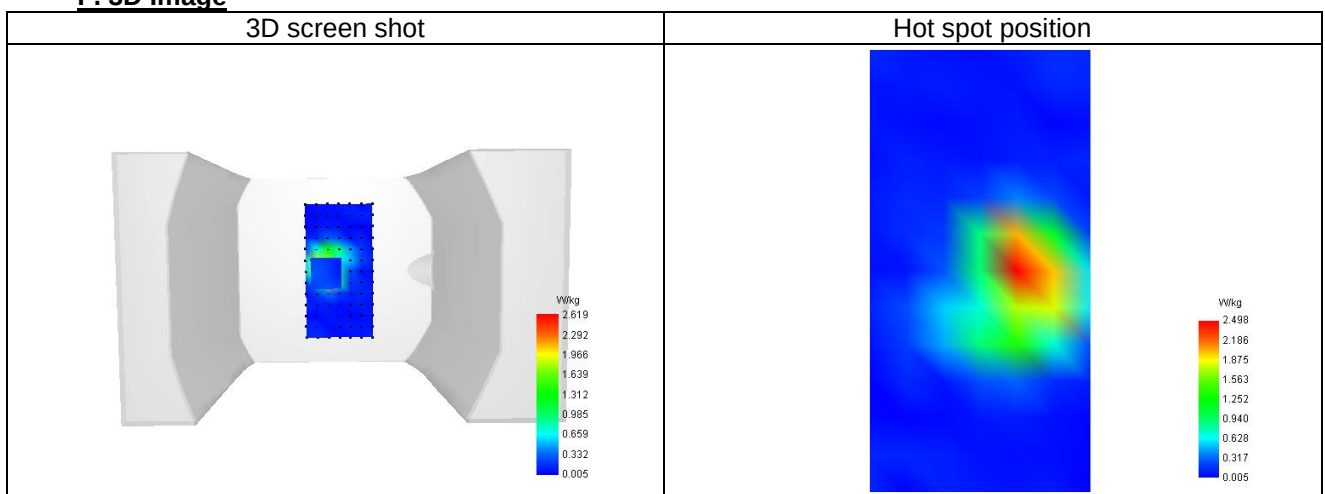

Plot 5


Date of measurement: 10/12/2024

A. Experimental conditions.

Probe	SN 26/23 EPGO420
ConvF	0.96
Area Scan	surf_sam_plan.txt
Zoom Scan	5x5x7,dx=8mm dy=8mm dz=5.0mm
Phantom	Validation plane
Device Position	Body
Band	Band 4 (1700)
Signal	WCDMA
Mode	Release 99
Connection Type	RMC, 12.2 kbps

B. Permittivity


Frequency (MHz)	1752.600
Relative permittivity (real part)	39.520
Relative permittivity (imaginary part)	14.085
Conductivity (S/m)	1.369

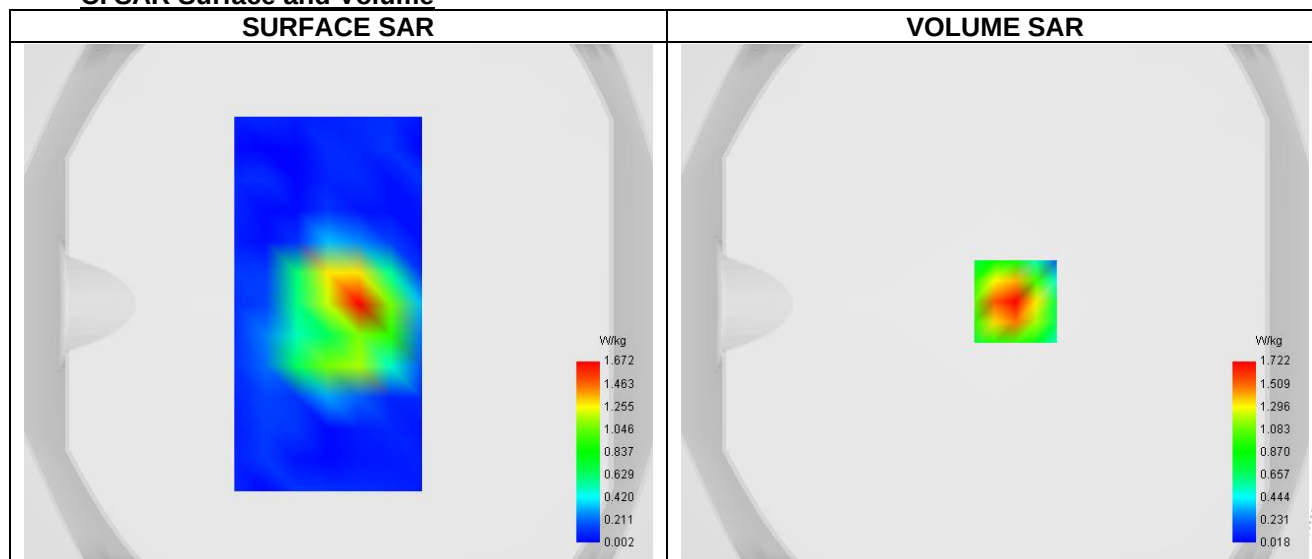C. SAR Surface and Volume

D. SAR 1g & 10g


SAR 10g (W/Kg)	0.908
SAR 1g (W/Kg)	1.606
Variation (%)	-0.170
Horizontal validation criteria: minimum distance (mm)	0.000000
Vertical validation criteria: SAR ratio M2/M1 (%)	0.000000

E. Z Axis Scan

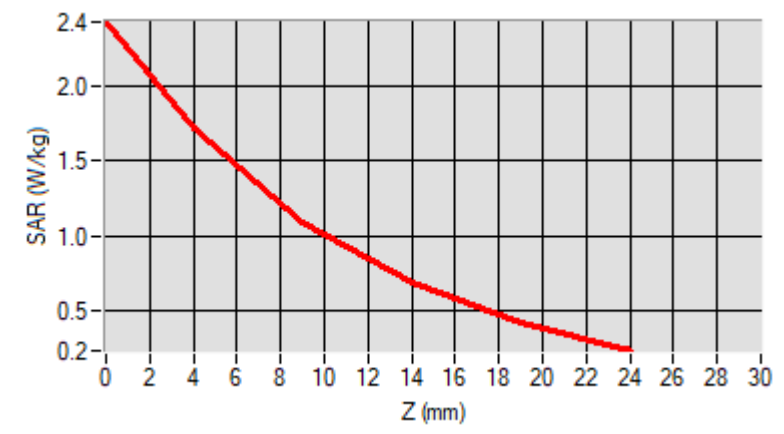Z (mm)	0.00	4.00	9.00	14.00	19.00
SAR (W/Kg)	2.431	1.722	1.093	0.679	0.411



F. 3D Image

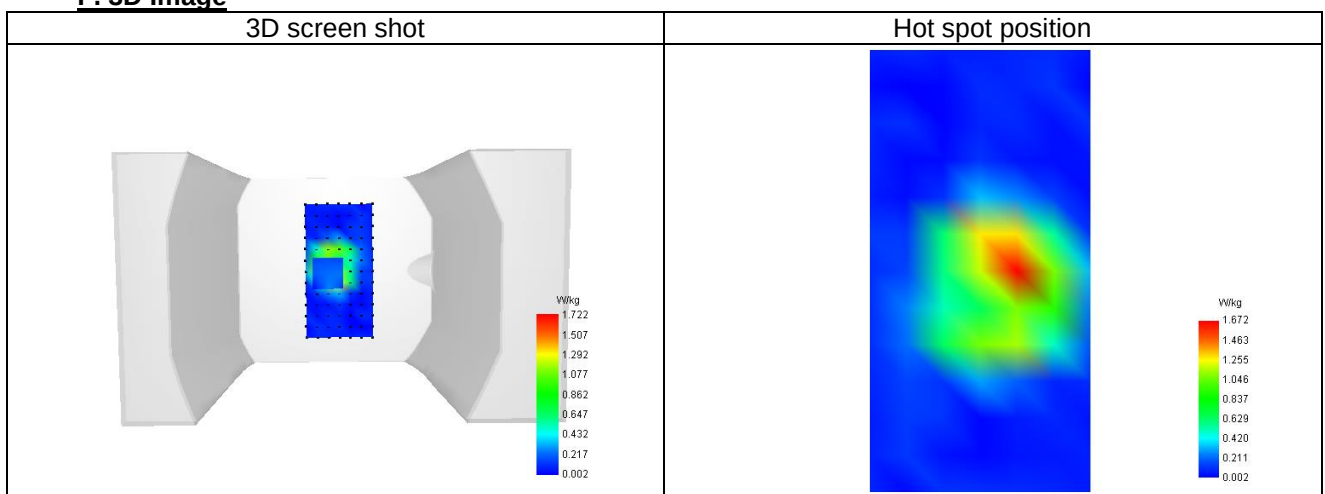

Plot 6


Date of measurement: 29/11/2024

A. Experimental conditions.

Probe	SN 26/23 EPGO420
ConvF	0.81
Area Scan	surf_sam_plan.txt
Zoom Scan	5x5x7,dx=8mm dy=8mm dz=5.0mm
Phantom	Validation plane
Device Position	Body
Band	Band 5 (850)
Signal	WCDMA
Mode	Release 99
Connection Type	RMC, 12.2 kbps

B. Permittivity

Frequency (MHz)	836.400
Relative permittivity (real part)	40.706
Relative permittivity (imaginary part)	19.598
Conductivity (S/m)	0.869

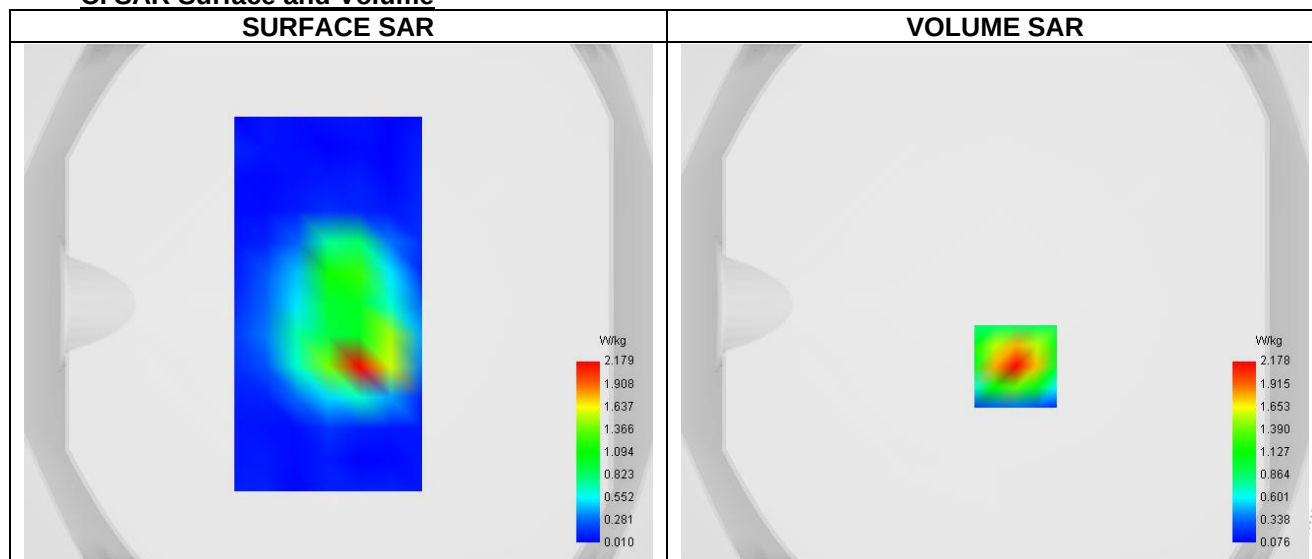C. SAR Surface and Volume


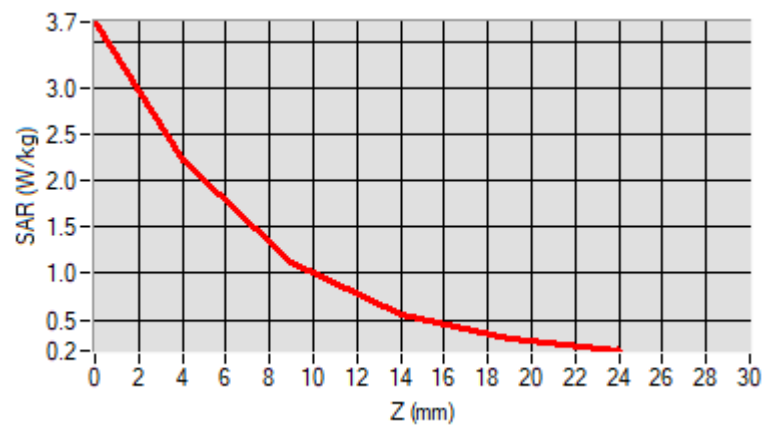
Maximum location: X=8.00, Y=-24.00 ; SAR Peak: 3.74 W/kg

D. SAR 1g & 10g


SAR 10g (W/Kg)	0.983
SAR 1g (W/Kg)	2.038
Variation (%)	3.410
Horizontal validation criteria: minimum distance (mm)	0.000000
Vertical validation criteria: SAR ratio M2/M1 (%)	0.000000

E. Z Axis Scan

Z (mm)	0.00	4.00	9.00	14.00	19.00
SAR (W/Kg)	3.712	2.213	1.111	0.559	0.303



F. 3D Image

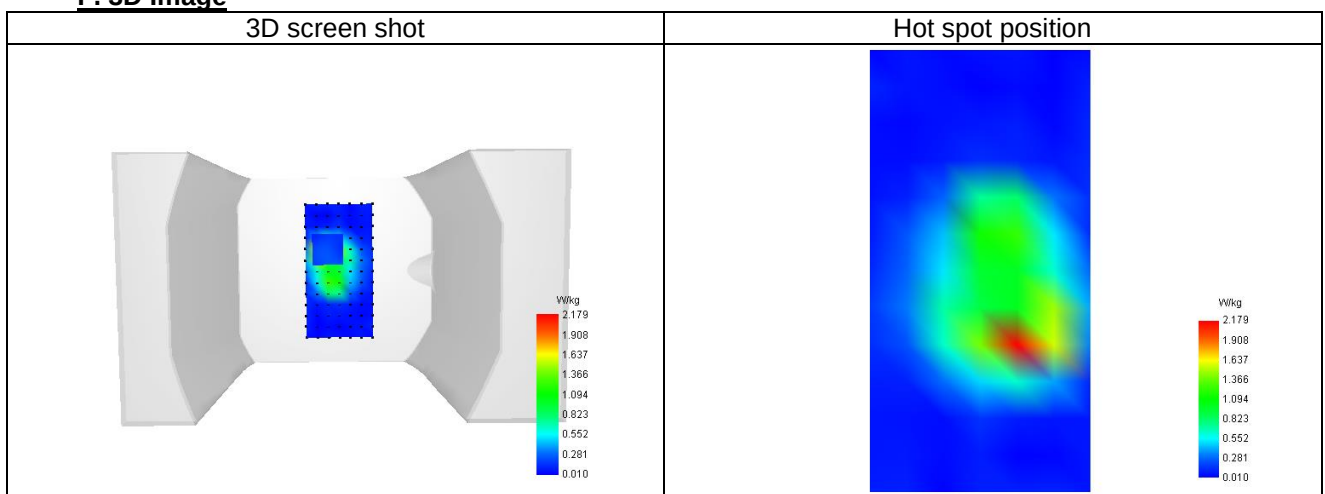

Plot 7


Date of measurement: 10/12/2024

A. Experimental conditions.

Probe	SN 26/23 EPGO420
ConvF	1.04
Area Scan	surf_sam_plan.txt
Zoom Scan	5x5x7,dx=8mm dy=8mm dz=5.0mm
Phantom	Validation plane
Device Position	Body
Band	LTE band 2
Signal	LTE FDD
Cell Bandwidth	20 Mhz
Modulation	SC-OFDM - QPSK
RB offset	5
RB size	20

B. Permittivity

Frequency (MHz)	1880.000
Relative permittivity (real part)	38.494
Relative permittivity (imaginary part)	13.455
Conductivity (S/m)	1.412

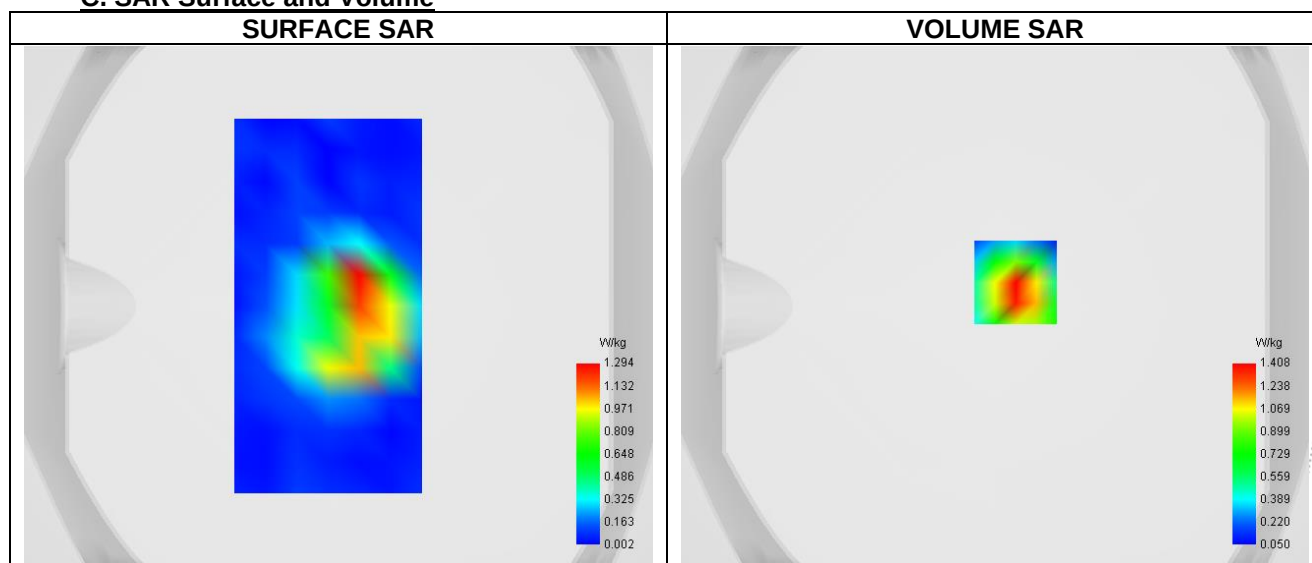C. SAR Surface and Volume


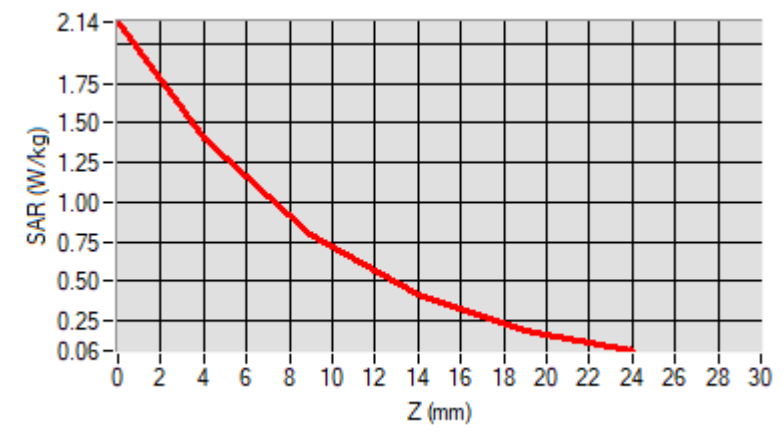
Maximum location: X=8.00, Y=9.00 ; SAR Peak: 2.21 W/kg

D. SAR 1g & 10g


SAR 10g (W/Kg)	0.657
SAR 1g (W/Kg)	1.525
Variation (%)	-4.180
Horizontal validation criteria: minimum distance (mm)	0.000000
Vertical validation criteria: SAR ratio M2/M1 (%)	0.000000

E. Z Axis Scan

Z (mm)	0.00	4.00	9.00	14.00	19.00
SAR (W/Kg)	2.137	1.408	0.790	0.410	0.188



F. 3D Image

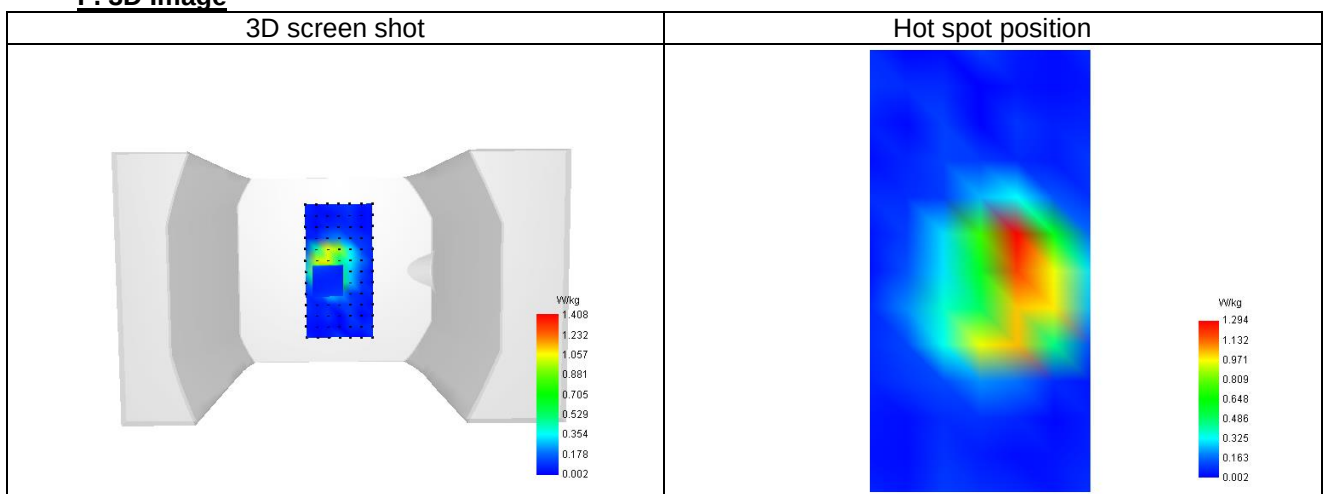

Plot 8


Date of measurement: 10/12/2024

A. Experimental conditions.

Probe	SN 26/23 EPGO420
ConvF	0.96
Area Scan	surf_sam_plan.txt
Zoom Scan	5x5x7,dx=8mm dy=8mm dz=5.0mm
Phantom	Validation plane
Device Position	Body
Band	LTE band 4
Signal	LTE FDD
Cell Bandwidth	20 Mhz
Modulation	SC-OFDM - QPSK
RB offset	5
RB size	20

B. Permittivity


Frequency (MHz)	1732.500
Relative permittivity (real part)	39.520
Relative permittivity (imaginary part)	14.120
Conductivity (S/m)	1.369

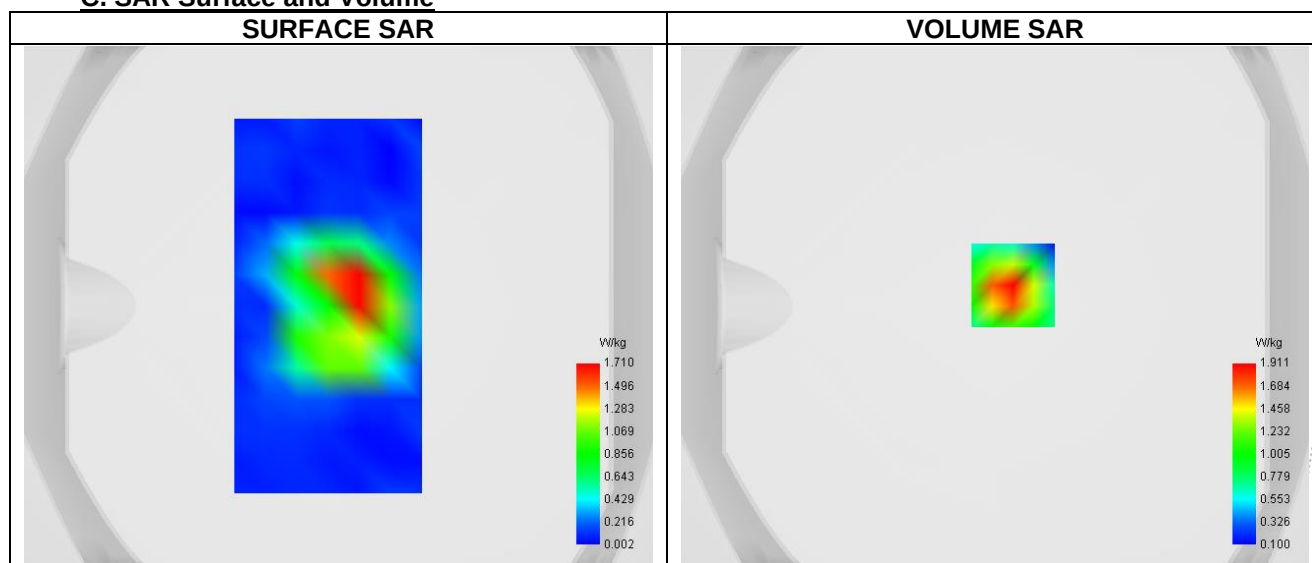C. SAR Surface and Volume

D. SAR 1g & 10g


SAR 10g (W/Kg)	0.967
SAR 1g (W/Kg)	1.797
Variation (%)	2.150
Horizontal validation criteria: minimum distance (mm)	0.000000
Vertical validation criteria: SAR ratio M2/M1 (%)	0.000000

E. Z Axis Scan

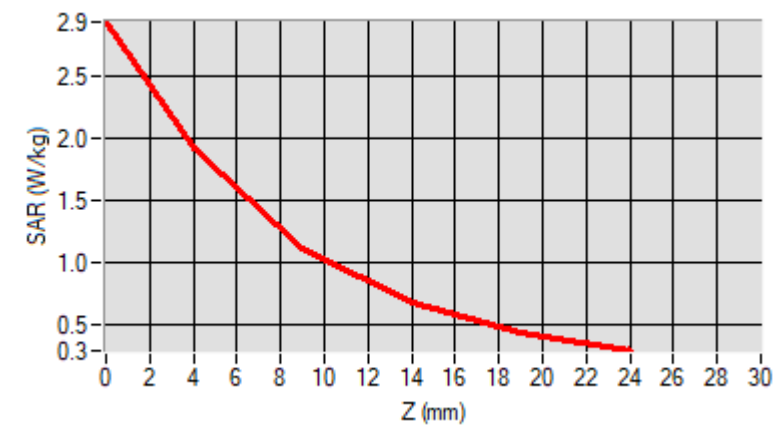Z (mm)	0.00	4.00	9.00	14.00	19.00
SAR (W/Kg)	2.927	1.911	1.108	0.663	0.427



F. 3D Image

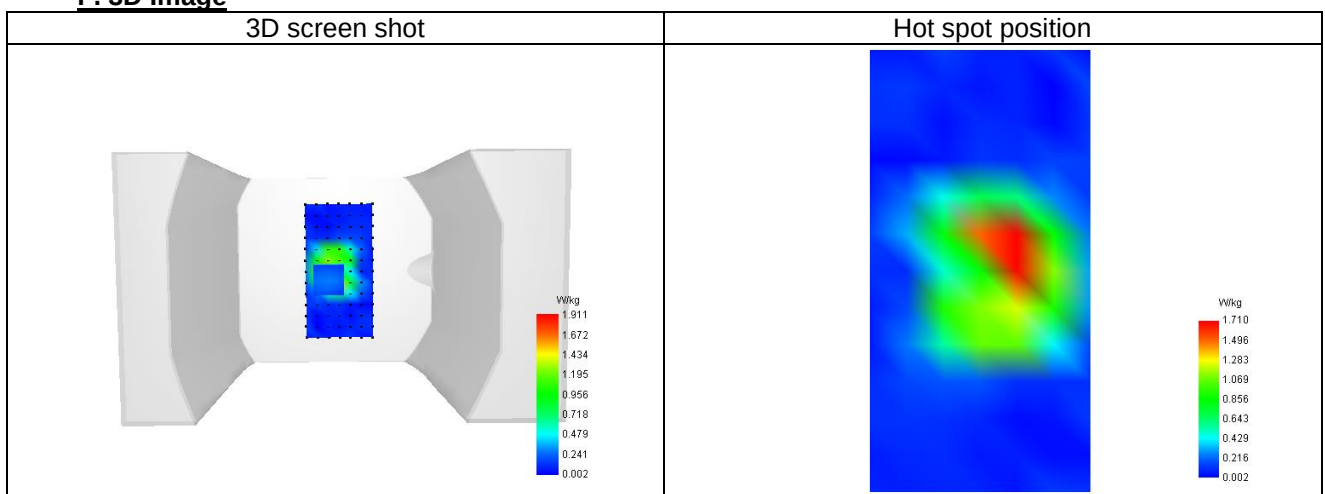

Plot 9


Date of measurement: 29/11/2024

A. Experimental conditions.

Probe	SN 26/23 EPGO420
ConvF	0.81
Area Scan	surf_sam_plan.txt
Zoom Scan	5x5x7,dx=8mm dy=8mm dz=5.0mm
Phantom	Validation plane
Device Position	Body
Band	LTE band 5
Signal	LTE FDD
Cell Bandwidth	10 Mhz
Modulation	SC-OFDM - QPSK
RB offset	5
RB size	20

B. Permittivity

Frequency (MHz)	844.000
Relative permittivity (real part)	40.706
Relative permittivity (imaginary part)	19.400
Conductivity (S/m)	0.869

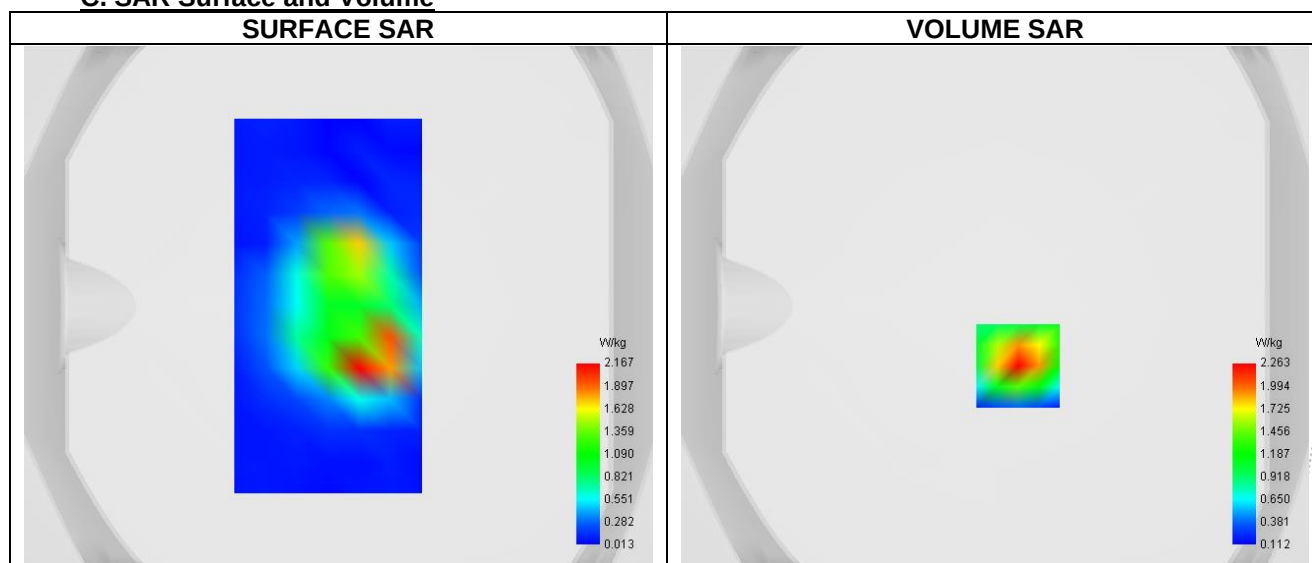C. SAR Surface and Volume


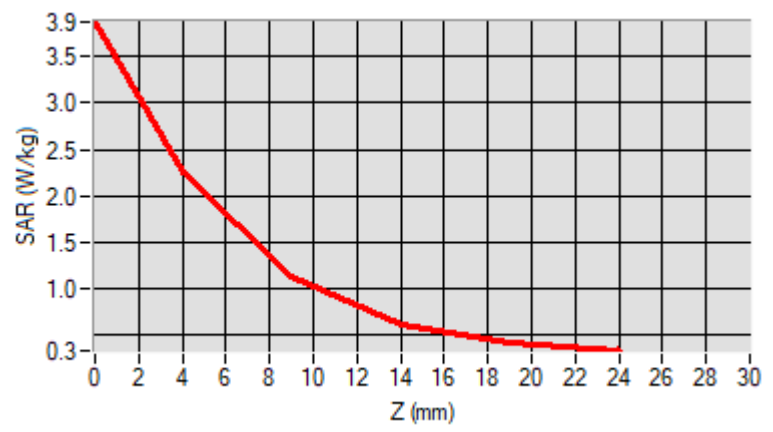
Maximum location: X=9.00, Y=-23.00 ; SAR Peak: 3.91 W/kg

D. SAR 1g & 10g


SAR 10g (W/Kg)	1.075
SAR 1g (W/Kg)	2.107
Variation (%)	-3.720
Horizontal validation criteria: minimum distance (mm)	0.000000
Vertical validation criteria: SAR ratio M2/M1 (%)	0.000000

E. Z Axis Scan

Z (mm)	0.00	4.00	9.00	14.00	19.00
SAR (W/Kg)	3.871	2.263	1.135	0.621	0.421



F. 3D Image

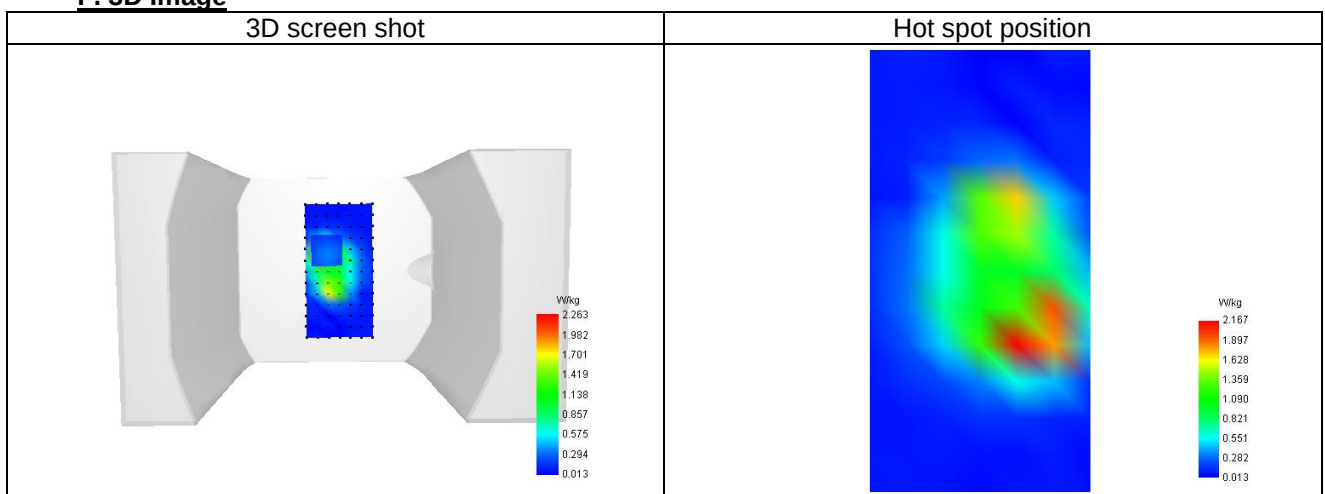

Plot 10


Date of measurement: 19/12/2024

A. Experimental conditions.

Probe	SN 26/23 EPGO420
ConvF	1.03
Area Scan	surf_sam_plan.txt
Zoom Scan	5x5x7,dx=8mm dy=8mm dz=5.0mm
Phantom	Validation plane
Device Position	Body
Band	LTE band 7
Signal	LTE FDD
Cell Bandwidth	20 Mhz
Modulation	SC-OFDM - QPSK
RB offset	5
RB size	20

B. Permittivity

Frequency (MHz)	2560.000
Relative permittivity (real part)	39.432
Relative permittivity (imaginary part)	13.404
Conductivity (S/m)	2.014

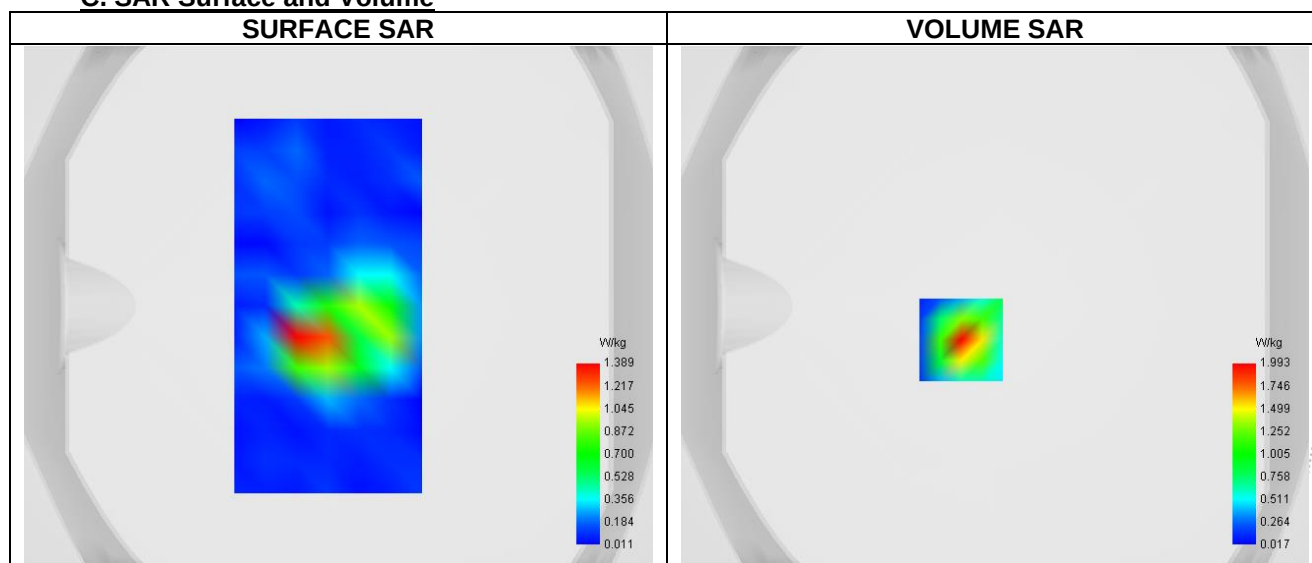C. SAR Surface and Volume


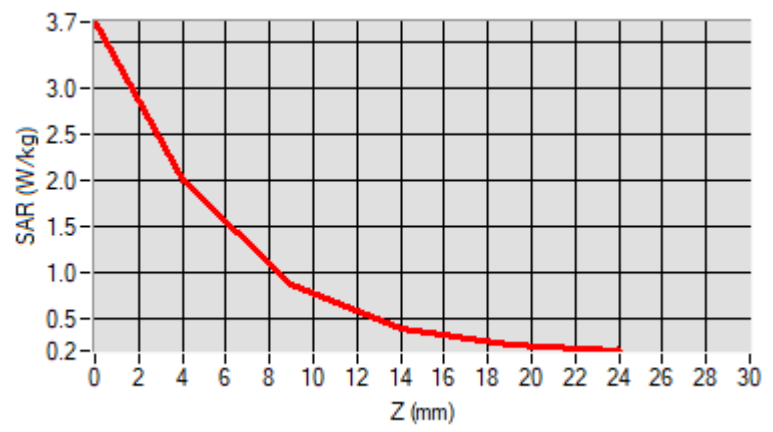
Maximum location: X=-13.00, Y=-13.00 ; SAR Peak: 3.71 W/kg

D. SAR 1g & 10g


SAR 10g (W/Kg)	0.780
SAR 1g (W/Kg)	1.834
Variation (%)	2.190
Horizontal validation criteria: minimum distance (mm)	0.000000
Vertical validation criteria: SAR ratio M2/M1 (%)	0.000000

E. Z Axis Scan

Z (mm)	0.00	4.00	9.00	14.00	19.00
SAR (W/Kg)	3.707	1.993	0.859	0.385	0.219



F. 3D Image

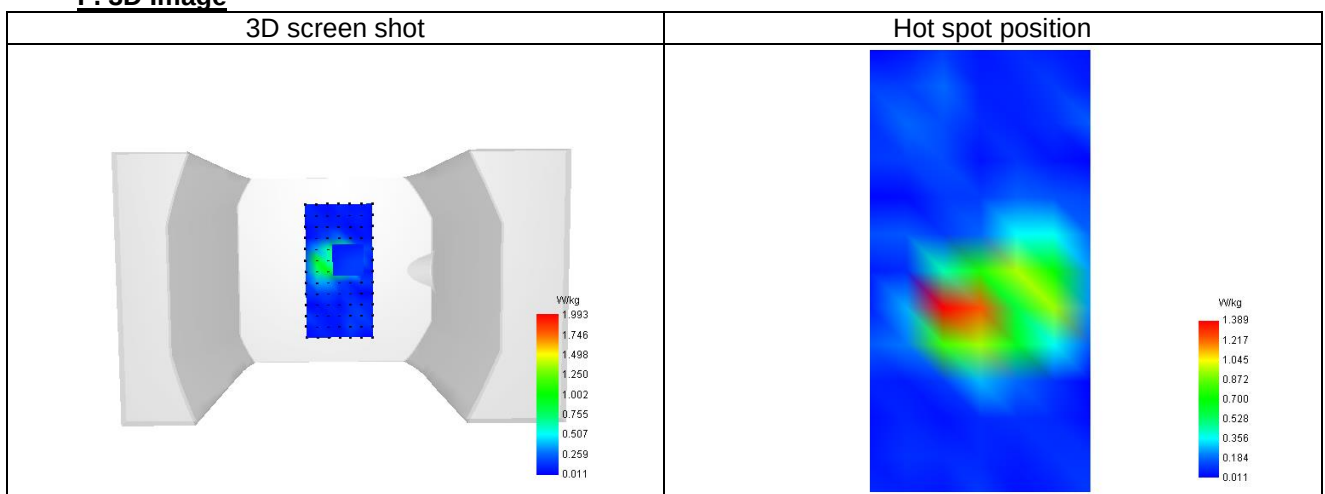

Plot 11


Date of measurement: 29/11/2024

A. Experimental conditions.

Probe	SN 26/23 EPGO420
ConvF	0.80
Area Scan	surf_sam_plan.txt
Zoom Scan	5x5x7,dx=8mm dy=8mm dz=5.0mm
Phantom	Validation plane
Device Position	Body
Band	LTE band 12
Signal	LTE FDD
Cell Bandwidth	10 Mhz
Modulation	SC-OFDM - QPSK
RB offset	5
RB size	20

B. Permittivity

Frequency (MHz)	704.000
Relative permittivity (real part)	40.272
Relative permittivity (imaginary part)	23.501
Conductivity (S/m)	0.859

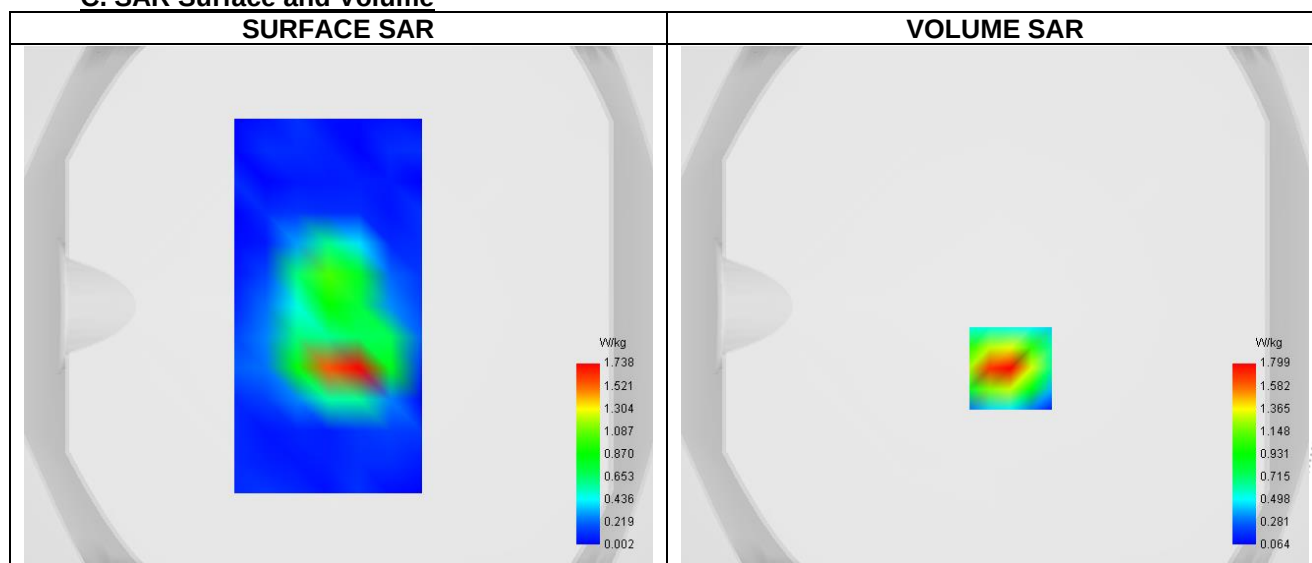C. SAR Surface and Volume


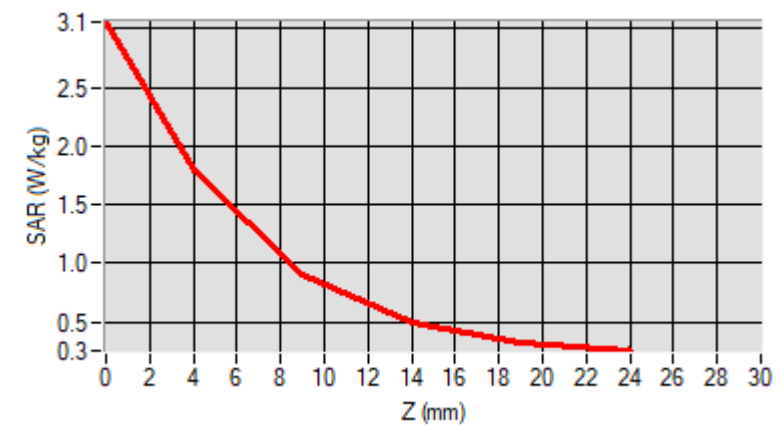
Maximum location: X=6.00, Y=-24.00 ; SAR Peak: 3.14 W/kg

D. SAR 1g & 10g


SAR 10g (W/Kg)	0.853
SAR 1g (W/Kg)	1.728
Variation (%)	-2.030
Horizontal validation criteria: minimum distance (mm)	0.000000
Vertical validation criteria: SAR ratio M2/M1 (%)	0.000000

E. Z Axis Scan

Z (mm)	0.00	4.00	9.00	14.00	19.00
SAR (W/Kg)	3.055	1.799	0.911	0.499	0.333



F. 3D Image

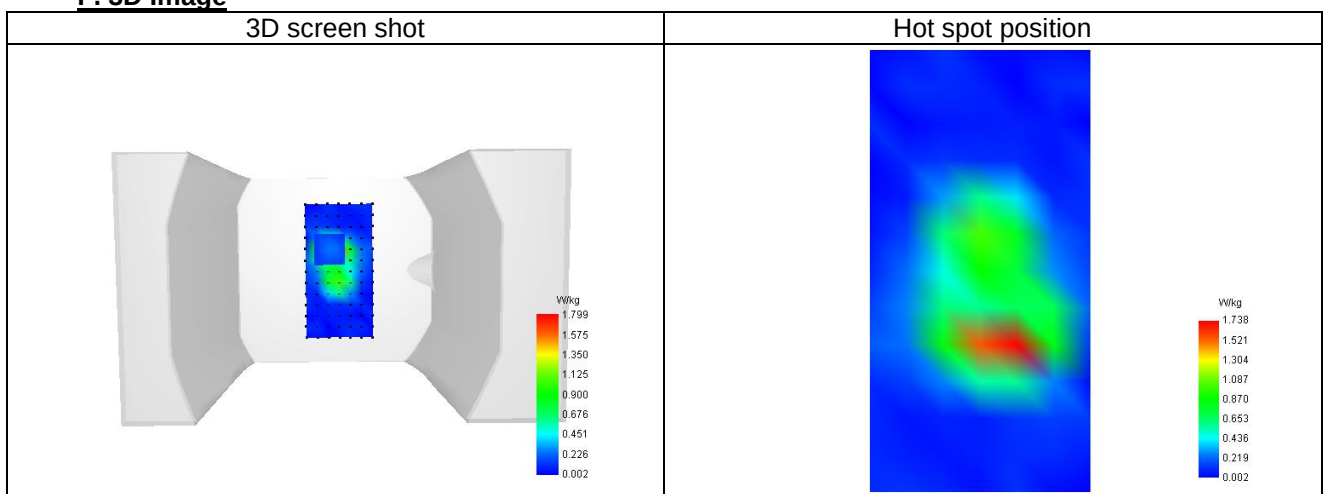

Plot 12


Date of measurement: 29/11/2024

A. Experimental conditions.

Probe	SN 26/23 EPGO420
ConvF	0.80
Area Scan	surf_sam_plan.txt
Zoom Scan	5x5x7,dx=8mm dy=8mm dz=5.0mm
Phantom	Validation plane
Device Position	Body
Band	LTE band 17
Signal	LTE FDD
Cell Bandwidth	10 Mhz
Modulation	SC-OFDM - QPSK
RB offset	5
RB size	20

B. Permittivity

Frequency (MHz)	710.000
Relative permittivity (real part)	40.272
Relative permittivity (imaginary part)	23.277
Conductivity (S/m)	0.859

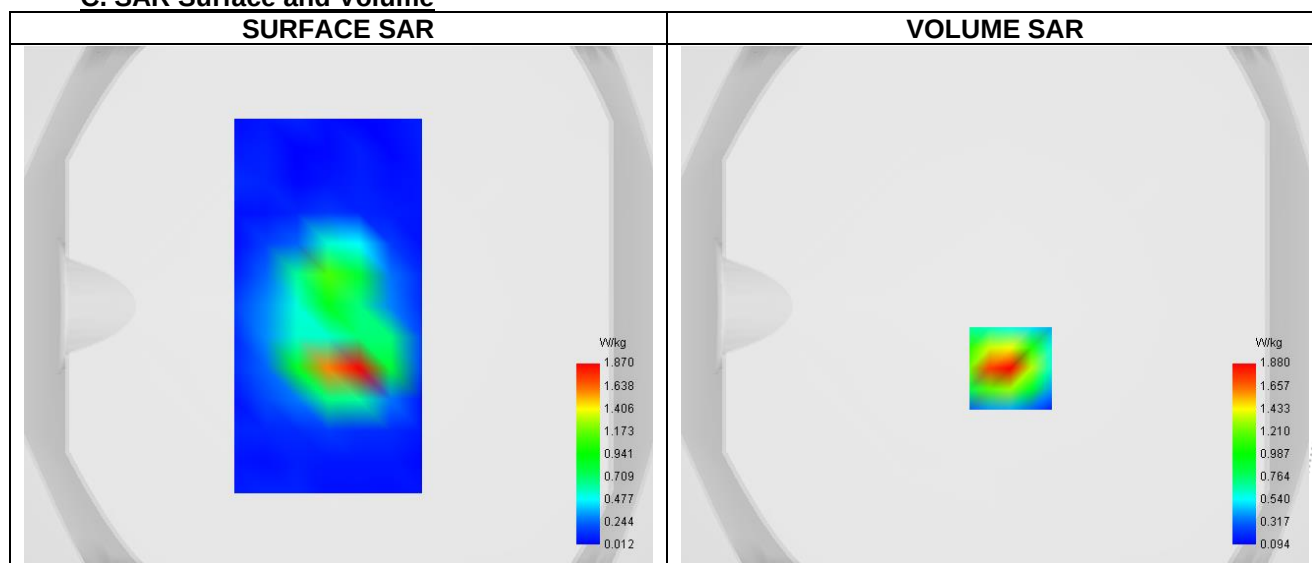C. SAR Surface and Volume


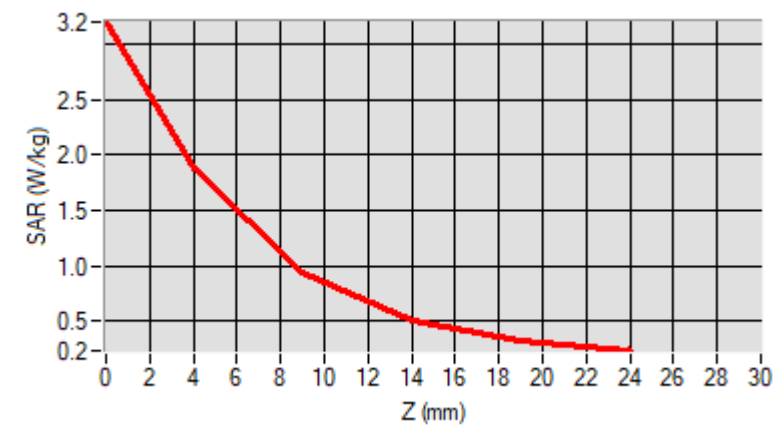
Maximum location: X=6.00, Y=-24.00 ; SAR Peak: 3.28 W/kg

D. SAR 1g & 10g


SAR 10g (W/Kg)	0.874
SAR 1g (W/Kg)	1.792
Variation (%)	-1.670
Horizontal validation criteria: minimum distance (mm)	0.000000
Vertical validation criteria: SAR ratio M2/M1 (%)	0.000000

E. Z Axis Scan

Z (mm)	0.00	4.00	9.00	14.00	19.00
SAR (W/Kg)	3.202	1.880	0.941	0.501	0.318



F. 3D Image

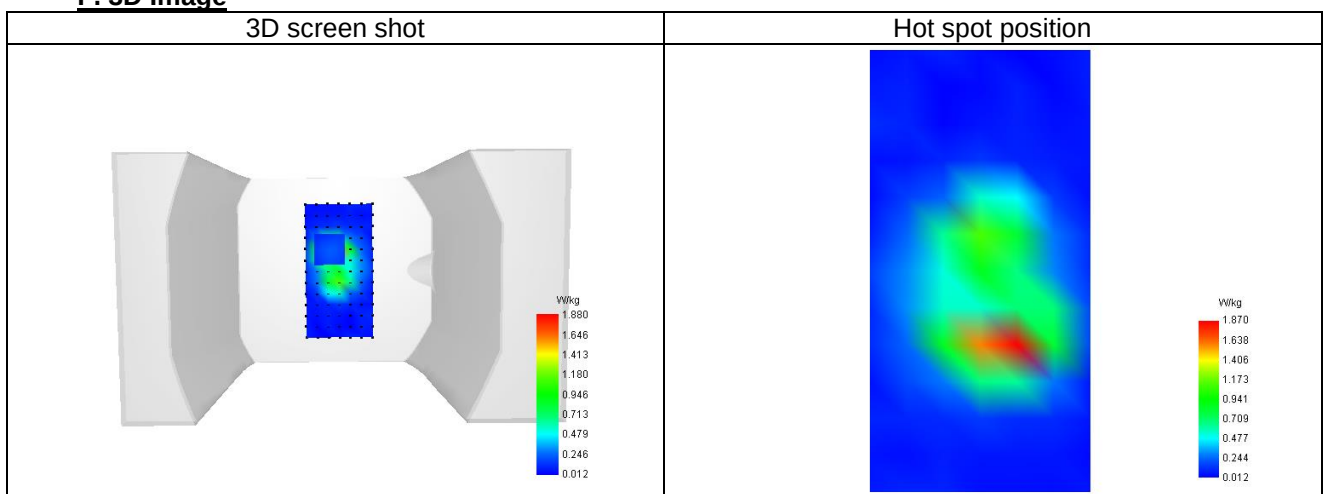

Plot 13


Date of measurement: 10/12/2024

A. Experimental conditions.

Probe	SN 26/23 EPGO420
ConvF	0.96
Area Scan	surf_sam_plan.txt
Zoom Scan	5x5x7,dx=8mm dy=8mm dz=5.0mm
Phantom	Validation plane
Device Position	Body
Band	LTE band 66
Signal	LTE FDD
Cell Bandwidth	20 Mhz
Modulation	SC-OFDM - QPSK
RB offset	5
RB size	20

B. Permittivity

Frequency (MHz)	1745.000
Relative permittivity (real part)	39.520
Relative permittivity (imaginary part)	14.065
Conductivity (S/m)	1.369

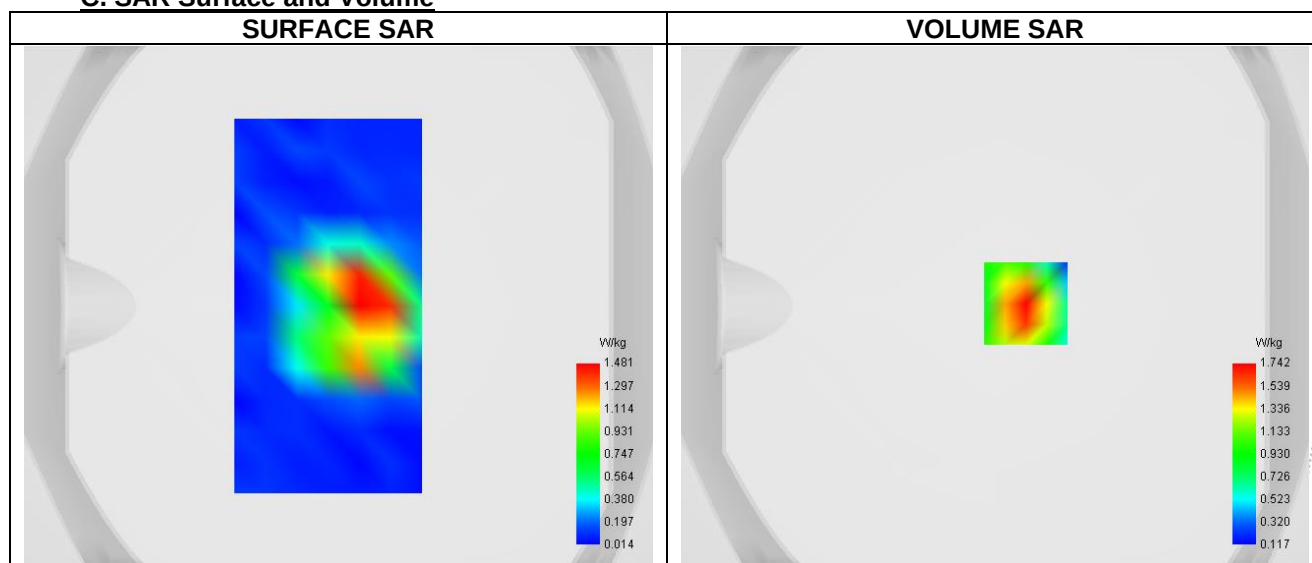C. SAR Surface and Volume


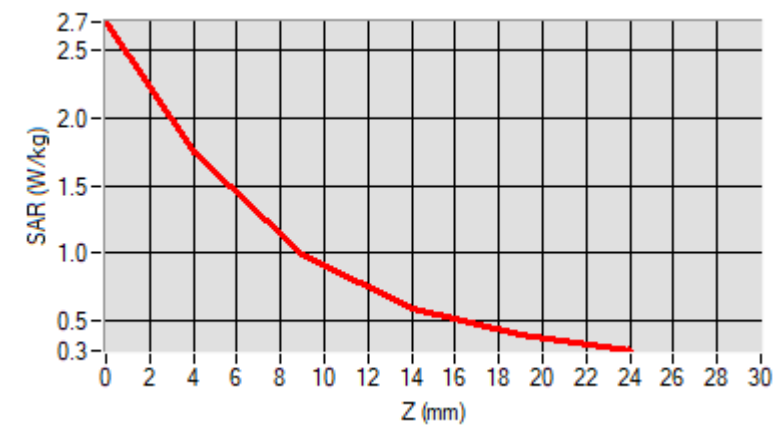
Maximum location: X=12.00, Y=1.00 ; SAR Peak: 2.75 W/kg

D. SAR 1g & 10g


SAR 10g (W/Kg)	0.907
SAR 1g (W/Kg)	1.635
Variation (%)	-0.200
Horizontal validation criteria: minimum distance (mm)	0.000000
Vertical validation criteria: SAR ratio M2/M1 (%)	0.000000

E. Z Axis Scan

Z (mm)	0.00	4.00	9.00	14.00	19.00
SAR (W/Kg)	2.708	1.742	0.997	0.597	0.397




F. 3D Image

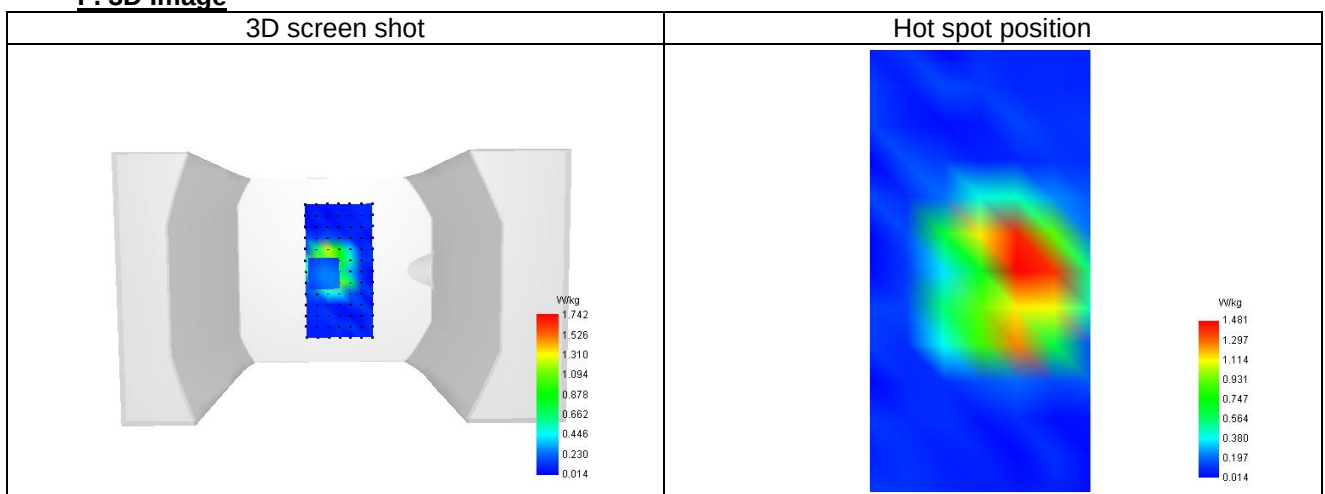

16 CALIBRATION CERTIFICATES

Probe-EPGO420 Calibration Certificate
SID750Dipole Calibration Certificate
SID835Dipole Calibration Certificate
SID1800Dipole Calibration Certificate
SID1900Dipole Calibration Certificate
SID2100Dipole Calibration Certificate
SID2450Dipole Calibration Certificate
SID2600Dipole Calibration Certificate

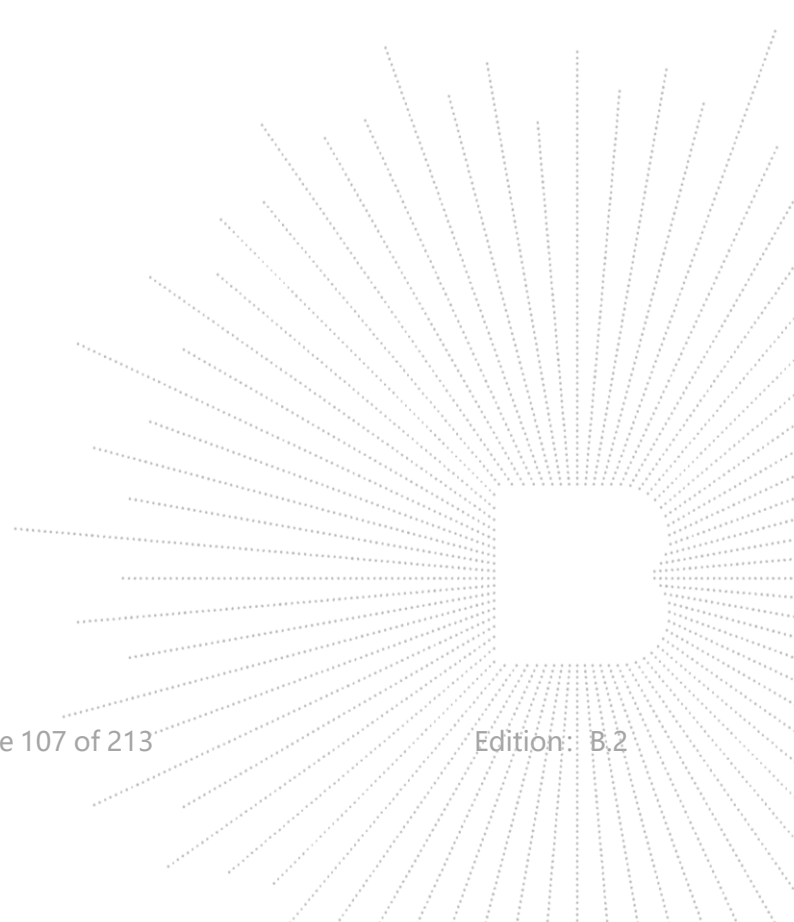



COMOSAR E-Field Probe Calibration Report

Ref : ACR.199.1.23.BES.A

SHENZHEN BCTC TECHNOLOGY CO., LTD.

1 ~2/ F, NO. B FACTORY BUILDING, PENGZHOU
INDUSTRIAL PARK, FUYUAN 1ST ROAD,
TANGWEI COMMUNITY, FUHAI STREET, BAO'AN
DISTRICT, SHENZHEN, GUANGDONG, CHINA
MVG COMOSAR DOSIMETRIC E-FIELD PROBE
SERIAL NO.: 2623-EPGO-420

Calibrated at MVG

Z.I. de la pointe du diable

Technopôle Brest Iroise – 295 avenue Alexis de Rochon

29280 PLOUZANE - FRANCE

Calibration date: 7/18/2024



Accreditations #2-6789
Scope available on www.cofrac.fr

The use of the Cofrac brand and the accreditation references is prohibited from any reproduction.

Summary:

This document presents the method and results from an accredited COMOSAR Dosimetric E-Field Probe calibration performed at MVG, using the CALIPROBE test bench, for use with a MVG COMOSAR system only. The test results covered by accreditation are traceable to the International System of Units (SI).

Page: 1/11


COMOSAR E-FIELD PROBE CALIBRATION REPORT

Ref: ACR.199.1.23 BES.A

	<i>Name</i>	<i>Function</i>	<i>Date</i>	<i>Signature</i>
<i>Prepared by :</i>	Cyrille ONNEE	Measurement Responsible	7/18/2024	
<i>Checked & approved by:</i>	Jérôme Luc	Technical Manager	7/18/2024	
<i>Authorized by:</i>	Yann Toutain	Laboratory Director	7/18/2024	

Yann
Toutain ID

Signature numérique
de Yann Toutain ID
Date : 2024.07.18
10:38:49 +02'00'

	<i>Customer Name</i>
<i>Distribution :</i>	Shenzhen BCTC Technology Co., Ltd.

<i>Issue</i>	<i>Name</i>	<i>Date</i>	<i>Modifications</i>
A	Cyrille ONNEE	7/18/2024	Initial release

Page: 2/11

Template_ACR.DDD.N.YY.MVGB.ISSUE_COMOSAR Probe vL

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.



TABLE OF CONTENTS

1	Device Under Test	4
2	Product Description	4
2.1	General Information	4
3	Measurement Method	4
3.1	Sensitivity	4
3.2	Linearity	5
3.3	Isotropy	5
3.4	Boundary Effect	5
4	Measurement Uncertainty	6
5	Calibration Results	6
5.1	Calibration in air	6
5.2	Calibration in liquid	7
6	Verification Results	9
7	List of Equipment	10

Page: 3/11

Template_ACR.DDD.N.YY.MVGB.ISSUE_COMOSAR Probe vL

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.



1 DEVICE UNDER TEST

Device Under Test	
Device Type	COMOSAR DOSIMETRIC E FIELD PROBE
Manufacturer	MVG
Model	SSE2
Serial Number	2623-EPGO-420
Product Condition (new / used)	New
Frequency Range of Probe	0.15 GHz-7.5GHz
Resistance of Three Dipoles at Connector	Dipole 1: R1=0.228 MΩ Dipole 2: R2=0.238 MΩ Dipole 3: R3=0.230 MΩ

2 PRODUCT DESCRIPTION

2.1 GENERAL INFORMATION

MVG's COMOSAR E field Probes are built in accordance to the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards.



Figure 1 – MVG COMOSAR Dosimetric E field Probe

Probe Length	330 mm
Length of Individual Dipoles	24.5 mm
Maximum external diameter	8 mm
Probe Tip External Diameter	2.55 mm
Distance between dipoles / probe extremity	12.7 mm

3 MEASUREMENT METHOD

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards provide recommended practices for the probe calibrations, including the performance characteristics of interest and methods by which to assess their effect. All calibrations / measurements performed meet the fore-mentioned standards.

3.1 SENSITIVITY

The sensitivity factors of the three dipoles were determined using a two step calibration method (air and tissue simulating liquid) using waveguides as outlined in the standards for frequency range 600-7500MHz and using the calorimeter cell method (transfer method) as outlined in the standards for frequency 150-450 MHz.



3.2 LINEARITY

The evaluation of the linearity was done in free space using the waveguide, performing a power sweep to cover the SAR range 0.01W/kg to 100W/kg.

3.3 ISOTROPY

The axial isotropy was evaluated by exposing the probe to a reference wave from a standard dipole with the dipole mounted under the flat phantom in the test configuration suggested for system validations and checks. The probe was rotated along its main axis from 0 to 360 degrees in 15-degree steps. The hemispherical isotropy is determined by inserting the probe in a thin plastic box filled with tissue-equivalent liquid, with the plastic box illuminated with the fields from a half wave dipole. The dipole is rotated about its axis (0°–180°) in 15° increments. At each step the probe is rotated about its axis (0°–360°).

3.4 BOUNDARY EFFECT

The boundary effect is defined as the deviation between the SAR measured data and the expected exponential decay in the liquid when the probe is oriented normal to the interface. To evaluate this effect, the liquid filled flat phantom is exposed to fields from either a reference dipole or waveguide. With the probe normal to the phantom surface, the peak spatial average SAR is measured and compared to the analytical value at the surface.

The boundary effect uncertainty can be estimated according to the following uncertainty approximation formula based on linear and exponential extrapolations between the surface and $d_{be} + d_{step}$ along lines that are approximately normal to the surface:

$$SAR_{uncertainty} [\%] = \delta SAR_{be} \frac{(d_{be} + d_{step})^2}{2d_{step}} \frac{(e^{-d_{be}/\delta} - e^{-d_{step}/\delta})}{\delta/2} \quad \text{for } (d_{be} + d_{step}) < 10 \text{ mm}$$

where

$SAR_{uncertainty}$	is the uncertainty in percent of the probe boundary effect
d_{be}	is the distance between the surface and the closest <i>zoom-scan</i> measurement point, in millimetre
Δ_{step}	is the separation distance between the first and second measurement points that are closest to the phantom surface, in millimetre, assuming the boundary effect at the second location is negligible
δ	is the minimum penetration depth in millimetres of the head tissue-equivalent liquids defined in this standard, i.e., $\delta \approx 14 \text{ mm}$ at 3 GHz;
ΔSAR_{be}	in percent of SAR is the deviation between the measured SAR value, at the distance d_{be} from the boundary, and the analytical SAR value.

The measured worst case boundary effect $SAR_{uncertainty}[\%]$ for scanning distances larger than 4mm is 1.0% Limit, 2%).



4 MEASUREMENT UNCERTAINTY

The guidelines outlined in the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards were followed to generate the measurement uncertainty associated with a SAR probe calibration using the waveguide or calorimetric cell technique depending on the frequency.

The estimated expanded uncertainty (k=2) in calibration for SAR (W/kg) is +/-11% for the frequency range 150-450MHz.


The estimated expanded uncertainty (k=2) in calibration for SAR (W/kg) is +/-14% for the frequency range 600-7500MHz.

5 CALIBRATION RESULTS

Ambient condition	
Liquid Temperature	20 +/- 1 °C
Lab Temperature	20 +/- 1 °C
Lab Humidity	30-70 %

5.1 CALIBRATION IN AIR

The following curve represents the measurement in waveguide of the voltage picked up by the probe toward the E-field generated inside the waveguide.

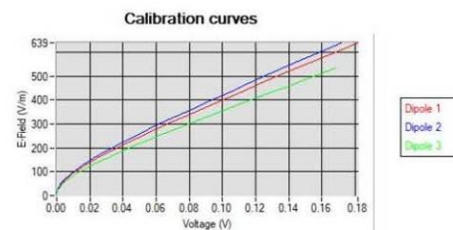

From this curve, the sensitivity in air is calculated using the below formula.

$$E^2 = \sum_{i=1}^3 \frac{V_i (1 + V_i / DCP_i)}{Norm_i}$$

where

Vi=voltage readings on the 3 channels of the probe

DCPi=diode compression point given below for the 3 channels of the probe

Normi=dipole sensitivity given below for the 3 channels of the probe



Normx dipole 1 ($\mu\text{V}/(\text{V}/\text{m})^2$)	Normy dipole 2 ($\mu\text{V}/(\text{V}/\text{m})^2$)	Normz dipole 3 ($\mu\text{V}/(\text{V}/\text{m})^2$)
1.21	1.09	1.56

DCP dipole 1 (mV)	DCP dipole 2 (mV)	DCP dipole 3 (mV)
106	109	103

5.2 CALIBRATION IN LIQUID

The calorimeter cell or the waveguide is used to determine the calibration in liquid using the formula below.

$$ConvF = \frac{E_{liquid}^2}{E_{air}^2}$$

The E-field in the liquid is determined from the SAR measurement according to the below formula.

$$E_{liquid}^2 = \frac{\rho SAR}{\sigma}$$

where

σ =the conductivity of the liquid

ρ =the volumetric density of the liquid

SAR=the SAR measured from the formula that depends on the setup used. The SAR formulas are given below

For the calorimeter cell (150-450 MHz), the formula is:

$$SAR = c \frac{dT}{dt}$$

where

c =the specific heat for the liquid

dT/dt =the temperature rises over the time

For the waveguide setup (600-75000 MHz), the formula is:

$$SAR = \frac{4P_W}{ab\delta} e^{-\frac{2z}{\delta}}$$

where

a =the larger cross-sectional of the waveguide

b =the smaller cross-sectional of the waveguide

δ =the skin depth for the liquid in the waveguide

P_W =the power delivered to the liquid

Page: 7/11

Template_ACR.DDD.N.YY.MVGB.ISSUE_COMOSAR Probe v1

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.



COMOSAR E-FIELD PROBE CALIBRATION REPORT

Ref: ACR.199.1.23.BES.A

The below table summarize the ConvF for the calibrated liquid. The curves give examples for the measured SAR depending on the voltage in some liquid.

Liquid	Frequency (MHz*)	ConvF
HL450	450	0.86
BL450	450	0.78
HL750	750	0.80
BL750	750	0.87
HL850	835	0.81
BL850	835	0.80
HL900	900	0.76
BL900	900	0.87
HL1800	1800	0.96
BL1800	1800	1.01
HL1900	1900	1.04
BL1900	1900	1.11
HL2100	2100	1.00
BL2100	2100	1.16
HL2300	2300	1.11
BL2300	2300	1.23
HL2450	2450	1.11
BL2450	2450	1.32
HL2600	2600	1.03
BL2600	2600	1.19
HL5200	5200	1.18
BL5200	5200	0.97
HL5400	5400	1.17
BL5400	5400	1.00
HL5600	5600	1.20
BL5600	5600	0.95
HL5800	5800	1.15
BL5800	5800	1.05

(*) Frequency validity is ± 50 MHz below 600MHz, ± 100 MHz from 600MHz to 6GHz and ± 700 MHz above 6GHz



Page: 8/11



Template_ACR.DDD.N.YY.MVGB.ISSUE_COMOSAR Probe v1

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.



6 VERIFICATION RESULTS

The figures below represent the measured linearity and axial isotropy for this probe. The probe specification is ± 0.2 dB for linearity and ± 0.15 dB for axial isotropy.

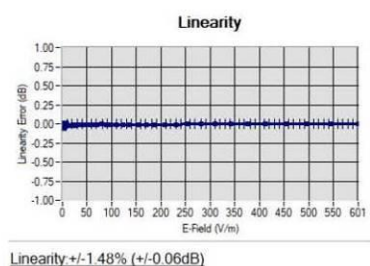



7 LIST OF EQUIPMENT

Equipment Summary Sheet				
Equipment Description	Manufacturer / Model	Identification No.	Current Calibration Date	Next Calibration Date
CALIPROBE Test Bench	Version 2	NA	Validated. No cal required.	Validated. No cal required.
Network Analyzer	Rohde & Schwarz ZVM	100203	08/2024	08/2027
Network Analyzer	Agilent 8753ES	MY40003210	10/2023	10/2027
Network Analyzer – Calibration kit	HP 85033D	3423A08186	06/2021	06/2027
Network Analyzer – Calibration kit	Rohde & Schwarz ZV-Z235	101223	07/2022	07/2025
Multimeter	Keithley 2000	4013982	02/2023	02/2026
Signal Generator	Rohde & Schwarz SMB	106589	03/2022	03/2025
Amplifier	MVG	MODU-023-C-0002	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.
Power Meter	NI-USB 5680	170100013	06/2024	06/2027
Power Meter	Keysight U2000A	SN: MY62340002	10/2022	10/2025
Directional Coupler	Krytar 158020	131467	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.
Fluoroptic Thermometer	LumaSense Luxtron 812	94264	09/2022	09/2025
Coaxial cell	MVG	SN 32/16 COAXCELL_	Validated. No cal required.	Validated. No cal required.
Waveguide	MVG	SN 32/16 WG2_1	Validated. No cal required.	Validated. No cal required.
Liquid transition	MVG	SN 32/16 WGLIQ_0G600_	Validated. No cal required.	Validated. No cal required.
Waveguide	MVG	SN 32/16 WG4_1	Validated. No cal required.	Validated. No cal required.
Liquid transition	MVG	SN 32/16 WGLIQ_0G900_	Validated. No cal required.	Validated. No cal required.
Waveguide	MVG	SN 32/16 WG6_1	Validated. No cal required.	Validated. No cal required.
Liquid transition	MVG	SN 32/16 WGLIQ_1G500_	Validated. No cal required.	Validated. No cal required.
Waveguide	MVG	SN 32/16 WG8_1	Validated. No cal required.	Validated. No cal required.

Page: 10/11

Template_ACR.DDD.N.YY.MVGB.ISSUE_COMOSAR Probe vL

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.


COMOSAR E-FIELD PROBE CALIBRATION REPORT

Ref: ACR.199.1.23 BES.A

Liquid transition	MVG	SN 32/16 WGLIQ_1G800B_1	Validated. No cal required.	Validated. No cal required.
Liquid transition	MVG	SN 32/16 WGLIQ_1G800H_	Validated. No cal required.	Validated. No cal required.
Waveguide	MVG	SN 32/16 WG10_1	Validated. No cal required.	Validated. No cal required.
Liquid transition	MVG	SN 32/16 WGLIQ_3G500_	Validated. No cal required.	Validated. No cal required.
Waveguide	MVG	SN 32/16 WG12_1	Validated. No cal required.	Validated. No cal required.
Liquid transition	MVG	SN 32/16 WGLIQ_5G000_	Validated. No cal required.	Validated. No cal required.
Waveguide	MVG	SN 32/16 WG14_1	Validated. No cal required.	Validated. No cal required.
Liquid transition	MVG	SN 32/16 WGLIQ_7G000_1	Validated. No cal required.	Validated. No cal required.
Temperature / Humidity Sensor	Testo 184 H1	44225320	06/2021	06/2024

Page: 11/11

Template_ACR.DDD.N.YY.MVGB.ISSUE_COMOSAR Probe vL

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.



SAR Reference Dipole Calibration Report

Ref : ACR.329.8.21.BES.A

SHENZHEN BCTC TECHNOLOGY CO., LTD.

**1 ~2/ F, NO. B FACTORY BUILDING, PENGZHOU
INDUSTRIAL PARK, FUYUAN 1ST ROAD,
TANGWEI COMMUNITY, FUHAI STREET, BAO'AN
DISTRICT, SHENZHEN, GUANGDONG, CHINA
MVG COMOSAR REFERENCE DIPOLE**

FREQUENCY: 750 MHZ

SERIAL NO.: SN 47/21 DIP 0G750-620

Calibrated at MVG

Z.I. de la pointe du diable

Technopôle Brest Iroise – 295 avenue Alexis de Rochon

29280 PLOUZANE - FRANCE

Calibration date: 11/25/2021



Accreditations #2-6789 and #2-6814
Scope available on www.cofrac.fr

The use of the Cofrac brand and the accreditation references is prohibited from any reproduction.

Summary:

This document presents the method and results from an accredited SAR reference dipole calibration performed in MVG using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.