

ANNEX E CALIBRATION FOR PROBE AND DIPOLEF

F.1 E-Field Probe



COMOHAC E-Field Probe Calibration Report

Ref : ACR.93.12.17.SATU.A

SHENZHEN BALUN TECHNOLOGY CO.,LTD.
BLOCK B, FL 1, BAISHA SCIENCE AND TECHNOLOGY
PARK, SHAHE XI ROAD,
NANSAN DISTRICT, SHENZHEN, GUANGDONG
PROVINCE, P.R. CHINA 518055
MVG COMOHAC E-FIELD PROBE
SERIAL NO.: SN 03/16 EPH47

Calibrated at MVG US
2105 Barrett Park Dr. - Kennesaw, GA 30144



Calibration Date: 03/22/2017

Summary:

This document presents the method and results from an accredited COMOHAC E-Field Probe calibration performed in MVG USA using the CALIBAIR test bench, for use with a MVG COMOHAC system only. All calibration results are traceable to national metrology institutions.



| | Name | Function | Date | Signature |
|---------------|---------------|-----------------|----------|-----------|
| Prepared by : | Jérôme LUC | Product Manager | 4/3/2017 | |
| Checked by : | Jérôme LUC | Product Manager | 4/3/2017 | |
| Approved by : | Kim RUTKOWSKI | Quality Manager | 4/3/2017 | |

| | Customer Name |
|----------------|---|
| Distribution : | SHENZHEN BALUN TECHNOLOGY Co.,Ltd. |

| Issue | Date | Modifications |
|-------|----------|-----------------|
| A | 4/3/2017 | Initial release |
| | | |
| | | |
| | | |

**TABLE OF CONTENTS**

| | | |
|-----|---------------------------------------|---|
| 1 | Device Under Test | 4 |
| 2 | Product Description | 4 |
| 2.1 | General Information | 4 |
| 3 | Measurement Method | 4 |
| 3.1 | Linearity | 4 |
| 3.2 | Sensitivity | 5 |
| 3.3 | Isotropy | 5 |
| 3.4 | Probe Modulation Response | 5 |
| 4 | Measurement Uncertainty | 5 |
| 5 | Calibration Measurement Results | 5 |
| 5.1 | Sensitivity in air | 6 |
| 5.2 | Linearity | 7 |
| 5.3 | Isotropy | 7 |
| 6 | List of Equipment | 8 |



1 DEVICE UNDER TEST

| Device Under Test | |
|--|---|
| Device Type | COMOHAC E FIELD PROBE |
| Manufacturer | MVG |
| Model | SCE |
| Serial Number | SN 03/16 EPH47 |
| Product Condition (new / used) | New |
| Frequency Range of Probe | 0.7GHz-2.5GHz |
| Resistance of Three Dipoles at Connector | Dipole 1: R1=0.208 MΩ Dipole 2: R2=0.203 MΩ Dipole 3: R3=0.214 MΩ |

A yearly calibration interval is recommended.

2 PRODUCT DESCRIPTION

2.1 GENERAL INFORMATION

MVG's COMOHAC E field Probes are built in accordance to the ANSI C63.19 and IEEE 1309 standards.



Figure 1 – MVG COMOHAC E field Probe

| | |
|--|--------|
| Probe Length | 330 mm |
| Length of Individual Dipoles | 3.3 mm |
| Maximum external diameter | 8 mm |
| Probe Tip External Diameter | 5 mm |
| Distance between dipoles / probe extremity | 3 mm |

3 MEASUREMENT METHOD

All methods used to perform the measurements and calibrations comply with the ANSI C63.19 and IEEE 1309 standards.

3.1 LINEARITY

The linearity was determined using a standard dipole with the probe positioned 10 mm above the dipole. The input power of the dipole was adjusted from -15 to 36 dBm using a 1dB step (to cover the range 2V/m to 1000A/m).



3.2 SENSITIVITY

The sensitivity factors of the three dipoles were determined using the waveguide method outlined in the fore mentioned standards.

3.3 ISOTROPY

The axial isotropy was evaluated by exposing the probe to a reference wave from a standard dipole. The probe was rotated along its main axis from 0 - 360 degrees in 15 degree steps.

3.4 PROBE MODULATION RESPONSE

The modulation factor was determined by illuminating the probe with a reference wave from a standard dipole 10 mm away, applying first a CW signal and then a modulated signal (both at same power level). The modulation factor is the ratio, in linear units, of the CW to modulated signal reading.

4 MEASUREMENT UNCERTAINTY

The guidelines outlined in the IEEE 1528 and IEC/CEI 62209 standards were followed to generate the measurement uncertainty associated with an E-field probe calibration using the waveguide technique. All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of $k=2$, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

| Uncertainty analysis of the probe calibration in waveguide | | | | | |
|--|-----------------------|--------------------------|------------|----|--------------------------|
| ERROR SOURCES | Uncertainty value (%) | Probability Distribution | Divisor | ci | Standard Uncertainty (%) |
| Incident or forward power | 3.00% | Rectangular | $\sqrt{3}$ | 1 | 1.732% |
| Reflected power | 3.00% | Rectangular | $\sqrt{3}$ | 1 | 1.732% |
| Field homogeneity | 3.00% | Rectangular | $\sqrt{3}$ | 1 | 1.732% |
| Field probe positioning | 5.00% | Rectangular | $\sqrt{3}$ | 1 | 2.887% |
| Field probe linearity | 3.00% | Rectangular | $\sqrt{3}$ | 1 | 1.732% |
| Combined standard uncertainty | | | | | 4.509% |
| Expanded uncertainty 95 % confidence level $k = 2$ | | | | | 9.0% |

5 CALIBRATION MEASUREMENT RESULTS

| Calibration Parameters | |
|------------------------|-------|
| Lab Temperature | 21 °C |

Page: 5/8


*This document shall not be reproduced, except in full or in part, without the written approval of MVG.
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.*




| | |
|--------------|------|
| Lab Humidity | 45 % |
|--------------|------|


5.1 SENSITIVITY IN AIR

| Normx dipole 1 ($\mu\text{V}/(\text{V}/\text{m})^2$) | Normy dipole 2 ($\mu\text{V}/(\text{V}/\text{m})^2$) | Normz dipole 3 ($\mu\text{V}/(\text{V}/\text{m})^2$) |
|---|---|---|
| 3.69 | 4.41 | 4.60 |
| DCP dipole 1 (mV) | DCP dipole 2 (mV) | DCP dipole 3 (mV) |
| 106 | 117 | 121 |

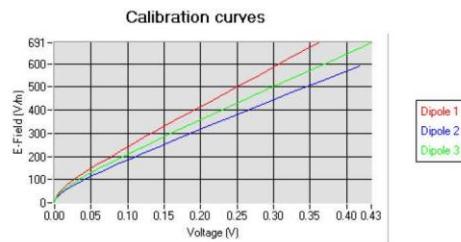

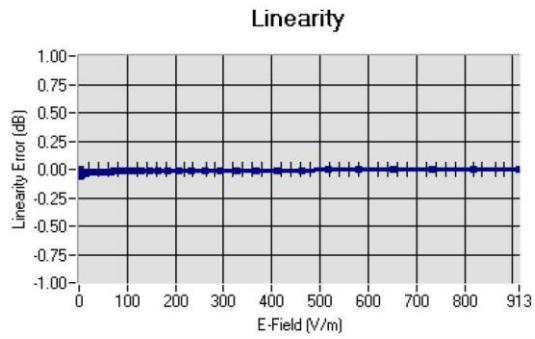5.2 LINEARITY

Linearity: +/-1.32% (+/-0.06dB)

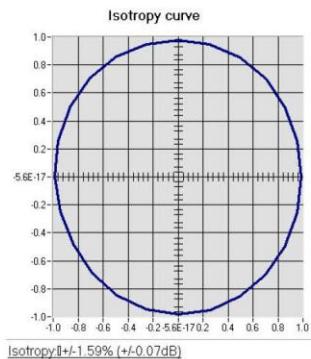5.3 ISOTROPY

Isotropy: +/-1.59% (+/-0.07dB)

**6 LIST OF EQUIPMENT**

| Equipment Summary Sheet | | | | |
|-------------------------------|----------------------|--------------------|---|---|
| Equipment Description | Manufacturer / Model | Identification No. | Current Calibration Date | Next Calibration Date |
| HAC positioning ruler | MVG | TABH12 SN 42/09 | Validated. No cal required. | Validated. No cal required. |
| COMOHAC Test Bench | Version 2 | NA | Validated. No cal required. | Validated. No cal required. |
| Network Analyzer | Rhode & Schwarz ZVA | SN100132 | 02/2016 | 02/2019 |
| Reference Probe | MVG | EPH28 SN 08/11 | 10/2016 | 10/2017 |
| Reference Probe | MVG | HPH38 SN31/10 | 10/2016 | 10/2017 |
| Multimeter | Keithley 2000 | 1188656 | 01/2017 | 01/2020 |
| Signal Generator | Agilent E4438C | MY49070581 | 01/2017 | 01/2020 |
| Amplifier | Aethercomm | SN 046 | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter | HP E4418A | US38261498 | 01/2017 | 01/2020 |
| Power Sensor | HP ECP-E26A | US37181460 | 01/2017 | 01/2020 |
| Directional Coupler | Narda 4216-20 | 01386 | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Waveguide | Mega Industries | 069Y7-158-13-712 | Validated. No cal required. | Validated. No cal required. |
| Waveguide Transition | Mega Industries | 069Y7-158-13-701 | Validated. No cal required. | Validated. No cal required. |
| Waveguide Termination | Mega Industries | 069Y7-158-13-701 | Validated. No cal required. | Validated. No cal required. |
| Temperature / Humidity Sensor | Control Company | 150798832 | 10/2015 | 10/2017 |

Page: 8/8

*This document shall not be reproduced, except in full or in part, without the written approval of MVG.
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.*

F.2 T-coil Probe

**COMOHAC T-coil Probe Calibration Report**

Ref : ACR.93.14.17.SATU.A

SHENZHEN BALUN TECHNOLOGY CO.,LTD.
BLOCK B, FL 1, BAISHA SCIENCE AND TECHNOLOGY
PARK, SHAHE XI ROAD,
NANSHAN DISTRICT, SHENZHEN, GUANGDONG
PROVINCE, P.R. CHINA 518055
MVG COMOHAC T-COIL PROBE
SERIAL NO.: SN 46/15 TCP34

Calibrated at MVG US
2105 Barrett Park Dr. - Kennesaw, GA 30144



Calibration Date: 03/22/2017

Summary:

This document presents the method and results from an accredited COMOHAC T-coil Probe calibration performed in MVG USA using the COMOHAC test bench, for use with a MVG COMOHAC system only. All calibration results are traceable to national metrology institutions.



COMOHAC T-COIL PROBE CALIBRATION REPORT

Ref: ACR.93.14.17.SATU.A

| | Name | Function | Date | Signature |
|---------------|---------------|-----------------|----------|-----------|
| Prepared by : | Jérôme LUC | Product Manager | 4/3/2017 | |
| Checked by : | Jérôme LUC | Product Manager | 4/3/2017 | |
| Approved by : | Kim RUTKOWSKI | Quality Manager | 4/3/2017 | |

| Distribution : | Customer Name |
|----------------|---|
| | SHENZHEN BALUN TECHNOLOGY Co.,Ltd. |

| Issue | Date | Modifications |
|-------|----------|-----------------|
| A | 4/3/2017 | Initial release |
| | | |
| | | |
| | | |

Page: 2/7

*This document shall not be reproduced, except in full or in part, without the written approval of MVG.
The information contained herein is to be used only for the purpose for which it is submitted and is not to
be released in whole or part without written approval of MVG.*

**TABLE OF CONTENTS**

| | | |
|-----|---|---|
| 1 | Device Under Test | 4 |
| 2 | Product Description | 4 |
| 2.1 | General Information | 4 |
| 3 | Measurement Method | 4 |
| 3.1 | Sensitivity | 4 |
| 3.2 | Linearity | 4 |
| 3.3 | Signal to Noise Measurement of the Calibration System | 5 |
| 4 | Measurement Uncertainty | 5 |
| 5 | Calibration Measurement Results | 5 |
| 5.1 | Sensitivity | 6 |
| 5.2 | Linearity | 6 |
| 5.3 | Signal to Noise measurement of the Calibration System | 6 |
| 6 | List of Equipment | 7 |



1 DEVICE UNDER TEST

| Device Under Test | |
|--------------------------------|----------------------|
| Device Type | COMOHAC T-COIL PROBE |
| Manufacturer | MVG |
| Model | STCOIL |
| Serial Number | SN 46/15 TCP34 |
| Product Condition (new / used) | New |
| Frequency Range of Probe | 200-5000 Hz |

A yearly calibration interval is recommended.

2 PRODUCT DESCRIPTION

2.1 GENERAL INFORMATION

MVG's COMOHAC T-coil Probes are built in accordance to the ANSI C63.19 and IEEE 1027 standards.



Figure 1 – MVG COMOHAC T-coil Probe

| | |
|---------------------|-----------------------------------|
| Coil Dimension | 6.55 mm length * 2.29 mm diameter |
| DC resistance | 860.6 Ω |
| Wire size | 51AWG |
| Inductance at 1 kHz | 132.1 mH at 1 kHz |

3 MEASUREMENT METHOD

All methods used to perform the measurements and calibrations comply with the ANSI C63.19 and IEEE 1027 standards. All measurements were performed using a Helmholtz coil built according to the specifications outlined in ANSI C63.19 and IEEE 1027.

3.1 SENSITIVITY

The T-coil was positioned within the Helmholtz coil in axial orientation. Using an audio generator connected to the input of the Helmholtz coil, a known field (1 A/m) was generated within the coil and the T-coil probe reading recorded over the frequency range of 100 Hz to 1000 Hz.

3.2 LINEARITY

The T-coil probe was positioned within the Helmholtz coil in axial orientation. The audio generator connected to the input of the Helmholtz coil was adjusted to obtain a field within the coil from 0 dB A/m to -50 dB A/m and the T-coil reading recorded at each power level (10 dB steps).

Page: 4/7

*This document shall not be reproduced, except in full or in part, without the written approval of MVG.
The information contained herein is to be used only for the purpose for which it is submitted and is not to
be released in whole or part without written approval of MVG.*



3.3 SIGNAL TO NOISE MEASUREMENT OF THE CALIBRATION SYSTEM

The T-coil probe was positioned within the Helmholtz coil in axial orientation. The audio generator connected to the input of the Helmholtz coil was adjusted to obtain a field of -50 dB A/m. The T-coil reading was recorded. The audio generator is then turned off and the T-coil reading recorded.

4 MEASUREMENT UNCERTAINTY

The guideline outlined in the IEEE ANSI C63.19 standard was followed to generate the measurement uncertainty for validation measurements. All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of $k=2$, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

| Uncertainty analysis of the T-coil probe calibration | | | | | |
|---|---------------------|-------------|------------|---------------------|-----------------|
| Uncertainty Component | Tol. (\pm dB) | Prob. Dist. | Div. | Uncertainty (dB) | Uncertainty (%) |
| Current/Voltage Accuracy | 0.224 | R | $\sqrt{3}$ | 0.13 | |
| Acoustic/ Signal Source drift | 0.008 | R | $\sqrt{3}$ | 0.00 | |
| Probe coil sensitivity | 0.2 | R | $\sqrt{3}$ | 0.12 | |
| Positioning accuracy | 0.4 | R | $\sqrt{3}$ | 0.23 | |
| Acoustic Signal Receive Accuracy | 0.03 | R | $\sqrt{3}$ | 0.02 | |
| Acoustic Signal Receive Linearity | 0.006 | R | $\sqrt{3}$ | 0.00 | |
| System repeatability | 0.4 | N | 1 | 0.40 | |
| Combined Standard Uncertainty | | N | 1 | 0.49 | |
| Expanded uncertainty (confidence level of 95%, $k=2$) | | N | $k=2$ | 1.00 | 12.0 |

5 CALIBRATION MEASUREMENT RESULTS

| Calibration Parameters | |
|------------------------|------|
| Lab Temperature | 21°C |
| Lab Humidity | 45% |




COMOHAC T-COIL PROBE CALIBRATION REPORT


Ref: ACR.93.14.17.SATU.A

5.1 SENSITIVITY

Probe coil sensitivity relative to sensitivity at 1000 Hz

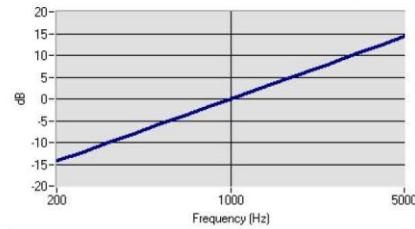

| | Measured | Required |
|---------------------------------|-------------------|--------------------------|
| Sensitivity at 1 kHz | -60.19 dB (V/A/m) | -60.5 +/- 0.5 dB (V/A/m) |
| Max. deviation from Sensitivity | 0.40 dB | +/- 0.5 dB |

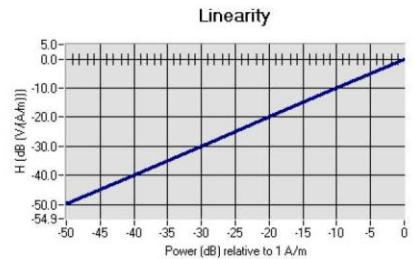5.2 LINEARITY

| | Measured | Required |
|-----------------|----------|------------|
| Linearity Slope | 0.09 dB | +/- 0.5 dB |

5.3 SIGNAL TO NOISE MEASUREMENT OF THE CALIBRATION SYSTEM

| | Measured | Required |
|-----------------|---------------|--|
| Signal to Noise | -63.14 dB A/m | 'Reading with -50 dB A/m in coil' – 'no signal applied' > 10 dB |

Page: 6/7

*This document shall not be reproduced, except in full or in part, without the written approval of MVG.
The information contained herein is to be used only for the purpose for which it is submitted and is not to
be released in whole or part without written approval of MVG.*

**6 LIST OF EQUIPMENT**

| Equipment Summary Sheet | | | | |
|-------------------------------|----------------------|--------------------|-----------------------------|-----------------------------|
| Equipment Description | Manufacturer / Model | Identification No. | Current Calibration Date | Next Calibration Date |
| COMOHAC Test Bench | Version 2 | NA | Validated. No cal required. | Validated. No cal required. |
| Audio Generator | National Instruments | 15222AE | 02/2017 | 02/2020 |
| Reference Probe | MVG | TCP 18 SN 47/10 | 10/2016 | 10/2017 |
| Multimeter | Keithley 2000 | 1188656 | 01/2017 | 01/2020 |
| Helmholtz Coil | MVG | HC07 SN47/10 | Validated. No cal required. | Validated. No cal required. |
| Temperature / Humidity Sensor | Control Company | 150798832 | 10/2015 | 10/2017 |

F.3 800-950MHz Dipole

**HAC Reference Dipole Calibration Report**

Ref : ACR.75.23.17.SATU.A

SHENZHEN BALUN TECHNOLOGY CO.,LTD.
BLOCK B, FL 1, BAISHA SCIENCE AND TECHNOLOGY
PARK, SHAHE XI ROAD,
NANSHAN DISTRICT, SHENZHEN, GUANGDONG
PROVINCE, P.R. CHINA 518055
MVG COMOHAC REFERENCE DIPOLE
FREQUENCY: 800-950MHZ
SERIAL NO.: SN 18/12 DHA41

Calibrated at MVG US
2105 Barrett Park Dr. - Kennesaw, GA 30144



02/17/2017

Summary:

This document presents the method and results from an accredited HAC reference dipole calibration performed in MVG USA using the COMOHAC test bench. All calibration results are traceable to national metrology institutions.



HAC REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.75.19.15.SATU.A

| | Name | Function | Date | Signature |
|---------------|---------------|-----------------|-----------|---------------|
| Prepared by : | Jérôme LUC | Product Manager | 2/25/2017 | |
| Checked by : | Jérôme LUC | Product Manager | 2/25/2017 | |
| Approved by : | Kim RUTKOWSKI | Quality Manager | 2/25/2017 | Kim RUTKOWSKI |

| | Customer Name |
|----------------|---|
| Distribution : | SHENZHEN BALUN TECHNOLOGY Co.,Ltd. |

| Issue | Date | Modifications |
|-------|-----------|-----------------|
| A | 2/25/2017 | Initial release |
| | | |
| | | |
| | | |

Page: 2/8

*This document shall not be reproduced, except in full or in part, without the written approval of MVG.
The information contained herein is to be used only for the purpose for which it is submitted and is not to
be released in whole or part without written approval of MVG.*

**TABLE OF CONTENTS**

| | | |
|-----|--------------------------------------|---|
| 1 | Introduction..... | 4 |
| 2 | Device Under TEst..... | 4 |
| 3 | Product Description | 4 |
| 3.1 | General Information | 4 |
| 4 | Measurement Method | 4 |
| 4.1 | Return Loss Requirements | 5 |
| 4.2 | Reference Dipole Calibration | 5 |
| 5 | Measurement Uncertainty..... | 5 |
| 5.1 | Return Loss | 5 |
| 5.2 | Validation Measurement | 5 |
| 6 | Calibration Measurement Results..... | 6 |
| 6.1 | Return Loss | 6 |
| 6.2 | Validation measurement | 6 |
| 7 | List of Equipment | 8 |



1 INTRODUCTION

This document contains a summary of the requirements set forth by the ANSI C63.19 standard for reference dipoles used for HAC measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

2 DEVICE UNDER TEST

| Device Under Test | |
|--------------------------------|--------------------------------------|
| Device Type | COMOHAC 800-950 MHz REFERENCE DIPOLE |
| Manufacturer | MVG |
| Model | SIDB835 |
| Serial Number | SN 18/12 DHA41 |
| Product Condition (new / used) | Used |

A yearly calibration interval is recommended.

3 PRODUCT DESCRIPTION

3.1 GENERAL INFORMATION

MVG's COMOHAC Validation Dipoles are built in accordance to the ANSI C63.19 standard. The product is designed for use with the COMOHAC system only.



Figure 1 – MVG COMOHAC Validation Dipole

4 MEASUREMENT METHOD

The ANSI C63.19 standard outlines the requirements for reference dipoles to be used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standard.

Page: 4/8

*This document shall not be reproduced, except in full or in part, without the written approval of MVG.
The information contained herein is to be used only for the purpose for which it is submitted and is not to
be released in whole or part without written approval of MVG.*



4.1 RETURN LOSS REQUIREMENTS

The dipole used for HAC system validation measurements and checks must have a return loss of -10 dB or better. The return loss measurement shall be performed in free space.

4.2 REFERENCE DIPOLE CALIBRATION

The IEEE ANSI C63-19 standard states that the dipole used for validation measurements and checks must be scanned with the E and H field probe, with the dipole 10 mm below the probe. The E and H field strength plots are compared to the simulation results obtained by MVG.

5 MEASUREMENT UNCERTAINTY

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of $k=2$, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

5.1 RETURN LOSS

The following uncertainties apply to the return loss measurement:

| Frequency band | Expanded Uncertainty on Gain |
|----------------|------------------------------|
| 400-6000MHz | 0.1 dB |

5.2 VALIDATION MEASUREMENT


The guideline outlined in the IEEE ANSI C63.19 standard was followed to generate the measurement uncertainty for validation measurements.

| Uncertainty analysis of the probe calibration in waveguide | | | | | |
|--|-----------------------|--------------------------|------------|------------------|--------------------------|
| ERROR SOURCES | Uncertainty value (%) | Probability Distribution | Divisor | Uncertainty (dB) | Standard Uncertainty (%) |
| RF reflections | 0.1 | R | $\sqrt{3}$ | 0.06 | |
| Field probe conv. Factor | 0.4 | R | | 0.23 | |
| Field probe anisotropy | 0.25 | R | | 0.14 | |
| Positioning accuracy | 0.2 | R | | 0.12 | |
| Probe cable placement | 0.1 | R | | 0.06 | |
| System repeatability | 0.2 | R | $\sqrt{3}$ | 0.12 | |
| EUT repeatability | 0.4 | N | 1 | 0.40 | |
| Combined standard uncertainty | | | | 0.52 | |
| Expanded uncertainty 95 % confidence level $k = 2$ | | | | 1.00 | 13.0 |



HAC REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.75.23.17.SATU.A

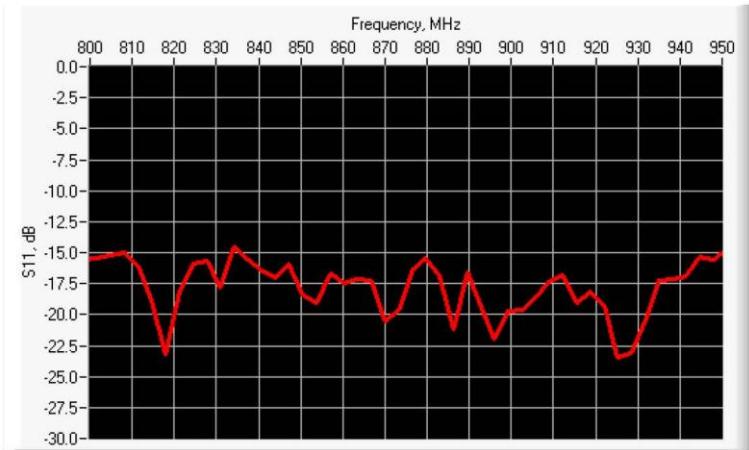6 CALIBRATION MEASUREMENT RESULTS**6.1 RETURN LOSS**

| Frequency (MHz) | Worst Case Return Loss (dB) | Requirement (dB) |
|-----------------|-----------------------------|------------------|
| 800-950 MHz | -14.53 | -10 |

6.2 VALIDATION MEASUREMENT

The IEEE ANSI C63.19 standard states that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss requirements. The system validations measurement results are then compared to MVG's simulated results.

Measurement Condition

| | |
|---|-----------------|
| Software Version | OpenHAC V2 |
| HAC positioning ruler | SN 42/09 TABH12 |
| E-Field probe | SN 08/11 EPH28 |
| H-Field probe | SN 31/10 HPH38 |
| Distance between dipole and sensor center | 10 mm |
| E-field scan size | X=150mm/Y=20mm |
| H-field scan size | X=40mm/Y=20mm |
| Scan resolution | dx=5mm/dy=5mm |
| Frequency | 835 MHz |
| Input power | 20 dBm |
| Lab Temperature | 21°C |
| Lab Humidity | 45% |

Page: 6/8

*This document shall not be reproduced, except in full or in part, without the written approval of MVG.
The information contained herein is to be used only for the purpose for which it is submitted and is not to
be released in whole or part without written approval of MVG.*





HAC REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.75.23.17.SATU.A

Measurement Result

| | Measured | Internal Requirement |
|---------------|----------|----------------------|
| E field (V/m) | 220.88 | 220.4 |
| H field (A/m) | 0.45 | 0.445 |

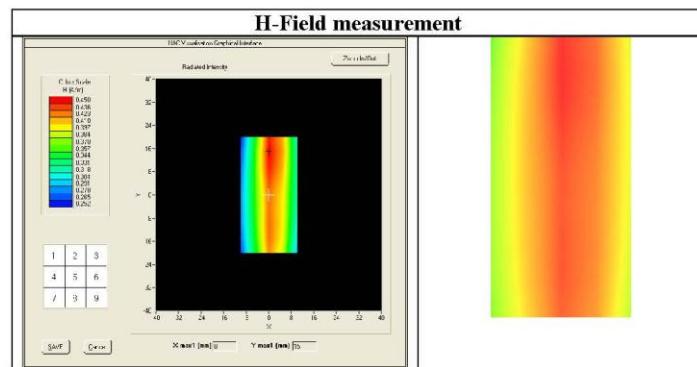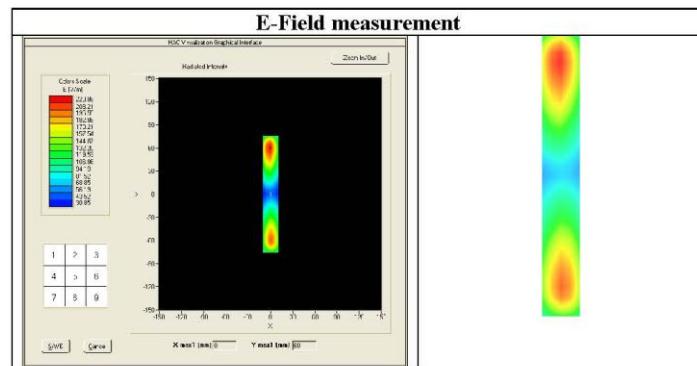

Page: 7/8

This document shall not be reproduced, except in full or in part, without the written approval of MVG.
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.



7 LIST OF EQUIPMENT

| Equipment Summary Sheet | | | | |
|---------------------------------|----------------------|--------------------|---|---|
| Equipment Description | Manufacturer / Model | Identification No. | Current Calibration Date | Next Calibration Date |
| HAC positioning ruler | MVG | TABH12 SN 42/09 | Validated. No cal required. | Validated. No cal required. |
| COMOHAC Test Bench | Version 2 | NA | Validated. No cal required. | Validated. No cal required. |
| Network Analyzer | Rhode & Schwarz ZVA | SN100132 | 02/2016 | 02/2019 |
| Reference Probe | MVG | EPH28 SN 08/11 | 10/2016 | 10/2017 |
| Reference Probe | MVG | HPH38 SN31/10 | 10/2016 | 10/2017 |
| Multimeter | Keithley 2000 | 1188656 | 01/2017 | 01/2020 |
| Signal Generator | Agilent E4438C | MY49070581 | 01/2017 | 01/2020 |
| Amplifier | Aethercomm | SN 046 | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter | HP E4418A | US38261498 | 01/2017 | 01/2020 |
| Power Sensor | HP ECP-E26A | US37181460 | 01/2017 | 01/2020 |
| Directional Coupler | Narda 4216-20 | 01386 | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature and Humidity Sensor | Control Company | 150798832 | 10/2015 | 10/2017 |

F.4 1700-2000MHz Dipole

**HAC Reference Dipole Calibration Report**

Ref : ACR.75.24.17.SATU.A

SHENZHEN BALUN TECHNOLOGY CO.,LTD.
BLOCK B, FL 1, BAISHA SCIENCE AND TECHNOLOGY
PARK, SHAHE XI ROAD,
NANSAN DISTRICT, SHENZHEN, GUANGDONG
PROVINCE, P.R. CHINA 518055
MVG COMOHAC REFERENCE DIPOLE
FREQUENCY: 1700-2000MHZ
SERIAL NO.: SN 18/12 DHB46

Calibrated at MVG US
2105 Barrett Park Dr. - Kennesaw, GA 30144



02/17/2017

Summary:

This document presents the method and results from an accredited HAC reference dipole calibration performed in MVG USA using the COMOHAC test bench. All calibration results are traceable to national metrology institutions.



HAC REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.75.24.17.SATU.A

| | Name | Function | Date | Signature |
|---------------|---------------|-----------------|-----------|-----------|
| Prepared by : | Jérôme LUC | Product Manager | 2/25/2017 | |
| Checked by : | Jérôme LUC | Product Manager | 2/25/2017 | |
| Approved by : | Kim RUTKOWSKI | Quality Manager | 2/25/2017 | |

| | Customer Name |
|----------------|---|
| Distribution : | SHENZHEN BALUN TECHNOLOGY Co.,Ltd. |

| Issue | Date | Modifications |
|-------|-----------|-----------------|
| A | 2/25/2017 | Initial release |
| | | |
| | | |
| | | |

Page: 2/8

*This document shall not be reproduced, except in full or in part, without the written approval of MVG.
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.*



TABLE OF CONTENTS

| | | |
|-----|--------------------------------------|---|
| 1 | Introduction..... | 4 |
| 2 | Device Under TEst..... | 4 |
| 3 | Product Description | 4 |
| 3.1 | General Information | 4 |
| 4 | Measurement Method | 4 |
| 4.1 | Return Loss Requirements | 5 |
| 4.2 | Reference Dipole Calibration | 5 |
| 5 | Measurement Uncertainty..... | 5 |
| 5.1 | Return Loss | 5 |
| 5.2 | Validation Measurement | 5 |
| 6 | Calibration Measurement Results..... | 6 |
| 6.1 | Return Loss | 6 |
| 6.2 | Validation measurement | 6 |
| 7 | List of Equipment | 8 |



1 INTRODUCTION

This document contains a summary of the requirements set forth by the ANSI C63.19 standard for reference dipoles used for HAC measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

2 DEVICE UNDER TEST

| Device Under Test | |
|--------------------------------|--|
| Device Type | COMOHAC 1700-2000 MHz REFERENCE DIPOLE |
| Manufacturer | MVG |
| Model | SIDB1900 |
| Serial Number | SN 18/12 DHB46 |
| Product Condition (new / used) | Used |

A yearly calibration interval is recommended.

3 PRODUCT DESCRIPTION

3.1 GENERAL INFORMATION

MVG's COMOHAC Validation Dipoles are built in accordance to the ANSI C63.19 standard. The product is designed for use with the COMOHAC system only.



Figure 1 – MVG COMOHAC Validation Dipole

4 MEASUREMENT METHOD

The ANSI C63.19 standard outlines the requirements for reference dipoles to be used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standard.

Page: 4/8

*This document shall not be reproduced, except in full or in part, without the written approval of MVG.
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.*



4.1 RETURN LOSS REQUIREMENTS

The dipole used for HAC system validation measurements and checks must have a return loss of -10 dB or better. The return loss measurement shall be performed in free space.

4.2 REFERENCE DIPOLE CALIBRATION

The IEEE ANSI C63-19 standard states that the dipole used for validation measurements and checks must be scanned with the E and H field probe, with the dipole 10 mm below the probe. The E and H field strength plots are compared to the simulation results obtained by MVG.

5 MEASUREMENT UNCERTAINTY

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of $k=2$, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

5.1 RETURN LOSS

The following uncertainties apply to the return loss measurement:

| Frequency band | Expanded Uncertainty on Gain |
|----------------|------------------------------|
| 400-6000MHz | 0.1 dB |

5.2 VALIDATION MEASUREMENT


The guideline outlined in the IEEE ANSI C63.19 standard was followed to generate the measurement uncertainty for validation measurements.

| Uncertainty analysis of the probe calibration in waveguide | | | | | |
|--|-----------------------|--------------------------|------------|------------------|--------------------------|
| ERROR SOURCES | Uncertainty value (%) | Probability Distribution | Divisor | Uncertainty (dB) | Standard Uncertainty (%) |
| RF reflections | 0.1 | R | $\sqrt{3}$ | 0.06 | |
| Field probe conv. Factor | 0.4 | R | | 0.23 | |
| Field probe anisotropy | 0.25 | R | | 0.14 | |
| Positioning accuracy | 0.2 | R | | 0.12 | |
| Probe cable placement | 0.1 | R | | 0.06 | |
| System repeatability | 0.2 | R | $\sqrt{3}$ | 0.12 | |
| EUT repeatability | 0.4 | N | 1 | 0.40 | |
| Combined standard uncertainty | | | | 0.52 | |
| Expanded uncertainty 95 % confidence level $k = 2$ | | | | 1.00 | 13.0 |



6 CALIBRATION MEASUREMENT RESULTS

6.1 RETURN LOSS

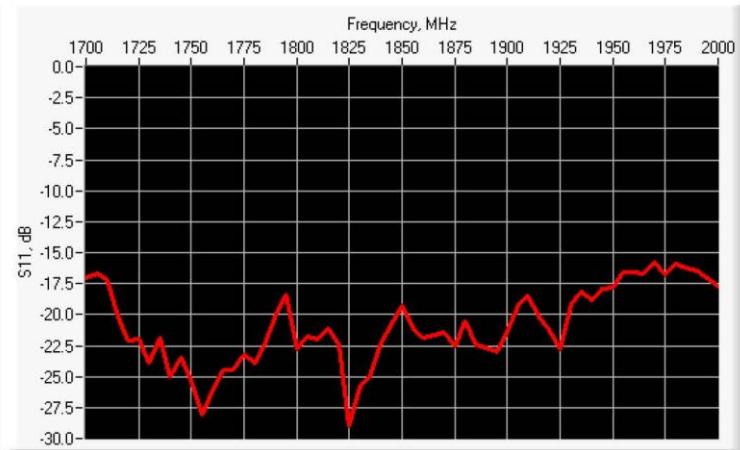

| Frequency (MHz) | Worst Case Return Loss (dB) | Requirement (dB) |
|-----------------|-----------------------------|------------------|
| 1700-2000 MHz | -15.78 | -10 |

6.2 VALIDATION MEASUREMENT

The IEEE ANSI C63.19 standard states that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss requirements. The system validations measurement results are then compared to MVG's simulated results.

Measurement Condition

| | |
|---|-----------------|
| Software Version | OpenHAC V2 |
| HAC positioning ruler | SN 42/09 TABH12 |
| E-Field probe | SN 08/11 EPH28 |
| H-Field probe | SN 31/10 HPH38 |
| Distance between dipole and sensor center | 10 mm |
| E-field scan size | X=150mm/Y=20mm |
| H-field scan size | X=40mm/Y=20mm |
| Scan resolution | dx=5mm/dy=5mm |
| Frequency | 1900 MHz |
| Input power | 20 dBm |
| Lab Temperature | 21°C |
| Lab Humidity | 45% |

Page: 6/8

*This document shall not be reproduced, except in full or in part, without the written approval of MVG.
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.*





HAC REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.75.24.17.SATU.A

Measurement Result

| | Measured | Internal Requirement |
|---------------|----------|----------------------|
| E field (V/m) | 161.34 | 153.4 |
| H field (A/m) | 0.45 | 0.445 |

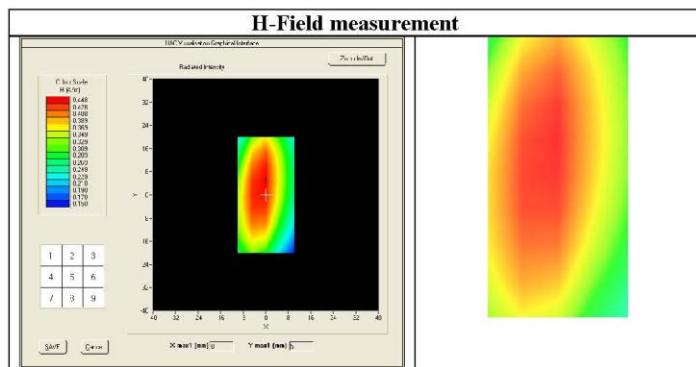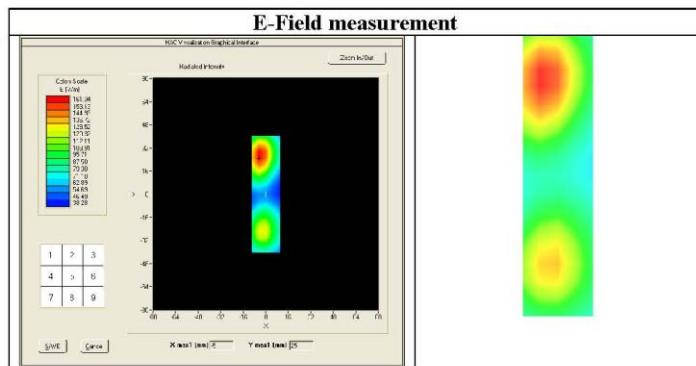

Page: 7/8

This document shall not be reproduced, except in full or in part, without the written approval of MVG.
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.



7 LIST OF EQUIPMENT

| Equipment Summary Sheet | | | | |
|---------------------------------|----------------------|--------------------|---|---|
| Equipment Description | Manufacturer / Model | Identification No. | Current Calibration Date | Next Calibration Date |
| HAC positioning ruler | MVG | TABH12 SN 42/09 | Validated. No cal required. | Validated. No cal required. |
| COMOHAC Test Bench | Version 2 | NA | Validated. No cal required. | Validated. No cal required. |
| Network Analyzer | Rhode & Schwarz ZVA | SN100132 | 02/2016 | 02/2019 |
| Reference Probe | MVG | EPH28 SN 08/11 | 10/2016 | 10/2017 |
| Reference Probe | MVG | HPH38 SN31/10 | 10/2016 | 10/2017 |
| Multimeter | Keithley 2000 | 1188656 | 01/2017 | 01/2020 |
| Signal Generator | Agilent E4438C | MY49070581 | 01/2017 | 01/2020 |
| Amplifier | Aethercomm | SN 046 | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter | HP E4418A | US38261498 | 01/2017 | 01/2020 |
| Power Sensor | HP ECP-E26A | US37181460 | 01/2017 | 01/2020 |
| Directional Coupler | Narda 4216-20 | 01386 | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature and Humidity Sensor | Control Company | 150798832 | 10/2015 | 10/2017 |

F.5 TMFS Calibration Report

**COMOHAC TMFS Calibration Report**

Ref : ACR.93.17.17.SATU.A

SHENZHEN BALUN TECHNOLOGY CO.,LTD.
BLOCK B, FL 1, BAISHA SCIENCE AND TECHNOLOGY
PARK, SHAHE XI ROAD,
NANSAN DISTRICT, SHENZHEN, GUANGDONG PROVINCE, P.R.
CHINA 518055

MVG COMOHAC MAGNETIC FIELD SIMULATOR
SERIAL NO.: SN 24/16 TMFS 27

Calibrated at MVG US
2105 Barrett Park Dr. - Kennesaw, GA 30144



Calibration Date: 03/22/2017

Summary:

This document presents the method and results from an accredited COMOHAC TMFS calibration performed in MVG USA using the COMOHAC test bench, for use with a MVG COMOHAC system only. All calibration results are traceable to national metrology institutions.



COMOHAC TMFS' PROBE CALIBRATION REPORT

Ref: ACR.93.17.17.SATU.A

| | Name | Function | Date | Signature |
|---------------|---------------|-----------------|----------|-----------|
| Prepared by : | Jérôme LUC | Product Manager | 4/3/2017 | |
| Checked by : | Jérôme LUC | Product Manager | 4/3/2017 | |
| Approved by : | Kim RUTKOWSKI | Quality Manager | 4/3/2017 | |

| Distribution : | Customer Name |
|----------------|---|
| | SHENZHEN BALUN TECHNOLOGY Co.,Ltd. |

| Issue | Date | Modifications |
|-------|----------|-----------------|
| A | 4/3/2017 | Initial release |
| | | |
| | | |
| | | |

Page: 2/7

*This document shall not be reproduced, except in full or in part, without the written approval of MVG.
The information contained herein is to be used only for the purpose for which it is submitted and is not to
be released in whole or part without written approval of MVG.*

**TABLE OF CONTENTS**

| | | |
|-----|--|---|
| 1 | Device Under Test | 4 |
| 2 | Product Description | 4 |
| 2.1 | General Information | 4 |
| 3 | Measurement Method | 4 |
| 3.1 | Maximum Axial and Radial Magnetic Field Values | 4 |
| 4 | Measurement Uncertainty..... | 4 |
| 5 | Calibration Measurement Results..... | 5 |
| 5.1 | Maximum Axial and Radial Magnetic Field Values | 6 |
| 6 | List of Equipment | 7 |



COMOHAC TMFS® PROBE CALIBRATION REPORT

Ref: ACR.93.17.17.SATU.A

1 DEVICE UNDER TEST

| Device Under Test | |
|--------------------------------|----------------------------------|
| Device Type | COMOHAC Magnetic Field Simulator |
| Manufacturer | MVG |
| Model | STMFS |
| Serial Number | SN 24/16 TMFS 27 |
| Product Condition (new / used) | New |
| Frequency Range | 200-5000 Hz |

A yearly calibration interval is recommended.

2 PRODUCT DESCRIPTION**2.1 GENERAL INFORMATION**

MVG's COMOHAC T-coil Probes are built in accordance to the ANSI C63.19 and ANSI S3.22-2003 standards.



Figure 1 – MVG COMOHAC Magnetic Field Simulator

3 MEASUREMENT METHOD

All methods used to perform the measurements and calibrations comply with the ANSI C63.19. All measurements were performed with the TMFS in the standard device test configuration, with the TMFS in free space, 10 mm below the coil center.

3.1 MAXIMUM AXIAL AND RADIAL MAGNETIC FIELD VALUES

An audio signal was fed into the TMFS and the magnetic field measured and recorded over an area scan with the T-coil probe in three orientations; axial and two radial. The maximum magnetic field is recorded for all three T-coil orientations.

4 MEASUREMENT UNCERTAINTY

The guideline outlined in the IEEE ANSI C63.19 standard was followed to generate the measurement uncertainty for validation measurements. All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of $k=2$, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

Page: 4/7

*This document shall not be reproduced, except in full or in part, without the written approval of MVG.
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.*



| Uncertainty analysis of the probe calibration in Helmholtz Coil | | | | | |
|---|-------------|-------------|------------|------------------|-----------------|
| Uncertainty Component | Tol. (± dB) | Prob. Dist. | Div. | Uncertainty (dB) | Uncertainty (%) |
| Reflections | 0.1 | R | $\sqrt{3}$ | 0.06 | |
| Acoustic noise | 0.1 | R | $\sqrt{3}$ | 0.06 | |
| Probe coil sensitivity | 0.49 | R | $\sqrt{3}$ | 0.28 | |
| Reference signal level | 0.25 | R | $\sqrt{3}$ | 0.14 | |
| Positioning accuracy | 0.2 | R | $\sqrt{3}$ | 0.12 | |
| Cable loss | 0.1 | N | 1 | 0.05 | |
| Frequency analyzer | 0.15 | R | $\sqrt{3}$ | 0.09 | |
| System repeatability | 0.2 | N | 1 | 0.20 | |
| Repeatability of the WD | 0.1 | N | 1 | 0.10 | |
| Combined standard uncertainty | | N | 1 | 0.43 | |
| Expanded uncertainty 95 % confidence level k = 2 | | N | 2 | 0.85 | 10.3% |

5 CALIBRATION MEASUREMENT RESULTS

| Calibration Parameters | |
|---------------------------------------|-----------------|
| Software | OpenHAC V2 |
| HAC positioning ruler | SN 42/09 TABH12 |
| T-Coil probe | SN 47/10 TCP18 |
| Distance between TMFS and coil center | 10 mm |
| Frequency | 1025 Hz |
| Scan Size | X=70mm/Y=70mm |
| Scan Resolution | dx=5mm/dy=5mm |
| Output level | 0.5 VAC |
| Lab Temperature | 21°C |
| Lab Humidity | 45% |




COMOHAC TMFS® PROBE CALIBRATION REPORT

Ref: ACR.93.17.17.SATU.A

5.1 MAXIMUM AXIAL AND RADIAL MAGNETIC FIELD VALUES

| Test Description | Measured Magnetic Field | |
|-------------------------|--------------------------------|---------------------------|
| | Location | Intensity (dB A/m) |
| Axial | Max | -13.34 |
| Radial H | Right side | -19.93 |
| | Left side | -19.25 |
| Radial V | Upper side | -19.56 |
| | Lower side | -18.55 |

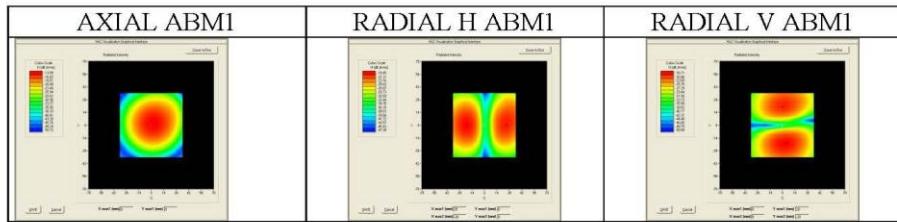



COMOHAC TMFS® PROBE CALIBRATION REPORT

Ref: ACR.93.17.17.SATU.A

6 LIST OF EQUIPMENT

| Equipment Summary Sheet | | | | |
|-------------------------------|----------------------|--------------------|-----------------------------|-----------------------------|
| Equipment Description | Manufacturer / Model | Identification No. | Current Calibration Date | Next Calibration Date |
| COMOHAC Test Bench | Version 2 | NA | Validated. No cal required. | Validated. No cal required. |
| HAC positioning ruler | MVG | TABH12 SN 42/09 | Validated. No cal required. | Validated. No cal required. |
| Audio Generator | National Instruments | 15222AE | 02/2017 | 02/2020 |
| Reference Probe | MVG | TCP 18 SN 47/10 | 10/2016 | 10/2017 |
| Multimeter | Keithley 2000 | 1188656 | 01/2017 | 01/2020 |
| Temperature / Humidity Sensor | Control Company | 150798832 | 10/2015 | 10/2017 |