

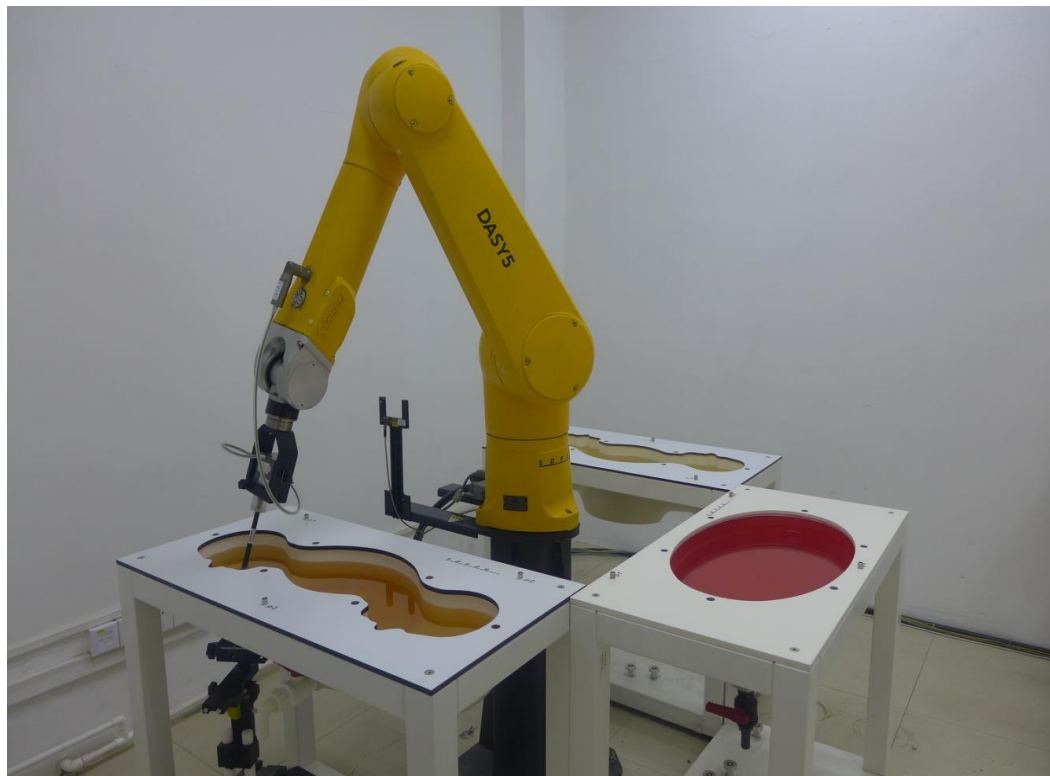


# **Appendix D**

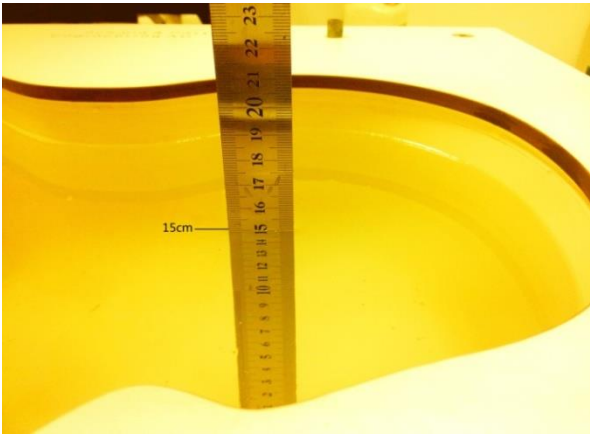
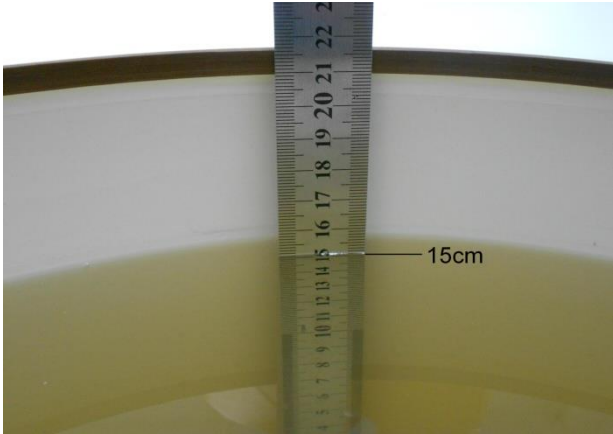
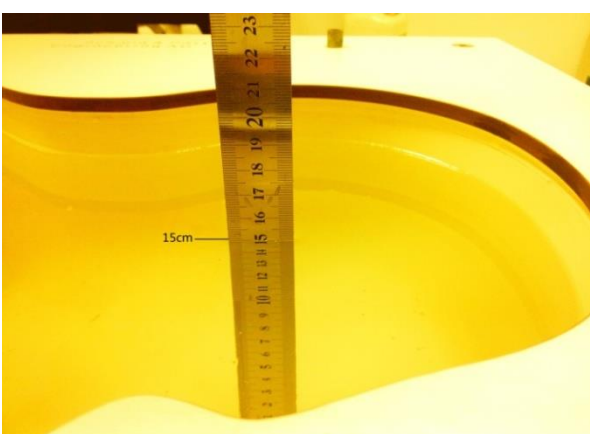
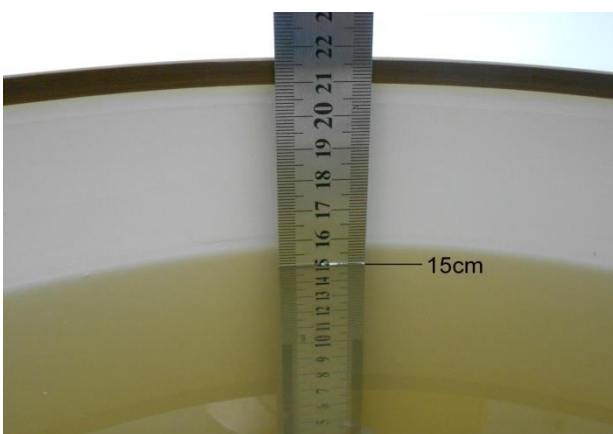
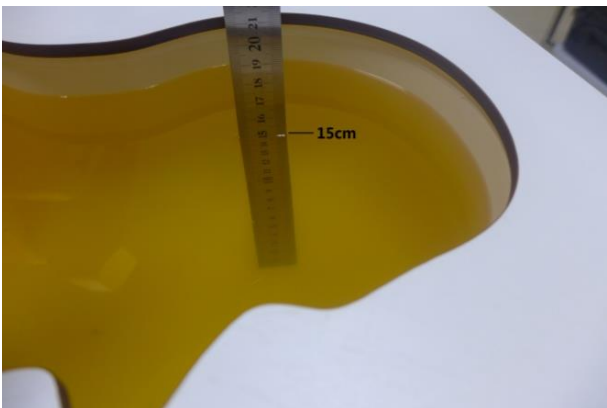
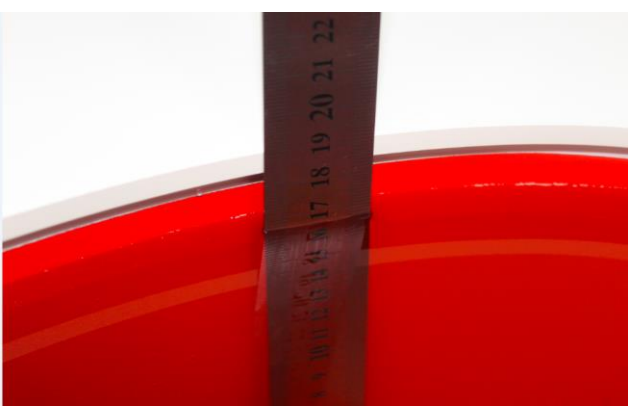
## **Photographs**

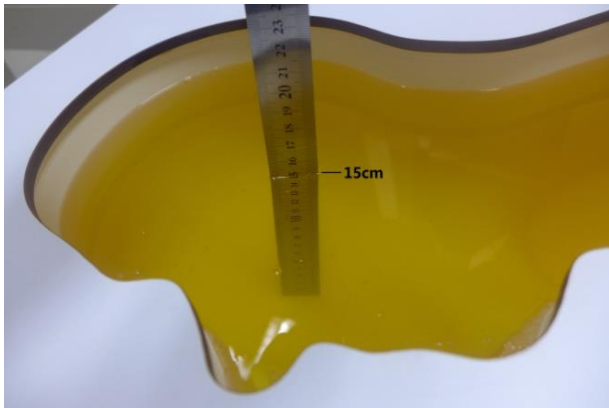

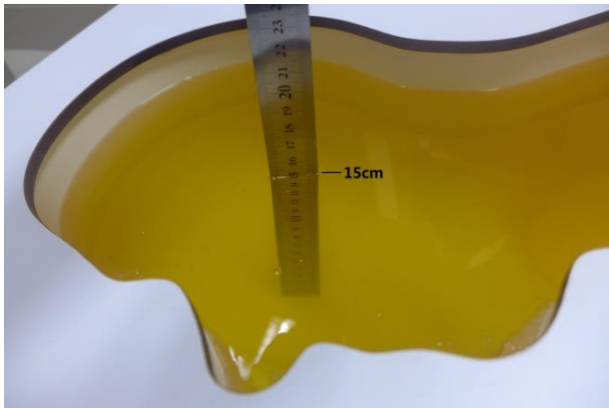

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

## **1. SAR measurement System**

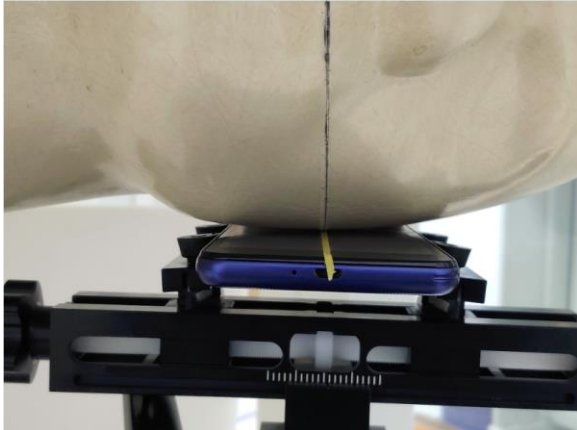
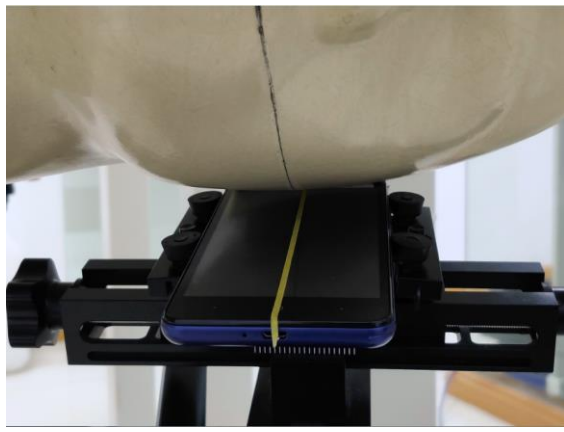
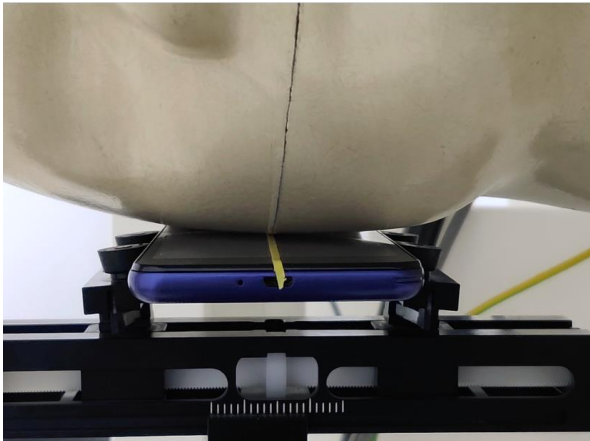
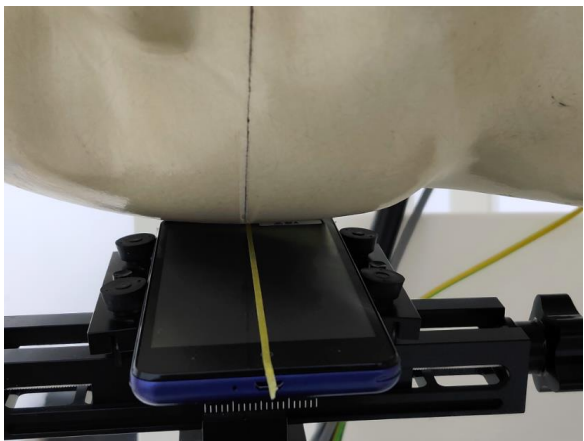
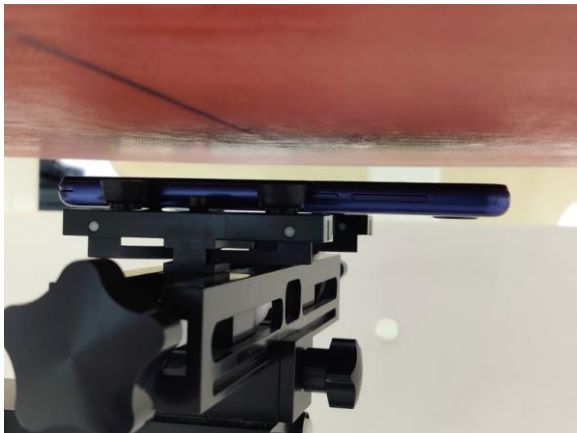
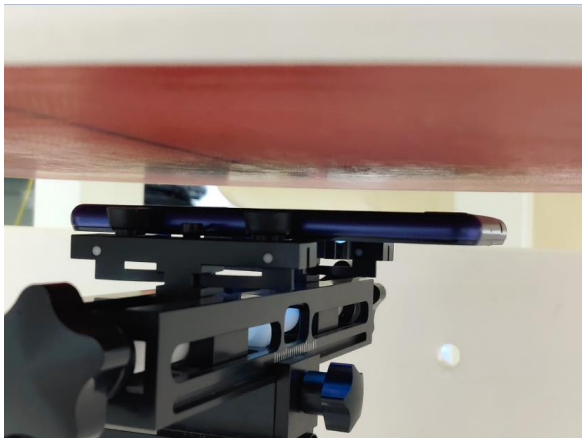


## 2. Photographs of Tissue Simulate Liquid

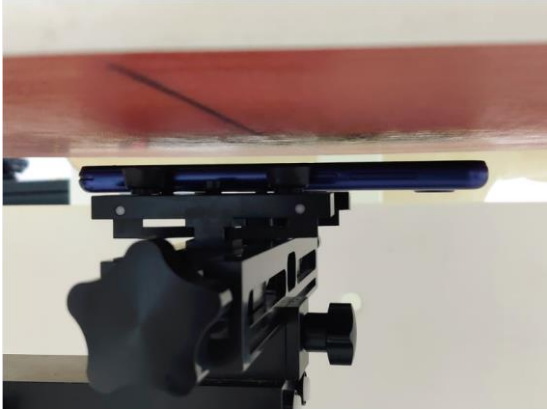
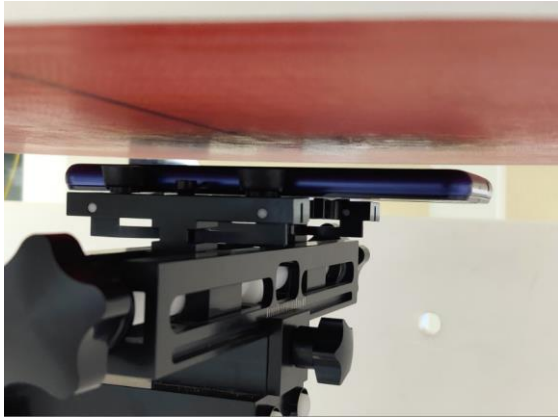
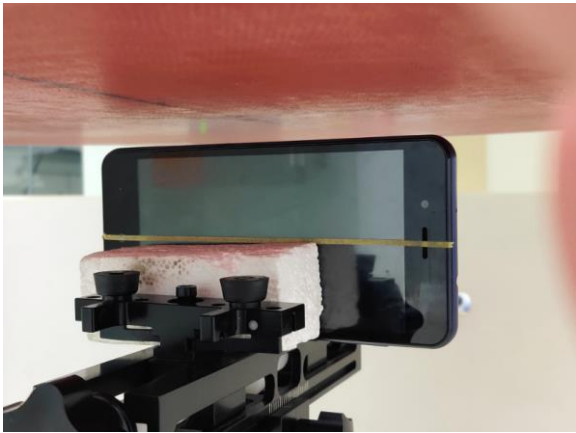
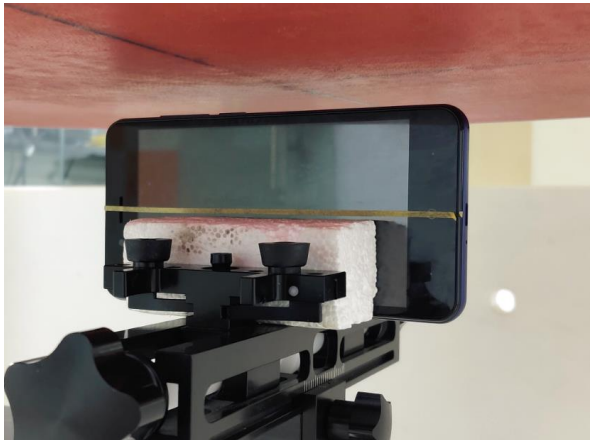

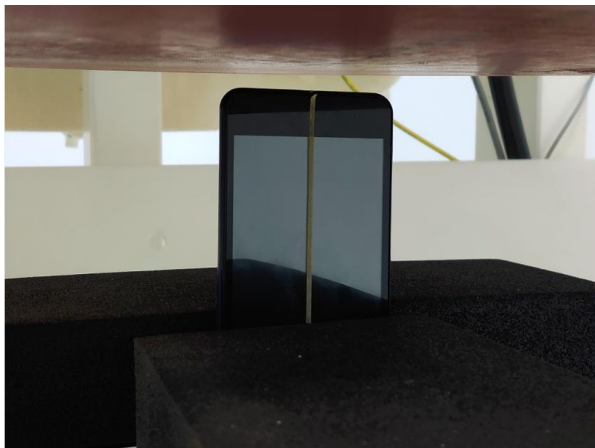
<p><b>Photo 1: Tissue Simulant Liquid for Head 750</b></p>	<p><b>Photo 2: Tissue Simulant Liquid for Body 750</b></p>
	
<p><b>Photo 3: Tissue Simulant Liquid for Head 835</b></p>	<p><b>Photo 4: Tissue Simulant Liquid for Body 835</b></p>
	
<p><b>Photo 5: Tissue Simulant Liquid for Head 1900</b></p>	<p><b>Photo 6: Tissue Simulant Liquid for Body 1900</b></p>
	

<p><b>Photo 7: Tissue Simulant Liquid for Head 2450</b></p>	<p><b>Photo 8: Tissue Simulant Liquid for Body 2450</b></p>
	
<p><b>Photo 9: Tissue Simulant Liquid for Head 2600</b></p>	<p><b>Photo 10: Tissue Simulant Liquid for Body 2600</b></p>
	

### 3. Photographs of EUT test position

Photo 11: Left touch cheek	Photo 12: Left tilted 15 degree
	
Photo 13: Right touch cheek	Photo 14: Right tilted 15 degree
	
Photo 15: Front side 15mm	Photo 16: Back side 15mm
	



<p><b>Photo 17: Front side 10mm</b></p>	<p><b>Photo 18: Back side 10mm</b></p>
	
<p><b>Photo 19: Left side 10mm</b></p>	<p><b>Photo 20: Right side 10mm</b></p>
	
<p><b>Photo 21: Top side 10mm</b></p>	<p><b>Photo 22: Bottom side 10mm</b></p>
	

## 4. EUT Constructional Details

