



DASY/EASY – Parameters of Probe: EX3DV4 – SN:3982

Frequency Response of E-Field

Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz] ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
750	41.9	0.89	10.73	10.73	10.73	0.40	0.75	± 12.1%
835	41.5	0.90	10.32	10.32	10.32	0.28	1.03	± 12.1%
1750	40.1	1.37	8.78	8.78	8.78	0.22	1.05	± 12.1%
1900	40.0	1.40	8.40	8.40	8.40	0.26	0.98	± 12.1%
3300	38.2	2.71	7.41	7.41	7.41	0.40	1.01	± 13.3%
3500	37.9	2.91	7.10	7.10	7.10	0.45	0.93	± 13.3%
3700	37.7	3.12	6.78	6.78	6.78	0.41	1.05	± 13.3%
4100	37.2	3.53	6.71	6.71	6.71	0.40	1.20	± 13.3%
4400	36.9	3.84	6.48	6.48	6.48	0.35	1.35	± 13.3%
4600	36.7	4.04	6.34	6.34	6.34	0.45	1.25	± 13.3%
4800	36.4	4.25	6.30	6.30	6.30	0.45	1.30	± 13.3%
4950	36.3	4.40	5.99	5.99	5.99	0.45	1.30	± 13.3%
5250	35.9	4.71	5.70	5.70	5.70	0.45	1.30	± 13.3%
5600	35.5	5.07	5.12	5.12	5.12	0.50	1.20	± 13.3%
5750	35.4	5.22	5.14	5.14	5.14	0.50	1.20	± 13.3%

^C Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequency below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.


^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.



In Collaboration with
s p e a g
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504
E-mail: cttl@chinattl.com [Http://www.chinattl.cn](http://www.chinattl.cn)

Frequency Response of E-Field (TEM-Cell: ifi110 EXX, Waveguide: R22)

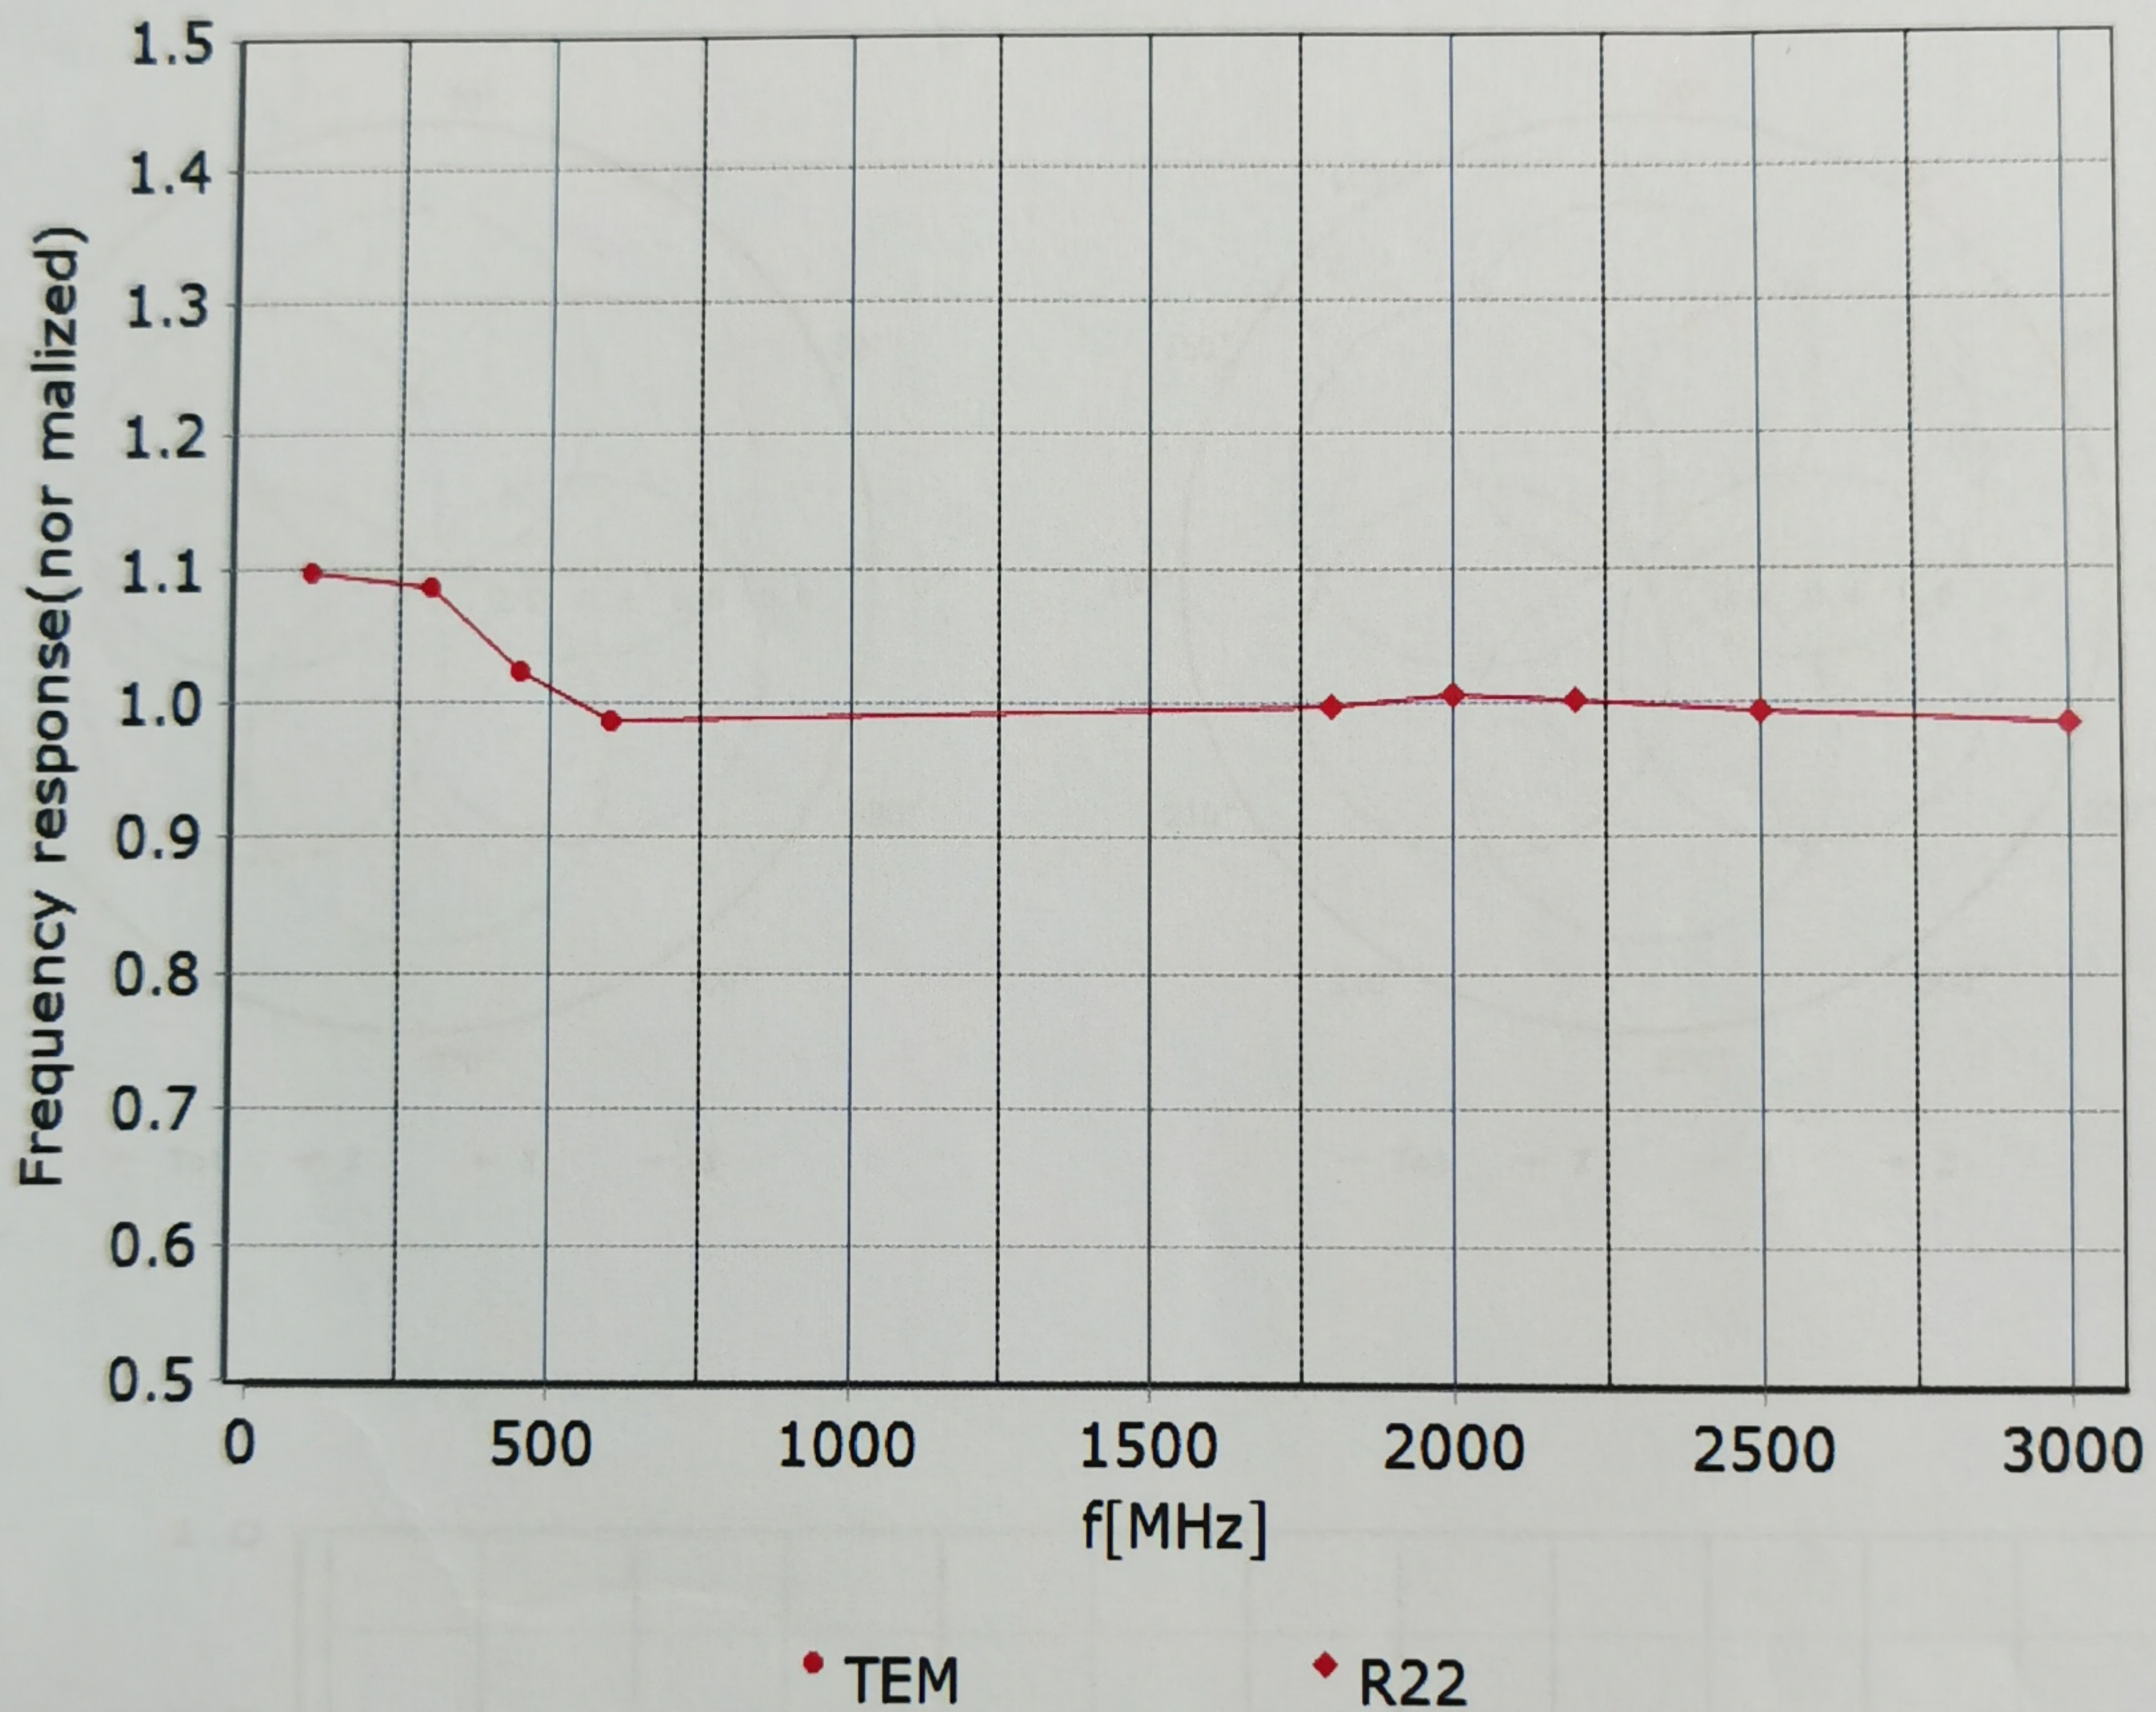

Uncertainty of Frequency Response of E-field: $\pm 7.4\%$ ($k=2$)






In Collaboration with
s p e a g
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504
E-mail: cttl@chinattl.com [Http://www.chinattl.cn](http://www.chinattl.cn)

Receiving Pattern (Φ), $\theta=0^\circ$

f=600 MHz, TEM

f=1800 MHz, R22

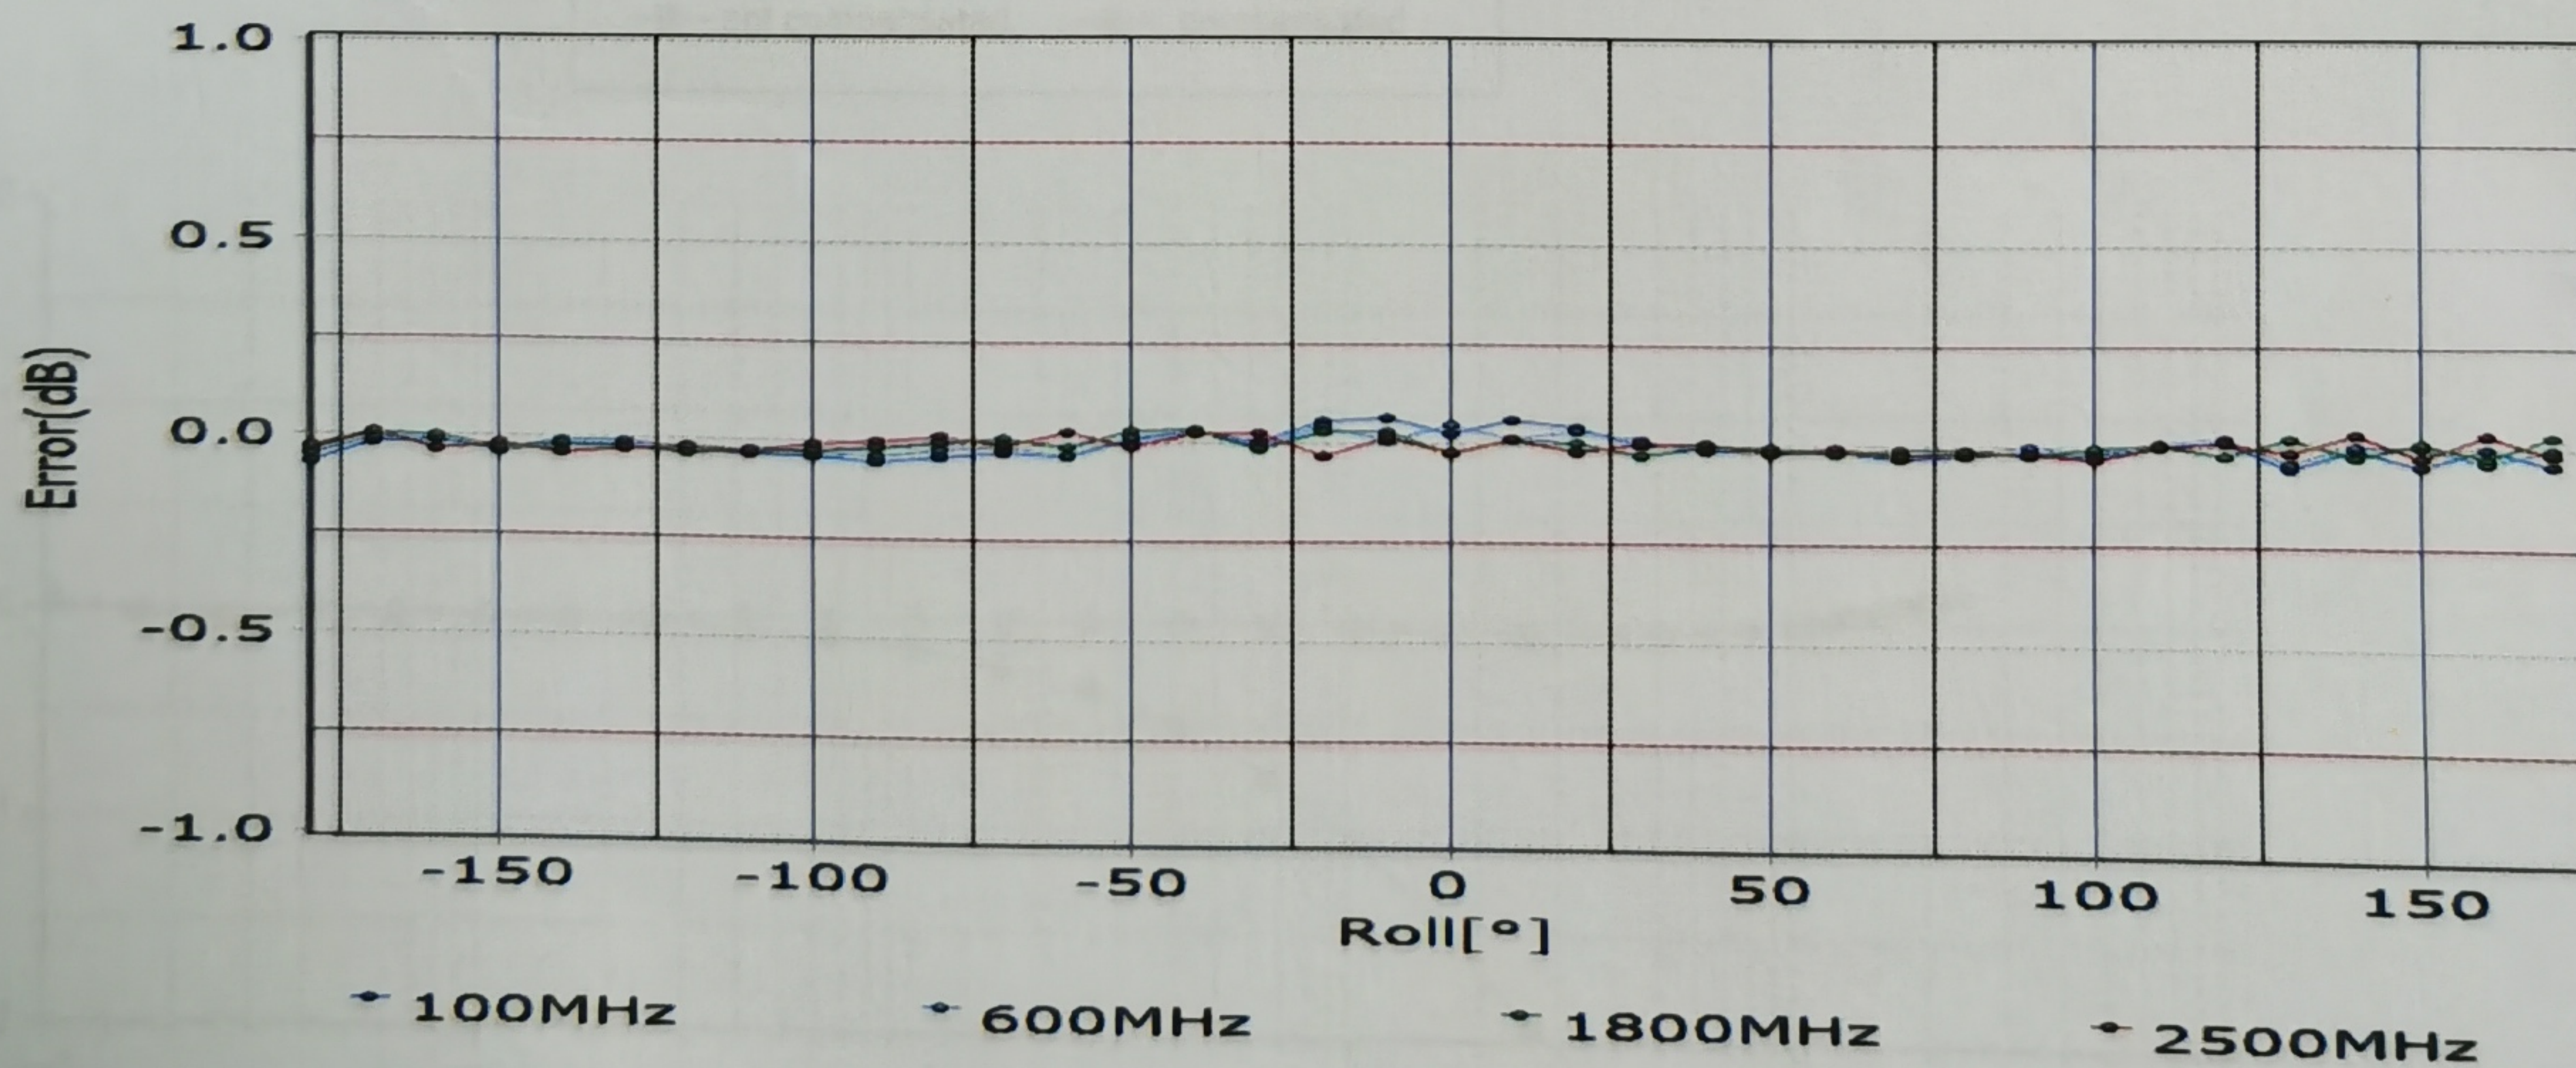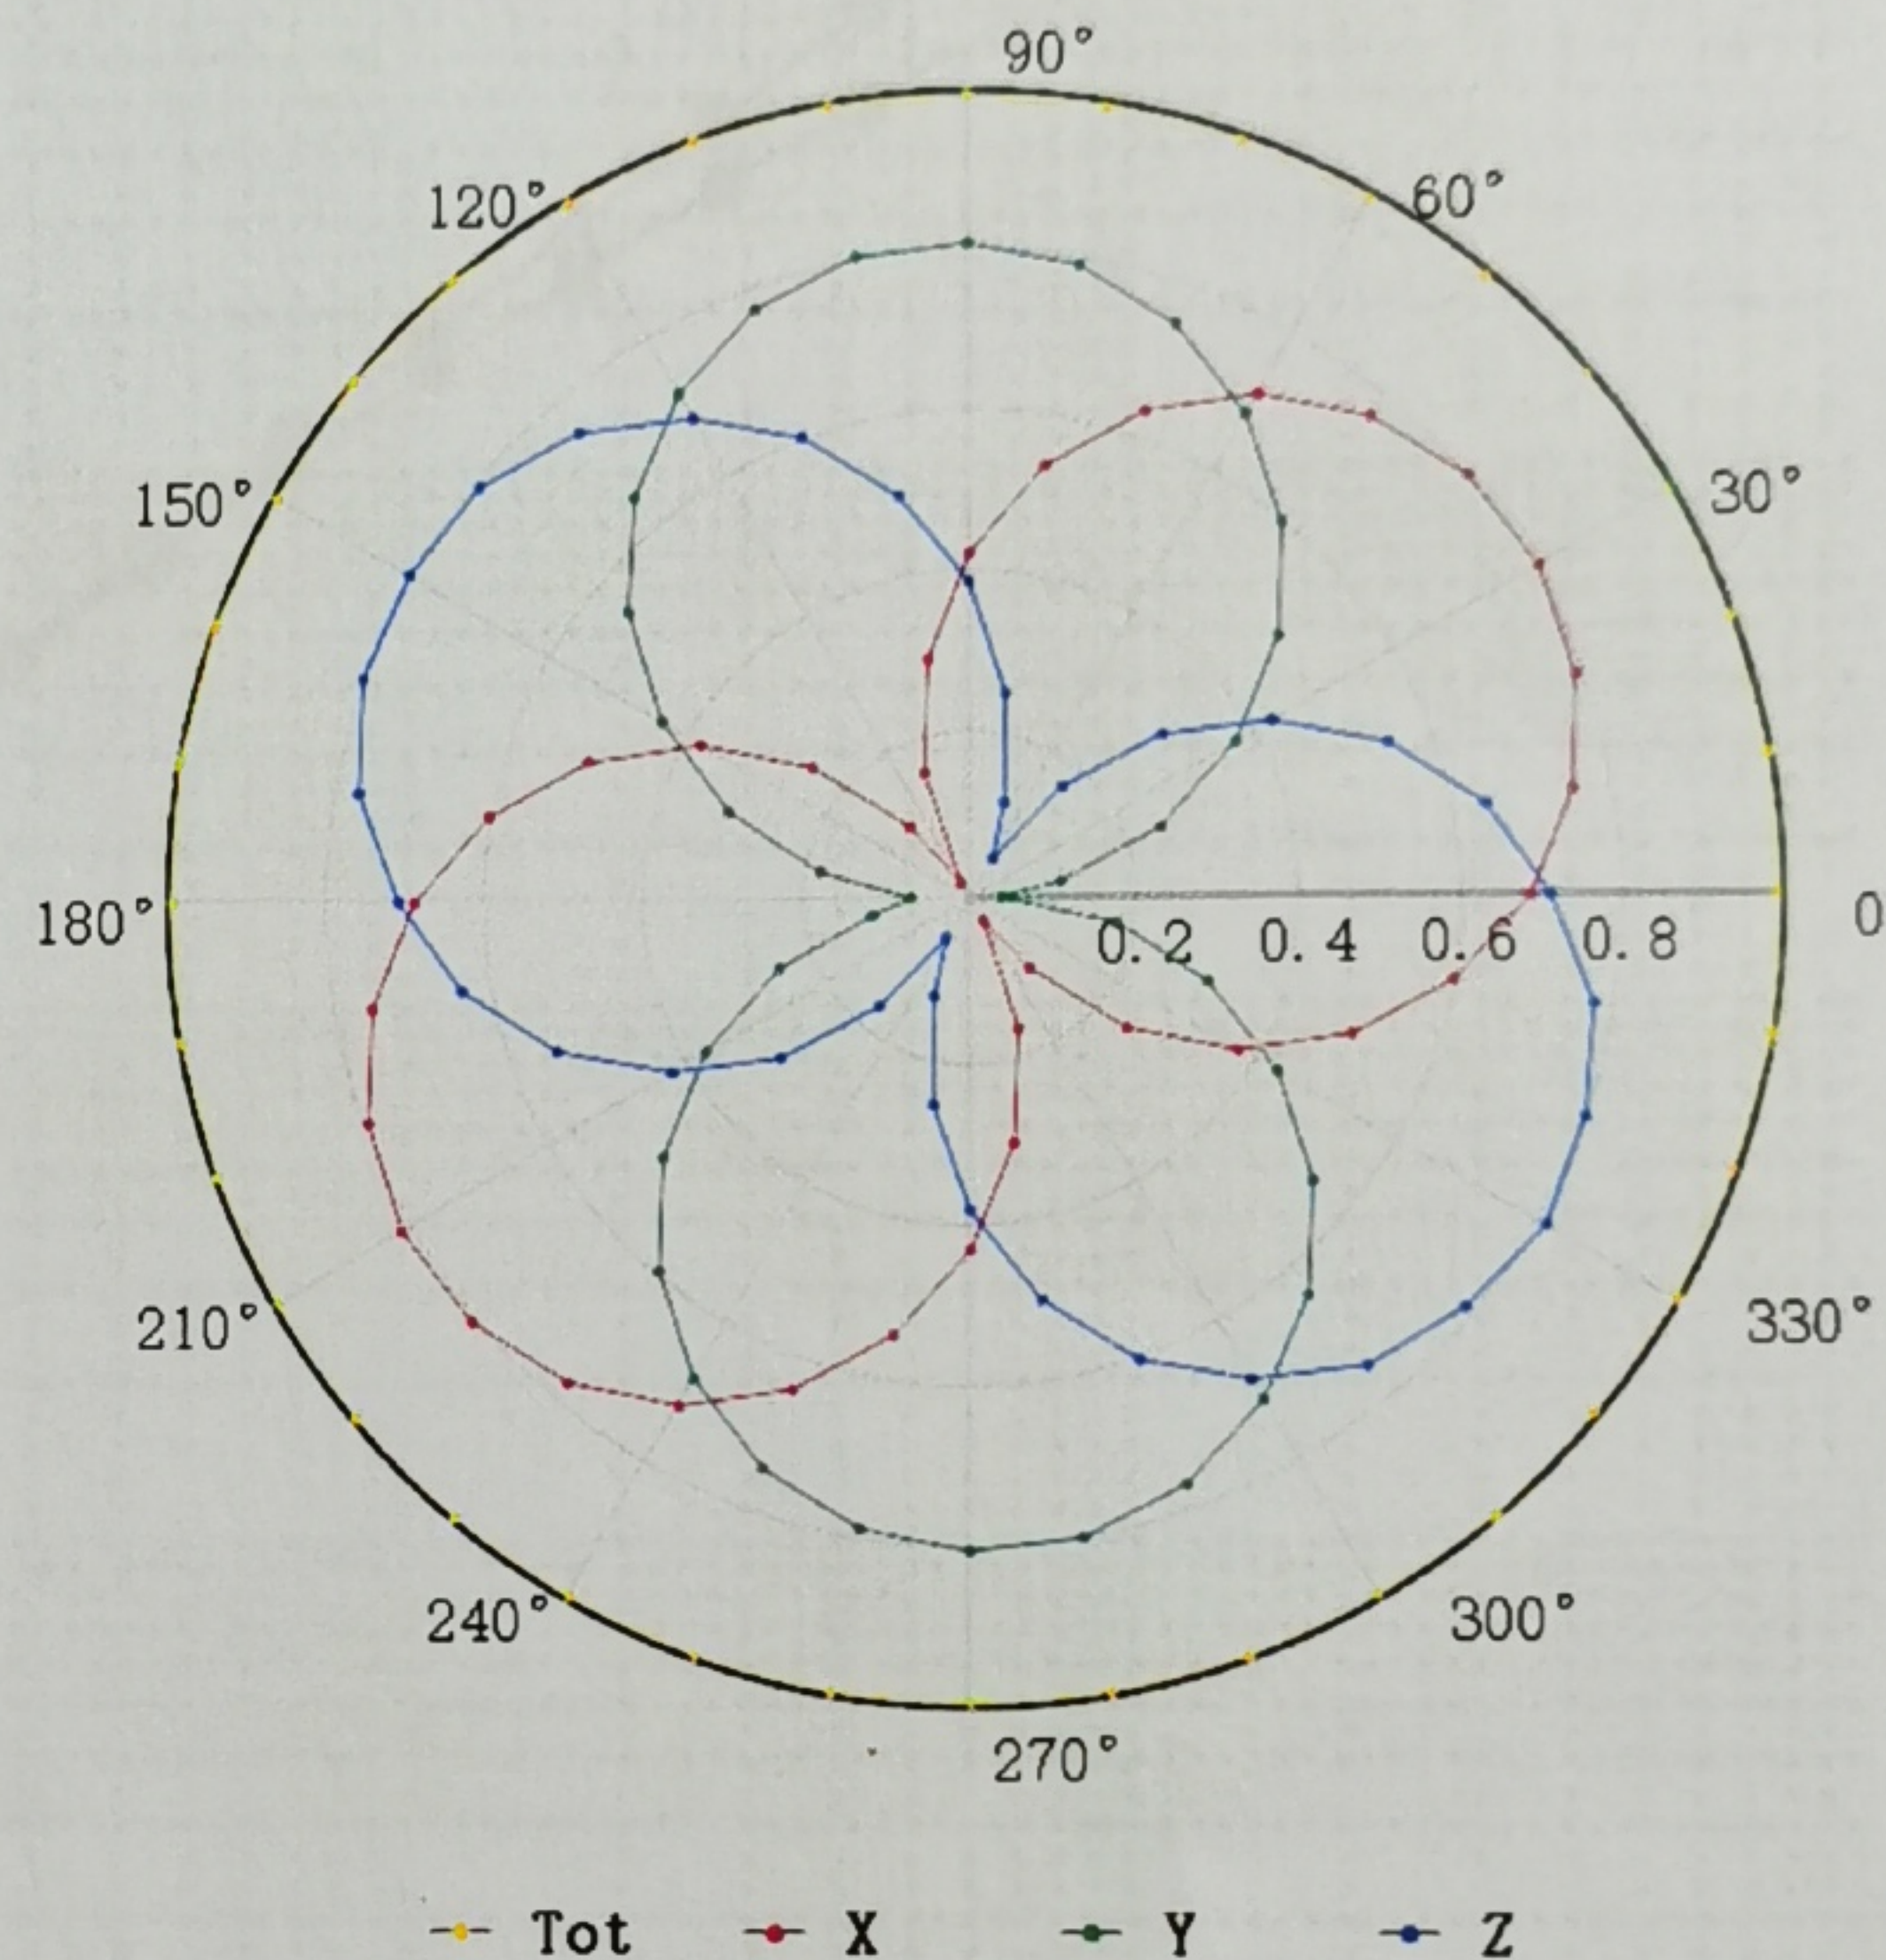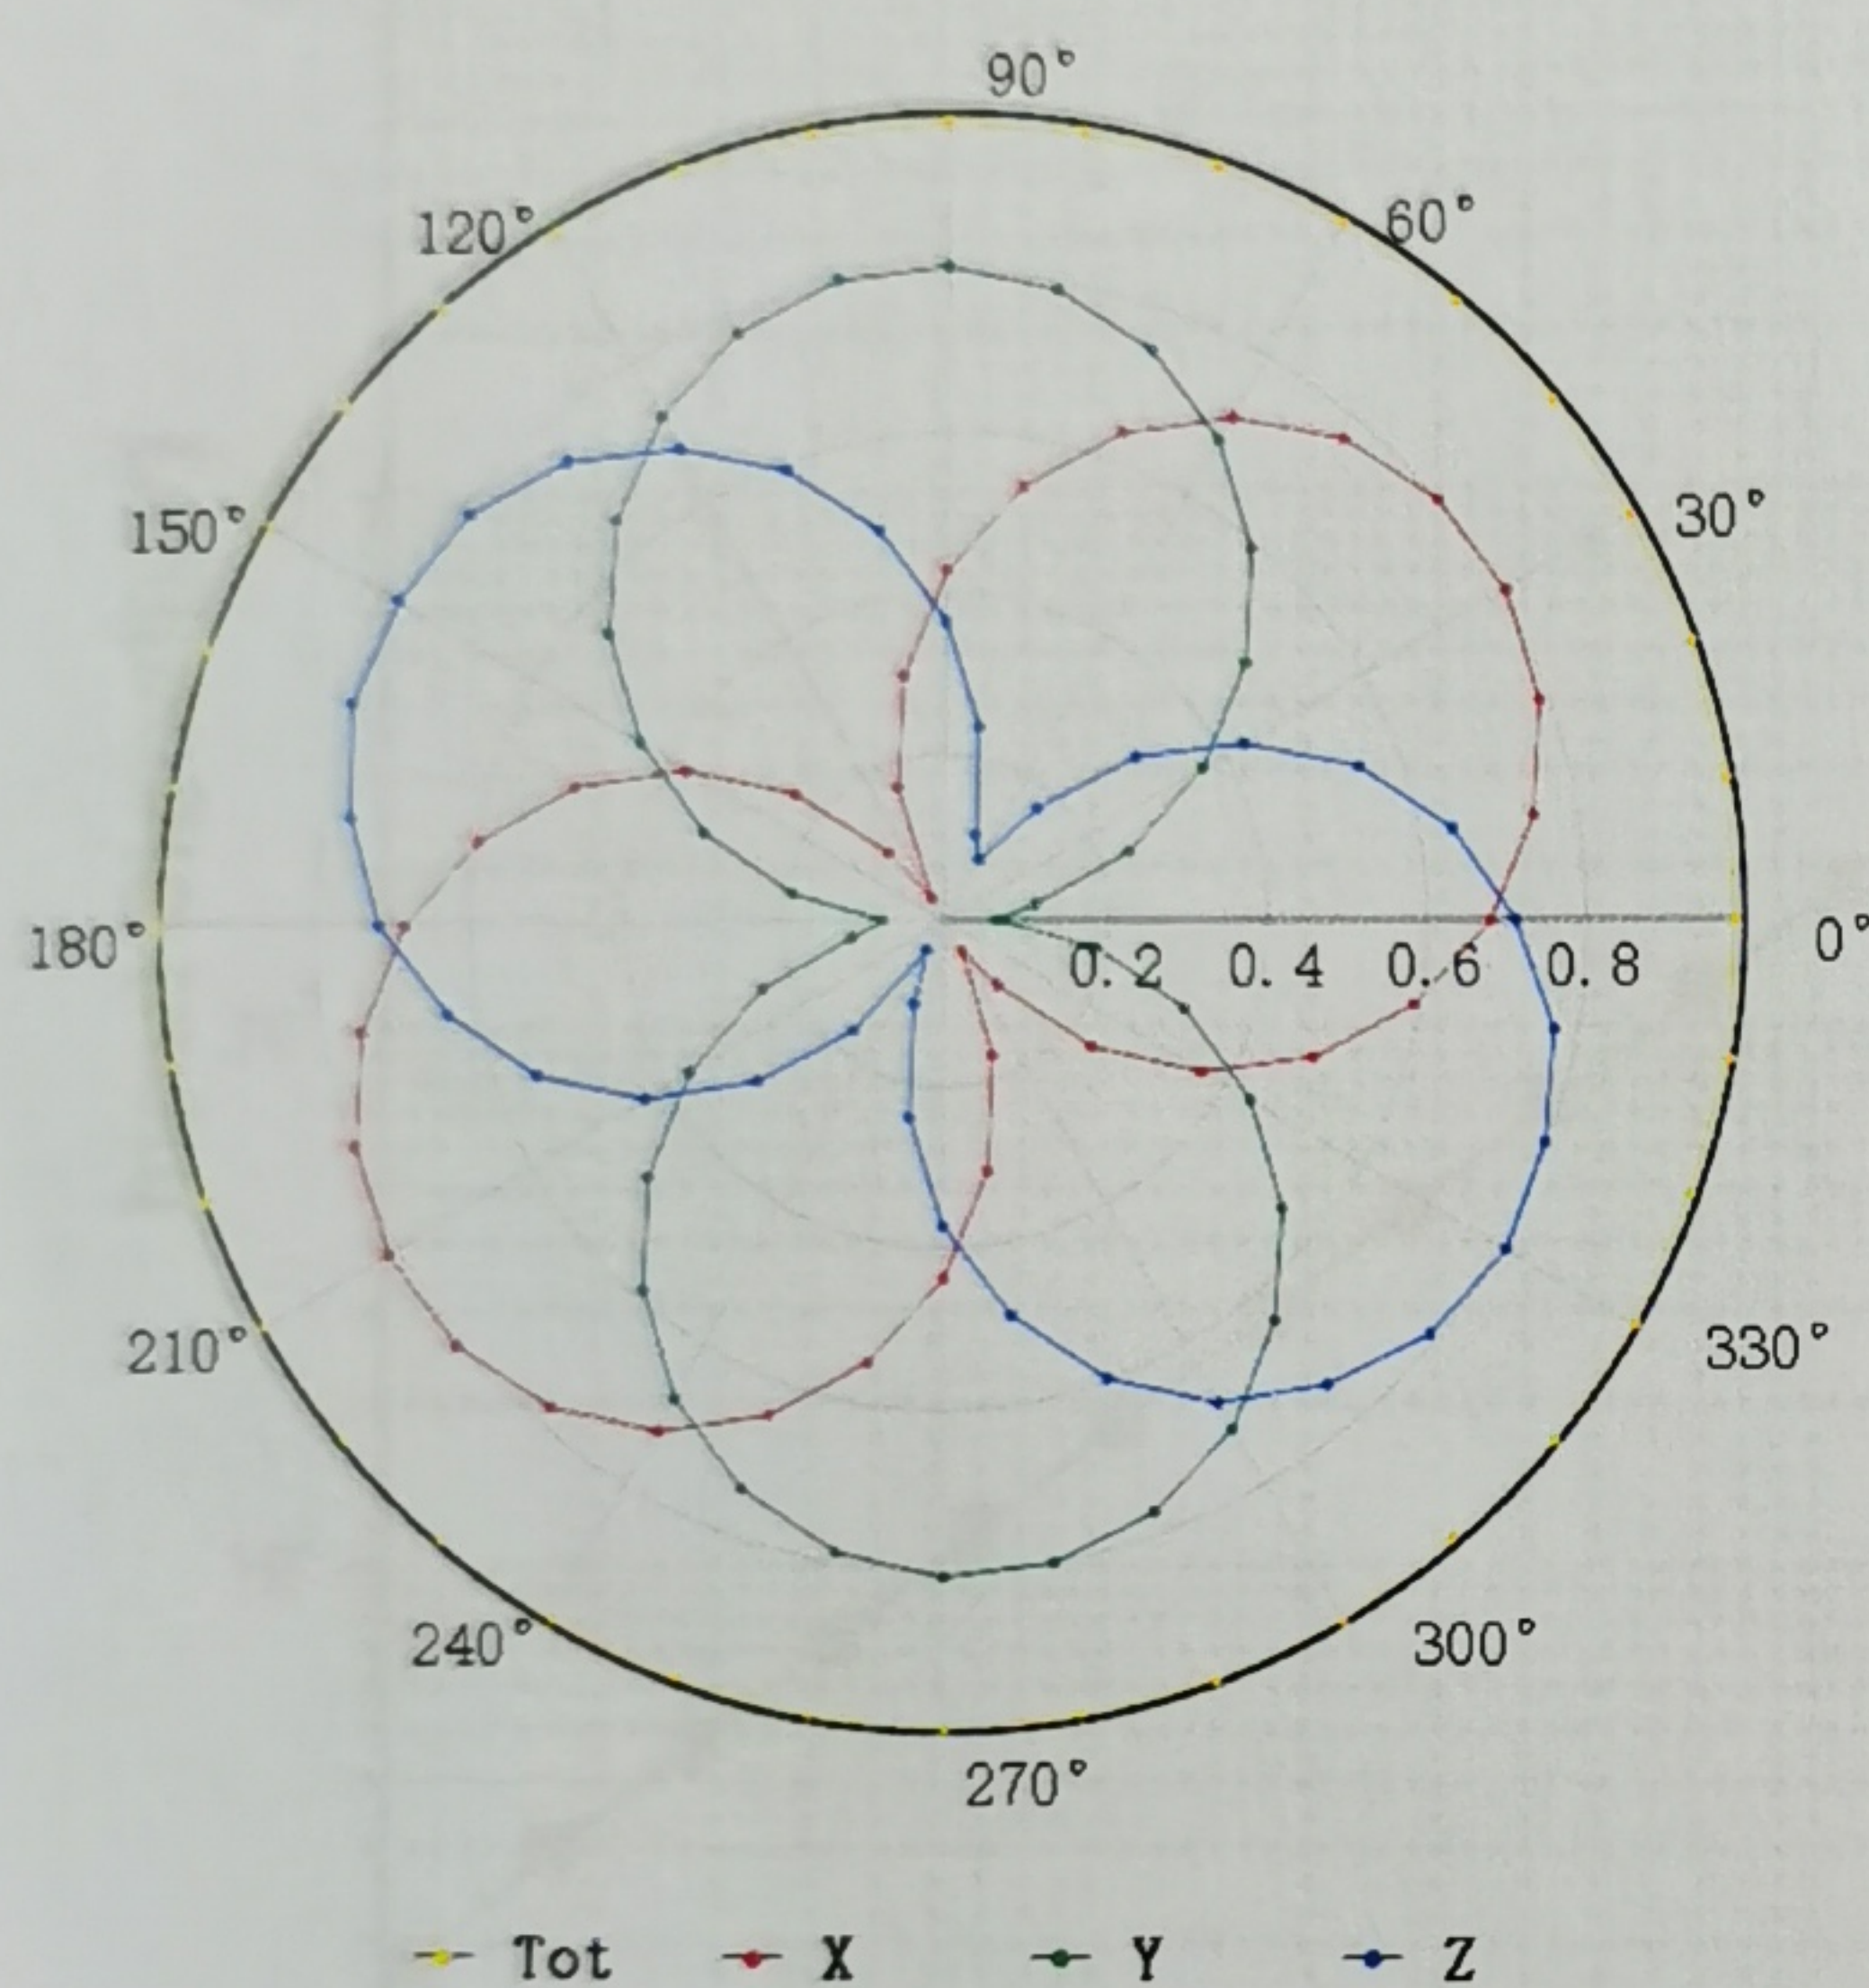

Uncertainty of Axial Isotropy Assessment: $\pm 1.2\%$ ($k=2$)