

## ANNEX B – RELEVANT PAGES FROM CALIBRATION REPORTS

DAE4 Sn:546

 <p>In Collaboration with <b>s p e a g</b> CALIBRATION LABORATORY</p> <p>Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-6236633-2312 Fax: +86-10-62364633-2304 E-mail: sctt@ttcal.com.cn <a href="http://www.ttcal.com">http://www.ttcal.com</a></p> <p>Client : <b>SRTC</b> Certificate No: Z18-60400</p> <p><b>CALIBRATION CERTIFICATE</b></p> <p>Object DAE4 - SN: 546</p> <p>Calibration Procedure(s) FF-Z11-002-01 Calibration Procedure for the Data Acquisition Electronics (DAE)</p> <p>Calibration date: October 16, 2018</p> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility; environment temperature(22±0.5)°C and humidity&lt;70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date/Calibrated by, Certificate No.</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Process Calibrator 753</td> <td>1971018</td> <td>20-Jun-18 (CTTL, No.J1BX05034)</td> <td>June-19</td> </tr> </tbody> </table> <p>Calibrated by: Name: Yu Zongying Function: SAR Test Engineer Signature: </p> <p>Reviewed by: Name: Lin Hao Function: SAR Test Engineer Signature: </p> <p>Approved by: Name: Qi Dianyuan Function: SAR Project Leader Signature: </p> <p>Issued: October 17, 2018</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p>Certificate No: Z18-60400 Page 1 of 3</p>	Primary Standards	ID #	Cal Date/Calibrated by, Certificate No.	Scheduled Calibration	Process Calibrator 753	1971018	20-Jun-18 (CTTL, No.J1BX05034)	June-19	 <p>In Collaboration with <b>s p e a g</b> CALIBRATION LABORATORY</p> <p>Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-6236633-2312 Fax: +86-10-62364633-2304 E-mail: sctt@ttcal.com.cn <a href="http://www.ttcal.com">http://www.ttcal.com</a></p> <p><b>Glossary:</b> DAE data acquisition electronics Connector angle information used in DASY system to align probe sensor X to the robot coordinate system.</p> <p><b>Methods Applied and Interpretation of Parameters:</b></p> <ul style="list-style-type: none"> <li>• <b>DC Voltage Measurement:</b> Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.</li> <li>• <b>Connector angle:</b> The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.</li> <li>• The report provides only calibration results for DAE, it does not contain other performance test results.</li> </ul> <p>Certificate No: Z18-60400 Page 2 of 3</p>
Primary Standards	ID #	Cal Date/Calibrated by, Certificate No.	Scheduled Calibration						
Process Calibrator 753	1971018	20-Jun-18 (CTTL, No.J1BX05034)	June-19						

 <p>In Collaboration with <b>s p e a g</b> CALIBRATION LABORATORY</p> <p>Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-6236633-2312 Fax: +86-10-62364633-2304 E-mail: sctt@ttcal.com.cn <a href="http://www.ttcal.com">http://www.ttcal.com</a></p> <p><b>DC Voltage Measurement</b> A/D - Counter Resolution nominal High Range: 8.192V, Full range = -100...+300 mV Low Range: 0.192V, Full range = -1...+3mV DASY measurement parameters: Auto Zero time: 3 sec; Measuring time: 3 sec</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Calibration Factors</th> <th>X</th> <th>Y</th> <th>Z</th> </tr> </thead> <tbody> <tr> <td>High Range</td> <td>405.306 ± 0.15% (n=2)</td> <td>404.259 ± 0.15% (n=2)</td> <td>404.180 ± 0.15% (n=2)</td> </tr> <tr> <td>Low Range</td> <td>3.98093 ± 0.7% (n=2)</td> <td>3.95978 ± 0.7% (n=2)</td> <td>3.98021 ± 0.7% (n=2)</td> </tr> </tbody> </table> <p><b>Connector Angle</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>Connector Angle to be used in DASY system</td> <td>238° ± 1°</td> </tr> </table> <p>Certificate No: Z-8-60403 Page 3 of 3</p>	Calibration Factors	X	Y	Z	High Range	405.306 ± 0.15% (n=2)	404.259 ± 0.15% (n=2)	404.180 ± 0.15% (n=2)	Low Range	3.98093 ± 0.7% (n=2)	3.95978 ± 0.7% (n=2)	3.98021 ± 0.7% (n=2)	Connector Angle to be used in DASY system	238° ± 1°
Calibration Factors	X	Y	Z											
High Range	405.306 ± 0.15% (n=2)	404.259 ± 0.15% (n=2)	404.180 ± 0.15% (n=2)											
Low Range	3.98093 ± 0.7% (n=2)	3.95978 ± 0.7% (n=2)	3.98021 ± 0.7% (n=2)											
Connector Angle to be used in DASY system	238° ± 1°													

## ES3DV3 Sn:3127

CLIENT CERTIFICATE		Certificate No.: Z18-60398		
Object	ES3DV3 - SN:3127			
Calibration Procedure(s)	FF-Z11-004-01 Calibration Procedures for Dosimetric E-field Probes			
Calibration date:	November 02, 2018			
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.				
All calibrations have been conducted in the closed laboratory facility; environment temperature(22±2)°C and humidity<70%.				
Calibration Equipment used (M&TE critical for calibration)				
Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration	
Power Meter	NRP2	101919	20-Jun-18 (CITL, No.J18X05032)	Jun-19
Power sensor	NRP-Z91	101547	20-Jun-18 (CITL, No.J18X05032)	Jun-19
Power sensor	NRP-Z91	101548	20-Jun-18 (CITL, No.J18X05032)	Jun-19
Reference 10dB Attenuator	18N50W-10dB	09-Feb-18(CITL, No.J18X01133)	Feb-20	
Reference 20dB Attenuator	18N50W-20dB	09-Feb-18(CITL, No.J18X01132)	Feb-20	
Reference Probe EX3DV3	SN 3846	25-Jan-18(SPEAG No.EX3-3846, Jan18)	Jan-19	
DAE4	SN 777	15-Dec-17(SPEAG, No.DAE-777_Dect17)	Dec-18	
Secondary Standards				
Signal Generator MG3700A	6201052605	21-Jun-18 (CITL, No.J18X05033)	Jun-19	
Network Analyzer E5071C	MY46110673	14-Jan-18 (CITL, No.J18X00561)	Jan-19	
Calibrated by:	Yu Zongying	SAR Test Engineer		
Reviewed by:	Lin Hao	SAR Test Engineer		
Approved by:	Qi Dianyuan	SAR Project Leader		
Issued: November 04, 2018				
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.				

Certificate No: Z18-60398

Page 1 of 11



In Collaboration with  
**TTL** SPEAG  
CALIBRATION LABORATORY  
Add: No. 51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62106313-2112 Fax: +86-10-6210633-2504  
E-mail: [cttl@cttl.com](mailto:cttl@cttl.com) <http://www.cttl.com>

中国认可  
国际互认  
校准  
CALIBRATION  
CNAS L017/0

In Collaboration with  
**speag**  
CALIBRATION LABORATORY  
Add: No. 51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62106313-2112 Fax: +86-10-62106463-2504  
E-mail: [cttl@cttl.com](mailto:cttl@cttl.com) <http://www.cttl.com>

**Glossary:**

- TSL:** tissue simulating liquid
- NCRM<sub>x,y,z</sub>:** sensitivity in free space
- Conf:** confidence interval around NCRM<sub>x,y,z</sub>
- DOP:** diode compression point
- OF:** over factor (1/N<sub>ULY</sub>)<sup>1/2</sup> of the RF signal
- A,B,C,D:** modulation dependent linearization parameters
- Polarization φ:** @ rotation around probe axis
- Polarization θ:** @ rotation around axis that is in the plane normal to probe axis (at measurement center), i.e. B=0 is normal to probe axis
- Connector Angle:** information used in DASY system to align probe sensor X to the root coordinate system
- Calibration is Performed According to the Following Standards:**
  - a) IEEE Std 1801-2012, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
  - b) IEC 62203-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2012
  - c) IEC 62208-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2012
  - d) IEC 626664, "SAR Measurement Requirements for 100 MHz to 6 GHz"
- Methods Applied and Interpretation of Parameters:**
  - NCRM<sub>x,y,z</sub>: Assessed for E-field polarization (0° to 900MHz in TEM-cell: >1800MHz: waveguide). The NCRM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NCRM<sub>x,y,z</sub> does not effect the E'-field uncertainty inside TSL (see below ConvF).
  - NORMT<sub>x,y,z</sub> = NCRM<sub>x,y,z</sub>\*frequency response (see Frequency Response Chart). This linear scaling is included in DASY4 software versions older than 4.2. The uncertainty of the frequency response is included in the assessed uncertainty of ConvF.
  - DCP<sub>x,y,z</sub>: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
  - PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal amplitude.
  - Ax,y,z; Bx,y,z; Cx,y,z: Ax,y,z are numerical linearization parameters assessed based on the data of cover sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
  - ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature) transducers. These parameters are used to correct the measured values for deviations on power measurements for f>800MHz. The new adaptions are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The same adaptions correspond to NCRM<sub>x,y,z</sub> ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency adaption was used in DASY version 4.4 and higher which allows extending the validity from 500MHz to 100MHz.
  - Spherical isotropy (ID deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
  - ConvF: The value of ConvF corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
  - Connector Angle: The angle is assessed using the information gained by determining the NCRM<sub>x,y,z</sub> (no uncertainty required).

Certificate No: Z18-60398

Page 2 of 11

## Probe ES3DV3

SN: 3127

Calibrated: November 02, 2018

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system)

Certificate No: Z18-60398

Page 3 of 11



**DASY/EASY – Parameters of Probe: ES3DV3 - SN: 3127**

**Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm( $\mu$ V/Vm) <sup>a</sup>	1.27	1.26	1.21	±10.0%
DCP(mV) <sup>b</sup>	103.3	104.4	105.0	

**Modulation Calibration Parameters**

UID	Communication System Name	A dB	B dB/ $\mu$ V	C	D dB	VR mV	Unc <sup>c</sup> (k=2)
0	CW	X 0.0	0.0	1.0	0.00	285.6	±2.2%
		Y 0.0	0.0	1.0		287.9	
		Z 0.0	0.0	1.0		282.9	

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

<sup>a</sup>The uncertainty of Norm. V/V is not reflect the E<sup>2</sup> field uncertainty inside TBL (see Page 5 and Page 6).  
<sup>b</sup>Numerical linearization parameter uncertainty not required.  
<sup>c</sup>Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.



**DASY/EASY – Parameters of Probe: ES3DV3 - SN: 3127**

**Calibration Parameter Determined in Head Tissue Simulating Media**

f [MHz] <sup>d</sup>	Relative Permittivity <sup>e</sup>	Conductivity [S/m] <sup>f</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>g</sup>	Depth <sup>h</sup> (mm)	Unc. (k=2)
750	41.9	0.89	6.34	6.34	6.34	0.40	1.35	±12.1%
835	41.5	0.90	6.18	6.18	6.18	0.35	1.58	±12.1%
1810	4.00	1.40	5.07	5.07	5.07	0.66	1.24	±12.1%
2000	4.00	1.40	4.96	4.96	4.96	0.70	1.20	±12.1%
2300	3.95	1.67	4.79	4.79	4.79	0.90	1.08	±12.1%
2450	3.92	1.80	4.66	4.66	4.66	0.90	1.08	±12.1%
2600	3.90	1.96	4.40	4.40	4.40	0.80	1.21	±12.1%

<sup>d</sup> Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>e</sup> At frequency below 3 GHz, the validity of tissue parameters (c and d) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (c and d) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>f</sup>Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: Z18-60398

Page 5 of 11

Certificate No: Z18-60398

Page 4 of 11



**DASY/EASY – Parameters of Probe: ES3DV3 - SN: 3127**

**Calibration Parameter Determined in Body Tissue Simulating Media**

f [MHz] <sup>d</sup>	Relative Permittivity <sup>e</sup>	Conductivity [S/m] <sup>f</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>g</sup>	Depth <sup>h</sup> (mm)	Unc. (k=2)
750	55.5	0.98	6.33	6.33	6.33	0.40	1.40	±12.1%
835	55.2	0.97	6.13	6.13	6.13	0.37	1.62	±12.1%
1810	53.3	1.52	4.78	4.78	4.78	0.65	1.27	±12.1%
2000	53.3	1.52	4.80	4.80	4.80	0.67	1.27	±12.1%
2300	52.9	1.81	4.46	4.46	4.46	0.90	1.15	±12.1%
2450	52.7	1.06	4.31	4.31	4.31	0.70	1.28	±12.1%
2600	52.5	2.10	4.14	4.14	4.14	0.90	1.10	±12.1%


<sup>d</sup> Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>e</sup> At frequency below 3 GHz, the validity of tissue parameters (c and d) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (c and d) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>f</sup>Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.



**Frequency Response of E-Field (TEM-Cell: Ifi110 EXX, Waveguide: R22)**

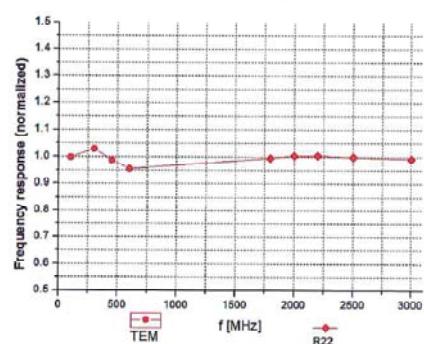

Uncertainty of Frequency Response of E-field: ±7.4% (k=2)

Certificate No: Z18-60398


Page 6 of 11

Certificate No: Z18-60398

Page 7 of 11

In Collaboration with  
**TTL speag**  
CALIBRATION LABORATORY

Add: No.31 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62305433-2512 Fax: +86-10-62304633-2504  
E-mail: ctfl@chinatl.com <http://www.chinatl.com>

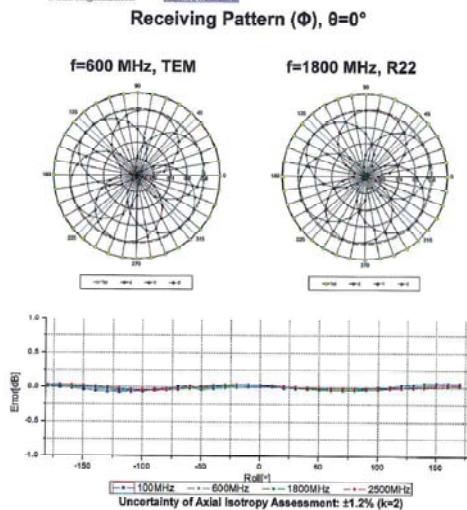


Certificate No: Z18-60398

Page 8 of 11

In Collaboration with  
**TTL speag**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: ctfl@chinatl.com <http://www.chinatl.com>

**Dynamic Range f(SAR<sub>head</sub>)**  
(TEM cell, f = 900 MHz)

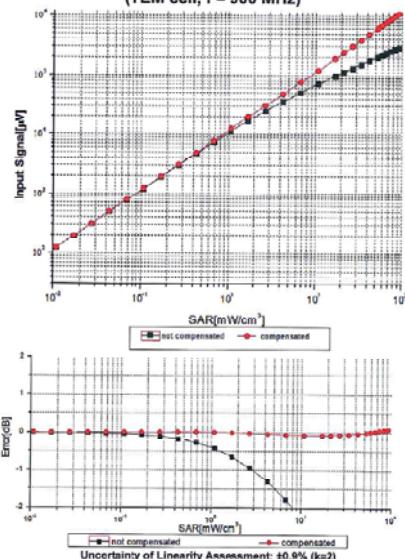


Certificate No: Z18-60398

Page 9 of 11


In Collaboration with  
**TTL speag**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: ctfl@chinatl.com <http://www.chinatl.com>

**Conversion Factor Assessment**

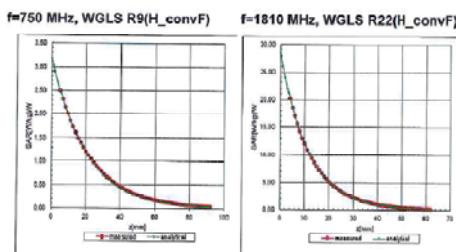

**Deviation from Isotropy in Liquid**

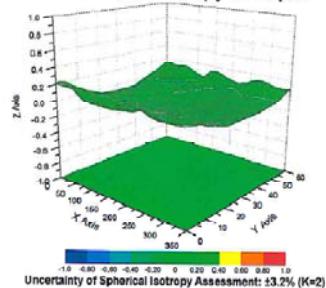

Certificate No: Z18-60398

Page 10 of 11

In Collaboration with  
**TTL speag**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2518 Fax: +86-10-62304633-2209  
E-mail: ctfl@chinatl.com <http://www.chinatl.com>

**Appendix: Modulation Calibration Parameters**

UID	Communication System Name	PAR	A dB	B dB- $\mu$ V	C	VR mV	Unc <sup>E</sup> (%)
0	CW	0.00	X 0.0	0.0	1.0	282.3	$\pm 2.5\%$
			Y 0.0	0.0	1.0	280.9	
			Z 0.0	0.0	1.0	275.1	
10012	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps)	1.87	X 2.77	68.02	18.46	143.0	$\pm 1.8\%$
			Y 2.75	68.05	18.52	145.0	
			Z 2.71	67.79	18.25	142.3	
10100	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	5.67	X 6.13	66.4	18.97	141.9	$\pm 1.9\%$
			Y 6.15	66.49	19.06	144.2	
			Z 6.09	66.32	18.90	140.9	
10108	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	5.80	X 6.09	66.24	19.07	139.5	$\pm 1.9\%$
			Y 6.10	66.33	19.15	141.5	
			Z 6.05	66.19	19.05	138.0	
10154	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	5.75	X 5.81	65.85	18.93	136.1	$\pm 1.9\%$
			Y 5.82	65.92	19.01	137.8	
			Z 5.79	65.89	18.97	134.7	
10169	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	5.73	X 4.84	65.92	19.20	130.8	$\pm 1.9\%$
			Y 4.82	65.98	19.27	131.3	
			Z 4.80	66.00	19.29	129.1	
10175	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	5.72	X 4.88	66.14	19.40	131.6	$\pm 1.9\%$
			Y 4.83	66.08	19.33	130.9	
			Z 4.79	66.02	19.29	129.3	
10297	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	5.81	X 6.19	66.61	19.42	141.9	$\pm 1.9\%$
			Y 6.13	66.43	19.26	140.7	
			Z 6.14	66.52	19.33	139.6	

Certificate No: Z17-97142

Page 12 of 12

## DAE4 Sn:720



Client : SRTC Certificate No: Z18-60399

### CALIBRATION CERTIFICATE

Object DAE4 - SN: 720

Calibration Procedure(s) FF-Z11-002-01  
Calibration Procedure for the Data Acquisition Electronics (DAE)

Calibration date: October 15, 2018

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(20±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Process Calibrator 753	1971018	20-Jun-18 (CTTL, No.J18X05034)	June-19

Calibrated by:	Name	Function	Signature
Reviewed by:	Yu Zongying	SAR Test Engineer	
Approved by:	Lin Hao	SAR Test Engineer	

Approved by: Qi Dianyuan SAR Project Leader

Issued: October 17, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z18-60399

Page 1 of 3



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-6239633-2512 Fax: +86-10-6239633-2504  
E-mail: ctll@chinatlc.com Http://www.chinatlc.com

### Glossary:

DAE data acquisition electronics  
Connector angle information used in DASY system to align probe sensor X to the robot coordinate system.

### Methods Applied and Interpretation of Parameters:

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The report provide only calibration results for DAE, it does not contain other performance test results.

Certificate No: Z18-60399

Page 2 of 3



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-6239633-2512 Fax: +86-10-6239633-2504  
E-mail: ctll@chinatlc.com Http://www.chinatlc.com

### DC Voltage Measurement

A/D - Converter Resolution nominal  
High Range: 1LSB = 8.1µV, full range = -100...+300 mV  
Low Range: 1LSB = 81mV, full range = -1.....+30V  
DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	403.343 ± 0.15% (k=2)	404.773 ± 0.15% (k=2)	403.205 ± 0.15% (k=2)
Low Range	3.96574 ± 0.7% (k=2)	3.98569 ± 0.7% (k=2)	3.96685 ± 0.7% (k=2)

### Connector Angle

Connector Angle to be used in DASY system	25° ± 1°
---	----------

Certificate No: Z18-60399

Page 3 of 3

<p style="text-align: center;"><b>EX3DV4 Sn:3708 (1/7)</b></p> <div style="border: 1px solid black; padding: 10px; margin-bottom: 10px;"> <p><b>Calibration Laboratory of</b> Schmid &amp; Partner Engineering AG Zugstrasse 43, 8034 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA: Multilateral Agreement for the recognition of calibration certificates</p> <p>Client: <b>SRTC (Aiden)</b>      Certificate No: EX3-3708_Oct18</p> <p><b>CALIBRATION CERTIFICATE</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 20%;">Object:</td> <td>EX3DV4 - SN:3708</td> </tr> <tr> <td>Calibration procedure(s):</td> <td>QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v4, QA CAL-23.v5, QA CAL-25.v6 Calibration procedure for dosimetric E-field probes</td> </tr> <tr> <td>Calibration date:</td> <td>October 22, 2018</td> </tr> <tr> <td colspan="2">This calibration certificate documents the traceability to national standards, which realize the physical units of measurement (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</td> </tr> <tr> <td colspan="2">All calibrations have been conducted in the closed laboratory facility, environment temperature (<math>22 \pm 1^\circ\text{C}</math>) and humidity &lt; 70%.</td> </tr> <tr> <td colspan="2">Calibration Equipment used (MATE: critical for calibration)</td> </tr> <tr> <td colspan="2"> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Primary Standards</th> <th>ID</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter NRP</td> <td>SN_104776</td> <td>08-Apr-18 (No. 217-20073705873)</td> <td>Apr-19</td> </tr> <tr> <td>Power meter HP-291</td> <td>SN_104777</td> <td>08-Apr-18 (No. 217-20073705874)</td> <td>Apr-19</td> </tr> <tr> <td>Power meter HP-291</td> <td>SN_103345</td> <td>08-Apr-18 (No. 217-209173)</td> <td>Apr-19</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN_98277 (20dB)</td> <td>08-Apr-18 (No. 217-20883)</td> <td>Apr-19</td> </tr> <tr> <td>Reference Probe ES/NV</td> <td>SN_3013</td> <td>30-Dec-17 (No. ES3-9013_Cert17)</td> <td>Dec-18</td> </tr> <tr> <td>DAS4</td> <td>SN_660</td> <td>21-Dec-17 (No. DA64-986_Cert17)</td> <td>Dec-18</td> </tr> <tr> <td>Secondary Standards</td> <td>ID</td> <td>Check Date (In-house)</td> <td>Scheduled Check</td> </tr> <tr> <td>Power meter E4419B</td> <td>SN_GB12500074</td> <td>08-Apr-18 (In-house check Jun-18)</td> <td>In-house check Jun-19</td> </tr> <tr> <td>Power meter E4415A</td> <td>SN_MV14000077</td> <td>08-Apr-18 (In-house check Jun-18)</td> <td>In-house check Jun-19</td> </tr> <tr> <td>Power meter E4415A</td> <td>SN_MV14000078</td> <td>08-Apr-18 (In-house check Jun-18)</td> <td>In-house check Jun-19</td> </tr> <tr> <td>RF generator HP 8648C</td> <td>SN_U5940000722</td> <td>08-Aug-18 (In-house check Jun-18)</td> <td>In-house check Jun-19</td> </tr> <tr> <td>Network Analyzer 93029A</td> <td>SN_US101000477</td> <td>31-Mar-14 (In-house check Oct-16)</td> <td>In-house check Oct-19</td> </tr> </tbody> </table> </td> </tr> <tr> <td colspan="2">Calibrated by: <b>Giulio Lanza</b>      Function: Laboratory Technician      </td> </tr> <tr> <td colspan="2">Approved by: <b>Karin Pröbstli</b>      Function: Technical Manager      </td> </tr> <tr> <td colspan="2">Issued: October 23, 2018</td> </tr> </table> </div> <p>Certificate No: EX3-3708_Oct18      Page 1 of 39</p>	Object:	EX3DV4 - SN:3708	Calibration procedure(s):	QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v4, QA CAL-23.v5, QA CAL-25.v6 Calibration procedure for dosimetric E-field probes	Calibration date:	October 22, 2018	This calibration certificate documents the traceability to national standards, which realize the physical units of measurement (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.		All calibrations have been conducted in the closed laboratory facility, environment temperature ( $22 \pm 1^\circ\text{C}$ ) and humidity < 70%.		Calibration Equipment used (MATE: critical for calibration)		<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Primary Standards</th> <th>ID</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter NRP</td> <td>SN_104776</td> <td>08-Apr-18 (No. 217-20073705873)</td> <td>Apr-19</td> </tr> <tr> <td>Power meter HP-291</td> <td>SN_104777</td> <td>08-Apr-18 (No. 217-20073705874)</td> <td>Apr-19</td> </tr> <tr> <td>Power meter HP-291</td> <td>SN_103345</td> <td>08-Apr-18 (No. 217-209173)</td> <td>Apr-19</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN_98277 (20dB)</td> <td>08-Apr-18 (No. 217-20883)</td> <td>Apr-19</td> </tr> <tr> <td>Reference Probe ES/NV</td> <td>SN_3013</td> <td>30-Dec-17 (No. ES3-9013_Cert17)</td> <td>Dec-18</td> </tr> <tr> <td>DAS4</td> <td>SN_660</td> <td>21-Dec-17 (No. DA64-986_Cert17)</td> <td>Dec-18</td> </tr> <tr> <td>Secondary Standards</td> <td>ID</td> <td>Check Date (In-house)</td> <td>Scheduled Check</td> </tr> <tr> <td>Power meter E4419B</td> <td>SN_GB12500074</td> <td>08-Apr-18 (In-house check Jun-18)</td> <td>In-house check Jun-19</td> </tr> <tr> <td>Power meter E4415A</td> <td>SN_MV14000077</td> <td>08-Apr-18 (In-house check Jun-18)</td> <td>In-house check Jun-19</td> </tr> <tr> <td>Power meter E4415A</td> <td>SN_MV14000078</td> <td>08-Apr-18 (In-house check Jun-18)</td> <td>In-house check Jun-19</td> </tr> <tr> <td>RF generator HP 8648C</td> <td>SN_U5940000722</td> <td>08-Aug-18 (In-house check Jun-18)</td> <td>In-house check Jun-19</td> </tr> <tr> <td>Network Analyzer 93029A</td> <td>SN_US101000477</td> <td>31-Mar-14 (In-house check Oct-16)</td> <td>In-house check Oct-19</td> </tr> </tbody> </table>		Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration	Power meter NRP	SN_104776	08-Apr-18 (No. 217-20073705873)	Apr-19	Power meter HP-291	SN_104777	08-Apr-18 (No. 217-20073705874)	Apr-19	Power meter HP-291	SN_103345	08-Apr-18 (No. 217-209173)	Apr-19	Reference 20 dB Attenuator	SN_98277 (20dB)	08-Apr-18 (No. 217-20883)	Apr-19	Reference Probe ES/NV	SN_3013	30-Dec-17 (No. ES3-9013_Cert17)	Dec-18	DAS4	SN_660	21-Dec-17 (No. DA64-986_Cert17)	Dec-18	Secondary Standards	ID	Check Date (In-house)	Scheduled Check	Power meter E4419B	SN_GB12500074	08-Apr-18 (In-house check Jun-18)	In-house check Jun-19	Power meter E4415A	SN_MV14000077	08-Apr-18 (In-house check Jun-18)	In-house check Jun-19	Power meter E4415A	SN_MV14000078	08-Apr-18 (In-house check Jun-18)	In-house check Jun-19	RF generator HP 8648C	SN_U5940000722	08-Aug-18 (In-house check Jun-18)	In-house check Jun-19	Network Analyzer 93029A	SN_US101000477	31-Mar-14 (In-house check Oct-16)	In-house check Oct-19	Calibrated by: <b>Giulio Lanza</b> Function: Laboratory Technician 		Approved by: <b>Karin Pröbstli</b> Function: Technical Manager 		Issued: October 23, 2018		<p><b>Calibration Laboratory of</b> Schmid &amp; Partner Engineering AG Zugstrasse 43, 8034 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA: Multilateral Agreement for the recognition of calibration certificates</p> <p><b>Glossary:</b></p> <ul style="list-style-type: none"> <li>TSL: tissue simulating liquid</li> <li>NORMx,y,z: sensitivity in TSL</li> <li>ConvF: sensitivity in TSL (NORMx,y,z)</li> <li>DCP: dielectric calibration point</li> <li>CF: crest factor (1/industry cycle) of the RF signal</li> <li>A, B, C, D: numerical linearization parameters</li> <li>Polarization <math>\theta</math>: rotation around probe axis</li> <li>Polarization <math>\phi</math>: rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., <math>\phi = 0</math> is normal to probe axis</li> <li>Connector Angle: information used in DASY system to align probe sensor X to the robot coordinate system</li> </ul> <p><b>Calibration is Performed According to the Following Standards:</b></p> <ol style="list-style-type: none"> <li>IEEE Std 1566-2014, "Standard Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2014</li> <li>IEC 62209-1, "Measurement procedures for the assessment of Specific Absorption Rate (SAR) from head-mounted devices", March 2016</li> <li>IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010</li> <li>KOB 85590, "Standard practice for determining the peak spatial averaged specific absorption rate (SAR) in the head from wireless communications devices", March 2010</li> </ol> <p><b>Method Applied and Interpretation of Parameters:</b></p> <ul style="list-style-type: none"> <li>• <b>Power <math>P_{ave}</math>, Asperad:</b> For E-field polarization <math>\theta = 0^\circ</math> (<math>0 \leq f \leq 900 \text{ MHz}</math> in TEM-cell; <math>f = 1800 \text{ MHz}</math>; R2 waveguide). <math>NORMx,y,z</math> are only intermediate values, i.e., the uncertainty of <math>NORMx,y,z</math> does not affect the E-field uncertainty inside TSL (see below ConvF).</li> <li>• <b>NORMx,y,z:</b> Uncertainty of the frequency response (see Frequency Response Chart). This linearization is included in DASY software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.</li> <li>• <b>DCP,x,y,z:</b> DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal. DCP does not depend on frequency nor media.</li> <li>• <b>PAR:</b> PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.</li> <li>• <b>Ax,y,z, Bx,y,z, Cx,y,z, Dx,y,z, Vx,y,z:</b> A, B, C, D are numerical linearization parameters assessed based on power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.</li> <li>• <b>ConvF and Frequency Effect Parameters:</b> Assessed at flat phantom using the Power Spectral Density Transfer Function for the frequency range of interest. These parameters are used for calculation of the field distributions based on power measurements for <math>f &gt; 800 \text{ MHz}</math>. The same setups are used for assessment of the parameters applied for boundary compensation (depth, depth of which typical uncertainty values are given). These parameters are used in DASY 4 software. The term "ConvF" corresponds to the value of the uncertainty of the field distribution in TSL, corresponds to the term "ConvF" when the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from <math>\pm 50 \text{ MHz}</math> to <math>\pm 100 \text{ MHz}</math>.</li> <li>• <b>numerical isotropy (3D deviation from isotropy):</b> In a field of low gradients realized using a flat phantom exposed by a patch antenna.</li> <li>• <b>Sensor Offset:</b> The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe test). No tolerance required.</li> <li>• <b>Connector Angle:</b> The angle is assessed using the information gained by determining the <math>NORMx</math> (no uncertainty required).</li> </ul> <p>Certificate No: EX3-3708_Oct18      Page 2 of 39</p>																									
Object:	EX3DV4 - SN:3708																																																																																																	
Calibration procedure(s):	QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v4, QA CAL-23.v5, QA CAL-25.v6 Calibration procedure for dosimetric E-field probes																																																																																																	
Calibration date:	October 22, 2018																																																																																																	
This calibration certificate documents the traceability to national standards, which realize the physical units of measurement (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.																																																																																																		
All calibrations have been conducted in the closed laboratory facility, environment temperature ( $22 \pm 1^\circ\text{C}$ ) and humidity < 70%.																																																																																																		
Calibration Equipment used (MATE: critical for calibration)																																																																																																		
<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Primary Standards</th> <th>ID</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter NRP</td> <td>SN_104776</td> <td>08-Apr-18 (No. 217-20073705873)</td> <td>Apr-19</td> </tr> <tr> <td>Power meter HP-291</td> <td>SN_104777</td> <td>08-Apr-18 (No. 217-20073705874)</td> <td>Apr-19</td> </tr> <tr> <td>Power meter HP-291</td> <td>SN_103345</td> <td>08-Apr-18 (No. 217-209173)</td> <td>Apr-19</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN_98277 (20dB)</td> <td>08-Apr-18 (No. 217-20883)</td> <td>Apr-19</td> </tr> <tr> <td>Reference Probe ES/NV</td> <td>SN_3013</td> <td>30-Dec-17 (No. ES3-9013_Cert17)</td> <td>Dec-18</td> </tr> <tr> <td>DAS4</td> <td>SN_660</td> <td>21-Dec-17 (No. DA64-986_Cert17)</td> <td>Dec-18</td> </tr> <tr> <td>Secondary Standards</td> <td>ID</td> <td>Check Date (In-house)</td> <td>Scheduled Check</td> </tr> <tr> <td>Power meter E4419B</td> <td>SN_GB12500074</td> <td>08-Apr-18 (In-house check Jun-18)</td> <td>In-house check Jun-19</td> </tr> <tr> <td>Power meter E4415A</td> <td>SN_MV14000077</td> <td>08-Apr-18 (In-house check Jun-18)</td> <td>In-house check Jun-19</td> </tr> <tr> <td>Power meter E4415A</td> <td>SN_MV14000078</td> <td>08-Apr-18 (In-house check Jun-18)</td> <td>In-house check Jun-19</td> </tr> <tr> <td>RF generator HP 8648C</td> <td>SN_U5940000722</td> <td>08-Aug-18 (In-house check Jun-18)</td> <td>In-house check Jun-19</td> </tr> <tr> <td>Network Analyzer 93029A</td> <td>SN_US101000477</td> <td>31-Mar-14 (In-house check Oct-16)</td> <td>In-house check Oct-19</td> </tr> </tbody> </table>		Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration	Power meter NRP	SN_104776	08-Apr-18 (No. 217-20073705873)	Apr-19	Power meter HP-291	SN_104777	08-Apr-18 (No. 217-20073705874)	Apr-19	Power meter HP-291	SN_103345	08-Apr-18 (No. 217-209173)	Apr-19	Reference 20 dB Attenuator	SN_98277 (20dB)	08-Apr-18 (No. 217-20883)	Apr-19	Reference Probe ES/NV	SN_3013	30-Dec-17 (No. ES3-9013_Cert17)	Dec-18	DAS4	SN_660	21-Dec-17 (No. DA64-986_Cert17)	Dec-18	Secondary Standards	ID	Check Date (In-house)	Scheduled Check	Power meter E4419B	SN_GB12500074	08-Apr-18 (In-house check Jun-18)	In-house check Jun-19	Power meter E4415A	SN_MV14000077	08-Apr-18 (In-house check Jun-18)	In-house check Jun-19	Power meter E4415A	SN_MV14000078	08-Apr-18 (In-house check Jun-18)	In-house check Jun-19	RF generator HP 8648C	SN_U5940000722	08-Aug-18 (In-house check Jun-18)	In-house check Jun-19	Network Analyzer 93029A	SN_US101000477	31-Mar-14 (In-house check Oct-16)	In-house check Oct-19																																													
Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration																																																																																															
Power meter NRP	SN_104776	08-Apr-18 (No. 217-20073705873)	Apr-19																																																																																															
Power meter HP-291	SN_104777	08-Apr-18 (No. 217-20073705874)	Apr-19																																																																																															
Power meter HP-291	SN_103345	08-Apr-18 (No. 217-209173)	Apr-19																																																																																															
Reference 20 dB Attenuator	SN_98277 (20dB)	08-Apr-18 (No. 217-20883)	Apr-19																																																																																															
Reference Probe ES/NV	SN_3013	30-Dec-17 (No. ES3-9013_Cert17)	Dec-18																																																																																															
DAS4	SN_660	21-Dec-17 (No. DA64-986_Cert17)	Dec-18																																																																																															
Secondary Standards	ID	Check Date (In-house)	Scheduled Check																																																																																															
Power meter E4419B	SN_GB12500074	08-Apr-18 (In-house check Jun-18)	In-house check Jun-19																																																																																															
Power meter E4415A	SN_MV14000077	08-Apr-18 (In-house check Jun-18)	In-house check Jun-19																																																																																															
Power meter E4415A	SN_MV14000078	08-Apr-18 (In-house check Jun-18)	In-house check Jun-19																																																																																															
RF generator HP 8648C	SN_U5940000722	08-Aug-18 (In-house check Jun-18)	In-house check Jun-19																																																																																															
Network Analyzer 93029A	SN_US101000477	31-Mar-14 (In-house check Oct-16)	In-house check Oct-19																																																																																															
Calibrated by: <b>Giulio Lanza</b> Function: Laboratory Technician 																																																																																																		
Approved by: <b>Karin Pröbstli</b> Function: Technical Manager 																																																																																																		
Issued: October 23, 2018																																																																																																		
<p>EX3DV4 - SN:3708      October 22, 2018</p> <p style="text-align: center;"><b>Probe EX3DV4</b></p> <p style="text-align: center;"><b>SN:3708</b></p> <p>Manufactured: July 21, 2009 Calibrated: October 22, 2018</p> <p>Calibrated for DASY/EASY Systems (Note: non-compatible with DASY2 system!)</p> <p>Certificate No: EX3-3708_Oct18      Page 3 of 39</p>	<p>EX3DV4 - SN:3708      October 22, 2018</p> <p style="text-align: center;"><b>DASY/EASY - Parameters of Probe: EX3DV4 - SN:3708</b></p> <p><b>Basic Calibration Parameters</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th></th> <th>Sensor X</th> <th>Sensor Y</th> <th>Sensor Z</th> <th>Unc. (m%</th> </tr> </thead> <tbody> <tr> <td>Norm. (<math>\mu\text{W}/\text{Vm}^2</math>)<sup>a</sup></td> <td>0.20</td> <td>0.35</td> <td>0.42</td> <td><math>\pm 10.1\%</math></td> </tr> <tr> <td>DCP (mV)<sup>b</sup></td> <td>95.4</td> <td>105.6</td> <td>100.4</td> <td></td> </tr> </tbody> </table> <p><b>Modulation Calibration Parameters</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>UID</th> <th>Communication System Name</th> <th>A</th> <th>B</th> <th>C</th> <th>D</th> <th>VR</th> <th>Unc. (%)</th> </tr> </thead> <tbody> <tr> <td>S</td> <td>GW</td> <td>X: 0.0</td> <td>0.0</td> <td>1.0</td> <td>0.00</td> <td>134.7</td> <td><math>\pm 3.5\%</math></td> </tr> <tr> <td></td> <td></td> <td>Y: 0.0</td> <td>0.0</td> <td>1.0</td> <td></td> <td>130.6</td> <td></td> </tr> <tr> <td></td> <td></td> <td>Z: 0.0</td> <td>0.0</td> <td>1.0</td> <td></td> <td>146.9</td> <td></td> </tr> </tbody> </table> <p>Note: For details on UID parameters see Appendix.</p> <p><b>Sensor Model Parameters</b></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th></th> <th>G1</th> <th>G2</th> <th><math>\alpha</math></th> <th>T1</th> <th>T2</th> <th>T3</th> <th>T4</th> <th>T5</th> <th>T6</th> </tr> <tr> <th></th> <th>IF</th> <th>IF</th> <th></th> <th>ms</th> <th>ms</th> <th>ms</th> <th>ms</th> <th>ms</th> <th>ms</th> </tr> </thead> <tbody> <tr> <td>X</td> <td>35.84</td> <td>270.1</td> <td>4.07</td> <td>9.85</td> <td>3.02</td> <td>3.92</td> <td>0.90</td> <td>0.762</td> <td>1.009</td> </tr> <tr> <td>Y</td> <td>46.04</td> <td>231.1</td> <td>34.08</td> <td>13.47</td> <td>0.801</td> <td>3.012</td> <td>1.768</td> <td>0.195</td> <td>1.005</td> </tr> <tr> <td>Z</td> <td>38.84</td> <td>292.2</td> <td>35.97</td> <td>11.65</td> <td>0.630</td> <td>3.031</td> <td>0.000</td> <td>0.809</td> <td>1.008</td> </tr> </tbody> </table> <p>The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> <p><sup>a</sup> The uncertainties of Norm. X,Y,Z do not affect the E<sup>2</sup>-field uniformity inside TSL (see Pages 5 and 6).</p> <p><sup>b</sup> Maximum linearization parameter (momentum) not measured.</p> <p>Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed as the square of the mean value.</p> <p>Certificate No: EX3-3708_Oct18      Page 4 of 39</p>		Sensor X	Sensor Y	Sensor Z	Unc. (m%	Norm. ( $\mu\text{W}/\text{Vm}^2$ ) <sup>a</sup>	0.20	0.35	0.42	$\pm 10.1\%$	DCP (mV) <sup>b</sup>	95.4	105.6	100.4		UID	Communication System Name	A	B	C	D	VR	Unc. (%)	S	GW	X: 0.0	0.0	1.0	0.00	134.7	$\pm 3.5\%$			Y: 0.0	0.0	1.0		130.6				Z: 0.0	0.0	1.0		146.9			G1	G2	$\alpha$	T1	T2	T3	T4	T5	T6		IF	IF		ms	ms	ms	ms	ms	ms	X	35.84	270.1	4.07	9.85	3.02	3.92	0.90	0.762	1.009	Y	46.04	231.1	34.08	13.47	0.801	3.012	1.768	0.195	1.005	Z	38.84	292.2	35.97	11.65	0.630	3.031	0.000	0.809	1.008
	Sensor X	Sensor Y	Sensor Z	Unc. (m%																																																																																														
Norm. ( $\mu\text{W}/\text{Vm}^2$ ) <sup>a</sup>	0.20	0.35	0.42	$\pm 10.1\%$																																																																																														
DCP (mV) <sup>b</sup>	95.4	105.6	100.4																																																																																															
UID	Communication System Name	A	B	C	D	VR	Unc. (%)																																																																																											
S	GW	X: 0.0	0.0	1.0	0.00	134.7	$\pm 3.5\%$																																																																																											
		Y: 0.0	0.0	1.0		130.6																																																																																												
		Z: 0.0	0.0	1.0		146.9																																																																																												
	G1	G2	$\alpha$	T1	T2	T3	T4	T5	T6																																																																																									
	IF	IF		ms	ms	ms	ms	ms	ms																																																																																									
X	35.84	270.1	4.07	9.85	3.02	3.92	0.90	0.762	1.009																																																																																									
Y	46.04	231.1	34.08	13.47	0.801	3.012	1.768	0.195	1.005																																																																																									
Z	38.84	292.2	35.97	11.65	0.630	3.031	0.000	0.809	1.008																																																																																									

## EX3DV4 Sn:3708 (2/7)

EX3DV4-SN:3708

October 22, 2018

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3708

## Calibration Parameter Determined in Head Tissue Simulating Media

$f$ [MHz] <sup>a</sup>	Relative Permittivity <sup>b</sup>	Conductivity [S/m] <sup>c</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>d</sup>	Depth <sup>e</sup> [mm]	Unc. [k=2]
450	43.5	0.87	9.79	9.79	9.79	0.14	1.20	± 13.3 %
750	41.9	0.89	9.59	9.59	9.59	0.14	0.90	± 12.0 %
835	41.5	0.90	9.16	9.16	9.16	0.51	0.82	± 12.0 %
1450	40.5	1.20	8.60	8.60	8.60	0.33	0.80	± 12.0 %
1750	40.1	1.37	8.20	8.20	8.20	0.28	0.94	± 12.0 %
1800	40.0	1.40	7.89	7.89	7.89	0.35	0.85	± 12.0 %
2000	40.0	1.40	7.86	7.86	7.86	0.34	0.80	± 12.0 %
2300	39.5	1.87	7.51	7.51	7.51	0.29	0.86	± 12.0 %
2450	39.2	1.80	7.13	7.13	7.13	0.38	0.86	± 12.0 %
2600	39.0	1.96	7.01	7.01	7.01	0.38	0.87	± 12.0 %
5200	36.0	4.06	5.48	5.48	5.48	0.40	1.80	± 13.1 %
6300	35.9	4.78	5.25	5.25	5.25	0.40	1.80	± 13.1 %
6800	35.5	5.07	4.84	4.84	4.84	0.40	1.80	± 13.1 %
5800	35.3	5.27	5.04	5.04	5.04	0.40	1.80	± 13.1 %

<sup>a</sup> Frequency validity above 300 MHz or a 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty of frequency response is ± 6.3% (k=2). The uncertainty of SAR values is ± 10% (k=2). The uncertainty of ConvF validity below 300 MHz is ± 10, 20, 40, 60 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 10% (k=2).

<sup>b</sup> At 1 GHz the uncertainty of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF assessments.

<sup>c</sup> AlphaDepth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3.6 GHz as any distance larger than half the probe tip diameter from the boundary.

EX3DV4-SN:3708

October 22, 2018

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3708

## Calibration Parameter Determined in Body Tissue Simulating Media

$f$ [MHz] <sup>a</sup>	Relative Permittivity <sup>b</sup>	Conductivity [S/m] <sup>c</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>d</sup>	Depth <sup>e</sup> [mm]	Unc. [k=2]
450	56.7	0.94	10.35	10.35	10.35	0.08	1.20	± 13.3 %
750	55.5	0.96	9.51	9.51	9.51	0.50	0.85	± 12.0 %
835	55.2	0.97	9.33	9.33	9.33	0.47	0.84	± 12.0 %
1450	54.0	1.90	7.84	7.84	7.84	0.38	0.80	± 12.0 %
1750	53.4	1.49	7.89	7.89	7.89	0.37	0.85	± 12.0 %
1900	53.3	1.52	7.56	7.56	7.56	0.42	0.84	± 12.0 %
2000	53.3	1.52	7.53	7.53	7.53	0.41	0.85	± 12.0 %
2300	52.9	1.81	7.34	7.34	7.34	0.39	0.88	± 12.0 %
2450	52.7	1.95	7.19	7.19	7.19	0.32	0.85	± 12.0 %
2600	52.6	2.16	7.14	7.14	7.14	0.32	0.85	± 12.0 %
5200	49.0	5.30	4.53	4.53	4.53	0.50	1.90	± 13.1 %
5300	48.9	5.42	4.41	4.41	4.41	0.50	1.90	± 13.1 %
5800	48.5	5.77	3.99	3.99	3.99	0.50	1.90	± 13.1 %
6800	48.2	6.00	4.21	4.21	4.21	0.50	1.90	± 13.1 %

<sup>a</sup> Frequency validity above 300 MHz or a 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty of frequency response is ± 6.3% (k=2). The uncertainty of SAR values is ± 10% (k=2). The uncertainty of ConvF validity below 300 MHz is ± 10, 20, 40, 60 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 10% (k=2).

<sup>b</sup> At 1 GHz the uncertainty of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. All frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF assessments.

<sup>c</sup> AlphaDepth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3.6 GHz as any distance larger than half the probe tip diameter from the boundary.

Certificate No: EX3-3708\_Oct18


Page 5 of 39

Certificate No: EX3-3708\_Oct18

Page 6 of 39

EX3DV4-SN:3708

October 22, 2018

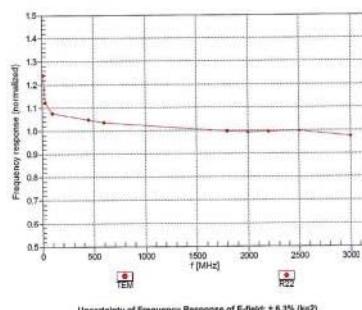Frequency Response of E-Field  
(TEM-Cell:rfl110 EXX, Waveguide: R22)



Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Certificate No: EX3-3708\_Oct18

Page 7 of 39

EX3DV4-SN:3708

October 22, 2018

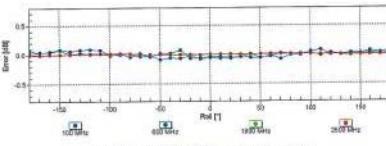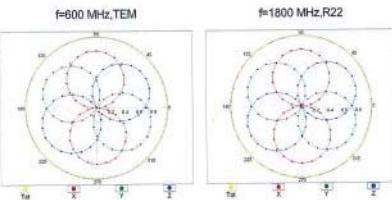Receiving Pattern ( $\phi$ ),  $\theta = 0^\circ$ 

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: EX3-3708\_Oct18


Page 8 of 39

### EX3DV4 Sn:3708 (3/7)

EX3DV4-SN:3708

October 22, 2018

**Dynamic Range f(SAR<sub>head</sub>)**  
 (TEM cell,  $f_{res} = 1900$  MHz)

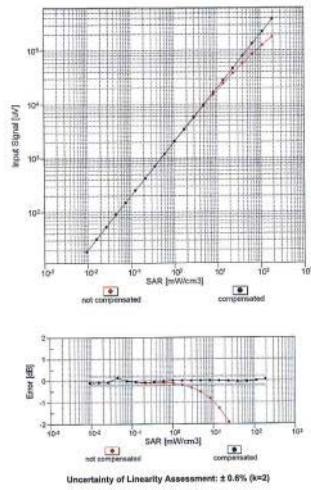



Certificate No: EX3-3708\_Oct18

Page 9 of 39

EX3DV4-SN:3708

October 22, 2018

#### Conversion Factor Assessment

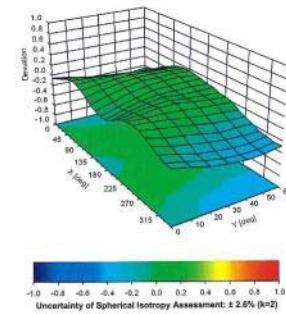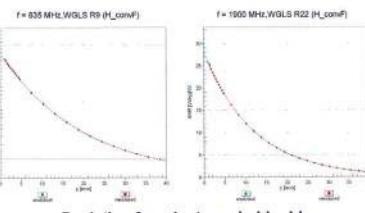

Certificate No: EX3-3708\_Oct18

Page 10 of 39

EX3DV4-SN:3708

October 22, 2018

#### DASY/EASY - Parameters of Probe: EX3DV4 - SN:3708

##### Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	0.5
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

CertPoste No: EX3-3708\_Oct18

Page 11 of 39









750V3 Sn:1101 (1/2)

<p><b>SRTC</b>  The State Radio monitoring_center Testing Center  国家无线电监测中心检测中心</p> <p><b>750V3 Sn:1101 (1/2)</b></p> <p>Client SRTC Certificate No.: Z17-97134</p> <p><b>CALIBRATION CERTIFICATE</b></p> <p><b>Object:</b> D750V3 - SN: 1101</p> <p><b>Calibration Procedure(s):</b> FF-Z11-003-01 Calibration Procedures for dipole validation kits</p> <p><b>Calibration date:</b> September 13, 2017</p> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility; environment temperature(22±3)°C and humidity&lt;70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1"> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date/(Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> <tr> <td>Power Meter NRV/D</td> <td>102196</td> <td>02-Mar-17 (CTTL, No.J17X01254)</td> <td>Mar-18</td> </tr> <tr> <td>Power sensor NR/ZS</td> <td>100596</td> <td>02-Mar-17 (CTTL, No.J17X01254)</td> <td>Mar-18</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7433</td> <td>26-Sep-16(SPEAG, No EX3-7433_Sep16)</td> <td>Sep-17</td> </tr> <tr> <td>DAE4</td> <td>SN 1331</td> <td>19-Jan-17(CTTL-SPEAG, No.Z17-97015)</td> <td>Jan-18</td> </tr> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date/(Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> <tr> <td>Signal Generator E4438C</td> <td>MY49071430</td> <td>13-Jan-17 (CTTL, No.J17X0286)</td> <td>Jan-18</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY48111013</td> <td>13-Jan-17 (CTTL, No.J17X00285)</td> <td>Jan-18</td> </tr> </table> <p>Calibrated by: Zhao Jing      Function: SAR Test Engineer      Signature: </p> <p>Reviewed by: Yu Zongying      Function: SAR Test Engineer      Signature: </p> <p>Approved by: Qiu Dianyuan      Function: SAR Project Leader      Signature: </p> <p>Issued: September 16, 2017</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory</p> <p>Certificate No: Z17-97134      Page 1 of 8</p>	Primary Standards	ID #	Cal Date/(Calibrated by, Certificate No.)	Scheduled Calibration	Power Meter NRV/D	102196	02-Mar-17 (CTTL, No.J17X01254)	Mar-18	Power sensor NR/ZS	100596	02-Mar-17 (CTTL, No.J17X01254)	Mar-18	Reference Probe EX3DV4	SN 7433	26-Sep-16(SPEAG, No EX3-7433_Sep16)	Sep-17	DAE4	SN 1331	19-Jan-17(CTTL-SPEAG, No.Z17-97015)	Jan-18	Secondary Standards	ID #	Cal Date/(Calibrated by, Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY49071430	13-Jan-17 (CTTL, No.J17X0286)	Jan-18	Network Analyzer E5071C	MY48111013	13-Jan-17 (CTTL, No.J17X00285)	Jan-18	<p><b>TTL</b>  In Collaboration with  CALIBRATION LABORATORY</p> <p>Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  Tel: +86-10-62304013-2079   Fax: +86-10-62304013-2504  E-mail: ctllj@sohu.com   http://www.ctllj.net</p> <p><b>CNAS</b>  中国认可  CNAS L0570  CALIBRATION</p> <p>Add: No. 51 Xueyuan Road, Haidian District, Beijing, 100191, China  Tel: +86-10-62304013-2079   Fax: +86-10-62304013-2504  E-mail: cnas@ctllj.net   http://www.cnasl.net</p> <p><b>Glossary:</b></p> <ul style="list-style-type: none"> <li>TSL tissue simulating liquid</li> <li>ComIF sensitivity in TSL / NORMxyz</li> <li>N/A not applicable or not measured</li> </ul> <p><b>Calibration is Performed According to the Following Standards:</b></p> <ol style="list-style-type: none"> <li>a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013</li> <li>b) IEC 62209-1, "Measurement procedure for assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices- Part 1: Device used next to the ear (Frequency range of 300MHz to 6GHz)", July 2018</li> <li>c) IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010</li> </ol> <p>d) KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz</p> <p><b>Additional Documentation:</b></p> <p>e) DASY4.5 System Handbook</p> <p><b>Methods Applied and Interpretation of Parameters:</b></p> <ul style="list-style-type: none"> <li>▪ <b>Measurement Conditions:</b> Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.</li> <li>▪ <b>Antenna Parameters with TSL:</b> The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.</li> <li>▪ <b>Feed Point Impedance and Return Loss:</b> These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflectance. No uncertainty required.</li> <li>▪ <b>Electrical Delay:</b> One-way delay between the SMA connector and the antenna feed point. No uncertainty required.</li> <li>▪ <b>SAR measured:</b> SAR measured at the stated antenna input power.</li> <li>▪ <b>SAR normalized:</b> SAR as measured, normalized to an input power of 1 W at the antenna connector.</li> <li>▪ <b>SAR for nominal TSL parameters:</b> The measured TSL parameters are used to calculate the nominal SAR result.</li> </ul> <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor <math>k=2</math>, which for a normal distribution Corresponds to a coverage probability of approximately 95%.</p> <p>Certificate No: Z17-97134      Page 2 of 8</p>																																																																		
Primary Standards	ID #	Cal Date/(Calibrated by, Certificate No.)	Scheduled Calibration																																																																																																
Power Meter NRV/D	102196	02-Mar-17 (CTTL, No.J17X01254)	Mar-18																																																																																																
Power sensor NR/ZS	100596	02-Mar-17 (CTTL, No.J17X01254)	Mar-18																																																																																																
Reference Probe EX3DV4	SN 7433	26-Sep-16(SPEAG, No EX3-7433_Sep16)	Sep-17																																																																																																
DAE4	SN 1331	19-Jan-17(CTTL-SPEAG, No.Z17-97015)	Jan-18																																																																																																
Secondary Standards	ID #	Cal Date/(Calibrated by, Certificate No.)	Scheduled Calibration																																																																																																
Signal Generator E4438C	MY49071430	13-Jan-17 (CTTL, No.J17X0286)	Jan-18																																																																																																
Network Analyzer E5071C	MY48111013	13-Jan-17 (CTTL, No.J17X00285)	Jan-18																																																																																																
<p><b>SPEAG</b>  In Collaboration with  CALIBRATION LABORATORY</p> <p>Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  Tel: +86-10-62304013-2079   Fax: +86-10-62304013-2504  E-mail: ctllj@sohu.com   http://www.ctllj.net</p> <p><b>Measurement Conditions</b>  DASY system configuration, as far as not given on page 1.</p> <table border="1"> <tr> <td>DASY Version</td> <td>DASY52</td> <td>52.10.0.1446</td> </tr> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>16 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>750 MHz ± 1 MHz</td> <td></td> </tr> </table> <p><b>Head TSL parameters</b>  The following parameters and calculations were applied.</p> <table border="1"> <tr> <td>Nominal Head TSL parameters</td> <td>Temperature</td> <td>Permittivity</td> <td>Conductivity</td> </tr> <tr> <td>22.0 °C</td> <td>41.9</td> <td>0.88 mho/m</td> <td></td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>41.5 ± 6 %</td> <td>0.88 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>&lt;1.0 °C</td> <td>—</td> <td>—</td> </tr> </table> <p><b>SAR result with Head TSL</b></p> <table border="1"> <tr> <td>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>2.05 mW/g</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>8.26 mW/g ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>1.34 mW/g</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>5.39 mW/g ± 18.7 % (k=2)</td> </tr> </table> <p><b>Body TSL parameters</b>  The following parameters and calculations were applied.</p> <table border="1"> <tr> <td>Nominal Body TSL parameters</td> <td>Temperature</td> <td>Permittivity</td> <td>Conductivity</td> </tr> <tr> <td>22.0 °C</td> <td>55.5</td> <td>0.98 mho/m</td> <td></td> </tr> <tr> <td>Measured Body TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>55.4 ± 6 %</td> <td>0.95 mho/m ± 6 %</td> </tr> <tr> <td>Body TSL temperature change during test</td> <td>&lt;1.0 °C</td> <td>—</td> <td>—</td> </tr> </table> <p><b>SAR result with Body TSL</b></p> <table border="1"> <tr> <td>SAR averaged over 1 cm<sup>3</sup> (1 g) of Body TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>2.15 mW/g</td> </tr> <tr> <td>SAR for nominal Body TSL parameters</td> <td>normalized to 1W</td> <td>8.49 mW/g ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm<sup>3</sup> (10 g) of Body TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>1.42 mW/g</td> </tr> <tr> <td>SAR for nominal Body TSL parameters</td> <td>normalized to 1W</td> <td>5.73 mW/g ± 18.7 % (k=2)</td> </tr> </table> <p>Certificate No: Z17-97134      Page 3 of 8</p>	DASY Version	DASY52	52.10.0.1446	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	16 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	750 MHz ± 1 MHz		Nominal Head TSL parameters	Temperature	Permittivity	Conductivity	22.0 °C	41.9	0.88 mho/m		Measured Head TSL parameters	(22.0 ± 0.2) °C	41.5 ± 6 %	0.88 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition		SAR measured	250 mW input power	2.05 mW/g	SAR for nominal Head TSL parameters	normalized to 1W	8.26 mW/g ± 18.8 % (k=2)	SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition		SAR measured	250 mW input power	1.34 mW/g	SAR for nominal Head TSL parameters	normalized to 1W	5.39 mW/g ± 18.7 % (k=2)	Nominal Body TSL parameters	Temperature	Permittivity	Conductivity	22.0 °C	55.5	0.98 mho/m		Measured Body TSL parameters	(22.0 ± 0.2) °C	55.4 ± 6 %	0.95 mho/m ± 6 %	Body TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition		SAR measured	250 mW input power	2.15 mW/g	SAR for nominal Body TSL parameters	normalized to 1W	8.49 mW/g ± 18.8 % (k=2)	SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	Condition		SAR measured	250 mW input power	1.42 mW/g	SAR for nominal Body TSL parameters	normalized to 1W	5.73 mW/g ± 18.7 % (k=2)	<p><b>SPEAG</b>  In Collaboration with  CALIBRATION LABORATORY</p> <p>Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  Tel: +86-10-62304013-2079   Fax: +86-10-62304013-2504  E-mail: ctllj@sohu.com   http://www.ctllj.net</p> <p><b>Appendix (Additional assessments outside the scope of CNAS L0570)</b></p> <p><b>Antenna Parameters with Head TSL</b></p> <table border="1"> <tr> <td>Impedance, transformed to feed point</td> <td>53.9Ω ± 0.24Ω</td> </tr> <tr> <td>Return Loss</td> <td>-28.4dB</td> </tr> </table> <p><b>Antenna Parameters with Body TSL</b></p> <table border="1"> <tr> <td>Impedance, transformed to feed point</td> <td>52.0Ω ± 2.22Ω</td> </tr> <tr> <td>Return Loss</td> <td>-30.6dB</td> </tr> </table> <p><b>General Antenna Parameters and Design</b></p> <table border="1"> <tr> <td>Electrical Delay (one direction)</td> <td>1.136 ns</td> </tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.  The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded. The same principle is explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The dipole arms are still according to the Standard.  No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.</p> <p><b>Additional EUT Data</b></p> <table border="1"> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </table> <p>Certificate No: Z17-97134      Page 4 of 8</p>	Impedance, transformed to feed point	53.9Ω ± 0.24Ω	Return Loss	-28.4dB	Impedance, transformed to feed point	52.0Ω ± 2.22Ω	Return Loss	-30.6dB	Electrical Delay (one direction)	1.136 ns	Manufactured by	SPEAG
DASY Version	DASY52	52.10.0.1446																																																																																																	
Extrapolation	Advanced Extrapolation																																																																																																		
Phantom	Triple Flat Phantom 5.1C																																																																																																		
Distance Dipole Center - TSL	16 mm	with Spacer																																																																																																	
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																																																																		
Frequency	750 MHz ± 1 MHz																																																																																																		
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity																																																																																																
22.0 °C	41.9	0.88 mho/m																																																																																																	
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.5 ± 6 %	0.88 mho/m ± 6 %																																																																																																
Head TSL temperature change during test	<1.0 °C	—	—																																																																																																
SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition																																																																																																		
SAR measured	250 mW input power	2.05 mW/g																																																																																																	
SAR for nominal Head TSL parameters	normalized to 1W	8.26 mW/g ± 18.8 % (k=2)																																																																																																	
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition																																																																																																		
SAR measured	250 mW input power	1.34 mW/g																																																																																																	
SAR for nominal Head TSL parameters	normalized to 1W	5.39 mW/g ± 18.7 % (k=2)																																																																																																	
Nominal Body TSL parameters	Temperature	Permittivity	Conductivity																																																																																																
22.0 °C	55.5	0.98 mho/m																																																																																																	
Measured Body TSL parameters	(22.0 ± 0.2) °C	55.4 ± 6 %	0.95 mho/m ± 6 %																																																																																																
Body TSL temperature change during test	<1.0 °C	—	—																																																																																																
SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition																																																																																																		
SAR measured	250 mW input power	2.15 mW/g																																																																																																	
SAR for nominal Body TSL parameters	normalized to 1W	8.49 mW/g ± 18.8 % (k=2)																																																																																																	
SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	Condition																																																																																																		
SAR measured	250 mW input power	1.42 mW/g																																																																																																	
SAR for nominal Body TSL parameters	normalized to 1W	5.73 mW/g ± 18.7 % (k=2)																																																																																																	
Impedance, transformed to feed point	53.9Ω ± 0.24Ω																																																																																																		
Return Loss	-28.4dB																																																																																																		
Impedance, transformed to feed point	52.0Ω ± 2.22Ω																																																																																																		
Return Loss	-30.6dB																																																																																																		
Electrical Delay (one direction)	1.136 ns																																																																																																		
Manufactured by	SPEAG																																																																																																		