

Array Spectrophotometer ST-700d


ST-700d is an array spectrophotometer developed by 3nh using its own spectroscopic core technology. It uses a built-in silicon photodiode array (40 sets of dual columns) sensors and an industrial-grade MCU. The powerful data processing capability ensures the stability and accuracy of the measurement data. The array spectrophotometer ST-700d can easily control the repeatability ΔE^*ab within 0.022, and the inter-instrument error ΔE^*ab within 0.2. It can be used for accurate color measurement in various occasions and conditions, and the large-size touch screen can view the measurement results more easily and convenient. The measurement data of the instrument is consistent with other competing products from Japan, the United States, and Europe.

The array spectrophotometer ST-700d is equipped with three measurement apertures : $\Phi 8mm$, $\Phi 4mm$, and $1x3mm$. It has wider adaptability, accurate color measurement and stable performance. It is used in plastic electronics, paint and coatings, textile printing and dyeing, printed paper products, automobiles, medical care, cosmetics and food industries, and also are widely used in scientific research institutions and laboratories.

Features of Array Spectrophotometer ST-700d



1、 Silicon photodiode array (dual 40 array) sensor

Larger area dual 40 array sensor, will not be saturated under strong light, sensitivity is higher under weak light, and the spectrum response range is wider, which ensures the measurement speed, accuracy, stability and consistency of the instrument. Master the core technology, developed from same platform as international standards with full compatibility.

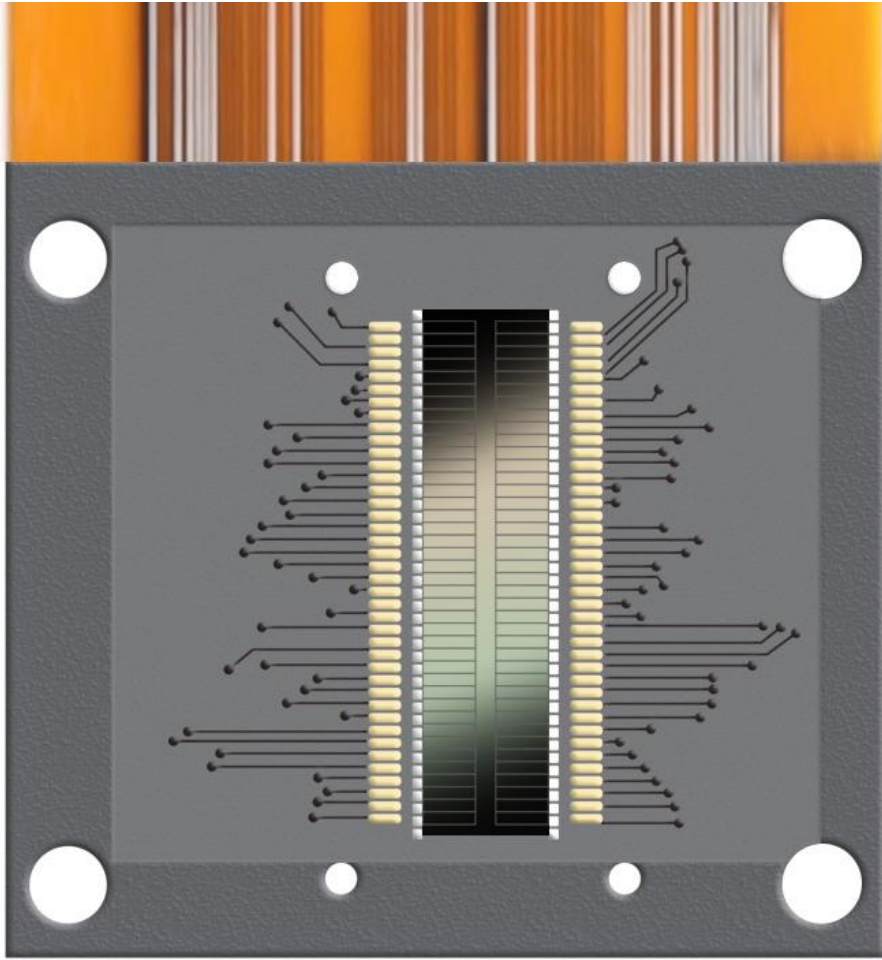


2、 Adopt Full-band balanced LED light source + UV light source

The array spectrophotometer ST-700d adopts 400~700nm full-band balanced LED light source and UV light source as the instrument lighting source, which has sufficient spectral distribution in the visible light range, avoiding the spectrum lack of white light LED in specific bands. It can also easily measure fluorescent materials and ensures the accuracy of the instrument measurement results.

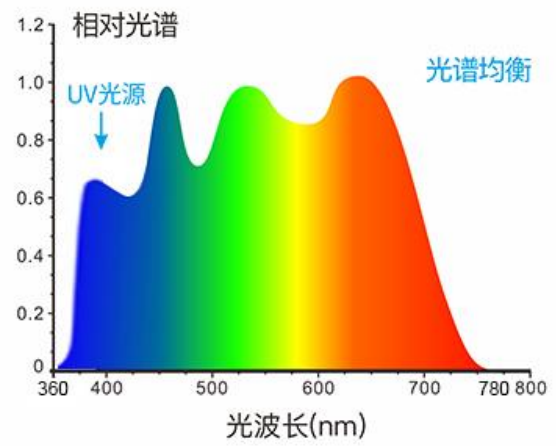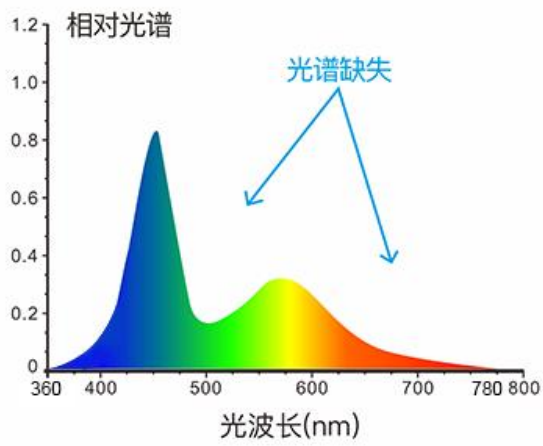

3、Grating Spectroscopic Technology

Adopting plane grating spectroscopic technology, it has higher resolution and makes color measurement more accurate.

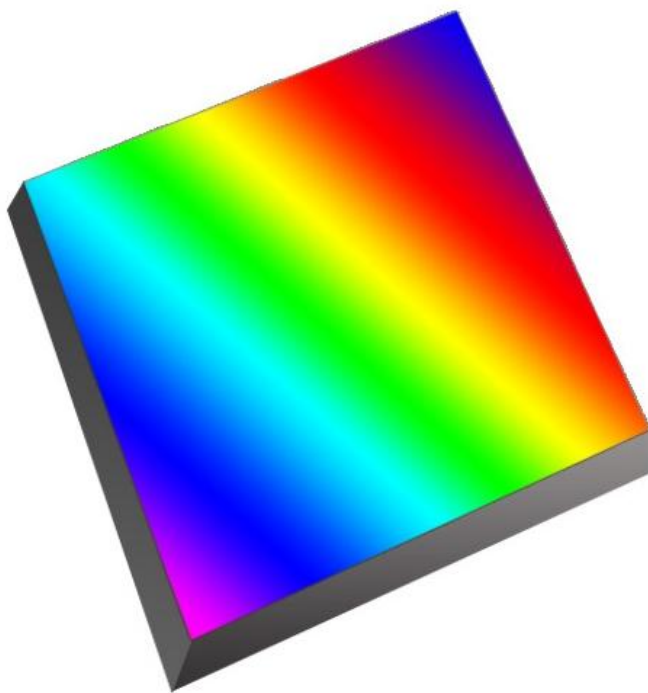

4、Non-contact automatic whiteboard Calibration

The array spectrophotometer ST-700d is equipped with an intelligent calibration base, which can be used for non-contact automatic whiteboard calibration. The professional-grade standard whiteboard

reflectance $R\% \geq 95\%$ has good surface uniformity and high stability, and can obtain repeatable and accurate data.



5、Novel fashion design based on ergonomics

The large-size touch screen is more convenient to check the measurement results and color judgment. The position of the hand grip and the measurement button are carefully designed to meet different grip habits. The smooth and fine surface is derived from the high-precision appearance processing art.



6. Equipped with three measuring apertures to meet the needs of more sample measurement

The array spectrophotometer ST-700d is equipped with $\varnothing 8\text{mm}$ platform aperture, $\varnothing 4\text{mm}$ platform aperture, and $1 \times 3\text{mm}$ aperture as standard accessory, which meets the measurement needs of most special samples.



7、 Camera framing positioning can clearly observe the measured area

The array spectrophotometer ST-700d has a built-in camera for viewing and positioning. Through the real-time viewing of the camera, it can accurately determine whether the measured part of the object is at the center of the target, which improves the measurement efficiency and accuracy.



8、 Excellent inter-instrument Error and repeatability

Repeatability $\Delta E^*ab \leq 0.022$, inter-instrument error $\Delta E^*ab \leq 0.2$, the data is stable and reliable, ensuring the consistency of measurement data of multiple devices, which can be used for color matching and accurate color transfer.




9、Multiple Color Measurement Spaces and Observation Light Sources

Provide CIE LAB, XYZ, Yxy, LCh, CIE LUV, s-RGB, HunterLab, βxy , DIN Lab99, Munsell(C/2) color spaces, and multiple observation light sources: D65, A, C, D50, D55, D75, F1, F2(CWF), F3, F4, F5, F6, F7(DLF), F8, F9, F10(TPL5), F11(TL84), F12(TL83/U30), B, U35, NBF, ID50, ID65, LED-B1, LED-B2, LED-B3, LED-B4, LED-B5, LED-BH1, LED-RGB1, LED-V1, LED-V2, LED-C2, LED-C3, LED-C5. The light source can be customized (a total of 41 kinds of light sources, some of which are realized through the host computer/APP), which can meet the special measurement requirements under different measurement conditions.




10、 Using the Internationally Universal D/8 SCI/SCE Synthesis Technology

Use D/8 (SCI/SCE) to measure the structure, reflect the color itself more objectively, reduce the influence of the surface texture of the object on the test result, and meet the standards: CIE No.15, GB/T 3978, GB 2893, GB/T 18833, ISO7724-1, ASTM E1164, DIN5033 Teil7.

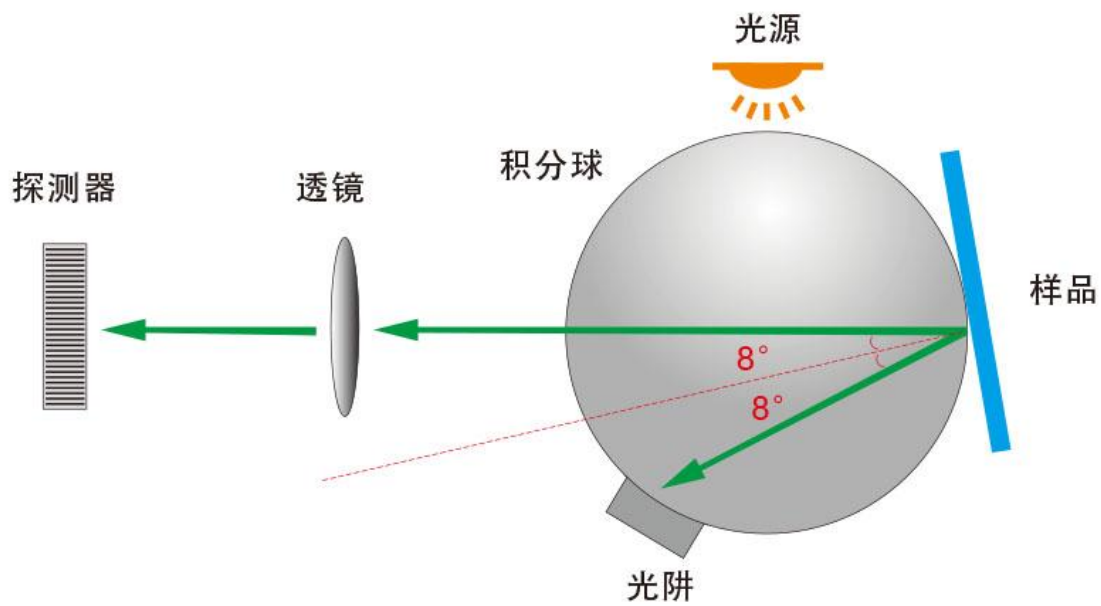

11、 Dual Optical Path System for More Accurate Color Measurement

Dual optical path system, the optical resolution in the visible light range is less than 10nm, and can measure the SCI and SCE spectra of samples at the same time.

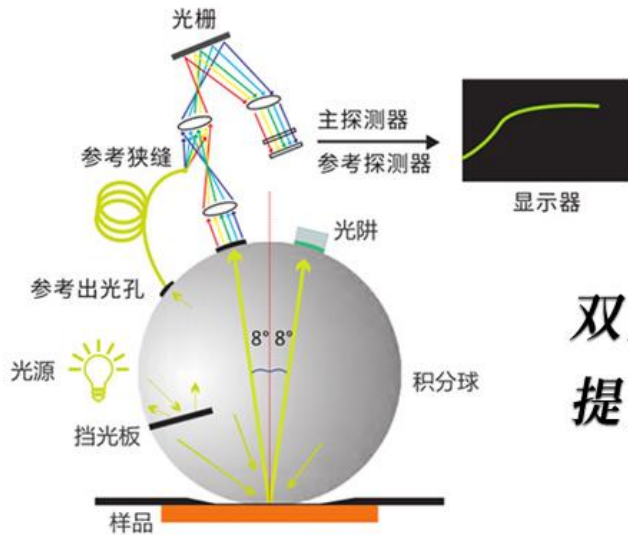

双光学引擎，
提升不只一点点！

12、Support Android, IOS, Windows, WeChat Applet, Harmony OS.

The array spectrophotometer ST-700d supports Android, IOS, Windows, WeChat applets, and Harmony OS, and is suitable for quality monitoring and color data management in various industries. Codify the user's color management with data, compare color differences, generate test reports, provide a variety of color space measurement data, and customize the customer's color management work.



Android



ISO手机/电脑



鸿蒙 HarmonyOS



微信小程序



Windows



3nh 云配色

Technical Parameters of Array Spectrophotometer ST-700d

Product Name	Array Spectrophotometer ST-700d
Optical Geometry	D/8 (diffused illumination, 8-degree viewing angle) SCI & SCE; Include UV & Exclude UV. Conform to Standards: CIE No.15,GB/T 3978,GB 2893,GB/T 18833,ISO7724-1,ASTM E1164,DIN5033 Teil7
Integrating Sphere Size	Φ40mm

Light Source	Combined Full Spectrum LED Lamp, UV Lamp.
Spectroscopic Method	Plane Grating
Sensor	Large-area silicon photodiode array (40 pairs of dual columns)
Wavelength Range	400~700nm
Wavelength Interval	10nm
Reflectance Range	0~200%
Measuring Apertures	Three Apertures: 8mm Platform + 4mm Platform + 1*3mm
Locating Method	Cross Locating + Camera Locating
Whiteboard Calibration	Non-contact automatic whiteboard Calibration
SCI/SCE	Measure SCI+SCE at the same time
Color Spaces	CIE LAB,XYZ,Yxy,LCh,CIE LUV,s-RGB,HunterLab, β_{xy} ,DIN Lab99 Munsell(C/2)
Color Difference Formula	ΔE^*_{ab} , ΔE^*_{uv} , ΔE^*_{94} , $\Delta E^*_{cmc}(2:1)$, $\Delta E^*_{cmc}(1:1)$, ΔE^*_{00} , DIN ΔE_{99} , ΔE (Hunter)
Other Colorimetric Index	Spectrum Reflectance Rate, WI(ASTM E313-00, ASTM E313-73, CIE/ISO, AATCC, Hunter, TaubeBergerStensby),

	<p>YI(ASTM D1925,ASTM E313-00,ASTM E313-73)</p> <p>Metamerism Index Mt,</p> <p>Staining Fastness, Color Fastness, Strength (dye strength, tinting strength), Opacity</p> <p>8-degree Gloss, 555 Index, Blackness (My,dM) , Color Density CMYK(A,T,E,M), Tint(ASTM E313-00), Munsell (Some functions are realized through the computer)</p>
Observer Angle	2°/10°
Illuminants	<p>D65,A,C,D50,D55,D75,F1,F2(CWF),F3,F4, F5, F6,F7(DLF),F8,F9, F10(TPL5),F11(TL84),F12(TL83/U30),B,U35,NBF,</p> <p>ID50,ID65,LED-B1,LED-B2,LED-B3,LED-B4,LED-B5,LED-BH1,LED-RGB1,LED-V1,LED-V2,LED-C2,LED-C3,LED-C5, Light source can be customized(a total of 41 kinds of light sources, some of which are realized through the host computer/APP)</p>
Displayed Data	<p>Spectrogram/Values, Samples Chromaticity Values, Color Difference Values/Graph, PASS/FAIL Result, Color Simulation, Color Offset</p>
Measuring Time	About 1.5s
Repeatability	<p>Chromaticity Value: MAV/SCI, within ΔE^*ab 0.022 (after warm-up and calibration, the average value of measuring 30 times on the whiteboard at intervals of 5s)</p> <p>Spectral reflectance: MAV/SCI, standard deviation within 0.07% (400~700nm)</p>
Inter-instrument Error	MAV/SCI, ΔE^*ab within 0.2 (The average value of measuring BCRA series II 12 color tiles)
Display Accuracy	0.01
Measurement	Single measurement, average measurement (2~99 times)

nt Mode	
Data Storage	APP mass storage
Accuracy Guarantee	Guarantee passing the Grade 1 metrology
Dimension	Length X Width X Height=114X70X208mm
Weight	About 435g (Calibration Base not included)
Battery	Lithium battery, 3.7V, 5000mAh, 8500 times measurements within 8 hours
Illuminant Life Span	More than 1.5 million measurements in 10 years
Display	TFT True Color 3.5inch, Capacitive Touch Screen
Data Port	USB, Bluetooth®5.0
Data Storage	500 pcs standard samples, 20,000 pcs samples (one piece of data can include SCI+SC E at the same time), APP/PC mass storage
Software Support	Andriod, IOS, Windows, Wechat APplet, Harmony OS.
Language	Simplified Chinese, Traditional Chinese, English
Operating Environment	0~40°C, 0~85%RH (no condensing), Altitude < 2000m
Storage Environment	-20~50°C, 0~85%RH (no condensing)
Standard Accessory	Power adapter, USB cable, Manual, Quality Management Software (official website do wnload), Calibration Box, Protective Cover, Wrist Strap, Measuring Apertures
Optional Accessory	Micro-printer, Powder Test Box.

cessory	
Note:	Technical parameters are for reference only, subject to actual sales.

Warning: Changes or modifications to this unit not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

NOTE: This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

FCC Statement:

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures :

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

The product is a portable device and meets the exposure assessment requirements for portable devices.