


GENERAL NOTES:


1. MAKE FROM PET .003" THICK INDIGO GLOSS, BACKGROUND COLOR WHITE, PRINT COLOR BLACK; ADHESIVE .002" THICK 3M 220.
2. FINISHED PART MUST BE ROHS COMPLIANT.
3. SEE AGILE FOR APPROVAL AND REVISION HISTORY.
4. ALL DIMENSIONS IN MILLIMETERS UNLESS OTHERWISE NOTED.
5. FONT: CALIBRI 5 PT; CENTER EXACT TEXT IN AREA PROVIDED PER DIMENSIONS SHOWN.
6. FONT: ARIAL NARROW 4 PT; LOCATE EXACT TEXT PER DIMENSIONS SHOWN.
7. LOCATE SANMINA LOGO AS SHOWN.

REVISION HISTORY		
ZONE	REV.	DESCRIPTION
ALL	001	INITIAL RELEASE
ALL	PRELIMINARY	ADDITION OF LANGUAGE AND FONT CHANGE

PRELIMINARY

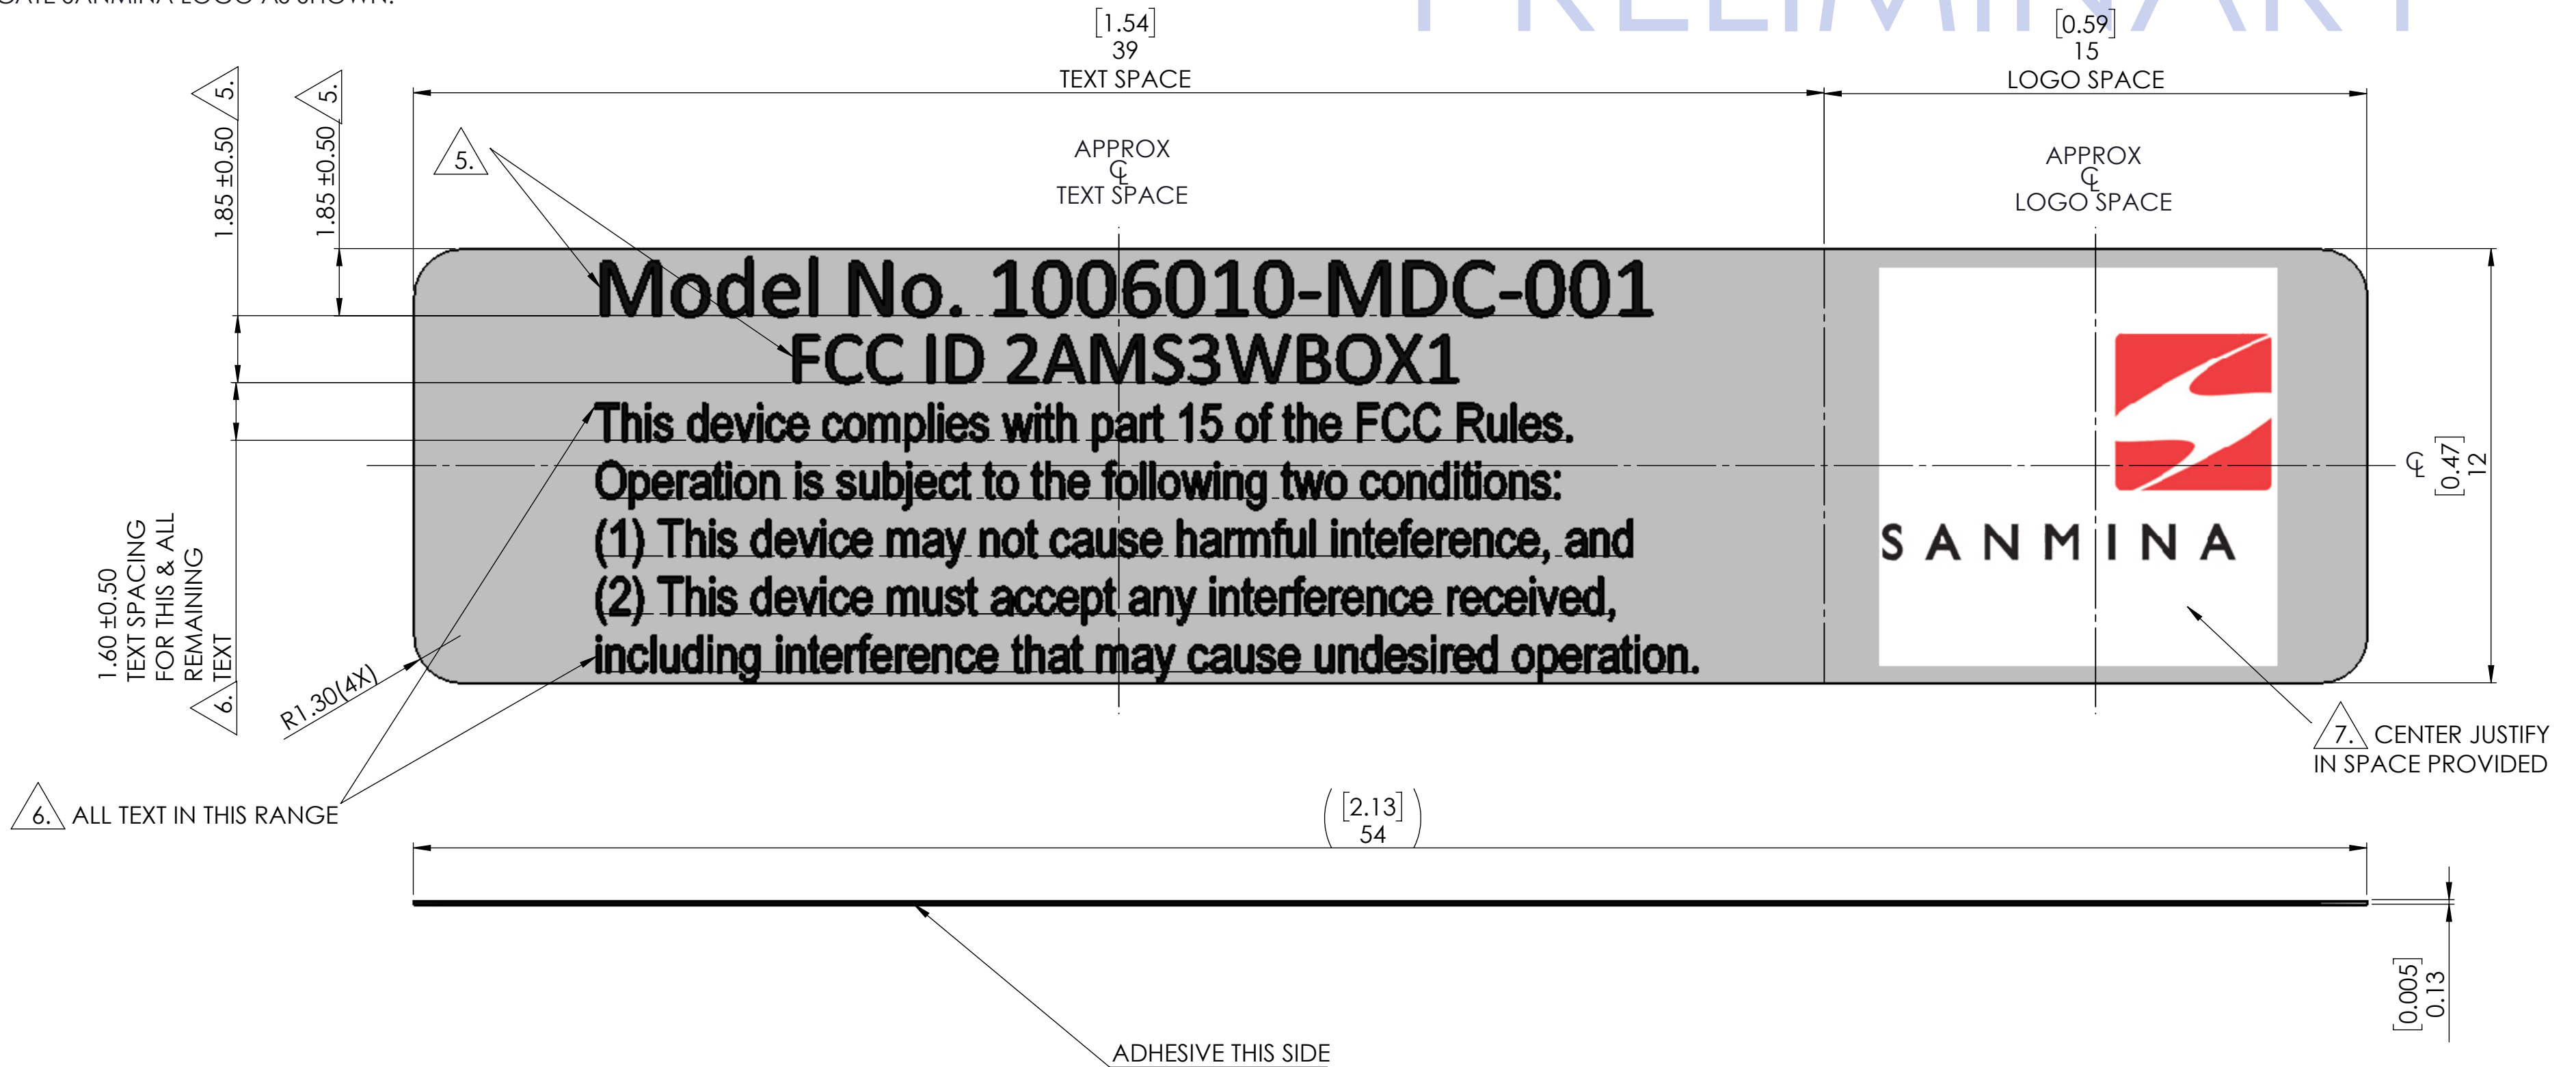

UNLESS OTHERWISE SPECIFIED		
INTERPRET PER ASME Y14.100	DIMENSIONAL TOLERANCES ON: (PER ASME Y14.5M-1994)	
THREADS PER ASME Y14.6	MILLIMETERS	DECIMALS ANGLES
REMOVE ALL BURRS AND BREAK ALL SHARP EDGES	X ± 0.25	XX ± 0.01 ± DEG
IDENTIFY BY BAG AND OR TAG PER MIL-STD-130M	XX ± 0.125	XXX ± 0.005
SURFACE FINISH 125 ✓	MATERIAL	1.
	FINISH	

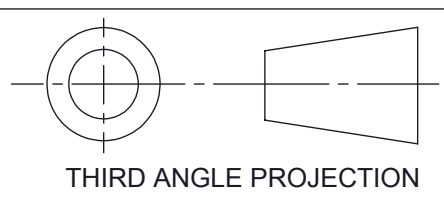

DO NOT SCALE DRAWING

SANMINA		
MEDICAL ENGINEERING WORLDWIDE MEDICAL DIVISION		
TITLE: Label, Certification		
SIZE C	CAGE CODE 17981	DWG NO. 1006020-MDC-001
SCALE	UNIT WT	SHEET 1 OF 1