


Appendix D



Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

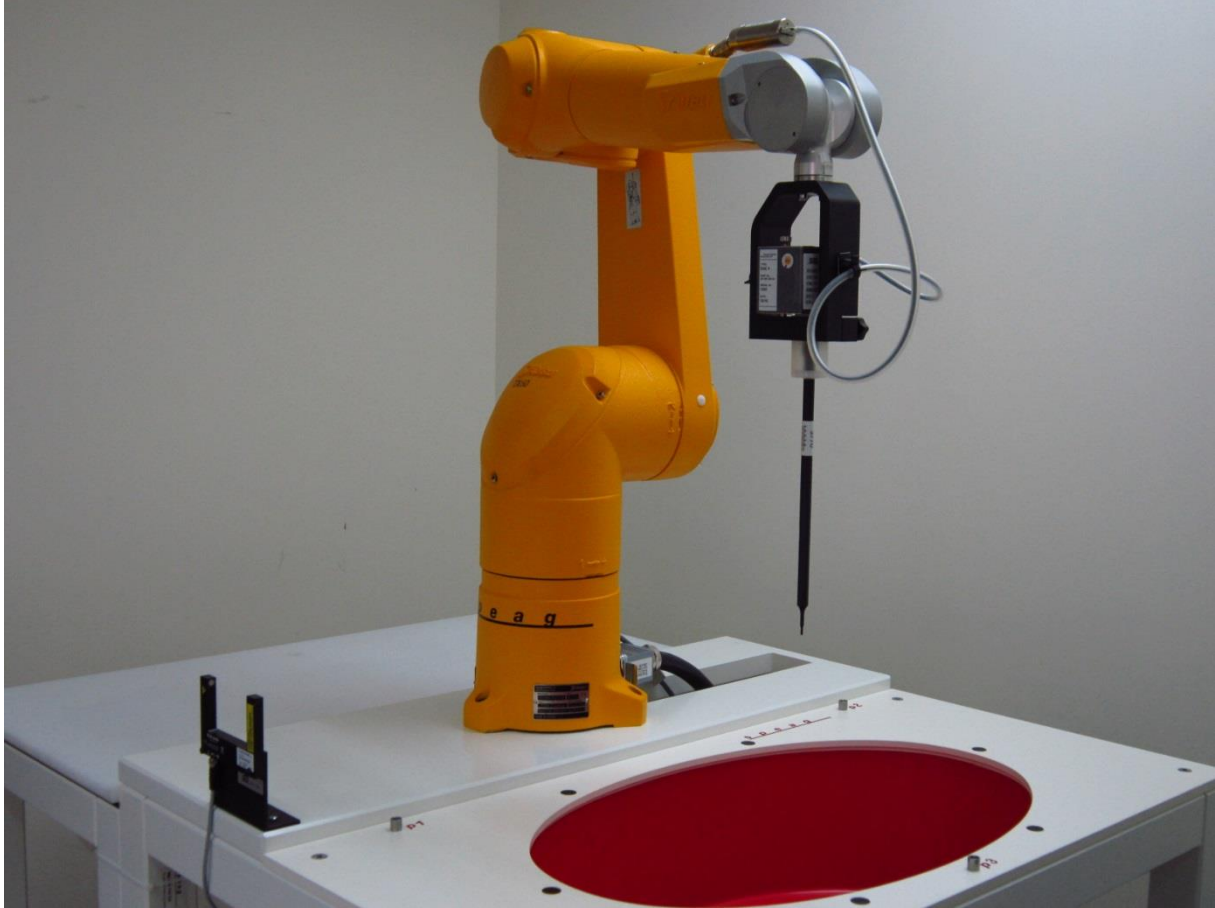

2. Photographs of Tissue Simulate Liquid

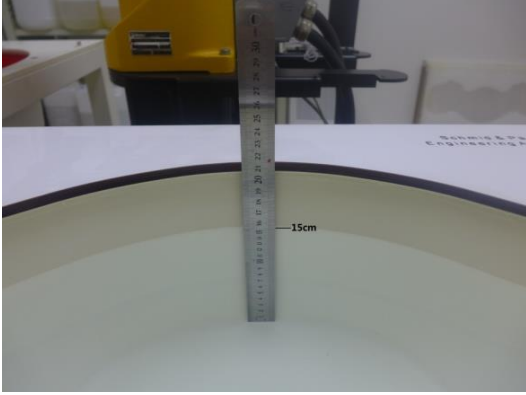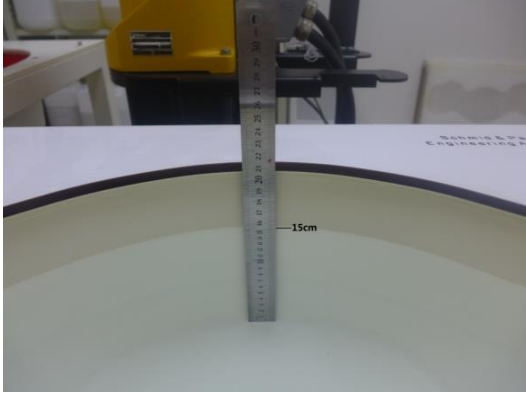Photo 1: Tissue Simulant Liquid for Head 2450	Photo 2: Tissue Simulant Liquid for Head 5GHz
	

3. Photographs of EUT test position

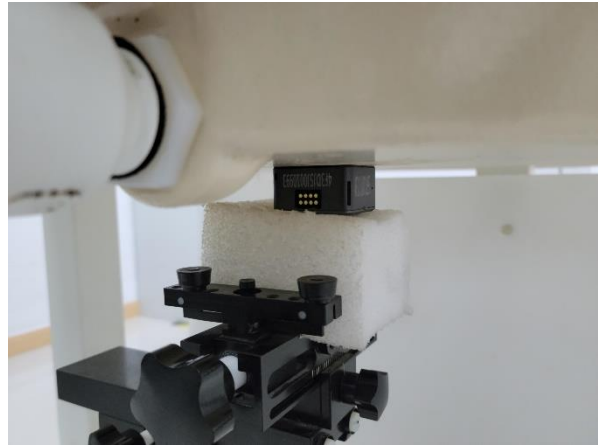
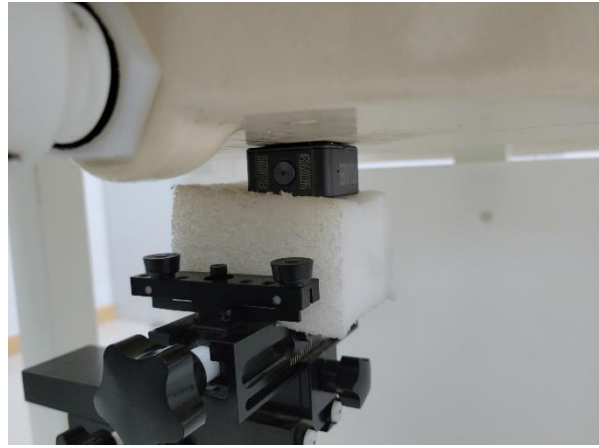
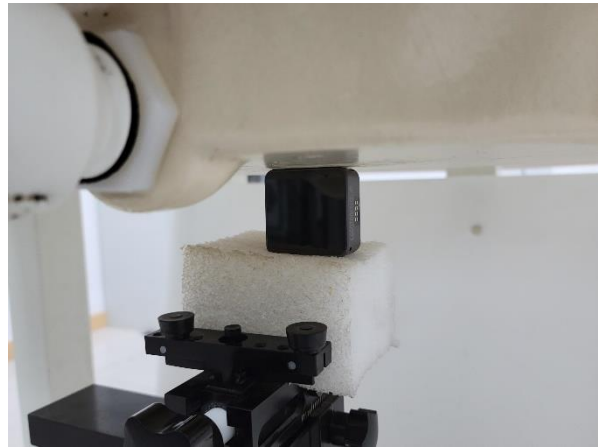
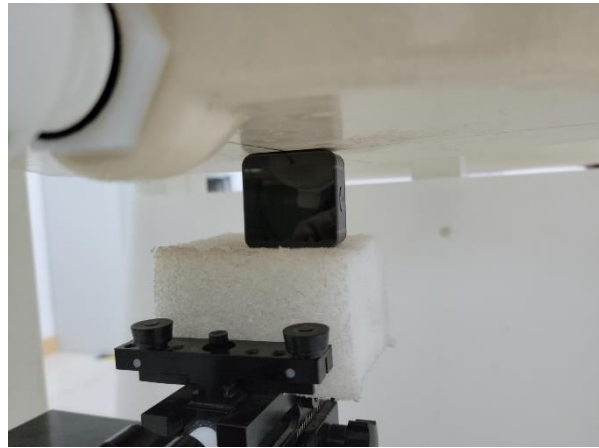

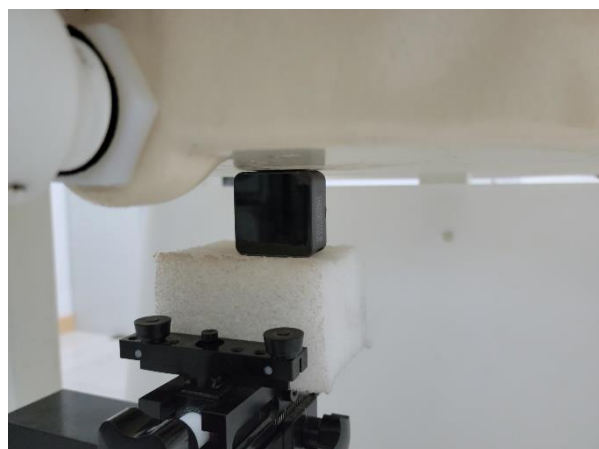
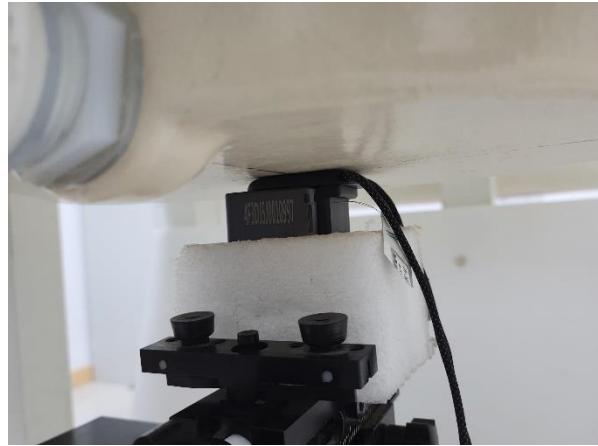
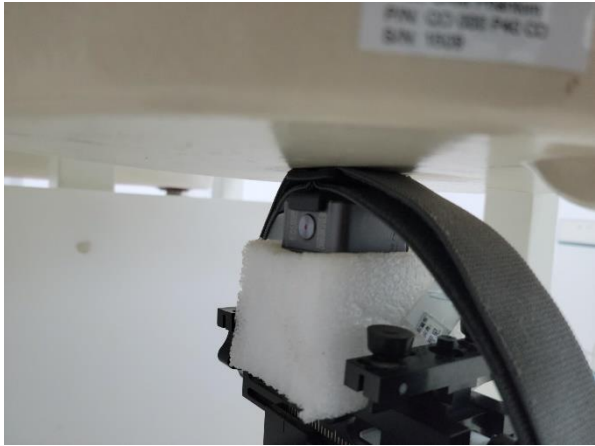
<p>Photo 3: Limbs SAR Back side 0mm</p>	<p>Photo 4: Limbs SAR Front side 0mm</p>
	
<p>Photo 5: Limbs SAR Right side 0mm</p>	<p>Photo 6: Limbs SAR Left side 0mm</p>
	
<p>Photo 7: Limbs SAR Bottom side 0mm</p>	<p>Photo 8: Limbs SAR Top side 0mm</p>
	

Photo 9: Body SAR Back side 0mm	Photo 10: Head SAR Back side 0mm
 A photograph showing the back side of a device's body. A white, rectangular SAR measurement probe is attached to a black mounting bracket. A black cable is connected to the top of the probe. The device's back cover is visible above the probe.	 A photograph showing the back side of a device's head. A white, rectangular SAR measurement probe is attached to a black mounting bracket. A black cable is connected to the top of the probe. A black strap is visible on the right side of the head. A small white label with text is visible in the upper right corner of the image.

4. EUT Constructional Details

Details please Refer to the <External Photos> & <Internal Photos>.