

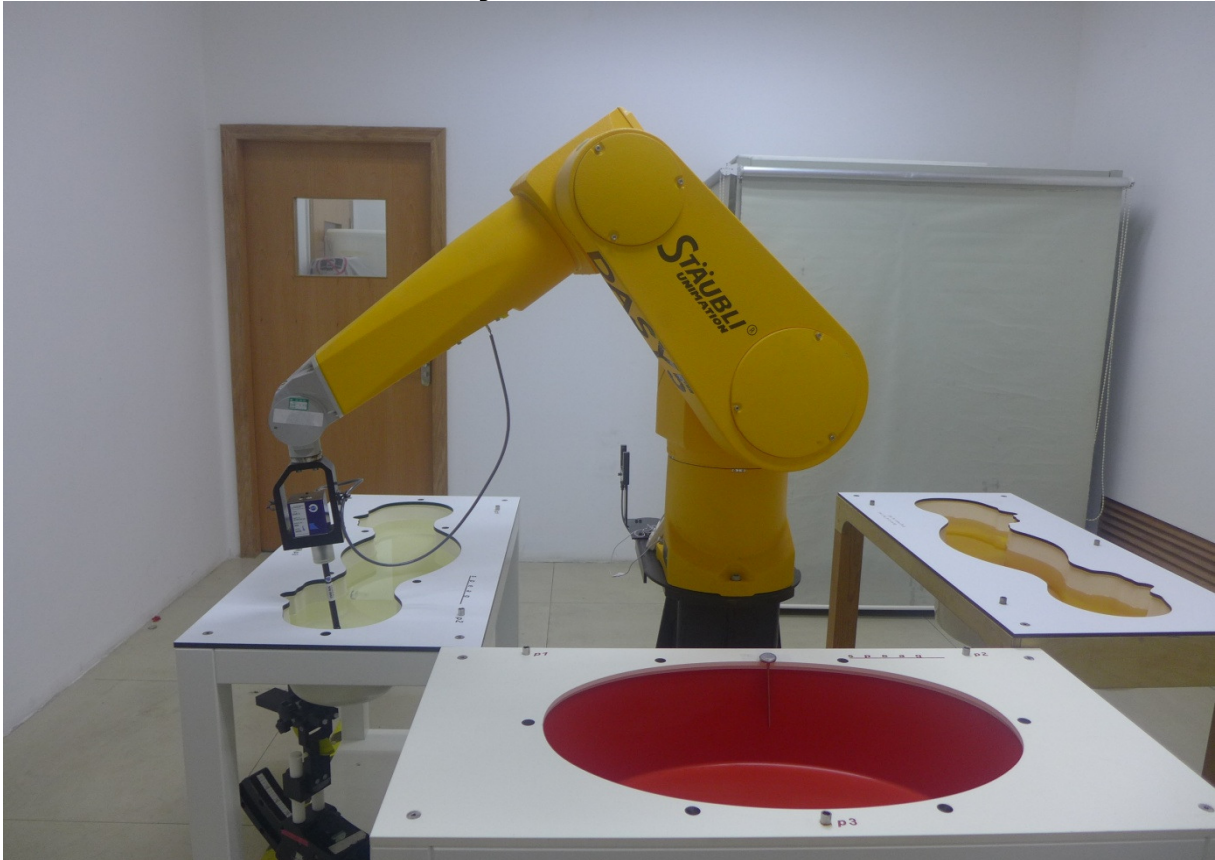


# **Appendix D**

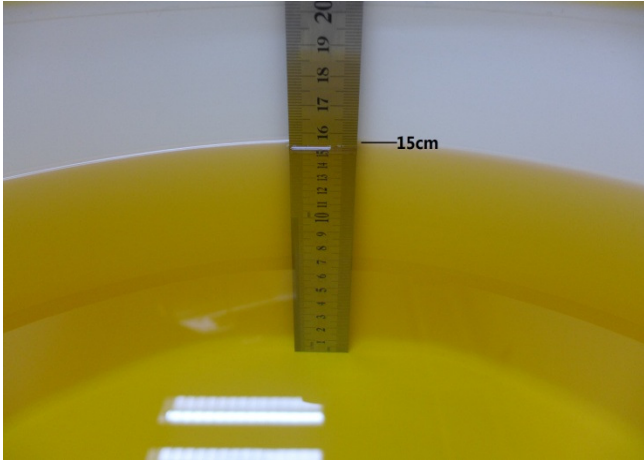
## **Photographs**

|  |
|--|
| 1. SAR measurement System                |
| 2. Photographs of Tissue Simulate Liquid |
| 3. Photographs of EUT test position      |
| 4. EUT Constructional Details            |

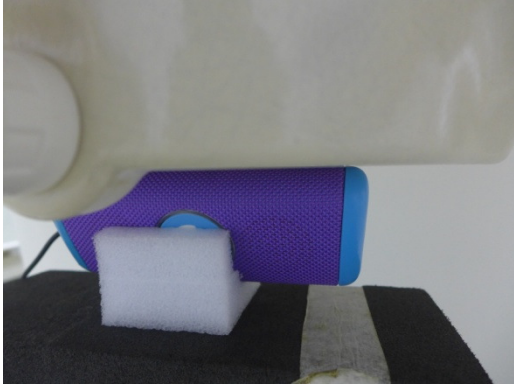
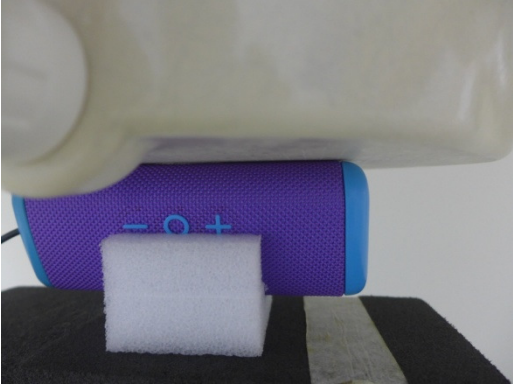
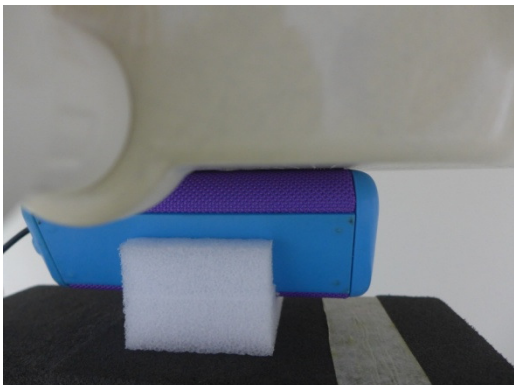

## 1. SAR measurement System



## 2. Photographs of Tissue Simulate Liquid

| Photo 1: Tissue Simulant Liquid for Body 2450                                     | N/A |
|---|-----|
|  | N/A |

### 3. Photographs of EUT test position

| Photo 2: Side 1  | Photo 3: Side 2   |
|--|---|
|  A photograph showing the left side of a purple and blue EUT. The device is resting on a white foam block on a black and white striped surface. A white plastic component is visible above the device.      |  A photograph showing the right side of the purple and blue EUT. The device is resting on a white foam block on a black and white striped surface. A white plastic component is visible above the device. The text "- 0 +" is visible on the purple part of the device. |
| Photo 4: Side 3  | Photo 5: Side 4   |
|  A photograph showing the front side of the purple and blue EUT. The device is resting on a white foam block on a black and white striped surface. A white plastic component is visible above the device. |  A photograph showing the back side of the purple and blue EUT. The device is resting on a white foam block on a black and white striped surface. A white plastic component is visible above the device.  |

## 4. EUT Constructional Details

Photo 6: Front View

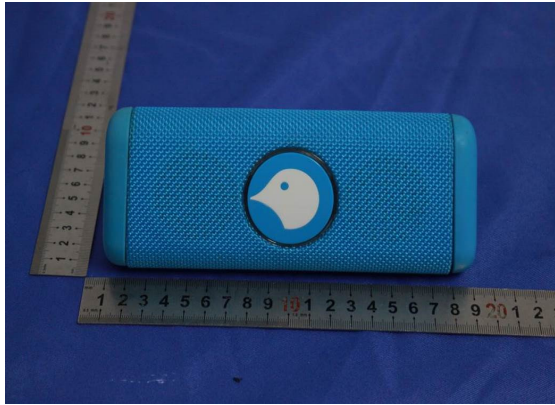


Photo 7: Back View



Photo 8: Bottom View

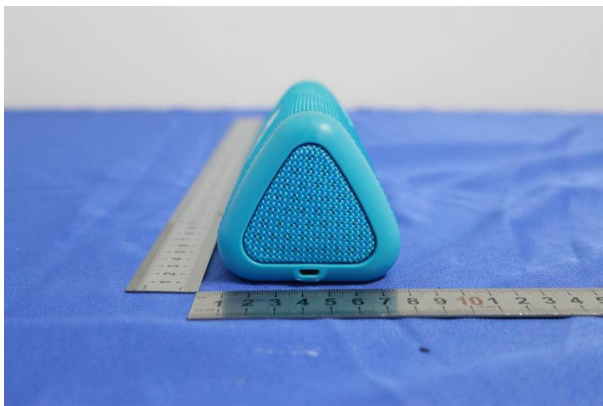


Photo 9: Up View

