

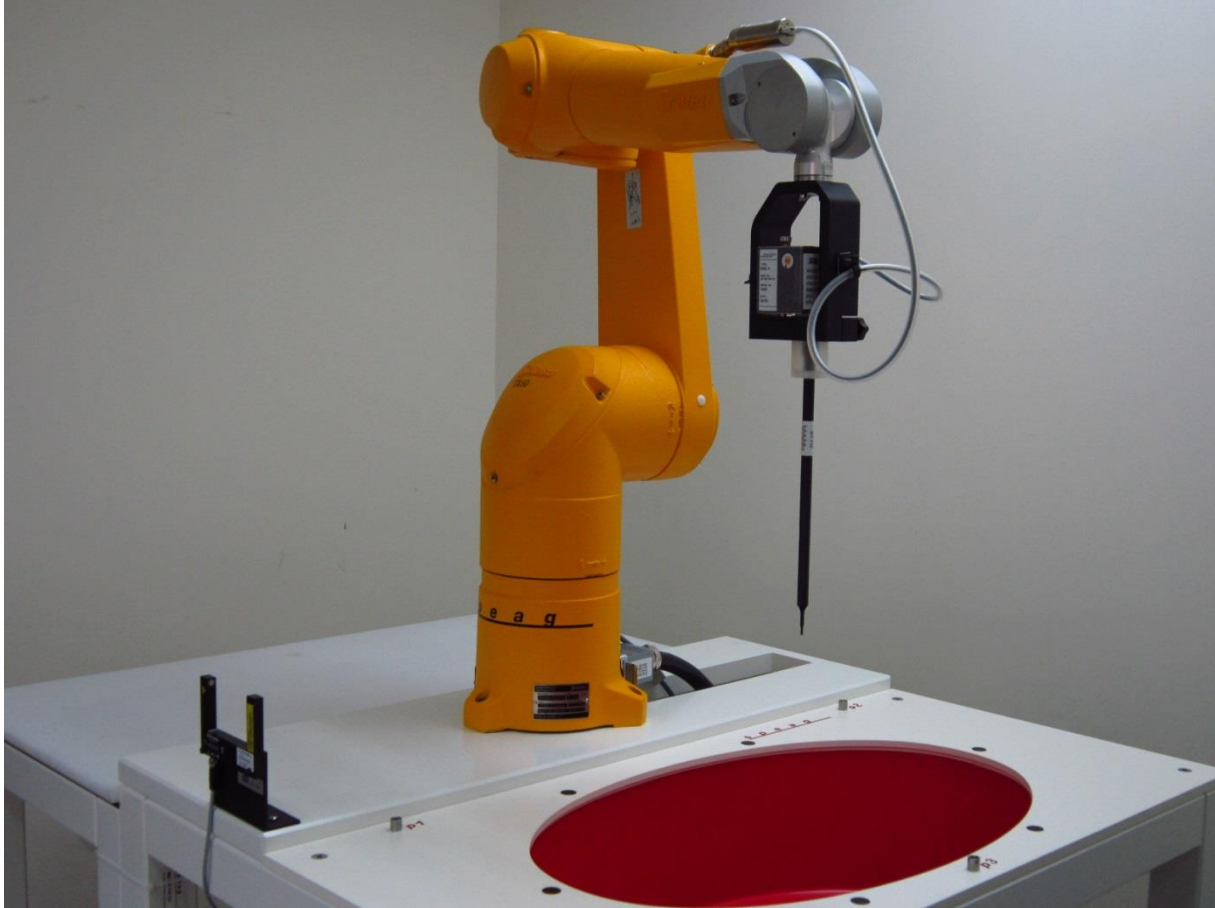


Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

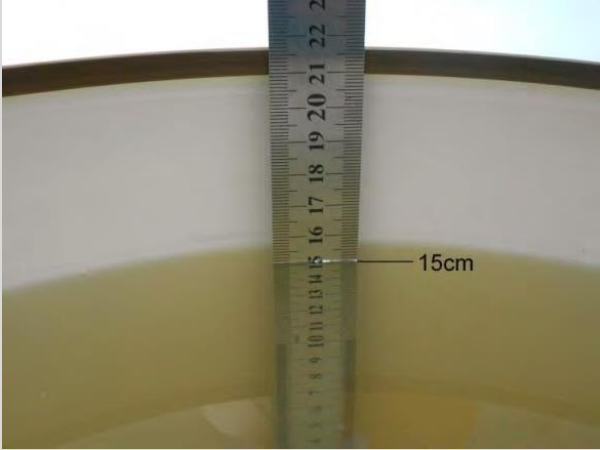
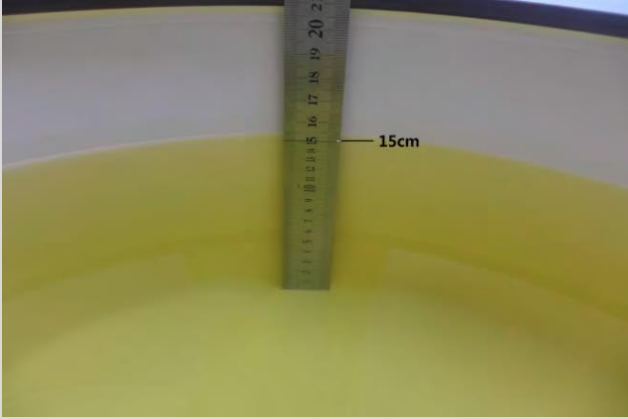
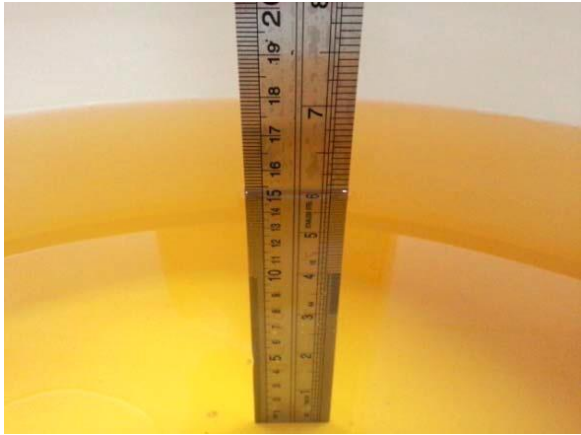
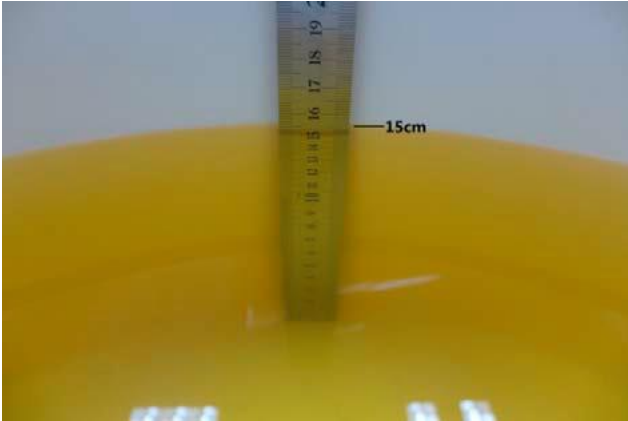

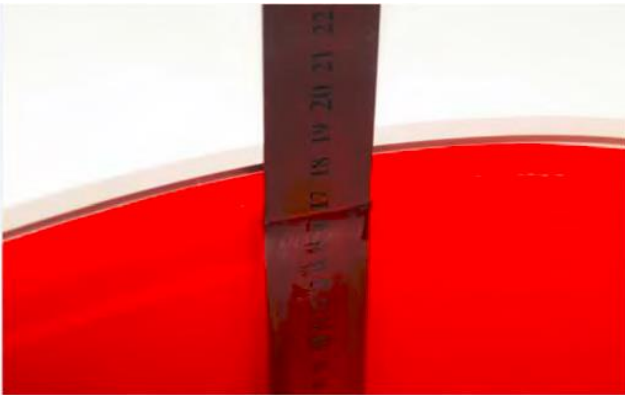
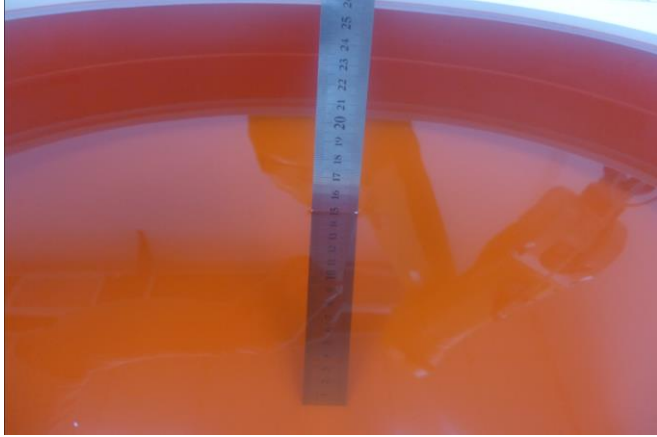
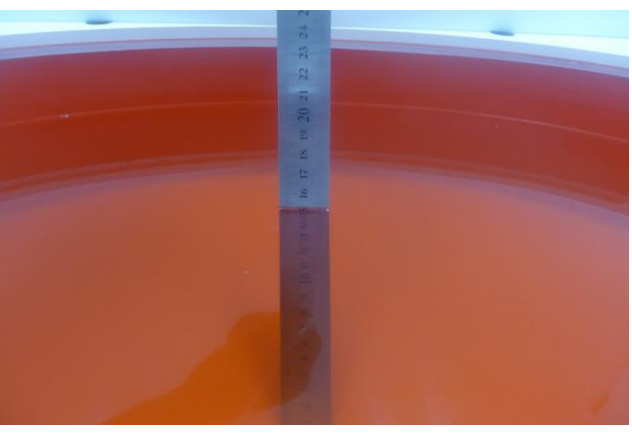
<p>Photo 1: Tissue Simulant Liquid for Head 750</p>	<p>Photo 2: Tissue Simulant Liquid for Body 750</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 1750</p>	<p>Photo 4: Tissue Simulant Liquid for Body 1750</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 2450</p>	<p>Photo 6: Tissue Simulant Liquid for Body 2450</p>
	

Photo 7: Tissue Simulant Liquid for Head 5G	Photo 8: Tissue Simulant Liquid for Body 5G
	

3. Photographs of EUT test position






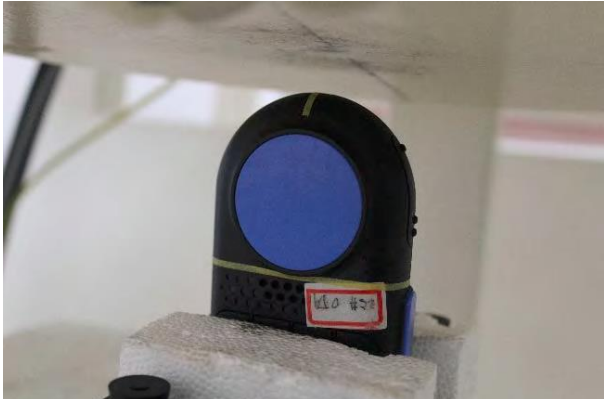
<p>Photo 9: Front side 10mm</p>	<p>Photo 10: Back side 10mm</p>
	
<p>Photo 11: Left side 10mm</p>	<p>Photo 12: Right side 10mm</p>
	
<p>Photo 13: Top side 10mm</p>	<p>Photo 14: Bottom side 10mm</p>
	

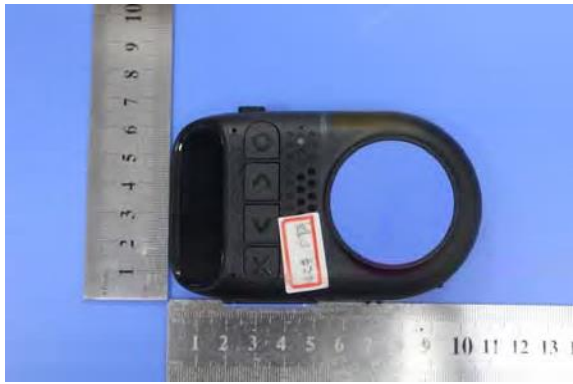

Photo 15: Front side 25mm



Photo 16: Back side 0mm with Back Splint



4. EUT Constructional Details

Photo 17: Front View	Photo 18: Back View
	
Photo 19: Front View with Front Splint	Photo 20: Front View with Front Splint
