

10591- AAA	IEEE 802.11n (HT Mixed, 20MHz, MCS0, 90pc duty cycle)	X	4.75	66.52	16.35	0.46	130.0	±9.6 %
		Y	4.81	66.52	16.40		130.0	
		Z	4.78	66.51	16.34		130.0	
10592- AAA	IEEE 802.11n (HT Mixed, 20MHz, MCS1, 90pc duty cycle)	X	4.89	66.84	16.48	0.46	130.0	± 9.6 %
		Y	4.97	66.86	16.53		130.0	
		Z	4.93	66.84	16.47		130.0	
10593- AAA	IEEE 802.11n (HT Mixed, 20MHz, MCS2, 90pc duty cycle)	X	4.81	66.73	16.35	0.46	130.0	± 9.6 %
	2 W L L L L L L L L L L L L L L L L L L	Y	4.89	66.77	16.41		130.0	
	NIS	Z	4.85	66.73	16.34		130.0	
10594- AAA	IEEE 802.11n (HT Mixed, 20MHz, MCS3, 90pc duty cycle)	X	4.86	66.91	16.51	0.46	130.0	± 9.6 %
		Y	4.94	66.93	16.56		130.0	
		Z	4.90	66.91	16.50		130.0	
10595- AAA	IEEE 802.11n (HT Mixed, 20MHz, MCS4, 90pc duty cycle)	x	4.83	66.85	16.40	0.46	130.0	±9.6 %
		Y	4.91	66.88	16.46		130.0	
		Z	4.87	66.85	16.39		130.0	1.2.1.1
10596- AAA	IEEE 802.11n (HT Mixed, 20MHz, MCS5, 90pc duty cycle)	X	4.76	66.83	16.40	0.46	130.0	± 9.6 %
		Y	4.85	66.87	16.46		130.0	
		Z	4.80	66.83	16.38		130.0	
10597- AAA	IEEE 802.11n (HT Mixed, 20MHz, MCS6, 90pc duty cycle)	X	4.71	66.72	16.27	0.46	130.0	± 9.6 %
		Y	4.79	66.78	16.35		130.0	
		Z	4.75	66.73	16.26	and the second second	130.0	
10598- IEEE 802.11n (HT Mixed, 20MHz, AAA MCS7, 90pc duty cycle)		X	4.70	66.97	16.55	0.46	130.0	± 9.6 %
		Y	4.78	67.01	16.60	-	130.0	
		Z	4.74	66.98	16.54		130.0	
10599- AAA IEEE 802.11n (HT Mixed, 40MHz, MCS0, 90pc duty cycle)	X	5.41	67.02	16.56	0.46	130.0	± 9.6 %	
		Y	5.48	67.08	16.61		130.0	
		Z	5.45	67.06	16.56		130.0	
10600- AAA	IEEE 802.11n (HT Mixed, 40MHz, MCS1, 90pc duty cycle)	X	5.53	67.40	16.73	0.46	130.0	± 9.6 %
	0.066	Y	5.61	67.47	16.78		130.0	
		Z	5.56	67.40	16.70		130.0	
10601- AAA	IEEE 802.11n (HT Mixed, 40MHz, MCS2, 90pc duty cycle)	X	5.43	67.18	16.64	0.46	130.0	± 9.6 %
		Y	5.50	67.24	16.68		130.0	
	17.030 C 10 C 10 B B 10 C 10 K 20 C	Z	5.46	67.19	16.61		130.0	
10602- AAA	IEEE 802.11n (HT Mixed, 40MHz, MCS3, 90pc duty cycle)	X	5.54	67.27	16.59	0.46	130.0	± 9.6 %
		Y	5.59	67.24	16.60		130.0	
	100 I I I I I I I I I I I I I I I I I I	Z	5.55	67.21	16.54		130.0	
10603- AAA	IEEE 802.11n (HT Mixed, 40MHz, MCS4, 90pc duty cycle)	х	5.60	67.54	16.87	0.46	130.0	± 9.6 %
		Y	5.68	67.57	16.90		130.0	
		Z	5.63	67.52	16.83		130.0	
10604- AAA	IEEE 802.11n (HT Mixed, 40MHz, MCS5, 90pc duty cycle)	X	5.46	67.15	16.66	0.46	130.0	± 9.6 %
	All the second se	Y	5.48	67.04	16.62		130.0	
		Z	5.46	67.05	16.58		130.0	
10605- AAA	IEEE 802.11n (HT Mixed, 40MHz, MCS6, 90pc duty cycle)	X	5.53	67.33	16.74	0.46	130.0	± 9.6 %
	Land Land Land Land Land Land Land Land	Y	5.59	67.35	16.77		130.0	
		Z	5.55	67.31	16.70		130.0	
10606- AAA	IEEE 802.11n (HT Mixed, 40MHz, MCS7, 90pc duty cycle)	X	5.26	66.63	16.24	0.46	130.0	± 9.6 %
		Y	5.35	66.76	16.34		130.0	

EX3DV4- SN:3759

December 16, 2016

Certificate No: EX3-3759_Dec16

Page 35 of 38



10607- AAA	IEEE 802.11ac WiFi (20MHz, MCS0, 90pc duty cycle)	X	4.58	65.82	15.97	0.46	130.0	±9.6 %
		Y	4.64	65.82	16.01		130.0	
		Z	4.61	65.80	15.95		130.0	
10608- AAA	IEEE 802.11ac WiFi (20MHz, MCS1, 90pc duty cycle)	X	4.75	66.20	16.13	0.46	130.0	±9.6 %
		Y	4.83	66.22	16.18		130.0	-
		Z	4.79	66.19	16.11		130.0	
10609- AAA	IEEE 802.11ac WiFi (20MHz, MCS2, 90pc duty cycle)	X	4.64	66.03	15.95	0.46	130.0	±9.6 %
		Y	4.72	66.07	16.02		130.0	
		Z	4.68	66.02	15.94		130.0	
10610- AAA	IEEE 802.11ac WiFi (20MHz, MCS3. 90pc duty cycle)	X	4.69	66.20	16.12	0.46	130.0	±9.6 %
	Superior The Second Second	Y	4.77	66.23	16.17		130.0	
		Z	4.73	66.19	16.11		130.0	
10611- AAA	IEEE 802.11ac WiFi (20MHz, MCS4, 90pc duty cycle)	X	4.61	65.99	15.96	0.46	130.0	± 9.6 %
		Y	4.69	66.03	16.02		130.0	
		Z	4.64	65.99	15.95		130.0	
10612- AAA	IEEE 802.11ac WiFi (20MHz, MCS5, 90pc duty cycle)	X	4.61	66.12	16.00	0.46	130.0	±9.6 %
		Y	4.70	66.18	16.06		130.0	-
	NY STATES AND A STATES	Z	4.65	66.12	15.98		130.0	
10613- AAA	IEEE 802.11ac WiFi (20MHz, MCS6, 90pc duty cycle)	X	4.61	65.99	15.87	0.46	130.0	±9.6 %
		Y	4.70	66.08	15.96		130.0	
	1.55	Z	4.65	66.00	15.86		130.0	
10614- AAA	IEEE 802.11ac WiFi (20MHz, MCS7, 90pc duty cycle)	X	4.56	66.21	16.12	0.46	130.0	±9.6 %
		Y	4.64	66.25	16.18		130.0	
		Z	4.60	66.21	16.11		130.0	
10615- AAA	IEEE 802.11ac WiFi (20MHz, MCS8, 90pc duty cycle)	X	4.60	65.81	15.72	0.46	130.0	±9.6 %
		Y	4.69	65.87	15.81		130.0	
		Z	4.64	65.79	15.71		130.0	
10616- AAA	IEEE 802.11ac WiFi (40MHz, MCS0, 90pc duty cycle)	x	5.23	66.28	16.18	0.46	130.0	±9.6 %
		Y	5.29	66.33	16.22		130.0	
		Z	5.26	66.29	16.17		130.0	
10617- AAA	IEEE 802.11ac WiFi (40MHz, MCS1, 90pc duty cycle)	X	5.29	66.46	16.24	0.46	130.0	± 9.6 %
		Y	5.36	66.48	16.27		130.0	
		Z	5.32	66.45	16.21		130.0	
10618- AAA	IEEE 802.11ac WiFi (40MHz, MCS2, 90pc duty cycle)	X	5.18	66.47	16.26	0.46	130.0	± 9.6 %
7		Y	5.24	66.50	16.29		130.0	
	20065	Z	5.21	66.46	16.24		130.0	
10619- AAA	IEEE 802.11ac WiFi (40MHz, MCS3, 90pc duty cycle)	X	5.19	66.25	16.09	0.46	130.0	± 9.6 %
	West of the second s	Y	5.26	66.32	16.14		130.0	
		Z	5.22	66.26	16.07		130.0	
10620- AAA	IEEE 802.11ac WiFi (40MHz, MCS4, 90pc duty cycle)	X	5.28	66.29	16.16	0.46	130.0	±9.6 %
		Y	5.36	66.37	16.22		130.0	
		Z	5.31	66.31	16.14		130.0	
10621- AAA	IEEE 802.11ac WiFi (40MHz, MCS5, 90pc duty cycle)	×	5.29	66.47	16.37	0.46	130.0	± 9.6 %
		Y	5.35	66.48	16.39		130.0	
	A LONG TO A LONG THE CONSTRUCT OF	Z	5.32	66.47	16.35		130.0	
10622- AAA	IEEE 802.11ac WiFi (40MHz, MCS6, 90pc duty cycle)	X	5.30	66.62	16.44	0.46	130.0	± 9.6 %
		_			10.10		100.0	
	A REAL TO BE REAL AND A REAL AND A REAL AND A	Y	5.36	66.63	16.45		130.0	

EX3DV4- SN:3759

December 16, 2016

Certificate No: EX3-3759_Dec16

Page 36 of 38



10623- AAA	IEEE 802.11ac WiFi (40MHz, MCS7, 90pc duty cycle)	X	5.18	66.12	16.05	0.46	130.0	±9.6 %
		Y	5.24	66.18	16.11		130.0	
	A ZER CONTRACTOR OF STATES	Z	5.21	66.13	16.03		130.0	
10624- AAA	IEEE 802.11ac WiFi (40MHz, MCS8, 90pc duty cycle)	X	5.37	66.33	16.23	0.46	130.0	± 9.6 %
		Y	5.43	66.38	16.27		130.0	
		Z	5.40	66.34	16.21	7.1.1.1	130.0	
10625- AAA	IEEE 802.11ac WiFi (40MHz, MCS9, 90pc duty cycle)	X	5.66	67.10	16.66	0.46	130.0	± 9.6 %
		Y	5.80	67.35	16.80		130.0	
		Z	5.73	67.22	16.70		130.0	
10626- AAA	IEEE 802.11ac WiFi (80MHz, MCS0, 90pc duty cycle)	×	5.54	66.36	16.15	0.46	130.0	± 9.6 %
		Y	5.58	66.40	16.18		130.0	1
		Z	5.56	66.37	16.13		130.0	
10627- AAA	IEEE 802.11ac WiFi (80MHz, MCS1, 90pc duty cycle)	X	5.76	66.90	16.39	0.46	130.0	± 9.6 %
		Y	5.82	66.93	16.41		130.0	
3		Z	5.78	66.89	16.35		130.0	
10628- AAA	IEEE 802.11ac WiFi (80MHz, MCS2, 90pc duty cycle)	X	5.55	66.39	16.06	0.46	130.0	± 9.6 %
		Y	5.62	66.51	16.13		130.0	
		Z	5.58	66.43	16.05		130.0	
10629- AAA	IEEE 802.11ac WiFi (80MHz, MCS3, 90pc duty cycle)	X	5.63	66.46	16.09	0.46	130.0	± 9.6 %
		Y	5.71	66.59	16.17		130.0	
		Z	5.65	66.47	16.07		130.0	
10630- AAA	IEEE 802.11ac WiFi (80MHz, MCS4, 90pc duty cycle)	X	5.98	67.71	16.72	0.46	130.0	± 9.6 %
		Y	6.12	68.01	16.88		130.0	
	A AND THE REPORT OF A DESCRIPTION OF A D	Z	6.03	67.80	16.73	2.2	130.0	
10631- AAA	IEEE 802.11ac WiFi (80MHz, MCS5, 90pc duty cycle)	X	5.93	67.68	16.90	0.46	130.0	± 9.6 %
		Y	6.03	67.84	16.98		130.0	
		Z	5.98	67.75	16.91		130.0	
10632- AAA	IEEE 802.11ac WiFi (80MHz, MCS6, 90pc duty cycle)	X	5.74	67.01	16.58	0.46	130.0	± 9.6 %
		Y	5.79	67.00	16.58		130.0	
		Z	5.76	66.99	16.55		130.0	
10633- AAA	IEEE 802.11ac WiFi (80MHz, MCS7, 90pc duty cycle)	X	5.62	66.59	16.20	0.46	130.0	± 9.6 %
		Y	5.68	66.67	16.24		130.0	
		Z	5.65	66.62	16.18		130.0	
10634- AAA	IEEE 802.11ac WiFi (80MHz, MCS8, 90pc duty cycle)	Х	5.60	66.63	16.28	0.46	130.0	± 9.6 %
		Y	5.67	66.70	16.32		130.0	
		Z	5.64	66.66	16.27		130.0	
10635- AAA	IEEE 802.11ac WiFi (80MHz, MCS9, 90pc duty cycle)	X	5.47	65.91	15.63	0.46	130.0	± 9.6 %
		Y	5.56	66.05	15.73		130.0	
		Z	5.51	65.94	15.62		130.0	
10636- AAA	IEEE 1602.11ac WiFi (160MHz, MCS0, 90pc duty cycle)	X	5.95	66.72	16.24	0.46	130.0	± 9.6 %
1 S		Y	5.99	66.78	16.28		130.0	
1000-		Z	5.97	66.73	16.22		130.0	
10637- AAA	IEEE 1602.11ac WiFi (160MHz, MCS1, 90pc duty cycle)	x	6.10	67.09	16.41	0.46	130.0	± 9.6 %
		Y	6.14	67.14	16.44		130.0	
		Z	6.11	67.09	16.38	11	130.0	
10638- AAA	IEEE 1602.11ac WiFi (160MHz, MCS2, 90pc duty cycle)	X	6.10	67.06	16.37	0.46	130.0	± 9.6 %
_		Y	6.15	67.12	16.41		130.0	
		Z	6.12	67.07	16.35		130.0	

EX3DV4- SN:3759

December 16, 2016

Certificate No: EX3-3759_Dec16

Page 37 of 38



December 16, 2016

10639- AAA	IEEE 1602.11ac WiFi (160MHz, MCS3, 90pc duty cycle)	X	6.07	67.01	16.39	0.46	130.0	±9.6 %
		Y	6.13	67.09	16.44	-	130.0	
		Z	6.10	67.03	16.38		130.0	
10640- AAA	IEEE 1602.11ac WiFi (160MHz, MCS4, 90pc duty cycle)	X	6.07	66.99	16.32	0.46	130.0	±9.6 %
		Y	6.14	67.11	16.39		130.0	
		Z	6.09	67.02	16.31		130.0	
10641- AAA	IEEE 1602.11ac WiFi (160MHz, MCS5, 90pc duty cycle)	X	6.13	66.94	16.31	0.46	130.0	±9.6 %
		Y	6.17	66.99	16.35		130.0	
		Z	6.14	66.93	16.28		130.0	
10642- AAA 90pc duty cycle)	X	6.17	67.20	16.62	0.46	130.0	±9.6 %	
		Y	6.22	67.26	16.65		130.0	
		Z	6.19	67.22	16.61		130.0	
10643- IEEE 1602.11ac WiFi (160MHz, MCS7, AAA 90pc duty cycle)	X	6.00	66.86	16.34	0.46	130.0	±9.6 %	
		Y	6.05	66.94	16.39		130.0	
		Z	6.02	66.87	16.31		130.0	
10644- AAA	IEEE 1602.11ac WiFi (160MHz, MCS8, 90pc duty cycle)	X	6.13	67.25	16.56	0.46	130.0	±9.6 %
		Y	6.22	67.46	16.67		130.0	
		Z	6.17	67.33	16.57		130.0	
10645- AAA	IEEE 1602.11ac WiFi (160MHz, MCS9, 90pc duty cycle)	X	6.30	67.39	16.59	0.46	130.0	±9.6 %
		Y	6.61	68.18	16.99		130.0	
		Z	6.44	67.75	16.73		130.0	
10646- AAC	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL Subframe=2,7)	X	11.76	96.35	31.88	9.30	60.0	±9.6 %
		Y	19.05	107.46	35.85		60.0	
		Z	11.88	94.80	30.95		60.0	
10647- AAB	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Subframe=2,7)	X	10.62	94.79	31.49	9.30	60.0	±9.6 %
		Y	16.98	105.61	35.43		60.0	
		Z	10.96	93.72	30.71		60.0	
10648- AAA	CDMA2000 (1x Advanced)	X	0.66	63.03	10.35	0.00	150.0	±9.6 %
		Y	0.70	63.32	10.86		150.0	
		Z	0.69	63.19	10.65		150.0	-

EX3DV4- SN:3759

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Certificate No: EX3-3759_Dec16

Page 38 of 38



ANNEX B

DIPOLE CALIBRATION REPORTS

COMMERCIAL-IN-CONFIDENCE



ccredited by the Swiss Accreditat the Swiss Accreditation Service	is one of the signatories	to the EA	creditation No.: SCS 0108
ultilateral Agreement for the re	cognition of calibration of		D450V2 1004 Dee16
lient TÜV SÜD UK		Certificate No	: D450V3-1094_Dec16
ALIBRATION C	ERTIFICATE		
Dbject	D450V3 - SN: 109	94	
Calibration procedure(s)	QA CAL-15.v8		
	Calibration procee	dure for dipole validation kits belo	ow 700 MHz
Calibration date:	December 08, 20	16	
		onal standards, which realize the physical un	
The measurements and the unce	rtainties with confidence pr	obability are given on the following pages an	d are part of the certificate.
		, , , ,	
		y facility: environment temperature (22 ± 3)°(
All calibrations have been conduc	ted in the closed laborator		
All calibrations have been conduc	ted in the closed laborator		
All calibrations have been conduc Calibration Equipment used (M&1	ted in the closed laborator		
All calibrations have been conduc Calibration Equipment used (M&1 Primary Standards	cted in the closed laborator	y facility: environment temperature (22 \pm 3)°C	C and humidity < 70%.
All calibrations have been conduc Calibration Equipment used (M&1 Primary Standards Power meter NRP	ted in the closed laborator I'E critical for calibration)	y facility: environment temperature (22 ± 3)°0 Cal Date (Certificate No.)	C and humidity < 70%. Scheduled Calibration Apr-17 Apr-17
All calibrations have been conduc Calibration Equipment used (M&1 Primary Standards Power meter NRP Power sensor NRP-Z91	ted in the closed laborator IE critical for calibration) ID # SN: 104778	y facility: environment temperature (22 ± 3)°0 Cal Date (Certificate No.) 06-Apr-16 (No. 217-02288/02289)	C and humidity < 70%. Scheduled Calibration Apr-17
All calibrations have been conduc Calibration Equipment used (M&1 Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91	ted in the closed laborator IE critical for calibration) ID # SN: 104778 SN: 103244	y facility: environment temperature (22 ± 3)°0 <u>Cal Date (Certificate No.)</u> 06-Apr-16 (No. 217-02288/02289) 06-Apr-16 (No. 217-02288)	C and humidity < 70%. Scheduled Calibration Apr-17 Apr-17
All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator	ted in the closed laborator IC critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245	y facility: environment temperature (22 ± 3)°0 Cal Date (Certificate No.) 06-Apr-16 (No. 217-02288/02289) 06-Apr-16 (No. 217-02288) 06-Apr-16 (No. 217-02289)	C and humidity < 70%. Scheduled Calibration Apr-17 Apr-17 Apr-17 Apr-17
All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Fype-N mismatch combination	ted in the closed laborator re critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 5277 (20x)	y facility: environment temperature (22 ± 3)°0 Cal Date (Certificate No.) 06-Apr-16 (No. 217-02288/02289) 06-Apr-16 (No. 217-02288) 06-Apr-16 (No. 217-02289) 05-Apr-16 (No. 217-02293)	C and humidity < 70%. Scheduled Calibration Apr-17 Apr-17 Apr-17 Apr-17 Apr-17
All calibrations have been conduc Calibration Equipment used (M&1 Primary Standards Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ET3DV6	ted in the closed laborator TE critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 5277 (20x) SN: 5047.2 / 06327	Cal Date (Certificate No.) 06-Apr-16 (No. 217-02288/02289) 06-Apr-16 (No. 217-02288) 06-Apr-16 (No. 217-02289) 05-Apr-16 (No. 217-02293) 05-Apr-16 (No. 217-02293) 05-Apr-16 (No. 217-02293)	C and humidity < 70%. Scheduled Calibration Apr-17 Apr-17 Apr-17 Apr-17 Apr-17 Apr-17
All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Fype-N mismatch combination Reference Probe ET3DV6 DAE4	ted in the closed laborator TE critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 5277 (20x) SN: 5047.2 / 06327 SN: 1507	y facility: environment temperature (22 ± 3)°0 Cal Date (Certificate No.) 06-Apr-16 (No. 217-02288/02289) 06-Apr-16 (No. 217-02288) 06-Apr-16 (No. 217-02289) 05-Apr-16 (No. 217-02293) 05-Apr-16 (No. 217-02295) 31-Dec-15 (No. ET3-1507_Dec15)	C and humidity < 70%. Scheduled Calibration Apr-17 Apr-17 Apr-17 Apr-17 Apr-17 Dec-16
All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Fype-N mismatch combination Reference Probe ET3DV6 DAE4 Secondary Standards	ID # SN: 104778 SN: 103244 SN: 103245 SN: 5277 (20x) SN: 5047.2 / 06327 SN: 1507 SN: 654	y facility: environment temperature (22 ± 3)°0 Cal Date (Certificate No.) 06-Apr-16 (No. 217-02288/02289) 06-Apr-16 (No. 217-02289) 05-Apr-16 (No. 217-02293) 05-Apr-16 (No. 217-02293) 05-Apr-16 (No. 217-02295) 31-Dec-15 (No. ET3-1507_Dec15) 12-Aug-16 (No. DAE4-654_Aug16)	C and humidity < 70%. Scheduled Calibration Apr-17 Apr-17 Apr-17 Apr-17 Apr-17 Dec-16 Aug-17
All calibrations have been conduct Calibration Equipment used (M&T Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Fype-N mismatch combination Reference Probe ET3DV6 DAE4 Secondary Standards Power meter E4419B	ted in the closed laborator TE critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 5277 (20x) SN: 5047.2 / 06327 SN: 654 ID #	y facility: environment temperature (22 ± 3)°0 Cal Date (Certificate No.) 06-Apr-16 (No. 217-02288/02289) 06-Apr-16 (No. 217-02289) 05-Apr-16 (No. 217-02293) 05-Apr-16 (No. 217-02293) 05-Apr-16 (No. 217-02295) 31-Dec-15 (No. E13-1507_Dec15) 12-Aug-16 (No. DAE4-654_Aug16) Check Date (in house)	C and humidity < 70%. Scheduled Calibration Apr-17 Apr-17 Apr-17 Apr-17 Apr-17 Apr-17 Dec-16 Aug-17 Scheduled Check
All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ET3DV6 DAE4 Secondary Standards Power meter E4419B Power sensor E4412A	ted in the closed laborator TE critical for calibration) ID # SN: 104778 SN: 103244 SN: 103244 SN: 103245 SN: 5277 (20x) SN: 5047.2 / 06327 SN: 507 SN: 654 ID # SN: GB41293874	y facility: environment temperature (22 ± 3)°0 Cal Date (Certificate No.) 06-Apr-16 (No. 217-02288/02289) 06-Apr-16 (No. 217-02289) 05-Apr-16 (No. 217-02293) 05-Apr-16 (No. 217-02295) 31-Dec-15 (No. E13-1507_Dec15) 12-Aug-16 (No. DAE4-654_Aug16) Check Date (in house) 06-Apr-16 (No. 217-02285/02284)	C and humidity < 70%. Scheduled Calibration Apr-17 Apr-17 Apr-17 Apr-17 Apr-17 Apr-17 Dec-16 Aug-17 Scheduled Check In house check: Jun-18
All calibrations have been conduct Calibration Equipment used (M&T Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Fype-N mismatch combination Reference Probe ET3DV6 DAE4 Secondary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A	ted in the closed laborator TE critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 5277 (20x) SN: 5047.2 / 06327 SN: 554 ID # SN: GB41293874 SN: MY41498087	Cal Date (Certificate No.) 06-Apr-16 (No. 217-02288/02289) 06-Apr-16 (No. 217-02288) 06-Apr-16 (No. 217-02289) 05-Apr-16 (No. 217-02293) 05-Apr-16 (No. 217-02295) 31-Dec-15 (No. ET3-1507_Dec15) 12-Aug-16 (No. 217-02285/02284) 06-Apr-16 (No. 217-02285/02284) 06-Apr-16 (No. 217-02285)	C and humidity < 70%. Scheduled Calibration Apr-17 Apr-17 Apr-17 Apr-17 Apr-17 Apr-17 Dec-16 Aug-17 Scheduled Check In house check; Jun-18 In house check; Jun-18
All calibrations have been conduct Calibration Equipment used (M&T Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Fype-N mismatch combination Reference Probe ET3DV6 DAE4 Secondary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A RF generator HP 8648C	ted in the closed laborator TE critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 5277 (20x) SN: 5047.2 / 06327 SN: 507 SN: 654 ID # SN: GB41293874 SN: MY41498087 SN: 000110210	Cal Date (Certificate No.) 06-Apr-16 (No. 217-02288/02289) 06-Apr-16 (No. 217-02288) 06-Apr-16 (No. 217-02289) 05-Apr-16 (No. 217-02293) 05-Apr-16 (No. 217-02295) 31-Dec-15 (No. ET3-1507_Dec15) 12-Aug-16 (No. 217-02285/02284) 06-Apr-16 (No. 217-02285/02284) 06-Apr-16 (No. 217-02285)	C and humidity < 70%. Scheduled Calibration Apr-17 Apr-17 Apr-17 Apr-17 Apr-17 Apr-17 Dec-16 Aug-17 Scheduled Check In house check: Jun-18 In house check: Jun-18 In house check: Jun-18
All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ET3DV6 DAE4 Secondary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A RF generator HP 8648C	ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: 5277 (20x) SN: 5047.2 / 06327 SN: 654 ID # SN: 6841293874 SN: WY41498087 SN: 000110210 SN: US3642U01700	Cal Date (Certificate No.) 06-Apr-16 (No. 217-02288/02289) 06-Apr-16 (No. 217-02288) 06-Apr-16 (No. 217-02283) 05-Apr-16 (No. 217-02293) 05-Apr-16 (No. 217-02293) 05-Apr-16 (No. 217-02295) 31-Dec-15 (No. ET3-1507_Dec15) 12-Aug-16 (No. DAE4-654_Aug16) Check Date (in house) 06-Apr-16 (No. 217-02285/02284) 06-Apr-16 (No. 217-02284) 06-Apr-16 (No. 217-02284)	C and humidity < 70%. Scheduled Calibration Apr-17 Apr-17 Apr-17 Apr-17 Apr-17 Dec-16 Aug-17 Scheduled Check In house check: Jun-18 In house check: Jun-18
All calibrations have been conduct Calibration Equipment used (M&1 Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ET3DV6 DAE4 Secondary Standards Power meter E4419B Power sensor E4412A RF generator HP 8648C Network Analyzer HP 8753E	ted in the closed laborator FE critical for calibration) ID # SN: 104778 SN: 103244 SN: 503245 SN: 5277 (20x) SN: 5047.2 / 06327 SN: 654 ID # SN: GB41293874 SN: GB41293874 SN: MY41498087 SN: 000110210 SN: US3642U01700 SN: US37390585	Cal Date (Certificate No.) 06-Apr-16 (No. 217-02288/02289) 06-Apr-16 (No. 217-02288) 06-Apr-16 (No. 217-02289) 05-Apr-16 (No. 217-02293) 05-Apr-16 (No. 217-02293) 05-Apr-16 (No. 217-02295) 31-Dec-15 (No. ET3-1507_Dec15) 12-Aug-16 (No. 217-02285/02284) 06-Apr-16 (No. 217-02285/02284) 06-Apr-16 (No. 217-02285/02284) 06-Apr-16 (No. 217-02285)	C and humidity < 70%. Scheduled Calibration Apr-17 Apr-17 Apr-17 Apr-17 Dec-16 Aug-17 Scheduled Check In house check: Jun-18 In house check: Jun-18
All calibrations have been conduct Calibration Equipment used (M&1 Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ET3DV6 DAE4 Secondary Standards Power sensor E4419B Power sensor E4412A Power sensor E4412A RF generator HP 8648C Network Analyzer HP 8753E	ted in the closed laborator FE critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 5277 (20x) SN: 5047.2 / 06327 SN: 654 ID # SN: GB41293874 SN: MY41498087 SN: 000110210 SN: US3642U01700 SN: US37390585 Name	Cal Date (Certificate No.) 06-Apr-16 (No. 217-02288/02289) 06-Apr-16 (No. 217-02288) 06-Apr-16 (No. 217-02289) 05-Apr-16 (No. 217-02293) 05-Apr-16 (No. 217-02295) 31-Dec-15 (No. ET3-1507_Dec15) 12-Aug-16 (No. 217-02285/02284) 06-Apr-16 (No. 217-02285) 06-Apr-16 (No. 217-02285) 06-Apr-16 (No. 217-02285/02284) 06-Apr-16 (No. 217-02285) 06-Apr-16 (No. 217-02284) 04-Aug-99 (in house check Jun-16) 18-Oct-01 (in house check Oct-16)	C and humidity < 70%. Scheduled Calibration Apr-17 Apr-17 Apr-17 Apr-17 Dec-16 Aug-17 Scheduled Check In house check: Jun-18 In house check: Jun-18
	ted in the closed laborator FE critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 5277 (20x) SN: 5047.2 / 06327 SN: 654 ID # SN: GB41293874 SN: MY41498087 SN: 000110210 SN: US3642U01700 SN: US37390585 Name	Cal Date (Certificate No.) 06-Apr-16 (No. 217-02288/02289) 06-Apr-16 (No. 217-02288) 06-Apr-16 (No. 217-02289) 05-Apr-16 (No. 217-02293) 05-Apr-16 (No. 217-02295) 31-Dec-15 (No. ET3-1507_Dec15) 12-Aug-16 (No. 217-02285/02284) 06-Apr-16 (No. 217-02285) 06-Apr-16 (No. 217-02285) 06-Apr-16 (No. 217-02285/02284) 06-Apr-16 (No. 217-02285) 06-Apr-16 (No. 217-02284) 04-Aug-99 (in house check Jun-16) 18-Oct-01 (in house check Oct-16)	C and humidity < 70%. Scheduled Calibration Apr-17 Apr-17 Apr-17 Apr-17 Dec-16 Aug-17 Scheduled Check In house check: Jun-18 In house check: Jun-18

Certificate No: D450V3-1094_Dec16

Page 1 of 8

COMMERCIAL-IN-CONFIDENCE



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S

Schweizerischer Kalibrierdienst Service suisse d'étalonnage

C Servizio svizzero di taratura

S Swiss Calibration Service

Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D450V3-1094_Dec16

Page 2 of 8



Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	ELI4 Flat Phantom	Shell thickness: 2 ± 0.2 mm
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	43.5	0.87 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	43.4 ± 6 %	0.87 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	and the state of the second
SAR measured	250 mW input power	1.11 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	4.44 W/kg ± 18.1 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR averaged over 10 cm ³ (10 g) of Head TSL SAR measured	condition 250 mW input power	0.748 W/kg

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	56.7	0.94 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	57.6 ± 6 %	0.96 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	1.18 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	4.66 W/kg ± 18.1 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	0.798 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	3.15 W/kg ± 17.6 % (k=2)

Certificate No: D450V3-1094_Dec16

Page 3 of 8



Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	60.5 Ω - 2.3 jΩ
Return Loss	- 20.2 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	57.3 Ω - 7.5 jΩ	
Return Loss	- 20.2 dB	

General Antenna Parameters and Design

Electrical Delay (one direction)	1.349 ns	
----------------------------------	----------	--

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	September 15, 2015

Certificate No: D450V3-1094_Dec16

Page 4 of 8



DASY5 Validation Report for Head TSL

Date: 08.12.2016

Test Laboratory: SPEAG, Zurich, Switzerland


DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN: 1094

Communication System: UID 0 - CW; Frequency: 450 MHz Medium parameters used: f = 450 MHz; $\sigma = 0.87$ S/m; $\epsilon_r = 43.4$; $\rho = 1000$ kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ET3DV6 SN1507; ConvF(6.58, 6.58, 6.58); Calibrated: 31.12.2015;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 12.08.2016
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Head Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 39.10 V/m; Power Drift = -0.02 dB Peak SAR (extrapolated) = 1.58 W/kg SAR(1 g) = 1.11 W/kg; SAR(10 g) = 0.748 W/kg Maximum value of SAR (measured) = 1.19 W/kg

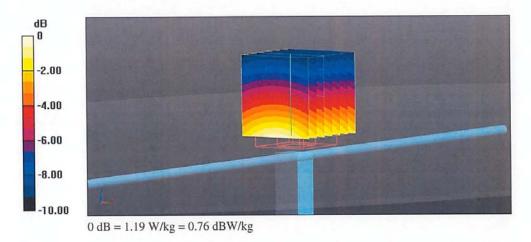


Page 5 of 8

Certificate No: D450V3-1094_Dec16



Impedance Measurement Plot for Head TSL

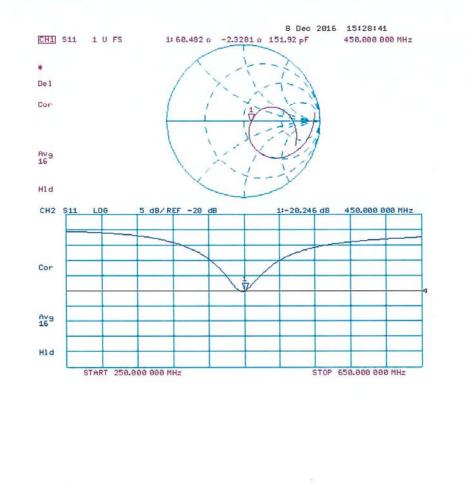

Certificate No: D450V3-1094_Dec16

Page 6 of 8



DASY5 Validation Report for Body TSL

Date: 08.12.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 450 MHz D450V3; Type: D450V3; Serial: D450V3 - SN: 1094


Communication System: UID 0 - CW; Frequency: 450 MHz Medium parameters used: f = 450 MHz; $\sigma = 0.96 \text{ S/m}$; $\varepsilon_r = 57.6$; $\rho = 1000 \text{ kg/m}^3$ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ET3DV6 SN1507; ConvF(6.99, 6.99, 6.99); Calibrated: 31.12.2015;
- Sensor-Surface: 4mm (Mechanical Surface Detection) .
- Electronics: DAE4 Sn654; Calibrated: 12.08.2016 •
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372) .

Dipole Calibration for Body Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 37.12 V/m; Power Drift = -0.01 dB Peak SAR (extrapolated) = 1.81 W/kg SAR(1 g) = 1.18 W/kg; SAR(10 g) = 0.798 W/kg Maximum value of SAR (measured) = 1.26 W/kg

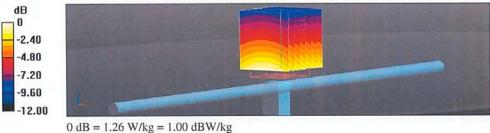


Certificate No: D450V3-1094_Dec16

Page 7 of 8



Impedance Measurement Plot for Body TSL

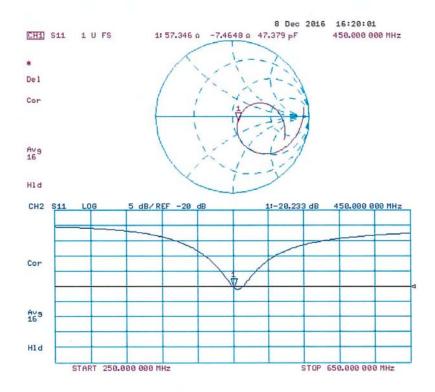

Certificate No: D450V3-1094_Dec16

Page 8 of 8