


Impedance Plot for SN 29/15 DIP 2G450-393


2450 Head

Calibrated impedance: $52.3\Omega + 3.4j\Omega$; Measurement impedance: $55.8\Omega + 1.6j\Omega$ (within 5Ω)

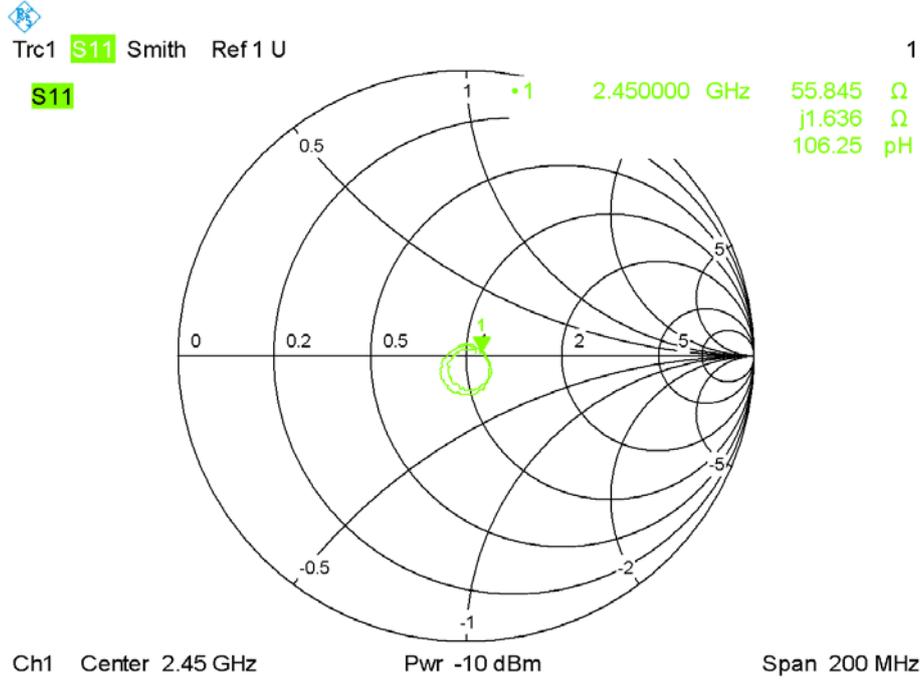

Date: 29.MAY.2023 10:49:23

Calibrated return loss: -27.80dB; Measurement return loss: -24.53dB (within 20%)

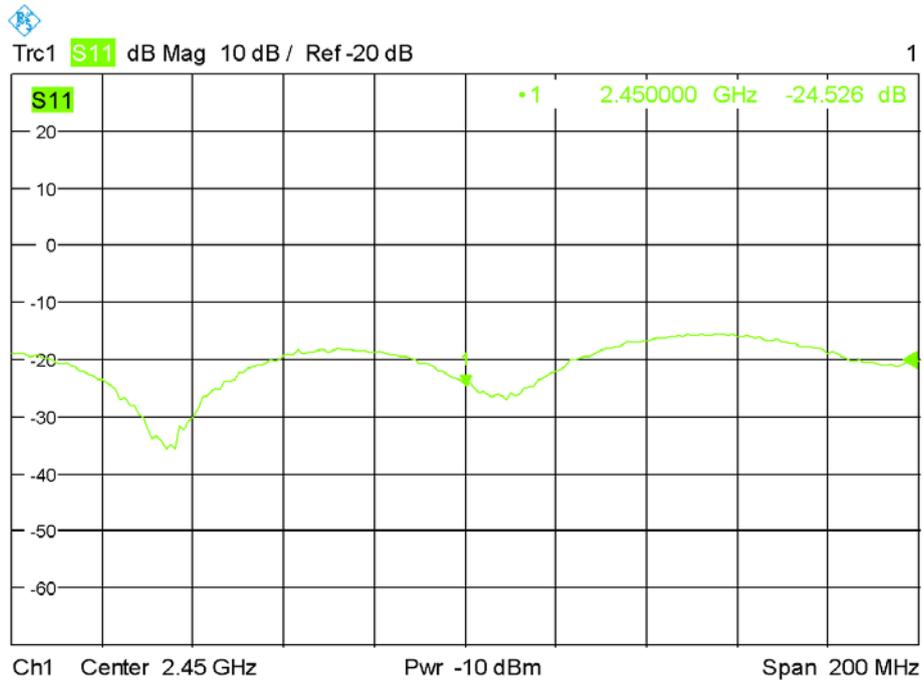

Date: 29.MAY.2023 10:50:11