

Appendix C for KSCR230900155101

Calibration Certificate

Object	Apply	No	Model	SN	Calibration Date	Due date of calibration
Dipole	☒	1	D750V3	1188	2022/03/29	2025/03/28
	☒	2	D835V2	4d114	2022/03/31	2025/03/30
	☐	3	D900V2	1d079	2022/06/07	2025/06/06
	☒	4	D1800V2	2d170	2022/03/31	2025/03/30
	☒	5	D1900V2	5d136	2022/06/07	2025/06/06
	☐	6	D2000V2	1041	2022/06/06	2025/06/05
	☒	7	D2300V2	1096	2022/03/31	2025/03/30
	☒	8	D2450V2	817	2022/04/01	2025/03/31
	☒	9	D2600V2	1158	2022/03/31	2025/03/30
	☒	10	D5GHzV2	1095	2022/06/01	2025/05/31
DAE	☒	11	DAE4	1305	2023/04/13	2024/04/12
Probe	☒	12	EX3DV4	7833	2023/08/24	2024/08/23

1 Dipole


1.1 D750V3 - SN 1188

TTL Calibration Laboratory		CAICT	
In Collaboration with CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42104633-2512 Fax: +86-10-42104633-2504 E-mail: csl@china-test.com http://www.china-test.com		In Collaboration with CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42104633-2512 Fax: +86-10-42104633-2504 E-mail: csl@china-test.com http://www.china-test.com	
Client: SGS-CN		Certificate No: Z22-60103	
CALIBRATION CERTIFICATE			
Object: D750V3 - SN: 1188			
Calibration Procedure(s): FF-211-003-01 Calibration Procedures for dipole validation kits			
Calibration date: March 29, 2022			
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity<70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Power Meter NRP2	100277	24-Sep-21 (CTTL No J21X08326)	Sep-22
Power sensor NSP6S	104291	24-Sep-21 (CTTL No J21X08326)	Sep-22
Reference Probe EX30V4	SN 7307	26-May-21 (SPEAG No EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No J22X00409)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No J22X00406)	Jan-23
Calibrated by:	Name: Zhao Jing	Function: SAR Test Engineer	Signature: [Signature]
Reviewed by:	Name: Lin Hao	Function: SAR Test Engineer	Signature: [Signature]
Approved by:	Name: Qi Diqiyuan	Function: SAR Project Leader	Signature: [Signature]
Issued: April 3, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60103		Page 1 of 6	

TTL Calibration Laboratory		CAICT	
In Collaboration with CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42104633-2512 Fax: +86-10-42104633-2504 E-mail: csl@china-test.com http://www.china-test.com		In Collaboration with CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42104633-2512 Fax: +86-10-42104633-2504 E-mail: csl@china-test.com http://www.china-test.com	
Glossary: TSL: tissue simulating liquid Conf: sensitivity in TSL / NORMs y,z N/A: not applicable or not measured			
Calibration is Performed According to the Following Standards: a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz); October 2020 b) KDB 855664, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation: c) DASYS4.5 System Handbook			
Methods Applied and Interpretation of Parameters: • Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. • Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. • Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. • Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. • SAR measured: SAR measured at the stated antenna input power. • SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. • SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60103		Page 1 of 6	

TTL Calibration Laboratory		CAICT	
In Collaboration with CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42104633-2512 Fax: +86-10-42104633-2504 E-mail: csl@china-test.com http://www.china-test.com		In Collaboration with CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42104633-2512 Fax: +86-10-42104633-2504 E-mail: csl@china-test.com http://www.china-test.com	
Measurement Conditions DASY system configuration, as far as not given on page 1			
DASY Version	DASY52	V52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	15 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	750 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	42.0	0.90 nH/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 6 %	0.89 nH/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	2.07 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	1.37 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (k=2)	
Certificate No: Z22-60103		Page 3 of 6	

TTL Calibration Laboratory		CAICT	
In Collaboration with CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42104633-2512 Fax: +86-10-42104633-2504 E-mail: csl@china-test.com http://www.china-test.com		In Collaboration with CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42104633-2512 Fax: +86-10-42104633-2504 E-mail: csl@china-test.com http://www.china-test.com	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	53.60-1.13jΩ		
Return Loss	-26.7dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	0.947 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small and caps are added to the dipole arms in order to improve matching when cabled according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60103		Page 4 of 6	

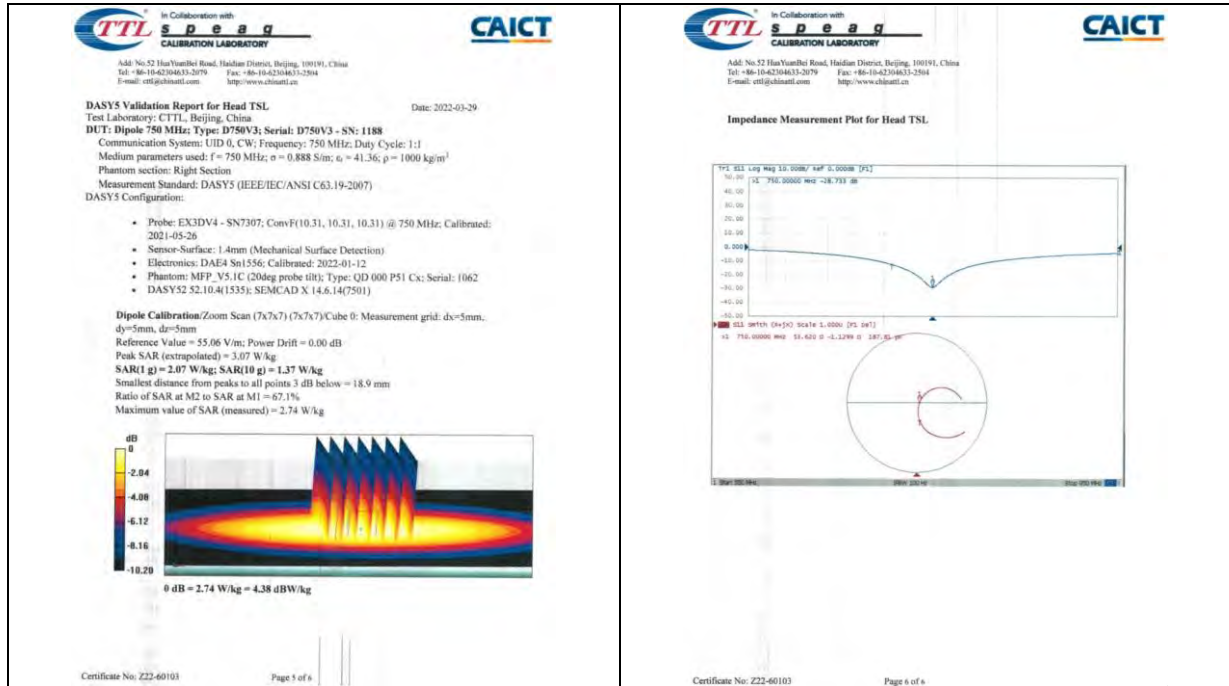

1.2 D835V2 - SN 4d114

TTL **s p e e a g**
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42346633-2079 Fax: +86-10-42346633-2564
E-mail: cti@china.ttl.com http://www.china.ttl.com

CAICT

In Collaboration with

Client: SGS-CN Certificate No: Z22-60104

CALIBRATION CERTIFICATE

Object: D835V2 - SN: 4d114

Calibration Procedure(s): PF-Z11-003-01
Calibration Procedures for dipole validation kits

Calibration date: March 31, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Power sensor NRPBS	104291	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY46071430	15-Jan-22 (CTTL No.J22X00409)	Jan-23
Network Analyzer E5071C	MY46110873	14-Jan-22 (CTTL No.J22X00405)	Jan-23

Calibrated by: Zhao Jing SAR Test Engineer
Reviewed by: Lin Hao SAR Test Engineer
Approved by: Qi Diqian SAR Project Leader

Issued: April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60104 Page 1 of 5

TTL **s p e e a g**
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42346633-2079 Fax: +86-10-42346633-2564
E-mail: cti@china.ttl.com http://www.china.ttl.com

CAICT

In Collaboration with

Glossary:

TSL	issue simulating liquid
ConvF	sensitivity in TSL / NORMx.y.z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices - Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- KDB 665664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:


- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60104 Page 2 of 5

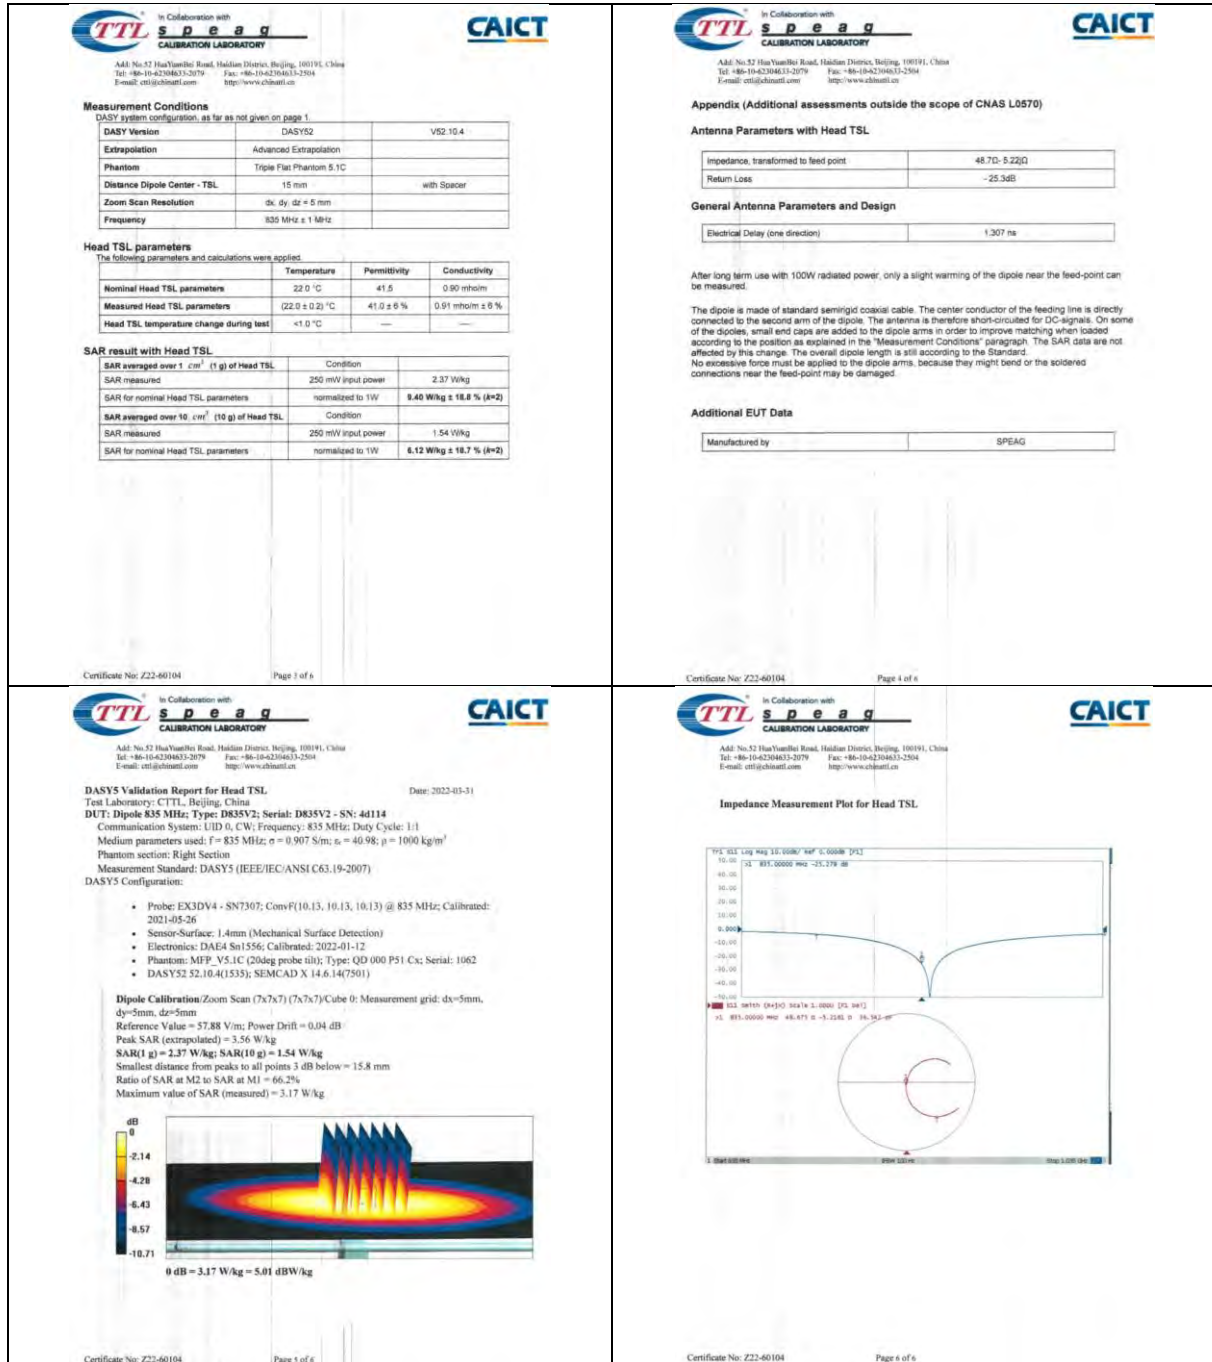


1.3 D900V2 - SN 1d079

TTL Calibration Laboratory		CAICT	
Add: No.52 HuaYuan Road, Haidian District, Beijing, 100191 Tel: +86-10-62106137-3117 E-mail: cti@sgs.com.cn		Add: No.52 HuaYuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62106137-3117 E-mail: cti@sgs.com.cn	
Client	SGS-CN	Certificate No.	Z22-60184
CALIBRATION CERTIFICATE			
Object	D900V2 - SN: 1d079		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date:	June 7, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (23±1)°C and humidity <70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No. J21X08326)	Sep-22
Power sensor NRP85	104291	24-Sep-21 (CTTL No. J21X08326)	Sep-22
Reference Probe EX3DVA	SN 7464	26-Jan-22 (SPEAG No. EX3-7464_Jan22)	Jan-23
DAE4	SN 1586	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E2438C	MY49071430	13-Jan-22 (CTTL No. J22X00406)	Jan-23
Network Analyzer E5071C	MY49110473	14-Jan-22 (CTTL No. J22X00406)	Jan-23
Calibrated by:	Name	Function	Signature
	Zhao Jing	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Dianyan	SAR Project Leader	
Issued: June 13, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60184		Page 1 of 6	

TTL Calibration Laboratory		CAICT	
Add: No.52 HuaYuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62106137-3117 E-mail: cti@sgs.com.cn		Add: No.52 HuaYuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62106137-3117 E-mail: cti@sgs.com.cn	
Glossary:			
TSL	tissue simulating liquid		
ConvF	sensitivity in TSL / NORM.y,z		
N/A	not applicable or not measured		
Calibration is Performed According to the Following Standards:			
a) IEC/IEEE 62209-1529, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices-Part 1529: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020			
b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
c) DASYS4 System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in this certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.			
• Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.			
• Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60184		Page 1 of 6	

TTL Calibration Laboratory		CAICT	
Add: No.52 HuaYuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62106137-3117 E-mail: cti@sgs.com.cn		Add: No.52 HuaYuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62106137-3117 E-mail: cti@sgs.com.cn	
Measurement Conditions			
DASYS system configuration, as far as is given on page 1			
DASYS Version	DASYS2	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	15 mm	with Spacer	
Zoom Scan Resolution	0x, dy, dz = 5 mm		
Frequency	900 MHz ± 1 MHz		
Head TSL parameters			
The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.97 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	42.1 ± 6 %	0.98 mho/m ± 6 %
Head TSL temperature change during test	<±0.5 °C	—	—
SAR result with Head TSL			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	2.75 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	11.0 W/kg ± 16.8 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	1.75 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	7.09 W/kg ± 16.7 % (k=2)	
Certificate No: Z22-60184		Page 4 of 6	

TTL Calibration Laboratory		CAICT	
Add: No.52 HuaYuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62106137-3117 E-mail: cti@sgs.com.cn		Add: No.52 HuaYuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62106137-3117 E-mail: cti@sgs.com.cn	
Appendix (Additional assessments outside the scope of CNAS L0670)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	48 (10-9-450)		
Return Loss	-23.3 dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.312 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60184		Page 4 of 6	

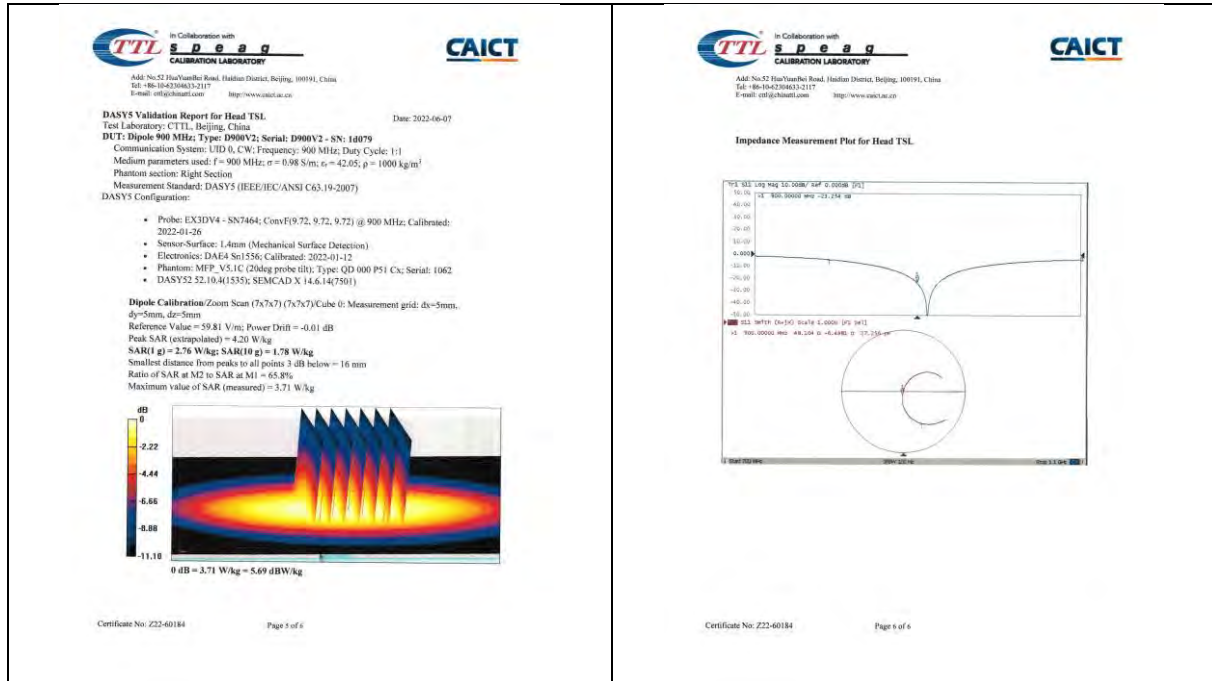

1.4 D1800V2 - SN 2d170

TTL Calibration Laboratory
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-4230603-2117
E-mail: cti@china.ttl.com

CAICT

Client: **SGS-CN** Certificate No: **Z22-60105**

CALIBRATION CERTIFICATE

Object: **D1800V2 - SN: 2d170**

Calibration Procedure(s): **FF-Z11-003-01**
Calibration Procedures for dipole validation kits

Calibration date: **March 31, 2022**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22±3)°C and humidity <70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EK3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00409)	Jan-23

Calibrated by: **Zhao Jing** SAR Test Engineer
Reviewed by: **Lin Hao** SAR Test Engineer
Approved by: **Qi Diqian** SAR Project Leader

Issued: April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60105 Page 1 of 6

TTL Calibration Laboratory
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-4230603-2117
E-mail: cti@china.ttl.com

CAICT

Glossary:
TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORM_{x,y,z}
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
b) KDB 855664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:
c) DASY4/5 System Handbook



Methods Applied and Interpretation of Parameters:
• **Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
• **Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
• **Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
• **Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
• **SAR measured:** SAR measured at the stated antenna input power.
• **SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
• **SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60105 Page 2 of 6

In Collaboration with TTL s p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinatest.com http://www.chinatest.cn			
Measurement Conditions DASY system configuration, as far as not given on page 1.			
DASY Version	DASY52	S2.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	1800 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.0 ± 6 %	1.41 mho/m ± 6 %
Head TSL temperature change during test	< 1.0 °C	—	—
SAR result with Head TSL			
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	9.73 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	38.9 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	5.11 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	20.4 W/kg ± 18.7 % (k=2)	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	47.90 - j2.54 Ω		
Return Loss	-29.4 dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.116 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		

Certificate No: Z22-60105 Page 3 of 6

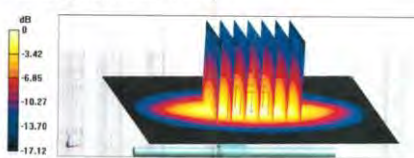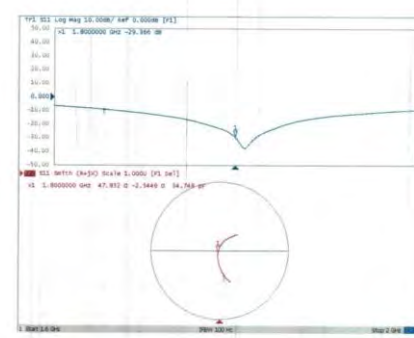In Collaboration with TTL s p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinatest.com http://www.chinatest.cn			
DASY5 Validation Report for Head TSL Date: 2022-03-31			
Test Laboratory: CTTL, Beijing, China			
DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN: 2d170			
Communication System: UID 0, CW; Frequency: 1800 MHz; Duty Cycle: 1:1			
Medium parameters used: f = 1800 MHz; σ = 1.411 S/m; ε = 40.62; ρ = 1000 kg/m ³			
Phantom section: Right Section			
Measurement Standard: DASY5 (IEEE/ANSI C63.19-2007)			
DASY5 Configuration:			
• Probe: EX3DV4 - SN7307; ConvF(8.34, 8.34, 8.34) @ 1800 MHz; Calibrated: 2021-05-26			
• Sensor-Surface: 1.4mm (Mechanical Surface Detection)			
• Electronics: DAE4 Sn1556; Calibrated: 2022-01-12			
• Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062			
• DASY52 S2.10.4(1535); SEMCAD X 14.6.14(7501)			
Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm			
Reference Value = 98.14 V/m; Power Drift = 0.03 dB			
Peak SAR (extrapolated) = 18.2 W/kg			
SAR(1 g) = 9.73 W/kg; SAR(10 g) = 5.11 W/kg			
Smallest distance from peaks to all points 3 dB below = 10 mm			
Ratio of SAR at M2 to SAR at M1 = 54%			
Maximum value of SAR (measured) = 15.2 W/kg			
			
Impedance Measurement Plot for Head TSL			
			

Certificate No: Z22-60105 Page 6 of 6


1.5 D1900V2 - SN 5d136

TTL Calibration Laboratory		CAICT	
Add: No. 52 Huayuan Road, Haidian District, Beijing, 100191 Tel: +86-10-42046122-117 E-mail: csl@ttslab.com		Add: No. 52 Huayuan Road, Haidian District, Beijing, 100191 Tel: +86-10-42046122-117 E-mail: csl@ttslab.com	
Client: SGS-CN	Certificate No: Z22-60185		
CALIBRATION CERTIFICATE			
Object	D1900V2 - SN 5d136		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date:	June 7, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility; environment temperature (23±1)°C and humidity <70%.			
Calibration Equipment used (M&E critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No. J21X08326)	Sep-22
Power sensor NRP85	104291	24-Sep-21 (CTTL No. J21X08326)	Sep-22
Reference Probe EXSDV4	SN 7404	28-Jan-22 (SPEAG No. EX3-7404_Jan22)	Jan-23
DAEA	SN 1558	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No. J22X00409)	Jan-23
Network Analyzer E5071C	MY48110073	14-Jan-22 (CTTL No. J22X00406)	Jan-23
Calibrated by:	Name: Zhao Jing	Function: SAR Test Engineer	Signature: [Signature]
Reviewed by:	Name: Lin Hao	Function: SAR Test Engineer	Signature: [Signature]
Approved by:	Name: Qi Dianyan	Function: SAR Project Leader	Signature: [Signature]
Issued: June 13, 2022			
The calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60185		Page 1 of 8	

TTL Calibration Laboratory		CAICT	
Add: No. 52 Huayuan Road, Haidian District, Beijing, 100191 Tel: +86-10-42046122-117 E-mail: csl@ttslab.com		Add: No. 52 Huayuan Road, Haidian District, Beijing, 100191 Tel: +86-10-42046122-117 E-mail: csl@ttslab.com	
Measurement Conditions QAS system configuration, as far as not given on page 1:			
DASY Version	DASY52	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	1900 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	45.0	1.40 nS/m
Measured Head TSL parameters	(22.0 ± 0.3) °C	39.9 ± 0.5 %	1.39 nS/m ± 0.5 %
Head TSL temperature change during test	+1.0 °C		
SAR result with Head TSL			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition:	3.65 W/kg	
SAR measured	250 mW input power	40.0 W/kg ± 16.8 % (k=2)	
SAR for nominal Head TSL parameters	normalized to 1W	40.0 W/kg ± 16.8 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition:	5.18 W/kg	
SAR measured	250 mW input power	20.8 W/kg ± 18.7 % (k=2)	
SAR for nominal Head TSL parameters	normalized to 1W	20.8 W/kg ± 18.7 % (k=2)	
Certificate No: Z22-60185		Page 3 of 8	

TTL Calibration Laboratory		CAICT	
Add: No. 52 Huayuan Road, Haidian District, Beijing, 100191 Tel: +86-10-42046122-117 E-mail: csl@ttslab.com		Add: No. 52 Huayuan Road, Haidian District, Beijing, 100191 Tel: +86-10-42046122-117 E-mail: csl@ttslab.com	
Glossary:			
TSL	Issue simulating liquid		
ConF	sensitivity in TSL / NORM x y z		
N/A	not applicable or not measured		
Calibration is Performed According to the Following Standards:			
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020			
b) KDB 855884, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
c) DASY4/5 System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.			
• Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.			
• Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60185		Page 2 of 8	

TTL Calibration Laboratory		CAICT	
Add: No. 52 Huayuan Road, Haidian District, Beijing, 100191 Tel: +86-10-42046122-117 E-mail: csl@ttslab.com		Add: No. 52 Huayuan Road, Haidian District, Beijing, 100191 Tel: +86-10-42046122-117 E-mail: csl@ttslab.com	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	51.5Ω ± 1.5Ω		
Return Loss	22.4dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.108 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60185		Page 4 of 8	

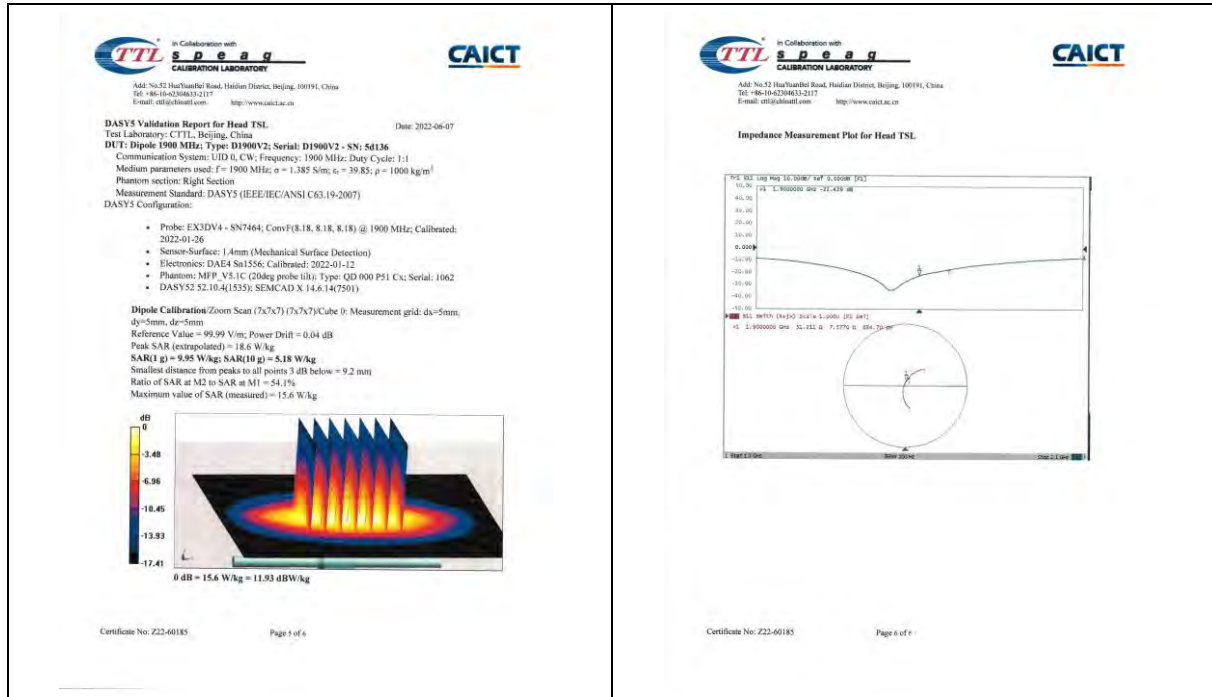

1.6 D2000V2 - SN 1041

TTL **speaq** **CAICT**

Address: No. 52 Huayuan Road, Huailian District, Beijing, 100191, China
Tel: +86-10-6258633-3117
E-mail: ttl@ttsl.com.cn

Client: **SGS-CN** Certificate No: **Z22-60186**

CALIBRATION CERTIFICATE

Object: D2000V2 - SN 1041

Calibration Procedure(s): FF-Z11-003-01
Calibration Procedure for dipole validation kits

Calibration date: June 6, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No. J21K08328)	Sep-22
Power sensor NRP5	104291	24-Sep-21 (CTTL No. J21K08328)	Sep-22
Reference Probe EX3DV4	SN 7464	26-Jan-22 (SPEAG No. EX3-7464_Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No. Z22K00408)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No. Z22K00408)	Jan-23

Calibrated by: Zhao Jing SAR Test Engineer

Reviewed by: Lin Hao SAR Test Engineer

Approved by: Qi Danyuan SAR Project Leader

Issued: June 13, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60186 Page 1 of 6

TTL **speaq** **CAICT**

Address: No. 52 Huayuan Road, Huailian District, Beijing, 100191, China
Tel: +86-10-6258633-3117
E-mail: ttl@ttsl.com.cn

Glossary:

TSL: Issue simulating liquid

ConvF: sensitivity in TSL / NORM x y,z

N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-Head and Body-Mounted Wireless Communication Devices: Part 1528 Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020

b) KDB 865564, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY4/S System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameter with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60186 Page 2 of 6

In Collaboration with
TTL **s p e a g**
CALIBRATION LABORATORY

ADD: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62366322-2117
E-mail: cti@china.ttl.com http://www.caict.ac.cn

CAICT

In Collaboration with
TTL **s p e a g**
CALIBRATION LABORATORY

ADD: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62366322-2117
E-mail: cti@china.ttl.com http://www.caict.ac.cn

CAICT

Measurement Conditions

DASY system configuration, as far as not given on page 1:

DASY Version	DASY52	52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom S.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2000 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied:

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.9 °C	40.0	1.40 mho/cm
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.2 ± 6 %	1.36 mho/cm ± 6 %
Head TSL temperature change during test	<1.0 °C	—	—

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition
SAR measured	250 mW input power
SAR for nominal Head TSL parameters	normalized to 1W
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition
SAR measured	250 mW input power
SAR for nominal Head TSL parameters	normalized to 1W

Certificate No: Z23-60186

Page 3 of 8

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	48.4Ω ± 0.74Ω
Return Loss	-34.8dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.08 ns
----------------------------------	---------

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small and large caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: Z23-60188

Page 8 of 8

In Collaboration with
TTL **s p e a g**
CALIBRATION LABORATORY

ADD: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62366322-2117
E-mail: cti@china.ttl.com http://www.caict.ac.cn

CAICT

In Collaboration with
TTL **s p e a g**
CALIBRATION LABORATORY

ADD: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62366322-2117
E-mail: cti@china.ttl.com http://www.caict.ac.cn

CAICT

DASY5 Validation Report for Head TSL

Test Laboratory: CTTL, Beijing, China

Date: 2022-06-06

DUT: Dipole 2000 MHz; Type: D2000V2; Serial: D2000V2; SN: 1041

Communication System: UTD 0, CW; Frequency: 2000 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2000 MHz; σ = 1.392 S/m; ε = 40.21; ρ = 1000 kg/m³

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 - SN7464; ConvF(R2, R2, R2) @ 2000 MHz; Calibrated: 2022-01-26
- Sensor Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA64 Sn1556; Calibrated: 2022-01-12
- Phantom: MPP_V5.1C (204kg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52: S2.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube (t: Measurement grid: dx=5mm, dy=5mm, dz=5mm)

Reference Value = 103.4 V/m; Power Drift = 0.03 dB


Peak SAR (extrapolated) = 19.6 W/kg

SAR(1 g) = 10.4 W/kg; SAR(10 g) = 5.3 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 53.6%


Maximum value of SAR (measured) = 16.3 W/kg

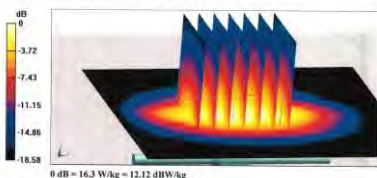

0 dB = 16.3 W/kg = 12.12 dBW/kg

Certificate No: Z23-60186

Page 5 of 6

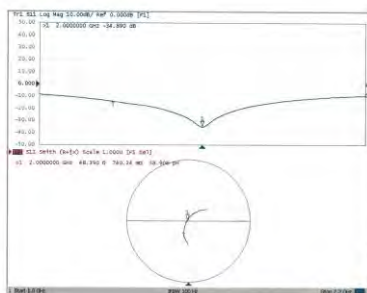


0 dB = 16.3 W/kg = 12.12 dBW/kg

Certificate No: Z23-60188

Page 6 of 6

1.7 D2300V2 - SN 1096

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504 E-mail: cti@chinaul.com http://www.chinaul.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2509 Fax: +86-10-62304633-2504 E-mail: cti@chinaul.com http://www.chinaul.cn	
Client	SGS-CN	Certificate No.	Z22-60106
CALIBRATION CERTIFICATE			
Object	D2300V2 - SN 1096		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date	March 31, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Power sensor NRP8	104291	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EK3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23
Calibrated by:	Name	Function	Signature
	Zhao Jing	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Diqiyuan	SAR Project Leader	
Issued: April 6, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory			
Certificate No: Z22-60106		Page 1 of 6	
TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2509 Fax: +86-10-62304633-2504 E-mail: cti@chinaul.com http://www.chinaul.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2509 Fax: +86-10-62304633-2504 E-mail: cti@chinaul.com http://www.chinaul.cn	
Measurement Conditions DASY system configuration, as far as not given on page 1:			
DASY Version	DASY2	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	2300 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.5	1.67 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.8 ± 9 %	1.70 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	—	—
SAR result with Head TSL			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	12.4 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	49.2 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	5.88 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	23.4 W/kg ± 18.7 % (k=2)	
Certificate No: Z22-60106		Page 3 of 6	
TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2509 Fax: +86-10-62304633-2504 E-mail: cti@chinaul.com http://www.chinaul.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2509 Fax: +86-10-62304633-2504 E-mail: cti@chinaul.com http://www.chinaul.cn	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	46.20 - 4.56jΩ		
Return Loss	-26.6dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.083 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when backed according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60106		Page 4 of 6	

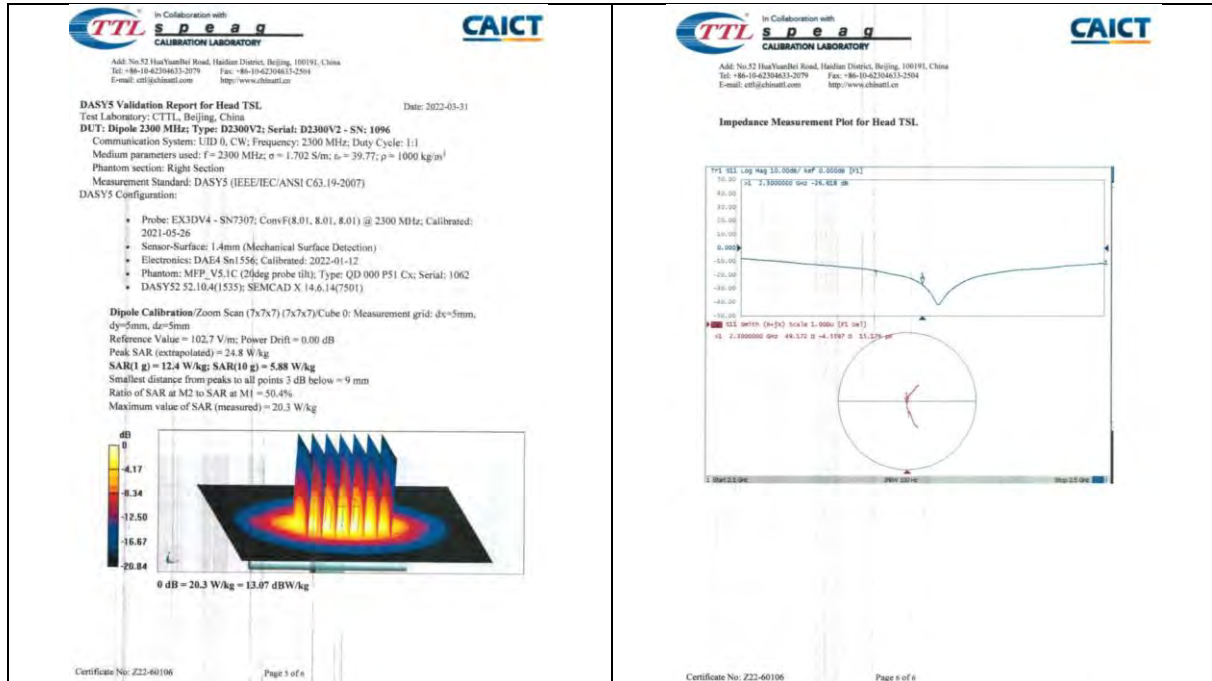

1.8 D2450V2 - SN 817

In Collaboration with
TTL Speaq
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42504633-2079 Fax: +86-10-42504633-2504
E-mail: csl@china.ttl.com http://www.china.ttl.com

CAICT

Client: **SGS-CN** Certificate No: **Z22-60107**

CALIBRATION CERTIFICATE

Object: **D2450V2 - SN 817**

Calibration Procedure(s): **FF-Z1(1-003-3)**
Calibration Procedures for dipole validation kits

Calibration date: **April 1, 2022**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements [B]. The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Power Meter: NRP2	106277	24-Sep-21 (CTTL No.J21X08320)	Sep-22
Power sensor: NRP8S	104291	24-Sep-21 (CTTL No.J21X08320)	Sep-22
Reference Probe EX3DV4	SN 7307	25-May-21(SPEAG.No EX3-7307_May21)	May-22
DAE4	SN 1555	12-Jan-22(CTTL-SPEAG.No Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No. J22X00409)	Jan-23
Network Analyzer E5071C	MY48110873	14-Jan-22 (CTTL No. J22X00406)	Jan-23

Calibrated by: **Zhao Jing** SAR Test Engineer

Reviewed by: **Liu Hao** SAR Test Engineer

Approved by: **Qi Dianyan** SAR Project Leader

Issued: April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60107 Page 1 of 5

In Collaboration with
TTL Speaq
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42504633-2079 Fax: +86-10-42504633-2504
E-mail: csl@china.ttl.com http://www.china.ttl.com

CAICT

Glossary:

TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORMix.y.z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
b) KDB 865684, "SAR Measurement Requirements for 100 MHz to 5 GHz"

Additional Documentation:


c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60107 Page 2 of 5

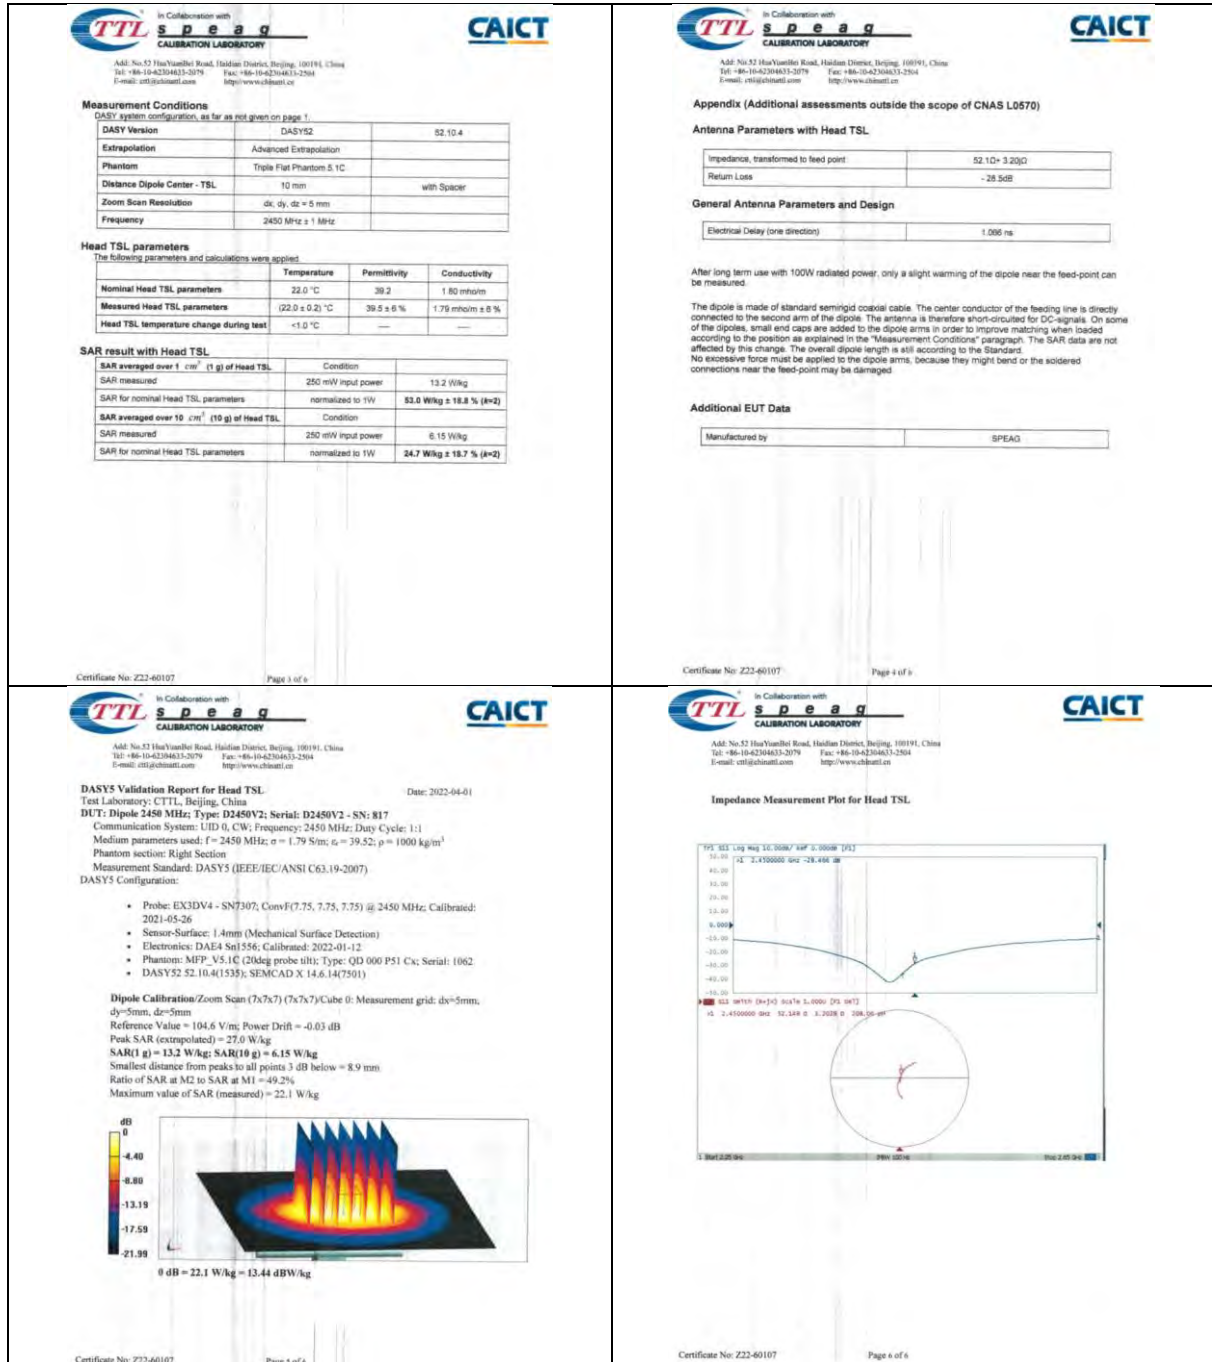


After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard serringid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

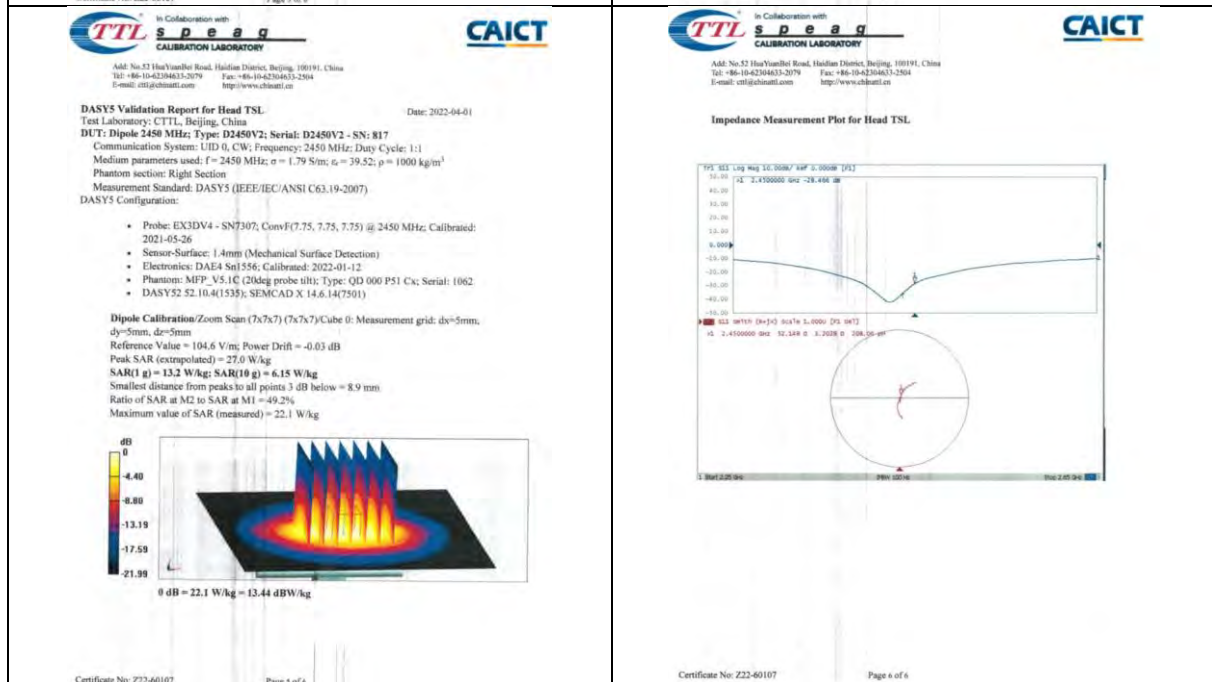


1.9 D2600V2 - SN 1158

TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504 E-mail: cti@china-test.com.cn http://www.china-test.com		Add: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china-test.com.cn http://www.china-test.com	
Client: SGS-CN		Certificate No: Z22-60108	
CALIBRATION CERTIFICATE			
Object	D2600V2 - SN 1158		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date	March 31, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity <70%.			
Calibration Equipment used (MSTE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106377	24-Sep-21 (CTTL No. J21X08326)	Sep-22
Power sensor NRP8	104291	24-Sep-21 (CTTL No. J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No. EX3-7307_May21)	May-22
DAE4	SN 1158	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator S4436C	MY48071430	13-Jan-22 (CTTL No. J22X00409)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No. J22X00409)	Jan-23
Calibrated by:	Name	Function	Signature
	Zhao Jing	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Dianyan	SAR Project Leader	
Issued: April 6, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60108		Page 1 of 6	

TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china-test.com.cn http://www.china-test.com		Add: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china-test.com.cn http://www.china-test.com	
Measurement Conditions DASY system configuration, as far as not given on page 1:			
DASY Version	DASY52	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom S.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	2600 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	38.0	1.96 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.7 ± 6 %	1.96 mho/m ± 6 %
Head TSL temperature change during test	±1.0 °C	—	
SAR result with Head TSL			
SAR averaged over 1 cm² (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	13.7 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	54.8 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm² (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	6.12 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	24.5 W/kg ± 18.7 % (k=2)	
Certificate No: Z22-60108		Page 3 of 6	

TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china-test.com.cn http://www.china-test.com		Add: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china-test.com.cn http://www.china-test.com	
Glossary:			
TSL	tissue simulating liquid		
ConvF	sensitivity in TSL / NORMx.y.z		
N/A	not applicable or not measured		
Calibration is Performed According to the Following Standards:			
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices - Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020			
b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
c) DASY4/S System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.			
• Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.			
• Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60108		Page 2 of 6	

TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china-test.com.cn http://www.china-test.com		Add: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china-test.com.cn http://www.china-test.com	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	49.90- 6.49jΩ		
Return Loss	-23.9dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.053 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.			
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60108		Page 4 of 6	

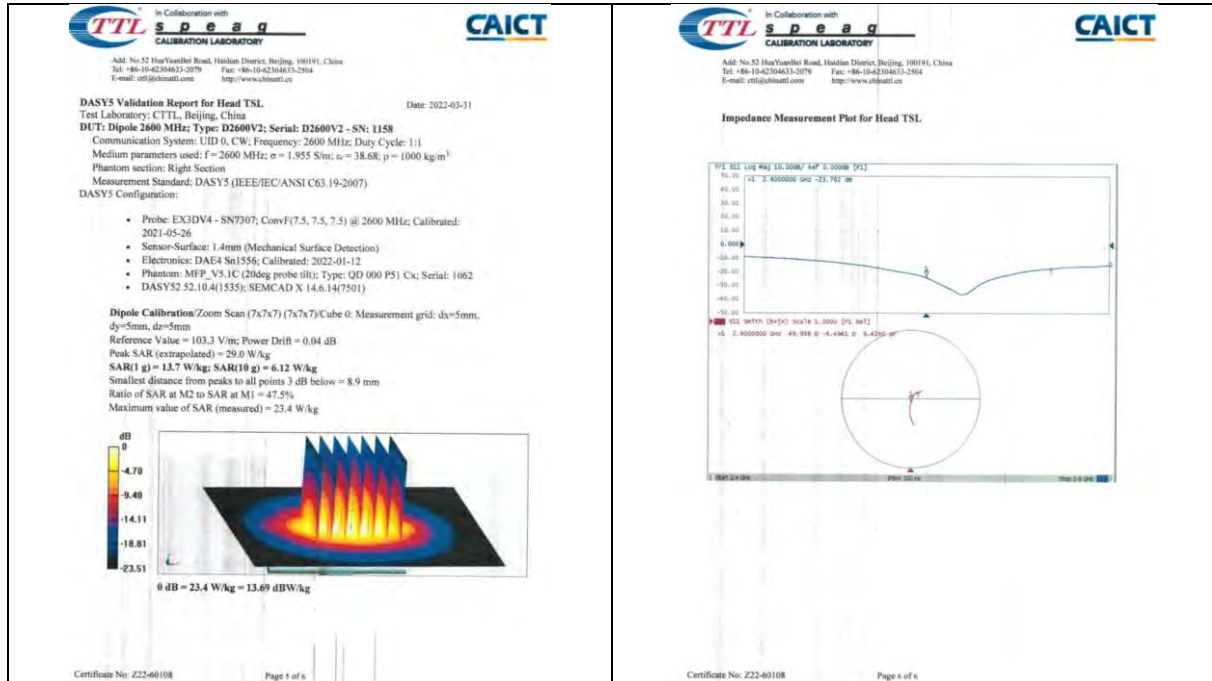

1.10 D5GHZV2 - SN 1095

TTL Speaq Calibration Laboratory
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62104613-2079 Fax: +86-10-62104613-2504
E-mail: cti@ttspeaq.com http://www.ttspeaq.com

CAICT

Client: SGS-CN Certificate No: Z22-60187

CALIBRATION CERTIFICATE

Object: D5GHZV2 - SN 1095

Calibration Procedure(s): FF-Z11-003-01
Calibration Procedures for dipole validation kit

Calibration date: June 1, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (23±1)°C and humidity<70%.

Calibration Equipment used (MSTE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21008328)	Sep-22
Power sensor NRP85	104291	24-Sep-21 (CTTL No.J21008328)	Sep-22
Reference Probe EX3DV4	SN 7464	26-Jan-22(SPEAG No EX3-7484, Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG No J22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No. J22000409)	Jan-23
Network Analyzer E5071C	MY46110873	14-Jan-22 (CTTL No. J22000406)	Jan-23

Calibrated by: Zhao Jing SAR Test Engineer

Reviewed by: Lin Hao SAR Test Engineer

Approved by: Qi Dianyan SAR Project Leader

Issued: June 8, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60187 Page 1 of 10

TTL Speaq Calibration Laboratory
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62104613-2079 Fax: +86-10-62104613-2504
E-mail: cti@ttspeaq.com http://www.ttspeaq.com

CAICT

Glossary:
TSL: Issue simulating liquid
CompF: sensitivity in TSL + NORM x y z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices-Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"





Additional Documentation:
c) DASY45 System Handbook





Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60187 Page 7 of 10

 In Collaboration with TTL Calibration Laboratory Add: No.52 HuaYuanBao Road, Haidian District, Beijing, 100191, China Tel: +86-10-62592117 E-mail: info@ttsl.com.cn http://www.ttsl.com.cn  CAICT Measurement Conditions The following parameters and calculations were applied. <table border="1"> <tr> <td>DASY Version</td> <td>DASY52</td> <td>52.10.4</td> </tr> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5-1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Dipcor</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>10 (5 x 4 mm, 40 x 4.4 mm)</td> <td>Grided Ratio = 1.4 (2 divisions)</td> </tr> <tr> <td>Frequency</td> <td>5200 MHz ± 1 MHz 5300 MHz ± 1 MHz 5500 MHz ± 1 MHz 5600 MHz ± 1 MHz</td> <td></td> </tr> </table> Head TSL parameters at 5200MHz The following parameters and calculations were applied. <table border="1"> <tr> <td></td> <td>Temperature</td> <td>Permittivity</td> <td>Conductivity</td> </tr> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>35.9</td> <td>4.68 mS/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>35.4 ± 6 %</td> <td>4.62 mS/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><1.0 °C</td> <td>—</td> <td>—</td> </tr> </table> SAR result with Head TSL at 5200MHz <table border="1"> <tr> <td>SAR averaged over 1 cm³ (1 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>100 mW input power</td> <td>7.75 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>77.6 W/kg ± 24.4 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm³ (10 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>2.22 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>22.1 W/kg ± 24.2 % (k=2)</td> </tr> </table> Certificate No: Z22-40187 Page 1 of 10	DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5-1C		Distance Dipole Center - TSL	10 mm	with Dipcor	Zoom Scan Resolution	10 (5 x 4 mm, 40 x 4.4 mm)	Grided Ratio = 1.4 (2 divisions)	Frequency	5200 MHz ± 1 MHz 5300 MHz ± 1 MHz 5500 MHz ± 1 MHz 5600 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	35.9	4.68 mS/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	35.4 ± 6 %	4.62 mS/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		SAR measured	100 mW input power	7.75 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	77.6 W/kg ± 24.4 % (k=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		SAR measured	250 mW input power	2.22 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	22.1 W/kg ± 24.2 % (k=2)	 In Collaboration with TTL Calibration Laboratory Add: No.52 HuaYuanBao Road, Haidian District, Beijing, 100191, China Tel: +86-10-62592117 E-mail: info@ttsl.com.cn http://www.ttsl.com.cn  CAICT Head TSL parameters at 5300MHz The following parameters and calculations were applied. <table border="1"> <tr> <td></td> <td>Temperature</td> <td>Permittivity</td> <td>Conductivity</td> </tr> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>35.9</td> <td>4.76 mS/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>35.2 ± 6 %</td> <td>4.73 mS/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><1.0 °C</td> <td>—</td> <td>—</td> </tr> </table> SAR result with Head TSL at 5300MHz <table border="1"> <tr> <td>SAR averaged over 1 cm³ (1 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>100 mW input power</td> <td>7.94 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>79.1 W/kg ± 24.4 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm³ (10 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>100 mW input power</td> <td>2.27 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>22.6 W/kg ± 24.2 % (k=2)</td> </tr> </table> Head TSL parameters at 5500MHz The following parameters and calculations were applied. <table border="1"> <tr> <td></td> <td>Temperature</td> <td>Permittivity</td> <td>Conductivity</td> </tr> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>35.9</td> <td>4.88 mS/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>34.8 ± 6 %</td> <td>4.84 mS/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><1.0 °C</td> <td>—</td> <td>—</td> </tr> </table> SAR result with Head TSL at 5500MHz <table border="1"> <tr> <td>SAR averaged over 1 cm³ (1 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>100 mW input power</td> <td>8.20 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>82.6 W/kg ± 24.4 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm³ (10 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>100 mW input power</td> <td>2.34 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>23.3 W/kg ± 24.2 % (k=2)</td> </tr> </table> Certificate No: Z22-40187 Page 2 of 10		Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	35.9	4.76 mS/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	35.2 ± 6 %	4.73 mS/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		SAR measured	100 mW input power	7.94 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	79.1 W/kg ± 24.4 % (k=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		SAR measured	100 mW input power	2.27 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	22.6 W/kg ± 24.2 % (k=2)		Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	35.9	4.88 mS/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	34.8 ± 6 %	4.84 mS/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		SAR measured	100 mW input power	8.20 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	82.6 W/kg ± 24.4 % (k=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		SAR measured	100 mW input power	2.34 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	23.3 W/kg ± 24.2 % (k=2)
DASY Version	DASY52	52.10.4																																																																																																																							
Extrapolation	Advanced Extrapolation																																																																																																																								
Phantom	Triple Flat Phantom 5-1C																																																																																																																								
Distance Dipole Center - TSL	10 mm	with Dipcor																																																																																																																							
Zoom Scan Resolution	10 (5 x 4 mm, 40 x 4.4 mm)	Grided Ratio = 1.4 (2 divisions)																																																																																																																							
Frequency	5200 MHz ± 1 MHz 5300 MHz ± 1 MHz 5500 MHz ± 1 MHz 5600 MHz ± 1 MHz																																																																																																																								
	Temperature	Permittivity	Conductivity																																																																																																																						
Nominal Head TSL parameters	22.0 °C	35.9	4.68 mS/m																																																																																																																						
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.4 ± 6 %	4.62 mS/m ± 6 %																																																																																																																						
Head TSL temperature change during test	<1.0 °C	—	—																																																																																																																						
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																																																																																								
SAR measured	100 mW input power	7.75 W/kg																																																																																																																							
SAR for nominal Head TSL parameters	normalized to 1W	77.6 W/kg ± 24.4 % (k=2)																																																																																																																							
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																																																																																																																								
SAR measured	250 mW input power	2.22 W/kg																																																																																																																							
SAR for nominal Head TSL parameters	normalized to 1W	22.1 W/kg ± 24.2 % (k=2)																																																																																																																							
	Temperature	Permittivity	Conductivity																																																																																																																						
Nominal Head TSL parameters	22.0 °C	35.9	4.76 mS/m																																																																																																																						
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.2 ± 6 %	4.73 mS/m ± 6 %																																																																																																																						
Head TSL temperature change during test	<1.0 °C	—	—																																																																																																																						
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																																																																																								
SAR measured	100 mW input power	7.94 W/kg																																																																																																																							
SAR for nominal Head TSL parameters	normalized to 1W	79.1 W/kg ± 24.4 % (k=2)																																																																																																																							
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																																																																																																																								
SAR measured	100 mW input power	2.27 W/kg																																																																																																																							
SAR for nominal Head TSL parameters	normalized to 1W	22.6 W/kg ± 24.2 % (k=2)																																																																																																																							
	Temperature	Permittivity	Conductivity																																																																																																																						
Nominal Head TSL parameters	22.0 °C	35.9	4.88 mS/m																																																																																																																						
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.8 ± 6 %	4.84 mS/m ± 6 %																																																																																																																						
Head TSL temperature change during test	<1.0 °C	—	—																																																																																																																						
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																																																																																								
SAR measured	100 mW input power	8.20 W/kg																																																																																																																							
SAR for nominal Head TSL parameters	normalized to 1W	82.6 W/kg ± 24.4 % (k=2)																																																																																																																							
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																																																																																																																								
SAR measured	100 mW input power	2.34 W/kg																																																																																																																							
SAR for nominal Head TSL parameters	normalized to 1W	23.3 W/kg ± 24.2 % (k=2)																																																																																																																							
 In Collaboration with TTL Calibration Laboratory Add: No.52 HuaYuanBao Road, Haidian District, Beijing, 100191, China Tel: +86-10-62592117 E-mail: info@ttsl.com.cn http://www.ttsl.com.cn  CAICT Head TSL parameters at 5600MHz The following parameters and calculations were applied. <table border="1"> <tr> <td></td> <td>Temperature</td> <td>Permittivity</td> <td>Conductivity</td> </tr> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>35.9</td> <td>5.07 mS/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>34.7 ± 6 %</td> <td>5.05 mS/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><1.0 °C</td> <td>—</td> <td>—</td> </tr> </table> SAR result with Head TSL at 5600MHz <table border="1"> <tr> <td>SAR averaged over 1 cm³ (1 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>100 mW input power</td> <td>8.12 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>80.8 W/kg ± 24.4 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm³ (10 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>100 mW input power</td> <td>2.38 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>22.9 W/kg ± 24.2 % (k=2)</td> </tr> </table> Head TSL parameters at 5800MHz The following parameters and calculations were applied. <table border="1"> <tr> <td></td> <td>Temperature</td> <td>Permittivity</td> <td>Conductivity</td> </tr> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>35.9</td> <td>5.27 mS/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>34.4 ± 6 %</td> <td>5.25 mS/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><1.0 °C</td> <td>—</td> <td>—</td> </tr> </table> SAR result with Head TSL at 5800MHz <table border="1"> <tr> <td>SAR averaged over 1 cm³ (1 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>100 mW input power</td> <td>7.71 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>76.7 W/kg ± 24.4 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm³ (10 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>100 mW input power</td> <td>2.16 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>21.6 W/kg ± 24.2 % (k=2)</td> </tr> </table> Certificate No: Z22-40187 Page 3 of 10		Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	35.9	5.07 mS/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	34.7 ± 6 %	5.05 mS/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		SAR measured	100 mW input power	8.12 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	80.8 W/kg ± 24.4 % (k=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		SAR measured	100 mW input power	2.38 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	22.9 W/kg ± 24.2 % (k=2)		Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	35.9	5.27 mS/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	34.4 ± 6 %	5.25 mS/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		SAR measured	100 mW input power	7.71 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	76.7 W/kg ± 24.4 % (k=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		SAR measured	100 mW input power	2.16 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	21.6 W/kg ± 24.2 % (k=2)	 In Collaboration with TTL Calibration Laboratory Add: No.52 HuaYuanBao Road, Haidian District, Beijing, 100191, China Tel: +86-10-62592117 E-mail: info@ttsl.com.cn http://www.ttsl.com.cn  CAICT Appendix (Additional assessments outside the scope of CNAS L0570) Antenna Parameters with Head TSL at 5200MHz <table border="1"> <tr> <td>Impedance, transformed to feed point</td> <td>48.1D-5.03jΩ</</td></tr></table>	Impedance, transformed to feed point	48.1D-5.03jΩ</																																																		
	Temperature	Permittivity	Conductivity																																																																																																																						
Nominal Head TSL parameters	22.0 °C	35.9	5.07 mS/m																																																																																																																						
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.7 ± 6 %	5.05 mS/m ± 6 %																																																																																																																						
Head TSL temperature change during test	<1.0 °C	—	—																																																																																																																						
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																																																																																								
SAR measured	100 mW input power	8.12 W/kg																																																																																																																							
SAR for nominal Head TSL parameters	normalized to 1W	80.8 W/kg ± 24.4 % (k=2)																																																																																																																							
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																																																																																																																								
SAR measured	100 mW input power	2.38 W/kg																																																																																																																							
SAR for nominal Head TSL parameters	normalized to 1W	22.9 W/kg ± 24.2 % (k=2)																																																																																																																							
	Temperature	Permittivity	Conductivity																																																																																																																						
Nominal Head TSL parameters	22.0 °C	35.9	5.27 mS/m																																																																																																																						
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.4 ± 6 %	5.25 mS/m ± 6 %																																																																																																																						
Head TSL temperature change during test	<1.0 °C	—	—																																																																																																																						
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																																																																																								
SAR measured	100 mW input power	7.71 W/kg																																																																																																																							
SAR for nominal Head TSL parameters	normalized to 1W	76.7 W/kg ± 24.4 % (k=2)																																																																																																																							
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																																																																																																																								
SAR measured	100 mW input power	2.16 W/kg																																																																																																																							
SAR for nominal Head TSL parameters	normalized to 1W	21.6 W/kg ± 24.2 % (k=2)																																																																																																																							
Impedance, transformed to feed point	48.1D-5.03jΩ</																																																																																																																								

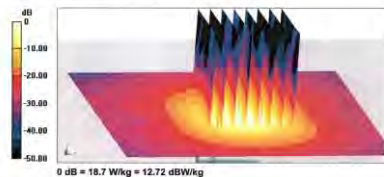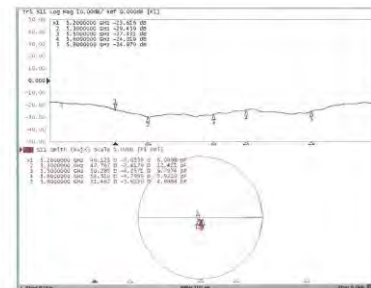  Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: cti@ttsl.com.cn http://www.caiict.com.cn General Antenna Parameters and Design <table border="1"><tr><td>Electrical Delay (one direction)</td><td>1.101 ns</td></tr></table> After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured. The dipole is made of standard semirigid coaxial cable. The carrier conductor of the feeding line is directly connected to the second arm of the dipole. This antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged. Additional EUT Data <table border="1"><tr><td>Manufactured by</td><td>SPEAQ</td></tr></table> Certificate No: Z22-60187 Page 1 of 6	Electrical Delay (one direction)	1.101 ns	Manufactured by	SPEAQ	  Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: cti@ttsl.com.cn http://www.caiict.com.cn DASY5 Validation Report for Head TSL Date: 2022-09-01 Test Laboratory: CTTL, Beijing, China DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1095 Communication System: CW; Frequency: 5200 MHz; Frequency: 5300 MHz; Frequency: 5500 MHz; Frequency: 5600 MHz; Frequency: 5800 MHz; Duty Cycle: 1:1 Medium parameters used: $f = 5200$ MHz; $\sigma = 4.82$ S/m; $\epsilon = 35.39$; $\rho = 1000$ kg/m³ Medium parameters used: $f = 5300$ MHz; $\sigma = 4.73$ S/m; $\epsilon = 35.19$; $\rho = 1000$ kg/m³ Medium parameters used: $f = 5500$ MHz; $\sigma = 4.939$ S/m; $\epsilon = 34.83$; $\rho = 1000$ kg/m³ Medium parameters used: $f = 5600$ MHz; $\sigma = 5.051$ S/m; $\epsilon = 34.89$; $\rho = 1000$ kg/m³ Medium parameters used: $f = 5800$ MHz; $\sigma = 5.247$ S/m; $\epsilon = 34.42$; $\rho = 1000$ kg/m³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C38.19-2007) DASY5 Configuration: - Probe: EX3DV4 - SN7484; ConvF(5.6, 5.6, 5.6) @ 5200 MHz; ConvF(5.32, 5.32, 5.32) @ 5300 MHz; ConvF(5.11, 5.11, 5.11) @ 5500 MHz; ConvF(4.91, 4.91, 4.91) @ 5600 MHz; ConvF(5.5, 5.5) @ 5800 MHz; Calibrated: 2022-01-26 - Sensor-Surface: 1.4mm (Mechanical Surface Detection) - Electronics: DA84 Sn1556; Calibrated: 2022-01-12 - Phantom: MPF_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062 - DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501) Dipole Calibration /Pin=100mW, d=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Reference Value = 60.80 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 29.8 W/kg SAR(1 g) = 7.73 W/kg; SAR(10 g) = 2.22 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 66.8% Maximum value of SAR (measured) = 19.3 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Reference Value = 61.08 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 31.5 W/kg SAR(1 g) = 7.94 W/kg; SAR(10 g) = 2.27 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 65.5% Maximum value of SAR (measured) = 19.0 W/kg Certificate No: Z22-60187 Page 2 of 6
Electrical Delay (one direction)	1.101 ns				
Manufactured by	SPEAQ				
  Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: cti@ttsl.com.cn http://www.caiict.com.cn Dipole Calibration /Pin=100mW, d=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Reference Value = 61.92 V/m; Power Drift = -0.08 dB Peak SAR (extrapolated) = 34.7 W/kg SAR(1 g) = 8.28 W/kg; SAR(10 g) = 2.34 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 63.9% Maximum value of SAR (measured) = 20.2 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Reference Value = 65.08 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 36.3 W/kg SAR(1 g) = 8.12 W/kg; SAR(10 g) = 2.3 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 62.5% Maximum value of SAR (measured) = 19.1 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Reference Value = 62.13 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 34.8 W/kg SAR(1 g) = 7.71 W/kg; SAR(10 g) = 2.16 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 61.6% Maximum value of SAR (measured) = 18.7 W/kg  Certificate No: Z22-60187 Page 3 of 6	  Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: cti@ttsl.com.cn http://www.caiict.com.cn Impedance Measurement Plot for Head TSL  Certificate No: Z22-60187 Page 4 of 6				

2 DAE4 - SN 1305

Calibration Laboratory of Schmid & Partner Engineering AG Zugheisenstrasse 51, 8004 Zurich, Switzerland		Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service	
Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates		Accreditation No.: SCS 0108	
Client: Auden Tessalon City, Taiwan		Certificate No.: DAE4-1305_Apr23	
CALIBRATION CERTIFICATE			
Object: DAE4 - SD D00 D04 BM - SN: 1305			
Calibration procedure(s): QA CAL-06.v30 Calibration procedure for the data acquisition electronics (DAE)			
Calibration date: April 13, 2023			
This calibration certificate documents the traceability to national standards, which resolve the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages, not any part of this certificate.			
All calibrations have been conducted in the closest laboratory facility: environmental temperature (22 ± 3) °C and humidity (45%).			
Calibration equipment used (MUTU critical for calibration)			
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Kettner Multimeter Type 2001	SPV 08102/6	29-Aug-22 (No.34386)	Aug-23
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Auto (DAE) Calibration Unit	SE UMS 903 AA 1002	27-Jan-23 (in house check)	In house check: Jan-24
Calibrator Box V0.1	SE UMS 908 AA 1002	27-Jan-23 (in house check)	In house check: Jan-24
Calibrated by:	Name: Adnan Gökçen	Function: Laboratory Technician	Signature:
Approved by:	Name: Sven Kuhn	Function: Technical Manager	Signature:
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: DAE4-1305_Apr23 Page: 1 of 3			

DC Voltage Measurement			
AD - Converter Resolution Nominal			
High Range: 1LSB = 6.1µV, full range = -100...+300 mV			
Low Range: 1LSB = 0.1mV, full range = -1...+3mV			
DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec			
Calibration Factors	X	Y	Z
High Range	403.819 ± 0.02% (k=2)	403.983 ± 0.02% (k=2)	404.309 ± 0.02% (k=2)
Low Range	3.98113 ± 1.50% (k=2)	3.99180 ± 1.50% (k=2)	3.99636 ± 1.50% (k=2)

Connector Angle	
Connector Angle to be used in DASY system	97.5 ± 1 °

Appendix (Additional assessments outside the scope of SCS0108)			
1. DC Voltage Linearity			
High Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	199995.15	1.24	0.00
Channel X + Input	20002.16	0.20	0.00
Channel X - Input	-19999.30	2.54	-0.01
Channel Y + Input	199993.50	-0.43	-0.00
Channel Y + Input	19999.85	-1.97	-0.01
Channel Y - Input	-20002.21	-0.38	0.00
Channel Z + Input	199995.45	1.29	0.00
Channel Z + Input	20000.56	-1.24	-0.01
Channel Z - Input	-20002.62	-0.64	0.00
Low Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	2001.11	0.15	0.01
Channel X + Input	201.71	0.58	0.29
Channel X - Input	-197.58	1.01	-0.51
Channel Y + Input	1999.81	-1.08	-0.05
Channel Y + Input	200.62	-0.55	-0.27
Channel Y - Input	-199.48	-0.85	0.43
Channel Z + Input	2000.44	-0.39	-0.02
Channel Z + Input	201.23	0.16	0.08
Channel Z - Input	-199.50	-0.73	0.37

2. Common mode sensitivity			
DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec			
	Common mode Input Voltage (mV)	High Range Average Reading (µV)	Low Range Average Reading (µV)
Channel X	200	7.78	6.27
	-200	-4.89	-4.86
Channel Y	200	-22.45	-23.58
	-200	22.23	21.98
Channel Z	200	-8.70	-9.29
	-200	8.76	8.65

3. Channel separation				
DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec				
	Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (µV)
Channel X	200	-	0.51	-3.80
Channel Y	200	8.86	-	2.36
Channel Z	200	10.72	5.96	-

Certificate No: DAE4-1305_Apr23		Page 3 of 3	

Certificate No: DAE4-1305_Apr23		Page 3 of 3	

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15876	18114
Channel Y	18301	17045
Channel Z	15957	13958

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input: 10M Ω

	Average (μ V)	min. Offset (μ V)	max. Offset (μ V)	Std. Deviation (μ V)
Channel X	1.73	0.47	2.81	0.44
Channel Y	-0.21	-2.38	1.70	0.54
Channel Z	0.13	-1.38	1.54	0.55

6. Input Offset Current

Nominal input circuitry offset current on all channels: <25nA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (Mohm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.5
Supply (- Vcc)	-7.6

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-5	-9

Certificate No: DAE4-1305_Apr23

Page 5 of 5

3 EX3DV4 - SN 7833

Calibration Laboratory of
Schmid & Partner
Engineering AG

Sigmundstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificatesB. Schweizerischer Kalibrierdienst
C. Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Client: SOS

Kunshan

Certificate No.

EX-7833_Aug23

CALIBRATION CERTIFICATE

Device: EX3DV4 - SN 7833

Calibration procedure(s): QA CAL-01 v1.0, QA CAL-12 v1.0, QA CAL-14 v7, QA CAL-23 v6,
QA CAL-25 v6
Calibration procedure for dosimetric E-field probes

Calibration date: August 24, 2023

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability as given on the following page are part of the certificate.
All calibrations have been conducted in the closest laboratory facility: uncontrolled temperature 20 $\pm$ 1/1°C and humidity < 75%.

Calibration Equipment used (MATE email for calibration)

Primary Standards	(1)	Cal. Date (Certificate No.)	Next Valid Calibration
Power meter RM22	SN 104778	30 May 23 No. 217-0384203601	Mar-24
Power sensor NRP-31	SN 133341	30 May 23 No. 217-0384203601	Mar-24
DOF DAK-3 (Integrated)	SN 7148	30 Oct 22 (DOF DAK-3 v144) (Oct22)	Oct-23
DOF DAK-12	SN 1014	27 Oct 22 (DOF DAK-12 v176) (Oct22)	Oct-23
Reference 50 dB Attenuator	SN 025852 (20v)	30 Mar 23 No. 217-0384203601	Mar-24
DAK4	SN 986	19 Mar 23 No. DAK4-662_May23	Mar-24
Reference Probe E53C02	SN 3013	25 Jan 23 No. E53-3013_May23	Jan-24
Secondary Standards	(2)	Check Date in house	Next Valid Calibration
Power meter E241B5	SN 0841206874	06 Apr 18 In house check Jun-23	In house check Jun-24
Power sensor E241B5	SN 1011168090	06 Apr 18 In house check Jun-23	In house check Jun-24
Power sensor E241B5	SN 0031102615	06 Apr 18 In house check Jun-23	In house check Jun-24
Ref. generator HP 85950	SN 035604071750	01 Aug 23 In house check Jun-23	In house check Jun-24
Network Analyzer E5366A	SN 0841089477	31 Mar 14 In house check Dec-23	In house check Dec-24

Calibrated by: Name: Jochen Kalmel, Position: Laboratory Technician, Signature: [Signature]

Approved by: Name: Gisel Kalmel, Position: Technical Manager, Signature: [Signature]

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Issued: August 28, 2023

Certificate No: EX-7833_Aug23

Page 1 of 32

Calibration Laboratory of
Schmid & Partner
Engineering AG

Sigmundstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificatesB. Schweizerischer Kalibrierdienst
C. Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Glossary

TSL: Total Summing Level
NORM_{xyz}: sensitivity in free space
Conf: confidence interval
DOF: degrees of freedom
A, B, C, D: modulation dependent inactivation parameters
Polarization: direction around probe axis
Polarization: direction around probe axis
normal to probe axis
Connector Angle: information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEC 61331-1:2009-1532: Measurement Procedure for The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1532: Human Models, Instrumentation And Procedures (Frequency Ranges of 4 MHz to 10 GHz), October 2009.
- IEC 61331-1:2009-1532: Measurement Procedure for The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1532: Human Models, Instrumentation And Procedures (Frequency Ranges of 4 MHz to 10 GHz), October 2009.

Methods Applied and Interpretation of Parameters:

- NORM_{xyz}: Assessed for E-field polarization ($\theta = 0$) ($f < 300$ MHz in TEH mode, $f > 300$ MHz in TEM mode). NORM_{xyz} are any intermediate values, i.e. the uncertainties of NORM_{xyz} do not affect the E-field uncertainty inside TSL (see below Conf).
- NORM_{xyz}: NORM_{xyz} frequency response (see Frequency Response Chart). This inactivation is implemented in DASY4 software version later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of Conf.
- DOF: DOF are numerical inactivation parameters assessed based on the data of power sweeps with CW signal. DOF does not depend on frequency nor media.
- RA: RA is the Ratio of Average Ratio that is not calibrated but determined based on the signal characteristics.
- A, B, C, D: A, B, C, D are numerical inactivation parameters determined based on the data of power sweeps for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the dose.
- Conf and Boundary Effect Parameters: Assessed in free phantom using E-field or Temperature Trigger Standard for 1 s (DOF=1) and in-house response using analytical field distributions based on power measurements for 1-300 MHz. The same setup is used for assessment of the parameters applied for boundary compensation (apex, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{xyz} "Dose" whereby the uncertainty corresponds to that given for Conf. A frequency dependent Conf is used in DASY version 4.4 and higher which allows extending the validity from 100 MHz to 100 MHz.
- Spatial history (3D division flow history): In a field of low gradients realized using a flat phantom exposed by a planar antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (in probe axis). No reference required.
- Connector Angle: The angle is assessed using the information gained by determining the NORM_{xyz} (no uncertainty required).

Certificate No: EX-7833_Aug23

Page 2 of 32

EX3DV4 - SN:7833

August 24, 2023

Parameters of Probe: EX3DV4 - SN:7833

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k = 2)
Norm $(\mu V/V/m)^2$ A	0.40	0.65	0.59	$\pm 10.1\%$
DOF (mv) B	111.0	108.3	108.3	$\pm 4.7\%$

Calibration Results for Modulation Response

UID	Communication System Name	A dB	B dB	C	D dB	VR mV	Max dev.	Max Unc ^a k = 2
0	CW	X 0.00 Y 0.00 Z 0.00	0.00 0.00 0.00	1.00 1.00 1.00	0.00 0.00 0.00	136.2 136.2 136.2	$\pm 0.2\%$	$\pm 4.7\%$
10352	Pulse Waveform (200Hz, 10%)	X 1.41 Y 1.37 Z 1.37	62.30 61.59 60.88	6.14 6.01 6.00	10.00 10.00 10.00	60.0 60.0 60.0	$\pm 3.2\%$	$\pm 9.8\%$
10353	Pulse Waveform (200Hz, 20%)	X 10.00 Y 10.00 Z 10.00	72.00 72.00 72.00	9.00 9.00 9.00	6.99 6.99 6.99	80.0 80.0 80.0	$\pm 2.9\%$	$\pm 9.8\%$
10354	Pulse Waveform (200Hz, 40%)	X 3.57 Y 3.56 Z 3.56	66.00 65.00 64.00	3.64 3.58 3.54	3.96 3.90 3.86	96.0 95.0 94.0	$\pm 2.8\%$	$\pm 9.8\%$
10355	Pulse Waveform (200Hz, 60%)	X 7.95 Y 7.95 Z 7.95	77.52 77.52 77.52	2.05 2.05 2.05	2.22 2.22 2.22	100.0 100.0 100.0	$\pm 1.7\%$	$\pm 9.8\%$
10357	QPSK Waveform, 1MHz	X 0.37 Y 0.37 Z 0.48	66.00 66.00 64.00	14.25 14.25 12.04	1.00 1.00 1.00	100.0 100.0 100.0	$\pm 3.9\%$	$\pm 9.8\%$
10358	QPSK Waveform, 10MHz	X 1.43 Y 1.39 Z 1.25	67.67 65.56 62.73	14.98 13.88 13.78	0.00 0.00 0.00	100.0 100.0 100.0	$\pm 0.9\%$	$\pm 9.8\%$
10396	64-QAM Waveform, 100KHz	X 1.77 Y 1.79 Z 1.76	65.62 65.30 64.45	18.47 18.35 18.14	3.01 3.01 3.01	100.0 100.0 100.0	$\pm 1.0\%$	$\pm 9.8\%$
10399	64-QAM Waveform, 40MHz	X 1.51 Y 1.51 Z 1.51	65.91 65.89 65.89	15.44 15.34 15.34	0.00 0.00 0.00	100.0 100.0 100.0	$\pm 2.1\%$	$\pm 9.8\%$
10414	WLAN CDD, 64-QAM, 40 MHz	X 3.87 Y 3.87 Z 3.87	66.00 66.00 66.00	15.69 15.69 15.69	3.00 3.00 3.00	100.0 100.0 100.0	$\pm 3.5\%$	$\pm 9.8\%$

Note: For details on UID parameters see Appendix

The reported uncertainty of measurement is based on the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^a The uncertainties of Norm X,Y,Z do not affect the 67% test uncertainty (see TS, see Page 5 and 6).

^b Precision parameter uncertainty for maximum specified field strength.

^c Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Certificate No: EX-7833_Aug23

Page 3 of 22

EX3DV4 - SN:7833

August 24, 2023

Parameters of Probe: EX3DV4 - SN:7833

Sensor Model Parameters

	C1 dB	C2 dB	A V/m	V1 mV/V	V2 mV/V	T3 mm	T4 mm	T5 mm	T6 mm
X	8.5	69.54	31.91	4.38	0.30	4.30	0.61	0.00	1.00
Y	8.5	69.77	32.80	4.19	0.30	4.30	0.61	0.00	1.00
Z	7.3	51.94	32.49	3.79	0.30	4.30	0.61	0.00	1.00

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle	30°
Mechanical Surface Detection Mode	disabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	16 mm
Tip Diameter	9 mm
Tip Length	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

Note: Measurement distance from surface can be increased to 3.4 mm for an Apple iPhone.

Certificate No: EX-7833_Aug23

Page 4 of 22

EX3DV4 - SN:7833

August 24, 2023

Parameters of Probe: EX3DV4 - SN:7833

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^a	Relative Permittivity ^b	Conductivity ^c (S/m)	CompF X	CompF Y	CompF Z	Alpha ^d	Depth ^e (mm)	Unc (k = 2)
750	41.9	0.09	7.85	8.96	8.55	0.43	1.27	$\pm 12.0\%$
835	41.5	0.90	7.57	8.62	8.54	0.42	1.27	$\pm 12.0\%$
1750	40.1	1.37	7.08	8.09	7.65	0.28	1.27	$\pm 12.0\%$
1900	40.0	1.40	6.39	7.26	5.93	0.31	1.27	$\pm 12.0\%$
2150	39.8	1.49	6.25	7.10	6.75	0.32	1.27	$\pm 12.0\%$
2300	39.5	1.57	6.07	6.82	6.58	0.33	1.27	$\pm 12.0\%$
2450	39.2	1.60	5.98	6.77	6.44	0.31	1.27	$\pm 12.0\%$
2600	39.0	1.95	5.11	6.91	6.68	0.30	1.27	$\pm 12.0\%$
3300	38.2	2.71	6.16	7.02	6.67	0.34	1.27	$\pm 14.0\%$
3500	37.9	2.91	5.61	6.40	6.07	0.36	1.27	$\pm 14.0\%$
3700	37.7	3.12	5.65	6.46	6.15	0.32	1.30	$\pm 14.0\%$
3900	37.5	3.32	6.07	6.91	6.66	0.38	1.27	$\pm 14.0\%$
4100	37.2	3.53	5.78	6.58	6.21	0.37	1.27	$\pm 14.0\%$
4200	37.1	3.63	5.41	6.17	5.88	0.36	1.27	$\pm 14.0\%$
4400	36.9	3.84	5.25	5.95	5.69	0.37	1.27	$\pm 14.0\%$
4600	36.7	4.04	5.88	6.44	6.12	0.36	1.30	$\pm 14.0\%$
4800	36.4	4.25	5.77	6.55	6.25	0.38	1.27	$\pm 14.0\%$
4950	36.3	4.40	5.26	5.93	5.69	0.41	1.30	$\pm 14.0\%$
5200	36.0	4.88	5.16	5.87	5.61	0.34	1.51	$\pm 14.0\%$
5300	35.9	4.76	5.02	5.70	5.39	0.32	1.63	$\pm 14.0\%$
5500	35.6	4.96	4.50	5.15	4.85	0.36	1.61	$\pm 14.0\%$
5600	35.5	5.07	4.33	4.92	4.65	0.41	1.54	$\pm 14.0\%$
5800	35.3	5.27	4.50	5.13	4.87	0.31	1.66	$\pm 14.0\%$

^a Frequency validity above 802.1084 of $\pm 10\%$ only applies for QMS v4.4 and higher (see Page 2), when it is specified to $\pm 10\%$. The uncertainty is the max of the center uncertainty of calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 802.1084 is $\pm 10\%$, $\pm 15\%$, $\pm 20\%$, $\pm 25\%$, $\pm 30\%$, $\pm 35\%$, $\pm 40\%$, $\pm 45\%$, $\pm 50\%$, $\pm 55\%$, $\pm 60\%$, $\pm 65\%$, $\pm 70\%$, $\pm 75\%$, $\pm 80\%$, $\pm 85\%$, $\pm 90\%$, $\pm 95\%$, $\pm 100\%$ respectively. Validity of CompF parameter is $\pm 10\%$, $\pm 15\%$, $\pm 20\%$, $\pm 25\%$, $\pm 30\%$, $\pm 35\%$, $\pm 40\%$, $\pm 45\%$, $\pm 50\%$, $\pm 55\%$, $\pm 60\%$, $\pm 65\%$, $\pm 70\%$, $\pm 75\%$, $\pm 80\%$, $\pm 85\%$, $\pm 90\%$, $\pm 95\%$, $\pm 100\%$ respectively.

^b The permittivity values are determined using data from the literature and are rounded to $\pm 10\%$.

^c The conductivity values are determined using data from the literature and are rounded to $\pm 10\%$.

^d AlphaDepth is determined during calibration. SPAD warns that the boundary effect due to the boundary effect after compensation is always less than $\pm 1\%$ for frequencies below 3 GHz and below $\pm 2\%$ for frequencies between 3-6 GHz and any distance larger than half the probe diameter from the boundary.

^e AlphaDepth is determined during calibration. SPAD warns that the boundary effect due to the boundary effect after compensation is always less than $\pm 1\%$ for frequencies below 3 GHz and below $\pm 2\%$ for frequencies between 3-6 GHz and any distance larger than half the probe diameter from the boundary.

Certificate No: EX-7833_Aug23

Page 5 of 22

EX3DV4 - SN:7833

August 24, 2023

Parameters of Probe: EX3DV4 - SN:7833

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^a	Relative Permittivity ^b	Conductivity ^c (S/m)	CompF X	CompF Y	CompF Z	Alpha ^d	Depth ^e (mm)	Unc (k = 2)
6500	34.5	6.07	6.74	5.36	4.91	0.20	2.00	$\pm 18.6\%$

^a Frequency validity at 6.5 GHz is $\pm 10\%$ only applies for QMS v4.4 and higher (see Page 2), when it is specified to $\pm 10\%$. The uncertainty is the max of the center uncertainty of calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 6500 MHz is $\pm 10\%$, $\pm 15\%$, $\pm 20\%$, $\pm 25\%$, $\pm 30\%$, $\pm 35\%$, $\pm 40\%$, $\pm 45\%$, $\pm 50\%$, $\pm 55\%$, $\pm 60\%$, $\pm 65\%$, $\pm 70\%$, $\pm 75\%$, $\pm 80\%$, $\pm 85\%$, $\pm 90\%$, $\pm 95\%$, $\pm 100\%$ respectively. Validity of CompF parameter is $\pm 10\%$, $\pm 15\%$, $\pm 20\%$, $\pm 25\%$, $\pm 30\%$, $\pm 35\%$, $\pm 40\%$, $\pm 45\%$, $\pm 50\%$, $\pm 55\%$, $\pm 60\%$, $\pm 65\%$, $\pm 70\%$, $\pm 75\%$, $\pm 80\%$, $\pm 85\%$, $\pm 90\%$, $\pm 95\%$, $\pm 100\%$ respectively.

^b The permittivity values are determined using data from the literature and are rounded to $\pm 10\%$.


^c The conductivity values are determined using data from the literature and are rounded to $\pm 10\%$.

^d AlphaDepth is determined during calibration. SPAD warns that the boundary effect due to the boundary effect after compensation is always less than $\pm 1\%$ for frequencies below 3 GHz and below $\pm 2\%$ for frequencies between 3-6 GHz and any distance larger than half the probe diameter from the boundary.

^e AlphaDepth is determined during calibration. SPAD warns that the boundary effect due to the boundary effect after compensation is always less than $\pm 1\%$ for frequencies below 3 GHz and below $\pm 2\%$ for frequencies between 3-6 GHz and any distance larger than half the probe diameter from the boundary.

Certificate No: EX-7833_Aug23

Page 6 of 22

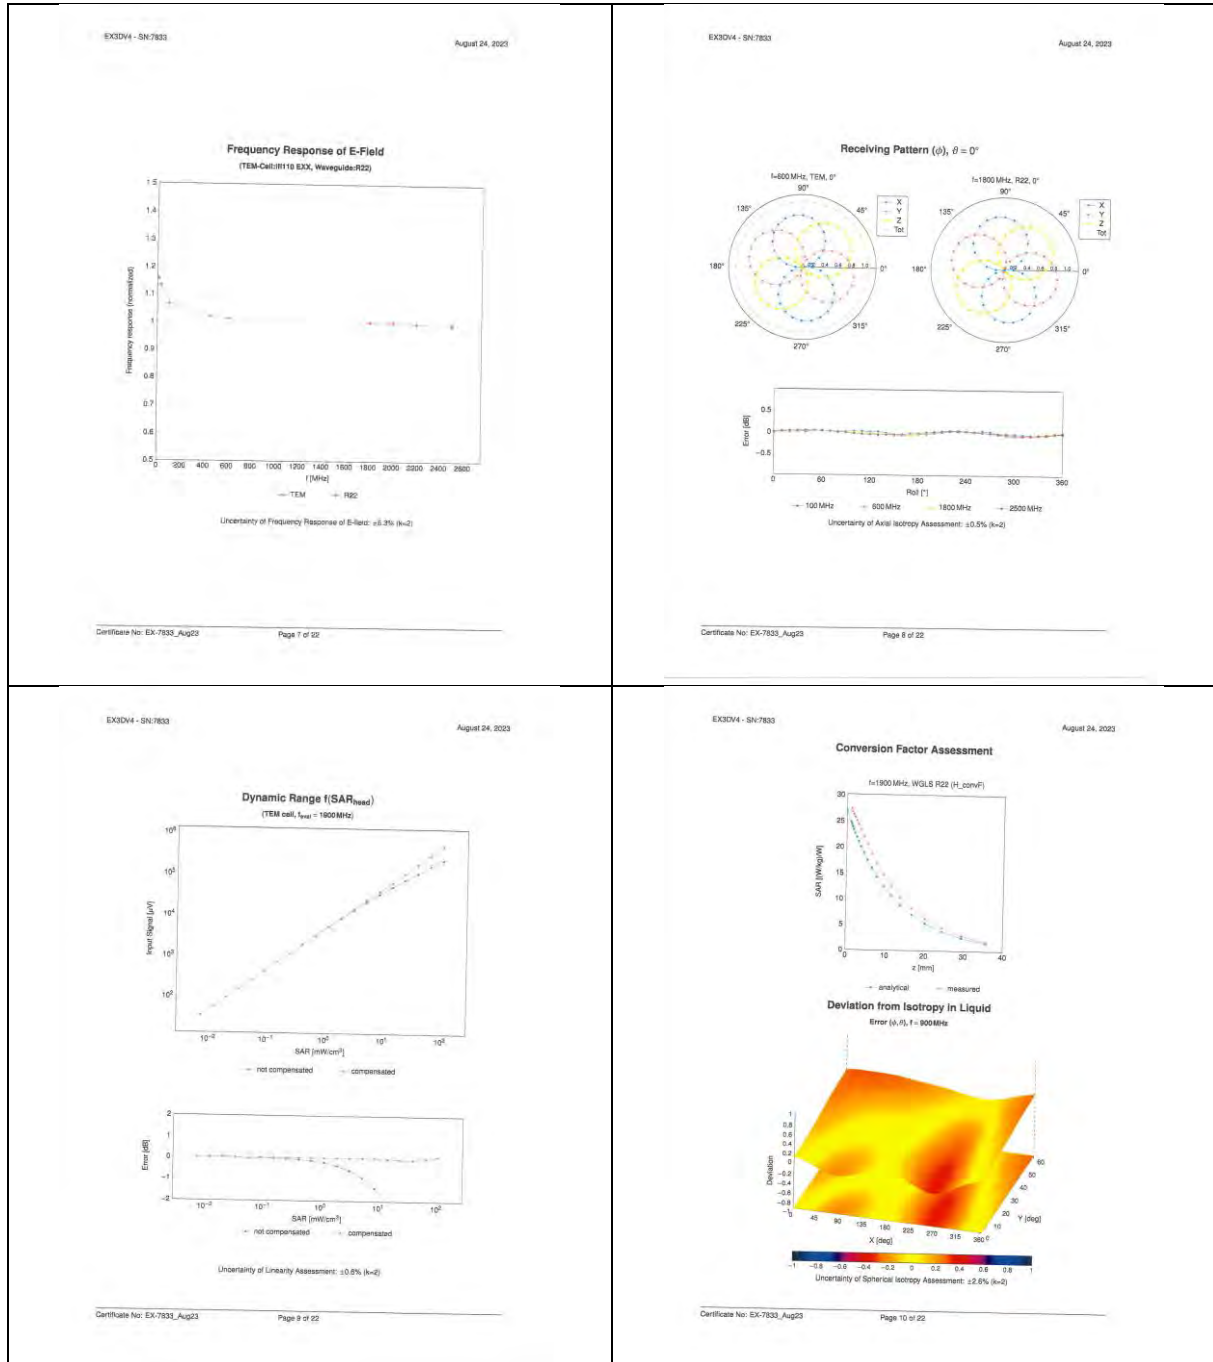

EX3DV4 - SN:7833 August 24, 2021

[illegible]

Certificate No: EX-7833_Aug23

Page 15 of 22

EXSDV4 - SN:7833 August 24, 2002

USP	Rev	Communication System Name	Category	Peak (dB)	Chn #
1531	AAZ	IEEE 802.11a WPAN (802.11a)	WPAN	8.40	28
1532	AAZ	IEEE 802.11b WPAN (802.11b)	WPAN	8.40	28
1533	AAZ	IEEE 802.11g WPAN (802.11g)	WPAN	8.40	28
1534	AAZ	IEEE 802.11n WPAN (802.11n)	WPAN	8.40	28
1535	AAZ	IEEE 802.11ac WPAN (802.11ac)	WPAN	8.40	28
1536	AAZ	IEEE 802.11ad WPAN (802.11ad)	WPAN	8.40	28
1537	AAZ	IEEE 802.11ah WPAN (802.11ah)	WPAN	8.40	28
1538	AAZ	IEEE 802.11ay WPAN (802.11ay)	WPAN	8.40	28
1539	AAZ	IEEE 802.11az WPAN (802.11az)	WPAN	8.40	28
1540	AAZ	IEEE 802.11ba WPAN (802.11ba)	WPAN	8.40	28
1541	AAZ	IEEE 802.11bb WPAN (802.11bb)	WPAN	8.40	28
1542	AAZ	IEEE 802.11bc WPAN (802.11bc)	WPAN	8.40	28
1543	AAZ	IEEE 802.11bd WPAN (802.11bd)	WPAN	8.40	28
1544	AAZ	IEEE 802.11be WPAN (802.11be)	WPAN	8.40	28
1545	AAZ	IEEE 802.11bf WPAN (802.11bf)	WPAN	8.40	28
1546	AAZ	IEEE 802.11bg WPAN (802.11bg)	WPAN	8.40	28
1547	AAZ	IEEE 802.11bh WPAN (802.11bh)	WPAN	8.40	28
1548	AAZ	IEEE 802.11bi WPAN (802.11bi)	WPAN	8.40	28
1549	AAZ	IEEE 802.11bj WPAN (802.11bj)	WPAN	8.40	28
1550	AAZ	IEEE 802.11bk WPAN (802.11bk)	WPAN	8.40	28
1551	AAZ	IEEE 802.11bl WPAN (802.11bl)	WPAN	8.40	28
1552	AAZ	IEEE 802.11bm WPAN (802.11bm)	WPAN	8.40	28
1553	AAZ	IEEE 802.11bn WPAN (802.11bn)	WPAN	8.40	28
1554	AAZ	IEEE 802.11bo WPAN (802.11bo)	WPAN	8.40	28
1555	AAZ	IEEE 802.11bp WPAN (802.11bp)	WPAN	8.40	28
1556	AAZ	IEEE 802.11bq WPAN (802.11bq)	WPAN	8.40	28
1557	AAZ	IEEE 802.11br WPAN (802.11br)	WPAN	8.40	28
1558	AAZ	IEEE 802.11bs WPAN (802.11bs)	WPAN	8.40	28
1559	AAZ	IEEE 802.11bt WPAN (802.11bt)	WPAN	8.40	28
1560	AAZ	IEEE 802.11bu WPAN (802.11bu)	WPAN	8.40	28
1561	AAZ	IEEE 802.11bv WPAN (802.11bv)	WPAN	8.40	28
1562	AAZ	IEEE 802.11bw WPAN (802.11bw)	WPAN	8.40	28
1563	AAZ	IEEE 802.11bx WPAN (802.11bx)	WPAN	8.40	28
1564	AAZ	IEEE 802.11by WPAN (802.11by)	WPAN	8.40	28
1565	AAZ	IEEE 802.11bz WPAN (802.11bz)	WPAN	8.40	28
1566	AAZ	IEEE 802.11c WPAN (802.11c)	WPAN	8.40	28
1567	AAZ	IEEE 802.11d WPAN (802.11d)	WPAN	8.40	28
1568	AAZ	IEEE 802.11e WPAN (802.11e)	WPAN	8.40	28
1569	AAZ	IEEE 802.11f WPAN (802.11f)	WPAN	8.40	28
1570	AAZ	IEEE 802.11g WPAN (802.11g)	WPAN	8.40	28
1571	AAZ	IEEE 802.11h WPAN (802.11h)	WPAN	8.40	28
1572	AAZ	IEEE 802.11i WPAN (802.11i)	WPAN	8.40	28
1573	AAZ	IEEE 802.11j WPAN (802.11j)	WPAN	8.40	28
1574	AAZ	IEEE 802.11k WPAN (802.11k)	WPAN	8.40	28
1575	AAZ	IEEE 802.11l WPAN (802.11l)	WPAN	8.40	28
1576	AAZ	IEEE 802.11m WPAN (802.11m)	WPAN	8.40	28
1577	AAZ	IEEE 802.11n WPAN (802.11n)	WPAN	8.40	28
1578	AAZ	IEEE 802.11o WPAN (802.11o)	WPAN	8.40	28
1579	AAZ	IEEE 802.11p WPAN (802.11p)	WPAN	8.40	28
1580	AAZ	IEEE 802.11q WPAN (802.11q)	WPAN	8.40	28
1581	AAZ	IEEE 802.11r WPAN (802.11r)	WPAN	8.40	28
1582	AAZ	IEEE 802.11s WPAN (802.11s)	WPAN	8.40	28
1583	AAZ	IEEE 802.11t WPAN (802.11t)	WPAN	8.40	28
1584	AAZ	IEEE 802.11u WPAN (802.11u)	WPAN	8.40	28
1585	AAZ	IEEE 802.11v WPAN (802.11v)	WPAN	8.40	28
1586	AAZ	IEEE 802.11w WPAN (802.11w)	WPAN	8.40	28
1587	AAZ	IEEE 802.11x WPAN (802.11x)	WPAN	8.40	28
1588	AAZ	IEEE 802.11y WPAN (802.11y)	WPAN	8.40	28
1589	AAZ	IEEE 802.11z WPAN (802.11z)	WPAN	8.40	28
1590	AAZ	IEEE 802.11aa WPAN (802.11aa)	WPAN	8.40	28
1591	AAZ	IEEE 802.11ab WPAN (802.11ab)	WPAN	8.40	28
1592	AAZ	IEEE 802.11ac WPAN (802.11ac)	WPAN	8.40	28
1593	AAZ	IEEE 802.11ad WPAN (802.11ad)	WPAN	8.40	28
1594	AAZ	IEEE 802.11ae WPAN (802.11ae)	WPAN	8.40	28
1595	AAZ	IEEE 802.11af WPAN (802.11af)	WPAN	8.40	28
1596	AAZ	IEEE 802.11ag WPAN (802.11ag)	WPAN	8.40	28
1597	AAZ	IEEE 802.11ah WPAN (802.11ah)	WPAN	8.40	28
1598	AAZ	IEEE 802.11ai WPAN (802.11ai)	WPAN	8.40	28
1599	AAZ	IEEE 802.11aj WPAN (802.11aj)	WPAN	8.40	28
1600	AAZ	IEEE 802.11ak WPAN (802.11ak)	WPAN	8.40	28
1601	AAZ	IEEE 802.11al WPAN (802.11al)	WPAN	8.40	28
1602	AAZ	IEEE 802.11am WPAN (802.11am)	WPAN	8.40	28
1603	AAZ	IEEE 802.11an WPAN (802.11an)	WPAN	8.40	28
1604	AAZ	IEEE 802.11ao WPAN (802.11ao)	WPAN	8.40	28
1605	AAZ	IEEE 802.11ap WPAN (802.11ap)	WPAN	8.40	28
1606	AAZ	IEEE 802.11aq WPAN (802.11aq)	WPAN	8.40	28
1607	AAZ	IEEE 802.11ar WPAN (802.11ar)	WPAN	8.40	28
1608	AAZ	IEEE 802.11as WPAN (802.11as)	WPAN	8.40	28
1609	AAZ	IEEE 802.11at WPAN (802.11at)	WPAN	8.40	28
1610	AAZ	IEEE 802.11au WPAN (802.11au)	WPAN	8.40	28
1611	AAZ	IEEE 802.11av WPAN (802.11av)	WPAN	8.40	28
1612	AAZ	IEEE 802.11aw WPAN (802.11aw)	WPAN	8.40	28
1613	AAZ	IEEE 802.11ax WPAN (802.11ax)	WPAN	8.40	28
1614	AAZ	IEEE 802.11ay WPAN (802.11ay)	WPAN	8.40	28
1615	AAZ	IEEE 802.11az WPAN (802.11az)	WPAN	8.40	28
1616	AAZ	IEEE 802.11ba WPAN (802.11ba)	WPAN	8.40	28
1617	AAZ	IEEE 802.11bb WPAN (802.11bb)	WPAN	8.40	28
1618	AAZ	IEEE 802.11bc WPAN (802.11bc)	WPAN	8.40	28
1619	AAZ	IEEE 802.11bd WPAN (802.11bd)	WPAN	8.40	28
1620	AAZ	IEEE 802.11be WPAN (802.11be)	WPAN	8.40	28
1621	AAZ	IEEE 802.11bf WPAN (802.11bf)	WPAN	8.40	28
1622	AAZ	IEEE 802.11bg WPAN (802.11bg)	WPAN	8.40	28
1623	AAZ	IEEE 802.11bh WPAN (802.11bh)	WPAN	8.40	28
1624	AAZ	IEEE 802.11bi WPAN (802.11bi)	WPAN	8.40	28
1625	AAZ	IEEE 802.11bj WPAN (802.11bj)	WPAN	8.40	28
1626	AAZ	IEEE 802.11bk WPAN (802.11bk)	WPAN	8.40	28
1627	AAZ	IEEE 802.11bl WPAN (802.11bl)	WPAN	8.40	28
1628	AAZ	IEEE 802.11bm WPAN (802.11bm)	WPAN	8.40	28
1629	AAZ	IEEE 802.11bn WPAN (802.11bn)	WPAN	8.40	28
1630	AAZ	IEEE 802.11bo WPAN (802.11bo)	WPAN	8.40	28
1631	AAZ	IEEE 802.11bp WPAN (802.11bp)	WPAN	8.40	28
1632	AAZ	IEEE 802.11bq WPAN (802.11bq)	WPAN	8.40	28
1633	AAZ	IEEE 802.11br WPAN (802.11br)	WPAN	8.40	28
1634	AAZ	IEEE 802.11bs WPAN (802.11bs)	WPAN	8.40	28
1635	AAZ	IEEE 802.11bt WPAN (802.11bt)	WPAN	8.40	28
1636	AAZ	IEEE 802.11bu WPAN (802.11bu)	WPAN	8.40	28
1637	AAZ	IEEE 802.11bv WPAN (802.11bv)	WPAN	8.40	28
1638	AAZ	IEEE 802.11bw WPAN (802.11bw)	WPAN	8.40	28
1639	AAZ	IEEE 802.11bx WPAN (802.11bx)	WPAN	8.40	28
1640	AAZ	IEEE 802.11by WPAN (802.11by)	WPAN	8.40	28
1641	AAZ	IEEE 802.11bz WPAN (802.11bz)	WPAN	8.40	28
1642	AAZ	IEEE 802.11c WPAN (802.11c)	WPAN	8.40	28
1643	AAZ	IEEE 802.11d WPAN (802.11d)	WPAN	8.40	28
1644	AAZ	IEEE 802.11e WPAN (802.11e)	WPAN	8.40	28
1645	AAZ	IEEE 802.11f WPAN (802.11f)	WPAN	8.40	28
1646	AAZ	IEEE 802.11g WPAN (802.11g)	WPAN	8.40	28
1647	AAZ	IEEE 802.11h WPAN (802.11h)	WPAN	8.40	28
1648	AAZ	IEEE 802.11i WPAN (802.11i)	WPAN	8.40	28
1649	AAZ	IEEE 802.11j WPAN (802.11j)	WPAN	8.40	28
1650	AAZ	IEEE 802.11k WPAN (802.11k)	WPAN	8.40	28
1651	AAZ	IEEE 802.11l WPAN (802.11l)	WPAN	8.40	28
1652	AAZ	IEEE 802.11m WPAN (802.11m)	WPAN	8.40	28
1653	AAZ	IEEE 802.11n WPAN (802.11n)	WPAN	8.40	28
1654	AAZ	IEEE 802.11o WPAN (802.11o)	WPAN	8.40	28
1655	AAZ	IEEE 802.11p WPAN (802.11p)	WPAN	8.40	28
1656	AAZ	IEEE 802.11q WPAN (802.11q)	WPAN	8.40	28
1657	AAZ	IEEE 802.11r WPAN (802.11r)	WPAN	8.40	28
1658	AAZ	IEEE 802.11s WPAN (802.11s)	WPAN	8.40	28
1659	AAZ	IEEE 802.11t WPAN (802.11t)	WPAN	8.40	28
1660	AAZ	IEEE 802.11u WPAN (802.11u)	WPAN	8.40	28
1661	AAZ	IEEE 802.11v WPAN (802.11v)	WPAN	8.40	28
1662	AAZ	IEEE 802.11w WPAN (802.11w)	WPAN	8.40	28
1663	AAZ	IEEE 802.11x WPAN (802.11x)	WPAN	8.40	28
1664	AAZ	IEEE 802.11y WPAN (802.11y)	WPAN	8.40	28
1665	AAZ	IEEE 802.11z WPAN (802.11z)	WPAN	8.40	28
1666	AAZ	IEEE 802.11aa WPAN (802.11aa)	WPAN	8.40	28
1667	AAZ	IEEE 802.11ab WPAN (802.11ab)	WPAN	8.40	28
1668	AAZ	IEEE 802.11ac WPAN (802.11ac)	WPAN	8.40	28
1669	AAZ	IEEE 802.11ad WPAN (802.11ad)	WPAN	8.40	28
1670	AAZ	IEEE 802.11ae WPAN (802.11ae)	WPAN	8.40	28
1671	AAZ	IEEE 802.11af WPAN (802.11af)	WPAN	8.40	28
1672	AAZ	IEEE 802.11ag WPAN (802.11ag)	WPAN	8.40	28
1673	AAZ	IEEE 802.11ah WPAN (802.11ah)	WPAN	8.40	28
1674	AAZ	IEEE 802.11ai WPAN (802.11ai)	WPAN	8.40	28
1675	AAZ	IEEE 802.11aj WPAN (802.11aj)	WPAN	8.40	28
1676	AAZ	IEEE 802.11ak WPAN (802.11ak)	WPAN	8.40	28
1677	AAZ	IEEE 802.11al WPAN (802.11al)	WPAN	8.40	28
1678	AAZ	IEEE 802.11am WPAN (802.11am)	WPAN	8.40	28
1679	AAZ	IEEE 802.11an WPAN (802.11an)	WPAN	8.40	28
1680	AAZ	IEEE 802.11ao WPAN (802.11ao)	WPAN	8.40	28
1681	AAZ	IEEE 802.11ap WPAN (802.11ap)	WPAN	8.40	28
1682	AAZ	IEEE 802.11aq WPAN (802.11aq)	WPAN	8.40	28
1683	AAZ	IEEE 802.11ar WPAN (802.11ar)	WPAN	8.40	28
1684	AAZ	IEEE 802.11as WPAN (802.11as)	WPAN	8.40	28
1685	AAZ	IEEE 802.11at WPAN (802.11at)	WPAN	8.40	28
1686	AAZ	IEEE 802.11au WPAN (802.11au)	WPAN	8.40	28
1687	AAZ	IEEE 802.11av WPAN (802.11av)	WPAN	8.40	28
1688	AAZ	IEEE 802.11aw WPAN (802.11aw)	WPAN	8.40	28
1689	AAZ	IEEE 802.11ax WPAN (802.11ax)	WPAN	8.40	28
1690	AAZ	IEEE 802.11ay WPAN (802.11ay)	WPAN	8.40	28
1691	AAZ	IEEE 802.11az WPAN (802.11az)	WPAN	8.40	28
1692	AAZ	IEEE 802.11ba WPAN (802.11ba)	WPAN	8.40	28
1693	AAZ	IEEE 802.11bb WPAN (802.11bb)	WPAN	8.40	28
1694	AAZ	IEEE 802.11bc WPAN (802.11bc)	WPAN	8.40	28
1695	AAZ	IEEE 802.11bd WPAN (802.11bd)	WPAN	8.40	28
1696	AAZ	IEEE 802.11be WPAN (802.11be)	WPAN	8.40	28
1697	AAZ	IEEE 802.11bf WPAN (802.11bf)	WPAN	8.40	28
1698	AAZ	IEEE 802.11bg WPAN (802.11bg)	WPAN	8.40	28
1699	AAZ	IEEE 802.11bh WPAN (802.11bh)	WPAN	8.40	28
1700	AAZ	IEEE 802.11bi WPAN (802.11bi)	WPAN	8.40	28

Certificate No: EX-7833_Aug23

Page 16 of 21

EX3DV4 - SN:7833 August 24, 2002

ISO	Ref	Configuration Signature Notes	Group	Min (dB)	Unit	dB
1009	AC	IEEE Std 1394-1995, 1394a, 1394b, 1394c, 1394d, 1394e, 1394f, 1394g, 1394h, 1394i, 1394j, 1394k, 1394l, 1394m, 1394n, 1394o, 1394p, 1394q, 1394r, 1394s, 1394t, 1394u, 1394v, 1394w, 1394x, 1394y, 1394z, 1394aa, 1394ab, 1394ac, 1394ad, 1394ae, 1394af, 1394ag, 1394ah, 1394ai, 1394aj, 1394ak, 1394al, 1394am, 1394an, 1394ao, 1394ap, 1394aq, 1394ar, 1394as, 1394at, 1394au, 1394av, 1394aw, 1394ax, 1394ay, 1394az, 1394ba, 1394bb, 1394bc, 1394bd, 1394be, 1394bf, 1394bg, 1394bh, 1394bi, 1394bj, 1394bk, 1394bl, 1394bm, 1394bn, 1394bo, 1394bp, 1394bq, 1394br, 1394bs, 1394bt, 1394bu, 1394bv, 1394bw, 1394bx, 1394by, 1394bz, 1394ca, 1394cb, 1394cc, 1394cd, 1394ce, 1394cf, 1394cg, 1394ch, 1394ci, 1394cj, 1394ck, 1394cl, 1394cm, 1394cn, 1394co, 1394cp, 1394cq, 1394cr, 1394cs, 1394ct, 1394cu, 1394cv, 1394cw, 1394cx, 1394cy, 1394cz, 1394da, 1394db, 1394dc, 1394dd, 1394de, 1394df, 1394dg, 1394dh, 1394di, 1394dj, 1394dk, 1394dl, 1394dm, 1394dn, 1394do, 1394dp, 1394dq, 1394dr, 1394ds, 1394dt, 1394du, 1394dv, 1394dw, 1394dx, 1394dy, 1394dz, 1394ea, 1394eb, 1394ec, 1394ed, 1394ee, 1394ef, 1394eg, 1394eh, 1394ei, 1394ej, 1394ek, 1394el, 1394em, 1394en, 1394eo, 1394ep, 1394eq, 1394er, 1394es, 1394et, 1394eu, 1394ev, 1394ew, 1394ex, 1394ey, 1394ez, 1394fa, 1394fb, 1394fc, 1394fd, 1394fe, 1394ff, 1394fg, 1394fh, 1394fi, 1394fj, 1394fk, 1394fl, 1394fm, 1394fn, 1394fo, 1394fp, 1394fq, 1394fr, 1394fs, 1394ft, 1394fu, 1394fv, 1394fw, 1394fx, 1394fy, 1394fz, 1394ga, 1394gb, 1394gc, 1394gd, 1394ge, 1394gf, 1394gg, 1394gh, 1394gi, 1394gj, 1394gk, 1394gl, 1394gm, 1394gn, 1394go, 1394gp, 1394gq, 1394gr, 1394gs, 1394gt, 1394gu, 1394gv, 1394gw, 1394gx, 1394gy, 1394gz, 1394ha, 1394hb, 1394hc, 1394hd, 1394he, 1394hf, 1394hg, 1394hi, 1394hj, 1394hk, 1394hl, 1394hm, 1394hn, 1394ho, 1394hp, 1394hq, 1394hr, 1394hs, 1394ht, 1394hu, 1394hv, 1394hw, 1394hx, 1394hy, 1394hz, 1394ia, 1394ib, 1394ic, 1394id, 1394ie, 1394if, 1394ig, 1394ih, 1394ii, 1394ij, 1394ik, 1394il, 1394im, 1394in, 1394io, 1394ip, 1394iq, 1394ir, 1394is, 1394it, 1394iu, 1394iv, 1394iw, 1394ix, 1394iy, 1394iz, 1394ja, 1394jb, 1394jc, 1394jd, 1394je, 1394jf, 1394jg, 1394jh, 1394ji, 1394jj, 1394jk, 1394jl, 1394jm, 1394jn, 1394jo, 1394jp, 1394jq, 1394jr, 1394js, 1394jt, 1394ju, 1394jv, 1394jw, 1394jx, 1394jy, 1394jz, 1394ka, 1394kb, 1394kc, 1394kd, 1394ke, 1394kf, 1394kg, 1394kh, 1394ki, 1394kj, 1394kk, 1394kl, 1394km, 1394kn, 1394ko, 1394kp, 1394kq, 1394kr, 1394ks, 1394kt, 1394ku, 1394kv, 1394kw, 1394kx, 1394ky, 1394kz, 1394la, 1394lb, 1394lc, 1394ld, 1394le, 1394lf, 1394lg, 1394lh, 1394li, 1394lj, 1394lk, 1394ll, 1394lm, 1394ln, 1394lo, 1394lp, 1394lq, 1394lr, 1394ls, 1394lt, 1394lu, 1394lv, 1394lw, 1394lx, 1394ly, 1394lz, 1394ma, 1394mb, 1394mc, 1394md, 1394me, 1394mf, 1394mg, 1394mh, 1394mi, 1394mj, 1394mk, 1394ml, 1394mm, 1394mn, 1394mo, 1394mp, 1394mq, 1394mr, 1394ms, 1394mt, 1394mu, 1394mv, 1394mw, 1394mx, 1394my, 1394mz, 1394na, 1394nb, 1394nc, 1394nd, 1394ne, 1394nf, 1394ng, 1394nh, 1394ni, 1394nj, 1394nk, 1394nl, 1394nm, 1394nn, 1394no, 1394np, 1394nq, 1394nr, 1394ns, 1394nt, 1394nu, 1394nv, 1394nw, 1394nx, 1394ny, 1394nz, 1394oa, 1394ob, 1394oc, 1394od, 1394oe, 1394of, 1394og, 1394oh, 1394oi, 1394oj, 1394ok, 1394ol, 1394om, 1394on, 1394oo, 1394op, 1394oq, 1394or, 1394os, 1394ot, 1394ou, 1394ov, 1394ow, 1394ox, 1394oy, 1394oz, 1394pa, 1394pb, 1394pc, 1394pd, 1394pe, 1394pf, 1394pg, 1394ph, 1394pi, 1394pj, 1394pk, 1394pl, 1394pm, 1394pn, 1394po, 1394pp, 1394pq, 1394pr, 1394ps, 1394pt, 1394pu, 1394pv, 1394pw, 1394px, 1394py, 1394pz, 1394qa, 1394qb, 1394qc, 1394qd, 1394qe, 1394qf, 1394qg, 1394qh, 1394qi, 1394qj, 1394qk, 1394ql, 1394qm, 1394qn, 1394qo, 1394qp, 1394qq, 1394qr, 1394qs, 1394qt, 1394qu, 1394qv, 1394qw, 1394qx, 1394qy, 1394qz, 1394ra, 1394rb, 1394rc, 1394rd, 1394re, 1394rf, 1394rg, 1394rh, 1394ri, 1394rj, 1394rk, 1394rl, 1394rm, 1394rn, 1394ro, 1394rp, 1394rq, 1394rr, 1394rs, 1394rt, 1394ru, 1394rv, 1394rw, 1394rx, 1394ry, 1394rz, 1394sa, 1394sb, 1394sc, 1394sd, 1394se, 1394sf, 1394sg, 1394sh, 1394si, 1394sj, 1394sk, 1394sl, 1394sm, 1394sn, 1394so, 1394sp, 1394sq, 1394sr, 1394ss, 1394st, 1394su, 1394sv, 1394sw, 1394sx, 1394sy, 1394sz, 1394ta, 1394tb, 1394tc, 1394td, 1394te, 1394tf, 1394tg, 1394th, 1394ti, 1394tj, 1394tk, 1394tl, 1394tm, 1394tn, 1394to, 1394tp, 1394tq, 1394tr, 1394ts, 1394tt, 1394tu, 1394tv, 1394tw, 1394tx, 1394ty, 1394tz, 1394ua, 1394ub, 1394uc, 1394ud, 1394ue, 1394uf, 1394ug, 1394uh, 1394ui, 1394uj, 1394uk, 1394ul, 1394um, 1394un, 1394uo, 1394up, 1394uq, 1394ur, 1394us, 1394ut, 1394uu, 1394uv, 1394uw, 1394ux, 1394uy, 1394uz, 1394va, 1394vb, 1394vc, 1394vd, 1394ve, 1394vf, 1394vg, 1394vh, 1394vi, 1394vj, 1394vk, 1394vl, 1394vm, 1394vn, 1394vo, 1394vp, 1394vq, 1394vr, 1394vs, 1394vt, 1394vu, 1394vv, 1394vw, 1394vx, 1394vy, 1394vz, 1394wa, 1394wb, 1394wc, 1394wd, 1394we, 1394wf, 1394wg, 1394wh, 1394wi, 1394wj, 1394wk, 1394wl, 1394wm, 1394wn, 1394wo, 1394wp, 1394wq, 1394wr, 1394ws, 1394wt, 1394wu, 1394wv, 1394ww, 1394wx, 1394wy, 1394wz, 1394xa, 1394xb, 1394xc, 1394xd, 1394xe, 1394xf, 1394xg, 1394xh, 1394xi, 1394xj, 1394xk, 1394xl, 1394xm, 1394xn, 1394xo, 1394xp, 1394xq, 1394xr, 1394xs, 1394xt, 1394xu, 1394xv, 1394xw, 1394xx, 1394xy, 1394xz, 1394ya, 1394yb, 1394yc, 1394yd, 1394ye, 1394yf, 1394yg, 1394yh, 1394yi, 1394yj, 1394yk, 1394yl, 1394ym, 1394yn, 1394yo, 1394yp, 1394yq, 1394yr, 1394ys, 1394yt, 1394yu, 1394yv, 1394yw, 1394yx, 1394yy, 1394yz, 1394za, 1394zb, 1394zc, 1394zd, 1394ze, 1394zf, 1394zg, 1394zh, 1394zi, 1394zj, 1394zk, 1394zl, 1394zm, 1394zn, 1394zo, 1394zp, 1394zq, 1394zr, 1394zs, 1394zt, 1394zu, 1394zv, 1394zw, 1394zx, 1394zy, 1394zz	WLAN	1.57	dBm	-18.5
1009	AC	IEEE Std 1394-1995, 1394a, 1394b, 1394c, 1394d, 1394e, 1394f, 1394g, 1394h, 1394i, 1394j, 1394k, 1394l, 1394m, 1394n, 1394o, 1394p, 1394q, 1394r, 1394s, 1394t, 1394u, 1394v, 1394w, 1394x, 1394y, 1394z, 1394aa, 1394ab, 1394ac, 1394ad, 1394ae, 1394af, 1394ag, 1394ah, 1394ai, 1394aj, 1394ak, 1394al, 1394am, 1394an, 1394ao, 1394ap, 1394aq, 1394ar, 1394as, 1394at, 1394au, 1394av, 1394aw, 1394ax, 1394ay, 1394az, 1394ba, 1394bb, 1394bc, 1394bd, 1394be, 1394bf, 1394bg, 1394bh, 1394bi, 1394bj, 1394bk, 1394bl, 1394bm, 1394bn, 1394bo, 1394bp, 1394bq, 1394br, 1394bs, 1394bt, 1394bu, 1394bv, 1394bw, 1394bx, 1394by, 1394bz, 1394ca, 1394cb, 1394cc, 1394cd, 1394ce, 1394cf, 1394cg, 1394ch, 1394ci, 1394cj, 1394ck, 1394cl, 1394cm, 1394cn, 1394co, 1394cp, 1394cq, 1394cr, 1394cs, 1394ct, 1394cu, 1394cv, 1394cw, 1394cx, 1394cy, 1394cz, 1394da, 1394db, 1394dc, 1394dd, 1394de, 1394df, 1394dg, 1394dh, 1394di, 1394dj, 1394dk, 1394dl, 1394dm, 1394dn, 1394do, 1394dp, 1394dq, 1394dr, 1394ds, 1394dt, 1394du, 1394dv, 1394dw, 1394dx, 1394dy, 1394dz, 1394ea, 1394eb, 1394ec, 1394ed, 1394ee, 1394ef, 1394eg, 1394eh, 1394ei, 1394ej, 1394ek, 1394el, 1394em, 1394en, 1394eo, 1394ep, 1394eq, 1394er, 1394es, 1394et, 1394eu, 1394ev, 1394ew, 1394ex, 1394ey, 1394ez, 1394fa, 1394fb, 1394fc, 1394fd, 1394fe, 1394ff, 1394fg, 1394fh, 1394fi, 1394fj, 1394fk, 1394fl, 1394fm, 1394fn, 1394fo, 1394fp, 1394fq, 1394fr, 1394fs, 1394ft, 1394fu, 1394fv, 1394fw, 1394fx, 1394fy, 1394fz, 1394ga, 1394gb, 1394gc, 1394gd, 1394ge, 1394gf, 1394gg, 1394gh, 1394gi, 1394gj, 1394gk, 1394gl, 1394gm, 1394gn, 1394go, 1394gp, 1394gq, 1394gr, 1394gs, 1394gt, 1394gu, 1394gv, 1394gw, 1394gx, 1394gy, 1394gz, 1394ha, 1394hb, 1394hc, 1394hd, 1394he, 1394hf, 1394hg, 1394hi, 1394hj, 1394hk, 1394hl, 1394hm, 1394hn, 1394ho, 1394hp, 1394hq, 1394hr, 1394hs, 1394ht, 1394hu, 1394hv, 1394hw, 1394hx, 1394hy, 1394hz, 1394ia, 1394ib, 1394ic, 1394id, 1394ie, 1394if, 1394ig, 1394ih, 1394ii, 1394ij, 1394ik, 1394il, 1394im, 1394in, 1394io, 1394ip, 1394iq, 1394ir, 1394is, 1394it, 1394iu, 1394iv, 1394iw, 1394ix, 1394iy, 1394iz, 1394ja, 1394jb, 1394jc, 1394jd, 1394je, 1394jf, 1394jg, 1394jh, 1394ji, 1394jj, 1394jk, 1394jl, 1394jm, 1394jn, 1394jo, 1394jp, 1394jq, 1394jr, 1394js, 1394jt, 1394ju, 1394jv, 1394jw, 1394jx, 1394jy, 1394jz, 1394ka, 1394kb, 1394kc, 1394kd, 1394ke, 1394kf, 1394kg, 1394kh, 1394ki, 1394kj, 1394kk, 1394kl, 1394km, 1394kn, 1394ko, 1394kp, 1394kq, 1394kr, 1394ks, 1394kt, 1394ku, 1394kv, 1394kw, 1394kx, 1394ky, 1394kz, 1394la, 1394lb, 1394lc, 1394ld, 1394le, 1394lf, 1394lg, 1394lh, 1394li, 1394lj, 1394lk, 1394ll, 1394lm, 1394ln, 1394lo, 1394lp, 1394lq, 1394lr, 1394ls, 1394lt, 1394lu, 1394lv, 1394lw, 1394lx, 1394ly, 1394lz, 1394ma, 1394mb, 1394mc, 1394md, 1394me, 1394mf, 1394mg, 1394mh, 1394mi, 1394mj, 1394mk, 1394ml, 1394mm, 1394mn, 1394mo, 1394mp, 1394mq, 1394mr, 1394ms, 1394mt, 1394mu, 1394mv, 1394mw, 1394mx, 1394my, 1394mz, 1394na, 1394nb, 1394nc, 1394nd, 1394ne, 1394nf, 1394ng, 1394nh, 1394ni, 1394nj, 1394nk, 1394nl, 1394nm, 1394nn, 1394no, 1394np, 1394nq, 1394nr, 1394ns, 1394nt, 1394nu, 1394nv, 1394nw, 1394nx, 1394ny, 1394nz, 1394oa, 1394ob, 1394oc, 1394od, 1394oe, 1394of, 1394og, 1394oh, 1394oi, 1394oj, 1394ok, 1394ol, 1394om, 1394on, 1394oo, 1394op, 1394oq, 1394or, 1394os, 1394ot, 1394ou, 1394ov, 1394ow, 1394ox, 1394oy, 1394oz, 1394pa, 1394pb, 1394pc, 1394pd, 1394pe, 1394pf, 1394pg, 1394ph, 1394pi, 1394pj, 1394pk, 1394pl, 1394pm, 1394pn, 1394po, 1394pp, 1394pq, 1394pr, 1394ps, 1394pt, 1394pu, 1394pv, 1394pw, 1394px, 1394py, 1394pz, 1394qa, 1394qb, 1394qc, 1394qd, 1394qe, 1394qf, 1394qg, 1394qh, 1394qi, 1394qj, 1394qk, 1394ql, 1394qm, 1394qn, 1394qo, 1394qp, 1394qq, 1394qr, 1394qs, 1394qt, 1394qu, 1394qv, 1394qw, 1394qx, 1394qy, 1394qz, 1394ra, 1394rb, 1394rc, 1394rd, 1394re, 1394rf, 1394rg, 1394rh, 1394ri, 1394rj, 1394rk, 1394rl, 1394rm, 1394rn, 1394ro, 1394rp, 1394rq, 1394rr, 1394rs, 1394rt, 1394ru, 1394rv, 1394rw, 1394rx, 1394ry, 1394rz, 1394sa, 1394sb, 1394sc, 1394sd, 1394se, 1394sf, 1394sg, 1394sh, 1394si, 1394sj, 1394sk, 1394sl, 1394sm, 1394sn, 1394so, 1394sp, 1394sq, 1394sr, 1394ss, 1394st, 1394su, 1394sv, 1394sw, 1394sx, 1394sy, 1394sz, 1394ta, 1394tb, 1394tc, 1394td, 1394te, 1394tf, 1394tg, 1394th, 1394ti, 1394tj, 1394tk, 1394tl, 1394tm, 1394tn, 1394to, 1394tp, 1394tq, 1394tr, 1394ts, 1394tt, 1394tu, 1394tv, 1394tw, 1394tx, 1394ty, 1394tz, 1394ua, 1394ub, 1394uc, 1394ud, 1394ue, 1394uf, 1394ug, 1394uh, 1394ui, 1394uj, 1394uk, 1394ul, 1394um, 1394un, 1394uo, 1394up, 1394uq, 1394ur, 1394us, 1394ut, 1394uu, 1394uv, 1394uw, 1394ux, 1394uy, 1394uz, 1394va, 1394vb, 1394vc, 1394vd, 1394ve, 1394vf, 1394vg, 1394vh, 1394vi, 1394vj, 1394vk, 1394vl, 1394vm, 1394vn, 1394vo, 1394vp, 1394vq, 1394vr, 1394vs, 1394vt, 1394vu, 1394vv, 1394vw, 1394vx, 1394vy, 1394vz, 1394wa, 1394wb, 1394wc, 1394wd, 1394we, 1394wf, 1394wg, 1394wh, 1394wi, 1394wj, 1394wk, 1394wl, 1394wm, 1394wn, 1394wo, 1394wp, 1394wq, 1394wr, 1394ws, 1394wt, 1394wu, 1394wv, 1394ww, 1394wx, 1394wy, 1394wz, 1394xa, 1394xb, 1394xc, 1394xd, 1394xe, 1394xf, 1394xg, 1394xh, 1394xi, 1394xj, 1394xk, 1394xl, 1394xm, 1394xn, 1394xo, 1394xp, 1394xq, 1394xr, 1394xs, 1394xt, 1394xu, 1394xv, 1394xw, 1394xx, 1394xy, 1394xz, 1394ya, 1394yb, 1394yc, 1394yd, 1394ye, 1394yf, 1394yg, 1394yh, 1394yi, 1394yj, 1394yk, 1394yl, 1394ym, 1394yn, 1394yo, 1394yp, 1394yq, 1394yr, 1394ys, 1394yt, 1394yu, 1394yv, 1394yw, 1394yx, 1394yy, 1394yz, 1394za, 1394zb, 1394zc, 1394zd, 1394ze, 1394zf, 1394zg, 1394zh, 1394zi, 1394zj, 1394zk, 1394zl, 1394zm, 1394zn, 1394zo, 1394zp, 1394zq, 1394zr, 1394zs, 1394zt, 1394zu, 1394zv, 1394zw, 1394zx, 1394zy, 1394zz	WLAN	1.57	dBm	-18.5
1010	AC	IEEE Std 1394-1995, 1394a, 1394b, 1394c, 1394d, 1394e, 1394f, 1394g, 1394h, 1394i, 1394j, 1394k, 1394l, 1394m, 1394n, 1394o, 1394p, 1394q, 1394r, 1394s, 1394t, 1394u, 1394v, 1394w, 1394x, 1394y, 1394z, 1394aa, 1394ab, 1394ac, 1394ad, 1394ae, 1394af, 1394ag, 1394ah, 1394ai, 1394aj, 1394ak, 1394al, 1394am, 1394an, 1394ao, 1394ap, 1394aq, 1394ar, 1394as, 1394at, 1394au, 1394av, 1394aw, 1394ax, 1394ay, 1394az, 1394ba, 1394bb, 1394bc, 1394bd, 1394be, 1394bf, 1394bg, 1394bh, 1394bi, 1394bj, 1394bk, 1394bl, 1394bm, 1394bn, 1394bo, 1394bp, 1394bq, 1394br, 1394bs, 1394bt, 1394bu, 1394bv, 1394bw, 1394bx, 1394by, 1394bz, 1394ca, 1394cb, 1394cc, 1394cd, 1394ce, 1394cf, 1394cg, 1394ch, 1394ci, 1394cj, 1394ck, 1394cl, 1394cm, 1394cn, 1394co, 1394cp, 1394cq, 1394cr, 1394cs, 1394ct, 1394cu, 1394cv, 1394cw, 1394cx, 1394cy, 1394cz, 1394da, 1394db, 1394dc, 1394dd, 1394de, 1394df, 1394dg, 1394dh, 1394di, 1394dj, 1394dk, 1394dl, 1394dm, 1394dn, 1394do, 1394dp, 1394dq, 1394dr, 1394ds, 1394dt, 1394du, 1394dv, 1394dw, 1394dx, 1394dy, 1394dz, 1394ea, 1394eb, 1394ec, 1394ed, 1394ee, 1394ef, 1394eg, 1394eh, 1394ei, 1394ej, 1394ek, 1394el, 1394em, 1394en, 1394eo, 1394ep, 1394eq, 1394er, 1394es, 1394et, 1394eu, 1394ev, 1394ew, 1394ex, 1394ey, 1394ez, 1394fa, 1394fb, 1394fc, 1394fd, 1394fe, 1394ff, 1394fg, 1394fh, 1394fi, 1394fj, 1394fk, 1394fl, 1394fm, 1394fn, 1394fo, 1394fp, 1394fq, 1394fr, 1394fs, 1394ft, 1394fu, 1394fv, 1394fw, 1394fx, 1394fy, 1394fz, 1394ga, 1394gb, 1394gc, 1394gd, 1394ge, 1394gf, 1394gg, 1394gh, 1394gi, 1394gj, 1394gk, 1394gl, 1394gm, 1394gn, 1394go, 1394gp, 1394gq, 1394gr, 1394gs, 1394gt, 1394gu, 1394gv, 1394gw, 1394gx, 1394gy, 1394gz, 1394ha, 1394hb, 1394hc, 1394hd, 1394he, 1394hf, 1394hg, 1394hi, 1394hj, 1394hk, 1394hl, 1394hm, 1394hn, 1394ho, 1394hp, 1394hq, 1394hr, 1394hs, 1394ht, 1394hu, 1394hv, 1394hw, 1394hx, 1394hy, 1394hz, 1394ia, 1394ib, 1394ic, 1394id, 1394ie, 1394if, 1394ig, 1394ih, 1394ii, 1394ij, 1394ik, 1394il, 1394im, 1394in, 1394io, 1394ip, 1394iq, 1394ir, 1394is, 1394it, 1394iu, 1394iv, 1394iw, 1394ix, 1394iy, 1394iz, 1394ja, 1394jb, 1394jc, 1394jd, 1394je, 1394jf, 1394jg, 1394jh, 1394ji, 1394jj, 1394jk, 1394jl, 1394jm, 1394jn, 1394jo, 1394jp, 1394jq, 1394jr, 1394js, 1394jt, 1394ju, 1394jv, 1394jw, 1394jx, 1394jy, 1394jz, 1394ka, 1394kb, 1394kc, 1394kd, 1394ke, 1394kf, 1394kg, 1394kh, 1394ki, 1394kj, 1394kk, 1394kl, 1394km, 1394kn, 1394ko, 1394kp, 1394kq, 1394kr, 1394ks, 1394kt, 1394ku, 1394kv, 1394kw, 1394kx, 1394ky, 1394kz, 1394la, 1394lb, 1394lc, 1394ld, 1394le, 1394lf, 1394lg, 1394lh, 1394li, 1394lj				

Certificate No: EX-7833, Aug23

Page 17 of 20

EX3DV4 - SN:7893 August 24, 2023

[illegible]

Certificate No: EX-7833 Aug23

Page 18 of 21

[illegible]

Certificate No: EX-7833 Aug21

Page 10 of 22

[illegible]

Certificate No: EX-7833 Aug29

Page 88 of 88

[illegible]

Certificate No: EX-7822, Aug22

DOI: 10.1002/for

[illegible]

Certificate No: FX-7833_Aug29

Page 50 of 60

4 Impedance and return loss

Dipole D750V3 SN 1188				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/3/29	-28.7	/	53.6	/
2023/3/29	-28.3	1.39%	53.2	0.4
Dipole D835V2 SN 4d114				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/3/31	-25.3	/	48.7	/
2023/3/31	-24.6	2.77%	49.1	0.4
Dipole D900V2 SN 1d079				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/7	-23.3	/	48.1	/
2023/6/7	-23.6	-1.29%	48.3	0.2
Dipole D1800V2 SN 2d170				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/3/31	-29.4	/	47.9	/
2023/3/31	-28.9	1.70%	47.2	0.7
Dipole D1900V2 SN 5d136				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/7	-22.4	/	51.2	/
2023/6/7	-22.9	-2.23%	51.6	-0.4
Dipole D2000V2 SN 1041				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/6	-34.9	/	48.4	/
2023/6/6	-33.5	4.01%	49.1	-0.7
Dipole D2300V2 SN 1096				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/3/31	-26.6	/	49.2	/
2023/3/31	-27.1	-1.88%	49.4	0.2
Dipole D2450V2 SN 817				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/4/1	-28.5	/	52.1	/
2023/4/1	-28.0	1.75%	51.6	0.5
Dipole D2600V2 SN 1158				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/3/31	-23.8	/	49.9	/
2023/3/31	-23.3	2.10%	50.3	0.4

Dipole D5GHzV2 SN 1095 for 5200				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/1	-23.6	/	46.1	/
2023/6/1	-23.1	2.12%	45.6	0.5
Dipole D5GHzV2 SN 1095 for 5300				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/1	-29.5	/	47.8	/
2023/6/1	-28.8	2.37%	46.9	0.9
Dipole D5GHzV2 SN 1095 for 5500				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/1	-27.4	/	50.3	/
2023/6/1	-27.6	-0.73%	50.8	-0.5
Dipole D5GHzV2 SN 1095 for 5600				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/1	-24.0	/	54.5	/
2023/6/1	-23.6	1.67%	54.9	-0.4
Dipole D5GHzV2 SN 1095 for 5800				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/1	-24.9	/	51.5	/
2023/6/1	-24.3	2.41%	51.0	0.5