

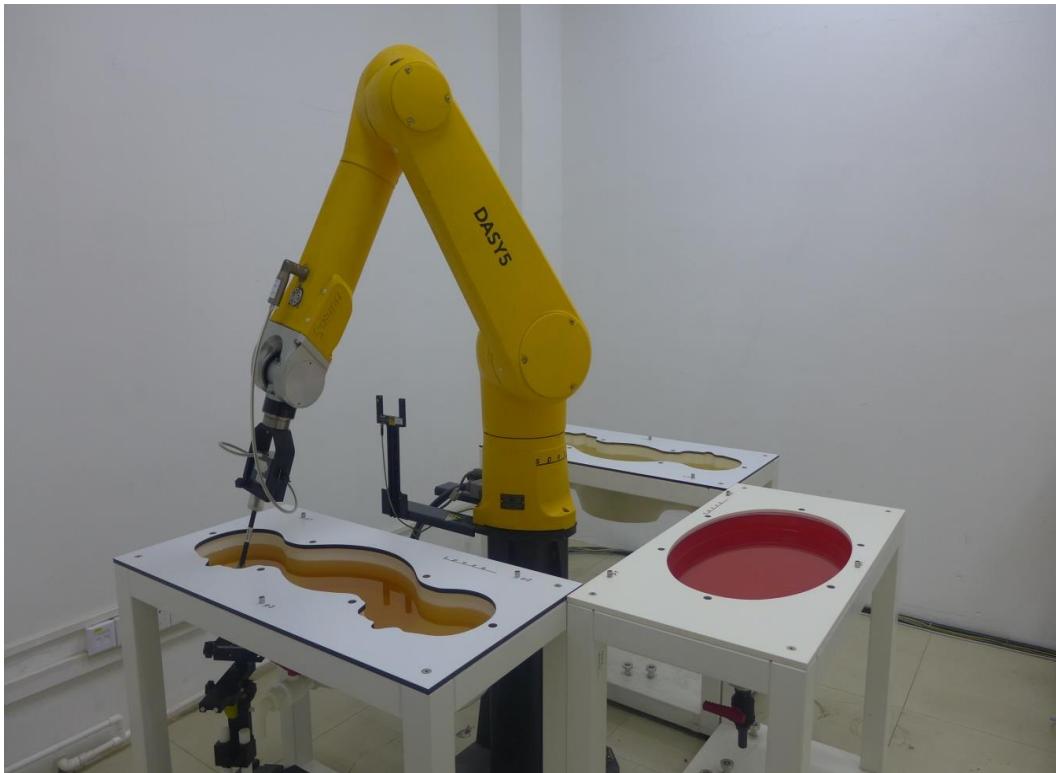


Appendix D

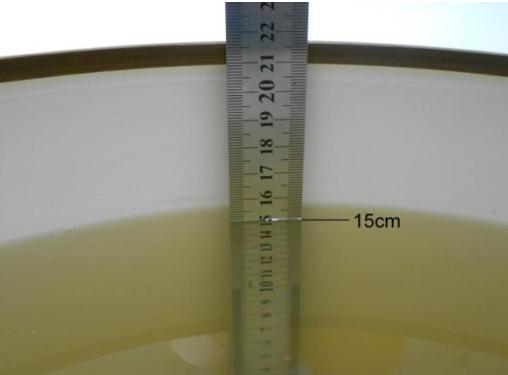
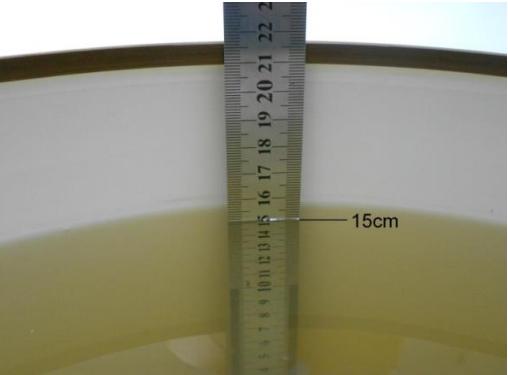
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 750MHz	Photo 2: Tissue Simulant Liquid for Head 835MHz
	
Photo 3: Tissue Simulant Liquid for Head 1750MHz	Photo 4: Tissue Simulant Liquid for Head 1900MHz
	

3. Photographs of EUT test position

Photo 5: Front side 25mm	Photo 6: Back side 0mm
	

4. EUT Constructional Details

Photo 7: Front View	Photo 8: Back View
	