


Label

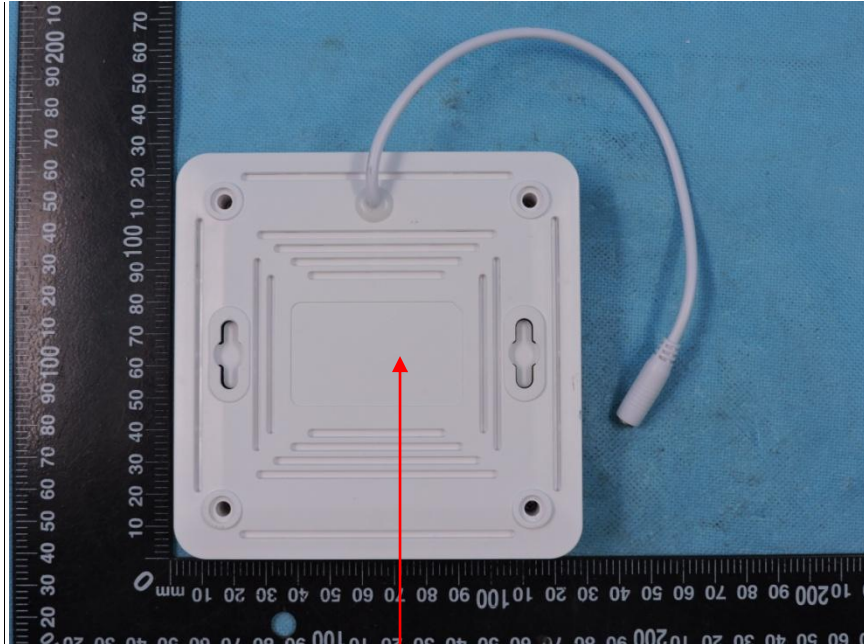

W:38MM

VitalCare

Model name: EX4M02-S

FCC ID: 2APQOEX4M02-S

Contains FCC ID:2AJFN-RTL00-01
2AD9QX4M05

This device complies with part 15 of the FCC Rules.
Operation is subject to the following two conditions: (1)
This device may not cause harmful interference, and (2)
this device must accept any interference received,
including interference that may cause undesired
operation.

L:30MM

Note: The label is silk-screen on the sample