


Trc1 S11 dB Mag 10 dB / Ref -20 dB Cal int 1

S11 •1 750.00000 MHz -23.050 dB


Ch1 Start 650 MHz Pwr -10 dBm Stop 850 MHz

# SN 29/15 DIP 0G835-383; 835Head

Calibrated impedance:  $56.3\Omega + 0.8j\Omega$ ; Measurement impedance:  $57.1\Omega - 5.0j\Omega$  (within  $5\Omega$ )

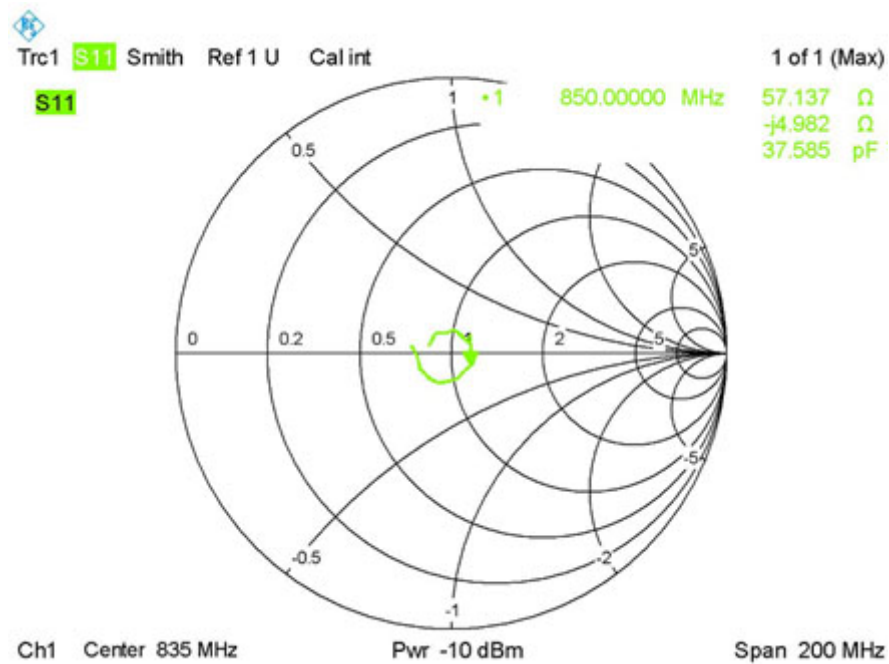


Calibrated return loss: -24.51dB; Measurement return loss: -22.89 dB (within 20%)

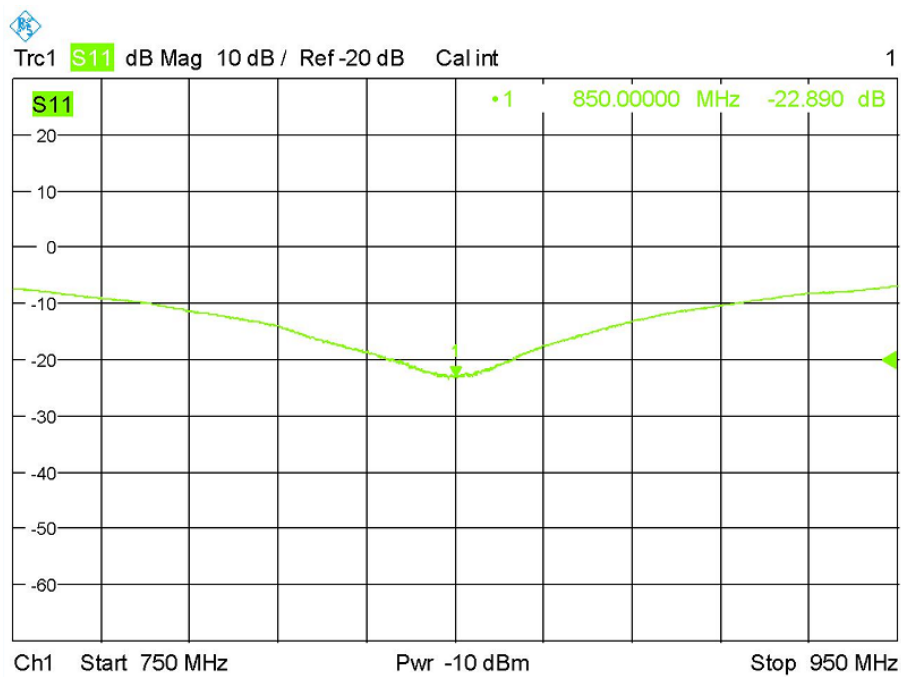


# SN 46/11 DIP 1G800-186; 1800Head

Calibrated impedance:  $46.7\Omega + 3.0j\Omega$ ; Measurement impedance:  $48.5\Omega + 2.3j\Omega$  (within  $5\Omega$ )

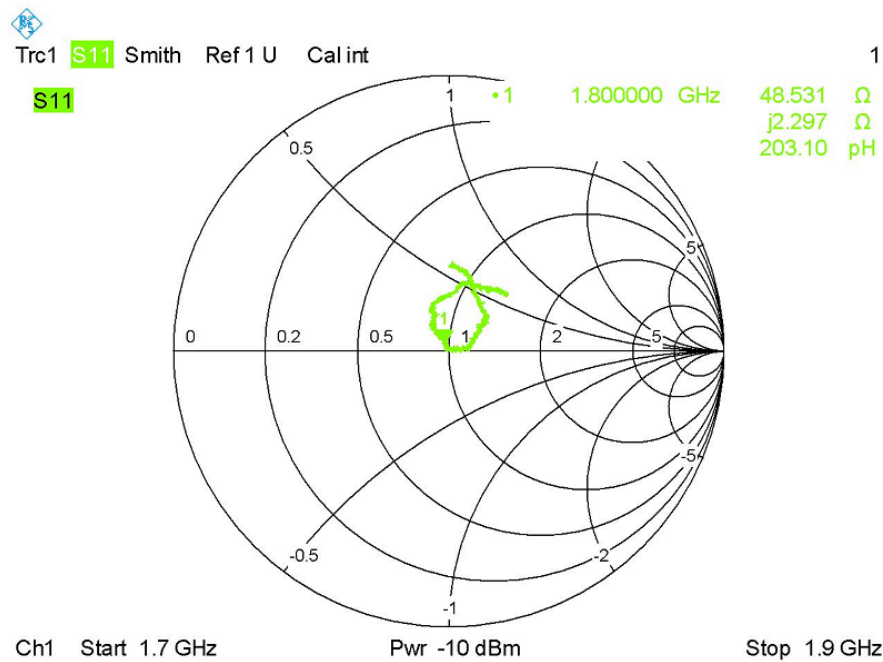


Calibrated return loss: -26.66dB; Measurement return loss: -27.3 dB (within 20%)

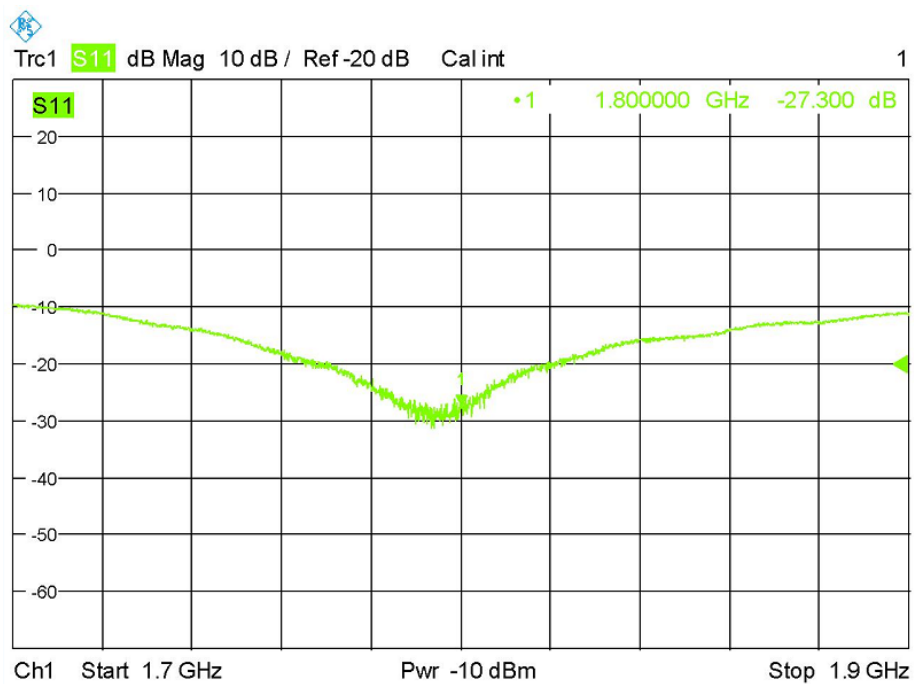


# SN 46/11 DIP 1G900-187; 1900Head

Calibrated impedance:  $50.7\Omega + 4.1j\Omega$ ; Measurement impedance:  $48.6\Omega + 2.9j\Omega$  (within  $5\Omega$ )

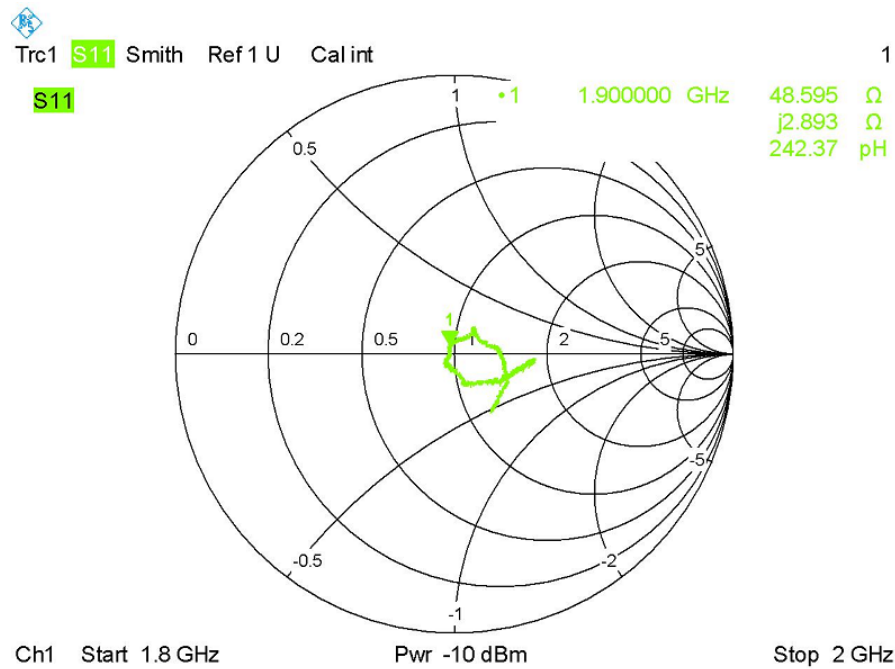


Calibrated return loss: -27.75dB; Measurement return loss: -28.54 dB (within 20%)

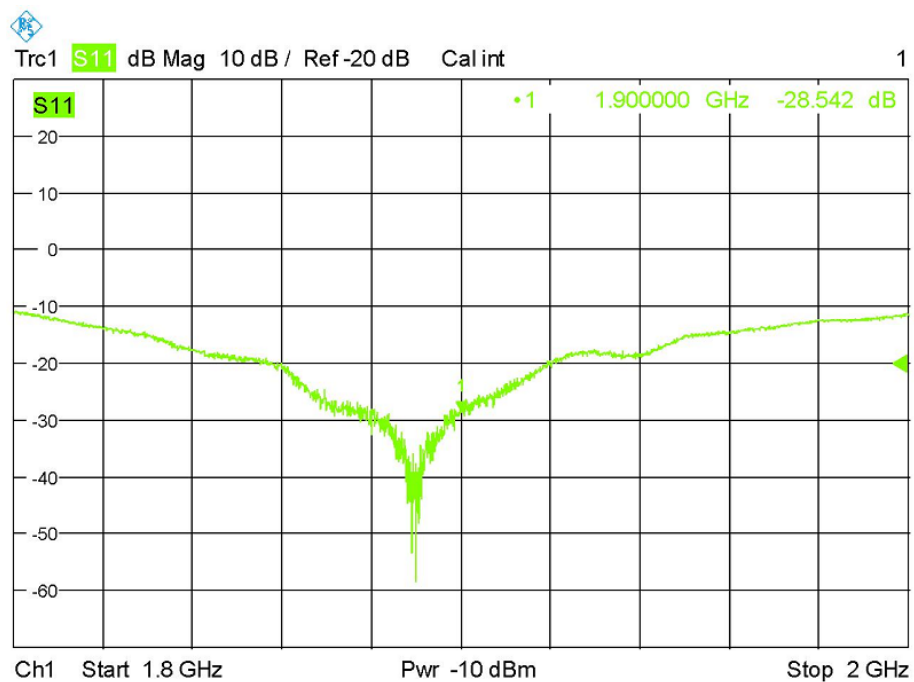


# SN 46/11 DIP 2G450-189; 2450Head

Calibrated impedance:  $49.8\Omega + 3.3j\Omega$ ; Measurement impedance:  $50.9\Omega - 2.1j\Omega$  (within  $5\Omega$ )

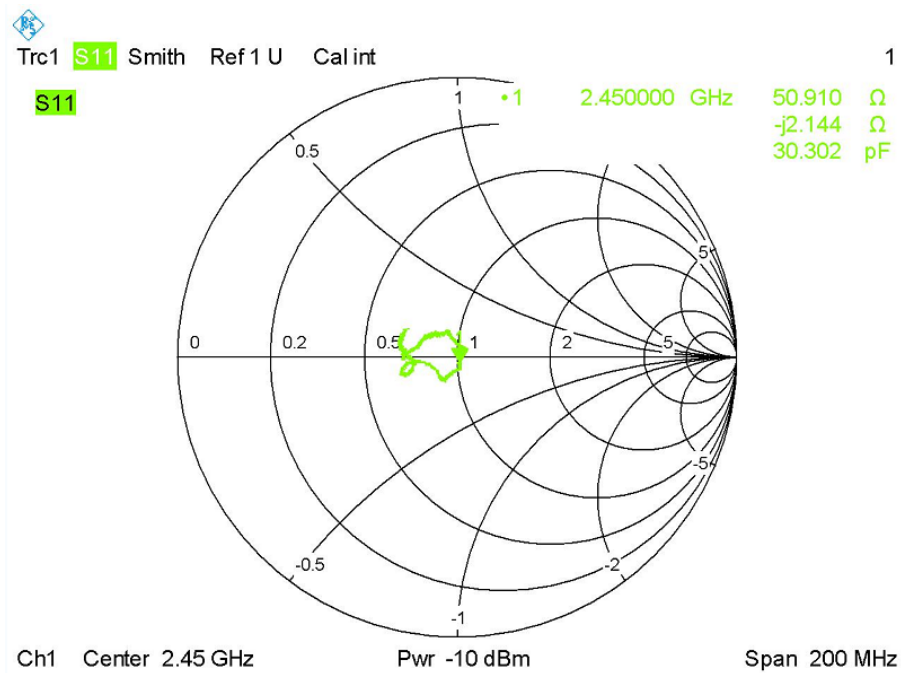


Calibrated return loss: -29.54dB; Measurement return loss: -31.08 dB (within 20%)

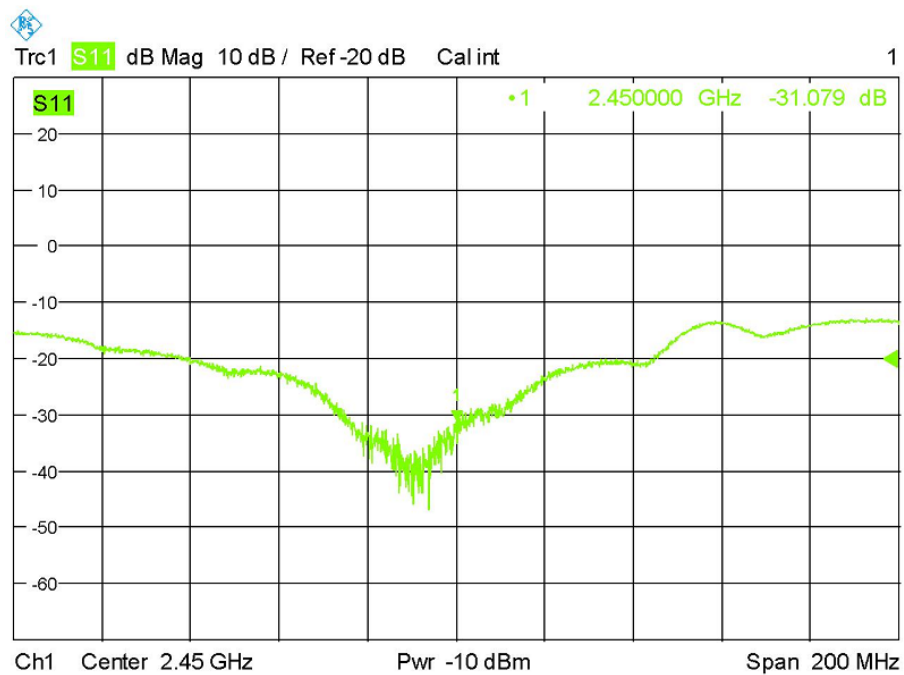

# SN 47/14 DIP 2G600-342; 2600Head

Calibrated impedance:  $55.5\Omega + 2.6j\Omega$ ; Measurement impedance:  $57.2\Omega + 3.2j\Omega$ (within  $5\Omega$ )

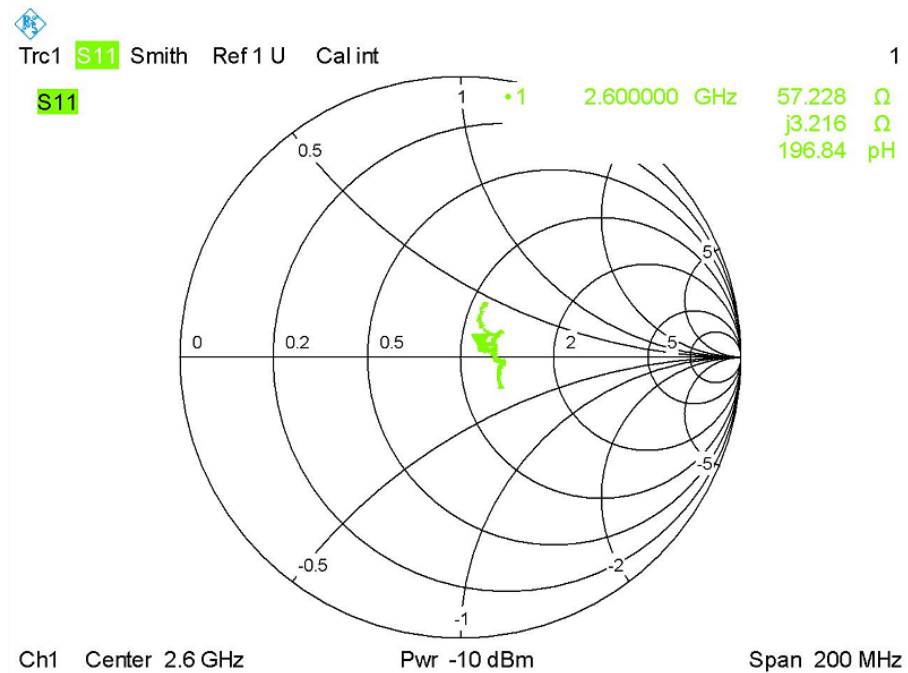

Calibrated return loss: -24.86dB; Measurement return loss: -23.1 dB(within 20%)

