RF Exposure Lab

802 N. Twin Oaks Valley Road, Suite 105 • San Marcos, CA 92069 • U.S.A. TEL (760) 471-2100 • FAX (760) 471-2121

http://www.rfexposurelab.com

CERTIFICATE OF COMPLIANCE R&D SAR EVALUATION

Privoro, LLC 3100 W. Ray Rd. #20 Chandler, AZ 85226		Dates of Test: Test Report Number:	July 5-16, 2022 SAR.20210706
FCC ID:	2APWUPM0708		
IC Certificate:	23953-PM0708		
Model(s):		CC ID: A3LSMG991U & IC ID: 649E-	
		542A & IC ID: 579C-E3542A) & M000	09 with iPhone 12
	(FCC ID: BCG-E3542A & IC		
Test Sample:	Engineering Unit Same as Pr	oduction	
Equipment Type:	Smart Phone SafeCase		
Classification:	Portable Transmitter Next to	Head and Body	
TX Frequency Range:	663 – 698 MHz; 699 – 716 M	Hz; 824 - 849 MHz; 1710 - 1755 MH	łz; 1850 – 1910 MHz;
. , , ,		90 MHz; 3550 - 3700 MHz; 2402 - 2	
Frequency Tolerance:	± 2.5 ppm		
Maximum RF Output:	See Data Sheets		
Signal Modulation:	QPSK, WCDMA, DSSS, OFE	DM. GFSK	
Antenna Type:	Internal	,	
Application Type:	Evaluation		
, ppiloulon i jpo.			

This wireless mobile and/or portable device has been shown to be compliant for localized specific absorption rate (SAR) for uncontrolled environment/general exposure limits specified in ANSI/IEEE Std. C95.1-1992 and had been tested in accordance with the measurement procedures specified in IEEE 1528-2013 and IEC 62209-2:2010 (See test report).

0 mm Head; 5 mm Body (iPhone) and 10 mm Body (Samsung)

0.502 W/kg Measured Head; 0.959 W/kg Measured Body

0.706 W/kg Measured Head; 1.205 W/kg Measured Body

KDB 447498 D01 v07, KDB 648474 D04 v01r03, KDB 941225 D01 v03r01 & D05 v02r05

Part 2, 15, 22, 24, 27

I attest to the accuracy of the data. All measurements were performed by myself or were made under my supervision and are correct to the best of my knowledge and belief. I assume full responsibility for the completeness of these measurements and vouch for the qualifications of all persons taking them.

RF Exposure Lab, LLC certifies that no party to this application is subject to a denial of Federal benefits that includes FCC benefits pursuant to Section 5301 of the Anti-Drug Abuse Act of 1988, 21 U.S.C. 853(a).

Jay M. Moulton Vice President

FCC Rule Parts:

KDB Test Methodology:

Separation Distance:

Max. Stand Alone SAR Value: Simultaneous SAR Value:





Table of Contents

1.	Introduction	4
	SAR Definition [5]	5
2.	SAR Measurement Setup	6
	Robotic System	6
	System Hardware	6
	System Electronics	7
	Probe Measurement System	7
3.	Definition of Reference Points	. 14
	Ear Reference Point	. 14
	Device Reference Points	. 14
4.	Test Configuration Positions	. 15
	Positioning for Cheek/Touch [5]	. 15
	Positioning for Ear / 15° Tilt [5]	. 16
	Body Worn Configurations	. 17
5.	Probe and Dipole Calibration	. 18
6.	Phantom & Simulating Tissue Specifications	. 19
	Head & Body Simulating Mixture Characterization	
7.	ANSI/IEEE C95.1 – 1992 RF Exposure Limits [2]	20
	Uncontrolled Environment	. 20
	Controlled Environment	
8.		
9.	= j =	
	Tissue Verification	
	Test System Verification	
10). SAR Test Data Summary	
	Procedures Used To Establish Test Signal	
	Device Test Condition	
11	. FCC 3G Measurement Procedures	
	11.1 Procedures Used to Establish RF Signal for SAR	24
	11.2 SAR Measurement Conditions for WCDMA/HSDPA/HSUPA	
	SAR Data Summary – Head Measurements (M0007)	
	SAR Data Summary – Body Measurements (M0007)	
	SAR Data Summary – WiFi Measurements (M0007)	
	SAR Data Summary – Simultaneous Evaluation (M0007)	
	SAR Data Summary – Head Measurements (M0008)	
	SAR Data Summary – Body Measurements (M0008)	
	SAR Data Summary – WiFi Measurements (M0008)	
	SAR Data Summary – Simultaneous Evaluation (M0008)	
12		
13		
14		
	opendix A – System Validation Plots and Data	
	opendix B – SAR Test Data Plots	
	ppendix C – Test Setup Photos	
	ppendix D – Probe Calibration Data Sheets	
	ppendix E – Dipole Calibration Data Sheets	
	ppendix F – DAE Calibration Data Sheets	
Ap	opendix G – Phantom Calibration Data Sheets	140



Comment/Revision	Date
Original Release	August 19, 2022

Note: The latest version supersedes all previous versions listed in the above table. The latest version shall be used.



1. Introduction

This measurement report shows the result of the Privoro Model M0007 with Samsung S21, M0008 with iPhone 12 & M0009 with iPhone 12 FCC ID 2APWUPM0708 with FCC Part 2, 1093, ET Docket 93-62 Rules for mobile and portable devices and IC Certificate: 23953-PM0708 with RSS102 Issue 5 & Safety Code 6. The FCC has adopted the guidelines for evaluating the environmental effects of radio frequency radiation in ET Docket 93-62 on August 6, 1996 to protect the public and workers from the potential hazards of RF emissions due to FCC regulated portable devices. [1], [6]

The test results recorded herein are based on a single type test of Privoro Model M0007 with Samsung S21 & M0008 with iPhone 12 and therefore apply only to the tested sample.

The Model M0008 with iPhone 12 and Model M0009 with iPhone 12 are electrically identical. The difference between the two cases is the mechanical front metal shutter on the device. On Model M0008, the mechanical front shutter covers the Face ID sensors and the front facing camera on the iPhone 12. On Model M0009, the mechanical front shutter covers the phone's front facing camera only and does not cover the phone's Face ID sensors. Testing was conducted only on the M0008 with iPhone 12.

The test procedures and limits, as described in ANSI C95.1 – 1999 Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz [2], ANSI C95.3 – 2002 Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields [3], and IEC 62209 Human exposure to radio frequency fields from handheld and body-mounted wireless communication devices - Human models, instrumentation, and procedures[5] were employed.



SAR Definition [5]

Specific Absorption Rate is defined as the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dV) of a given density (ρ).

$$SAR = \frac{d}{dt} \left(\frac{dW}{dm} \right) = \frac{d}{dt} \left(\frac{dW}{\rho dV} \right)$$

SAR is expressed in units of watts per kilogram (W/kg). SAR can be related to the electric field at a point by

$$SAR = \frac{\sigma \mid E \mid^2}{\rho}$$

where:

 σ = conductivity of the tissue (S/m)

 ρ = mass density of the tissue (kg/m³)

E = rms electric field strength (V/m)



2. SAR Measurement Setup

Robotic System

These measurements are performed using the DASY52 automated dosimetric assessment system. The DASY52 is made by Schmid & Partner Engineering AG (SPEAG) in Zurich, Switzerland and consists of high precision robotics system (Staubli), robot controller, Intel Core2 computer, near-field probe, probe alignment sensor, and the generic twin phantom containing the brain equivalent material. The robot is a six-axis industrial robot performing precise movements to position the probe to the location (points) of maximum electromagnetic field (EMF) (see Fig. 2.1).

System Hardware

A cell controller system contains the power supply, robot controller teach pendant (Joystick), and a remote control used to drive the robot motors. The PC consists of the HP Intel Core2 computer with Windows XP system and SAR Measurement Software DASY52, A/D interface card, monitor, mouse, and keyboard. The Staubli Robot is connected to the cell controller to allow software manipulation of the robot. A data acquisition electronic (DAE) circuit that performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. is connected to the Electro-optical coupler (EOC). The EOC performs the conversion from the optical into digital electric signal of the DAE and transfers data to the PC plug-in card.

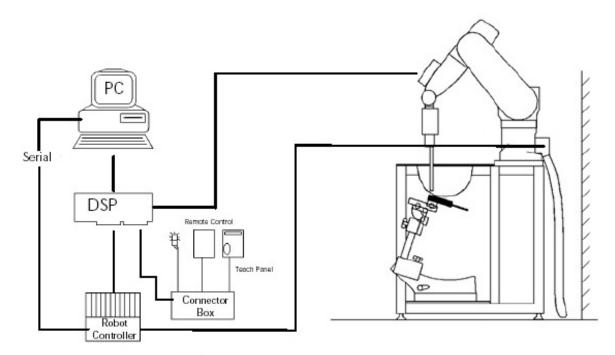


Figure 2.1 SAR Measurement System Setup



System Electronics

The DAE4 consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the PC-card is accomplished through an optical downlink for data and status information and an optical uplink for commands and clock lines. The mechanical probe mounting device includes two different sensor systems for frontal and sidewise probe contacts. They are also used for mechanical surface detection and probe collision detection. The robot uses its own controller with a built in VME-bus computer. The system is described in detail in.

Probe Measurement System

The SAR measurements were conducted with the dosimetric probe EX3DV4, designed in the classical triangular configuration (see Fig. 2.2) and optimized for dosimetric evaluation. The probe is constructed using the thick film technique; with printed resistive lines on ceramic substrates. The probe is equipped with an optical multi fiber line ending at the front of the probe tip. (see Fig. 2.3) It is connected to the EOC box on the robot arm and provides an automatic detection of the phantom surface. Half of the fibers are connected to a pulsed infrared transmitter, the other half to a synchronized receiver. As the probe approaches the surface, the reflection from the surface produces a coupling from the transmitting to the receiving fibers. This reflection increases first during the approach, reaches maximum and then decreases. If the probe is flatly touching the surface, the coupling is zero. The distance of the coupling maximum to the surface is independent of the surface reflectivity and largely independent of the surface to probe angle. The DASY52 software reads the reflection during a software approach and looks for the maximum using a 2nd order fitting. The approach is stopped at reaching the maximum.



DAE System



Probe Specifications

Calibration: In air from 10 MHz to 6.0 GHz In brain and muscle simulating tissue at Frequencies of 450 MHz, 835 MHz, 1750 MHz, 1900 MHz, 2450 MHz, 2600 MHz, 3500 MHz, 5200 MHz, 5300 MHz, 5600 MHz, 5800 MHz

- Frequency: 10 MHz to 6 GHz
- Linearity: ±0.2dB (30 MHz to 6 GHz)
- Dynamic: 10 mW/kg to 100 W/kg




Figure 2.2 Triangular Probe Configurations

- Range: Linearity: ±0.2dB
- Dimensions: Overall length: 330 mm
- Tip length: 20 mm
- Body diameter: 12 mm
- Tip diameter: 2.5 mm

Distance from probe tip to sensor center: 1 mm

Application: SAR Dosimetry Testing Compliance tests of wireless device



Figure 2.3 Probe Thick-Film Technique



Probe Calibration Process

Dosimetric Assessment Procedure

Each probe is calibrated according to a dosimetric assessment procedure described in with accuracy better than +/-10%. The spherical isotropy was evaluated with the procedure described in and found to be better than +/-0.25dB. The sensitivity parameters (Norm X, Norm Y, Norm Z), the diode compression parameter (DCP) and the conversion factor (Conv F) of the probe is tested.

Free Space Assessment

The free space E-field from amplified probe outputs is determined in a test chamber. This is performed in a TEM cell for frequencies below 1 GHz, and in a waveguide above 1GHz for free space. For the free space calibration, the probe is placed in the volumetric center of the cavity at the proper orientation with the field. The probe is then rotated 360 degrees until the three channels show the maximum reading. The power density readings equates to 1 mW/cm².

Temperature Assessment *

E-field temperature correlation calibration is performed in a flat phantom filled with the appropriate simulated brain tissue. The measured free space E-field in the medium, correlates to temperature rise in a dielectric medium. For temperature correlation calibration a RF transparent thermistor based temperature probe is used in conjunction with the E-field probe

$$SAR = C \frac{\Delta T}{\Delta t} \qquad SAR = \frac{|E|^2 \cdot \sigma}{\rho}$$

where:

=

С

where:

 Δt = exposure time (30 seconds),

 σ = simulated tissue conductivity,

heat capacity of tissue (brain or muscle), $\rho = \text{Tissue}$ density (1.25 g/cm³ for brain tissue)

 ΔT = temperature increase due to RF exposure.

SAR is proportional to $\Delta T / \Delta t$, the initial rate of tissue heating, before thermal diffusion takes place. Now it's possible to quantify the electric field in the simulated tissue by equating the thermally derived SAR to the E- field;




Figure 2.4 E-Field and Temperature Measurements at 900MHz




Figure 2.5 E-Field and Temperature Measurements at 1800MHz



Data Extrapolation

The DASY52 software automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given like below;

$$F_{i} = U_{i} + U_{i}^{2} \cdot \frac{\mathcal{G}}{dcp_{i}}$$
with V_{i} = compensated signal of channel i (i=x,y,z)
 U_{i} = input signal of channel i (i=x,y,z)
 cf = crest factor of exciting field (DASY parameter)
 dcp_{i} = diode compression point (DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

with

E-field probes:

$$E_{i} = \sqrt{\frac{V_{i}}{Norm_{i} \cdot ConvF}}$$
Norm

Vi.	= compensated signal of channel i (i = x,y,z)
Norm,	= sensor sensitivity of channel i (i = x,y,z)
	μV/(V/m) ² for E-field probes
ConvF	= sensitivity of enhancement in solution
E.	= electric field strength of channel i in V/m

The RSS value of the field components gives the total field strength (Hermetian magnitude):

 $E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$

The primary field data are used to calculate the derived field units.

$SAR = E_{bot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$	with	SAR Etor	 local specific absorption rate in W/g total field strength in V/m
p 1000		σ	= conductivity in [mho/m] or [Siemens/m]
		ρ	= equivalent tissue density in g/cm ³

The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pure} = \frac{E_{hut}^2}{3770}$$
 with $P_{pwe} = equivalent power density of a plane wave in W/cm2} = total electric field strength in V/m$



Scanning procedure

- The DASY installation includes predefined files with recommended procedures for measurements and system check. They are read-only document files and destined as fully defined but unmeasured masks. All test positions (head or body-worn) are tested with the same configuration of test steps differing only in the grid definition for the different test positions.
- The "reference" and "drift" measurements are located at the beginning and end of the batch process. They measure the field drift at one single point in the liquid over the complete procedure. The indicated drift is mainly the variation of the DUT's output power and should vary max. +/- 5 %.
- The highest integrated SAR value is the main concern in compliance test applications. These values can mostly be found at the inner surface of the phantom and cannot be measured directly due to the sensor offset in the probe. To extrapolate the surface values, the measurement distances to the surface must be known accurately. A distance error of 0.5mm could produce SAR errors of 6% at 1800 MHz. Using predefined locations for measurements is not accurate enough. Any shift of the phantom (e.g., slight deformations after filling it with liquid) would produce high uncertainties. For an automatic and accurate detection of the phantom surface, the DASY5 system uses the mechanical surface the indicated distance before starting the measurement.
- The "area scan" measures the SAR above the DUT or verification dipole on a parallel plane to the surface. It is used to locate the approximate location of the peak SAR with 2D spline interpolation. The robot performs a stepped movement along one grid axis while the local electrical field strength is measured by the probe. The probe is touching the surface of the SAM during acquisition of measurement values. The scan uses different grid spacings for different frequency measurements. Standard grid spacing for head measurements in frequency ranges 2GHz is 15 mm in x and y-dimension. For higher frequencies a finer resolution is needed, thus for the grid spacing is reduced according the following table:

Area scan grid spacing for different frequency ranges				
Frequency range Grid spacing				
≤ 2 GHz	≤ 15 mm			
2 – 4 GHz	≤ 12 mm			
4 – 6 GHz	≤ 10 mm			

Grid spacing and orientation have no influence on the SAR result. For special applications where the standard scan method does not find the peak SAR within the grid, e.g. mobile phones with flip cover, the grid can be adapted in orientation. Results of this coarse scan are shown in annex B.

• A "zoom scan" measures the field in a volume around the 2D peak SAR value acquired in the previous "coarse" scan. It uses a fine meshed grid where the robot moves the probe in steps along all the 3 axis (x,y and z-axis) starting at the bottom of the Phantom. The grid spacing for the cube measurement is varied according to the measured frequency range, the dimensions are given in the following table:

Zoom scan grid spacing and volume for different frequency ranges						
Frequency range	Grid spacing	Grid spacing	Minimum zoom			
r requericy range	for x, y axis	for z axis	scan volume			
≤ 2 GHz	≤ 8 mm	≤ 5 mm	≥ 30 mm			
2 – 3 GHz	≤ 5 mm	≤ 5 mm	≥ 28 mm			
3 – 4 GHz	≤ 5 mm	≤ 4 mm	≥ 28 mm			
4 – 5 GHz	≤ 4 mm	≤ 3 mm	≥ 25 mm			
5 – 6 GHz	≤ 4 mm	≤ 2 mm	≥ 22 mm			



DASY is also able to perform repeated zoom scans if more than 1 peak is found during area scan. In this document, the evaluated peak 1g and 10g averaged SAR values are shown in the 2D-graphics in annex B. Test results relevant for the specified standard (see section 3) are shown in table form in section 7.

Spatial Peak SAR Evaluation

The spatial peak SAR - value for 1 and 10 g is evaluated after the Cube measurements have been done. The basis of the evaluation are the SAR values measured at the points of the fine cube grid consisting of all points in the three directions x, y and z. The algorithm that finds the maximal averaged volume is separated into three different stages.

- The data between the dipole center of the probe and the surface of the phantom are extrapolated. This data cannot be measured since the center of the dipole is 1 to 2.7 mm away from the tip of the probe and the distance between the surface and the lowest measuring point is about 1 mm (see probe calibration sheet). The extrapolated data from a cube measurement can be visualized by selecting 'Graph Evaluated'.
- The maximum interpolated value is searched with a straight-forward algorithm. Around this maximum the SAR values averaged over the spatial volumes (1g or 10 g) are computed using the 3d-spline interpolation algorithm. If the volume cannot be evaluated (i.e., if a part of the grid was cut off by the boundary of the measurement area) the evaluation will be started on the corners of the bottom plane of the cube.
- All neighbouring volumes are evaluated until no neighbouring volume with a higher average value is found.

Extrapolation

The extrapolation is based on a least square algorithm [W. Gander, Computermathematik, p.168-180]. Through the points in the first 3 cm along the z-axis, polynomials of order four are calculated. These polynomials are then used to evaluate the points between the surface and the probe tip. The points, calculated from the surface, have a distance of 1 mm from each other.

Interpolation

The interpolation of the points is done with a 3d-Spline. The 3d-Spline is composed of three onedimensional splines with the "Not a knot"-condition [W. Gander, Computermathematik, p.141-150] (x, y and z -direction) [Numerical Recipes in C, Second Edition, p.123ff].

Volume Averaging

At First the size of the cube is calculated. Then the volume is integrated with the trapezoidal algorithm. 8000 points (20x20x20) are interpolated to calculate the average.

Advanced Extrapolation

DASY uses the advanced extrapolation option which is able to compensate boundary effects on E-field probes.



SAM PHANTOM

The SAM Twin Phantom V4.0 is constructed of a fiberglass shell integrated in a wooden table. The shape of the shell is based on data from an anatomical study designed to determine the maximum exposure in at least 90% of all users. It enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region. A cover prevents the evaporation of the liquid. Reference markings on the Phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points in the robot. (see Fig. 2.6)

Phantom Specification

Phantom:	SAM ⁻
Shell Material:	Viva
Thickness:	2.0 ±

SAM Twin Phantom (V4.0) Vivac Composite 2.0 ± 0.2 mm



Figure 2.6 SAM Twin Phantom

Device Holder for Transmitters

In combination with the SAM Twin Phantom V4.0 the Mounting Device (see Fig. 2.7), enables the rotation of the mounted transmitter in spherical coordinates whereby the rotation point is the ear opening. The devices can be easily, accurately, and repeat ably be positioned according to the FCC, CENELEC, IEC and IEEE specifications. The device holder can be locked at different phantom locations (left head, right head, flat phantom).



Figure 2.7 Mounting Device

Note: A simulating human hand is not used due to the complex anatomical and geometrical structure of the hand that may produce infinite number of configurations. To produce the worstcase condition (the hand absorbs antenna output power), the hand is omitted during the tests.



3. Definition of Reference Points

Ear Reference Point

Figure 3.2 shows the front, back and side views of the SAM Phantom. The point "M" is the reference point for the center of the mouth, "LE" is the left ear reference point (ERP), and "RE" is the right ERP. The ERPs are 15mm posterior to the entrance to the ear canal (EEC) along the B-M line (Back-Mouth), as shown in Figure 3.1. The plane passing through the two ear canals and M is defined as the Reference Plane. The line N-F (Neck-Front) is perpendicular to the reference plane and passing through the RE (or LE) is called the Reference Pivoting Line (see Figure 3.1). Line B-M is perpendicular to the N-F line. Both N-F and B-M lines are marked on the external phantom shell to facilitate handset positioning [5].




Figure 3.1 Close-up side view of ERP's



Figure 3.2 Front, back and side view of SAM

Device Reference Points

Two imaginary lines on the device need to be established: the vertical centerline and the horizontal line. The test device is placed in a normal operating position with the "test device reference point" located along the "vertical centerline" on the front of the device aligned to the "ear reference point" (See Fig. 3.3). The "test device reference point" is than located at the same level as the center of the ear reference point. The test device is positioned so that the "vertical centerline" is bisecting the front surface of the device at it's top and bottom edges, positioning the "ear reference point" on the outer surface of both the left and right head phantoms on the ear reference point [5].





Figure 3.3 Handset Vertical Center & Horizontal Line Reference Points





4. Test Configuration Positions

Positioning for Cheek/Touch [5]

 Position the device close to the surface of the phantom such that point A is on the (virtual) extension of the line passing through points RE and LE on the phantom (see Figure 4.1), such that the plane defined by the vertical center line and the horizontal line of the device is approximately parallel to the sagittal plane of the phantom.



Figure 4.1 Front, Side and Top View of Cheek/Touch Position

- 2. Translate the device towards the phantom along the line passing through RE and LE until the device touches the ear.
- 3. While maintaining the device in this plane, rotate it around the LE-RE line until the vertical centerline is in the plane normal to MB-NF including the line MB (called the reference plane).
- 4. Rotate the device around the vertical centerline until the device (horizontal line) is symmetrical with respect to the line NF.
- 5. While maintaining the vertical centerline in the reference plane, keeping point A on the line passing through RE and LE and maintaining the device contact with the ear, rotate the device about the line NF until any point on the device is in contact with a phantom point below the ear (cheek). See Figure 4.2.




Figure 4.2 Side view w/ relevant markings



Positioning for Ear / 15° Tilt [5]

With the test device aligned in the Cheek/Touch Position":

- 1. While maintaining the orientation of the device, retracted the device parallel to the reference plane far enough to enable a rotation of the device by 15 degrees.
- 2. Rotate the device around the horizontal line by 15 degrees.
- 3. While maintaining the orientation of the device, move the device parallel to the reference plane until any part of the device touches the head. (In this position, point A is located on the line RE-LE). The tilted position is obtained when the contact is on the pinna. If the contact is at any location other than the pinna, the angle of the device shall be reduced. The tilted position is obtained when any part of the device is in contact with the ear as well as a second part of the device is in contact with the head (see Figure 4.3).



Figure 4.3 Front, Side and Top View of Ear/15° Tilt Position



Body Worn Configurations

Body-worn operating configurations are tested with the accessories attached to the device and positioned against a flat phantom in a normal use configuration. A device with a headset output is tested with a headset connected to the device. Body dielectric parameters are used.

Accessories for Body-worn operation configurations are divided into two categories: those that do not contain metallic components and those that do contain metallic components. When multiple accessories that do not contain metallic components are supplied with the device, the device is tested with only the accessory that dictates the closest spacing to the body. Then, when multiple accessories that contain metallic components are supplied with the device, the device, the device is tested with each accessory that contains a unique metallic component. If multiple accessories share an identical metallic component (i.e. the same metallic belt-clip used with different holsters with no other metallic components) only the accessory that dictates the closest spacing to the body is tested.

Body-worn accessories may not always be supplied or available as options for some devices intended to be authorized for body-worn use. In this case, a test configuration where a separation distance between the back of the device and the flat phantom is used. All test position spacings are documented.

Transmitters that are designed to operate in front of a person's face, as in push-to-talk configurations, are tested for SAR compliance with the front of the device positioned to face the flat phantom. For devices that are carried next to the body such as a shoulder, waist or chest-worn transmitters, SAR compliance is tested with the accessory(ies), including headsets and microphones, attached to the device and positioned against a flat phantom in a normal use configuration.

In all cases SAR measurements are performed to investigate the worst-case positioning. Worst-case positioning is then documented and used to perform Body SAR testing.

In order for users to be aware of the body-worn operating requirements for meeting RF exposure compliance, operating instructions and cautions statements are included in the user's manual.



5. Probe and Dipole Calibration

See Appendix D and E.

6. Phantom & Simulating Tissue Specifications

Head & Body Simulating Mixture Characterization

The head and body mixtures consist of the material based on the table listed below. The mixture is calibrated to obtain proper dielectric constant (permittivity) and conductivity of the desired tissue. Body tissue parameters that have not been specified in IEEE1528 – 2013 are derived from the issue dielectric parameters computed from the 4-Cole-Cole equations.

Table 6.1 Typical composition of ingreatenes for hoode							
Ingredients		Simulating Tissue					
		750 MHz Head	900 MHz Head	1750 MHz Head	1900 MHz Head		
Mixing Percentage							
Water							
Sugar Salt		Proprietary Proprietary Purchased From Purchased From Pu Speag Speag	Purchased From	Proprietary Purchased From Speag	Proprietary Purchased From Speag		
						HEC	
Bactericide							1 0
DGBE							
Dielectric Constant Target		41.69	41.50	40.08	40.00		
Conductivity (S/m) Target		0.89	0.97	1.37	1.40		

Table 6.1 Typical Composition of Ingredients for Tissue

Ingredients		Simulating Tissue					
		2300 MHz Head	2550 MHz Head	3 GHz Head	2450 MHz Head		
Mixing Percentage							
Water							
Sugar		Proprietary	Proprietary Purchased From Speag	Proprietary Purchased From Speag	Proprietary Purchased From Speag		
Salt							
HEC		Speag					
Bactericide					1 0		
DGBE							
Dielectric Constant Target		39.47	39.07	Various	39.20		
Conductivity (S/m) Target		1.67	1.91	Various	1.80		



7. ANSI/IEEE C95.1 – 1992 RF Exposure Limits [2]

Uncontrolled Environment

Uncontrolled Environments are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure. The general population/uncontrolled exposure limits are applicable to situations in which the general public may be exposed or in which persons who are exposed as a consequence of their employment may not be made fully aware of the potential for exposure or cannot exercise control over their exposure. Members of the general public would come under this category when exposure is not employment-related; for example, in the case of a wireless transmitter that exposes persons in its vicinity.

Controlled Environment

Controlled Environments are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation). In general, occupational/controlled exposure limits are applicable to situations in which persons are exposed as a consequence of their employment, who have been made fully aware of the potential for exposure and can exercise control over their exposure. This exposure category is also applicable when the exposure is of a transient nature due to incidental passage through a location where the exposure levels may be higher than the general population/uncontrolled limits, but the exposed person is fully aware of the potential for exposure and can exercise control over his or her exposure by leaving the area or by some other appropriate means.

	UNCONTROLLED ENVIRONMENT General Population (W/kg) or (mW/g)	CONTROLLED ENVIROMENT Professional Population (W/kg) or (mW/g)			
SPATIAL PEAK SAR ¹ Head	1.60	8.00			
SPATIAL AVERAGE SAR ² Whole Body	0.08	0.40			
SPATIAL PEAK SAR ³ Hands, Feet, Ankles, Wrists	4.00	20.00			

Table 7.1 Human Exposure Limits

¹ The Spatial Peak value of the SAR averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

² The Spatial Average value of the SAR averaged over the whole body.

³ The Spatial Peak value of the SAR averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.



8. Measurement Uncertainty

Measurement uncertainty table is not required per KDB 865664 D01 v01 section 2.8.2 page 12. SAR measurement uncertainty analysis is required in the SAR report only when the highest measured SAR in a frequency band is \geq 1.5 W/kg for 1-g SAR. The equivalent ratio (1.5/1.6) should be applied to extremity and occupational exposure conditions. The highest reported value is less than 1.5 W/kg. Therefore, the measurement uncertainty table is not required.



9. System Validation

Tissue Verification

		750 MHz Head		900 MHz Head		1750 MHz Head		
Date(s)		Jul. 5, 2022		Jul. 7, 2022		Jul. 8, 2022		
Liquid Temperature (°C)	20.0	Target	Measured	Target	Measured	Target	Measured	
Dielectric Constant: ε		41.94	41.46	41.50	41.34	40.08	39.24	
Conductivity: σ		0.89	0.91	0.97	0.98	1.37	1.40	
		1900	MHz Head	2300 MHz Head		2550 MHz Head		
Date(s)		Jul.	11, 2022	Jul. 12, 2022		Jul. 13, 2022		
Liquid Temperature (°C)	20.0	Target	Measured	Target	Measured	Target	Measured	
Dielectric Constant: ε		40.00	39.87	39.47	38.18	39.07	38.95	
Conductivity: σ		1.40	1.39	1.67	1.69	1.91	1.94	
		3500	MHz Head	2450 MHz Head				
Date(s)		Jul. 14, 2022		Jul. 15, 2022				
Liquid Temperature (°C)	20.0	Target	Measured	Target	Measured			
Dielectric Constant: ε		37.93	37.00	39.20	38.34			
Conductivity: σ		2.91	2.96	1.80	1.81			

Table 9.1 Measured Tissue Parameters

See Appendix A for data printout.

Test System Verification

Prior to assessment, the system is verified to the $\pm 10\%$ of the specifications at the test frequency by using the system kit. Power is normalized to 1 watt. (Graphic Plots Attached)

Table 9.2 System Dipole Validation Target & Measured

	Test Frequency	Targeted SAR _{1g} (W/kg)	Measure SAR _{1g} (W/kg)	Tissue Used for Verification	Deviation (%)	Plot Number
05-Jul-2022	750 MHz	8.57	8.58	Head	+ 0.12	1
07-Jul-2022	900 MHz	11.20	11.50	Head	+ 2.68	2
08-Jul-2022	1750 MHz	37.70	37.80	Head	+ 0.27	3
11-Jul-2022	1900 MHz	40.40	41.50	Head	+ 2.72	4
12-Jul-2022	2300 MHz	49.60	49.80	Head	+ 0.40	5
13-Jul-2022	2550 MHz	55.30	56.40	Head	+ 1.99	6
14-Jul-2022	3500 MHz	67.00	67.80	Head	+ 1.19	7
15-Jul-2022	2450 MHz	54.10	54.60	Head	+ 0.92	8

See Appendix A for data plots.




Figure 9.1 Dipole Validation Test Setup



10. SAR Test Data Summary See Measurement Result Data Pages

See Appendix B for SAR Test Data Plots. See Appendix C for SAR Test Setup Photos.

Procedures Used To Establish Test Signal

The device was either placed into simulated transmit mode using the manufacturer's test codes or the actual transmission is activated through a base station simulator or similar equipment. See data pages for actual procedure used in measurement.

Device Test Condition

In order to verify that the device was tested at full power, conducted output power measurements were performed before and after each SAR measurement to confirm the output power unless otherwise noted. If a conducted power deviation of more than 5% occurred, the test was repeated. The power drift of each test is measured at the start of the test and again at the end of the test. The drift percentage is calculated by the formula ((end/start)-1)*100 and rounded to three decimal places. The drift percentage is calculated into the resultant SAR value on the data sheet for each test.

All testing was conducted based on the test plan submitted by the client.



11. FCC 3G Measurement Procedures

Power measurements were performed using a base station simulator under average power.

11.1 Procedures Used to Establish RF Signal for SAR

The device was placed into a simulated call using a base station simulator in a screen room. Such test signals offer a consistent means for testing SAR and recommended for evaluating SAR. The SAR measurement software calculates a reference point at the start and end of the test to check for power drifts. If conducted power deviations of more than 5% occurred, the tests were repeated.

11.2 SAR Measurement Conditions for WCDMA/HSDPA/HSUPA

Configure the call box 8960 to support all WCDMA tests in respect to the 3GPP 34.121 (listed in Table below). Measure the power at Ch4132, 4182 and 4233 for US cell; Ch9262, 9400 and 9538 for US PCS band.

For Rel99

For HSDPA Rel 6	 Set a Test Mode 1 loop back with a 12.2kbps Reference Measurement Channel (RMC). Set and send continuously Up power control commands to the device Measure the power at the device antenna connector using the power meter with average detector.
	 Establish a Test Mode 1 look back with both 1 12.2kbps RMC channel and a H-Set1 Fixed Reference Channel (FRC). With the 8960 this is accomplished by setting the signal Channel Coding to "Fixed Reference Channel" and configuring for HSET-1 QKSP. Set beta values and HSDPA settings for HSDPA Subtest1 according to Table below.
For HSUPA Rel 6	 Send continuously Up power control commands to the device Measure the power at the device antenna connector using the power meter with modulated average detector. Repeat the measurement for the HSDPA Subtest2, 3 and 4 as given in Table below.
	 Use UL RMC 12.2kbps and FRC H-Set1 QPSK, Test Mode 1 loop back. With the 8960 this is accomplished by setting the signal Channel Coding to "E-DCH Test Channel" and configuring the equipment category to Cat5_10ms. Set the Absolute Grant for HSUPA Subtest1 according to Table below. Set the device power to be at least 5dB lower than the Maximum output power Send power control bits to give one TPC_cmd = +1 command to the device. If device doesn't send any E-DPCH data with decreased E-TFCI within 500ms, then repeat this process until the decreased E-TFCI is reported. Confirm that the E-TFCI transmitted by the device is equal to the target E-TFCI in Table below. If the E-TFCI transmitted by the device is not equal to the target E-TFCI, then send power control bits to give one TPC_cmd = -1 command to the UE. If UE sends any E-DPCH data with decreased E-TFCI within 500 ms, send new power control bits to give one TPC_cmd = -1 command to the UE. Measure the power using the power meter with modulated average detector.



Report Number: SAR.20220706

Band	Mode	Bandwidth (MHz)	Channel	Frequency (MHz)	Data Rate	Avg Power (dBm)	Tune-up Pwr (dBm)					
	802.11b		1	2412	1	15.00	16.00					
		20	6	2437	ر Mbps	15.20	16.00					
			11	2462	winhs	15.10	16.00					
		20	1	2412	C	Net Deguined	15.00					
2450 MHz	802.11g		6	2437	6 Mbps		15.00					
			11	2462	winhs		15.00					
			1	2412		Not Required	15.00					
	802.11n	20	6	2437	MCS7		15.00					
			11	2462			15.00					

Power Measurements M0007

Power Measurements M0008

Band	Mode	Bandwidth (MHz)	Channel	Frequency (MHz)	Data Rate	Avg Power (dBm)	Tune-up Pwr (dBm)
			1	2412	1	15.20	16.00
	802.11b	20	6	2437	1	15.50	16.00
			11	2462	Mbps	15.30	16.00
		20	1	2412	C	Not Required	15.00
2450 MHz	802.11g		6	2437	6 Mbps		15.00
			11	2462	winhz		15.00
			1	2412	MCS7		15.00
	802.11n	20	6	2437			15.00
			11	2462			15.00

Power Measurements M0007

Band	Mode	Channel	Frequency (MHz)	Data Rate	Avg Power (dBm)	Tune-up Pwr (dBm)
2450 MHz	Bluetooth v4.0	0	2402		-21.66	-10.00
		19	2441	BLE GFSK	-19.17	-10.00
		39	2480		-15.42	-10.00

Power Measurements M0008

Band	Mode	Channel	Frequency (MHz)	Data Rate	Avg Power (dBm)	Tune-up Pwr (dBm)
2450 MHz	Bluetooth v4.0	0	2402		-21.66	-10.00
		19	2441	BLE GFSK	-19.17	-10.00
	V4.0	39	2480		-15.42	-10.00



SAR Data Summary – Head Measurements (M0007)

MEASUREMENT RESULTS

Plot	Frequency		Modulation	Position	RMC/RB	Test Setup/	Measured	Original
•	MHz	Ch.				Offset	SAR (W/Kg)	SAR (W/kg)
	707 5	22005		Pight Touch	1	24	0.289	0.287
707.5		23095	LIL	Right Touch	1	24	0.231	
0.20		26965	ITE	Right Touch 1		27	0.257	0.286
	030.5	20005	LIL	Right Touch	I	57	0.196	
	17/5 0	132322		Left Touch	1	37	0.241	0.244
	1745.0	132322	LIL	Leit Touch	1	51	0.165	
	1007.6	0528		Loft Touch	12.2 khpa	Toot Loop 1	0.216	0.235
	1907.0	9000	VCDIVIA	Leit Touch	12.2 K0p5	Test Loop T	0.159	
	2502.0	40620	I TE	Loft Touch	1	40	0.169	0.178
	2595.0	40020	LIE	E Left Touch		49	0.102	
1	2625	55000	I TE	Pight Touch	1	40	0.502	0.536
2	3025	22990	ILIE Right Touch 1			1 49		
	 1	Plot MHz 707.5 836.5 1745.0 1907.6 2593.0 1 3625	Plot MHz Ch. 707.5 23095 836.5 26865 1745.0 132322 1907.6 9538 2593.0 40620 1 3625 55990	Plot MHz Ch. 707.5 23095 LTE 836.5 26865 LTE 1745.0 132322 LTE 1907.6 9538 WCDMA 2593.0 40620 LTE 1 3625 55990 LTE	MHz Ch. Position 707.5 23095 LTE Right Touch 836.5 26865 LTE Right Touch 836.5 26865 LTE Right Touch 1745.0 132322 LTE Left Touch 1907.6 9538 WCDMA Left Touch 2593.0 40620 LTE Left Touch 1 3625 55990 LTE Right Touch	MHz Ch. Position Position RMC/RB 707.5 23095 LTE Right Touch 1 836.5 26865 LTE Right Touch 1 836.5 26865 LTE Right Touch 1 1745.0 132322 LTE Left Touch 1 1907.6 9538 WCDMA Left Touch 12.2 kbps 2593.0 40620 LTE Left Touch 1 1 3625 55990 LTE Right Touch 1	Mitz Ch. Position RMC/RB Offset 707.5 23095 LTE Right Touch 1 24 836.5 26865 LTE Right Touch 1 37 1745.0 132322 LTE Left Touch 1 37 1907.6 9538 WCDMA Left Touch 12.2 kbps Test Loop 1 2593.0 40620 LTE Left Touch 1 49 1 3625 55990 LTE Bight Touch 1 49	$ \begin{array}{c c c c c c c c c c c c c c c c c c c $

Head 1.6 W/kg (mW/g) averaged over 1 gram

- 1. Battery is fully charged for all tests. Power Measured
- 2. SAR Measurement Phantom Configuration SAR Configuration
- 3. Test Signal Call Mode
- 4. Test Configuration
- 5. Tissue Depth is at least 15.0 cm

Jay M. Moulton Vice President

- Left Head
- Head
- Test Code
- With Belt Clip
- Eli4 Right Head Body Base Station Simulator
- Without Belt Clip N/A

EIRP



SAR Data Summary – Body Measurements (M0007)

MEASUREMENT RESULTS

									-
Gap	Gap Plot	Frequency		Modulation	Position	RMC/RB	Test Setup/	Measured	Original
•		MHz	Ch.				Offset	SAR (W/kg)	SAR (W/kg)
		707.5	23095	LTE	Back	1	24	0.822	0.867
	707.5		23095	LIC	Back	I	24	0.731	
			26865	LTE	Back	1	37	0.657	0.770
		836.5	20005	LIL	Back	I	57	0.549	
		1745.0 132	132322	LTE	Bottom	1	37	0.702	0.694
10			132322			I	57	0.611	
mm	3	1907.6	9538	WCDMA	Back	12.2 kbps	Test Loop 1	0.959	1.082
	4	1907.0	9030	VCDIVIA	Back	12.2 K0p5		0.661	
		2593.0	40620	LTE	Bottom	1	49	0.832	0.876
		2595.0	40020		Bollom		49	0.718	
		3625	55990	LTE	Pight	1	49	0.503	0.528
		3025	22990	LIE	Right		49	0.418	

Head 1.6 W/kg (mW/g) averaged over 1 gram

EIRP

- 1. Battery is fully charged for all tests. Power Measured
- 2. SAR Measurement Phantom Configuration SAR Configuration
- 3. Test Signal Call Mode
- 4. Test Configuration
- 5. Tissue Depth is at least 15.0 cm

Jay M. Moulton Vice President

- . . .
- Left Head
- Head
- Test Code
- With Belt Clip
- Eli4 Right Head Body


ERP

Base Station Simulator Without Belt Clip



SAR Data Summary – WiFi Measurements (M0007)

MEASUREMENT RESULTS Measured Reported **End Power** Frequency Plot Modulation SAR Gap Position SAR MHz Ch. (dBm) (W/kg) (W/kg) 2412 DSSS 15.00 1 0.149 0.19 5 Left Touch 2437 6 DSSS 15.20 0.164 0.20 2462 DSSS 0.19 11 15.10 0.151 0 mm Left Tilt 15.20 0.12 2437 6 DSSS 0.103 ----Right Touch 2437 6 DSSS 15.20 0.116 0.14 ---------Right Tilt 2437 6 DSSS 15.20 0.0964 0.12 _____ Back 2437 6 DSSS 15.20 0.0856 0.10 10 mm Front 2437 6 DSSS 15.20 0.0649 0.08 -----Right 15.20 2437 DSSS 0.103 0.12 6 6 **Head Tissue** 1.6 W/kg (mW/g) averaged over 1 gram 1. Battery is fully charged for all tests. Power Measured Conducted ERP EIRP 2. SAR Measurement Right Head Phantom Configuration Left Head \boxtimes Eli4 SAR Configuration Head \boxtimes Body 3. Test Signal Call Mode Test Code Base Station Simulator 4. Test Configuration With Belt Clip Without Belt Clip N/A 5. Tissue Depth is at least 15.0 cm





SAR Data Summary – Simultaneous Evaluation (M0007)

MEASUREMENT RESULTS

Configuration	Frequency		Modulation	SAR ₁	SAR ₂	SAR ₂ Case ¹	SAR Total	
configuration	MHz	Ch.	Wouldton				JAN TUlai	
Head	2437	6	DSSS	0.502	0.20	0.004	0.706	
Body	2437	6	DSSS	0.959	0.12	0.004	1.083	
					1.6 W/kg (•,		

averaged over 1 gram

¹ – The Bluetooth transmitter is excluded from SAR testing due to the low power of the transmitter. The maximum power level is 4 dBm. Therefore, the SAR value was calculated. The following formula was used to calculate the SAR value for the Bluetooth transmitter.

[(max. power of channel, mW) / (min. test separation, mm)] * $\left[\sqrt{f_{(GHz)}/x}\right]$ W/kg, where x = 7.5 for 1 gram SAR

 $[0.1 \text{ mW} / 5 \text{ mm}] * [\sqrt{2.48/7.5}] = 0.01 \text{ W/kg}$

The sum of all transmitters is less than or equal to the limit; therefore, the simultaneous transmission meets the requirements.

SAR Data Summary – Head Measurements (M0008)

MEASUREMENT RESULTS

	1			n			P		
Gap	Plot	Frequency		Modulation	Position	RMC/RB	Test Setup/	Measured	Original
		MHz	Ch.				Offset	SAR (W/kg)	SAR (W/kg)
		680.5	133297	LTE	Right Touch	1	49	0.187	0.202
		000.5	133297	LIC	Right Touch	1	49	0.163	
	707.5		23095	LTE	Right Touch	1	24	0.142	0.154
		707.5	23095	LIL	Right Touch	1	24	0.129	
		836.6	4183	WCDMA	Right Touch	12.2 kbps	Test Loop 1	0.199	0.235
		030.0	4105	WODINA		12.2 Корз		0.158	
		1732.5	1413	WCDMA	Right Touch	12.2 kbps	Test Loop 1	0.357	0.399
0 mm		1752.5	1413	VCDIVIA	Right Fouch	12.2 Корз	Test Loop T	0.286	
0 mm		1907.6	9538	WCDMA	Right Touch	12.2 kbps	Test Loop 1	0.335	0.396
		1907.0	9000	VCDIVIA	Right Touch	12.2 K0p5	Test Loop T	0.273	
	7	2310.0	27710	LTE	Right Touch	1	24	0.455	0.480
	8	2310.0	21110	LIL	Right Touch	1	24	0.385	
		2593.0	40620	LTE	Right Touch	1	49	0.205	0.199
	2	2000.0	40020		Right Todell	1	49	0.110	
		3625	55990	LTE	Right Touch	1	49	0.256	0.295
		3025	22990			· ·	49	0.183	

Head 1.6 W/kg (mW/g) averaged over 1 gram

- 1. Battery is fully charged for all tests. Power Measured
- 2. SAR Measurement Phantom Configuration SAR Configuration
- ∐Left Head

With Belt Clip

Test Code

Head

EIRP

Eli4

ERP

Right Head

Body

Base Station Simulator

 $Without Belt Clip \qquad \boxtimes N/A$

- 3. Test Signal Call Mode
- 4. Test Configuration
- 5. Tissue Depth is at least 15.0 cm

SAR Data Summary – Body Measurements (M0008)

MEASUREMENT RESULTS

	1	1							
Gap	Plot	Frequency		Modulation	Position	RMC/RB	Test Setup/	Measured	Original
•		MHz	Ch.				Offset	SAR (W/kg)	SAR (W/kg)
		680.5	133297	LTE	Back	1	49	0.488	0.517
		000.0	133297	LIE	Back	1	49	0.392	
		707.5	23095	LTE	Back	1	24	0.728	0.741
		707.5	23095	LIL	Back	I	24	0.634	
		836.6	4183	WCDMA	Back	12.2 kbps	Test Loop 1	0.792	0.784
		030.0	4105	WODINA			Test Loop T	0.705	
		1732.5	1413	WCDMA	Bottom	12.2 kbps	Test Loop 1	0.922	0.943
5 mm		1752.5	1415	VCDIVIA				0.846	
5 11111	9	1907.6	9538	WCDMA	Bottom	12.2 kbps	bps Test Loop 1	0.941	0.997
	10	1907.0	9000	VCDIVIA	Bottom	12.2 KUPS	Test Loop T	0.777	
		2310.0	27710	LTE	Right	1	24	0.971	0.985
		2310.0	2//10	LIL	Right	1	24	0.864	
		2593.0	40620	LTE	Right	1	49	0.887	0.969
		2595.0	40020	LIL	NgIIt	1	49	0.794	
		3625	55990	LTE	Pight	1	49	0.856	0.849
		3025	22990	LIE	Right		49	0.739	

Head 1.6 W/kg (mW/g) averaged over 1 gram

EIRP

- 1. Battery is fully charged for all tests. Power Measured
- 2. SAR Measurement Phantom Configuration SAR Configuration
- ⊠Left Head
- Head
- Test Code
- With Belt Clip


ERP

- 3. Test Signal Call Mode
- 4. Test Configuration
- 5. Tissue Depth is at least 15.0 cm





SAR Data Summary – WiFi Measurements (M0008)

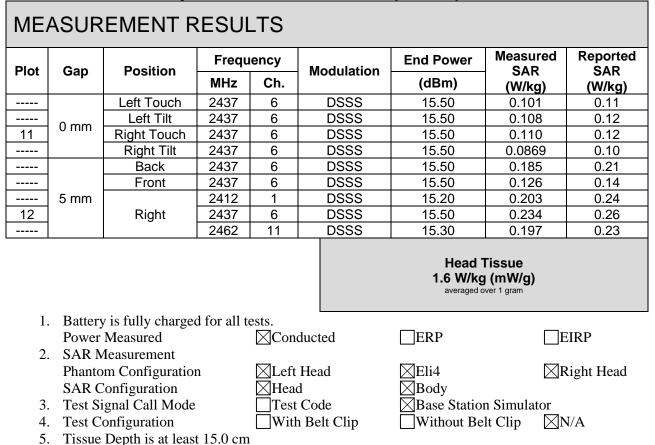





SAR Data Summary – Simultaneous Evaluation (M0008)

MEASUREMENT RESULTS												
Configuration	Frequ	ency	Modulation	SAR₁	SAR ₂	SAR₂ Case ¹	SAR Total					
configuration	MHz	Ch.	Modulation			SAN2 Case	SANTOLA					
Head	2437	6	DSSS	0.455	0.12	0.004	0.579					
Body	2437	6	DSSS	0.941	0.26	0.004	1.205					
					1.6 W/kg (averaged ove	•						

¹ – The Bluetooth transmitter is excluded from SAR testing due to the low power of the transmitter. The maximum power level is 4 dBm. Therefore, the SAR value was calculated. The following formula was used to calculate the SAR value for the Bluetooth transmitter.

[(max. power of channel, mW) / (min. test separation, mm)] * $\left[\sqrt{f_{(GHz)}/x}\right]$ W/kg, where x = 7.5 for 1 gram SAR

 $[0.1 \text{ mW} / 5 \text{ mm}] * [\sqrt{2.48}/7.5] = 0.004 \text{ W/kg}$

The sum of all transmitters is less than or equal to the limit; therefore, the simultaneous transmission meets the requirements.



12. Test Equipment List

Table 12.1 Equipment Specifications			
Туре	Calibration Due Date	Calibration Done Date	Serial Number
Staubli Robot TX60L	N/A	N/A	F07/55M6A1/A/01
Measurement Controller CS8c	N/A	N/A	1012
Twin SAM Phantom	N/A	N/A	1152
ELI5 Flat Phantom	N/A	N/A	2037
Device Holder	N/A	N/A	N/A
Data Acquisition Electronics 4	04/12/2022	04/12/2022	1416
SPEAG E-Field Probe EX3DV4	02/16/2023	02/16/2022	3662
Speag Validation Dipole D750V2	06/04/2023	06/04/2021	1053
Speag Validation Dipole D900V2	06/04/2023	06/04/2021	1d128
Speag Validation Dipole D1750V2	06/03/2023	06/03/2021	1061
Speag Validation Dipole D1900V2	06/04/2023	06/04/2021	5d147
Speag Validation Dipole D2300V2	06/03/2023	06/03/2021	1060
Speag Validation Dipole D2450V2	06/03/2023	06/03/2021	881
Speag Validation Dipole D2550V2	06/03/2023	06/03/2021	1003
Speag Validation Dipole D3500V2	04/13/2023	04/13/2021	1061
Agilent N1911A Power Meter	03/16/2023	03/16/2022	GB45100254
Agilent N1922A Power Sensor	03/17/2023	03/17/2022	MY45240464
Agilent (HP) 8561E Spectrum Analyzer	03/17/2023	03/17/2022	31720068
Agilent (HP) 83752A Synthesized Sweeper	03/17/2023	03/17/2022	3610A01048
Agilent (HP) 8753C Vector Network Analyzer	03/17/2023	03/17/2022	3135A01724
Agilent (HP) 85047A S-Parameter Test Set	03/16/2023	03/16/2022	2904A00595
Agilent 778D Dual Directional Coupler	N/A	N/A	MY48220184
Anritsu MT8820C	N/A	N/A	6201176199
MiniCircuits BW-N20W5+ Fixed 20 dB Attenuator	N/A	N/A	N/A
MiniCircuits SPL-10.7+ Low Pass Filter	N/A	N/A	R8979513746
Aprel Dielectric Probe Assembly	N/A	N/A	0011
Head Equivalent Matter (750 MHz)	N/A	N/A	N/A
Head Equivalent Matter (900 MHz)	N/A	N/A	N/A
Head Equivalent Matter (1750 MHz)	N/A	N/A	N/A
Head Equivalent Matter (1900 MHz)	N/A	N/A	N/A
Head Equivalent Matter (2300 MHz)	N/A	N/A	N/A
Head Equivalent Matter (2450 MHz)	N/A	N/A	N/A
Head Equivalent Matter (2550 MHz)	N/A	N/A	N/A
Head Equivalent Matter (3 GHz)	N/A	N/A	N/A

Table 12.1 Equipment Specifications



13. Conclusion

The SAR measurement indicates that the EUT complies with the RF radiation exposure limits of the FCC/ISED. These measurements are taken to simulate the RF effects exposure under worst-case conditions. Precise laboratory measures were taken to assure repeatability of the tests. The tested device complies with the requirements in respect to all parameters subject to the test. The test results and statements relate only to the item(s) tested.

Please note that the absorption and distribution of electromagnetic energy in the body is a very complex phenomena that depends on the mass, shape, and size of the body; the orientation of the body with respect to the field vectors; and, the electrical properties of both the body and the environment. Other variables that may play a substantial role in possible biological effects are those that characterize the environment (e.g. ambient temperature, air velocity, relative humidity, and body insulation) and those that characterize the individual (e.g. age, gender, activity level, debilitation, or disease). Because innumerable factors may interact to determine the specific biological outcome of an exposure to electromagnetic fields, any protection guide shall consider maximal amplification of biological effects as a result of field-body interactions, environmental conditions, and physiological variables.



14. References

[1] Federal Communications Commission, ET Docket 93-62, Guidelines for Evaluating the Environmental Effects of Radio Frequency Radiation, August 1996

[2] ANSI/IEEE C95.1 – 1992, American National Standard Safety Levels with respect to Human Exposure to Radio Frequency Electromagnetic Fields, 300kHz to 100GHz, New York: IEEE, 1992.

[3] ANSI/IEEE C95.3 – 1992, IEEE Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields – RF and Microwave, New York: IEEE, 1992.

[4] International Electrotechnical Commission, IEC 62209-2 (Edition 1.0), Human Exposure to radio frequency fields from hand-held and body mounted wireless communication devices – Human models, instrumentation, and procedures – Part 2: Procedure to determine the specific absorption rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz), March 2010.

[5] IEEE Standard 1528 – 2013, IEEE Recommended Practice for Determining the Peak-Spatial Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communication Devices: Measurement Techniques, June 2013.

[6] ISED, RSS – 102 Issue 5, Radio Frequency Exposure Compliance of Radiocommunication Apparatus (All Frequency Bands), March 2015.

[7] Health Canada, Safety Code 6, Limits of Human Exposure to Radiofrequency Electromagnetic Fields in the Frequency Range from 3kHz to 300 GHz, 2009.



Appendix A – System Validation Plots and Data

****	*****	******	******	****
Test Result f Tue 05/Jul/20 Freq Freque FCC_eH Limits FCC_SH Limits Test_e Epsilo Test_s Sigma ************** Freq 0.6700 0.6800 0.6805 0.6900 0.7000 0.7000 0.7075 0.7100 0.7255 0.7300 0.7400 0.7500 0.7600 0.7700 0.7700 0.7800	Cor UIM 22 for UIM for He for He of UIM ******* FCC_eH 42.36 42.31 42.307 42.25 42.20 42.163 42.15 42.10 42.073 42.05 41.99 41.84 41.79	Dielec ad Epsi ad Sign UIM ******* FCC_sH 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.89 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90 0.90	tric Pa ilon ma ******* Test_e 41.92 41.88 41.877 41.81 41.76 41.708 41.69 41.64 41.602 41.57 41.51 41.46 41.40 41.34 41.28	<pre>************************************</pre>
0.7900	41.73		41.22	
0.8000 41.68 0.90 41.18 0.94 * value interpolated				
<pre>************************************</pre>				
Freq 0.8000 0.8100 0.8200 0.8300 0.8366 0.8400 0.8500 0.8500 0.8600 0.8700 0.8800 0.8900 0.8976 0.9000 0.9100 0.9200	eH 41.68 41.63 41.58 41.53 41.51 41.50 41.50 41.50 41.50 41.50 41.50 41.50 41.50 41.50 41.50	sH 0.90 0.90 0.90 0.91 0.91 0.92 0.93 0.94 0.95 0.96 0.968 0.97 0.98 0.98	$\begin{array}{c} 41.52\\ 41.47\\ 41.41\\ 41.46\\ 41.44\\ 41.43\\ 41.43\\ 41.41\\ 41.39\\ 41.37\\ 41.36\\ 41.35 \end{array}$	

* value interpolated



Test Result for UIM Dielectric Parameter Fri 08/Jul/2022 Freq Frequency(GHz) eH Limits for Head Epsilon sH Limits for Head Sigma Test_e Epsilon of UIM Test_s Sigma of UIM FreqeHsHTest_e Test_s1.700040.161.3439.341.361.710040.141.3539.321.371.720040.131.3539.301.381.730040.111.3639.281.381.732640.1051.36339.2751.383*1.740040.091.3739.261.391.747540.0831.3739.2451.398*1.750040.081.3739.241.401.760040.061.3839.221.411.770040.051.3839.201.421.780040.031.3939.181.421.790040.021.3939.161.43 * value interpolated Test Result for UIM Dielectric Parameter Mon 11/Jul/2022 Freq Frequency(GHz) eH Limits for Head Epsilon sH Limits for Head Sigma Test_e Epsilon of UIM Test_s Sigma of UIM FreqeHsHTest_e Test_s1.850040.001.4039.971.371.860040.001.4039.951.381.870040.001.4039.931.381.880040.001.4039.911.391.882540.001.4039.9051.39*1.890040.001.4039.891.391.900040.001.4039.871.391.900640.001.4039.851.401.910040.001.4039.851.401.920040.001.4039.821.421.940040.001.4039.801.421.950040.001.4039.781.431.960040.001.4039.761.43 Freq eH sH Test_e Test_s

* value interpolated



Test Result for UIM Dielectric Parameter Tue 12/Jul/2022 Freq Frequency(GHz) FCC_eH Limits for Head Epsilon FCC_sH Limits for Head Sigma Test_e Epsilon of UIM Test_s Sigma of UIM ***** FCC_eH FCC_sH Test_e Test_s 39.48 1.66 38.2 1.68 39.47 1.67 38.18 1.69 Freq 2.2900 * value interpolated Test Result for UIM Dielectric Parameter Wed 13/Jul/2022 Freq Frequency(GHz) FCC_eH Limits for Head Epsilon FCC_sH Limits for Head Sigma Test_e Epsilon of UIM

```
Freq FCC_eH FCC_sH Test_e Test_s
FreqFCC_eH FCC_sH Test_e Test_s2.490039.151.8439.091.862.500039.141.8539.071.872.510039.121.8739.041.882.520039.111.8839.021.902.530039.101.8939.001.912.535039.0951.89538.9851.915*2.540039.091.9038.971.922.550039.061.9238.931.952.560039.061.9238.931.952.570039.051.9338.901.962.580039.031.9438.881.982.590039.021.9538.851.992.593039.0171.95338.8531.99*2.600039.011.9638.861.99
 2.6000
                             39.01 1.96 38.86 1.99
2.610039.001.9738.842.002.620038.981.9938.832.012.630038.972.0038.812.022.640038.962.0138.792.03
```

* value interpolated

Test_s Sigma of UIM



Test Result for UIM Dielectric Parameter Thu 14/Jul/2022 Freq Frequency(GHz) FCC_eH Limits for Head Epsilon FCC_sH Limits for Head Sigma Test_e Epsilon of UIM Test_s Sigma of UIM ***** FCC_eH FCC_sH Test_e Test_s 37.95 2.89 37.05 2.94 37.94 2.90 37.03 2.95 37.93 2.91 37.00 2.96 Freq 3.4800 3.4900 3.5000 3.5100 37.92 2.92 36.98 2.97 * value interpolated Test Result for UIM Dielectric Parameter Fri 15/Jul/2022 Freq Frequency(GHz) FCC_eH Limits for Head Epsilon FCC_sH Limits for Head Sigma Test_e Epsilon of UIM Test_s Sigma of UIM
 Freq
 FCC_eH FCC_sH Test_e Test_s

 2.4100
 39.26
 1.76
 38.44
 1.76
 2.4120 2.4200 2.4300 2.4370 2.4400 39.258 1.762 38.436 1.762* 39.25 1.77 38.42 1.77 39.24 1.78 38.40 1.78 39.226 1.787 38.393 1.794* 39.22 1.79 38.39 1.80 2.4500 39.20 1.80 38.34 1.81 2.4600 39.19 1.81 38.34 1.82 2.4620 39.186 1.812 38.336 1.822* 2.470039.171.8238.321.832.480039.161.8338.301.86

* value interpolated



Plot 1

DUT: Dipole 750 MHz D750V3; Type: D750V3; Serial: D750V3 - SN 1053


Communication System: CW; Frequency: 750 MHz; Duty Cycle: 1:1 Medium: HSL750; Medium parameters used (interpolated): f = 750 MHz; σ = 0.9 S/m; ϵ_r = 41.46; ρ = 1000 kg/m³ Phantom section: Flat Section

Test Date: Date: 7/5/2022; Ambient Temp: 23 °C; Tissue Temp: 21 °C Probe: EX3DV4 – SN3662; ConvF(9.23, 9.23, 9.23); Calibrated: 2/16/2022; Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1416; Calibrated: 4/12/2022 Phantom: ELI v5.0; Type: QDOVA002AA; Serial: 2037 Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Procedure Notes:

750 MHz Head/Verification/Area Scan (41x121x1): Interpolated grid: dx=1.500 mm, dy=1.500 mm Maximum value of SAR (interpolated) = 0.883 W/kg

750 MHz Head/Verification /Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 31.949 V/m; Power Drift = -0.03 dB Peak SAR (extrapolated) = 1.691 mW/g Pin= 100 mW SAR(1 g) = 0.858 mW/g; SAR(10 g) = 0.552 mW/g Maximum value of SAR (measured) = 0.888 W/kg

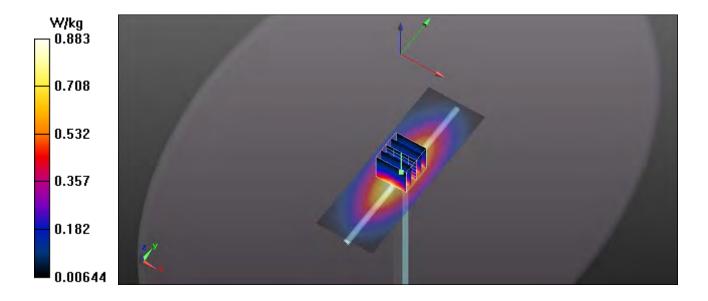



Plot 2

DUT: Dipole 900 MHz D900V2; Type: D900V2; Serial: D900V2 - SN:1d128

Communication System: CW; Frequency: 900 MHz; Duty Cycle: 1:1 Medium: HSL900; Medium parameters used: f = 900 MHz; σ = 0.98 S/m; ϵ_r = 41.34; ρ = 1000 kg/m³ Phantom section: Flat Section


Test Date: Date: 7/7/2022; Ambient Temp: 23 °C; Tissue Temp: 21 °C Probe: EX3DV4 – SN3662; ConvF(8.76, 8.76, 8.76); Calibrated: 2/16/2022; Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1416; Calibrated: 4/12/2022 Phantom: ELI v5.0; Type: QDOVA002AA; Serial: 2037 Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Procedure Notes:

900 MHz Head/Verification/Area Scan (5x11x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 1.19 W/kg

900 MHz Head/Verification/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 31.568 V/m; Power Drift = -0.02 dB Peak SAR (extrapolated) = 1.43 W/kg Pin= 100 mW SAR(1 g) = 1.15 W/kg; SAR(10 g) = 0.712 W/kg

Maximum value of SAR (measured) = 1.2 W/kg

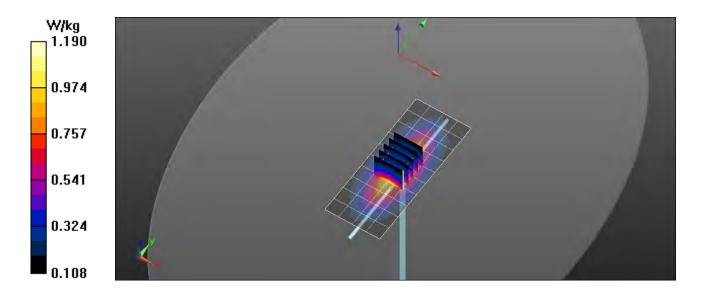



Plot 3

DUT: Dipole 1750 MHz D1750V2; Type: D1750V2; Serial: D1750V2 - SN:1061

Communication System: CW; Frequency: 1750 MHz; Duty Cycle: 1:1 Medium: HSL1750; Medium parameters used: f = 1750 MHz; σ = 1.4 S/m; ϵ_r = 39.24; ρ = 1000 kg/m³ Phantom section: Flat Section


Test Date: Date: 7/8/2022; Ambient Temp: 23 °C; Tissue Temp: 21 °C Probe: EX3DV4 – SN3662; ConvF(7.87, 7.87, 7.87); Calibrated: 2/16/2022; Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1416; Calibrated: 4/12/2022 Phantom: ELI v5.0; Type: QDOVA002AA; Serial: 2037 Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Procedure Notes:

1750 MHz Head/Verification/Area Scan (5x7x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 5.38 W/kg

1750 MHz Head/Verification/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 33.639 V/m; Power Drift = -0.02 dB Peak SAR (extrapolated) = 6.87 W/kg Pin= 100 mW SAR(1 g) = 3.78 W/kg; SAR(10 g) = 1.97 W/kg

Maximum value of SAR (measured) = 5.47 W/kg

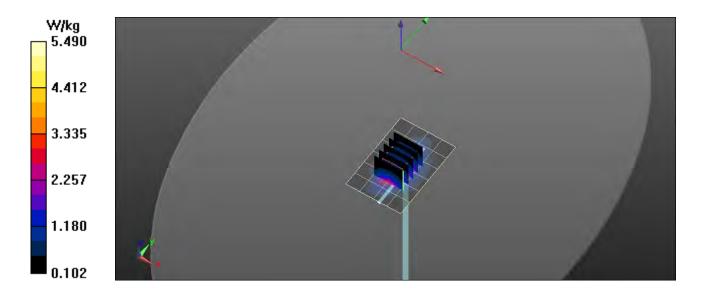



Plot 4

DUT: Dipole 1900 MHz D1900V2; Type: D1900V2; Serial: D1900V2 - SN: 5d147

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1 Medium: HSL1900; Medium parameters used: f = 1900 MHz; σ = 1.39 S/m; ϵ_r = 39.87; ρ = 1000 kg/m³ Phantom section: Flat Section


Test Date: Date: 7/11/2022; Ambient Temp: 23 °C; Tissue Temp: 21 °C Probe: EX3DV4 – SN3662; ConvF(7.66, 7.66, 7.66); Calibrated: 2/16/2022; Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1416; Calibrated: 4/12/2022 Phantom: ELI v5.0; Type: QDOVA002AA; Serial: 2037 Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Procedure Notes:

1900 MHz Head/Verification/Area Scan (5x7x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 5.52 W/kg

1900 MHz Head/Verification/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 32.186 V/m; Power Drift = -0.03 dB Peak SAR (extrapolated) = 7.25 W/kg Pin= 100 mW SAR(1 g) = 4.15 W/kg; SAR(10 g) = 2.16 W/kg

Maximum value of SAR (measured) = 5.79 W/kg

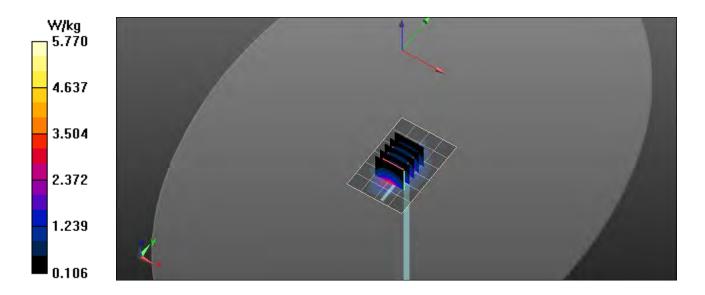



Plot 5

DUT: Dipole 2300 MHz D2300V2; Type: D2300V2; Serial: D2300V2 - SN: 1060

Communication System: CW; Frequency: 2300 MHz; Duty Cycle: 1:1 Medium: HSL2300; Medium parameters used: f = 2300 MHz; σ = 1.69 S/m; ϵ_r = 38.18; ρ = 1000 kg/m³ Phantom section: Flat Section


Test Date: Date: 7/12/2022; Ambient Temp: 23 °C; Tissue Temp: 21 °C Probe: EX3DV4 – SN3662; ConvF(7.54, 7.54, 7.54); Calibrated: 2/16/2022; Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1416; Calibrated: 4/12/2022 Phantom: ELI v5.0; Type: QDOVA002AA; Serial: 2037 Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Procedure Notes:

2300 MHz Head/Verification/Area Scan (61x101x1): Interpolated grid: dx=1.200 mm, dy=1.200 mm Maximum value of SAR (interpolated) = 7.83 W/kg

2300 MHz Head/Verification/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 55.297 V/m; Power Drift = -0.01 dB Peak SAR (extrapolated) = 11.06 W/kg Pin= 100 mW SAR(1 g) = 4.98 W/kg; SAR(10 g) = 2.42 W/kg

Maximum value of SAR (measured) = 8.93 W/kg

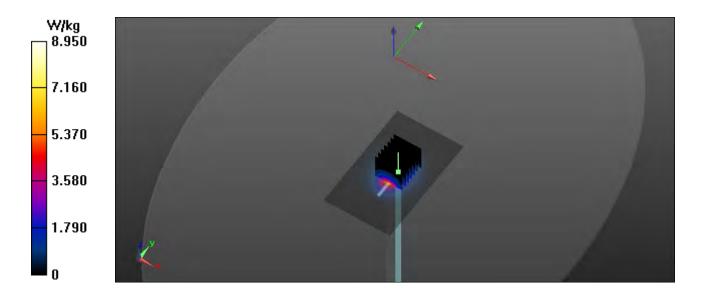



Plot 6

DUT: Dipole 2550 MHz D2550V2; Type: D2550V2; Serial: D2550V2 - SN:1003


Communication System: CW; Frequency: 2550 MHz; Duty Cycle: 1:1 Medium: HSL2550; Medium parameters used: f = 2550 MHz; σ = 1.94 S/m; ϵ_r = 38.95; ρ = 1000 kg/m³ Phantom section: Flat Section

Test Date: Date: 7/13/2022; Ambient Temp: 23 °C; Tissue Temp: 21 °C Probe: EX3DV4 – SN3662; ConvF(7.1, 7.1, 7.1); Calibrated: 2/16/2022; Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1416; Calibrated: 4/12/2022 Phantom: ELI v5.0; Type: QDOVA002AA; Serial: 2037 Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Procedure Notes:

2550 MHz Head/Verification/Area Scan (61x81x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm Maximum value of SAR (interpolated) = 9.18 W/kg

2550 MHz Head/Verification/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 54.541 V/m; Power Drift = -0.02 dB Peak SAR (extrapolated) = 11.5 W/kg Pin= 100 mW SAR(1 g) = 5.64 W/kg; SAR(10 g) = 2.48 W/kg Maximum value of SAR (measured) = 8.98 W/kg

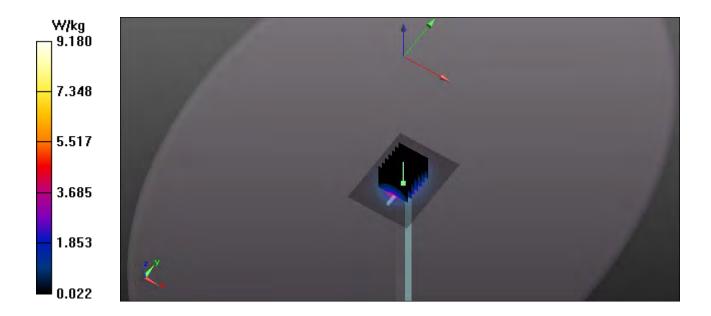



Plot 7

DUT: Dipole D3500V2; Type: D3500V2; Serial: D3500V2 - SN: 1061

Communication System: CW; Frequency: 3500 MHz; Duty Cycle: 1:1 Medium: HSL 3-6 GHz; Medium parameters used: f = 3500 MHz; σ = 2.96 S/m; ϵ_r = 37; ρ = 1000 kg/m³ Phantom section: Flat Section


Test Date: Date: 7/14/2022; Ambient Temp: 23 °C; Tissue Temp: 21 °C Probe: EX3DV4 – SN3662; ConvF(6.73, 6.73, 6.73); Calibrated: 2/16/2022; Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1416; Calibrated: 4/12/2022 Phantom: ELI v5.0; Type: QDOVA002AA; Serial: 2037 Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Procedure Notes:

3500 MHz Head/Verification/Area Scan (7x9x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (measured) = 1.62 W/kg

3500 MHz Head/Verification/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=4mm Reference Value = 14.849 V/m; Power Drift = -0.04 dB Peak SAR (extrapolated) = 3.64 W/kg P_{in}= 10 mW SAR(1 g) = 0.678 W/kg; SAR(10 g) = 0.256 W/kg

Maximum value of SAR (measured) = 1.68 W/kg

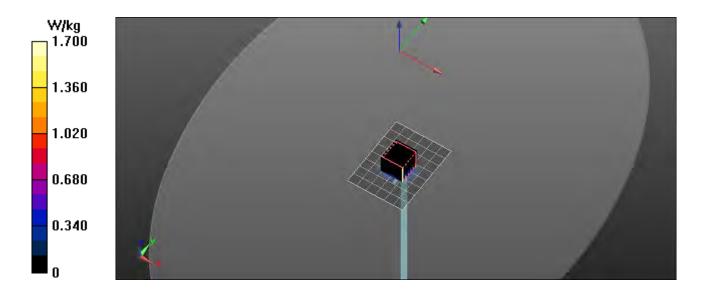



Plot 8

DUT: Dipole 2450 MHz D2450V2; Type: D2450V2; Serial: D2450V2 - SN: 881

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium: HSL2450; Medium parameters used: f = 2450 MHz; σ = 1.81 S/m; ϵ_r = 38.34; ρ = 1000 kg/m³ Phantom section: Flat Section


Test Date: Date: 7/15/2022; Ambient Temp: 23 °C; Tissue Temp: 21 °C Probe: EX3DV4 – SN3662; ConvF(7.28, 7.28, 7.28); Calibrated: 2/16/2022; Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1416; Calibrated: 4/12/2022 Phantom: ELI v5.0; Type: QDOVA002AA; Serial: 2037 Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Procedure Notes:

2450 MHz Head/Verification/Area Scan (61x101x1): Interpolated grid: dx=1.200 mm, dy=1.200 mm Maximum value of SAR (interpolated) = 8.22 W/kg

2450 MHz Head/Verification/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 56.025 V/m; Power Drift = -0.03 dB Peak SAR (extrapolated) = 11.05 W/kg Pin= 100 mW SAR(1 g) = 5.46 W/kg; SAR(10 g) = 2.52 W/kg

Maximum value of SAR (measured) = 8.96 W/kg

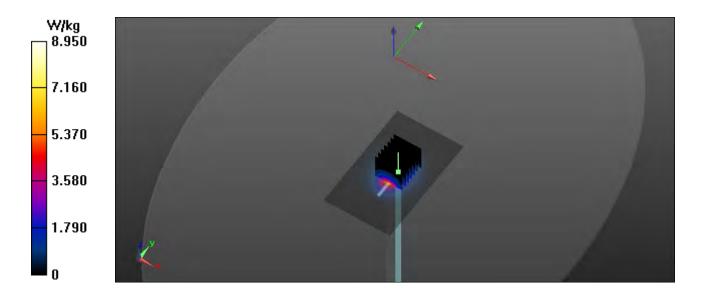



Appendix B – SAR Test Data Plots



Plot 1

DUT: Samsung S21; Type: Cell Phone; Serial: Test

Communication System: LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK); Frequency: 3625 MHz; Duty Cycle: 1:8.33681 Medium: HSL3-6GHz; Medium parameters used (interpolated): f = 3625 MHz; σ = 3.015 S/m; ϵ_r = 36.715; ρ = 1000 kg/m³ Phantom section: Right Section

Test Date: Date: 7/14/2022; Ambient Temp: 23 °C; Tissue Temp: 21 °C

Probe: EX3DV4 - SN3662; ConvF(6.53, 6.53, 6.53); Calibrated: 2/16/2022 Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1416; Calibrated: 4/12/2022 Phantom: SAM 1; Type: SAM Twin Phantom; Serial: 1152 Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Procedure Notes:


3600 Head/LTE B48 Samsung S21 Right Touch 1 RB 49 Offset Baseline Mid/Area Scan (10x16x1): Measurement grid: dx=10mm, dy=10mm

Info: Interpolated medium parameters used for SAR evaluation. Maximum value of SAR (measured) = 1.03 W/kg

3600 Head/LTE B48 Samsung S21 Right Touch 1 RB 49 Offset Baseline Mid/Zoom Scan (9x9x7)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=2mmReference Value = 4.590 V/m; Power Drift = 0.01 dB Peak SAR (extrapolated) = 1.67 W/kg SAR(1 g) = 0.502 W/kg; SAR(10 g) = 0.397 W/kg

Info: Interpolated medium parameters used for SAR evaluation. Maximum value of SAR (measured) = 1.14 W/kg

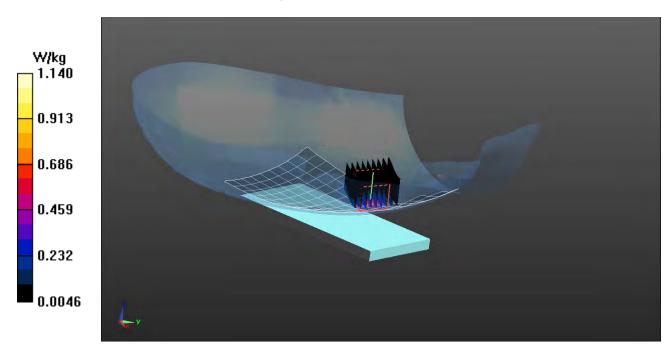



Plot 2

DUT: Samsung S21; Type: Cell Phone; Serial: Test

Communication System: LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK); Frequency: 3625 MHz; Duty Cycle: 1:8.33681 Medium: HSL3-6GHz; Medium parameters used (interpolated): f = 3625 MHz; σ = 3.015 S/m; ϵ_r = 36.715; ρ = 1000 kg/m³ Phantom section: Right Section

Test Date: Date: 7/14/2022; Ambient Temp: 23 °C; Tissue Temp: 21 °C

Probe: EX3DV4 - SN3662; ConvF(6.53, 6.53, 6.53); Calibrated: 2/16/2022 Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1416; Calibrated: 4/12/2022 Phantom: SAM 1; Type: SAM Twin Phantom; Serial: 1152 Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Procedure Notes:


3600 Head/LTE B48 Samsung S21 Right Touch 1 RB 49 Offset With Case Mid/Area Scan (10x16x1): Measurement grid: dx=10mm, dy=10mm

Info: Interpolated medium parameters used for SAR evaluation. Maximum value of SAR (measured) = 0.464 W/kg

3600 Head/LTE B48 Samsung S21 Right Touch 1 RB 49 Offset With Case Mid/Zoom Scan (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm

Reference Value = 1.358 V/m; Power Drift = 0.04 dB Peak SAR (extrapolated) = 0.510 W/kg SAR(1 g) = 0.421 W/kg; SAR(10 g) = 0.298 W/kg

Info: Interpolated medium parameters used for SAR evaluation. Maximum value of SAR (measured) = 0.460 W/kg

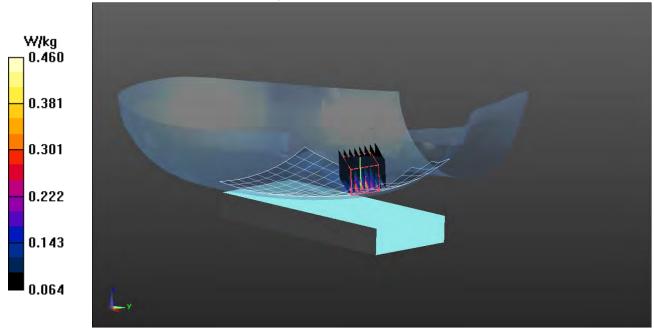



Plot 3

DUT: Samsung S21; Type: Cell Phone; Serial: Test

Communication System: UMTS (WCDMA); Frequency: 1880 MHz; Duty Cycle: 1:1 Medium: HSL1900; Medium parameters used: f = 1880 MHz; σ = 1.39 S/m; ϵ_r = 39.91; ρ = 1000 kg/m³ Phantom section: Flat Section

Test Date: Date: 7/11/2022; Ambient Temp: 23 °C; Tissue Temp: 21 °C


Probe: EX3DV4 - SN3662; ConvF(7.66, 7.66, 7.66); Calibrated: 2/16/2022 Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1416; Calibrated: 4/12/2022 Phantom: ELI v5.0; Type: QDOVA002AA; Serial: 2037 Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Procedure Notes:

1900 Body/WCDMA Samsung S21 Back Baseline Mid/Area Scan (7x13x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 1.30 W/kg

1900 Body/WCDMA Samsung S21 Back Baseline Mid/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 11.26 V/m; Power Drift = 0.02 dB Peak SAR (extrapolated) = 1.73 W/kg SAR(1 g) = 0.959 W/kg; SAR(10 g) = 0.423 W/kg Maximum value of SAR (measured) = 1.39 W/kg

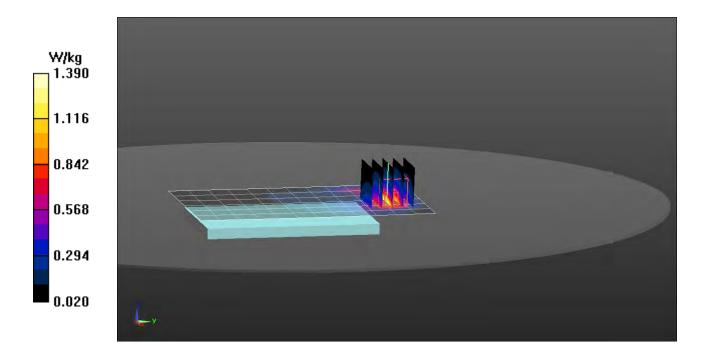



Plot 4

DUT: Samsung S21; Type: Cell Phone; Serial: Test

Communication System: UMTS (WCDMA); Frequency: 1880 MHz; Duty Cycle: 1:1 Medium: HSL1900; Medium parameters used: f = 1880 MHz; σ = 1.39 S/m; ϵ_r = 39.91; ρ = 1000 kg/m³ Phantom section: Flat Section

Test Date: Date: 7/11/2022; Ambient Temp: 23 °C; Tissue Temp: 21 °C


Probe: EX3DV4 - SN3662; ConvF(7.66, 7.66, 7.66); Calibrated: 2/16/2022 Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1416; Calibrated: 4/12/2022 Phantom: ELI v5.0; Type: QDOVA002AA; Serial: 2037 Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Procedure Notes:

1900 Body/WCDMA Samsung S21 Back With Case Mid/Area Scan (7x13x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 0.781 W/kg

1900 Body/WCDMA Samsung S21 Back With Case Mid/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 7.755 V/m; Power Drift = -0.01 dB Peak SAR (extrapolated) = 1.05 W/kg SAR(1 g) = 0.661 W/kg; SAR(10 g) = 0.397 W/kg Maximum value of SAR (measured) = 0.866 W/kg

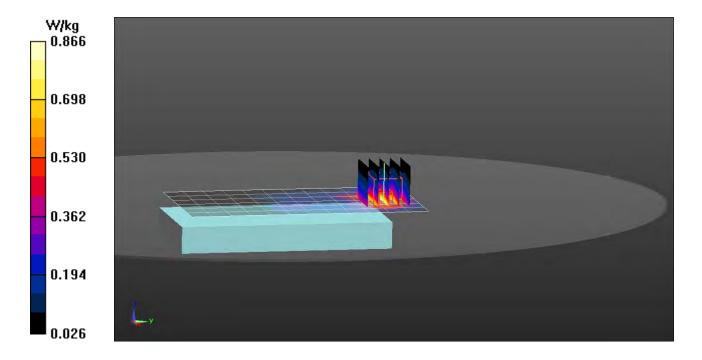



Plot 5

DUT: Samsung S21; Type: Cell Phone; Serial: Test

Communication System: WiFi 802.11b (DSSS, 11 Mbps); Frequency: 2437 MHz; Duty Cycle: 1:1 Medium: HSL2450; Medium parameters used (interpolated): f = 2437 MHz; σ = 1.794 S/m; ϵ_r = 38.393; ρ = 1000 kg/m³ Phantom section: Flat Section

Test Date: Date: 7/16/2022; Ambient Temp: 23 °C; Tissue Temp: 21 °C

Probe: EX3DV4 - SN3662; ConvF(7.28, 7.28, 7.28); Calibrated: 2/16/2022 Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1416; Calibrated: 4/12/2022 Phantom: SAM 1; Type: SAM Twin Phantom; Serial: 1152 Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Procedure Notes:


Head M0007/Samsung S21 Left Touch Mid/Area Scan (7x16x1): Measurement grid: dx=10mm, dy=10mm

Info: Interpolated medium parameters used for SAR evaluation. Maximum value of SAR (measured) = 0.232 W/kg

Head M0007/Samsung S21 Left Touch Mid/Zoom Scan (8x8x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 1.550 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 0.292 W/kg SAR(1 g) = 0.164 W/kg; SAR(10 g) = 0.090 W/kg

Info: Interpolated medium parameters used for SAR evaluation. Maximum value of SAR (measured) = 0.224 W/kg

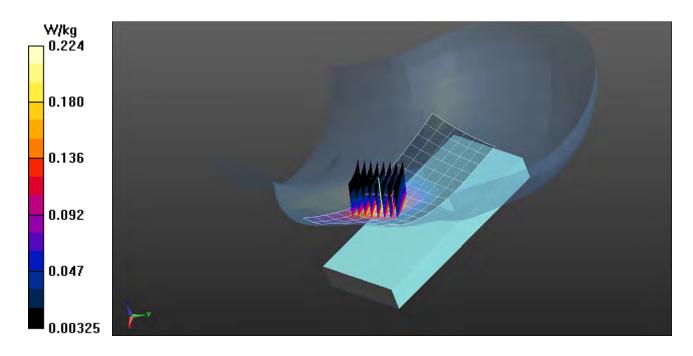



Plot 6

DUT: Samsung S21; Type: Cell Phone; Serial: Test

Communication System: WiFi 802.11b (DSSS, 11 Mbps); Frequency: 2437 MHz; Duty Cycle: 1:1 Medium: HSL2450; Medium parameters used (interpolated): f = 2437 MHz; σ = 1.794 S/m; ϵ_r = 38.393; ρ = 1000 kg/m³ Phantom section: Flat Section

Test Date: Date: 7/16/2022; Ambient Temp: 23 °C; Tissue Temp: 21 °C

Probe: EX3DV4 - SN3662; ConvF(7.28, 7.28, 7.28); Calibrated: 2/16/2022 Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1416; Calibrated: 4/12/2022 Phantom: ELI v5.0; Type: QDOVA002AA; Serial: 2037 Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)


Procedure Notes:

Body M0007/iPhone 13 Right Mid/Area Scan (10x17x1): Measurement grid: dx=10mm, dy=10mm

Info: Interpolated medium parameters used for SAR evaluation. Maximum value of SAR (measured) = 0.177 W/kg

Body M0007/iPhone 13 Right Mid/Zoom Scan (8x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 2.932 V/m; Power Drift = -0.03 dB Peak SAR (extrapolated) = 0.200 W/kg SAR(1 g) = 0.103 W/kg; SAR(10 g) = 0.041 W/kg

Info: Interpolated medium parameters used for SAR evaluation. Maximum value of SAR (measured) = 0.149 W/kg

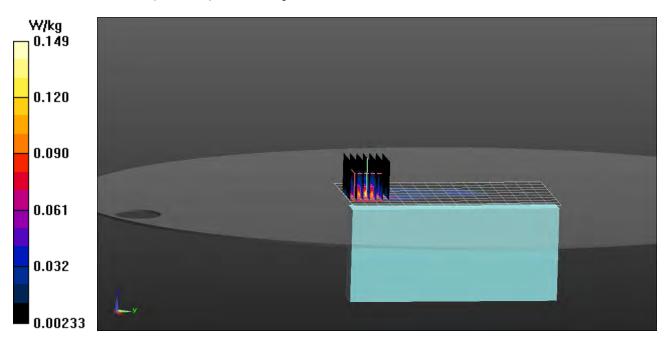



Plot 7

DUT: iPhone 12; Type: Cell Phone; Serial: Test

Communication System: LTE (SC-FDMA, 1 RB, 10 MHz, QPSK); Frequency: 2310 MHz; Duty Cycle: 1:1 Medium: HSL2300; Medium parameters used: f = 2310 MHz; σ = 1.7 S/m; ϵ_r = 38.16; ρ = 1000 kg/m³ Phantom section: Right Section

Test Date: Date: 7/12/2022; Ambient Temp: 23 °C; Tissue Temp: 21 °C


Probe: EX3DV4 - SN3662; ConvF(7.54, 7.54, 7.54); Calibrated: 2/16/2022 Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1416; Calibrated: 4/12/2022 Phantom: SAM 1; Type: SAM Twin Phantom; Serial: 1152 Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Procedure Notes:

2300 Head/LTE B30 iPhone 12 Right Touch 1 RB 24 Offset Baseline Mid/Area Scan (10x16x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (measured) = 0.656 W/kg

2300 Head/LTE B30 iPhone 12 Right Touch 1 RB 24 Offset Baseline Mid/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 1.593 V/m; Power Drift = 0.05 dB Peak SAR (extrapolated) = 0.901 W/kg **SAR(1 g) = 0.455 W/kg; SAR(10 g) = 0.223 W/kg** Maximum value of SAR (measured) = 0.661 W/kg

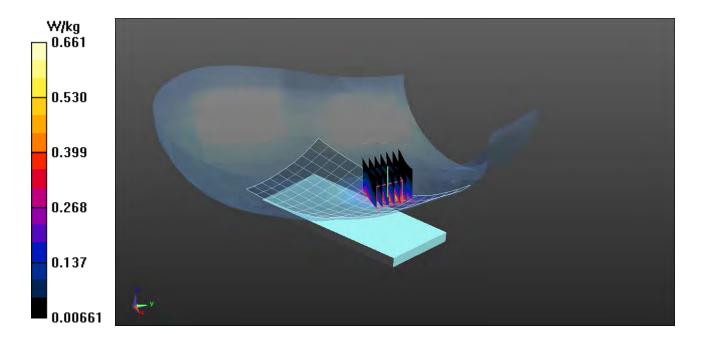



Plot 8

DUT: iPhone 12; Type: Cell Phone; Serial: Test

Communication System: LTE (SC-FDMA, 1 RB, 10 MHz, QPSK); Frequency: 2310 MHz; Duty Cycle: 1:1 Medium: HSL2300; Medium parameters used: f = 2310 MHz; σ = 1.7 S/m; ϵ_r = 38.16; ρ = 1000 kg/m³ Phantom section: Right Section

Test Date: Date: 7/12/2022; Ambient Temp: 23 °C; Tissue Temp: 21 °C


Probe: EX3DV4 - SN3662; ConvF(7.54, 7.54, 7.54); Calibrated: 2/16/2022 Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1416; Calibrated: 4/12/2022 Phantom: SAM 1; Type: SAM Twin Phantom; Serial: 1152 Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Procedure Notes:

2300 Head/LTE B30 iPhone 12 Right Touch 1 RB 24 Offset With Case Mid/Area Scan (10x16x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (measured) = 0.557 W/kg

2300 Head/LTE B30 iPhone 12 Right Touch 1 RB 24 Offset With Case Mid/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 2.715 V/m; Power Drift = 0.01 dB Peak SAR (extrapolated) = 0.748 W/kg SAR(1 g) = 0.385 W/kg; SAR(10 g) = 0.192 W/kg Maximum value of SAR (measured) = 0.561 W/kg

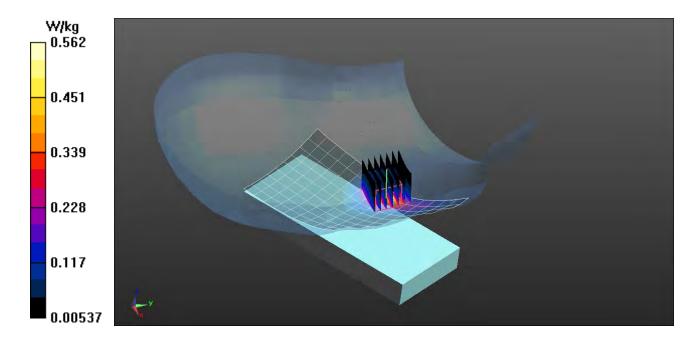



Plot 9

DUT: iPhone 12; Type: Cell Phone; Serial: Test

Communication System: UMTS (WCDMA); Frequency: 1880 MHz; Duty Cycle: 1:1 Medium: HSL1900; Medium parameters used: f = 1880 MHz; σ = 1.39 S/m; ϵ_r = 39.91; ρ = 1000 kg/m³ Phantom section: Flat Section


Test Date: Date: 7/11/2022; Ambient Temp: 23 °C; Tissue Temp: 21 °C

Probe: EX3DV4 - SN3662; ConvF(7.66, 7.66, 7.66); Calibrated: 2/16/2022 Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1416; Calibrated: 4/12/2022 Phantom: ELI v5.0; Type: QDOVA002AA; Serial: 2037 Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Procedure Notes:

1900 Body/WCDMA iPhone 12 Bottom Baseline Mid/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 2.25 W/kg

1900 Body/WCDMA iPhone 12 Bottom Baseline Mid/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 11.64 V/m; Power Drift = 0.02 dB Peak SAR (extrapolated) = 2.64 W/kg SAR(1 g) = 0.941 W/kg; SAR(10 g) = 0.432 W/kg Maximum value of SAR (measured) = 1.77 W/kg

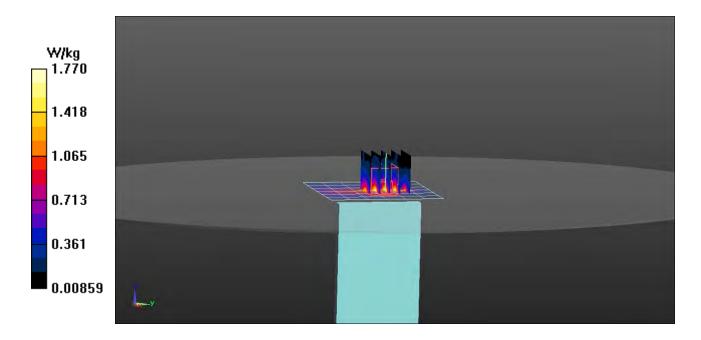



Plot 10

DUT: iPhone 12; Type: Cell Phone; Serial: Test

Communication System: UMTS (WCDMA); Frequency: 1880 MHz; Duty Cycle: 1:1 Medium: HSL1900; Medium parameters used: f = 1880 MHz; σ = 1.39 S/m; ϵ_r = 39.91; ρ = 1000 kg/m³ Phantom section: Flat Section

Test Date: Date: 7/11/2022; Ambient Temp: 23 °C; Tissue Temp: 21 °C


Probe: EX3DV4 - SN3662; ConvF(7.66, 7.66, 7.66); Calibrated: 2/16/2022 Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1416; Calibrated: 4/12/2022 Phantom: ELI v5.0; Type: QDOVA002AA; Serial: 2037 Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Procedure Notes:

1900 Body/WCDMA iPhone 12 Bottom With Case Mid/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 0.821 W/kg

1900 Body/WCDMA iPhone 12 Bottom With Case Mid/Zoom Scan (6x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 2.684 V/m; Power Drift = 0.03 dB Peak SAR (extrapolated) = 1.88 W/kg SAR(1 g) = 0.777 W/kg; SAR(10 g) = 0.330 W/kg Maximum value of SAR (measured) = 0.972 W/kg

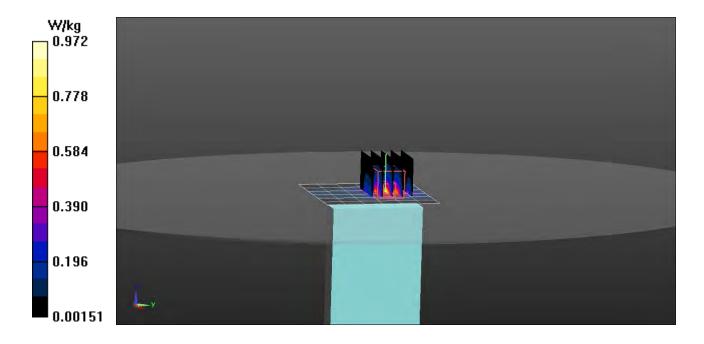



Plot 11

DUT: iPhone 12; Type: Cell Phone; Serial: Test

Communication System: WiFi 802.11b (DSSS, 11 Mbps); Frequency: 2437 MHz; Duty Cycle: 1:1 Medium: HSL2450; Medium parameters used (interpolated): f = 2437 MHz; σ = 1.794 S/m; ϵ_r = 38.393; ρ = 1000 kg/m³ Phantom section: Flat Section

Test Date: Date: 7/15/2022; Ambient Temp: 23 °C; Tissue Temp: 21 °C

Probe: EX3DV4 - SN3662; ConvF(7.28, 7.28, 7.28); Calibrated: 2/16/2022 Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1416; Calibrated: 4/12/2022 Phantom: SAM 1; Type: SAM Twin Phantom; Serial: 1152 Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Procedure Notes:


Head M0008/iPhone 12 Right Touch Mid/Area Scan (10x16x1): Measurement grid: dx=10mm, dy=10mm

Info: Interpolated medium parameters used for SAR evaluation. Maximum value of SAR (measured) = 0.151 W/kg

Head M0008/iPhone 12 Right Touch Mid/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 2.785 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 0.188 W/kg SAR(1 g) = 0.110 W/kg; SAR(10 g) = 0.064 W/kg

Info: Interpolated medium parameters used for SAR evaluation. Maximum value of SAR (measured) = 0.148 W/kg

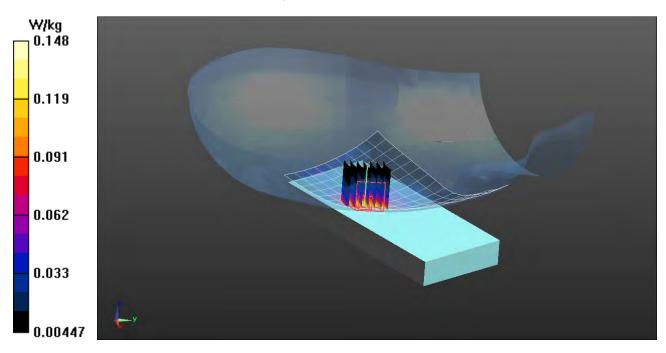



Plot 12

DUT: iPhone 12; Type: Cell Phone; Serial: Test

Communication System: WiFi 802.11b (DSSS, 11 Mbps); Frequency: 2437 MHz; Duty Cycle: 1:1 Medium: HSL2450; Medium parameters used (interpolated): f = 2437 MHz; σ = 1.794 S/m; ϵ_r = 38.393; ρ = 1000 kg/m³ Phantom section: Flat Section


Test Date: Date: 7/15/2022; Ambient Temp: 23 °C; Tissue Temp: 21 °C

Probe: EX3DV4 - SN3662; ConvF(7.28, 7.28, 7.28); Calibrated: 2/16/2022 Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1416; Calibrated: 4/12/2022 Phantom: ELI v5.0; Type: QDOVA002AA; Serial: 2037 Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

Procedure Notes:

Body M0008/iPhone 12 Right Mid/Area Scan (10x16x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (measured) = 0.366 W/kg

Body M0008/iPhone 12 Right Mid/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 2.086 V/m; Power Drift = 0.05 dB Peak SAR (extrapolated) = 0.833 W/kg SAR(1 g) = 0.234 W/kg; SAR(10 g) = 0.073 W/kg Maximum value of SAR (measured) = 0.541 W/kg

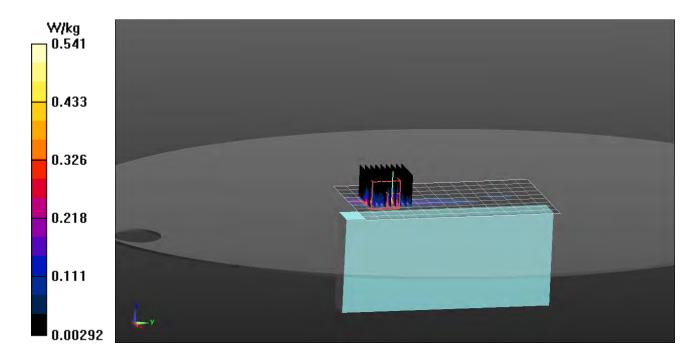



Appendix C – Test Setup Photos



Left Touch





Left Tilt






Right Touch





Right Tilt



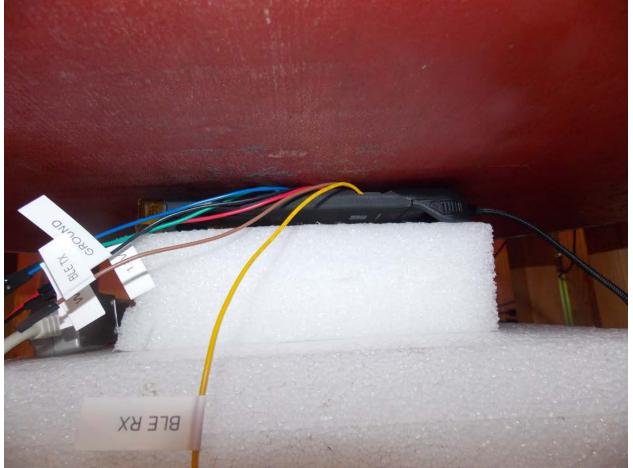

Body Back Configuration 5 mm Gap





Body Front Configuration 5 mm Gap





Body Right Configuration 5 mm Gap






Body Bottom Configuration 5 mm Gap





Front of Case (M0007)



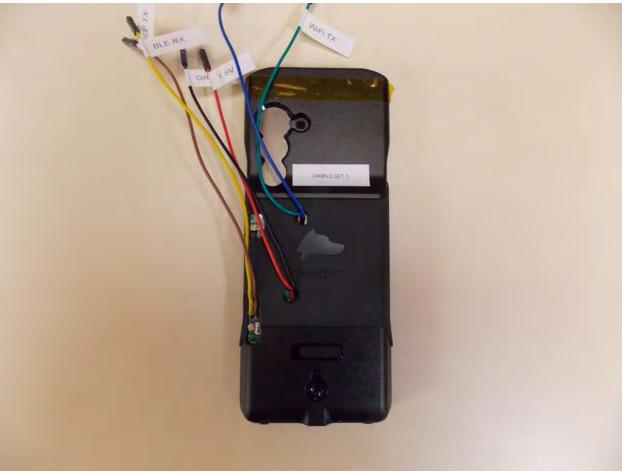

Back of Case (M0007)





Front of Device (M0008)



Report Number: SAR.20220706




Back of Device (M0008)



Appendix D – Probe Calibration Data Sheets

Calibration Laboratory of Schmid & Partner **Engineering AG** Zeughausstrasse 43, 8004 Zurich, Switzerland





- Service suisse d'étalonnage
- С Servizio svizzero di taratura
- S Swiss Calibration Service

S

Accreditation No.: SCS 0108

Certificate No: EX3-3662_Feb22

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client **RF Exposure Lab**

CALIBRATION	CERTIFICATE
Object	EX3DV4 - SN:3662
Calibration procedure(s)	QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v6, QA CAL-23.v5, QA CAL-25.v7 Calibration procedure for dosimetric E-field probes
Calibration date:	February 16, 2022
This calibration certificate doc	uments the traceability to national standards, which realize the physical units of measurements (SI).

The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03291/03292)	Apr-22
Power sensor NRP-Z91	SN: 103244	09-Apr-21 (No. 217-03291)	Apr-22
Power sensor NRP-Z91	SN: 103245	09-Apr-21 (No. 217-03292)	Apr-22
Reference 20 dB Attenuator	SN: CC2552 (20x)	09-Apr-21 (No. 217-03343)	Apr-22
DAE4	SN: 660	13-Oct-21 (No. DAE4-660_Oct21)	Oct-22
Reference Probe ES3DV2	SN: 3013	27-Dec-21 (No. ES3-3013_Dec21)	Dec-22
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (in house check Jun-20)	In house check: Jun-22
Power sensor E4412A	SN: MY41498087	06-Apr-16 (in house check Jun-20)	In house check: Jun-22
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-20)	In house check: Jun-22
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-20)	In house check: Jun-22
Network Analyzer E8358A	SN: US41080477	31-Mar-14 (in house check Oct-20)	In house check: Oct-22

	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	et le
Approved by:	Sved Kildin	Deputy Manager	S. 6
			Issued: February 18, 2022
This calibration certificate	e shall not be reproduced except in	full without written approval of the labor	oratory.

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst

S Service suisse d'étalonnage С

Servizio svizzero di taratura S

Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Accreditation No.: SCS 0108

Glossary:

TSL	tissue simulating liquid
NORMx,y,z	sensitivity in free space
ConvF	sensitivity in TSL / NORMx,y,z
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization 9	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices -Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- *NORMx*, *y*,*z*: Assessed for E-field polarization $\vartheta = 0$ (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E2-field uncertainty inside TSL (see below ConvF).
- NORM(f)x, v, z = NORMx, v, z * frequency response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx, y, z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \le 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx, y, z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (μV/(V/m) ²) ^A	0.42	0.49	0.48	± 10.1 %
DCP (mV) ^B	99.8	99.6	98.2	

Calibration Results for Modulation Response

UID	Communication System Name		A dB	B dB√μV	С	D dB	VR mV	Max dev.	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	147.3	±2.7 %	± 4.7 %
		Y	0.0	0.0	1.0		161.3		
		Z	0.0	0.0	1.0		168.0		

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	-94.7
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

Note: Measurement distance from surface can be increased to 3-4 mm for an Area Scan job.

f (MHz) ^c	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unc (k=2)
150	52.3	0.76	11.58	11.58	11.58	0.00	1.00	± 13.3 %
220	49.0	0.81	11.43	11.43	11.43	0.00	1.00	± 13.3 %
300	45.3	0.87	11.15	11.15	11.15	0.09	1.00	± 13.3 %
450	43.5	0.87	10.72	10.72	10.72	0.16	1.30	± 13.3 %
750	41.9	0.89	9.23	9.23	9.23	0.52	0.80	± 12.0 %
900	41.5	0.97	8.76	8.76	8.76	0.44	0.80	± 12.0 %
1450	40.5	1.20	8.18	8.18	8.18	0.37	0.80	± 12.0 %
1640	40.2	1.31	8.03	8.03	8.03	0.35	0.86	± 12.0 %
1750	40.1	1.37	7.87	7.87	7.87	0.32	0.86	± 12.0 %
1900	40.0	1.40	7.66	7.66	7.66	0.27	0.86	± 12.0 %
2300	39.5	1.67	7.54	7.54	7.54	0.34	0.90	± 12.0 %
2450	39.2	1.80	7.28	7.28	7.28	0.38	0.90	± 12.0 %
2600	39.0	1.96	7.10	7.10	7.10	0.38	0.90	± 12.0 %
3500	37.9	2.91	6.73	6.73	6.73	0.35	1.30	± 13.1 %
3700	37.7	3.12	6.53	6.53	6.53	0.35	1.30	± 13.1 %
5250	35.9	4.71	4.95	4.95	4.95	0.40	1.80	± 13.1 %
5600	35.5	5.07	4.66	4.66	4.66	0.40	1.80	± 13.1 %
5750	35.4	5.22	4.80	4.80	4.80	0.40	1.80	± 13.1 %

Calibration Parameter Determined in Head Tissue Simulating Media

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4-9 MHz, and ConvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters. ^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


[f (MHz) ^c	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unc (k=2)
	6500	34.5	6.07	5.50	5.50	5.50	0.20	2.00	± 18.6 %

Calibration Parameter Determined in Head Tissue Simulating Media

^c Frequency validity above 6GHz is ± 700 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.


^F At frequencies 6-10 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters. ^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than \pm 1% for frequencies below 3 GHz; below \pm 2% for frequencies between 3-6 GHz; and below \pm 4% for frequencies between 6-10 GHz at any distance larger than half the probe tip diameter from the boundary.

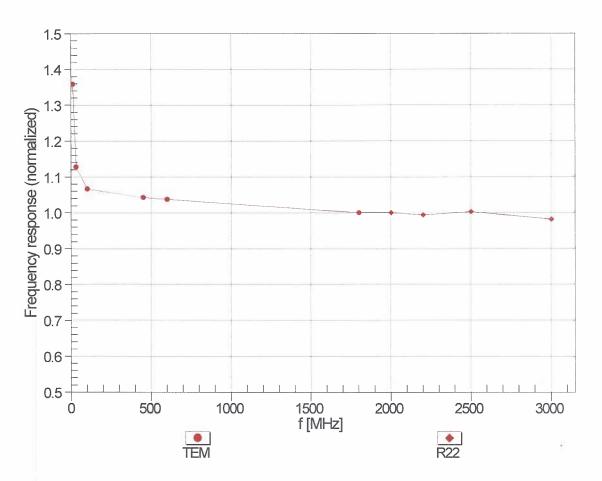


Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

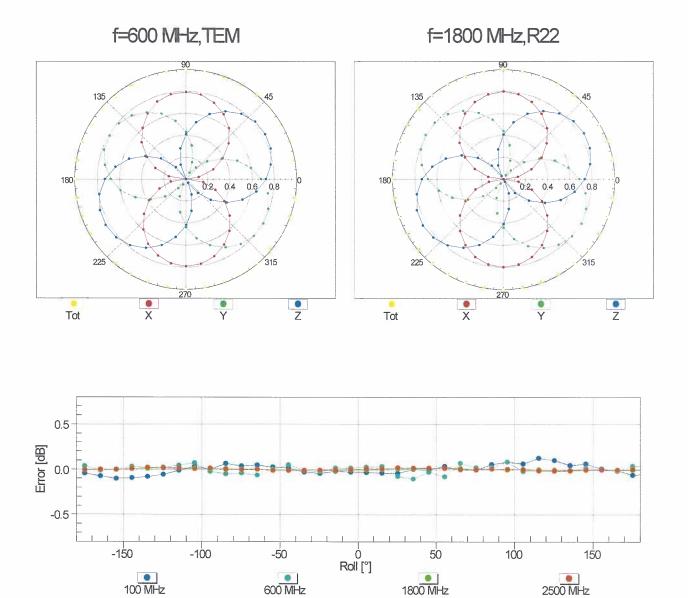


Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

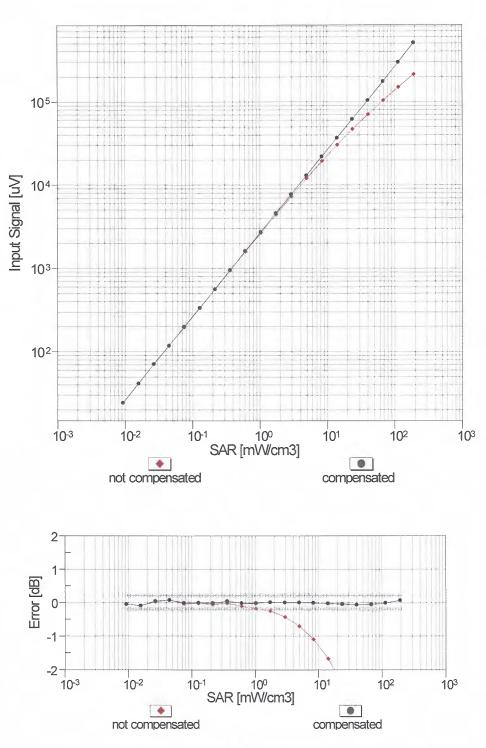

Dynamic Range f(SAR_{head}) (TEM cell , f_{eval}= 1900 MHz)

Uncertainty of Linearity Assessment: ± 0.6% (k=2)

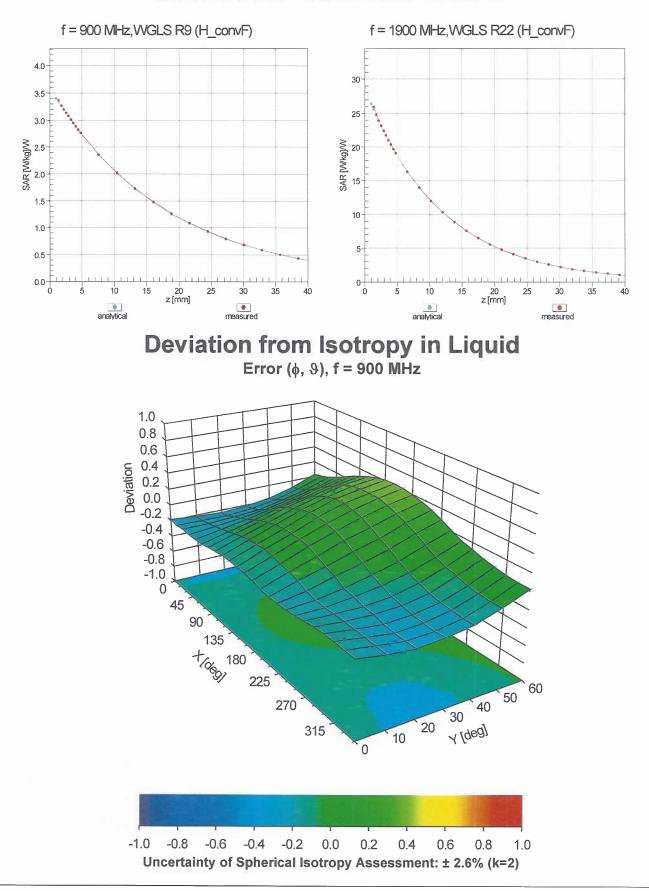

Conversion Factor Assessment



Appendix E – Dipole Calibration Data Sheets

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst Service suisse d'étalonnage

- C Servizio svizzero di taratura
- S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client RF Exposure Lab

Certificate No: D750V3-1053_Jun21

	RATI			

Object	D750V3 - SN:1053					
Calibration procedure(s)	QA CAL-05.v11 Calibration Procedure for SAR Validation Sources between 0.7-3 GHz					
Calibration date:	June 04, 2021					
The measurements and the uncerta	ainties with confidence pro	nal standards, which realize the physical units obbability are given on the following pages and a facility: environment temperature $(22 \pm 3)^{\circ}$ C and	re part of the certificate.			
Calibration Equipment used (M&TE	critical for calibration)					
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration			
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03291/03292)	Apr-22			
Power sensor NRP-Z91	SN: 103244	09-Apr-21 (No. 217-03291)	Apr-22			
Power sensor NRP-Z91	SN: 103245	09-Apr-21 (No. 217-03292)	Apr-22			
Reference 20 dB Attenuator	SN: BH9394 (20k)	09-Apr-21 (No. 217-03343)	Apr-22			
Type-N mismatch combination	SN: 310982 / 06327	09-Apr-21 (No. 217-03344)	Apr-22			
Reference Probe EX3DV4	SN: 7349	28-Dec-20 (No. EX3-7349_Dec20)	Dec-21			
DAE4	SN: 601	02-Nov-20 (No. DAE4-601_Nov20)	Nov-21			
Secondary Standards	ID #	Check Date (in house)	Scheduled Check			
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-20)	In house check: Oct-22			
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-20)	In house check: Oct-22			
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-20)	In house check: Oct-22			
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-20)	In house check: Oct-22			
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-20)	In house check: Oct-21			
	Name	Function	Signature			
Calibrated by:	Michael Weber	Laboratory Technician	11/11/1~			
			M.NEX			
Approved by:	Katja Pokovic	Technical Manager	M.Mess Le 45			
			Issued: June 8, 2021			

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst

- S Service suisse d'étalonnage
- С Servizio svizzero di taratura
- S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole • positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. • No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power. •
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the • nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	750 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.9	0.89 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	42.7 ± 6 %	0.91 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.17 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	8.57 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.41 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	5.58 W/kg ± 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	56.5 Ω + 0.1 jΩ
Return Loss	- 24.3 dB

General Antenna Parameters and Design

	Electrical Delay (one direction)	1.035 ns	
--	----------------------------------	----------	--

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

|--|

Extended Calibration

Usage of SAR dipoles calibrated less than 3 years ago but more than 1 year ago were confirmed in maintaining return loss (<-20 dB, within 20% of prior calibration) and impedance (within 5 ohm from prior calibration) requirements per extended calibrations in KDB Publication 865664 D01 v01r04.

		D750V3	SN: 1053 -	Head		
Date of Measurement	Return Loss (dB)	Δ%	Impedance Real (Ω)	ΔΩ	Impedance Imaginary (jΩ)	ΔΩ
6/4/2021	-24.3		56.5		0.1	
6/4/2022	-26.2	7.8	57.9	1.4	0.3	0.2

DASY5 Validation Report for Head TSL

Date: 04.06.2021

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN:1053


Communication System: UID 0 - CW; Frequency: 750 MHz Medium parameters used: f = 750 MHz; σ = 0.91 S/m; ϵ_r = 42.7; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:


- Probe: EX3DV4 SN7349; ConvF(10.11, 10.11, 10.11) @ 750 MHz; Calibrated: 28.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.11.2020
- Phantom: Flat Phantom 4.9 (front); Type: QD 00L P49 AA; Serial: 1001
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 59.74 V/m; Power Drift = 0.01 dB Peak SAR (extrapolated) = 3.30 W/kg **SAR(1 g) = 2.17 W/kg; SAR(10 g) = 1.41 W/kg** Smallest distance from peaks to all points 3 dB below: Larger than measurement grid (> 30mm) Ratio of SAR at M2 to SAR at M1 = 65.5% Maximum value of SAR (measured) = 2.93 W/kg

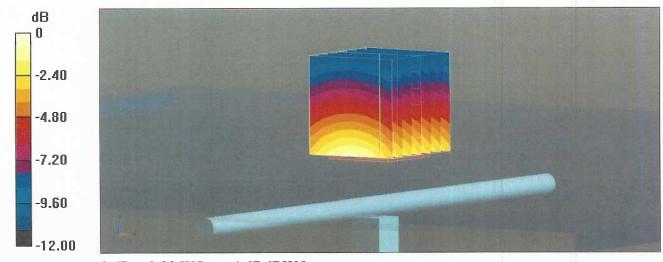

0 dB = 2.93 W/kg = 4.67 dBW/kg

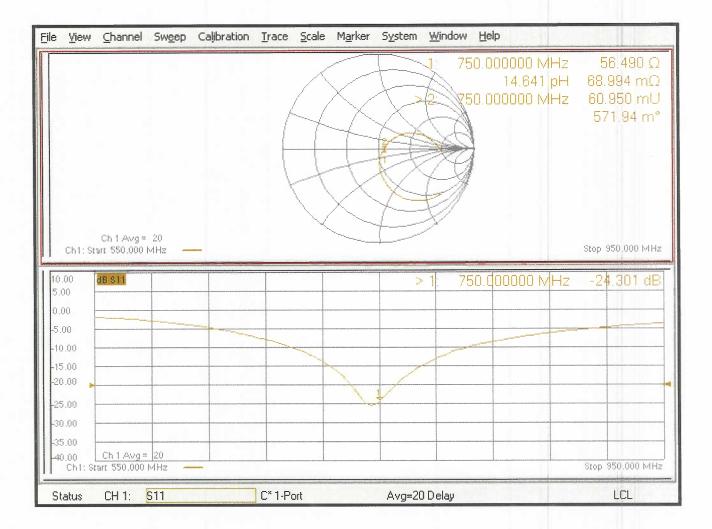

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst Service suisse d'étalonnage

C Servizio svizzero di taratura

S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Certificate No: D900V2-1d128_Jun21

CALIBRATION CERTIFICATE

RF Exposure Lab

Client

Object	D900V2 - SN:1d1	28	
Calibration procedure(s)	QA CAL-05.v11 Calibration Proce	dure for SAR Validation Sources b	etween 0.7-3 GHz
Calibration date:	June 04, 2021		and the second sec
		onal standards, which realize the physical units robability are given on the following pages and a	
All calibrations have been conducte	ed in the closed laborator	y facility: environment temperature (22 \pm 3)°C a	and humidity < 70%.
Calibration Equipment used (M&TE	critical for calibration)		
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03291/03292)	Apr-22
Power sensor NRP-Z91	SN: 103244	09-Apr-21 (No. 217-03291)	Apr-22
Power sensor NRP-Z91	SN: 103245	09-Apr-21 (No. 217-03292)	Apr-22
Reference 20 dB Attenuator	SN: BH9394 (20k)	09-Apr-21 (No. 217-03343)	Apr-22
Type-N mismatch combination	SN: 310982 / 06327	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe EX3DV4	SN: 7349	28-Dec-20 (No. EX3-7349_Dec20)	Dec-21
DAE4	SN: 601	02-Nov-20 (No. DAE4-601_Nov20)	Nov-21
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-20)	In house check: Oct-22
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-20)	In house check: Oct-21
	Name	Function	Signature
Calibrated by:	Michael Weber	Laboratory Technician	M. Heles
Approved by:	Katja Pokovic	Technical Manager	Jelly-
	ha ann an tha an the	full without written approval of the laboratory.	Issued: June 8, 2021

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst

S Service suisse d'étalonnage

С Servizio svizzero di taratura

S **Swiss Calibration Service**

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. • No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	900 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.97 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	42.3 ± 6 %	0.96 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.76 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	11.2 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.77 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	7.14 W/kg ± 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	51.0 Ω - 0.6 jΩ
Return Loss	- 38.5 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.412 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG

Extended Calibration

Usage of SAR dipoles calibrated less than 3 years ago but more than 1 year ago were confirmed in maintaining return loss (<-20 dB, within 20% of prior calibration) and impedance (within 5 ohm from prior calibration) requirements per extended calibrations in KDB Publication 865664 D01 v01r04.

D900V2 SN: 1d128 - Head						
Date of MeasurementReturn Loss (dB)Δ%Impedance Real (Ω)ΔΩImpedance Imaginary (jΩ)ΔΩ					ΔΩ	
6/4/2021	-38.5		51.0		-0.6	
6/4/2022	-37.2	-3.4	52.3	1.3	-0.8	-0.2

DASY5 Validation Report for Head TSL

Date: 04.06.2021

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 900 MHz; Type: D900V2; Serial: D900V2 - SN:1d128


Communication System: UID 0 - CW; Frequency: 900 MHz Medium parameters used: f = 900 MHz; $\sigma = 0.96$ S/m; $\epsilon_r = 42.3$; $\rho = 1000$ kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN7349; ConvF(9.62, 9.62, 9.62) @ 900 MHz; Calibrated: 28.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.11.2020
- Phantom: Flat Phantom 4.9 (front); Type: QD 00L P49 AA; Serial: 1001
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)


Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mmReference Value = 65.79 V/m; Power Drift = 0.03 dB Peak SAR (extrapolated) = 4.23 W/kg **SAR(1 g) = 2.76 W/kg; SAR(10 g) = 1.77 W/kg** Smallest distance from peaks to all points 3 dB below = 16 mm Ratio of SAR at M2 to SAR at M1 = 65% Maximum value of SAR (measured) = 3.74 W/kg

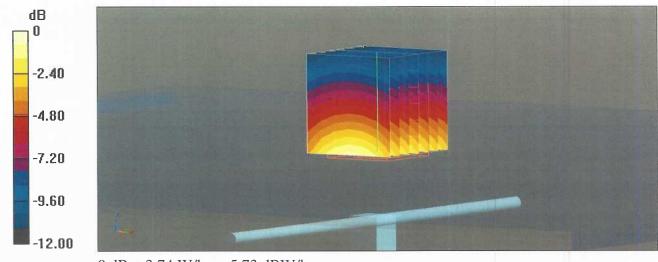

0 dB = 3.74 W/kg = 5.73 dBW/kg

Impedance Measurement Plot for Head TSL

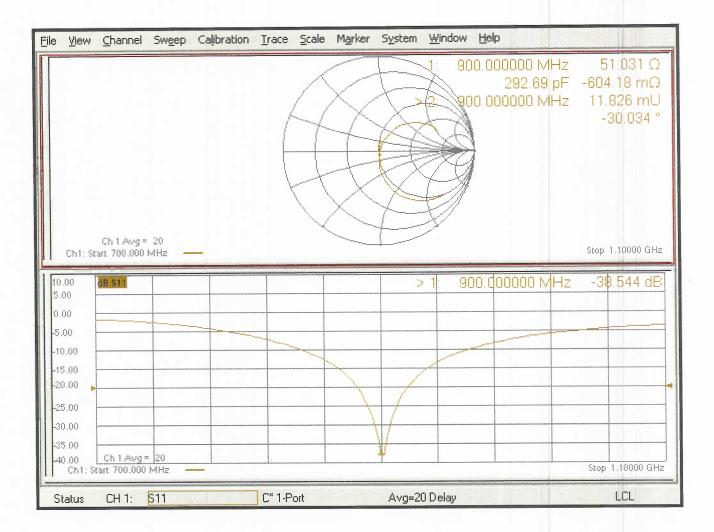

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Client





S Schweizerischer Kalibrierdienst

- C Service suisse d'étalonnage
 - Servizio svizzero di taratura
- S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Accreditation No.: SCS 0108

Certificate No: D1750V2-1061_Jun21

CALIBRATION CERTIFICATE

RF Exposure Lab

Object	D1750V2 - SN:1061
Calibration procedure(s)	QA CAL-05.v11 Calibration Procedure for SAR Validation Sources between 0.7-3 GHz
Calibration date:	June 03, 2021

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03291/03292)	Apr-22
Power sensor NRP-Z91	SN: 103244	09-Apr-21 (No. 217-03291)	Apr-22
Power sensor NRP-Z91	SN: 103245	09-Apr-21 (No. 217-03292)	Apr-22
Reference 20 dB Attenuator	SN: BH9394 (20k)	09-Apr-21 (No. 217-03343)	Apr-22
Type-N mismatch combination	SN: 310982 / 06327	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe EX3DV4	SN: 7349	28-Dec-20 (No. EX3-7349_Dec20)	Dec-21
DAE4	SN: 601	02-Nov-20 (No. DAE4-601_Nov20)	Nov-21
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-20)	In house check: Oct-22
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-20)	In house check: Oct-21
	Name	Function	Signature
Calibrated by:	Jeffrey Katzman	Laboratory Technician	1. totas
Approved by:	Katja Pokovic	Technical Manager	BBC
			Issued: June 8, 2021
This calibration certificate shall not	be reproduced except in	full without written approval of the laboratory	<i>.</i>

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst

S Service suisse d'étalonnage С

Servizio svizzero di taratura

S **Swiss Calibration Service**

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1750 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.1	1.37 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.7 ± 6 %	1.37 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.38 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	37.7 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	4.93 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	19.8 W/kg ± 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	49.4 Ω + 0.0 jΩ
Return Loss	- 44.5 dB

General Antenna Parameters and Design

Electrical Delay (one direction) 1.221 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

	Manufactured by		SPEAG
--	-----------------	--	-------

Extended Calibration

Usage of SAR dipoles calibrated less than 3 years ago but more than 1 year ago were confirmed in maintaining return loss (<-20 dB, within 20% of prior calibration) and impedance (within 5 ohm from prior calibration) requirements per extended calibrations in KDB Publication 865664 D01 v01r04.

D1750V2 SN: 1061 - Head						
Date of Measurement	Return Loss (dB)	Δ%	Impedance Real (Ω)	ΔΩ	Impedance Imaginary (jΩ)	ΔΩ
6/3/2021	-44.5		49.4		0.0	
6/4/2022	-42.3	-4.9	47.9	-1.5	-0.2	-0.2

DASY5 Validation Report for Head TSL

Date: 03.06.2021

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: D1750V2 - SN:1061


Communication System: UID 0 - CW; Frequency: 1750 MHz Medium parameters used: f = 1750 MHz; σ = 1.37 S/m; ϵ_r = 40.7; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:


- Probe: EX3DV4 SN7349; ConvF(8.67, 8.67, 8.67) @ 1750 MHz; Calibrated: 28.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.11.2020
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mmReference Value = 107.4 V/m; Power Drift = 0.08 dB Peak SAR (extrapolated) = 17.5 W/kg **SAR(1 g) = 9.38 W/kg; SAR(10 g) = 4.93 W/kg** Smallest distance from peaks to all points 3 dB below = 9.1 mm Ratio of SAR at M2 to SAR at M1 = 54% Maximum value of SAR (measured) = 14.6 W/kg

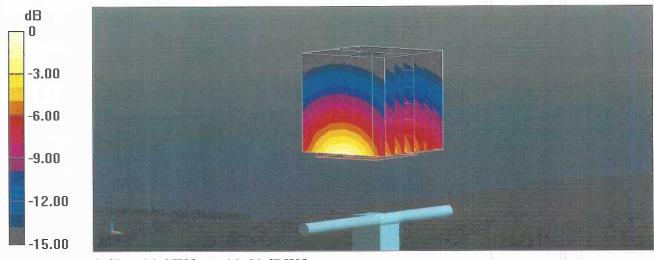

0 dB = 14.6 W/kg = 11.64 dBW/kg

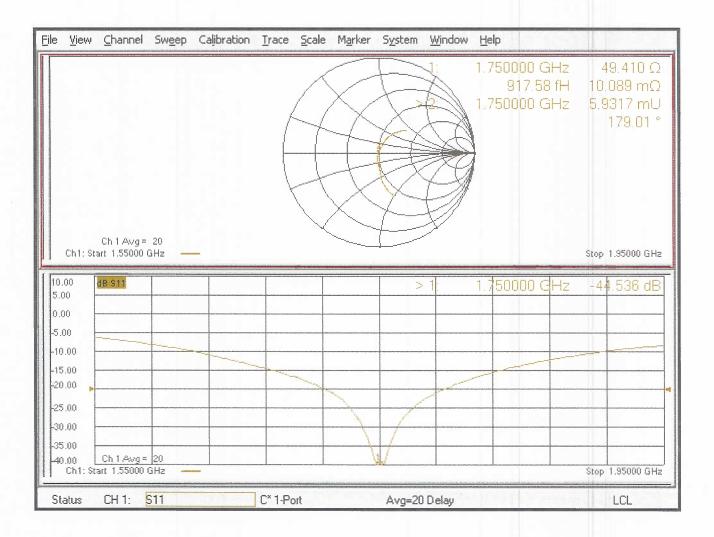

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst

- Service suisse d'étalonnage
- C Servizio svizzero di taratura
- S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Accreditation No.: SCS 0108

Client RF Exposure Lab

Certificate No: D1900V2-5d147_Jun21

CALIBRATION CERTIFICATE

Multilateral Agreement for the recognition of calibration certificates

Object	D1900V2 - SN:5d	1147	
Calibration procedure(s)	QA CAL-05.v11 Calibration Proce	dure for SAR Validation Sources	between 0.7-3 GHz
Calibration date:	June 04, 2021		
The measurements and the uncerta	ainties with confidence pr ed in the closed laborator	conal standards, which realize the physical un robability are given on the following pages an y facility: environment temperature (22 \pm 3)°C	d are part of the certificate.
	ł		
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03291/03292)	Apr-22
Power sensor NRP-Z91	SN: 103244	09-Apr-21 (No. 217-03291)	Apr-22
Power sensor NRP-Z91	SN: 103245	09-Apr-21 (No. 217-03292)	Apr-22
Reference 20 dB Attenuator	SN: BH9394 (20k)	09-Apr-21 (No. 217-03343)	Apr-22
Type-N mismatch combination	SN: 310982 / 06327	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe EX3DV4	SN: 7349	28-Dec-20 (No. EX3-7349_Dec20)	Dec-21
DAE4	SN: 601	02-Nov-20 (No. DAE4-601_Nov20)	Nov-21
Secondary Standards	D #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-20)	In house check: Oct-22
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-20)	In house check: Oct-21
	Name	Function	Signature
Calibrated by:	Michael Weber	Laboratory Technician	
Calibrated by.		Laboratory rectinician	MARKET
Approved by:	Katja Pokovic	Technical Manager	All of

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D1900V2-5d147_Jun21

Issued: June 8, 2021

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst

- S Service suisse d'étalonnage
- С Servizio svizzero di taratura
- S **Swiss Calibration Service**

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. • No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power. •
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the • nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

Head TSL parameters The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.9 ± 6 %	1.41 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.1 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	40.4 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.28 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.1 W/kg ± 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.3 Ω + 5.4 jΩ
Return Loss	- 24.2 dB

General Antenna Parameters and Design

Electrical Delay (one direction) 1.192 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG

Extended Calibration

Usage of SAR dipoles calibrated less than 3 years ago but more than 1 year ago were confirmed in maintaining return loss (<-20 dB, within 20% of prior calibration) and impedance (within 5 ohm from prior calibration) requirements per extended calibrations in KDB Publication 865664 D01 v01r04.

D1900V2 SN: 5d147 - Head								
Date of Measurement	Return Loss (dB)	Δ%	Impedance Real (Ω)	ΔΩ	Impedance Imaginary (jΩ)	ΔΩ		
6/4/2021	-24.2		53.3		5.4			
6/4/2022	-25.6	5.8	52.6	-0.7	5.7	0.3		

DASY5 Validation Report for Head TSL

Date: 04.06.2021

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d147


Communication System: UID 0 - CW; Frequency: 1900 MHz Medium parameters used: f = 1900 MHz; σ = 1.41 S/m; ϵ_r = 40.9; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN7349; ConvF(8.43, 8.43, 8.43) @ 1900 MHz; Calibrated: 28.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.11.2020
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)


Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 110.2 V/m; Power Drift = 0.04 dB Peak SAR (extrapolated) = 18.7 W/kg **SAR(1 g) = 10.1 W/kg; SAR(10 g) = 5.28 W/kg** Smallest distance from peaks to all points 3 dB below = 10 mm Ratio of SAR at M2 to SAR at M1 = 54.6% Maximum value of SAR (measured) = 15.6 W/kg

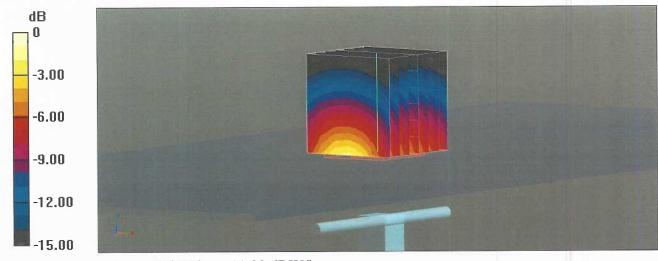

0 dB = 15.6 W/kg = 11.93 dBW/kg

Impedance Measurement Plot for Head TSL

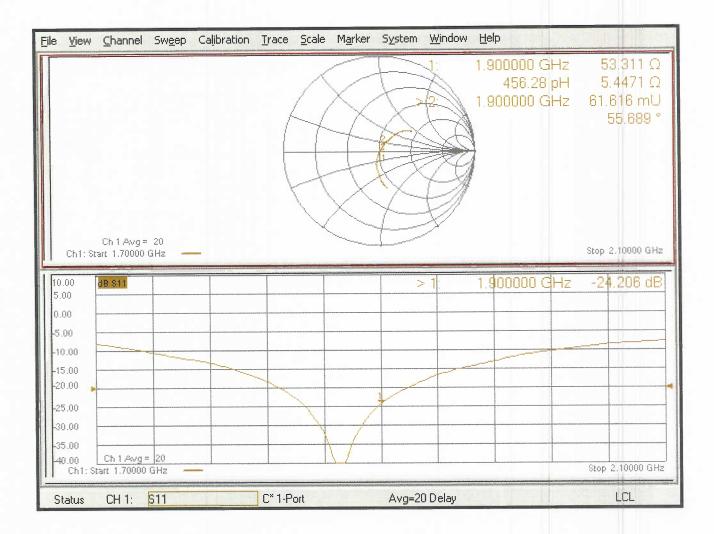

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst S

- Service suisse d'étalonnage
- С Servizio svizzero di taratura
- S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Accreditation No.: SCS 0108

Client RF Exposure La	b	C. C.	Certificate No: D2300V2-1060_Jun21
CALIBRATION C	ERIFICATE	-	
Object	D2300V2 - SN:10	060	
Calibration procedure(s)	QA CAL-05.v11 Calibration Proce	dure for SAR Validation	n Sources between 0.7-3 GHz
Calibration date:	June 03, 2021		
			e physical units of measurements (SI). ving pages and are part of the certificate.
All calibrations have been conducted	ed in the closed laborator	y facility: environment temperatu	ure (22 ± 3) °C and humidity < 70%.
Calibration Equipment used (M&TE	E critical for calibration)		
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03291/03	3292) Apr-22
Power sensor NRP-Z91	SN: 103244	09-Apr-21 (No. 217-03291)	Apr-22
Power sensor NRP-Z91	SN: 103245	09-Apr-21 (No. 217-03292)	Apr-22
Reference 20 dB Attenuator	SN: BH9394 (20k)	09-Apr-21 (No. 217-03343)	Apr-22
Type-N mismatch combination	SN: 310982 / 06327	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe EX3DV4	SN: 7349	28-Dec-20 (No. EX3-7349_De	Dec20) Dec-21
DAE4	SN: 601	02-Nov-20 (No. DAE4-601_N	Nov20) Nov-21
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oc	oct-20) In house check: Oct-22
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oc	oct-20) In house check: Oct-22
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oc	oct-20) In house check: Oct-22
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Od	Oct-20) In house check: Oct-22
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check O	
	Name	Function	Signature
Calibrated by:	Jeffrey Katzman	Laboratory Techr	
Approved by:	Kalja Pokovic	Technical Manag	ger ACGL
This calibration certificate shall not	be reproduced except in	full without written approval of th	Issued: June 8, 2021 the laboratory.

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst

S Service suisse d'étalonnage С

Servizio svizzero di taratura

S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2300 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity	
Nominal Head TSL parameters	22.0 °C	39.5	1.67 mho/m	
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.2 ± 6 %	1.70 mho/m ± 6 %	
Head TSL temperature change during test	< 0.5 °C			

SAR result with Head TSL

SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	12.6 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	49.6 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.00 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.8 W/kg ± 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	48.9 Ω - 4.6 jΩ
Return Loss	- 26.3 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.171 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Extended Calibration

Usage of SAR dipoles calibrated less than 3 years ago but more than 1 year ago were confirmed in maintaining return loss (<-20 dB, within 20% of prior calibration) and impedance (within 5 ohm from prior calibration) requirements per extended calibrations in KDB Publication 865664 D01 v01r04.

D2300V2 SN: 1060 - Head									
Date of Measurement	Return Loss (dB)	Δ%	Impedance (Ω)	ΔΩ	Impedance Imaginary (jΩ)	ΔΩ			
6/3/2021	-26.3		48.9		-4.6				
6/4/2022	-25.6	-2.7	47.3	-1.6	-4.4	0.2			

DASY5 Validation Report for Head TSL

Date: 03.06.2021

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2300 MHz; Type: D2300V2; Serial: D2300V2 - SN:1060


Communication System: UID 0 - CW; Frequency: 2300 MHz Medium parameters used: f = 2300 MHz; $\sigma = 1.7$ S/m; $\epsilon_r = 38.2$; $\rho = 1000$ kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN7349; ConvF(7.98, 7.98, 7.98) @ 2300 MHz; Calibrated: 28.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.11.2020
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)


Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mmReference Value = 117.4 V/m; Power Drift = 0.00 dB Peak SAR (extrapolated) = 23.2 W/kg **SAR(1 g) = 12.6 W/kg; SAR(10 g) = 6 W/kg** Smallest distance from peaks to all points 3 dB below = 9 mm Ratio of SAR at M2 to SAR at M1 = 54.1% Maximum value of SAR (measured) = 19.8 W/kg

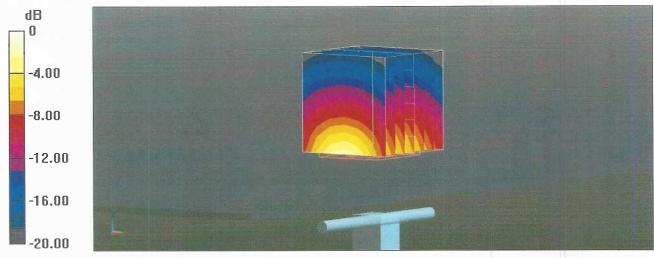

0 dB = 19.8 W/kg = 12.97 dBW/kg

Impedance Measurement Plot for Head TSL

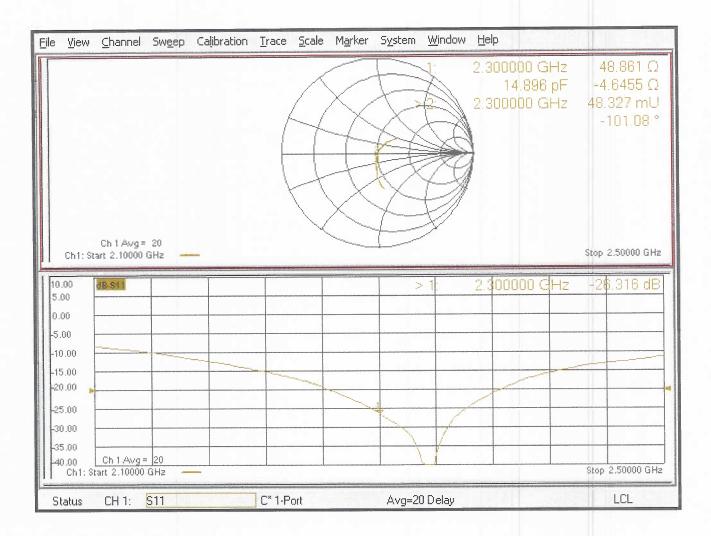

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst

- Service suisse d'étalonnage
- C Servizio svizzero di taratura
- S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

	Certil	icate	No:	<u>)</u> 24	45(W.	2-{	18	1_	Ju	n 2	1		
NORTH NO	-	3709 (L. 1968	NER STOR	-	24-12-10 C		27920	1995-1997.	1925		1000	1997	 1981 - S.	

Client RF Exposure Lab

		-	16. A	and the				
NEW COLOR	0.555555	25570.000	10120360		15% 25% 27%	的现在现在	ne cast	55777777782772

CALIBRATION CERTIEN

OAEIDIGAILEA	VERMINATE
Object	D2450V2 - SN:881
Calibration procedure(s)	QA CAL-05.v11 Calibration Procedure for SAR Validation Sources between 0.7-3 GHz
Calibration date:	June 03, 2021

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03291/03292)	Apr-22
Power sensor NRP-Z91	SN: 103244	09-Apr-21 (No. 217-03291)	Apr-22
Power sensor NRP-Z91	SN: 103245	09-Apr-21 (No. 217-03292)	Apr-22
Reference 20 dB Attenuator	SN: BH9394 (20k)	09-Apr-21 (No. 217-03343)	Apr-22
Type-N mismatch combination	SN: 310982 / 06327	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe EX3DV4	SN: 7349	28-Dec-20 (No. EX3-7349_Dec20)	Dec-21
DAE4	SN: 601	02-Nov-20 (No. DAE4-601_Nov20)	Nov-21
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-20)	In house check: Oct-22
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-20)	In house check: Oct-21
	Name	Function	Signature
Calibrated by:	Jeffrey Katzman	Laboratory Technician	J. https
Approved by:	Katja Pokovic	Technical Manager	all
		25	ants.
			Issued: June 8, 2021
This calibration certificate shall not	be reproduced except in	full without written approval of the laboratory	ý.

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst

S Service suisse d'étalonnage С

Servizio svizzero di taratura

S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Modular Flat Phantom		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	2450 MHz ± 1 MHz		

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	37.7 ± 6 %	1.87 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.9 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	54.1 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.34 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	25.0 W/kg ± 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	54.3 Ω + 4.3 jΩ
Return Loss	- 24.7 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.156 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG

Extended Calibration

Usage of SAR dipoles calibrated less than 3 years ago but more than 1 year ago were confirmed in maintaining return loss (<-20 dB, within 20% of prior calibration) and impedance (within 5 ohm from prior calibration) requirements per extended calibrations in KDB Publication 865664 D01 v01r04.

D2450V2 SN: 829 - Head							
Date of MeasurementReturn Loss (dB)Δ%Impedance Real (Ω)Impedance ΔΩImpedance Imaginary (jΩ)						ΔΩ	
6/3/2021	-24.7	_ ·	54.3		4.3		
6/3/2022 -25.3 2.4 55.2 0.9 4.1 -0.2							

DASY5 Validation Report for Head TSL

Date: 03.06.2021

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:881


Communication System: UID 0 - CW; Frequency: 2450 MHz Medium parameters used: f = 2450 MHz; $\sigma = 1.87$ S/m; $\epsilon_r = 37.7$; $\rho = 1000$ kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN7349; ConvF(7.96, 7.96, 7.96) @ 2450 MHz; Calibrated: 28.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.11.2020
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)


Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mmReference Value = 119.0 V/m; Power Drift = 0.05 dB Peak SAR (extrapolated) = 28.0 W/kg **SAR(1 g) = 13.9 W/kg; SAR(10 g) = 6.34 W/kg** Smallest distance from peaks to all points 3 dB below = 9 mm Ratio of SAR at M2 to SAR at M1 = 49.5% Maximum value of SAR (measured) = 23.1 W/kg

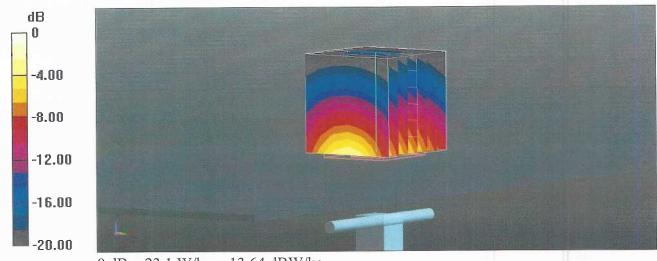

0 dB = 23.1 W/kg = 13.64 dBW/kg

Impedance Measurement Plot for Head TSL

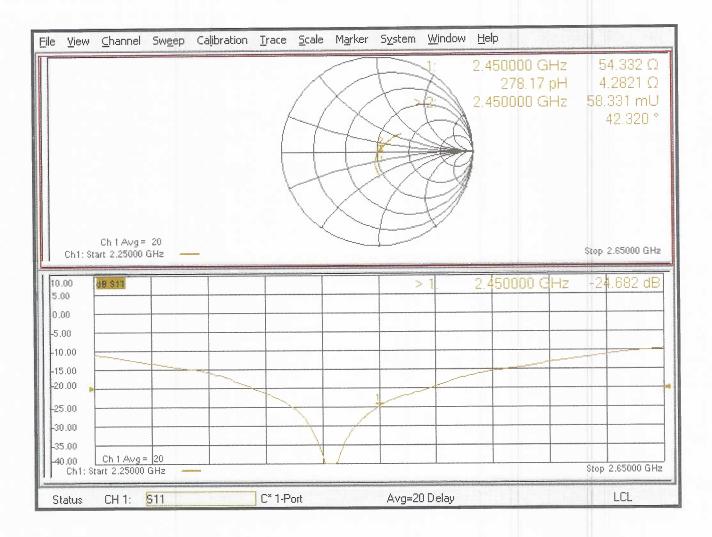

Calibration Laboratory of Schmid & Partner **Engineering AG** Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst S

- Service suisse d'étalonnage
- С Servizio svizzero di taratura
- S **Swiss Calibration Service**

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Certificate No: D2550V2-1003 Jun21

Client

RF Exposure Lab

Chern	та спроснім дар	
CAL	IBRATION CERTIFICATE	

Object	D2550V2 - SN:1003
Calibration procedure(s)	QA CAL-05.v11 Calibration Procedure for SAR Validation Sources between 0.7-3 GHz
Calibration date:	June 03, 2021

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03291/03292)	Apr-22
Power sensor NRP-Z91	SN: 103244	09-Apr-21 (No. 217-03291)	Apr-22
Power sensor NRP-Z91	SN: 103245	09-Apr-21 (No. 217-03292)	Apr-22
Reference 20 dB Attenuator	SN: BH9394 (20k)	09-Apr-21 (No. 217-03343)	Apr-22
Type-N mismatch combination	SN: 310982 / 06327	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe EX3DV4	SN: 7349	28-Dec-20 (No. EX3-7349_Dec20)	Dec-21
DAE4	SN: 601	02-Nov-20 (No. DAE4-601_Nov20)	Nov-21
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-20)	In house check: Oct-22
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-20)	In house check: Oct-21
	Name	Function	Signature
Calibrated by:	Jeffrey Katzman	Laboratory Technician	J. hito
Approved by:	Katja Pokovic	Technical Manager	ally
	u 1856 n. 20. (reampni, indernaminalis e usbezoldnegodzy (dobi) (1946))	full without written approval of the laboratory	Issued: June 8, 2021

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst

S Service suisse d'étalonnage С

Servizio svizzero di taratura

S **Swiss Calibration Service**

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossarv:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed • point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole • positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. ٠ No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna • connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2550 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.1	1.91 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	37.3 ± 6 %	1.98 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL

SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	14.2 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	55.3 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.28 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.7 W/kg ± 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	49.4 Ω - 3.5 jΩ
Return Loss	- 29.0 dB

General Antenna Parameters and Design

Electrical Delay (one direction) 1.156 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Extended Calibration

Usage of SAR dipoles calibrated less than 3 years ago but more than 1 year ago were confirmed in maintaining return loss (<-20 dB, within 20% of prior calibration) and impedance (within 5 ohm from prior calibration) requirements per extended calibrations in KDB Publication 865664 D01 v01r04.

D2550V2 SN: 1003 - Head							
Date of Measurement	Return Loss (dB)	Δ%	impedance (Ω)	ΔΩ	Impedance Imaginary (jΩ)	ΔΩ	
6/3/2021	-29.0		49.4		-3.5		
6/4/2022	-28.6	-1.4	48.5	-0.9	-3.8	-0.3	

DASY5 Validation Report for Head TSL

Date: 03.06.2021

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2550 MHz; Type: D2550V2; Serial: D2550V2 - SN:1003


Communication System: UID 0 - CW; Frequency: 2550 MHz Medium parameters used: f = 2550 MHz; σ = 1.98 S/m; ϵ_r = 37.3; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN7349; ConvF(7.85, 7.85, 7.85) @ 2550 MHz; Calibrated: 28.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.11.2020
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)


Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mmReference Value = 117.6 V/m; Power Drift = 0.07 dB Peak SAR (extrapolated) = 29.9 W/kg **SAR(1 g) = 14.2 W/kg; SAR(10 g) = 6.28 W/kg** Smallest distance from peaks to all points 3 dB below = 8.5 mm Ratio of SAR at M2 to SAR at M1 = 47.1% Maximum value of SAR (measured) = 24.3 W/kg

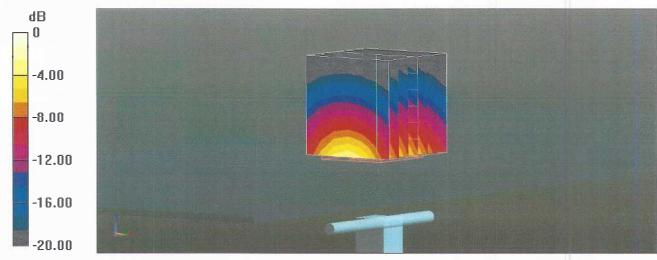

0 dB = 24.3 W/kg = 13.86 dBW/kg

Impedance Measurement Plot for Head TSL

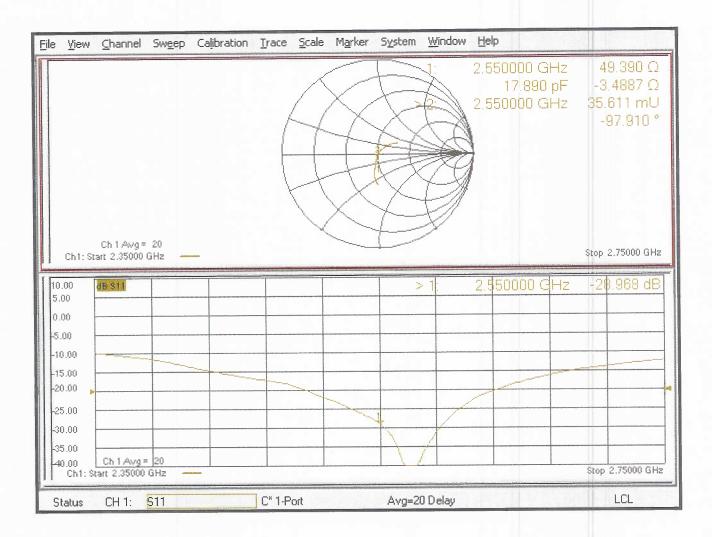

Calibration Laboratory of Schmid & Partner **Engineering AG** Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

RF Exposure Lab Client

Object

CALIBRATION CERTIFICATE

Certificate No: D3500V2-1061_Apr21

Object	D3500V2 - SN:1	061	
Calibration procedure(s)	그는 이 가지 않는 것이 있는 것이 가지 않는 것이 없다.	edure for SAR Validation Source	es between 3-10 GHz
Calibration date:	April 13, 2021		
The measurements and the unce	rtainties with confidence p	tional standards, which realize the physical u probability are given on the following pages a pry facility: environment temperature (22 ± 3)	and are part of the certificate.
Calibration Equipment used (M&			,
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03291/03292)	Apr-22
Power sensor NRP-Z91	SN: 103244	09-Apr-21 (No. 217-03291)	Apr-22 Apr-22
Power sensor NRP-Z91	SN: 103245	09-Apr-21 (No. 217-03292)	Apr-22
Reference 20 dB Attenuator	SN: BH9394 (20k)	09-Apr-21 (No. 217-03343)	Apr-22
Type-N mismatch combination	SN: 310982 / 06327	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe EX3DV4	SN: 3503	30-Dec-20 (No. EX3-3503_Dec20)	Dec-21
DAE4	SN: 601	02-Nov-20 (No. DAE4-601_Nov20)	Nov-21
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-20)	In house check: Oct-22
BE		,	

Name Function Signature Calibrated by: Michael Weber H.W.S.S. A. C. S.S. Laboratory Technician Approved by: Katja Pokovic

Technical Manager

15-Jun-15 (in house check Oct-20)

31-Mar-14 (in house check Oct-20)

Issued: April 15, 2021

In house check: Oct-22

In house check: Oct-21

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

SN: 100972

SN: US41080477

Certificate No: D3500V2-1061_Apr21

RF generator R&S SMT-06

Network Analyzer Agilent E8358A

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst

C Service suisse d'étalonnage

Servizio svizzero di taratura

S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	3500 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	37.9	2.91 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	37.3 ± 6 %	2.93 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	6.73 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	67.0 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.52 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	25.1 W/kg ± 19.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.5 Ω - 5.3 jΩ		
Return Loss	- 24.2 dB		

General Antenna Parameters and Design

Electrical Delay (one direction) 1.134 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by SPEAG	Manufactured by	
-----------------------	-----------------	--

Extended Calibration

Usage of SAR dipoles calibrated less than 3 years ago but more than 1 year ago were confirmed in maintaining return loss (<-20 dB, within 20% of prior calibration) and impedance (within 5 ohm from prior calibration) requirements per extended calibrations in KDB Publication 865664 D01 v01r04.

D3500V2 SN: 1061 - Head						
Date of MeasurementReturn Loss (dB)Δ%Impedance Real (Ω)Impedance ΔΩImpedance Imaginary (jΩ)Δ					ΔΩ	
4/13/2018	-24.2		53.5		-5.3	
4/22/2019	-23.9	-1.2	51.9	-1.6	-4.8	0.5

DASY5 Validation Report for Head TSL

Date: 13.04.2021

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 3500 MHz; Type: D3500V2; Serial: D3500V2 - SN: 1061


Communication System: UID 0 - CW; Frequency: 3500 MHz Medium parameters used: f = 3500 MHz; σ = 2.93 S/m; ϵ_r = 37.3; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN3503; ConvF(7.91, 7.91, 7.91) @ 3500 MHz; Calibrated: 30.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 02.11.2020
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)


Dipole Calibration for Head Tissue/Pin=100 mW, d=10mm 3500/Zoom Scan, dist=1.4mm

(8x8x8)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mmReference Value = 72.28 V/m; Power Drift = 0.02 dB Peak SAR (extrapolated) = 18.2 W/kg SAR(1 g) = 6.73 W/kg; SAR(10 g) = 2.52 W/kg Smallest distance from peaks to all points 3 dB below = 8 mm Ratio of SAR at M2 to SAR at M1 = 74.3% Maximum value of SAR (measured) = 12.7 W/kg

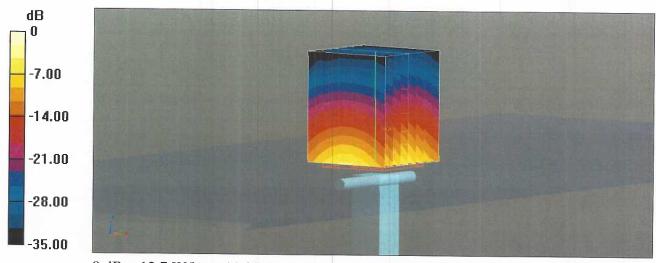

0 dB = 12.7 W/kg = 11.05 dBW/kg

Impedance Measurement Plot for Head TSL

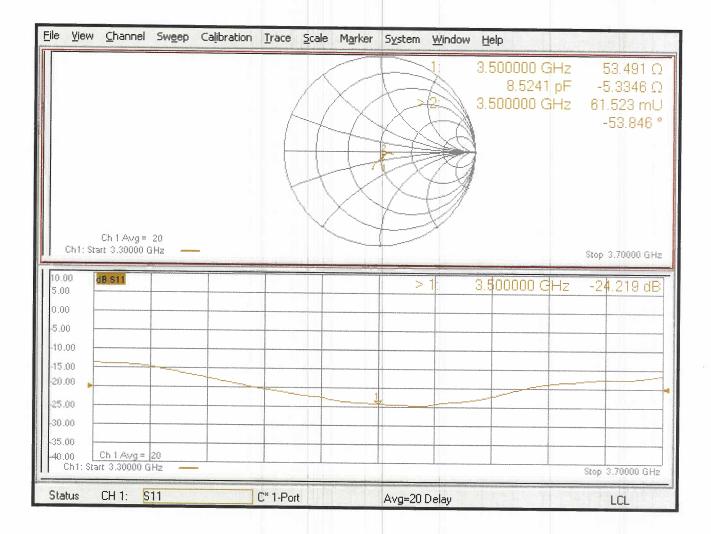



Appendix F – DAE Calibration Data Sheets

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client RF Exposure Lab

Certificate No: DAE4-1416_Apr22

Accreditation No.: SCS 0108

S

С

S

CALIBRATION C	ERTIFICATE				
Object	DAE4 - SD 000 D	04 BM - SN: 1416			
Calibration procedure(s)	QA CAL-06.v30 Calibration procedure for the data acquisition electronics (DAE)				
Calibration date:	April 12, 2022				
The measurements and the uncer	tainties with confidence pro	nal standards, which realize the physical un obability are given on the following pages ar	nd are part of the certificate.		
All calibrations have been conduc	ted in the closed laboratory	r facility: environment temperature (22 ± 3)°	C and humidity < 70%.		
Calibration Equipment used (M&T	E critical for calibration)				
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration		
Keithley Multimeter Type 2001	SN: 0810278	31-Aug-21 (No:31368)	Aug-22		
Secondary Standards	ID #	Check Date (in house)	Scheduled Check		
Auto DAE Calibration Unit	SE UWS 053 AA 1001	24-Jan-22 (in house check)	In house check: Jan-23		
Calibrator Box V2.1	SE UMS 006 AA 1002	24-Jan-22 (in house check)	In house check: Jan-23		
Calibrated by:	Name Adrian Gehring	Function Laboratory Technician	Signature		
Approved by:	Sven Kühn	Deputy Manager	i.V.R Muni		
This calibration cartificate shall no	t he reproduced except in f	ull without written approval of the laborator	Issued: April 12, 2022		

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst

Service suisse d'étalonnage

С Servizio svizzero di taratura S

Swiss Calibration Service

S

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary

DAE data acquisition electronics Connector angle information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by • comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically • by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a • result from the performance test and require no uncertainty.
 - ٠ DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - . *Common mode sensitivity:* Influence of a positive or negative common mode voltage on the differential measurement.
 - Channel separation: Influence of a voltage on the neighbor channels not subject to an • input voltage.
 - AD Converter Values with inputs shorted: Values on the internal AD converter • corresponding to zero input voltage
 - Input Offset Measurement. Output voltage and statistical results over a large number of . zero voltage measurements.
 - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - Input resistance: Typical value for information: DAE input resistance at the connector, • during internal auto-zeroing and during measurement.
 - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
 - Power consumption: Typical value for information. Supply currents in various operating modes.

DC Voltage Measurement

A/D - Converter Reso	lution nominal			
High Range:	1LSB =	6.1µV ,	full range =	-100+300 mV
Low Range:	1LSB =	61nV ,	full range =	-1+3mV
DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec				

Calibration Factors	X	Y	Z
High Range	403.562 ± 0.02% (k=2)	403.870 ± 0.02% (k=2)	404.137 ± 0.02% (k=2)
Low Range	3.97865 ± 1.50% (k=2)	3.99513 ± 1.50% (k=2)	3.97046 ± 1.50% (k=2)

Connector Angle

Connector Angle to be used in DASY system	107.5 ° ± 1 °
-------------------------------------------	---------------

Appendix (Additional assessments outside the scope of SCS0108)

High Range		Reading (μV)	Difference (µV)	Error (%)
Channel X	+ Input	199993.69	0.39	0.00
Channel X	+ Input	20001.91	0.04	0.00
Channel X	- Input	-20001.32	0.29	-0.00
Channel Y	+ Input	199995.49	2.37	0.00
Channel Y	+ Input	20001.59	-0.18	-0.00
Channel Y	- Input	-20002.90	-1.28	0.01
Channel Z	+ Input	199997.14	3.84	0.00
Channel Z	+ Input	20000.35	-1.29	-0.01
Channel Z	- Input	-20003.32	-1.40	0.01

1. DC Voltage Linearity

Low Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	2001.25	0.20	0.01
Channel X + Input	201.83	0.41	0.20
Channel X - Input	-198.42	0.20	-0.10
Channel Y + Input	2000.98	-0.02	-0.00
Channel Y + Input	200.80	-0.47	-0.23
Channel Y - Input	-199.14	-0.51	0.25
Channel Z + Input	2000.99	0.08	0.00
Channel Z + Input	200.25	-0.91	-0.45
Channel Z - Input	-200.06	-1.29	0.65

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (µV)
Channel X	200	-3.28	-4.95
	- 200	6.21	4.15
Channel Y	200	-6.92	-7.58
	- 200	6.27	6.10
Channel Z	200	-23.61	-23.40
	- 200	21.76	21.65

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Υ (μV)	Channel Z (μV)
Channel X	200	-	2.55	-3.59
Channel Y	200	7.33	-	2.96
Channel Z	200	8.86	6.81	-

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15996	17631
Channel Y	16152	16767
Channel Z	16134	15846

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec Input $10M\Omega$

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (μV)
Channel X	0.76	-0.27	1.42	0.33
Channel Y	-0.76	-2.04	0.57	0.45
Channel Z	-0.41	-1.10	0.34	0.30

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9



Appendix G – Phantom Calibration Data Sheets

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 1 245 9700, Fax +41 1 245 9779 info@speag.com, http://www.speag.com

Certificate of Conformity / First Article Inspection

Item	SAM Twin Phantom V4.0	
Type No	QD 000 P40 C	
Series No	TP-1150 and higher	
Manufacturer	SPEAG	
	Zeughausstrasse 43	
	CH-8004 Zürich	
	Switzerland	

Tests

The series production process used allows the limitation to test of first articles.

Complete tests were made on the pre-series Type No. QD 000 P40 AA, Serial No. TP-1001 and on the series first article Type No. QD 000 P40 BA, Serial No. TP-1006. Certain parameters have been retested using further series items (called samples) or are tested at each item.

Test	Requirement	Details	Units tested
Dimensions	Compliant with the geometry according to the CAD model.	IT'IS CAD File (*)	First article, Samples
Material thickness of shell	Compliant with the requirements according to the standards	2mm +/- 0.2mm in flat and specific areas of head section	First article, Samples, TP-1314 ff.
Material thickness at ERP	Compliant with the requirements according to the standards	6mm +/- 0.2mm at ERP	First article, All items
Material parameters	Dielectric parameters for required frequencies	300 MHz – 6 GHz: Relative permittivity < 5, Loss tangent < 0.05	Material samples
Material resistivity	The material has been tested to be compatible with the liquids defined in the standards if handled and cleaned according to the instructions. Observe technical Note for material compatibility.	DEGMBE based simulating liquids	Pre-series, First article, Material samples
Sagging	Compliant with the requirements according to the standards. Sagging of the flat section when filled with tissue simulating liquid.	< 1% typical < 0.8% if filled with 155mm of HSL900 and without DUT below	Prototypes, Sample testing

Standards

- [1] CENELEC EN 50361
- [2] IEEE Std 1528-2003
- [3] IEC 62209 Part I
- [4] FCC OET Bulletin 65, Supplement C, Edition 01-01
- (*) The IT'IS CAD file is derived from [2] and is also within the tolerance requirements of the shapes of the other documents.

Conformity

Based on the sample tests above, we certify that this item is in compliance with the uncertainty requirements of SAR measurements specified in standards [1] to [4].

Date

07.07.2005

a g e <u>p</u> <u>Ş</u>

Schmid & Pariner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland Phone 141 1 245 3700, Fax 44 14 245 9779 Info@epeag.com, http://www.speag.com

Signature / Stamp

Doc No 881 ~ QD 000 P40 C - F

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 9700, Fax +41 44 245 9779 info@speag.com, http://www.speag.com

Certificate of Conformity / First Article Inspection

ltem	Oval Flat Phantom ELI 4.0
Type No	QD OVA 001 B
Series No	1003 and higher
Manufacturer	Untersee Composites
	Knebelstrasse 8
	CH-8268 Mannenbach, Switzerland

Tests

Complete tests were made on the prototype units QD OVA 001 AA 1001, QD OVA 001 AB 1002, pre-series units QD OVA 001 BA 1003-1005 as well as on the series units QD OVA 001 BB, 1006 ff.

Test	Requirement	Details	Units tested
Material thickness	Compliant with the standard requirements	Bottom plate: 2.0mm +/- 0.2mm	ali
Material parameters	Dielectric parameters for required frequencies	< 6 GHz: Rel. permittivity = 4 +/-1, Loss tangent ≤ 0.05	Material sample
Material resistivity	The material has been tested to be compatible with the liquids defined in the standards if handled and cleaned according to the instructions.	DGBE based simulating liquids. Observe Technical Note for material compatibility.	Equivalent phantoms, Material sample
Shape	Thickness of bottom material, Internal dimensions, Sagging compatible with standards from minimum frequency	Bottom elliptical 600 x 400 mm Depth 190 mm, Shape is within tolerance for filling height up to 155 mm, Eventual sagging is reduced or elimínated by support via DUT	Prototypes, Sample testing

Standards

- CENELEC EN 50361-2001, « Basic standard for the measurement of the Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz – 3 GHz) », July 2001
- [2] IEEE 1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques, December 2003
- IEC 62209 1, "Specific Absorption Rate (SAR) in the frequency range of 300 MHz to 3 GHz Measurement Procedure, Part 1: Hand-held mobile wireless communication devices", February 2005
- [4] IEC 62209 2, Draft, "Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices – Human models, Instrumentation and Procedures – Part 2: Procedure to determine the Specific Absorption Rate (SAR) in the head and body for 30 MHz to 6 GHz Handheld and Body-Mounted Devices used in close proximity to the Body.", February 2005
- [5] OET Bulletin 65, Supplement C, "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields", Edition January 2001

Based on the tests above, we certify that this item is in compliance with the standards [1] to [5] if operated according to the specific requirements and considering the thickness. The dimensions are fully compliant with [4] from 30 MHz to 6 GHz. For the other standards, the minimum lower frequency limit is limited due to the dimensional requirements ([1]: 450 MHz, [2]: 300 MHz, [3]: 800 MHz, [5]: 375 MHz) and possibly further by the dimensions of the DUT. **S P 6 a G**

Date 28.4.2008 Signature / Stamp	Schmi <u>d &</u> Partner Engineering AG Zeughaugstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 9709, Fax +41,44,245 9779 info@speag.com; http://www.speag.com
----------------------------------	-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

Doc No 881 - QD OVA 001 B - D

1 (1)

Page