

ITEM NO.	PART NUMBER	DESCRIPTION	QTY.
1	8115527	LABEL, 4x2 ZEBRA PRINTER	1

REV.	ECR	DESCRIPTION	DATE	BY
01	1275	INITIAL RELEASE	1/30/2020	SLG


NOTES:
THE FOLLOWING ITEM CODE / SERIAL PREFIXES ARE APPROVED FOR THIS LABEL TEMPLATE

- 3117617
- 3117717
- 3117817
- 3117917
- 3118017
- 3118117
- 3118217
- 3118317
- 3118417

ARTWORK LOCATION: S:\ERP\BarTender\SyteLine
ARTWORK FILE NAME: 4x2 Mobius Battery Label 5.0

NOTES, UNLESS OTHERWISE SPECIFIED:

1. APPROVED LABEL: MaxTRAN PART # L-ZP-40201P. ALTERNATES REQUIRE ENGINEERING APPROVAL.
2. LABEL CONSTRUCTION: 2 MIL, OPAQUE, GLOSS-WHITE, THERMAL TRANSFER POLYESTER FILM. PERMANENT AGGRESSIVE ADHESIVE. SUPPLIED IN 3" CORE ROLLS WITH BACKING PERFORATED BETWEEN LABELS.
3. LABEL TO MEET REQUIREMENTS OF THE FOLLOWING STANDARD(S):
 - ANSI/UL 969, MARKING & LABELING SYSTEMS.
4. REFERENCE: INTENDED APPLICATIONS REQUIRE:
 - DURABILITY RELATED TO PERMANENT ADHESION TO ALUMINUM AND POLYESTER POWDER COAT.
 - RESISTANCE TO UV LIGHT AND HEALTH INSTITUTION CLEANING SOLVENTS.
 - COMPATIBILITY WITH ZEBRA ZT410 PRINTERS.
 - COMPATIBILITY WITH PRINTER RIBBON(S): 8115528.

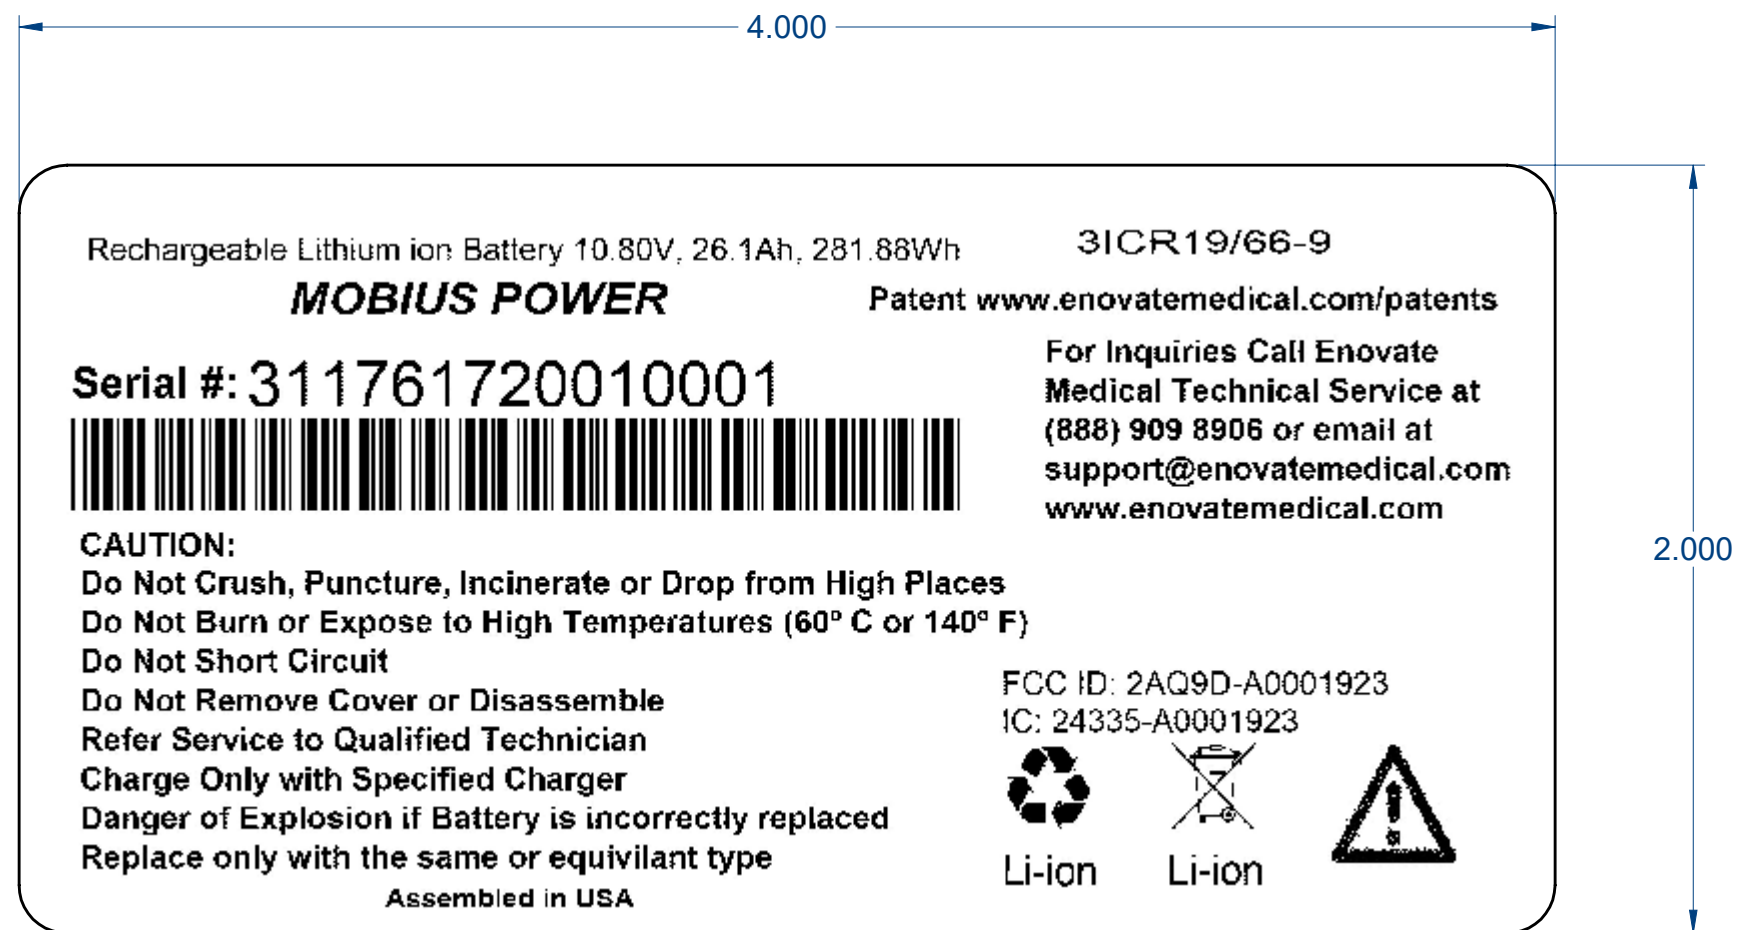

SERIAL #	SERIAL # BREAKDOWN		
	MODEL	DATE YYMM	SERIAL #
311761720010001	3117617	2001	0001

THIS DOCUMENT IS UNCONTROLLED WHEN PRINTED

DIMENSIONS INCH UNLESS OTHERWISE NOTED, ALL MM DIMENSIONS ARE IN [BRACKETS] AND REFERENCE. SEE MODEL FOR ANY FEATURES NOT DIMENSIONED.	ALL EDGES MUST BE FREE OF BURRS. BREAK ALL EDGES TO .005"-.015" UNLESS OTHERWISE NOTED. ALL THREADS TO BE FREE OF POWDER COAT. ALL SURFACES MUST BE FREE OF GREASE/OIL. ALL CIRCLED AND GD&T DIMENSIONS ARE CRITICAL INSPECTION DIMENSIONS	PROPRIETARY AND CONFIDENTIAL: THIS DRAWING WAS DEVELOPED FROM CONFIDENTIAL INFORMATION AND MAY NOT BE DUPLICATED OR THE INFORMATION DISCLOSED WITHOUT WRITTEN AUTHORIZATION FROM ENOVATE MEDICAL. <input type="checkbox"/> CRITICAL COMPONENT <input checked="" type="checkbox"/> RoHS	3RD ANGLE PROJECTION 	PART NUMBER M0002043	DWG REV 01	 www.enovatemedical.com
				DESCRIPTION LABEL, MOBIUS 5.0 BLE BATTERY		

Rechargeable Lithium Ion Battery 10.80V, 26.1Ah, 281.88Wh

3ICR19/66-9

MOBIUS POWER

Patent www.enovatedmedical.com/patents

Serial #: 311761720020005

For Inquiries Call Enovate
Medical Technical Service at
(888) 909 8906 or email at
support@enovatedmedical.com
www.enovatedmedical.com



CAUTION:

- Do Not Crush, Puncture, Incinerate or Drop from High Places
- Do Not Burn or Expose to High Temperatures (60° C or 140° F)
- Do Not Short Circuit
- Do Not Remove Cover or Disassemble
- Refer Service to Qualified Technician
- Charge Only with Specified Charger
- Danger of Explosion if Battery is incorrectly replaced
- Replace only with the same or equivalent type

FCC ID: 2AQ9D-A0001923

IC: 24335-A0001923



Li-ion



Li-ion



Assembled in USA

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.