

**EMC Test Report****Application for FCC Grant of Equipment Authorization  
Canada Certification****Innovation, Science and Economic Development Canada  
RSS-Gen Issue 5 / RSS-247 Issue 2  
FCC Part 15 Subpart C****Model: A0001923**IC CERTIFICATION #: 24335-A0001923  
FCC ID: 2AQ9D-A0001923APPLICANT: Enovate Medical  
1152 Park Avenue  
Murfreesboro, TN 37129TEST SITE(S): National Technical Systems  
41039 Boyce Road.  
Fremont, CA. 94538-2435

IC SITE REGISTRATION #: 2845B-4

PROJECT NUMBER: PR106495

REPORT DATE: February 11, 2020

REISSUE DATE: February 19, 2020

FINAL TEST DATES: January 6, 7 and 9, 2020

TOTAL NUMBER OF PAGES: 51



This report and the information contained herein represent the results of testing test articles identified and selected by the client performed to specifications and/or procedures selected by the client. National Technical Systems (NTS) makes no representations, expressed or implied, that such testing is adequate (or inadequate) to demonstrate efficiency, performance, reliability, or any other characteristic of the articles being tested, or similar products. This report should not be relied upon as an endorsement or certification by NTS of the equipment tested, nor does it represent any statement whatsoever as to its merchantability or fitness of the test article, or similar products, for a particular purpose. This report shall not be reproduced except in full



**VALIDATING SIGNATORIES**

PROGRAM MGR

Deniz Demirci  
Senior Wireless / EMC Engineer

TECHNICAL REVIEWER:

Deniz Demirci  
Senior Wireless / EMC Engineer

FINAL REPORT PREPARER:

David Guidotti  
Senior Technical Writer

QUALITY ASSURANCE DELEGATE

Jesse Reel  
Quality Assurance



**REVISION HISTORY**

Rev#	Date	Comments	Modified By
-	February 11, 2020	First release	
1	February 19, 2020	Notes added to state the EUT was pre-scanned in all three orientations.	Deniz Demirci

## TABLE OF CONTENTS

<b>VALIDATING SIGNATORIES .....</b>	<b>2</b>
<b>REVISION HISTORY .....</b>	<b>3</b>
<b>TABLE OF CONTENTS .....</b>	<b>4</b>
<b>SCOPE.....</b>	<b>5</b>
<b>OBJECTIVE .....</b>	<b>5</b>
<b>STATEMENT OF COMPLIANCE.....</b>	<b>6</b>
<b>DEVIATIONS FROM THE STANDARDS.....</b>	<b>6</b>
<b>TEST RESULTS SUMMARY .....</b>	<b>7</b>
DIGITAL TRANSMISSION SYSTEMS (2400 – 2483.5MHZ) .....	7
MEASUREMENT UNCERTAINTIES.....	8
<b>EQUIPMENT UNDER TEST (EUT) DETAILS.....</b>	<b>9</b>
GENERAL.....	9
ANTENNA SYSTEM .....	9
ENCLOSURE.....	9
MODIFICATIONS.....	9
SUPPORT EQUIPMENT.....	9
EUT INTERFACE PORTS .....	10
EUT OPERATION .....	10
<b>TEST SITE.....</b>	<b>11</b>
GENERAL INFORMATION.....	11
CONDUCTED EMISSIONS CONSIDERATIONS .....	11
RADIATED EMISSIONS CONSIDERATIONS .....	11
<b>MEASUREMENT INSTRUMENTATION .....</b>	<b>12</b>
RECEIVER SYSTEM .....	12
INSTRUMENT CONTROL COMPUTER .....	12
LINE IMPEDANCE STABILIZATION NETWORK (LISN).....	12
FILTERS/ATTENUATORS .....	13
ANTENNAS.....	13
ANTENNA MAST AND EQUIPMENT TURNTABLE.....	13
INSTRUMENT CALIBRATION.....	13
<b>TEST PROCEDURES .....</b>	<b>14</b>
EUT AND CABLE PLACEMENT .....	14
CONDUCTED EMISSIONS.....	14
RADIATED EMISSIONS.....	14
CONDUCTED EMISSIONS FROM ANTENNA PORT .....	17
BANDWIDTH MEASUREMENTS .....	17
SPECIFICATION LIMITS AND SAMPLE CALCULATIONS .....	18
CONDUCTED EMISSIONS SPECIFICATION LIMITS: FCC 15.207; FCC 15.107(A), RSS GEN .....	18
GENERAL TRANSMITTER RADIATED EMISSIONS SPECIFICATION LIMITS .....	19
OUTPUT POWER LIMITS – DIGITAL TRANSMISSION SYSTEMS .....	20
TRANSMIT MODE SPURIOUS RADIATED EMISSIONS LIMITS – FHSS AND DTS SYSTEMS.....	20
SAMPLE CALCULATIONS - CONDUCTED EMISSIONS .....	21
SAMPLE CALCULATIONS - RADIATED EMISSIONS.....	21
<b>APPENDIX A TEST EQUIPMENT CALIBRATION DATA .....</b>	<b>22</b>
<b>APPENDIX B TEST DATA .....</b>	<b>23</b>
<b>END OF REPORT .....</b>	<b>51</b>

## **SCOPE**

An electromagnetic emissions test has been performed on the Enovate Medical model A0001923, pursuant to the following rules:

RSS-Gen Issue 5 “General Requirements for Compliance of Radio Apparatus”  
RSS 247 Issue 2 “Digital Transmission Systems (DTSs), Frequency Hopping Systems (FHSS) and Licence-Exempt Local Area Network (LE-LAN) Devices”  
FCC Part 15 Subpart C

Conducted and radiated emissions data has been collected, reduced, and analyzed within this report in accordance with measurement guidelines set forth in the following reference standards and as outlined in National Technical Systems test procedures:

ANSI C63.10-2013  
FCC DTS Measurement Guidance KDB558074

The intentional radiator above has been tested in a simulated typical installation to demonstrate compliance with the relevant Industry Canada performance and procedural standards.

Final system data was gathered in a mode that tended to maximize emissions by varying orientation of EUT, orientation of power and I/O cabling, antenna search height, and antenna polarization.

Every practical effort was made to perform an impartial test using appropriate test equipment of known calibration. All pertinent factors have been applied to reach the determination of compliance.

National Technical Systems is accredited by the A2LA, certificate number 0214.26, to perform the test(s) listed in this report, except where noted otherwise.

## **OBJECTIVE**

The primary objective of the manufacturer is compliance with the regulations outlined in the previous section.

Prior to marketing in the USA, all unlicensed transmitters and transceivers require certification. Receive-only devices operating between 30 MHz and 960 MHz are subject to either certification or a manufacturer’s declaration of conformity, with all other receive-only devices exempt from the technical requirements.

Prior to marketing in Canada, Class I transmitters, receivers and transceivers require certification. Class II devices are required to meet the appropriate technical requirements but are exempt from certification requirements.

Certification is a procedure where the manufacturer submits test data and technical information to a certification body and receives a certificate or grant of equipment authorization upon successful completion of the certification body's review of the submitted documents. Once the equipment authorization has been obtained, the label indicating compliance must be attached to all identical units, which are subsequently manufactured.

Maintenance of compliance is the responsibility of the manufacturer. Any modification of the product which may result in increased emissions should be checked to ensure compliance has been maintained (i.e., printed circuit board layout changes, different line filter, different power supply, harnessing or I/O cable changes, etc.).

### **STATEMENT OF COMPLIANCE**

The tested sample of Enovate Medical model A0001923 complied with the requirements of the following regulations:

RSS-Gen Issue 5 "General Requirements for Compliance of Radio Apparatus"

RSS 247 Issue 2 "Digital Transmission Systems (DTSS), Frequency Hopping Systems (FHSS) and Licence-Exempt Local Area Network (LE-LAN) Devices"

FCC Part 15 Subpart C

Maintenance of compliance is the responsibility of the manufacturer. Any modifications to the product should be assessed to determine their potential impact on the compliance status of the device with respect to the standards detailed in this test report.

The test results recorded herein are based on a single type test of Enovate Medical model A0001923 and therefore apply only to the tested sample. The sample was selected and prepared by Cameron Boone of Enovate Medical.

### **DEVIATIONS FROM THE STANDARDS**

No deviations were made from the published requirements listed in the scope of this report.

## TEST RESULTS SUMMARY

### DIGITAL TRANSMISSION SYSTEMS (2400 – 2483.5MHz)

FCC Rule Part	RSS Rule Part	Description	Measured Value / Comments	Limit / Requirement	Result
15.247(a)	RSS 247 5.2	Digital Modulation	Systems uses GFSK modulation	System must utilize a digital transmission technology	Complies
15.247 (a) (2)	RSS 247 5.2 (1)	6 dB Bandwidth	698 kHz	>500 kHz	Complies
15.247 (b) (3)	RSS 247 5.4 (4)	Output Power	0.9 dBm (Watts) EIRP = 0.002 W <small>Note 1</small>	1 Watt, EIRP limited to 4 Watts.	Complies
15.247(e)	RSS 247 5.2 (2)	Power Spectral Density	-0.9 dBm/30 kHz	8 dBm/3 kHz	Complies
15.247(d)	RSS 247 5.5	Antenna Port Spurious Emissions	margin >20 dBc	< -20 dBc	Complies
15.247(d) / 15.209	RSS 247 5.5	Radiated Spurious Emissions 9 kHz – 25 GHz	49.7 dBμV/m @ 7320.1 MHz (-4.3 dB)	Refer to the limits section (p19) for restricted bands, all others < -20 dBc	Complies

Note 1: EIRP calculated using antenna gains of 2.5 dBi max. for the highest EIRP system.

### GENERAL REQUIREMENTS APPLICABLE TO ALL BANDS

FCC Rule Part	RSS Rule part	Description	Measured Value / Comments	Limit / Requirement	Result (margin)
15.203	-	RF Connector	Integral antenna	Unique or integral antenna required	Complies
15.407 (b) (6)	RSS-Gen Table 4	AC Conducted Emissions	47.9 dBμV @ 0.184 MHz (-6.4 dB)	Refer to page 18	Complies
15.247 (i) / 15.407 (f)	RSS 102	RF Exposure Requirements	Refer to MPE calculations in separate exhibit, RSS 102 declaration and User Manual statements.	Refer to OET 65, FCC Part 1 and RSS 102	Complies
-	RSS-Gen 6.8	User Manual	Integral antenna	Statement for products with detachable antenna	Complies
-	RSS-Gen 8.4	User Manual	Refer to user manual	Statement for all products	Complies
-	RSP-100 RSS-Gen 6.7	Occupied Bandwidth	1.07 MHz	Information only	N/A

**MEASUREMENT UNCERTAINTIES**

ISO/IEC 17025 requires that an estimate of the measurement uncertainties associated with the emissions test results be included in the report. The measurement uncertainties given below are based on a 95% confidence level and were calculated in accordance with UKAS document LAB 34.

Measurement Type	Measurement Unit	Frequency Range	Expanded Uncertainty
RF power, conducted (power meter)	dBm	25 to 7000 MHz	$\pm 0.5$ dB
RF power, conducted (Spectrum analyzer)	dBm	25 to 7000 MHz	$\pm 0.7$ dB
Conducted emission of transmitter	dBm	25 to 26500 MHz	$\pm 0.7$ dB
Radiated emission (field strength)	dB $\mu$ V/m	25 to 1000 MHz	$\pm 3.6$ dB
		1000 to 40000 MHz	$\pm 6.0$ dB
Conducted Emissions (AC Power)	dB $\mu$ V	0.15 to 30 MHz	$\pm 2.4$ dB



## EQUIPMENT UNDER TEST (EUT) DETAILS

### GENERAL

The Enovate Medical model A0001923 is a Battery pack with BLE. Since the EUT would be placed on a tabletop during operation, the EUT was treated as tabletop equipment during testing to simulate the end-user environment. The radio is battery operated. The electrical rating of the charger of the EUT is 120 Volts, 60 Hz, 0.25 Amps.

The sample was received on January 6, 2020 and tested on January 6, 7 and 9, 2020. The EUT consisted of the following component(s):

Company	Model	Description	Serial Number	FCC ID
Enovate Medical	A0001923	Battery pack	-	2AQ9D-A0001923

### ANTENNA SYSTEM

Integral antenna

### ENCLOSURE

The EUT enclosure is primarily constructed of plastic. It measures approximately 13 cm wide by 10 cm deep by 32 cm high.

### MODIFICATIONS

No modifications were made to the EUT during the time the product was at NTS Silicon Valley.

### SUPPORT EQUIPMENT

No local support equipment was used during testing.

The following equipment was used as local support equipment for AC Conducted Emission testing:

Company	Model	Description	Serial Number	FCC ID
Enovate Medical	MOBIUSPOWER	Charger	311697112517	-

The following equipment was used as remote support equipment:

Company	Model	Description	Serial Number	FCC ID
Raspberry Pi	PI 3	Support computer	-	-

The remote support equipment was used to configure the EUT. It was not connected during testing.

**EUT INTERFACE PORTS**

The I/O cabling configuration during testing was as follows:

Port	Connected To	Description	Cable(s)	
			Shielded or Unshielded	Length(m)
None	-	-	-	-

**EUT OPERATION**

During emissions testing the EUT was configured to transmit at the required channels with maximum rated RF power.

## TEST SITE

### GENERAL INFORMATION

Final test measurements were taken at the test sites listed below. Pursuant to section 2.948 of the FCC’s Rules and section 6.2 of RSS-GEN, NTS has been recognized as an accredited test laboratory by the Commission and Innovation, Science and Economic Development Canada. A description of the facilities employed for testing is maintained by NTS.

Site	Company / Registration Numbers		Location
	FCC	Canada	
Chamber 4	US1031	2845B (Wireless test lab #US0027)	41039 Boyce Road Fremont, CA 94538-2435

ANSI C63.4 recommends that ambient noise at the test site be at least 6 dB below the allowable limits. Ambient levels are below this requirement. The test site(s) contain separate areas for radiated and conducted emissions testing. Results from testing performed in this chamber have been correlated with results from an open area test site. Considerable engineering effort has been expended to ensure that the facilities conform to all pertinent requirements of ANSI C63.4.

### CONDUCTED EMISSIONS CONSIDERATIONS

Conducted emissions testing is performed in conformance with ANSI C63.10. Measurements are made with the EUT connected to the public power network through a nominal, standardized RF impedance, which is provided by a line impedance stabilization network, known as a LISN. A LISN is inserted in series with each current-carrying conductor in the EUT power cord.

### RADIATED EMISSIONS CONSIDERATIONS

The FCC has determined that radiation measurements made in a shielded enclosure are not suitable for determining levels of radiated emissions. Radiated measurements are performed in an open field environment or in a semi-anechoic chamber. The test sites are maintained free of conductive objects within the CISPR defined elliptical area incorporated in ANSI C63.4 guidelines and meet the Normalized Site Attenuation (NSA) requirements of ANSI C63.4.

## **MEASUREMENT INSTRUMENTATION**

### **RECEIVER SYSTEM**

An EMI receiver as specified in CISPR 16-1-1 is used for emissions measurements. The receivers used can measure over the frequency range of 9 kHz up to 2000 MHz. These receivers allow both ease of measurement and high accuracy to be achieved. The receivers have Peak, Average, and CISPR (Quasi-peak) detectors built into their design so no external adapters are necessary. The receiver automatically sets the required bandwidth for the CISPR detector used during measurements. If the repetition frequency of the signal being measured is below 20 Hz, peak measurements are made in lieu of Quasi-Peak measurements.

For measurements above the frequency range of the receivers, a spectrum analyzer is utilized because it provides visibility of the entire spectrum along with the precision and versatility required to support engineering analysis. Average measurements above 1000 MHz are performed on the spectrum analyzer using the linear-average method with a resolution bandwidth of 1 MHz and a video bandwidth of 10 Hz, unless the signal is pulsed in which case the average (or video) bandwidth of the measuring instrument is reduced to onset of pulse desensitization and then increased.

### **INSTRUMENT CONTROL COMPUTER**

Software is used to view and convert receiver measurements to the field strength at an antenna or voltage developed at the LISN measurement port, which is then compared directly with the appropriate specification limit. This provides faster, more accurate readings by performing the conversions described under Sample Calculations within the Test Procedures section of this report. Results are printed in a graphic and/or tabular format, as appropriate. A personal computer is used to record all measurements made with the receivers. The software used for radiated and conducted emissions measurements is NTS EMI Test Software (rev 2.10)

### **LINE IMPEDANCE STABILIZATION NETWORK (LISN)**

Line conducted measurements utilize a 50  $\mu$  Line Impedance Stabilization Network as the monitoring point. The LISN used also contains a 250  $\mu$ H CISPR adapter. This network provides for calibrated radio frequency noise measurements by the design of the internal low pass and high pass filters on the EUT and measurement ports, respectively.

**FILTERS/ATTENUATORS**

External filters and precision attenuators are often connected between the receiving antenna or LISN and the receiver. This eliminates saturation effects and non-linear operation due to high amplitude transient events.

**ANTENNAS**

A loop antenna is used below 30 MHz. For the measurement range 30 MHz to 1000 MHz either a combination of a biconical antenna and a log periodic or a bi-log antenna is used. Above 1000 MHz, horn antennas are used. The antenna calibration factors to convert the received voltage to an electric field strength are included with appropriate cable loss and amplifier gain factors to determine an overall site factor, which is then programmed into the test receivers or incorporated into the test software.

**ANTENNA MAST AND EQUIPMENT TURNTABLE**

The antennas used to measure the radiated electric field strength are mounted on a non-conductive antenna mast equipped with a motor-drive to vary the antenna height. Measurements below 30 MHz are made with the loop antenna at a fixed height of 1 m above the ground plane.

ANSI C63.10 specifies that the test height above ground for table mounted devices shall be 80 cm for testing below 1 GHz and 1.5 m for testing above 1 GHz. Floor mounted equipment shall be placed on the ground plane if the device is normally used on a conductive floor or separated from the ground plane by insulating material from 3 to 12 mm if the device is normally used on a non-conductive floor as specified in ANSI C63.4. During radiated measurements, the EUT is positioned on a motorized turntable in conformance with this requirement.

**INSTRUMENT CALIBRATION**

All test equipment is regularly checked to ensure that performance is maintained in accordance with the manufacturer's specifications. All antennas are calibrated at regular intervals with respect to tuned half-wave dipoles. An exhibit of this report contains the list of test equipment used and calibration information.

## TEST PROCEDURES

### EUT AND CABLE PLACEMENT

The regulations require that interconnecting cables be connected to the available ports of the unit and that the placement of the unit and the attached cables simulate the worst case orientation that can be expected from a typical installation, so far as practicable. To this end, the position of the unit and associated cabling is varied within the guidelines of ANSI C63.10, and the worst-case orientation is used for final measurements.

### CONDUCTED EMISSIONS

Conducted emissions are measured at the plug end of the power cord supplied with the EUT. Excess power cord length is wrapped in a bundle between 30 and 40 cm in length near the center of the cord. Preliminary measurements are made to determine the highest amplitude emission relative to the specification limit for all the modes of operation. Placement of system components and varying of cable positions are performed in each mode. A final peak mode scan is then performed in the position and mode for which the highest emission was noted on all current carrying conductors of the power cord.

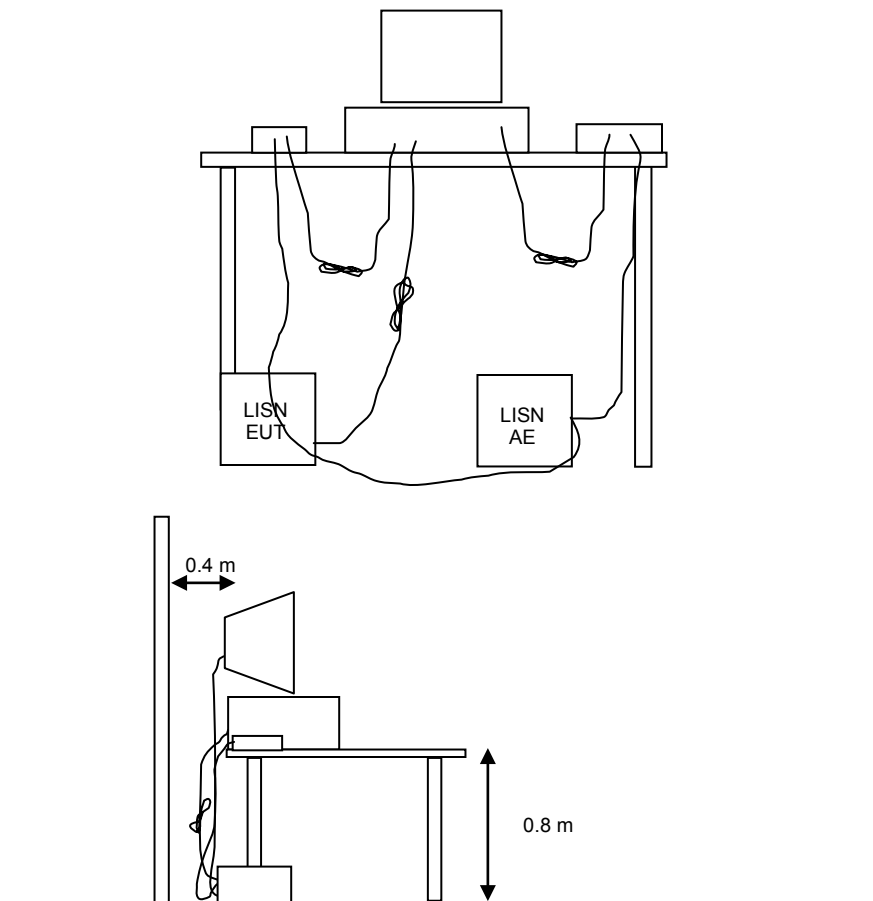



Figure 1 Typical Conducted Emissions Test Configuration

**RADIATED EMISSIONS**


A preliminary scan of the radiated emissions is performed in which all significant EUT frequencies are identified with the system in a nominal configuration. At least two scans are performed, one scan for each antenna polarization (horizontal and vertical; loop parallel and perpendicular to the EUT). During the preliminary scans, the EUT is rotated through 360°, the antenna height is varied (for measurements above 30 MHz) and cable positions are varied to determine the highest emission relative to the limit. Preliminary scans may be performed in a fully anechoic chamber for the purposes of identifying the frequencies of the highest emissions from the EUT.

Final maximization is a phase in which the highest amplitude emissions identified in the spectral search are viewed while the EUT azimuth angle is varied from 0 to 360 degrees relative to the receiving antenna. The azimuth, which results in the highest emission is then maintained while varying the antenna height from 1 to 4 m (for measurements above 30 MHz, measurements below 30 MHz are made with the loop antenna at a fixed height of 1 m). The result is the identification of the highest amplitude for each of the highest peaks. Each recorded level is corrected in the receiver using appropriate factors for cables, connectors, antennas, and preamplifier gain.

When testing above 18 GHz, the receive antenna is located at 1 meter from the EUT and the antenna height is restricted to a maximum of 2.5 m.

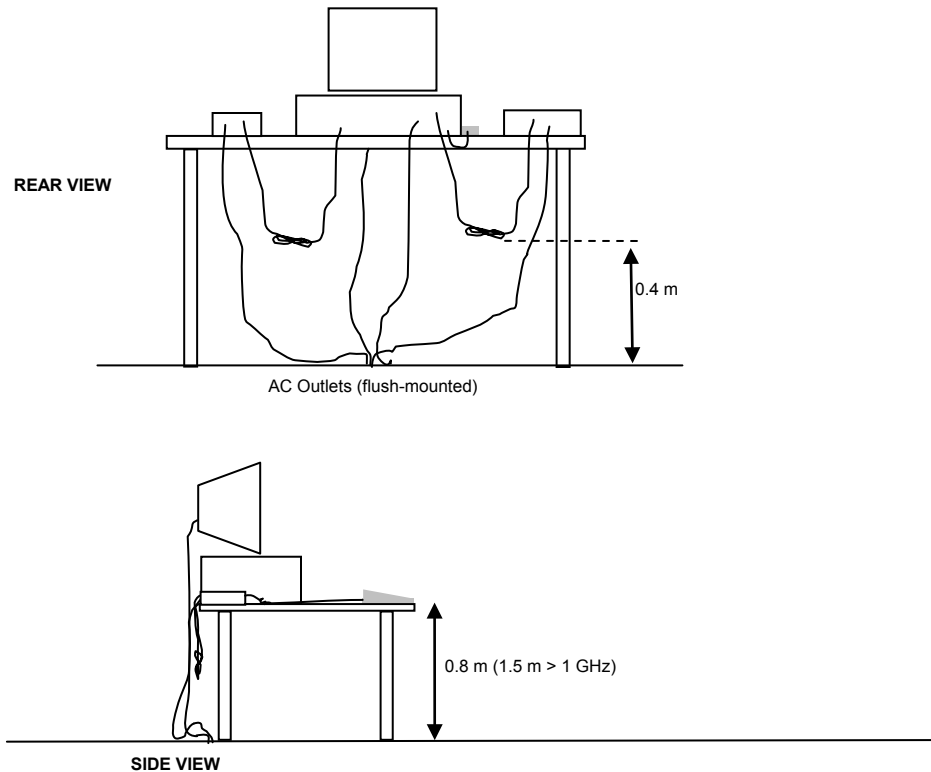


Typical Test Configuration for Radiated Field Strength Measurements

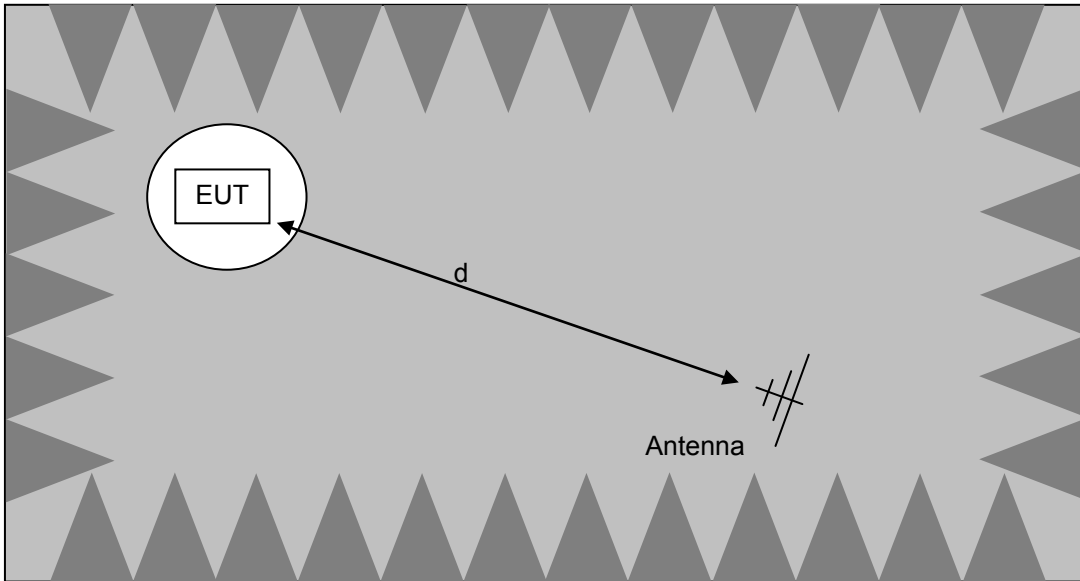

The anechoic materials on the walls and ceiling ensure compliance with the normalized site attenuation requirements of CISPR 16 / CISPR 22 / ANSI C63.4 for an alternate test site at the measurement distances used.

Floor-standing equipment is placed on the floor with insulating supports between the unit and the ground plane.

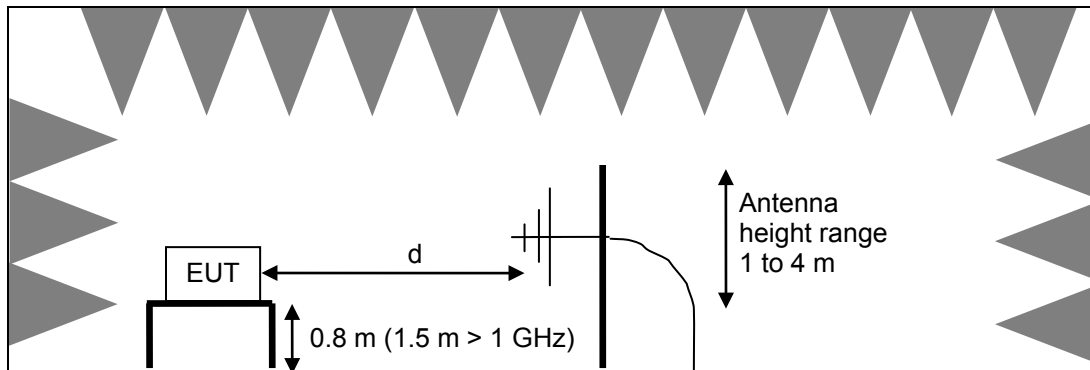


Test Configuration for Radiated Field Strength Measurements  
Semi-Anechoic Chamber, Plan and Side Views



**CONDUCTED EMISSIONS FROM ANTENNA PORT**

Direct measurements of power, bandwidth and power spectral density are performed, where possible, with the antenna port of the EUT connected to either the power meter or spectrum analyzer via a suitable attenuator and/or filter. These are used to ensure that the front end of the measurement instrument is not overloaded by the fundamental transmission.

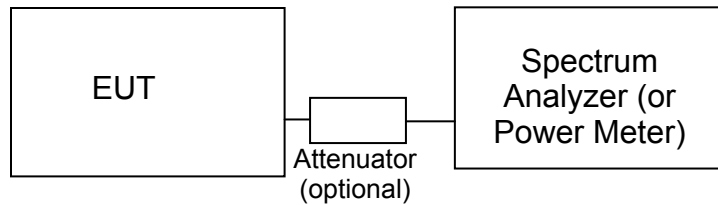

Test Configuration for Antenna Port Measurements

Measurement bandwidths (video and resolution) are set in accordance with the relevant standards and NTS Silicon Valley’s test procedures for the type of radio being tested. When power measurements are made using a resolution bandwidth less than the signal bandwidth the power is calculated by summing the power across the signal bandwidth using either the analyzer channel power function or by capturing the trace data and calculating the power using software. In both cases the summed power is corrected to account for the equivalent noise bandwidth (ENBW) of the resolution bandwidth used.

If power averaging is used (typically for certain digital modulation techniques), the EUT is configured to transmit continuously. Power averaging is performed using either the built-in function of the analyzer or, if the analyzer does not feature power averaging, using external software. In both cases the average power is calculated over a number of sweeps (typically 100). When the EUT cannot be configured to continuously transmit then either the analyzer is configured to perform a gated sweep to ensure that the power is averaged over periods that the device is transmitting or power averaging is disabled and a max-hold feature is used.

If a power meter is used to make output power measurements the sensor head type (peak or average) is stated in the test data table.

**BANDWIDTH MEASUREMENTS**

The 6 dB, 20 dB, 26 dB and/or 99% signal bandwidth are measured using the bandwidths recommended by ANSI C63.10 and RSS GEN.

**SPECIFICATION LIMITS AND SAMPLE CALCULATIONS**

The limits for conducted emissions are given in units of microvolts, and the limits for radiated emissions are given in units of microvolts per meter at a specified test distance. Data is measured in the logarithmic form of decibels relative to one microvolt, or dB microvolts (dB $\mu$ V). For radiated emissions, the measured data is converted to the field strength at the antenna in dB microvolts per meter (dB $\mu$ V/m). The results are then converted to the linear forms of  $\mu$ V and  $\mu$ V/m for comparison to published specifications.

For reference, converting the specification limits from linear to decibel form is accomplished by taking the base ten logarithm, then multiplying by 20. These limits in both linear and logarithmic form are as follows:

**CONDUCTED EMISSIONS SPECIFICATION LIMITS: FCC 15.207; FCC 15.107(a), RSS GEN**

The table below shows the limits for the emissions on the AC power line from an intentional radiator and a receiver.

Frequency (MHz)	Average Limit (dB $\mu$ V)	Quasi Peak Limit (dB $\mu$ V)
0.150 to 0.500	Linear decrease on logarithmic frequency axis between 56.0 and 46.0	Linear decrease on logarithmic frequency axis between 66.0 and 56.0
0.500 to 5.000	46.0	56.0
5.000 to 30.000	50.0	60.0

**GENERAL TRANSMITTER RADIATED EMISSIONS SPECIFICATION LIMITS**

The table below shows the limits for the spurious emissions from transmitters that fall in restricted bands<sup>1</sup>.

Frequency Range (MHz)	Limit (μV/m)	Limit (dBμV/m @ 3m)
0.009-0.490	2400/F <sub>KHz</sub> @ 300 m	67.6-20*log <sub>10</sub> (F <sub>KHz</sub> ) @ 300 m
0.490-1.705	24000/F <sub>KHz</sub> @ 30 m	87.6-20*log <sub>10</sub> (F <sub>KHz</sub> ) @ 30 m
1.705 to 30	30 @ 30 m	29.5 @ 30 m
30 to 88	100 @ 3 m	40 @ 3 m
88 to 216	150 @ 3 m	43.5 @ 3 m
216 to 960	200 @ 3 m	46.0 @ 3 m
Above 960	500 @ 3 m	54.0 @ 3 m

<sup>1</sup> The restricted bands are detailed in FCC 15.205 and RSS-Gen Table 7

**OUTPUT POWER LIMITS – DIGITAL TRANSMISSION SYSTEMS**

The table below shows the limits for output power and output power density. Where the signal bandwidth is less than 20 MHz the maximum output power is reduced to the power spectral density limit plus 10 times the log of the bandwidth (in MHz).

Operating Frequency (MHz)	Output Power	Power Spectral Density
902 – 928	1 Watt (30 dBm)	8 dBm/3 kHz
2400 – 2483.5	1 Watt (30 dBm)	8 dBm/3 kHz
5725 – 5850	1 Watt (30 dBm)	8 dBm/3 kHz

The maximum permitted output power is reduced by 1 dB for every dB the antenna gain exceeds 6 dBi. Fixed point-to-point applications using the 5725 – 5850 MHz band are not subject to this restriction.

**TRANSMIT MODE SPURIOUS RADIATED EMISSIONS LIMITS – FHSS and DTS SYSTEMS**

The limits for unwanted (spurious) emissions from the transmitter falling in the restricted bands are those specified in the general limits sections of FCC Part 15 and RSS 210. All other unwanted (spurious) emissions shall be at least 20 dB below the level of the highest in-band signal level (30 dB if the power is measured using the sample detector/power averaging method).

**SAMPLE CALCULATIONS - CONDUCTED EMISSIONS**

Receiver readings are compared directly to the conducted emissions specification limit (decibel form) as follows:

$$R_r - S = M$$

where:

$R_r$  = Receiver Reading in dB $\mu$ V

S = Specification Limit in dB $\mu$ V

M = Margin to Specification in +/- dB

**SAMPLE CALCULATIONS - RADIATED EMISSIONS**

Receiver readings are compared directly to the specification limit (decibel form). The receiver internally corrects for cable loss, preamplifier gain, and antenna factor. The calculations are in the reverse direction of the actual signal flow, thus cable loss is added and the amplifier gain is subtracted. The Antenna Factor converts the voltage at the antenna coaxial connector to the field strength at the antenna elements.

A distance factor, when used for electric field measurements above 30MHz, is calculated by using the following formula:

$$F_d = 20 * \text{LOG}_{10} (D_m/D_s)$$

where:

$F_d$  = Distance Factor in dB

$D_m$  = Measurement Distance in meters

$D_s$  = Specification Distance in meters

For electric field measurements below 30 MHz the extrapolation factor is either determined by making measurements at multiple distances or a theoretical value is calculated using the formula:

$$F_d = 40 * \text{LOG}_{10} (D_m/D_s)$$

Measurement Distance is the distance at which the measurements were taken and Specification Distance is the distance at which the specification limits are based. The antenna factor converts the voltage at the antenna coaxial connector to the field strength at the antenna elements.

The margin of a given emission peak relative to the limit is calculated as follows:

$$R_c = R_r + F_d$$

and

$$M = R_c - L_s$$

where:

$R_r$  = Receiver Reading in dB $\mu$ V/m

$F_d$  = Distance Factor in dB

$R_c$  = Corrected Reading in dB $\mu$ V/m

$L_s$  = Specification Limit in dB $\mu$ V/m

M = Margin in dB Relative to Spec

## Appendix A Test Equipment Calibration Data

<u>Manufacturer</u>	<u>Description</u>	<u>Model</u>	<u>Asset #</u>	<u>Calibrated</u>	<u>Cal Due</u>
<b>Radiated Emissions, 1 - 18 GHz, 06-Jan-20</b>					
National Technical Systems	NTS EMI Software (rev 2.10)	N/A	WC022452	N/A	
Hewlett Packard	Spectrum Analyzer (Red)	8564E (84125C)	WC055584	10/10/2019	10/10/2020
Micro-Tronics	Filter (High Pass)	HPM50111-01	WC062506	11/25/2019	11/25/2020
EMCO	Horn Antenna	3115	WC062583	7/9/2018	7/9/2020
Hewlett Packard	Microwave Preamplifier, 1-26.5GHz	8449B	WC064416	7/18/2019	7/18/2020
Rohde & Schwarz	EMI Test Receiver, 20 Hz-7 GHz	ESIB 7	WC064492	6/22/2019	6/22/2020
<b>Radiated Emissions, 18 - 25 GHz, 06-Jan-20</b>					
Hewlett Packard	Spectrum Analyzer (Red)	8564E (84125C)	WC055584	10/10/2019	10/10/2020
Hewlett Packard	Microwave Preamplifier Head, 18-40 GHz (Red)	84125C EMI Test Head	WC055586	10/4/2019	10/4/2020
A. H. Systems	Antenna, Horn, 18-40GHz	SAS-574	WC064555	7/8/2019	7/8/2021
<b>Radiated Emissions, 0.009 - 1,000 MHz, 06-Jan-20</b>					
National Technical Systems	NTS EMI Software (rev 2.10)	N/A	WC022452	N/A	
Rhode & Schwarz	Loop Antenna	HFH2-Z2	WC062457	1/5/2018	2/5/2020
Sunol Sciences	Biconilog, 30-3000 MHz	JB3	WC064454	3/11/2019	3/11/2021
Rohde & Schwarz	EMI Test Receiver, 20 Hz-7 GHz	ESIB 7	WC064492	6/22/2019	6/22/2020
Hewlett Packard	9KHz-1300MHz pre-amp	8447F	WC064718	12/2/2019	12/2/2020
<b>Conducted Emissions - AC Power Ports, 07-Jan-20</b>					
National Technical Systems	NTS EMI Software (rev 2.10)	N/A	WC022452	N/A	
EMCO	LISN, 10 kHz-100 MHz	3825/2	WC064407	6/13/2019	6/13/2020
Rohde & Schwarz	EMI Test Receiver, 20 Hz-7 GHz	ESIB 7	WC064492	6/22/2019	6/22/2020
Rohde & Schwarz	Pulse Limiter	ESH3-Z2	WC072359	6/24/2019	6/24/2020
<b>Radio Antenna Port (Power and Spurious Emissions), 09-Jan-20</b>					
National Technical Systems	NTS Capture Analyzer Software (rev 4.0)	N/A	WC022706	N/A	
Agilent Technologies	Analyzer (Spectrum)	E4446A	WC055650	7/18/2019	7/18/2020



## **Appendix B Test Data**

TL106495 Pages 24 – 50



## EMC Test Data

Client:	Enovate Medical	PR Number:	PR106495
Product:	A0001923	T-Log Number:	TL106495-RANA
System Configuration:	-	Project Manager:	Deepa Shetty
Contact:	Steven Godbey	Project Engineer:	Deniz Demirci
Emissions Standard(s):	FCC 15.247, RSS 247, FCC 15B, ICES-003	Class:	B
Immunity Standard(s):	-	Environment:	-

# EMC Test Data

For The

## Enovate Medical

Product

A0001923

Date of Last Test: 1/9/2020





# EMC Test Data

Client:	Enovate Medical	Job Number:	PR106495
Model:	A0001923	T-Log Number:	TL106495-RANA
Contact:	Steven Godbey	Project Manager:	Deepa Shetty
Standard:	FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator:	Deniz Demirci
		Class:	N/A

## RSS-247 and FCC 15.247 (DTS) Antenna Port Measurements Power, PSD, Bandwidth and Spurious Emissions

### Test Specific Details

Objective: The objective of this test session is to perform final qualification testing of the EUT with respect to the specification listed above.

Date of Test: 1/9/2020  
 Test Engineer: M. Birgani  
 Test Location: Lab 4

Config. Used: 2  
 Config Change: -  
 EUT Voltage: Battery

### General Test Configuration

The EUT was connected to the spectrum analyzer or power meter via a suitable attenuator. All measurements were made on a single chain.

All measurements have been corrected to allow for the external attenuators used.

**Ambient Conditions:**                      Temperature:        20-21 °C  
    Rel. Humidity:        42-45 %

### Summary of Results

Run #	Pwr setting	Avg Pwr	Test Performed	Limit	Pass / Fail	Result / Margin
1	1	-	Output Power	15.247(b)	Pass	0.9 dBm
2	1	-	Power spectral Density (PSD)	15.247(d)	Pass	-0.9 dBm/30 kHz
3	1	-	Minimum 6 dB Bandwidth	15.247(a)	Pass	0.70 MHz
3	1	-	99% Bandwidth	RSS GEN	-	1.07 MHz
4	1	-	Spurious emissions	15.247(b)	Pass	margin >20 dBc

### Modifications Made During Testing

No modifications were made to the EUT during testing

### Deviations From The Standard

No deviations were made from the requirements of the standard.



# EMC Test Data

Client:	Enovate Medical	Job Number:	PR106495
Model:	A0001923	T-Log Number:	TL106495-RANA
Contact:	Steven Godbey	Project Manager:	Deepa Shetty
Standard:	FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator:	Deniz Demirci
		Class:	N/A


## Sample Notes

Sample S/N: 31183159070483  
 Driver: Minicom  
 Antenna: Integral

## Procedure Comments:

Measurements performed in accordance with FCC KDB 558074 and ANSI C63.10

Mode	Data Rate	Duty Cycle (x)	Constant DC?	T (ms)	Pwr Cor Factor*	Lin Volt Cor Factor**	Min VBW for FS (Hz)
BLE	1 Mbps	94.7%	Yes	2.116	0.2	0.5	473

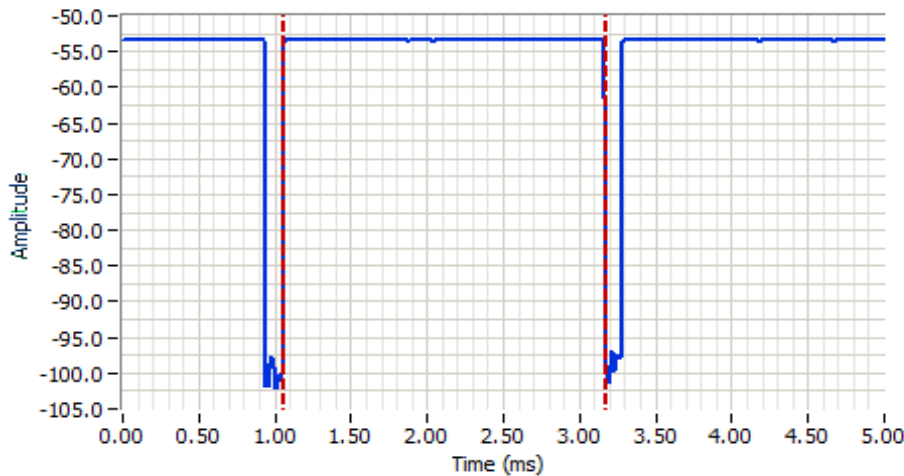

### Analyzer Settings

Rohde&Schwarz,ESI  
 CF: 2440.000 MHz  
 SPAN: 0.000 MHz  
 RB: 1.000 MHz  
 VB: 3.000 MHz  
 Detector: POS  
 Attn: 0 DB  
 RL Offset: 0.0 DB  
 Sweep Time: 5.0ms  
 Ref Lvl: -40.0 DBM

### Comments

BLE 1Mbps  
 Off time: 0.119 ms  
 On time: 2.116 ms  
 Duty cycle: 94.7%

Cursor 1	1.058201	0.0	
Cursor 2	3.174603	0.0	

Delta Time (ms) 2.116

Delta Amplitude 0.0






# EMC Test Data

Client: Enovate Medical	Job Number: PR106495
Model: A0001923	T-Log Number: TL106495-RANA
Contact: Steven Godbey	Project Manager: Deepa Shetty
Standard: FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator: Deniz Demirci
	Class: N/A

Run #1: Output Power  
Mode: BLE

Power Setting	Frequency (MHz)	Output Power		Antenna Gain (dBi)	Result	EIRP		Output Power	
		(dBm)	mW			dBm	W	(dBm)	mW
1	2402	0.9	1.2	2.5	Pass	3.4	0.002		
1	2440	0.8	1.2	2.5	Pass	3.3	0.002		
1	2480	0.7	1.2	2.5	Pass	3.2	0.002		

Note 1: Output power measured using a spectrum analyzer with RB: 3 MHz VB: 8MHz peak, spurious limit is -20 dBc.

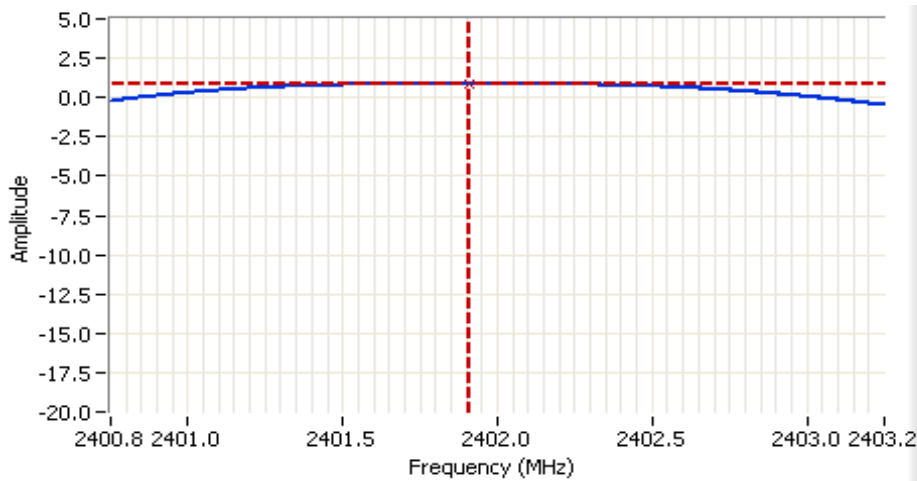

**Analyzer Settings**  
 Agilent Technologies, E4446A  
 CF: 2402.000 MHz  
 SPAN: 2.500 MHz  
 RB: 3.000 MHz  
 VB: 8.000 MHz  
 Detector: POS  
 Attn: 10 DB  
 RL Offset: 11.0 DB  
 Sweep Time: 1.1ms  
 Ref Lvl: 10.0 DBM

**Comments**  
 Power: 0.9 dBm

Cursor 1	2401.911161	0.9	
	0.000000	0.0	






# EMC Test Data

Client: Enovate Medical	Job Number: PR106495
Model: A0001923	T-Log Number: TL106495-RANA
Contact: Steven Godbey	Project Manager: Deepa Shetty
Standard: FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator: Deniz Demirci
	Class: N/A

Run #2: Power spectral Density  
Mode: BLE

Power Setting	Frequency (MHz)	PSD	Limit	Result
		(dBm/30 kHz) <sup>Note 1</sup>	dBm/3 kHz	
1	2402	-1.3	8.0	Pass
1	2440	-0.9	8.0	Pass
1	2480	-1.0	8.0	Pass

Note 1: Test performed per method PKSPD, in KDB 558074. Power spectral density measured using:  $3 \text{ kHz} \leq \text{RBW} \leq 100 \text{ kHz}$ ,  $\text{VBW}=3*\text{RBW}$ , peak detector, span =  $1.5*\text{DTS BW}$ , auto sweep time, max hold.

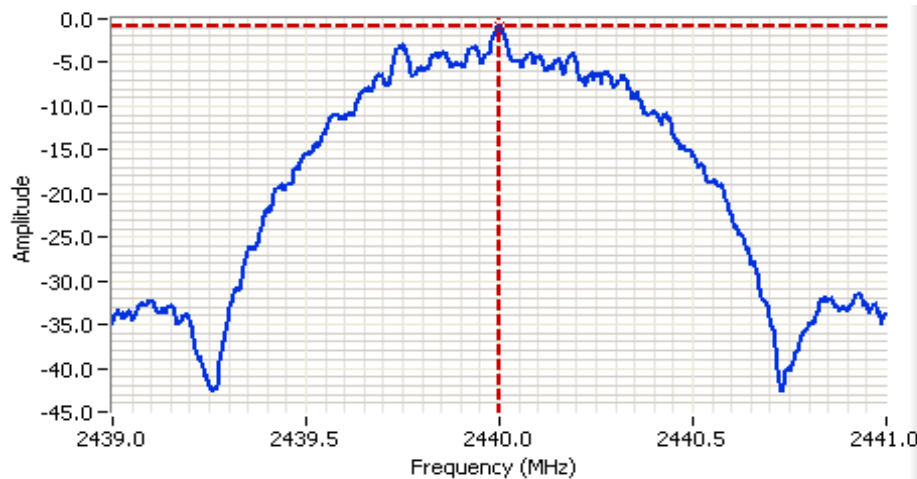

**Analyzer Settings**  
 Agilent Technologies, E4446A  
 CF: 2440.000 MHz  
 SPAN: 2.000 MHz  
 RB: 30.0 kHz  
 VB: 100 kHz  
 Detector: POS  
 Attn: 10 DB  
 RL Offset: 11.0 DB  
 Sweep Time: 2.1ms  
 Ref Lvl: 0.0 DBM

**Comments**  
 PSD: -0.9 dBm/30kHz

Cursor 1	2439.998999	-0.9	
	0.000000	0.0	





# EMC Test Data


Client: Enovate Medical	Job Number: PR106495
Model: A0001923	T-Log Number: TL106495-RANA
Contact: Steven Godbey	Project Manager: Deepa Shetty
Standard: FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator: Deniz Demirci
	Class: N/A

### Run #3: Signal Bandwidth

Mode: BLE

Power Setting	Frequency (MHz)	Bandwidth (MHz)		RBW Setting (MHz)	
		DTS	99%	DTS	99%
1	2402	0.70	1.05	0.1	0.03
1	2440	0.71	1.07	0.1	0.03
1	2480	0.72	1.06	0.1	0.03

Note 1: DTS BW: RBW=100 kHz, VBW ≥ 3\*RBW, peak detector, max hold, auto sweep time, Span 2-5 times measured BW.  
 99% BW: RBW=1-5% of 99%BW, VBW ≥ 3\*RBW, peak detector, max hold, auto sweep time. Span 1.5-5 times OBW.

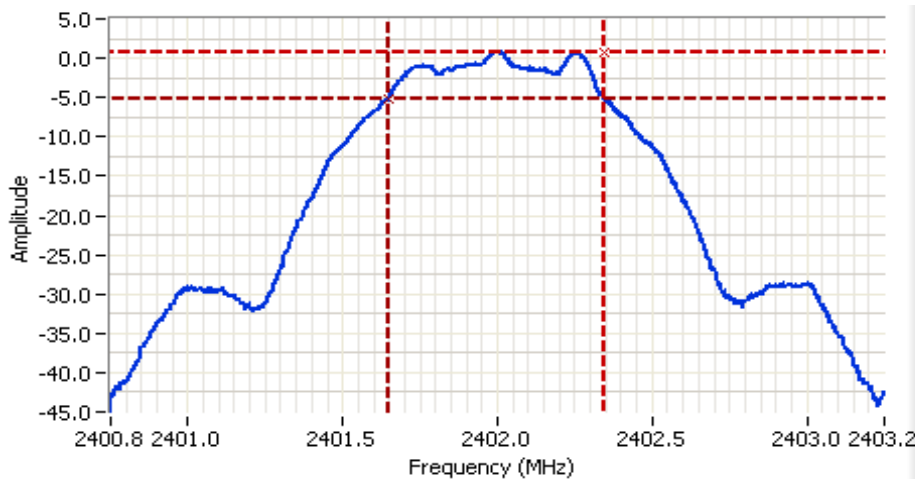

**Analyzer Settings**  
 Agilent Technologies, E4446A  
 CF: 2402.000 MHz  
 SPAN: 2.500 MHz  
 RB: 100 kHz  
 VB: 300 kHz  
 Detector: POS  
 Attn: 10 DB  
 RL Offset: 11.0 DB  
 Sweep Time: 1.1ms  
 Ref Lvl: 10.0 DBM

**Comments**  
 DTS BW: 698 kHz

Cursor 1 2402.346597 0.8

Cursor 2 2401.648398 -5.2

Delta Freq. 698 kHz


Delta Amplitude 6.0





# EMC Test Data

Client: Enovate Medical	Job Number: PR106495
Model: A0001923	T-Log Number: TL106495-RANA
Contact: Steven Godbey	Project Manager: Deepa Shetty
Standard: FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator: Deniz Demirci
	Class: N/A

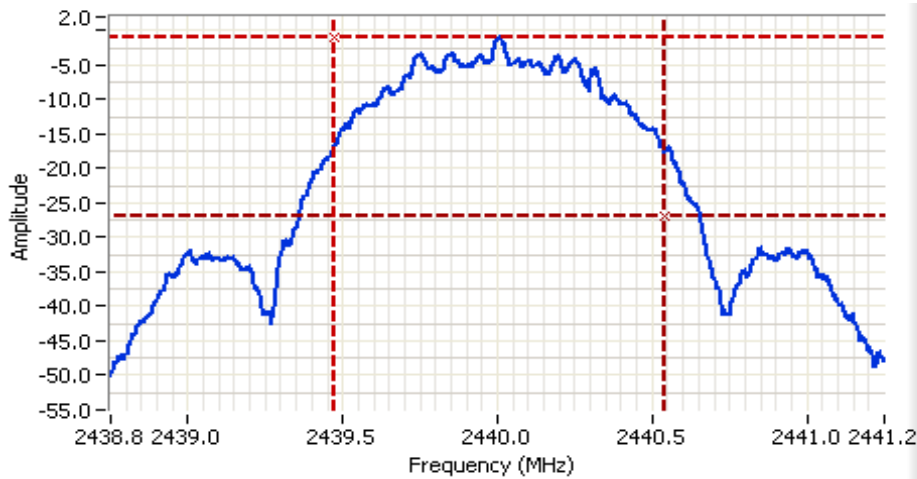

**Analyzer Settings**  
Agilent Technologies, E4446A  
CF: 2440.000 MHz  
SPAN: 2.500 MHz  
RB: 30.0 kHz  
VB: 100 kHz  
Detector: POS  
Attn: 10 DB  
RL Offset: 11.0 DB  
Sweep Time: 2.7ms  
Ref Lvl: 10.0 DBM

**Comments**  
99% BW: 1.065 MHz

Cursor 1	2439.472500	-1.0		Delta Freq.	1.065
Cursor 2	2440.537500	-27.0		Delta Amplitude	26.0






# EMC Test Data

Client: Enovate Medical	Job Number: PR106495
Model: A0001923	T-Log Number: TL106495-RANA
Contact: Steven Godbey	Project Manager: Deepa Shetty
Standard: FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator: Deniz Demirci
	Class: N/A

## Run #4: Out of Band Spurious Emissions

Frequency (MHz)	Power Setting	Mode	Limit	Result
2402	1	BLE	-20 dBc	Pass

Additional plot showing compliance with -20 dBc limit from 2390 MHz to 2400 MHz. Radiated measurements used to show compliance with the limits in the restricted band below 2390 MHz.

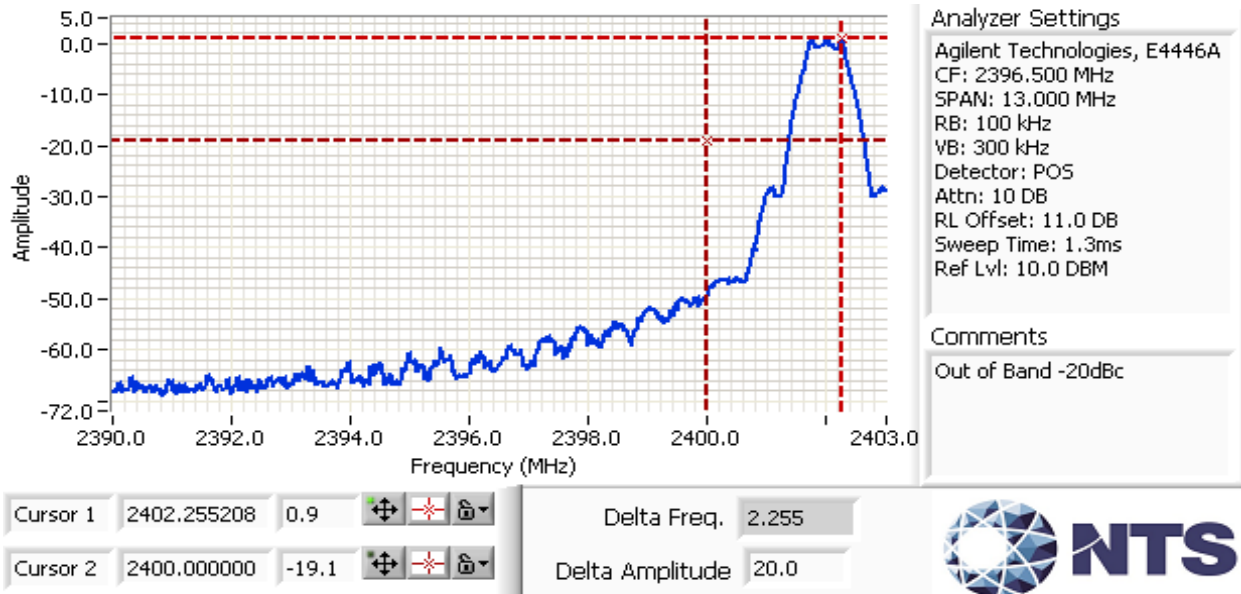



# EMC Test Data

Client:	Enovate Medical	Job Number:	PR106495
Model:	A0001923	T-Log Number:	TL106495-RANA
Contact:	Steven Godbey	Project Manager:	Deepa Shetty
Standard:	FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator:	Deniz Demirci
		Class:	N/A

## RSS-247 and FCC 15.247 (DTS) Radiated Spurious Emissions

### Test Specific Details

Objective: The objective of this test session is to perform final qualification testing of the EUT with respect to the specification listed above.

### General Test Configuration

The EUT and all local support equipment were located on the turntable for radiated spurious emissions testing.

For radiated emissions testing the measurement antenna was located 3 meters from the EUT, unless otherwise noted.

### Ambient Conditions:

Temperature: 22-23 °C  
Rel. Humidity: 43-45 %

### Summary of Results - Device Operating in the 2400-2483.5 MHz Band

Run #	Mode	Channel	Target Power	Power Setting	Test Performed	Limit	Result / Margin
1	BLE	37 2402 MHz	0 dBm	1	Radiated Emissions, 1 - 25 GHz	FCC Part 15.209 / 15.247( c)	48.1 dBµV/m @ 7206.0 MHz (-5.9 dB)
	BLE	17 2440 MHz	0 dBm	1	Radiated Emissions, 1 - 25 GHz		49.7 dBµV/m @ 7320.1 MHz (-4.3 dB)
	BLE	39 2480 MHz	0 dBm	1	Radiated Emissions, 1 - 25 GHz		48.4 dBµV/m @ 7440.0 MHz (-5.6 dB)
2	BLE	37 2402 MHz	0 dBm	1	Band Edge 2390 - 2483.5 MHz	15.247( c)	35.7 dBµV/m @ 2375.3 MHz (-18.3 dB)
	BLE	39 2480 MHz	0 dBm	1			37.1 dBµV/m @ 2483.5 MHz (-16.9 dB)

### Modifications Made During Testing

No modifications were made to the EUT during testing

### Deviations From The Standard

No deviations were made from the requirements of the standard.





# EMC Test Data

Client:	Enovate Medical	Job Number:	PR106495
Model:	A0001923	T-Log Number:	TL106495-RANA
Contact:	Steven Godbey	Project Manager:	Deepa Shetty
Standard:	FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator:	Deniz Demirci
		Class:	N/A

## Sample Notes

Sample S/N: 311761516030250  
 Driver: Minicom  
 Antenna: Integral

## Procedure Comments:

Measurements performed in accordance with FCC KDB 558074  
 Peak measurements performed with: RBW=1 MHz, VBW=3 MHz, peak detector, max hold, auto sweep time  
 Unless otherwise stated/noted, emission has duty cycle  $\geq 98\%$  and was measured using RBW=1 MHz, VBW=10 Hz, peak detector, linear average mode, auto sweep time, max hold.  
 2.4GHz band reject filter used

Mode	Data Rate	Duty Cycle (x)	Constant DC?	T (ms)	Pwr Cor Factor*	Lin Volt Cor Factor**	Min VBW for FS (Hz)
BLE	1 Mbps	94.7%	Yes	2.116	0.2	0.5	473

## Measurement Specific Notes:

Note 1:	Emission in non-restricted band, but limit of 15.209 used.
Note 2:	Emission in non-restricted band, the limit was set 20 dB below the level of the fundamental and measured in 100 kHz.
Note 4:	EUT was pre-scanned in all 3 orientations. Pre-scan results show EUT upright orientation has the highest spurious emission. Final measurements were taken with EUT upright orientation.
Note 6:	Emission has non constant duty cycle $< 98\%$ , average measurement performed: RBW=1 MHz, VBW> 1/T, peak detector, linear average mode, sweep time auto, max hold. Max hold for $50^*(1/DC)$ traces

Date of Test: 01/06/19  
 Test Engineer: Deniz Demirci; M. Birgani  
 Test Location: Chamber #4

Config. Used: 1  
 Config Change: -  
 EUT Voltage: Battery



# EMC Test Data


Client:	Enovate Medical	Job Number:	PR106495
Model:	A0001923	T-Log Number:	TL106495-RANA
Contact:	Steven Godbey	Project Manager:	Deepa Shetty
Standard:	FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator:	Deniz Demirci
		Class:	N/A

Run #1: Radiated Spurious Emissions, 1,000 - 25,000 MHz. Operating Mode: BLE

Run #1a: Low Channel

Channel: 37 - 2402 MHz      Mode: BLE  
 Tx Chain: Main              Data Rate: 1 Mbps



Frequency MHz	Level dB $\mu$ V/m	Pol v/h	15.209 / 15.247		Detector Pk/QP/Avg	Azimuth degrees	Height meters	Comments
			Limit	Margin				
2338.070	40.0	H	54.0	-14.0	AVG	158	2.0	Note 6 - RB 1 MHz;VB 1 kHz;Peak
2338.050	48.8	H	74.0	-25.2	PK	158	2.0	POS; RB 1 MHz; VB: 3 MHz
2402.320	98.6	H	-	-	PK	162	1.8	POS; RB 3 MHz; VB: 10 MHz
4804.060	41.0	H	54.0	-13.0	AVG	54	2.5	Note 6 - RB 1 MHz;VB 1 kHz;Peak
4804.050	49.8	H	74.0	-24.2	PK	54	2.5	RB 1 MHz;VB 3 MHz;Peak
7205.980	48.1	H	54.0	-5.9	AVG	190	2.0	Note 1 - RB 1 MHz;VB 1 kHz;Peak
7206.450	56.5	H	74.0	-17.5	PK	190	2.0	RB 1 MHz;VB 3 MHz;Peak
17890.000	45.9	V	74.0	-28.1	Peak	251	2.0	Noise floor reading

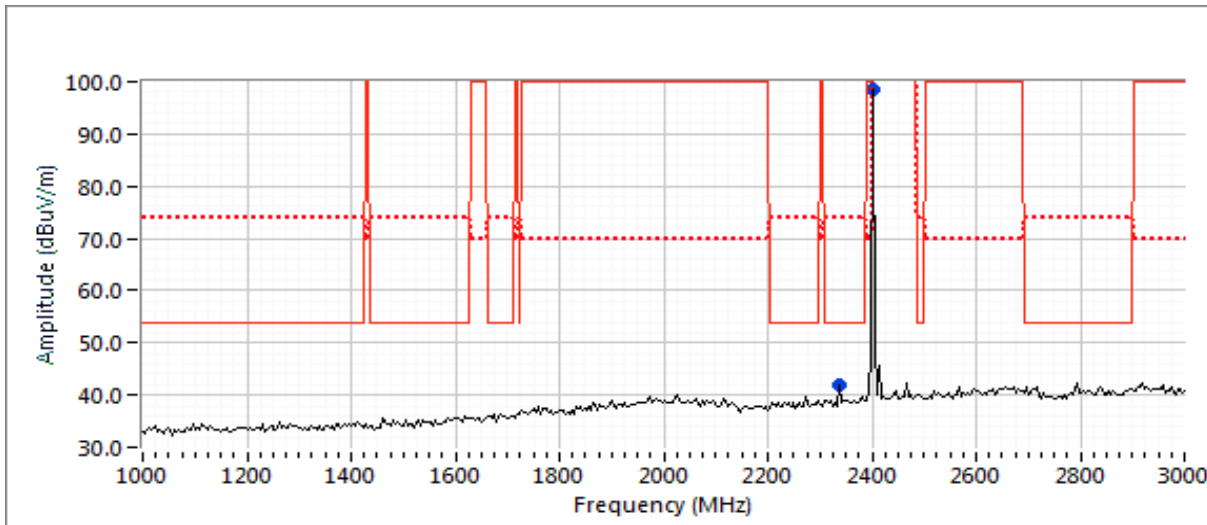



# EMC Test Data



Client:	Enovate Medical	Job Number:	PR106495
Model:	A0001923	T-Log Number:	TL106495-RANA
Contact:	Steven Godbey	Project Manager:	Deepa Shetty
Standard:	FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator:	Deniz Demirci
		Class:	N/A

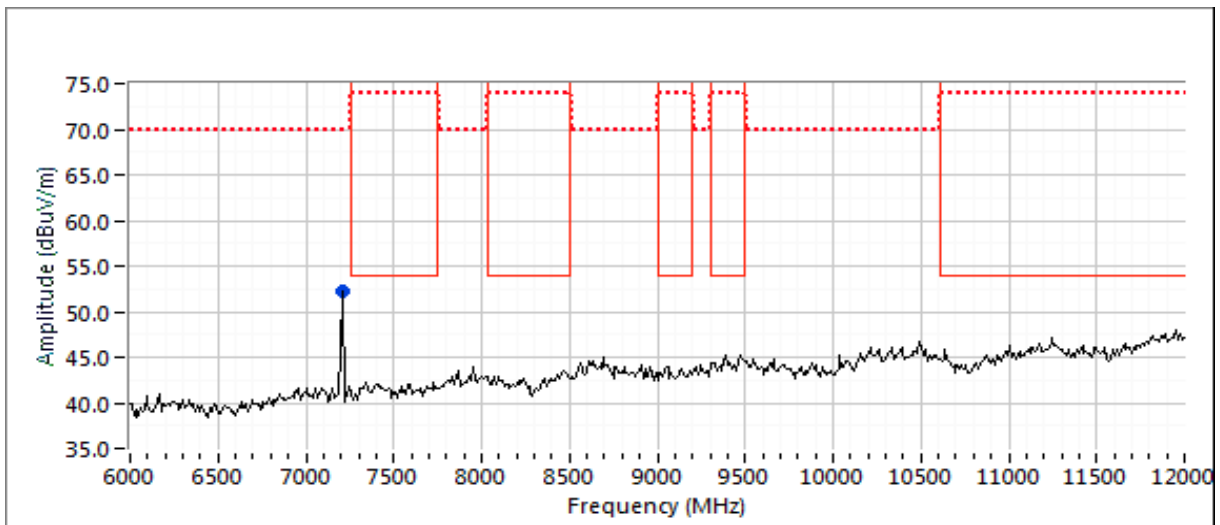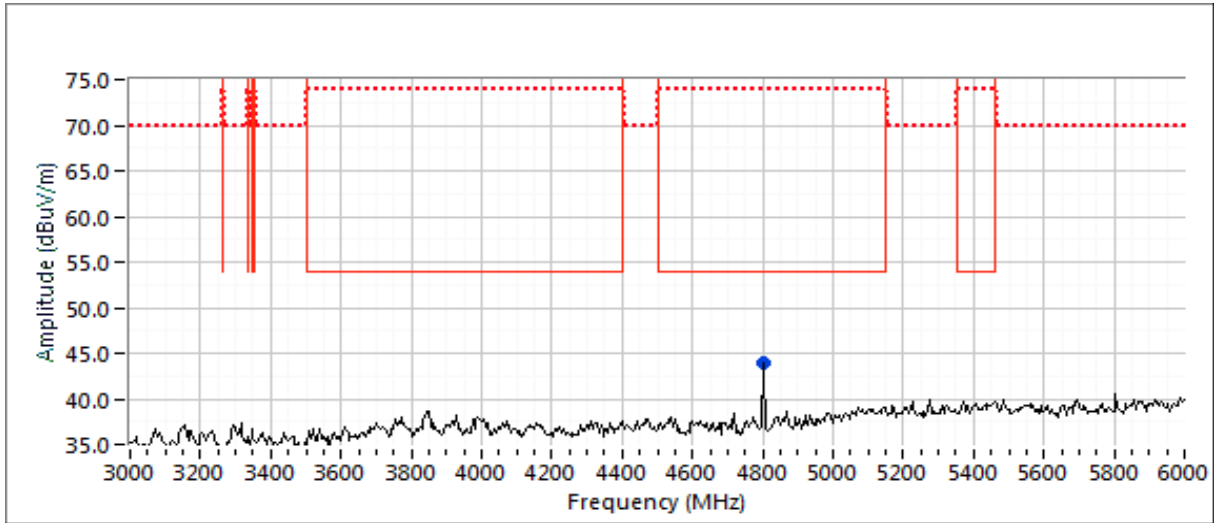



# EMC Test Data

Client:	Enovate Medical	Job Number:	PR106495
Model:	A0001923	T-Log Number:	TL106495-RANA
Contact:	Steven Godbey	Project Manager:	Deepa Shetty
Standard:	FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator:	Deniz Demirci
		Class:	N/A

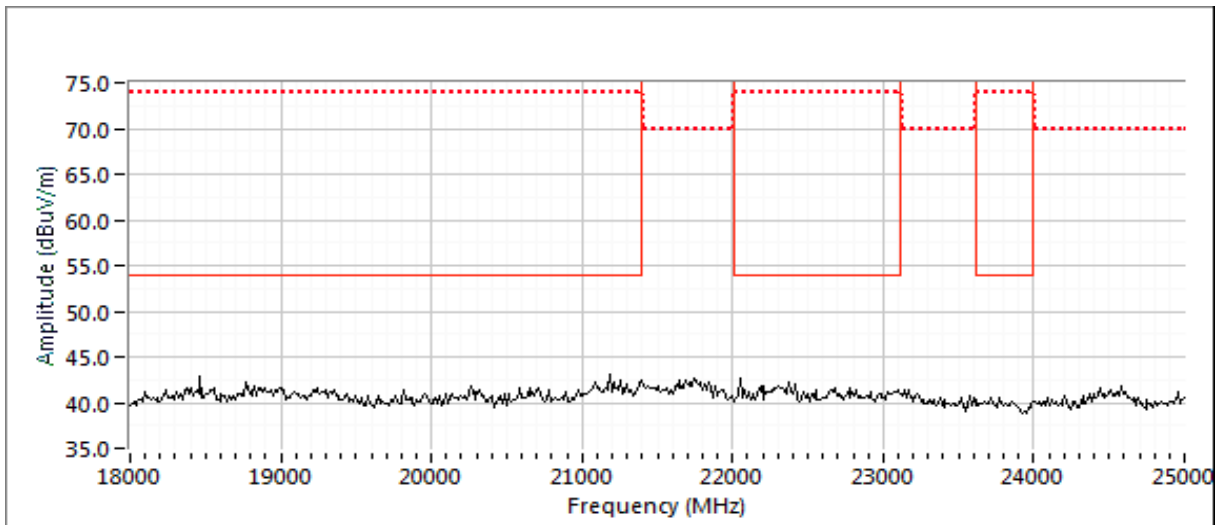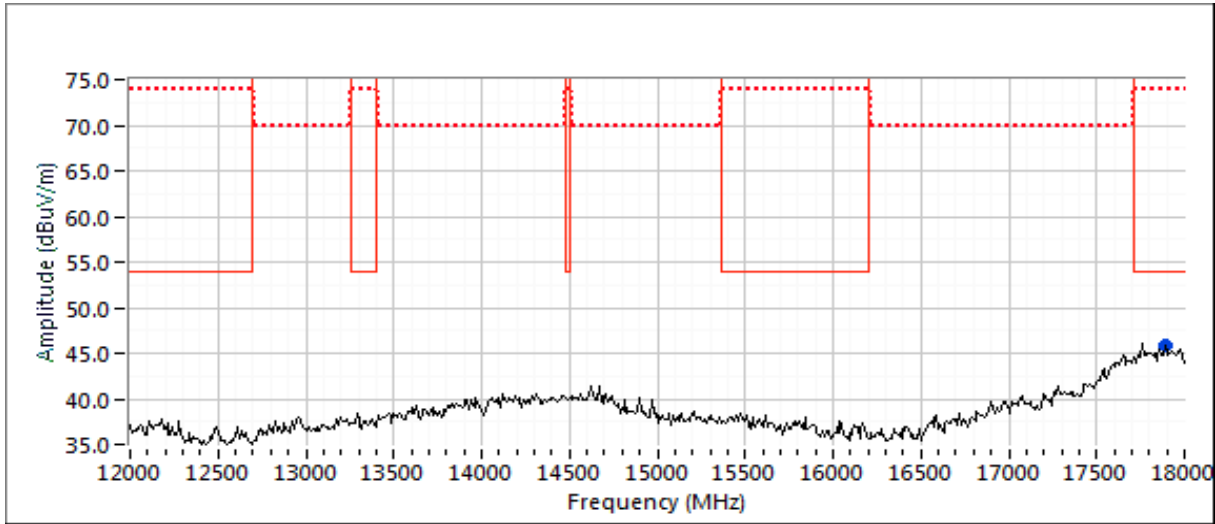




# EMC Test Data

Client:	Enovate Medical	Job Number:	PR106495
Model:	A0001923	T-Log Number:	TL106495-RANA
Contact:	Steven Godbey	Project Manager:	Deepa Shetty
Standard:	FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator:	Deniz Demirci
		Class:	N/A

## Run #1b: Center Channel

Channel: 17 - 2440 MHz      Mode: BLE  
 Tx Chain: Main              Data Rate: 1 Mbps



Frequency MHz	Level dB $\mu$ V/m	Pol v/h	15.209 / 15.247		Detector Pk/QP/Avg	Azimuth degrees	Height meters	Comments
			Limit	Margin				
2440.010	97.9	H	-	-	PK	165	2.1	POS; RB 3 MHz; VB: 10 MHz
4879.980	42.1	H	54.0	-11.9	AVG	230	1.2	Note 6 - RB 1 MHz;VB 1 kHz;Peak
4880.010	50.8	H	74.0	-23.2	PK	230	1.2	RB 1 MHz;VB 3 MHz;Peak
7320.050	49.7	H	54.0	-4.3	AVG	184	2.1	Note 6 - RB 1 MHz;VB 1 kHz;Peak
7320.750	57.9	H	74.0	-16.1	PK	184	2.1	RB 1 MHz;VB 3 MHz;Peak
17890.000	46.4	H	74.0	-27.6	Peak	285	2.0	Noise floor reading

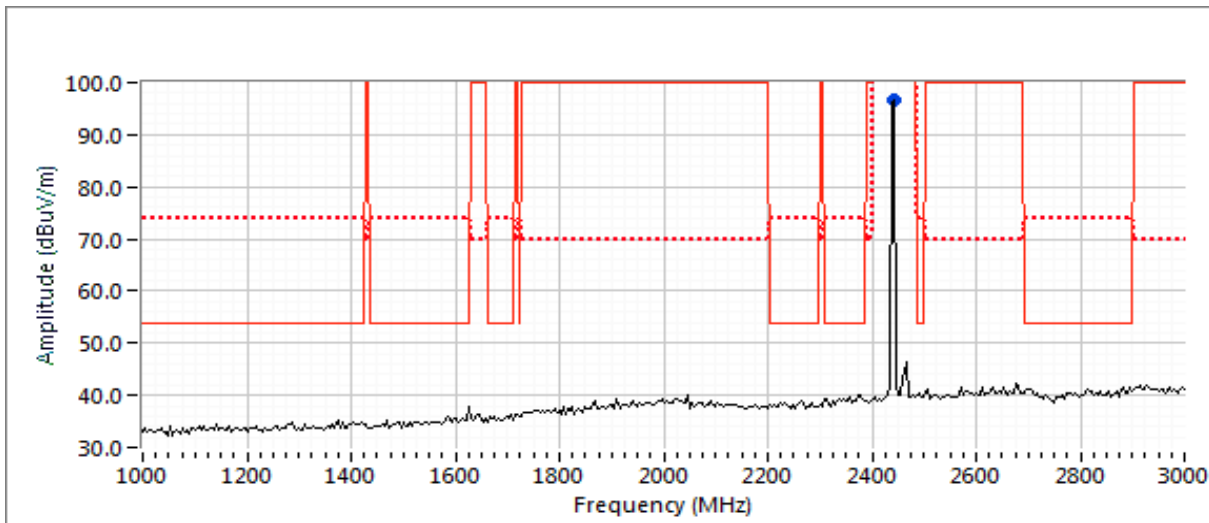



# EMC Test Data



Client:	Enovate Medical	Job Number:	PR106495
Model:	A0001923	T-Log Number:	TL106495-RANA
Contact:	Steven Godbey	Project Manager:	Deepa Shetty
Standard:	FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator:	Deniz Demirci
		Class:	N/A

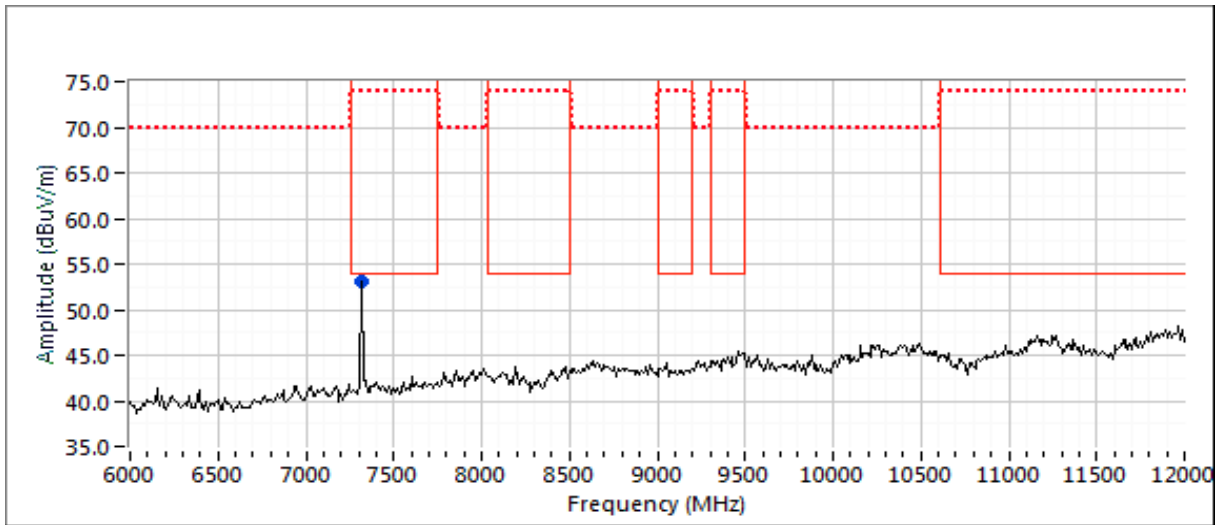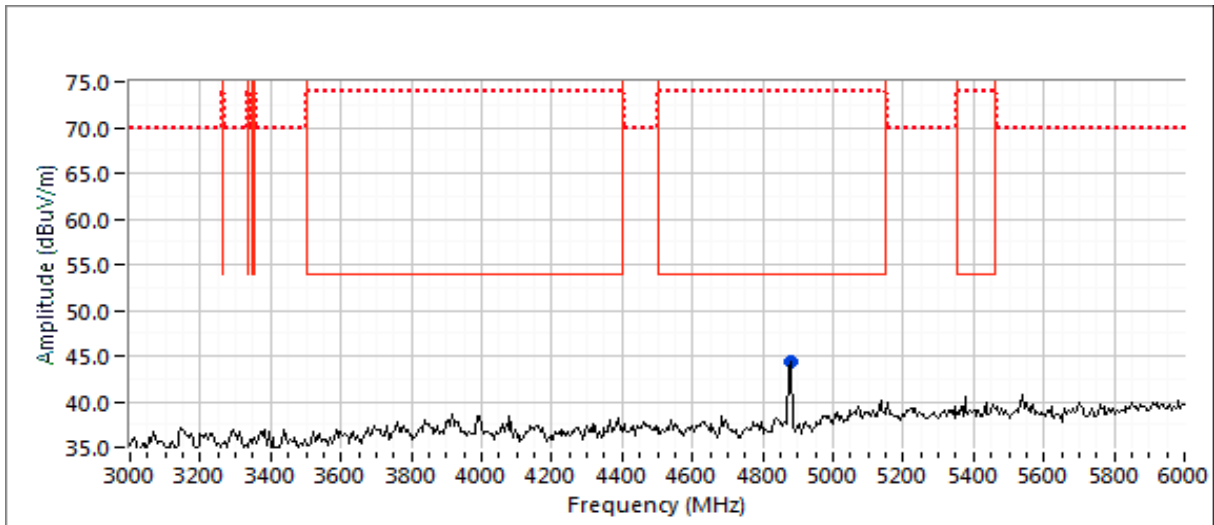



# EMC Test Data

Client:	Enovate Medical	Job Number:	PR106495
Model:	A0001923	T-Log Number:	TL106495-RANA
Contact:	Steven Godbey	Project Manager:	Deepa Shetty
Standard:	FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator:	Deniz Demirci
		Class:	N/A

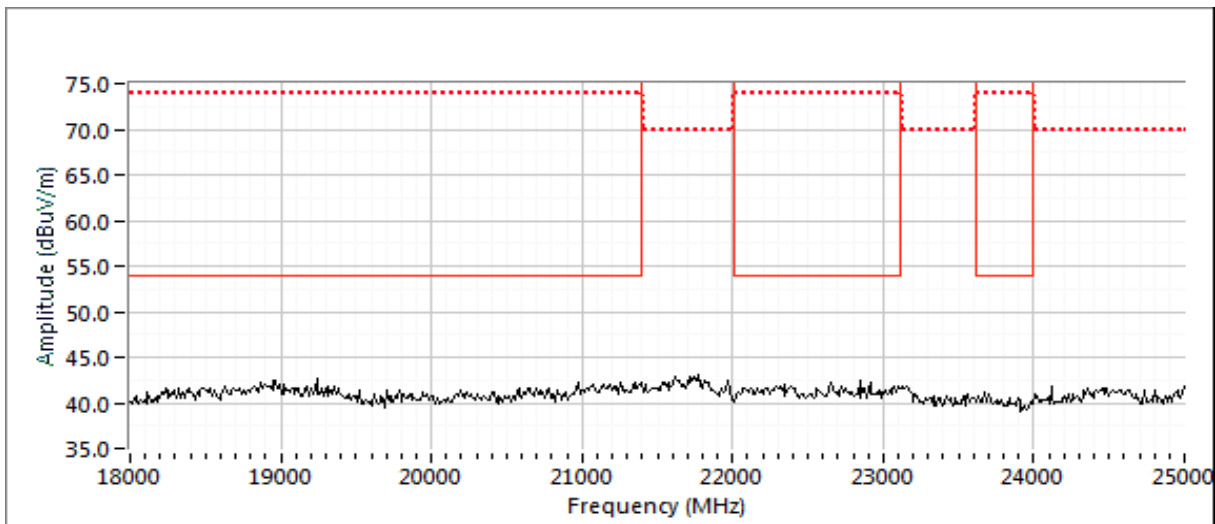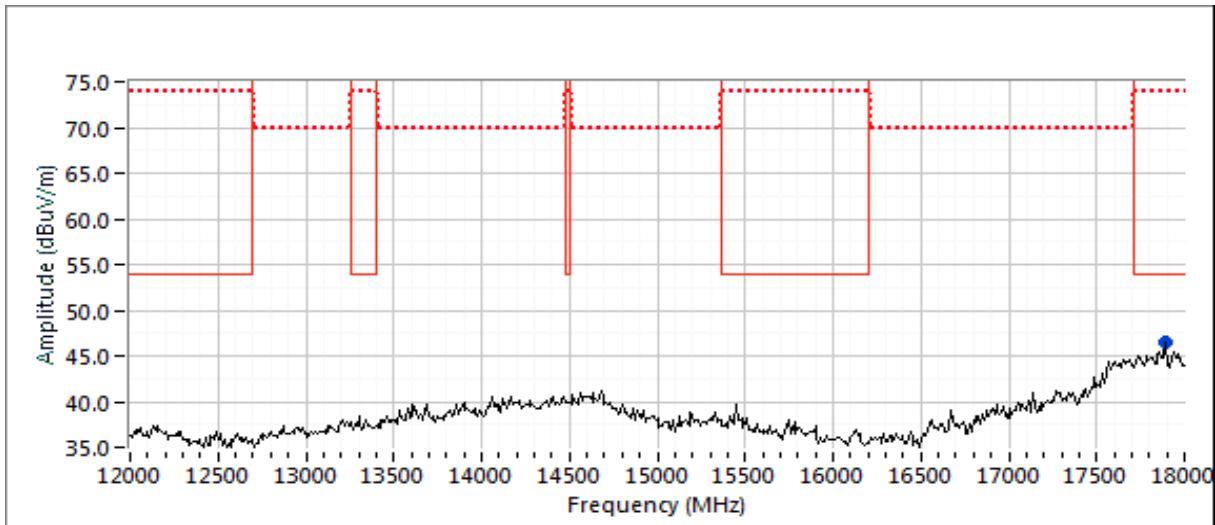




# EMC Test Data

Client: Enovate Medical	Job Number: PR106495
Model: A0001923	T-Log Number: TL106495-RANA
Contact: Steven Godbey	Project Manager: Deepa Shetty
Standard: FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator: Deniz Demirci
	Class: N/A

## Run #1c: High Channel

Channel: 39 - 2480 MHz      Mode: BLE  
 Tx Chain: Main              Data Rate: 1 Mbps

Frequency MHz	Level dB $\mu$ V/m	Pol v/h	15.209 / 15.247		Detector Pk/QP/Avg	Azimuth degrees	Height meters	Comments
			Limit	Margin				
2479.990	97.7	H	-	-	PK	160	1.5	POS; RB 3 MHz; VB: 10 MHz
4960.020	42.2	V	54.0	-11.8	AVG	151	2.0	Note 6 - RB 1 MHz;VB 1 kHz;Peak
4960.520	50.5	V	74.0	-23.5	PK	151	2.0	RB 1 MHz;VB 3 MHz;Peak
7440.040	48.4	H	54.0	-5.6	AVG	184	2.3	Note 6 - RB 1 MHz;VB 1 kHz;Peak
7439.470	56.7	H	74.0	-17.3	PK	184	2.3	RB 1 MHz;VB 3 MHz;Peak
17850.000	46.0	V	74.0	-28.0	Peak	111	1.5	Noise floor reading


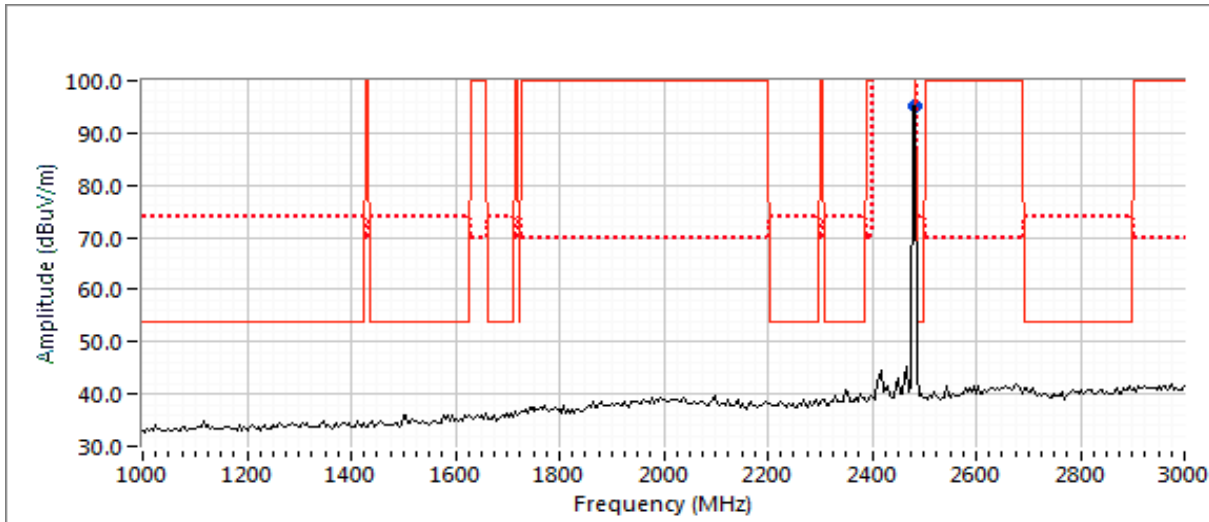






# EMC Test Data



Client:	Enovate Medical	Job Number:	PR106495
Model:	A0001923	T-Log Number:	TL106495-RANA
Contact:	Steven Godbey	Project Manager:	Deepa Shetty
Standard:	FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator:	Deniz Demirci
		Class:	N/A

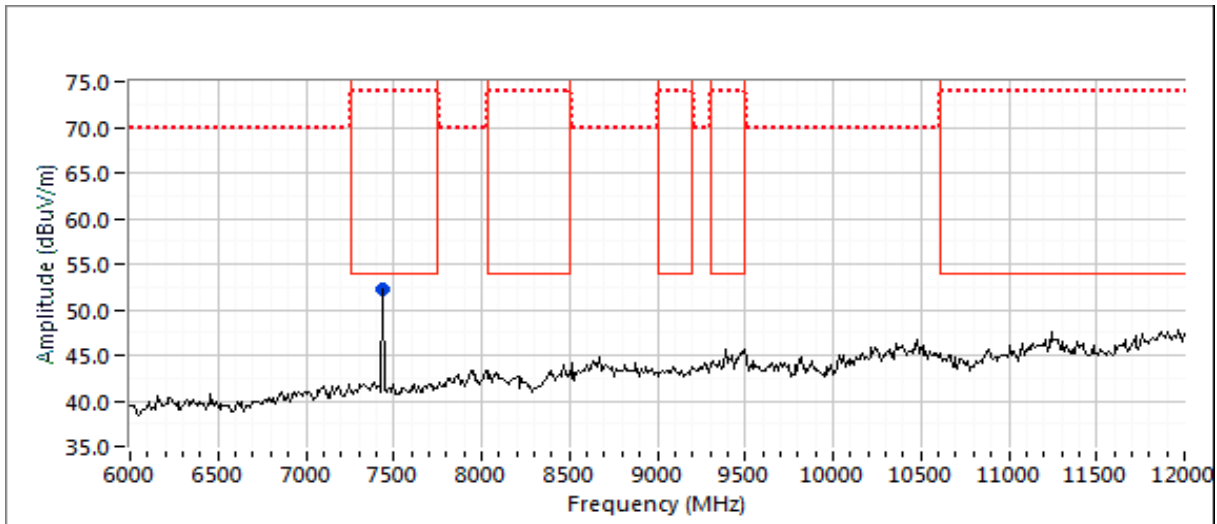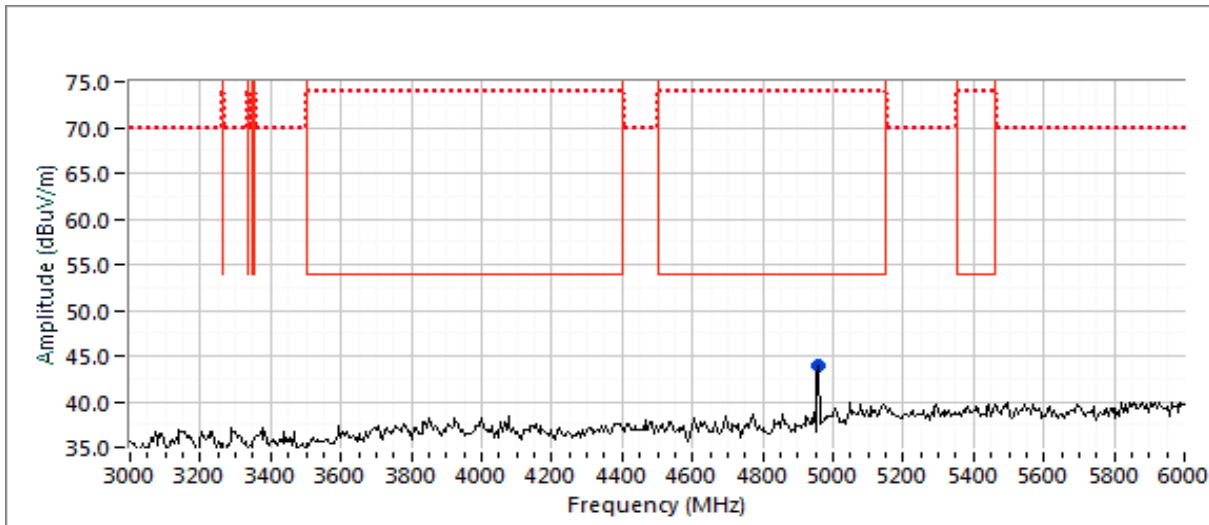



# EMC Test Data

Client:	Enovate Medical	Job Number:	PR106495
Model:	A0001923	T-Log Number:	TL106495-RANA
Contact:	Steven Godbey	Project Manager:	Deepa Shetty
Standard:	FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator:	Deniz Demirci
		Class:	N/A

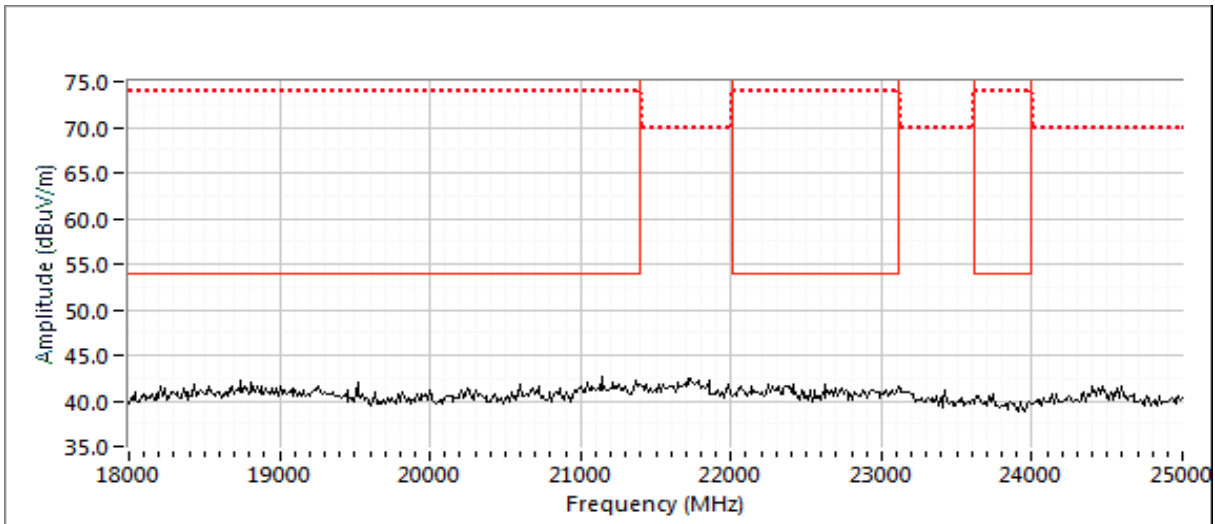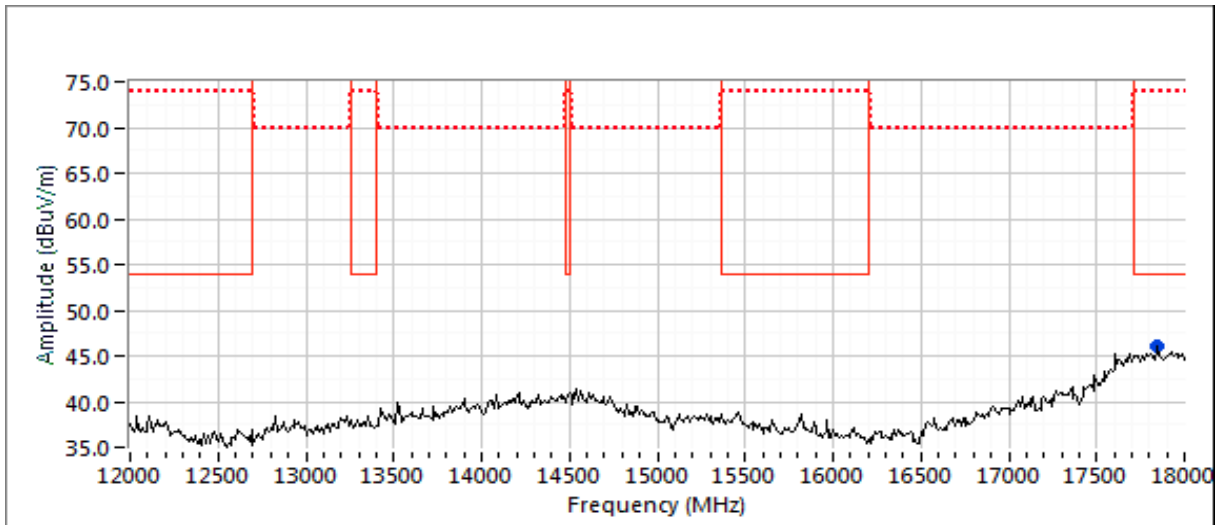



# EMC Test Data

Client:	Enovate Medical	Job Number:	PR106495
Model:	A0001923	T-Log Number:	TL106495-RANA
Contact:	Steven Godbey	Project Manager:	Deepa Shetty
Standard:	FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator:	Deniz Demirci
		Class:	N/A


Run #2: Radiated Spurious Emissions, Restricted band edge.

Run #2a: Low Channel

Channel: 37 - 2402 MHz      Mode: BLE  
 Tx Chain: Main              Data Rate: 1 Mbps

### Band Edge

Frequency	Level	Pol	15.209 / 15.247		Detector	Azimuth	Height	Comments
MHz	dB $\mu$ V/m	v/h	Limit	Margin	Pk/QP/Avg	degrees	meters	
2375.250	35.7	H	54.0	-18.3	AVG	165	2.5	Note 6 - RB 1 MHz; VB: 500 Hz
2389.440	55.5	H	74.0	-18.5	PK	165	2.5	POS; RB 1 MHz; VB: 3 MHz
2354.490	32.3	V	54.0	-21.7	AVG	137	2.1	POS; RB 1 MHz; VB: 500 Hz
2382.950	47.4	V	74.0	-26.6	PK	137	2.1	POS; RB 1 MHz; VB: 3 MHz

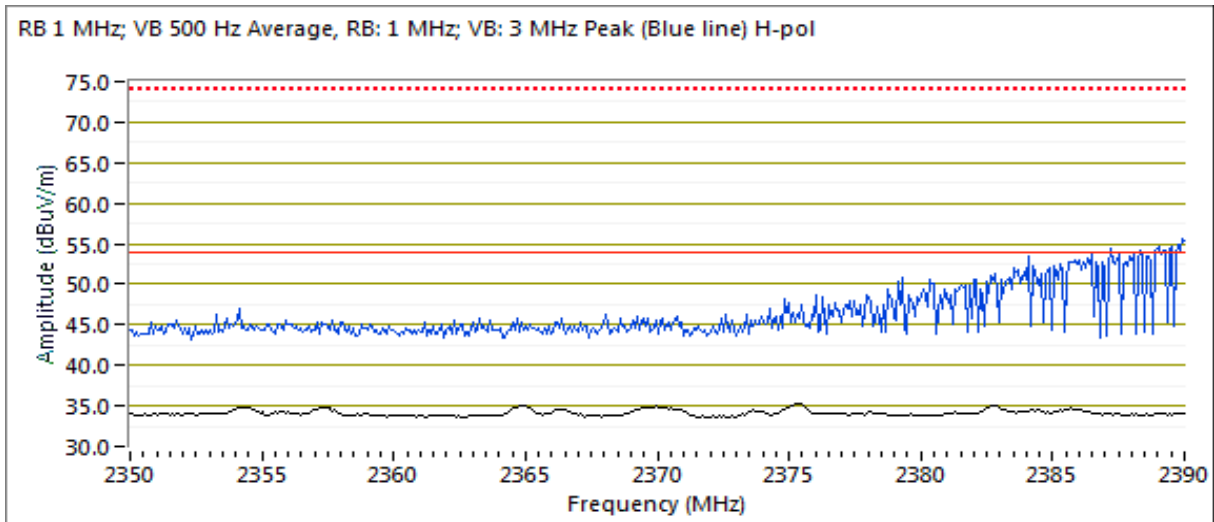



# EMC Test Data


Client:	Enovate Medical	Job Number:	PR106495
Model:	A0001923	T-Log Number:	TL106495-RANA
Contact:	Steven Godbey	Project Manager:	Deepa Shetty
Standard:	FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator:	Deniz Demirci
		Class:	N/A

## Run #2b: High Channel

Channel: 39 - 2480 MHz      Mode: BLE  
 Tx Chain: Main              Data Rate: 1 Mbps

## Band Edge

Frequency MHz	Level dB $\mu$ V/m	Pol v/h	15.209 / 15.247		Detector Pk/QP/Avg	Azimuth degrees	Height meters	Comments
			Limit	Margin				
2483.510	37.1	H	54.0	-16.9	AVG	153	1.3	Note 6 - RB 1 MHz; VB: 500 Hz
2483.600	57.1	H	74.0	-16.9	PK	153	1.3	POS; RB 1 MHz; VB: 3 MHz
2483.630	34.3	V	54.0	-19.7	AVG	0	1.1	Note 6 - RB 1 MHz; VB: 500 Hz
2484.040	48.2	V	74.0	-25.8	PK	0	1.1	POS; RB 1 MHz; VB: 3 MHz

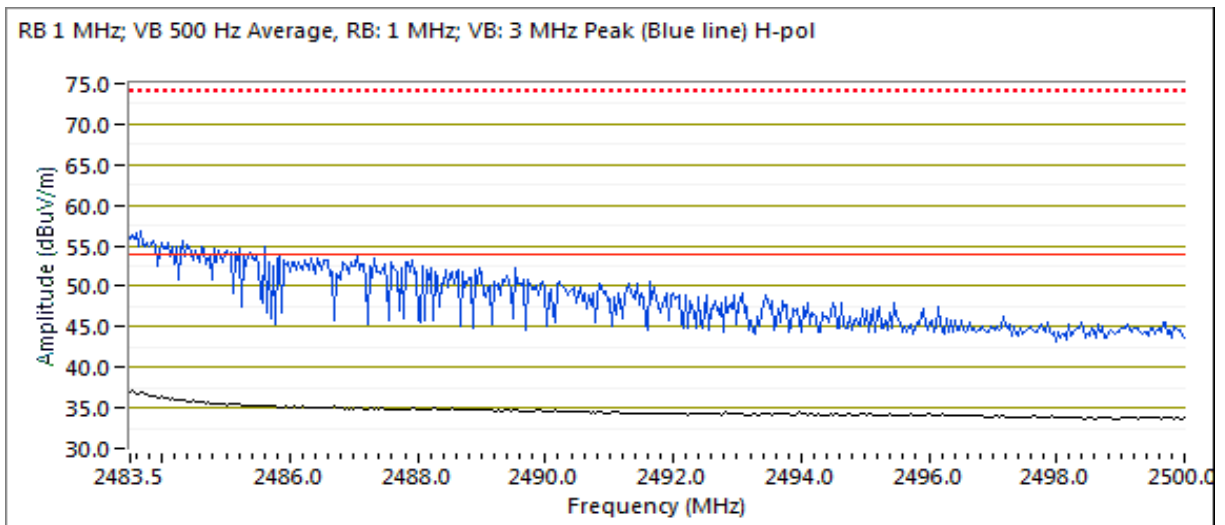



# EMC Test Data

Client: Enovate Medical	Job Number: PR106495
Model: A0001923	T-Log Number: TL106495-RANA
	Project Manager: Deepa Shetty
Contact: Steven Godbey	Project Coordinator: Deniz Demirci
Standard: FCC 15.247, RSS 247, FCC 15B, ICES-003	Class: N/A

## RSS-247 and FCC 15.247 (DTS) Radiated Spurious Emissions

### Test Specific Details

Objective: The objective of this test session is to perform final qualification testing of the EUT with respect to the specification listed above.

Date of Test: 1/6/2020	Config. Used: 1
Test Engineer: M. Birgani	Config Change: -
Test Location: Chamber #4	EUT Voltage: Battery

### General Test Configuration

The EUT was located on the turntable for radiated emissions testing. No support equipment was used  
The test distance and extrapolation factor (if used) are detailed under each run description.

Ambient Conditions:	Temperature: 22-24 °C
	Rel. Humidity: 40-42 %

### Summary of Results

Run #		Test Performed			Limit	Result	Margin
Run #	Mode	Channel	Target Power	Power Setting	Test Performed	Limit	Result / Margin
1	BLE	17 2440 MHz	0 dBm	1	Radiated Emissions, 9 kHz - 1 GHz	FCC Part 15.209	26.5 dBµV/m @ 79.58 MHz (-13.5 dB)

### Modifications Made During Testing

No modifications were made to the EUT during testing

### Deviations From The Standard

No deviations were made from the requirements of the standard.

### Sample Notes

Sample S/N: 311761516030250  
 Driver: Minicom  
 Antenna: Integral



Frequency Range	Test Distance	Limit Distance	Extrapolation Factor
0.009 - 0.490 MHz	3	300	-80.0
0.490 - 30.0 MHz	3	30	-40.0
30 - 1000 MHz	3	3	0.0



# EMC Test Data

Client: Enovate Medical	Job Number: PR106495
Model: A0001923	T-Log Number: TL106495-RANA
Contact: Steven Godbey	Project Manager: Deepa Shetty
Standard: FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator: Deniz Demirci
	Class: N/A

## Run #1: Radiated Emissions, 9 kHz - 1000 MHz, FCC 15.209

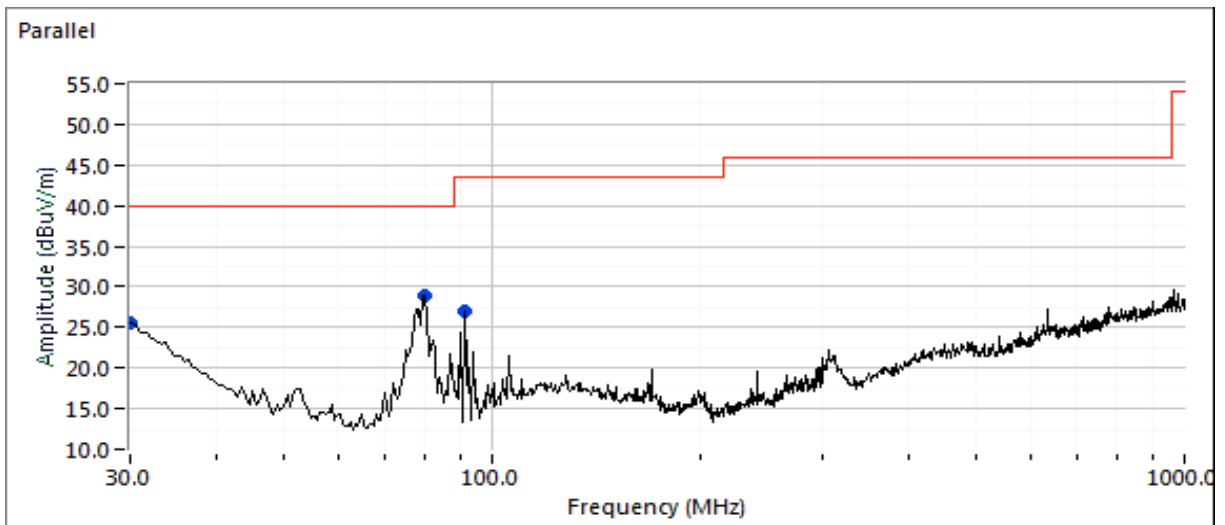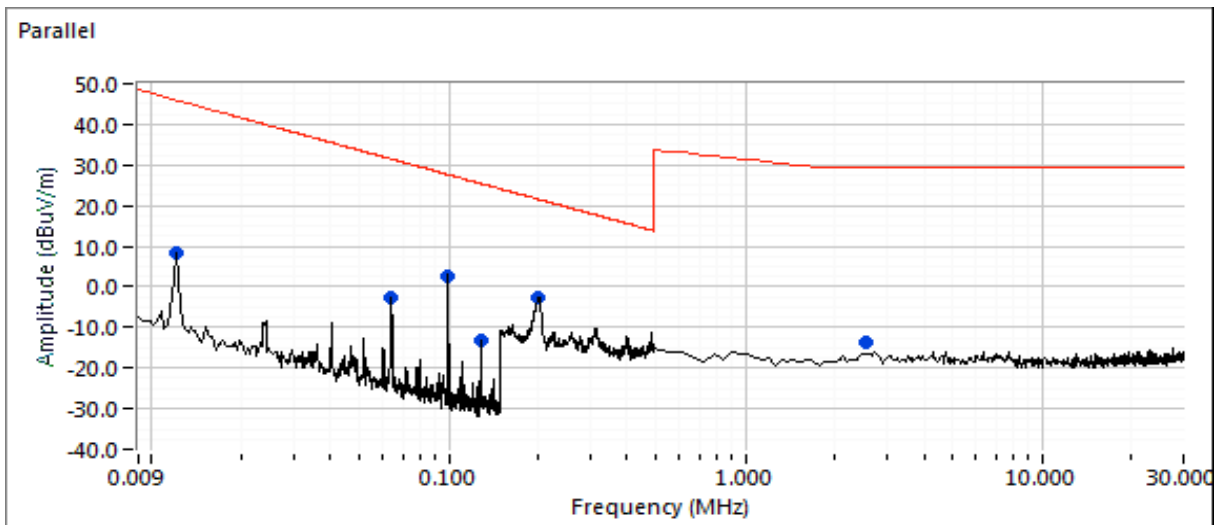



# EMC Test Data

Client:	Enovate Medical	Job Number:	PR106495
Model:	A0001923	T-Log Number:	TL106495-RANA
Contact:	Steven Godbey	Project Manager:	Deepa Shetty
Standard:	FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Coordinator:	Deniz Demirci
		Class:	N/A

## Run #1: Radiated Emissions, 9 kHz - 1000 MHz, FCC 15.209

Frequency MHz	Level dB $\mu$ V/m	Pol V/H	FCC 15.209		Detector Pk/QP/Avg	Azimuth degrees	Height meters	Comments
			Limit	Margin				
79.582	26.5	V	40.0	-13.5	QP	290	1.0	QP (1.00s)
2.560	-13.7	H	0.0	-13.7	Peak	65	1.3	Peak reading with QP limit
30.818	20.5	H	40.0	-19.5	QP	199	1.0	QP (1.00s)
0.200	-2.5	H	21.6	-24.1	Peak	20	1.3	Peak reading with QP limit
0.100	2.5	H	27.6	-25.1	Peak	122	1.3	Peak reading with QP limit
91.106	10.5	H	43.5	-33.0	QP	100	1.0	QP (1.00s)
0.064	-2.5	H	31.5	-34.0	Peak	122	1.3	Peak reading with QP limit
0.012	8.4	H	45.9	-37.5	Peak	122	1.3	Peak reading with QP limit
0.128	-13.1	H	25.4	-38.5	Peak	122	1.3	Peak reading with QP limit

Note 1:	Preliminary measurements indicates that measured emissions are not related to the transmit channel.
Note 4:	EUT was pre-scanned in all 3 orientations. Pre-scan results show EUT upright orientation has the highest spurious emission. Final measurements were taken with EUT upright orientation.



# EMC Test Data

Client:	Enovate Medical	PR Number:	PR106495
Model:	A0001923	T-Log Number:	TL106495-RANA
Contact:	Steven Godbey	Project Manager:	Deepa Shetty
Standard:	FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Engineer:	Deniz Demirci
		Class:	B

## Conducted Emissions

*(NTS Silicon Valley, Fremont Facility, Semi-Anechoic Chamber)*

### Test Specific Details

Objective: The objective of this test session is to perform final qualification testing of the EUT with respect to the specification listed above.

Date of Test: 1/7/2020  
 Test Engineer: M. Birgani  
 Test Location: Chamber #4

Config. Used: 3  
 Config Change: -  
 EUT Voltage: 120 V/60 Hz

### General Test Configuration

For tabletop equipment, the EUT was located on a table inside the semi-anechoic chamber, 40 cm from a vertical coupling plane and 80 cm from the LISN. No remote support equipment was used.

Ambient Conditions:                      Temperature:        22-24 °C  
    Rel. Humidity:      40-42 %

### Summary of Results

Run #	Test Performed	Limit	Result	Margin
1	CE, AC Power 120 V/60 Hz	Class B	Pass	47.9 dBµV @ 0.184 MHz (-6.4 dB)

### Modifications Made During Testing

No modifications were made to the EUT during testing

### Deviations From The Standard

No deviations were made from the requirements of the standard.







# EMC Test Data

Client: Enovate Medical	PR Number: PR106495
Model: A0001923	T-Log Number: TL106495-RANA
Contact: Steven Godbey	Project Manager: Deepa Shetty
Standard: FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Engineer: Deniz Demirci
	Class: B

Run #1: AC Power Port Conducted Emissions, 0.15 - 30 MHz, 120 V/60 Hz

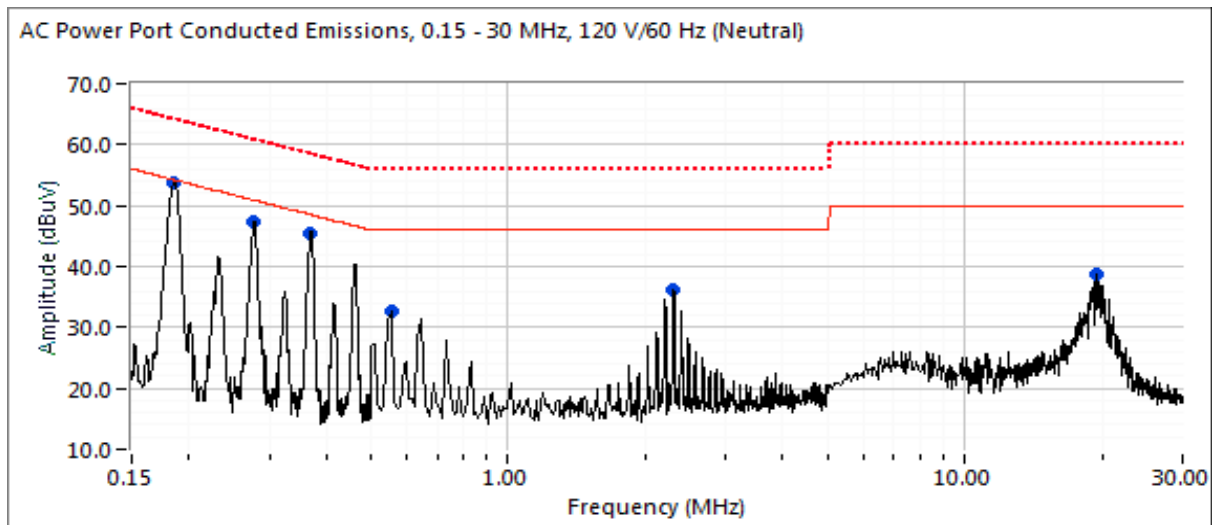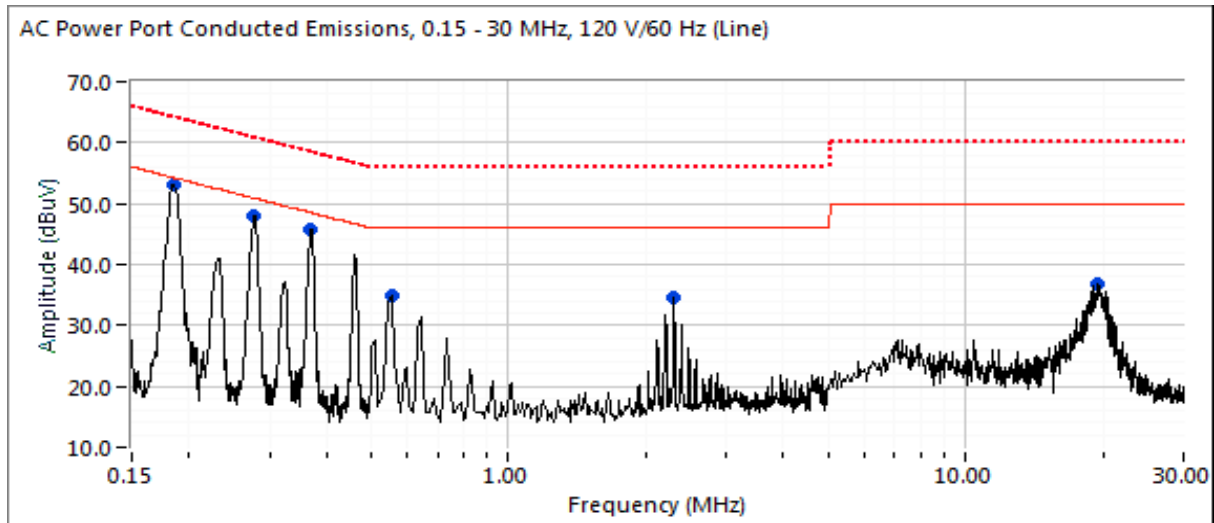



# EMC Test Data

Client:	Enovate Medical	PR Number:	PR106495
Model:	A0001923	T-Log Number:	TL106495-RANA
Contact:	Steven Godbey	Project Manager:	Deepa Shetty
Standard:	FCC 15.247, RSS 247, FCC 15B, ICES-003	Project Engineer:	Deniz Demirci
		Class:	B

Run #1: AC Power Port Conducted Emissions, 0.15 - 30 MHz, 120 V/60 Hz  
 Preliminary peak readings captured during pre-scan (peak readings vs. average limit)

Frequency MHz	Level dB $\mu$ V	AC Line	Class B		Detector QP/Ave	Comments
			Limit	Margin		
0.185	53.8	Neutral	54.2	-0.4	Peak	
0.184	53.0	Line	54.2	-1.2	Peak	
0.369	45.8	Line	48.5	-2.7	Peak	
0.277	48.1	Line	50.9	-2.8	Peak	
0.367	45.5	Neutral	48.5	-3.0	Peak	
0.277	47.3	Neutral	50.9	-3.6	Peak	
2.305	36.3	Neutral	46.0	-9.7	Peak	
0.549	35.0	Line	46.0	-11.0	Peak	
19.439	38.6	Neutral	50.0	-11.4	Peak	
2.300	34.6	Line	46.0	-11.4	Peak	

### Final quasi-peak and average readings

Frequency MHz	Level dB $\mu$ V	AC Line	Class B		Detector QP/Ave	Comments
			Limit	Margin		
0.184	47.9	Line	54.3	-6.4	AVG	AVG (0.10s)
0.185	46.8	Neutral	54.2	-7.4	AVG	AVG (0.10s)
0.367	39.6	Neutral	48.6	-9.0	AVG	AVG (0.10s)
0.277	41.7	Line	50.9	-9.2	AVG	AVG (0.10s)
0.369	39.3	Line	48.5	-9.2	AVG	AVG (0.10s)
0.277	41.7	Neutral	50.9	-9.2	AVG	AVG (0.10s)
0.185	53.0	Neutral	64.2	-11.2	QP	QP (1.00s)
0.184	52.8	Line	64.3	-11.5	QP	QP (1.00s)
0.277	47.9	Line	60.9	-13.0	QP	QP (1.00s)
0.369	44.4	Line	58.5	-14.1	QP	QP (1.00s)
0.277	46.7	Neutral	60.9	-14.2	QP	QP (1.00s)
0.367	44.4	Neutral	58.6	-14.2	QP	QP (1.00s)
2.305	27.0	Neutral	46.0	-19.0	AVG	AVG (0.10s)
2.300	26.8	Line	46.0	-19.2	AVG	AVG (0.10s)
2.305	35.3	Neutral	56.0	-20.7	QP	QP (1.00s)
0.549	24.4	Line	46.0	-21.6	AVG	AVG (0.10s)
2.300	32.7	Line	56.0	-23.3	QP	QP (1.00s)
0.549	30.6	Line	56.0	-25.4	QP	QP (1.00s)
19.439	29.6	Neutral	60.0	-30.4	QP	QP (1.00s)
19.439	16.5	Neutral	50.0	-33.5	AVG	AVG (0.10s)

***End of Report***

This page is intentionally blank and marks the last page of this test report.