

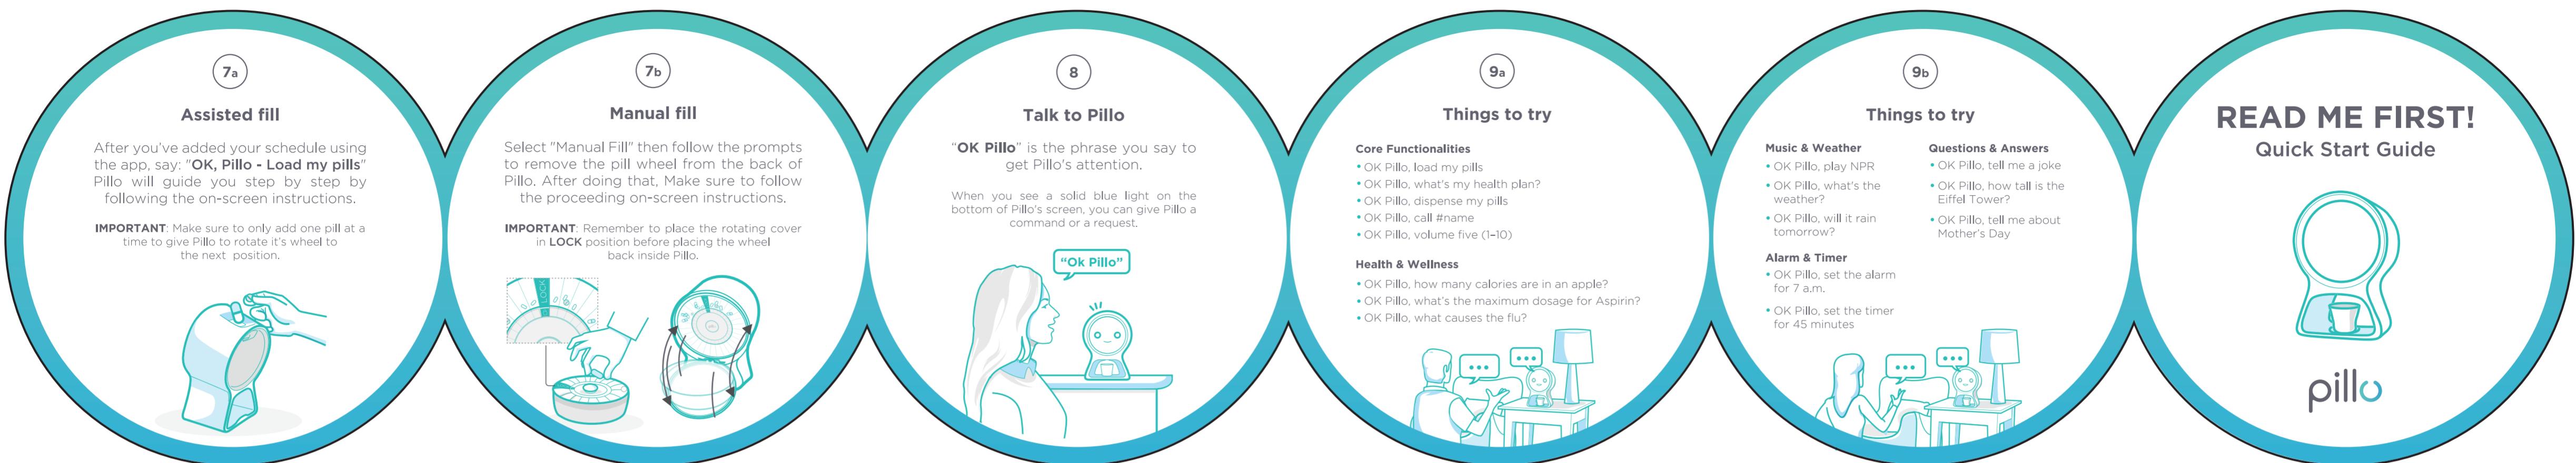


FRONT

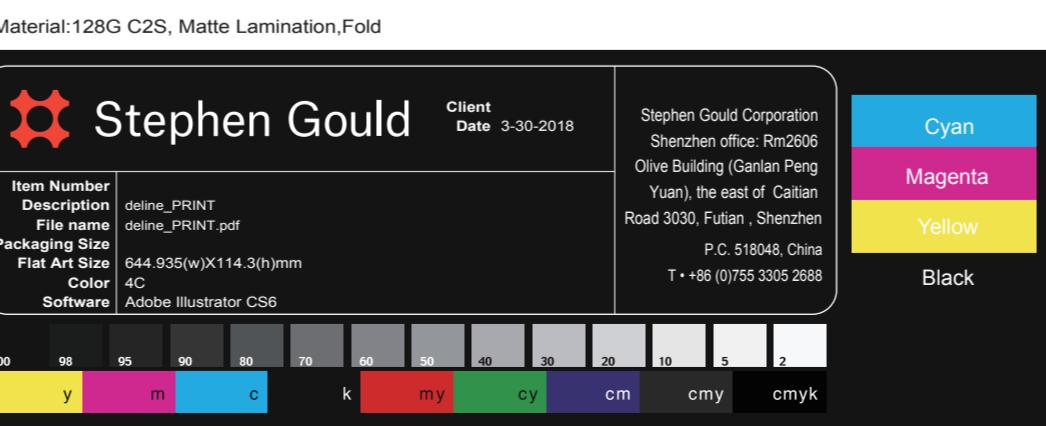

BACK

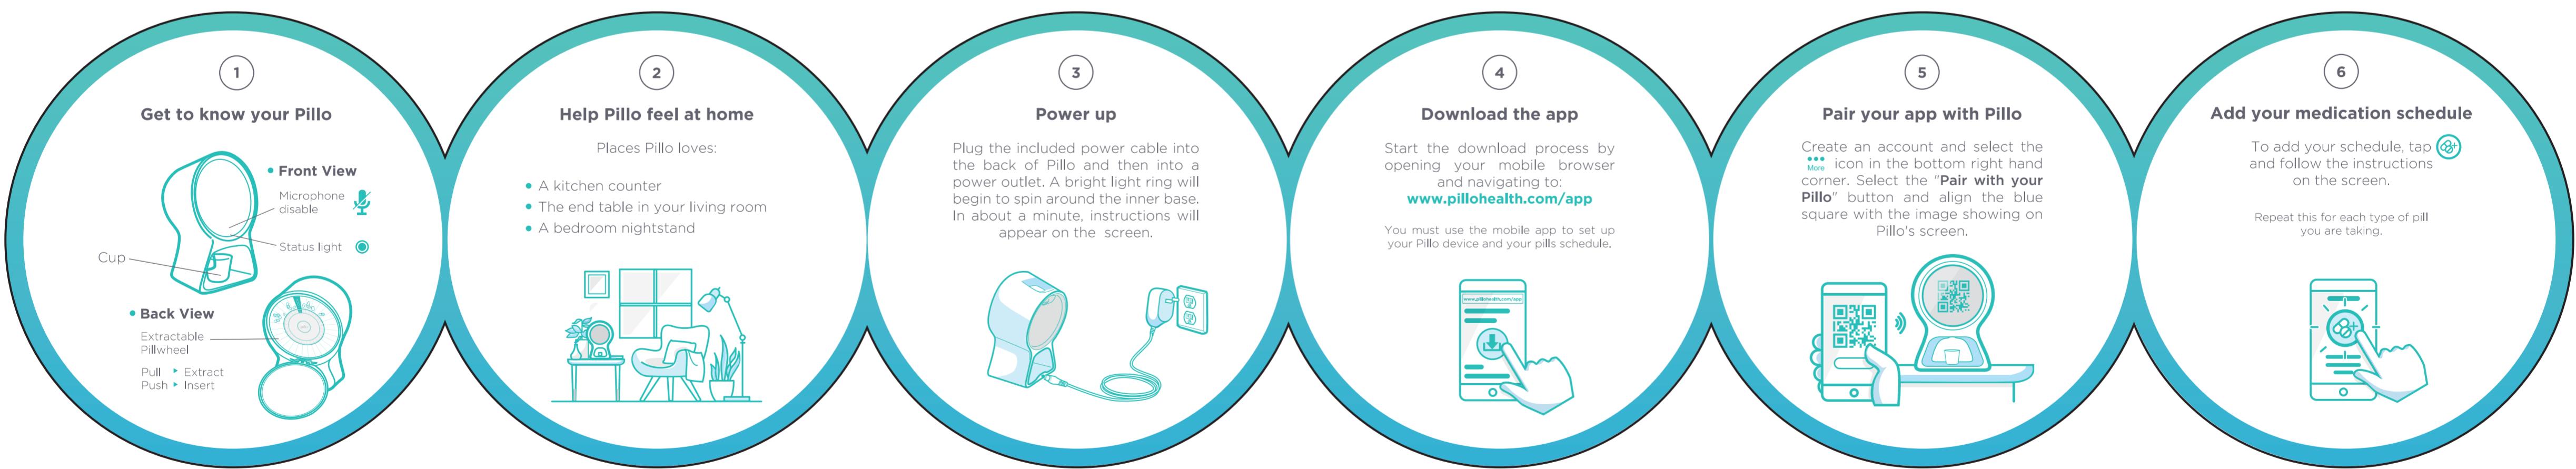

Model: S-EM010



INTENDED USE STATEMENT

The Pillo Medication Reminder and Dispenser System is intended for the medical purposes of:
a) providing alerts to the user, patients, or healthcare providers for pre-determined medication and nutritional supplement dosing schedules, and b) dispensing the appropriate oral dosage forms (pills, capsules, etc.) of solid medication and nutritional supplements.

SAFETY INFORMATION

1. Do not let power supply cord touch hot surfaces.
2. Do not mount near gas or electric heaters.
3. The use of accessory equipment not recommended by the manufacturer may cause an unsafe condition and void product warranty.
4. Do not use for other than intended purpose.
5. All servicing should be performed by qualified service personnel.
6. This device is not intended to be a diagnostic device.
7. Always check dispensed medication dose for accuracy.
8. Read all the information in the instruction manual and any other literature in the box before operating the unit.
9. To reduce the risk of injury keep hands off moving parts when in motion.
10. Wash pill-wheel and cup using water and soap, do not place in a dishwasher.

CAUTION

Do not overload power outlets. Plug the device into the appropriate voltage outlet.

⚠️ WARNING

Do not remove battery.

Do not plug or unplug the power cord into the electrical outlet with wet hands.

Equipment should be mounted in locations and at heights where the camera has enough field of view to allow face detection and where the camera has enough light to operate.

FCC STATEMENT

FCC ID: 2AQK6S-EM010

This device complies with part 15 of the FCC rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

NOTE: The manufacturer is not responsible for any radio or TV interference caused by unauthorized modifications or changes to this equipment. Such modifications or changes could void the user's authority to operate the equipment. **NOTE:** This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

FCC caution

Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

Important note

When using the product, maintain a distance of 20 cm from the body to ensure compliance with RF exposure requirements.

Industry Canada

This device complies with Industry Canada licence-exempt RSS standard(s). Operation is Subject to the following two conditions: (1) this device may not cause interference, and (2) this device must accept any interference, including interference that may cause undesired operation of the device.

Le présent appareil est conforme aux CNR d'Industrie Canada applicables aux appareils radio exempts de licence. L'exploitation est autorisée aux deux conditions suivantes : (1) l'appareil ne doit pas produire de brouillage, et (2) l'utilisateur de l'appareil doit accepter tout brouillage radioélectrique subi, même si le brouillage est susceptible d'en compromettre le fonctionnement.