

Report No: CCISE181212901

FCC SAR REPORT

Applicant:	Amcrest Industries LLC		
Address of Applicant:	16727 Park Row Dr. Houston, TX 77084 USA		
Equipment Under Test (E	EUT)		
Product Name:	Baby Monitor		
Model No.:	AC-2-M		
FCC ID:	2AR53AC2M		
Applicable standards:	FCC 47 CFR Part 2.1093		
Date of Test:	27 Dec., 2018 ~ 27 Dec., 2018		
Test Result:	Maximum Reported 1-g SAR (W/kg) Body: 0.652		

Authorized Signature:



Bruce Zhang Laboratory Manager

This report details the results of the testing carried out on one sample. The results contained in this test report do not relate to other samples of the same product and does not permit the use of the CCIS product certification mark. The manufacturer should ensure that all products in series production are in conformity with the product sample detailed in this report.

This report may only be reproduced and distributed in full. If the product in this report is used in any configuration other than that detailed in the report, the manufacturer must ensure the new system complies with all relevant standards.

This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.



2 Version

Version No.	Date	Description
00	27 Dec., 2018	Original

Prepared by:

Huheng Cai Report Clerk

27 Dec., 2018

Reviewed by:

Janet Wei Date:

Date:

27 Dec., 2018

Project Engineer

Project No.: CCISE1812129

CCIS

3		Contents	
1	С	OVER PAGE	1
2	v	/ERSION	2
3		CONTENTS	
4		SENERAL INFORMATION	
	4.1 4.2 4.3	CLIENT INFORMATION GENERAL DESCRIPTION OF EUT ENVIRONMENT OF TEST SITE	4
	4.4	TEST LOCATION	
5	IN	NTRODUCTION	6
	5.1 5.2	INTRODUCTION	
6	R	RESTART STATES STA	7
	6.1 6.2 6.3	UNCONTROLLED ENVIRONMENT CONTROLLED ENVIRONMENT RF Exposure Limits	7
7			
1	7.1 7.2 7.3	E-FIELD PROBE DATA ACQUISITION ELECTRONICS (DAE) ROBOT	9
	7.3 7.4	NOBUT	
	7.5	LIGHT BEAM UNIT	
	7.6 7.7	Phantom Device Holder	
	7.8	DATA STORAGE AND EVALUATION	
	7.9	TEST EQUIPMENT LIST	
8		ISSUE SIMULATING LIQUIDS	
9		AR SYSTEM VERIFICATION	
10	E	UT TESTING POSITION	
	10.1 10.2 10.3	BODY WORN ACCESSORY CONFIGURATIONS	20
11	M	IEASUREMENT PROCEDURES	
	11.1	SPATIAL PEAK SAR EVALUATION	22
	11.2		
	11.3 11.4		-
	11.5	SAR AVERAGED METHODS	24
	11.6		
13		SAR TEST RESULTS SUMMARY	
	13.1 13.2		
	13.2		
14	R	EFERENCE	30
AF	PEN	NDIX A: PLOTS OF SAR SYSTEM CHECK	31
AF	PEN	NDIX B: PLOTS OF SAR TEST DATA	33
AF	PEN	NDIX C: SYSTEM CALIBRATION CERTIFICATE	35





4 General Information

4.1 Client Information

Applicant:	Amcrest Industries LLC
Address of Applicant:	16727 Park Row Dr. Houston, TX 77084 USA
Manufacturer:	MeiZhou Guo Wei Electronics Co., Ltd.
	AD1 Section, Economic Development Area, Dongsheng Industrial District, Meizhou, Guangdong, China.)

4.2 General Description of EUT

Product Name:	Baby Monitor		
Model No.:	AC-2-M		
Category of device	Portable device		
Operation Frequency:	2402MHz~2480MHz	2402MHz~2480MHz	
Modulation technology:	GFSK		
Antenna Type:	Internal Antenna		
Antenna Gain:	2.0 dBi		
Dimensions (L*W*H):	137 mm (L)× 84 mm (W)×31 mm (H)		
Accessories information:	Adapter: Model: NBS05B059100VU Input: AC100-240V, 50/60Hz, 0.2A Output: DC 5.9V, 1.0A	Battery: Rechargeable Li-ion Battery 3.7V/1800mAh	



4.3 Environment of Test Site

Temperature:	18°C ~25 °C
Humidity:	35%~75% RH
Atmospheric Pressure:	1010 mbar

4.4 Test Location

Shenzhen Zhongjian Nanfang Testing Co., Ltd. Address: No. B-C, 1/F., Building 2, Laodong No.2 Industrial Park, Xixiang Road, Bao'an District, Shenzhen, Guangdong, China Tel: +86-755-23118282, Fax: +86-755-23116366 E-mail: info@ccis-cb.com



Report No: CCISE181212901

5 Introduction

5.1 Introduction

SAR is related to the rate at which energy is absorbed per unit mass in an object exposed to a radio field. The SAR distribution in a biological body is complicated and is usually carried out by experimental techniques or numerical modeling. The standard recommends limits for two tiers of groups, occupational/controlled and general population/uncontrolled, based on a person's awareness and ability to exercise control over his or her exposure. In general, occupational/controlled exposure limits are higher than the limits for general population/uncontrolled.

5.2 SAR Definition

The SAR definition is the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dv) of a given density (ρ). The equation description is as below:

$$SAR = \frac{d}{dt} \left(\frac{dU}{dm} \right) = \frac{d}{dt} \left(\frac{dU}{\rho dv} \right)$$

SAR is expressed in units of Watts per kilogram (W/kg) SAR measurement can be either related to the temperature elevation in tissue by

$$SAR = C \left(\frac{\delta T}{\delta t}\right)$$

Where: C is the specific heat capacity, δT is the temperature rise and δt is the exposure duration, or related to the electrical field in the tissue by

$$SAR = \frac{\sigma \cdot E^2}{\rho}$$

Where: σ is the conductivity of the tissue, ρ is the mass density of the tissue and E is the RMS electrical field strength. However for evaluating SAR of low power transmitter, electrical field measurement is typically applied.



6 **RF Exposure Limits**

6.1 Uncontrolled Environment

Uncontrolled Environments are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure. The general population/uncontrolled exposure limits are applicable to situations in which the general public may be exposed or in which persons who are exposed as a consequence of their employment may not be made fully aware of the potential for exposure or cannot exercise control over their exposure. Members of the general public would come under this category when exposure is not employment-related; for example, in the case of a wireless transmitter that exposes persons in its vicinity.

6.2 Controlled Environment

Controlled Environments are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation). In general, occupational/controlled exposure limits are applicable to situations in which persons are exposed as a consequence of their employment, who have been made fully aware of the potential for exposure and can exercise control over their exposure. This exposure category is also applicable when the exposure is of a transient nature due to incidental passage through a location where the exposure levels may be higher than the general population/uncontrolled limits, but the exposed person is fully aware of the potential for exposure and can exercise control over his or her exposure by leaving the area or by some other appropriate means.

6.3 **RF Exposure Limits**

SAR Human Exposure	Specified in ANSI/IEEE C95.1-1992 and Health Canada Safety C	Code 6
OAR Human Exposure	opeenied in Anomiele 630. 1-1352 and ficanti canada balety e	

HUMAN EXPOSURE LIMITS		
	UNCONTROLLED ENVIRONMENT	CONTROLLED ENVIRONMENT
	General Population (W/kg) or (mW/g)	Occupational (W/kg) or (mW/g)
SPATIAL PEAK SAR Brain	1.6	8.0
SPATIAL AVERAGE SAR Whole Body	0.08	0.4
SPATIAL PEAK SAR Hands, Feet, Ankles, Wrists	4.0	20

Note:

- 1. The Spatial Peak value of the SAR averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.
- 2. The Spatial Average value of the SAR averaged over the whole body.
- 3. The Spatial Peak value of the SAR averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.





7 SAR Measurement System

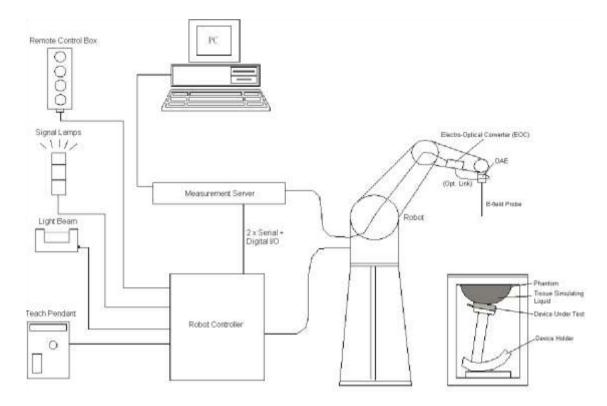


Fig. 8.1 SPEAG DASY System Configurations

The DASY system for performance compliance tests is illustrated above graphically. This system consists of the following items:

- > A standard high precision 6-axis robot with controller, a teach pendant and software
- A data acquisition electronic (DAE) attached to the robot arm extension
- > A dosimetric probe equipped with an optical surface detector system
- > The electro-optical converter (EOC) performs the conversion between optical and electrical signals
- A measurement server performs the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the accuracy of the probe positioning
- A computer operating Windows XP
- DASY software
- > Remove control with teach pendant and additional circuitry for robot safety such as warming lamps, etc.
- > The SAM twin phantom
- > A device holder
- Tissue simulating liquid
- Dipole for evaluating the proper functioning of the system

Component details are described in the following sub-sections.



7.1 E-Field Probe

The SAR measurement is conducted with the dosimetric probe (manufactured by SPEAG). The probe is specially designed and calibrated for use in liquid with high permittivity. The dosimetric probe has special calibration in liquid at different frequency. This probe has a built in optical surface detection system to prevent from collision with phantom.

> E-Field Probe Specification

<ex3dv4< th=""><th>Probe></th></ex3dv4<>	Probe>

Construction	Symmetrical design with triangular core Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents, e.g., DGBE)	
Frequency	10 MHz to 6 GHz; Linearity: ± 0.2 dB	
Directivity	± 0.3 dB in HSL (rotation around probe axis)	
	± 0.5 dB in tissue material (rotation normal to	
	probe axis)	
Dynamic Range	10 μ W/g to 100 mW/g; Linearity: ± 0.2 dB (noise: typically < 1 μ W/g)	
Dimensions	Overall length: 330 mm (Tip: 20mm)	
	Tip diameter: 2.5 mm (Body: 12mm)	
	Typical distance from probe tip to dipole	
	centers: 1 mm	· · · ·
		Fig. 8.2 Photo of E-Field Probe

> E-Field Probe Calibration

Each probe needs to be calibrated according to a dosimetric assessment procedure with accuracy better than \pm 10%. The spherical isotropy shall be evaluated and within \pm 0.25 dB. The sensitivity parameters (Norm X, Norm Y and Norm Z), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested. The calibration data can be referred to appendix E of this report.

7.2 Data Acquisition Electronics (DAE)

The Data acquisition electronics (DAE) consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gainswitching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock. The input impedance of the DAE is 200 MOhm; the inputs are symmetrical and floating. Common mode rejection is above 80 dB.




Fig. 8.3 Photo of DAE





7.3 Robot

The SPEAG DASY system uses the high precision robots (DASY5: TX60XL) type from Stäubli SA (France). For the 6-axis controller system, the robot controller version (DASY5: CS8c) from Stäubli is used. The Stäubli robot series have many features that are important for our application:

- High precision (repeatability 0.02 mm)
- High reliability (industrial design)
- Low maintenance costs (virtually maintenance free due to direct drive gears; no belt drives)
- Jerk-free straight movements
- Low ELF interference (motor control fields shielded via the closed metallic construction shields)



Fig. 8.4 Photo of Robot

7.4 Measurement Server

The measurement server is based on a PC/104 CPU board with CPU (DASY 5: 400MHz, Intel Celeron), chipdisk (DASY5: 128 MB), RAM (DASY5: 128 MB). The necessary circuits for communication with the DAE electronic box, as well as the 16 bit AD converter system for optical detection and digital I/O interface are contained on the DASY I/O board, which is directly connected to the PC/104 bus of the CPU board.

The measurement server performs all the real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operations.



Fig. 8.5 Photo of Server for DASY5

7.5 Light Beam Unit

The light beam switch allows automatic "tooling" of the probe. During the process, the actual position of the probe tip with respect to the robot arm is measured, as well as the probe length and the horizontal probe offset. The software then corrects all movements, such that the robot coordinates are valid for the probe tip.

The repeatability of this process is better than 0.1 mm. If a position has been taught with an aligned probe, the same position will be reached with another aligned probe within 0.1 mm, even if the other probe has different dimensions. During probe rotations, the probe tip will keep its actual position.



Fig. 8.6 Photo of Light Beam



7.6 Phantom

<SAM Twin Phantom>

Shell Thickness	2 ± 0.2 mm; Center ear point: 6 ± 0.2 mm	
Filling Volume Dimensions	Approx. 25 liters Length: 1000mm; Width: 500mm; Height: adjustable feet	
Measurement Areas	Left Head, Right Head, Flat phantom	Fig. 8.7 Photo of SAM Twin Phantom

The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections. A white cover is provided to tap the phantom during off-periods to prevent water evaporation and changes in the liquid parameters. On the phantom top, three reference markers are provided to identify the phantom position with respect to the robot.

<ELI4 Phantom >

The ELI4 phantom is intended for compliance testing of handheld and body-mounted wireless devices in the frequency range of 30MHz to 6 GHz. ELI4 is fully compatible with the latest draft of the standard IEC 62209-2 and all known tissue simulating liquids.

ELI4 has been optimized regarding its performance and can be integrated into a SPEAG standard phantom table. A cover prevents evaporation of the liquid. Reference markings on the phantom allow installation of the complete setup, including all predefined phantom positions and measurement grids, by teaching three points The phantom can be used with the following tissue simulating liquids:

- Water-sugar based liquids can be left permanently in the phantom. Always cover the liquid if the system is not in use; otherwise the parameters will change due to water evaporation.
- DGBE based liquids should be used with care. As DGBE is a softener for most plastics, the liquid should be taken out of the phantom and the phantom should be dried when the system is not in use (desirable at least once a week).
- Do not use other organic solvents without previously testing the phantom resistiveness.



Fig.8.8 Photo of ELI4 Phantom



7.7 Device Holder

<Device Holder for SAM Twin Phantom>

The SAR in the phantom is approximately inversely proportional to the square of the distance between the source and the liquid surface. For a source at 5 mm distance, a positioning uncertainty of \pm 0.5 mm would produce a SAR uncertainty of \pm 20 %. Accurate device positioning is therefore crucial for accurate and repeatable measurements. The positions in which the devices must be measured are defined by the standards. The DASY device holder is designed to cope with different positions given in the standard. It has two scales for the device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear reference points). The rotation center for both scales is the ear reference point (ERP). Thus the device needs no repositioning when changing the angles.

The DASY device holder is constructed of low-low POM material having the following dielectric parameters: relative permittivity $\varepsilon = 3$ and loss tangent $\delta = 0.02$. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.



Fig. 8.9 Photo of Device Holder



7.8 Data storage and Evaluation

Data Storage

The DASY software stores the assessed data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all the necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files. The post-processing software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verifications of the complete software setup even after the measurement and allows correction of erroneous parameter settings. For example, if a measurement has been performed with an incorrect crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be reevaluated.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type (e.g., [V/m], [mW/g]). Some of these units are not available in certain situations or give meaningless results, e.g., a SAR-output in a non-lose media, will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

Data Evaluation

The DASY post-processing software (SEMCAD) automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

Probe Parameters:	- Sensitivity - Conversion	Norm _i , a _{i0} , a _{i1} , a _{i2} ConvF _i
	- Diode compression point	dcp
Device Parameters:	- Frequency	f
	- Crest	cf
Media Parameters:	- Conductivity	σ
	- Density	ρ

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY components. In the direct measuring mode of the multi-meter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power.



The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp}$$

With

 V_i = compensated signal of channel i, (i = x, y, z)

- U_i = input signal of channel i, (i = x, y, z)
- cf = crest factor of exciting field (DASY parameter)
- dcpⁱ = diode compression point (DASY parameter)

From the compensated input signals, the primary field data for each channel can be evaluated:

E- Field Probes:
$$E_i = \sqrt{\frac{v_i}{Norm_i \cdot ConvF}}$$

I-Field Probes: $H_i = \sqrt{V_i} \cdot \frac{a_{i0} + a_{i1}f + a_{i2}f^2}{V_i}$

With

 V_i = compensated signal of channel i, (i = x, y, z) Norm_i = senor sensitivity of channel i, (i = x, y, z), $\mu V/(V/m)^2$ ConvF = sensitivity enhancement in solution a_{ii} = sensor sensitivity factors for H-field probes f = carrier frequency (GHz)

H

 E_i = electric field strength of channel i in V/m

Hi = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$

The primary field data are used to calculate the derived field units.

$$\mathsf{SAR} = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$$

With

SAR = local specific absorption rate in mW/g

E_{tot} = total field strength in V/m

 σ = conductivity in (mho/m) or (Siemens/m)

 ρ = equipment tissue density in g/cm³

Note that the density is set to 1, to account for actual head tissue density rather than the density of the tissue simulating liquid.



7.9 Test Equipment List

Manufacturer SPEAG	Equipment Description	Model	S/N		
SPEAG				Last Cal.	Due Date
	2450MHz System Validation Kit	D2450V2	910	06.15.2016	06.14.2019
SPEAG	Data Acquisition Electronics	DAE4	1373	03.22.2018	03.21.2019
SPEAG	Dosimetric E-Field Probe	EX3DV4	3924	07.19.2018	07.18.2019
SPEAG	DASY 52 Measurement Software	DASY 52	Version: 52.8.8.1222	N.C.R	N.C.R
SPEAG	DASY 52 File Conversion Software	SEMCAD X	Version: 14.6.10 (7331)	N.C.R	N.C.R
SPEAG	Phantom	Twin Phantom	1765	N.C.R	N.C.R
SPEAG	Phantom	ELI V5.0	1208	N.C.R	N.C.R
SPEAG	Phone Positioner	N/A	N/A	N.C.R	N.C.R
Stäubli	Robot	TX60L	F13/5P6VB1/A/01	N.C.R	N.C.R
R&S	Universal Radio Communication Tester	CMU200	113097	03.07.2018	03.06.2019
HP	Network Analyzer	8753D	3410A06291	03.19.2018	03.18.2019
Agilent	EPM Series Power Meter	E4418B	GB39512692	03.07.2018	03.06.2019
R&S	Spectrum Analyzer	FSP30	101454	03.07.2018	03.06.2019
Agilent	Power Sensor	8481A	MY41090341	03.07.2018	03.06.2019
R&S	Power Sensor	URV5-Z2	SEL0071	03.07.2018	03.06.2019
R&S	Signal Generator	SMX	835457/016	03.07.2018	03.06.2019
R&S	Signal Generator	SMR20	10080050	03.07.2018	03.06.2019
Huber Suhner	RF Cable	SUCOFLEX	12341	See N	lote 3
Huber Suhner	RF Cable	SUCOFLEX	17268	See N	lote 3
Huber Suhner	RF Cable	SUCOFLEX	2080	See N	lote 3
Weinschel	Attenuator	23-3-34	BL5513	See N	lote 3
Anritsu	Directional Coupler	MP654A	100217491	See N	lote 3
SPEAG	Dielectric Assessment Kit	3.5 Probe	1119	See N	lote 4
SPEAG	DAK Measurement Software	DAK	Version: DAK 3.5	N.C	C.R
Mini-circuits	Power amplifier	ZHL-42W	SC609401309	See N	lote 5

Note:

1. The calibration certificate of DASY can be referred to appendix C of this report.

2. Referring to KDB 865664 D01v01r04, the dipole calibration interval can be extended to 3 years with justification. The dipoles are also not physically damaged, or repaired during the interval.

3. The Insertion Loss calibration of Dual Directional Coupler and Attenuator were characterized via the network analyzer and compensated during system check.

- 4. The dielectric probe kit was calibrated via the network analyzer, with the specified procedure (calibrated in pure water) and calibration kit (standard) short circuit, before the dielectric measurement. The specific procedure and calibration kit are provided by Speag.
- 5. In system check we need to monitor the level on the power meter, and adjust the power amplifier level to have precise power level to the dipole; the measured SAR will be normalized to 1 W input power according to the ratio of 1 W to the input power to the dipole. For system check, the calibration of the power amplifier is deemed not critically required for correct measurement; the power meter is critical and we do have calibration for it

6. Attenuator insertion loss is calibrated by the network Analyzer, which the calibration is valid, before system check.

7. N.C.R means No Calibration Requirement.



8 Tissue Simulating Liquids

For the measurement of the field distribution inside the SAM phantom with DASY, the phantom must be filled with around 25 liters of homogeneous body tissue simulating liquid. For head SAR testing, the liquid height from the ear reference point (ERP) of the phantom to the liquid top surface is larger than 15 cm, which is shown in Fig. 9.1, for body SAR testing, the liquid height from the center of the flat phantom to liquid top surface is larger than 15 cm, which is shown in Fig. 9.2.

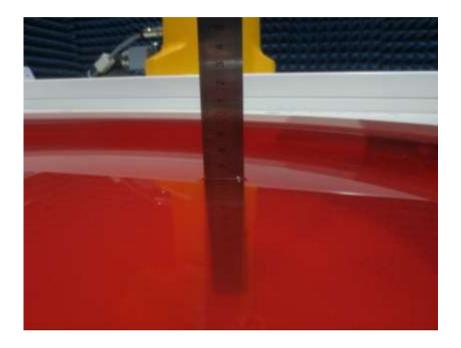


Fig. 9.6 Photo of Liquid Height for Body SAR of Twin Phantom (2000MHz~2600MHz) (depth>15cm)

The relative permittivity and conductivity of the tissue material should be within $\pm 5\%$ of the values given in the table below recommended by the FCC OET 65 supplement C and RSS 102 Issue 5.

Target Frequency	He	ad	Bo	dy
(MHz)	٤r	σ(S/m)	٤r	σ(S/m)
150	52.3	0.76	61.9	0.80
300	45.3	0.87	58.2	0.92
450	43.5	0.87	56.7	0.94
835	41.5	0.90	55.2	0.97
900	41.5	0.97	55.0	1.05
915	41.5	0.98	55.0	1.06
1450	40.5	1.20	54.0	1.30
1610	40.3	1.29	53.8	1.40
1800-2000	40.0	1.40	53.3	1.52
2450	39.2	1.80	52.7	1.95
3000	38.5	2.40	52.0	2.73
5800	35.3	5.27	48.2	6.00

($\epsilon r = relative permittivity, \sigma = conductivity and \rho = 1000 kg/m³)$

Project No.: CCISE1812129



The dielectric parameters of liquids were verified prior to the SAR evaluation using a Speag Dielectric Probe Kit and an Agilent Network Analyzer.

The following table shows the measuring results for simulating liquid.

Frequency (MHz)	Liquid Type	Liquid Temp. (℃)	Conductivity (σ)	Permittivity (εr)	Conductivity Target(σ)	Permittivity Target(εr)	Delta (σ)%	Delta (εr)%	Limit (%)	Date (mm/dd/yy)
2450	Body	22.6	1.96	52.43	1.95	52.7	0.51	-0.51	±5	12.27.2018



9 SAR System Verification

Each DASY system is equipped with one or more system validation kits. These units, together with the predefined measurement procedures within the DASY software, enable the user to conduct the system performance check and system validation. System validation kit includes a dipole, tripod holder to fix it underneath the flat phantom and a corresponding distance holder.

> Purpose of System Performance check

The system performance check verifies that the system operates within its specifications. System and operator errors can be detected and corrected. It is recommended that the system performance check be performed prior to any usage of the system in order to guarantee reproducible results. The system performance check uses normal SAR measurements in a simplified setup with a well characterized source. This setup was selected to give a high sensitivity to all parameters that might fail or vary over time. The system check does not intend to replace the calibration of the components, but indicates situations where the system uncertainty is exceeded due to drift or failure.

System Setup

In the simplified setup for system evaluation, the EUT is replaced by a calibrated dipole and the power source is replaced by a continuous wave that comes from a signal generator. The calibrated dipole must be placed beneath the flat phantom section of the SAM twin phantom with the correct distance holder. The distance holder should touch the phantom surface with a light pressure at the reference marking and be oriented parallel to the long side of the phantom. The equipment setup is shown below:

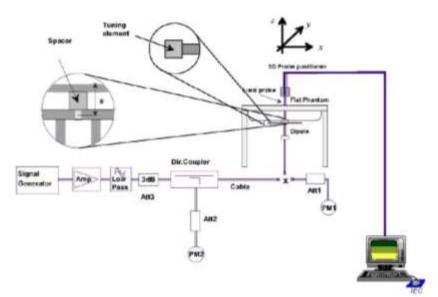


Fig.10.1 System Verification Setup Diagram



Fig.10.2 Photo of Dipole setup



> System Verification Results

Comparing to the original SAR value provided by SPEAG, the verification data should be within its specification of 10%. The table as below indicates the system performance check can meet the variation criterion and the plots can be referred to Appendix C of this report.

Date (mm/dd/yy)	Frequency (MHz)	Liquid Type	Power fed onto dipole (mW)	Measured 1g SAR (W/kg)	Normalized to 1W 1g SAR (W/kg)	1W Target 1g SAR (W/kg)	Deviation (%)
12.27.2018	2450	Body	40	2.14	53.5	51.8	3.28





10 EUT Testing Position

This EUT was tested in ten different positions. They are Front/Back/Right Side/Top Side/Bottom Side of the EUT with phantom 1 cm gap, as illustrated below, please refer to Appendix B for the test setup photos.

10.1 SAR Evaluations near the Mouth/Jaw Regions of the SAM Phantom

Antennas located near the bottom of a phone may require SAR measurements around the mouth and jaw regions of the SAM head phantom. This typically applies to clam-shell style phones that are generally longer in the unfolded normal use positions or to certain older style long rectangular phones.

Under these circumstances, the following procedures apply, adopted from the FCC guidance on SAR handsets document FCC KDB Publication 648474 D04v01r03. The SAR required in these regions of SAM should be measured using a flat phantom. The phone should be positioned with a separation distance of 4 mm between the ear reference point (ERP) and the outer surface of the flat phantom shell. While maintaining this distance at the ERP location, the low (bottom) edge of the phone should be lowered from the phantom to establish the same separation distance between the peak SAR locations identified by the truncated partial SAR distribution measured with the SAM phantom. The distance from the peak SAR location to the phone is determined by the straight line passing perpendicularly through the phantom surface. When it is not feasible to maintain 4 mm separation at the ERP while also establishing the required separation at the ERP. The phone should not be tilted to the left or right while placed in this inclined position to the flat phantom.

10.2 Body Worn Accessory Configurations

- > To position the device parallel to the phantom surface with either keypad up or down.
- > To adjust the device parallel to the flat phantom.
- To adjust the distance between the device surface and the flat phantom to 10 mm or holster surface and the flat phantom to 0 mm.





10.3 Wireless Router (Hotspot) Configurations

Some battery-operated handsets have the capability to transmit and receive internet connectivity through simultaneous transmission of WIFI in conjunction with a separate licensed transmitter. The FCC has provided guidance in KDB Publication 941225 D06 where SAR test considerations for handsets (L x W \geq

9 cm x 5 cm) are based on a composite test separation distance of 10 mm from the front, back and edges of the device with antennas 2.5 cm or closer to the edge of the device, determined from general mixed use conditions for this type of devices. Since the hotspot SAR results may overlap with the body-worn accessory SAR requirements, the more conservative configurations can be considered, thus excluding some body-worn accessory SAR tests.

When the user enables the personal wireless router functions for the handset, actual operations include simultaneous transmission of both the WIFI transmitter and another licensed transmitter. Both transmitters often do not transmit at the same transmitting frequency and thus cannot be evaluated for SAR under actual use conditions. Therefore, SAR must be evaluated for each frequency transmission and mode separately and summed with the WIFI transmitter according to KDB 648474 publication procedures. The "Portable Hotspot" feature on the handset was NOT activated, to ensure the SAR measurements were evaluated for a single transmission frequency RF signal.

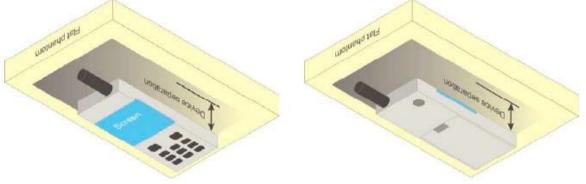


Fig.11.6 Illustration for Hotspot Position



11 Measurement Procedures

The measurement procedures are as bellows:

<Conducted power measurement>

- For WWAN power measurement, use base station simulator to configure EUT WWAN transition in conducted connection with RF cable, at maximum power in each supported wireless interface and frequency band.
- Read the WWAN RF power level from the base station simulator.
- For WLAN/BT power measurement, use engineering software to configure EUT WLAN/BT continuously transmission, at maximum RF power in each supported wireless interface and frequency band.
- Connect EUT RF port through RF cable to the power meter or spectrum analyzer, and measure WLAN/BT output power.

<Conducted power measurement>

- Use base station simulator to configure EUT WWAN transmission in radiated connection, and engineering software to configure EUT WLAN/BT continuously transmission, at maximum RF power, in the highest power channel.
- Place the EUT in positions as Appendix B demonstrates.
- Set scan area, grid size and other setting on the DASY software.
- Measure SAR results for the highest power channel on each testing position.
- Find out the largest SAR result on these testing positions of each band.
- Measure SAR results for other channels in worst SAR testing position if the Reported SAR or highest power channel is larger than 0.8 W/kg.

According to the test standard, the recommended procedure for assessing the peak spatial-average SAR value consists of the following steps:

- > Power reference measurement
- > Area scan
- Zoom scan
- Power drift measurement

11.1 Spatial Peak SAR Evaluation

The procedure for spatial peak SAR evaluation has been implemented according to the test standard. It can be conducted for 1g and 10g, as well as for user-specific masses. The DASY software includes all numerical procedures necessary to evaluate the spatial peak SAR value.

The base for the evaluation is a "cube" measurement. The measured volume must include the 1g and 10 g cubes with the highest averaged SAR values. For that purpose, the center of the measured volume is aligned to the interpolated peak SAR value of a previously performed area scan.

The entire evaluation of the spatial peak values is performed within the post-processing engine (SEMCAD). The system always gives the maximum values for 1g and 10g cubes. The algorithm to find the cube with highest averaged SAR is divided into the following stages:

- Extraction of the measured data (grid and values) from the Zoom Scan.
- Calculation of the SAR value at every measurement point based on all stored data (A/D values and measurement parameters).
- > Generation of a high-resolution mesh within the measured volume.
- Interpolation of all measured values form the measurement grid to the high-resolution grid
- Extrapolation of the entire 3-D field distribution to the phantom surface over the distance from sensor to surface
- Calculation of the averaged SAR within masses of 1g and 10g.





11.2 Power Reference Measurement

The Power Reference Measurement and Power Drift Measurement are for monitoring the power drift of the device under test in the batch process. The minimum distance of probe sensors to surface determines the closest measurement point to phantom surface. This distance cannot be smaller than the distance of sensor calibration points to probe tip as defined in the probe properties.

11.3 Area & Zoom Scan Procedures

First Area Scan is used to locate the approximate location(s) of the local peak SAR value(s). The measurement grid within an Area Scan is defined by the grid extent, grid step size and grid offset. Next, in order to determine the EM field distribution in a three-dimensional spatial extension, Zoom Scan is required. The Zoom Scan is performed around the highest E-field value to determine the averaged SAR-distribution over 10g. Area scan and zoom scan resolution setting follows KDB 865664 D01v01r04 quoted below.

			\leq 3 GHz	> 3 GHz
Maximum distance fro (geometric center of pr			$5 \pm 1 \mathrm{mm}$	$\frac{1}{2} \cdot 5 \cdot \ln(2) \pm 0.5 \text{ mm}$
Maximum probe angle surface normal at the n			30°±1°	20° ± 1°
			≤ 2 GHz: ≤ 15 mm 2 – 3 GHz: ≤ 12 mm	$\begin{array}{l} 3-4 \text{ GHz:} \leq 12 \text{ mm} \\ 4-6 \text{ GHz:} \leq 10 \text{ mm} \end{array}$
Maximum area scan sp	atial resol	ation: Δx _{Ana} , Δy _{Ana}		ion, is smaller than the above must be ≤ the corresponding device with at least one
Maximum zoom scan s	spatial reso	lution: Δx_{Zoon} , Δy_{Zoon}	$\leq 2 \text{ GHz}: \leq 8 \text{ mm}$ 2 - 3 GHz: $\leq 5 \text{ mm}^*$	$3 - 4 \text{ GHz} \le 5 \text{ mm}^4$ $4 - 6 \text{ GHz} \le 4 \text{ mm}^4$
	uniform	grid: ∆z _{Zoon} (n)	≤ 5 mm	$\begin{array}{c c} 3-4 \ \text{GHz:} \leq 4 \ \text{mm} \\ 4-5 \ \text{GHz:} \leq 3 \ \text{mm} \\ 5-6 \ \text{GHz:} \leq 2 \ \text{mm} \end{array}$
Maximum zoom scan spatial resolution, normal to phantom surface	graded	$\Delta z_{2com}(1)$: between 1 st two points closest to phantom surface	≤4 mm	$\begin{array}{l} 3-4 \ \text{GHz} \leq 3 \ \text{mm} \\ 4-5 \ \text{GHz} \leq 2.5 \ \text{mm} \\ 5-6 \ \text{GHz} \leq 2 \ \text{mm} \end{array}$
	grid	∆z _{2.oon} (n>1); between subsequent points	≤1.5∙∆	z _{Zoon} (n-1)
Mininum zoom scan volume	x, y, z		≥ 30 nm	$3 - 4 \text{ GHz} \ge 28 \text{ mm}$ $4 - 5 \text{ GHz} \ge 25 \text{ mm}$ $5 - 6 \text{ GHz} \ge 22 \text{ mm}$

KDB 447498 is \leq 1.4 W/kg, \leq 8 mm, \leq 7 mm and \leq 5 mm zoom scan resolution may be applied, respectively, for 2 GHz to 3 GHz, 3 GHz to 4 GHz and 4 GHz to 6 GHz.





11.4 Volume Scan Procedures

The volume scan is used for assess overlapping SAR distributions for antennas transmitting in different frequency bands. It is equivalent to an oversized zoom scan used in standalone measurements. The measurement volume will be used to enclose all the simultaneous transmitting antennas. For antennas transmitting simultaneously in different frequency bands, the volume scan is measured separately in each frequency band. In order to sum correctly to compute the 1g aggregate SAR, the EUT remain in the same test position for all measurements and all volume scan use the same spatial resolution and grid spacing. When all volume scan were completed, the software, SEMCAD post-processor scan combine and subsequently superpose these measurement data to calculating the multiband SAR.

11.5 SAR Averaged Methods

In DASY, the interpolation and extrapolation are both based on the modified Quadratic Shepard's method. The interpolation scheme combines a least-square fitted function method and a weighted average method which are the two basic types of computational interpolation and approximation.

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. The uncertainty increases with the extrapolation distance. To keep the uncertainty within 1% for the 1g and 10g cubes, the extrapolation distance should not be larger than 5 mm.

11.6 Power Drift Monitoring

All SAR testing is under the EUT install full charged battery and transmit maximum output power. In DASY measurement software, the power reference measurement and power drift measurement procedures are used for monitoring the power drift of EUT during SAR test. Both these procedures measure the field at a specified reference position before and after the SAR testing. The software will calculate the field difference in dB. If the power drifts more than 5%, the SAR will be retested.



12 RF Output Power

Frequency (MHz)	Average Power (dBm)
2410.875	20.93
2437.875	18.52
2471.625	18.46

Note:

- 1. Per KDB 248227 D01v02r02, choose the highest output power channel to test SAR and determine further SAR exclusion.
- Per KDB 248227 D01v02r02, In the 2.4 GHz band, separate SAR procedures are applied to DSSS and OFDM configurations to simplify DSSS test requirements. SAR is not required for the following 2.4 GHz OFDM conditions:

 When KDB Publication 447498 SAR test exclusion applies to the OFDM configuration.
 When the highest reported SAR for DSSS is adjusted by the ratio of OFDM to DSSS specified maximum output power and the adjusted SAR is ≤ 1.2 W/kg.
- 3. The output power of all data rate were pre-scan, just the worst case (the lowest data rate) of all mode were shown in report.
- 4. Per KDB 248227 D01V02r02 section 2.2, when the EUT in continuously transmitting mode, the actual duty cycle is 99.3%, so the duty cycle factor is 1.01.



13 SAR Test Results Summary

13.1 Standalone Body SAR

Plot No.	Band/Mode	Test Position	Freq. (MHz)	Ave. Power (dBm)	Power Drift (dB)	Tune-Up Limit (dBm)	Meas. SAR _{1g} (W/kg)	Scaling Factor	D.C Factor	Reported SAR _{1g} (W/kg)
1	2.4GHz/802.11b	Front	2410.875	20.93	-0.18	21.0	0.635	1.016	1.01	0.652
	2.4GHz/802.11b	Back	2410.875	20.93	-0.36	21.0	0.461	1.016	1.01	0.473
	2.4GHz/802.11b	Left	2410.875	20.93	-0.19	21.0	0.208	1.016	1.01	0.213
	2.4GHz/802.11b	Тор	2410.875	20.93	-0.36	21.0	0.094	1.016	1.01	0.096
Un	ANSI / IEEE C9 Spa controlled Expos	tial Peak					N/kg (mV aged ove	•		

Note:

- 1. Body-worn SAR testing was performed at 0mm separation, and this distance is determined by the handset manufacturer that there will be body-worn accessories that users may acquire at the time of equipment certification, to enable users to purchase aftermarket body-worn accessories with the required minimum separation.
- 2. Per KDB 447498 D01v06, for each exposure position, if the highest output channel Reported SAR ≤0.8W/kg, other channels SAR testing is not necessary.
- 3. Additional WLAN SAR testing was performed for simultaneous transmission analysis.
- 4. Per KDB 865664 D01v01r04, for each frequency band, repeated SAR measurement is required when the measured SAR is ≥0.8W/kg.
- 5. According to KDB 865664 D02v01r02, SAR plot is required for the highest measured SAR in each exposure configuration, wireless mode and frequency band combination.



13.2 Measurement Uncertainty

The component of uncertainly may generally be categorized according to the methods used to evaluate them. The evaluation of uncertainly by the statistical analysis of a series of observations is termed a Type A evaluation of uncertainty. The evaluation of uncertainty by means other than the statistical analysis of a series of observation is termed a Type B evaluation of uncertainty. Each component of uncertainty, however evaluated, is represented by an estimated standard deviation, termed standard uncertainty, which is determined by the positive square root of the estimated variance.

A Type A evaluation of standard uncertainty may be based on any valid statistical method for treating data. This includes calculating the standard deviation of the mean of a series of independent observations; using the method of least squares to fit a curve to the data in order to estimate the parameter of the curve and their standard deviations; or carrying out an analysis of variance in order to identify and quantify random effects in certain kinds of measurement.

A Type B evaluation of standard uncertainty is typically based on scientific judgment using all of the relevant information available. These may include previous measurement data, experience, and knowledge of the behavior and properties of relevant materials and instruments, manufacture's specification, data provided in calibration reports and uncertainties assigned to reference data taken from handbooks. Broadly speaking, the uncertainty is either obtained from an outdoor source or obtained from an assumed distribution, such as the normal distribution, rectangular or triangular distributions indicated in below Table.

Uncertainty Distributions	Normal	Rectangular	Triangular	U-Shape
Multi-plying Factor	1/k(b)	1/√3	1/√6	1/√2

Standard Uncertainty for Assumed Distribution

The combined standard uncertainty of the measurement result represents the estimated standard deviation of the result. It is obtained by combining the individual standard uncertainties of both Type A and Type B evaluation using the usual "root-sum-squares" (RSS) methods of combining standard deviations by taking the positive square root of the estimated variances.

Expanded uncertainty is a measure of uncertainty that defines an interval about the measurement result within which the measured value is confidently believed to lie. It is obtained by multiplying the combined standard uncertainty by a coverage factor. Typically, the coverage factor ranges from 2 to 3. Using a coverage factor allows the true value of a measured quantity to be specified with a defined probability within the specified uncertainty range. For purpose of this document, a coverage factor two is used, which corresponds to confidence interval of about 95 %. The DASY uncertainty Budget is shown in the following tables.



Uncertainty Component	Section	Uncert. Value	Prob. Dist.	Div.	(C _i) (1 g)	(C _i) (10 g)	Std. Unc. (1 g)	Std. Unc. (10 g)	Vi
Measurement System									
Probe Calibration	E.2.1	±7.4%	Ν	1	1	1	±7.4%	±7.4%	8
Axial Isotropy	E.2.2	±1.2%	R	√3	0.7	0.7	±0.49%	±0.49%	∞
Hemispherical Isotropy	E.2.2	±3.2%	R	√3	0.7	0.7	±1.29%	±1.29%	∞
Boundary Effects	E.2.3	±1.0%	R	$\sqrt{3}$	1	1	±0.58%	±0.58%	∞
Linearity	E.2.4	±0.9%	R	$\sqrt{3}$	1	1	±0.52%	±0.52%	∞
System Detection Limits	E.2.5	±0.25%	R	√3	1	1	±0.14%	±0.14%	8
Readout Electronics	E.2.6	±0.3%	Ν	1	1	1	±0.3%	±0.3%	8
Response Time	E.2.7	±0.8%	R	$\sqrt{3}$	1	1	±0.46%	±0.46%	∞
Integration Time	E.2.8	±2.6%	R	$\sqrt{3}$	1	1	±1.5%	±1.5%	∞
RF Ambient Noise	E.6.1	±3.0%	R	$\sqrt{3}$	1	1	±1.73%	±1.73%	8
RF Ambient Reflections	E.6.1	±3.0%	R	√3	1	1	±1.73%	±1.73%	8
Probe positioner mechanical tolerances	E.6.2	±0.4%	R	√3	1	1	±0.23%	±0.23%	8
Probe positioning tolerance with respect to the phantom shell surface	E.6.3	±2.9%	R	√3	1	1	±1.67%	±1.67%	8
Interpolation, extrapolation, and integration algorithm For max. SAR Evaluation.	E.5	±1.0%	R	√3	1	1	±0.58%	±0.58%	8
Test Sample Related	•							•	•
Device Positioning	E.4.2	±4.6%	N	1	1	1	±4.6%	±4.6%	M-1
Device Holder	E.4.1	±5.2%	N	1	1	1	±5.2%	±5.2%	M-1
Power Drift	6.6.2	±5.0%	R	√3	1	1	±2.89%	±2.89%	∞
Phantom and Setup		I		I	-		I		<u> </u>
Phantom Uncertainty	E.3.1	±4.0%	R	√3	1	1	±2.31%	±2.31%	∞
Liquid conductivity (measured value)	E.3.3	±3.51%	N	1	0.78	0.71	±2.74%	±2.49%	М
Liquid dielectric constant (measured value)	E.3.3	±3.4%	N	1	0.23	0.26	±0.78%	±0.88%	М
Liquid Conductivity - Temperature Uncertainty	E.3.4	±1.6%	R	$\sqrt{3}$	0.78	0.71	±0.72%	±0.66%	∞
Liquid Dielectric Constant - Temperature Uncertainty	E.3.4	±0.9%	R	√3	0.23	0.26	±0.12%	±0.14%	∞
	bined Stand	lard Uncerta	ainty (RS	S)	I		±11.61%	±11.55%	
Expanded U			• •	,			±23.23%	±23.10%	

Uncertainty Budget for frequency range 300 MHz to 3 GHz according to IEEE1528-2003



13.3 Measurement Conclusion

The SAR evaluation indicates that the EUT complies with the RF radiation exposure limits of the FCC and Industry Canada, with respect to all parameters subject to this test. These measurements were taken to simulate the RF effects of RF exposure under worst-case conditions. Precise laboratory measures were taken to assure repeatability of the tests. The results and statements relate only to the item(s) tested. Please note that the absorption and distribution of electromagnetic energy in the body are very complex phenomena that depend on the mass, shape, and size of the body, the orientation of the body with respect to the field vectors, and the electrical properties of both the body and the environment. Other variables that may play a substantial role in possible biological effects are those that characterize the environment (e.g. ambient temperature, air velocity, relative humidity, and body insulation) and those that characterize the individual (e.g. age, gender, activity level, debilitation, or disease). Because various factors may interact with one another to vary the specific biological outcome of an exposure to electromagnetic fields, any protection guide should consider maximal amplification of biological effects as a result of field-body interactions, environmental conditions, and physiological variables.



14 Reference

- [1]. FCC 47 CFR Part 2 "Frequency Allocations and Radio Treaty Matters; General Rules and Regulations"
- [2]. ANSI/IEEE Std. C95.1-1992, "IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz", September 1992
- [3]. IEEE Std. 1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- [4]. SPEAG DASY52 System Handbook
- [5]. FCC KDB 248227 D01 v02r02, "SAR GUIDANCE FOR IEEE 802.11 (Wi-Fi) TRANSMITTERS", October 2015
- [6]. FCC KDB 447498 D01 v06, "RF EXPOSURE PROCEDURES AND EQUIPMENT AUTHORIZATION POLICIES FOR MOBILE AND PORTABLE DEVICES", October 2015
- [7]. FCC KDB 616217 D04 v01r02, "SAR EVALUATION CONSIDERATIONS FOR LAPTOP, NOTEBOOK, NETBOOK AND TABLET COMPUTERS", October 2015
- [8]. FCC KDB 648474 D04 v01r03, "SAR EVALUATION CONSIDERATIONS FOR WIRELESS HANDSETS", October 2015
- [9]. FCC KDB 941225 D06 v02r01, " SAR EVALUATION PROCEDURES FOR PORTABLE DEVICES WITH WIRELESS ROUTER CAPABILITIES", October 2015
- [10]. FCC KDB 865664 D01 v01r04, "SAR MEASUREMENT REQUIREMENTS FOR 100 MHz TO 6 GHz", August 2015

Appendix A: Plots of SAR System Check





Test Laboratory: CCIS

Date/Time: 12.27.2018 08:14:19

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: SN:910

Communication System: UID 0, CW (0); Frequency: 2450 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2450 MHz; $\sigma = 1.962$ S/m; $\epsilon_r = 52.431$; $\rho = 1000$ kg/m³ Phantom section: Flat Section

DASY5 Configuration:


- Probe: EX3DV4 SN3924; ConvF(7.49, 7.49, 7.49); Calibrated: 07.19.2018;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1373; Calibrated: 03.22.2018
- Phantom: ELI v5.0; Type: QDOVA002AA; Serial: TP:1208
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

System Performance Check at Frequency 2450MHz Body Tissue/d=10mm, Pin=40 mW, dist=2.0mm (EX-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mmReference Value = 38.55 V/m; Power Drift = -0.12 dB Peak SAR (extrapolated) = 4.34 W/kg **SAR(1 g) = 2.14 W/kg; SAR(10 g) = 0.981 W/kg** Maximum value of SAR (measured) = 3.26 W/kg

System Performance Check at Frequency 2450MHz Body Tissue/d=10mm, Pin=40 mW, dist=2.0mm (EX-Probe)/Area Scan (51x61x1): Interpolated grid:

dx=1.200 mm, dy=1.200 mm Maximum value of SAR (interpolated) = 3.45 W/kg

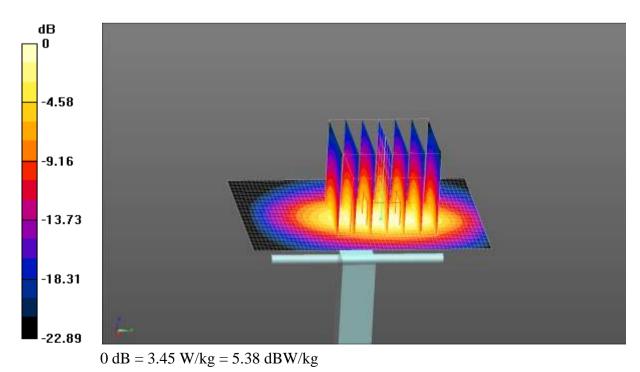

Project No.: CCISE1812129

Appendix B: Plots of SAR Test Data



Test Laboratory: CCIS

Date/Time: 12.27.2018 09:38:35

DUT: Baby Monitor; Type: AC-2-M; Serial: 1#

Communication System: UID 0, GFSK (0); Frequency: 2410.875 MHz; Duty Cycle: 1:1 Medium parameters used (interpolated): f = 2411 MHz; $\sigma = 1.938$ S/m; $\varepsilon_r = 52.785$; $\rho = 1000$ kg/m^3

Phantom section: Flat Section

DASY5 Configuration:


- Probe: EX3DV4 SN3924; ConvF(7.49, 7.49, 7.49); Calibrated: 07.19.2018; •
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1373: Calibrated: 03.22.2018
- Phantom: ELI v5.0; Type: QDOVA002AA; Serial: TP:1208
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

GFSK Body Front/Low Channel/Zoom Scan (5x5x7)/Cube 0: Measurement grid:

dx=5mm, dy=5mm, dz=5mm Reference Value = 14.14 V/m: Power Drift = -0.18 dBPeak SAR (extrapolated) = 1.24 W/kgSAR(1 g) = 0.635 W/kg; SAR(10 g) = 0.314 W/kgMaximum value of SAR (measured) = 0.998 W/kg

GFSK Body Front/Low Channel/Area Scan (51x51x1): Interpolated grid: dx=1.200

mm, dy=1.200 mm Maximum value of SAR (interpolated) = 0.882 W/kg

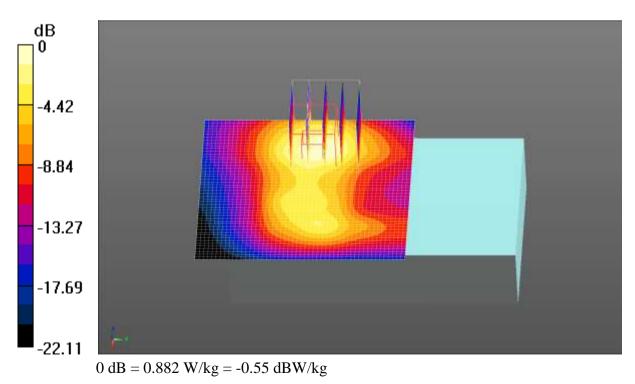



Appendix C: System Calibration Certificate



Calibration information for E-field probes

E-mail: cttl@chinatt Client CCIS	Church and a second sec	Certificate No: Z18-6	0226
CALIBRATION CE			
CALIBRATION CE	RIFICATE		
Object	EX3DV4	- SN:3924	
Calibration Procedure(s)	FF-Z11-0	04-01	
		on Procedures for Dosimetric E-field Probes	
Calibration date:	July 19, 2	2018	
	5diy 15, 2		
This calibration Certificate	documents the tra	aceability to national standards, which realize	ze the physical units of
		e uncertainties with confidence probability ar	e given on the following
pages and are part of the ce	rtificate.		
numidity<70%.	conducted in th	e closed laboratory facility: environment t	temperature(22±3)°C and
numidity<70%. Calibration Equipment used	conducted in th (M&TE critical for	calibration)	temperature(22±3)°C and Scheduled Calibration
numidity<70%. Calibration Equipment used	conducted in th (M&TE critical for		
numidity<70%. Calibration Equipment used Primary Standards	Conducted in th (M&TE critical for ID # (calibration) Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2	Conducted in th (M&TE critical for ID # (101919	calibration) Cal Date(Calibrated by, Certificate No.) 20-Jun-18 (CTTL, No.J18X05032)	Scheduled Calibration Jun-19
numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91	Conducted in th (M&TE critical for ID # 0 101919 101547	calibration) Cal Date(Calibrated by, Certificate No.) 20-Jun-18 (CTTL, No.J18X05032) 20-Jun-18 (CTTL, No.J18X05032)	Scheduled Calibration Jun-19 Jun-19
Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91	Conducted in th (M&TE critical for ID # (101919 101547 101548	calibration) Cal Date(Calibrated by, Certificate No.) 20-Jun-18 (CTTL, No.J18X05032) 20-Jun-18 (CTTL, No.J18X05032) 20-Jun-18 (CTTL, No.J18X05032)	Scheduled Calibration Jun-19 Jun-19 Jun-19
Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator	Conducted in th (M&TE critical for ID # (101919 101547 101548 18N50W-10dB 18N50W-20dB	calibration) Cal Date(Calibrated by, Certificate No.) 20-Jun-18 (CTTL, No.J18X05032) 20-Jun-18 (CTTL, No.J18X05032) 20-Jun-18 (CTTL, No.J18X05032) 09-Feb-18(CTTL, No.J18X01133)	Scheduled Calibration Jun-19 Jun-19 Jun-19 Feb-20
Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator Reference20dBAttenuator	Conducted in th (M&TE critical for ID # (101919 101547 101548 18N50W-10dB 18N50W-20dB	calibration) Cal Date(Calibrated by, Certificate No.) 20-Jun-18 (CTTL, No.J18X05032) 20-Jun-18 (CTTL, No.J18X05032) 20-Jun-18 (CTTL, No.J18X05032) 09-Feb-18(CTTL, No.J18X01133) 09-Feb-18(CTTL, No.J18X01132)	Scheduled Calibration Jun-19 Jun-19 Jun-19 Feb-20 Feb-20 Feb-20
Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator Reference20dBAttenuator Reference Probe EX3DV4	Conducted in th (M&TE critical for ID # (101919 101547 101548 18N50W-10dB 18N50W-20dB SN 3846	calibration) Cal Date(Calibrated by, Certificate No.) 20-Jun-18 (CTTL, No.J18X05032) 20-Jun-18 (CTTL, No.J18X05032) 20-Jun-18 (CTTL, No.J18X05032) 09-Feb-18(CTTL, No.J18X01133) 09-Feb-18(CTTL, No.J18X01132) 25-Jan-18(SPEAG,No.EX3-3846_Jan18)	Scheduled Calibration Jun-19 Jun-19 Jun-19 Feb-20 Feb-20 Jan-19
numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator Reference20dBAttenuator Reference Probe EX3DV4 DAE4	conducted in th (M&TE critical for ID # 0 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 3846 SN 777 ID #	calibration) Cal Date(Calibrated by, Certificate No.) 20-Jun-18 (CTTL, No.J18X05032) 20-Jun-18 (CTTL, No.J18X05032) 20-Jun-18 (CTTL, No.J18X05032) 09-Feb-18(CTTL, No.J18X01133) 09-Feb-18(CTTL, No.J18X01132) 25-Jan-18(SPEAG,No.EX3-3846_Jan18) 15-Dec-17(SPEAG, No.DAE4-777_Dec17) Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration Jun-19 Jun-19 Jun-19 Feb-20 Feb-20 Jan-19 Dec -18
numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-291 Power sensor NRP-291 Reference10dBAttenuator Reference20dBAttenuator Reference Probe EX3DV4 DAE4 Secondary Standards	conducted in th (M&TE critical for ID # 0 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 3846 SN 777 ID # 6201052605	calibration) Cal Date(Calibrated by, Certificate No.) 20-Jun-18 (CTTL, No.J18X05032) 20-Jun-18 (CTTL, No.J18X05032) 20-Jun-18 (CTTL, No.J18X05032) 09-Feb-18(CTTL, No.J18X01133) 09-Feb-18(CTTL, No.J18X01132) 25-Jan-18(SPEAG,No.EX3-3846_Jan18) 15-Dec-17(SPEAG, No.DAE4-777_Dec17)	Scheduled Calibration Jun-19 Jun-19 Jun-19 Feb-20 Feb-20 Jan-19 Dec -18 Scheduled Calibration
Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-291 Power sensor NRP-291 Reference10dBAttenuator Reference20dBAttenuator Reference Probe EX3DV4 DAE4 Secondary Standards SignalGeneratorMG3700A Network Analyzer E5071C	conducted in th (M&TE critical for ID # 0 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 3846 SN 777 ID # 6201052605	calibration) Cal Date(Calibrated by, Certificate No.) 20-Jun-18 (CTTL, No.J18X05032) 20-Jun-18 (CTTL, No.J18X05032) 20-Jun-18 (CTTL, No.J18X05032) 09-Feb-18(CTTL, No.J18X01133) 09-Feb-18(CTTL, No.J18X01132) 25-Jan-18(SPEAG,No.EX3-3846_Jan18) 15-Dec-17(SPEAG, No.DAE4-777_Dec17) Cal Date(Calibrated by, Certificate No.) 21-Jun-18 (CTTL, No.J18X05033)	Scheduled Calibration Jun-19 Jun-19 Jun-19 Feb-20 Feb-20 Jan-19 Dec -18 Scheduled Calibration Jun-19
humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-291 Power sensor NRP-291 Reference10dBAttenuator Reference20dBAttenuator Reference Probe EX3DV4 DAE4 Secondary Standards SignalGeneratorMG3700A	conducted in th (M&TE critical for ID # (101919 101547 101548 18N50W-10dB 18N50W-20dB SN 3846 SN 777 ID # 6201052605 MY46110673	calibration) Cal Date(Calibrated by, Certificate No.) 20-Jun-18 (CTTL, No.J18X05032) 20-Jun-18 (CTTL, No.J18X05032) 20-Jun-18 (CTTL, No.J18X05032) 09-Feb-18(CTTL, No.J18X01133) 09-Feb-18(CTTL, No.J18X01132) 25-Jan-18(SPEAG,No.EX3-3846_Jan18) 15-Dec-17(SPEAG, No.DAE4-777_Dec17) Cal Date(Calibrated by, Certificate No.) 21-Jun-18 (CTTL, No.J18X05033) 14-Jan-18 (CTTL, No.J18X00561)	Scheduled Calibration Jun-19 Jun-19 Jun-19 Feb-20 Feb-20 Jan-19 Dec -18 Scheduled Calibration Jun-19 Jan -19
humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-291 Power sensor NRP-291 Reference10dBAttenuator Reference20dBAttenuator Reference Probe EX3DV4 DAE4 Secondary Standards SignalGeneratorMG3700A Network Analyzer E5071C	conducted in th (M&TE critical for ID # (101919 101547 101548 18N50W-10dB 18N50W-20dB SN 3846 SN 777 ID # 6201052605 MY46110673 Name	calibration) Cal Date(Calibrated by, Certificate No.) 20-Jun-18 (CTTL, No.J18X05032) 20-Jun-18 (CTTL, No.J18X05032) 20-Jun-18 (CTTL, No.J18X05032) 09-Feb-18(CTTL, No.J18X01133) 09-Feb-18(CTTL, No.J18X01132) 25-Jan-18(SPEAG,No.EX3-3846_Jan18) 15-Dec-17(SPEAG, No.DAE4-777_Dec17) Cal Date(Calibrated by, Certificate No.) 21-Jun-18 (CTTL, No.J18X05033) 14-Jan-18 (CTTL, No.J18X00561) Function	Scheduled Calibration Jun-19 Jun-19 Jun-19 Feb-20 Feb-20 Jan-19 Dec -18 Scheduled Calibration Jun-19 Jan -19

Certificate No: Z18-60226

Page 1 of 11



 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2512
 Fax: +86-10-62304633-2504

 E-mail: ettl@chinattl.com
 Http://www.chinattl.com

Glossary:

tissue simulating liquid
sensitivity in free space
sensitivity in TSL / NORMx,y,z
diode compression point
crest factor (1/duty_cycle) of the RF signal
modulation dependent linearization parameters
Φ rotation around probe axis
θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i
θ=0 is normal to probe axis

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010

d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization θ=0 (f≤900MHz in TEM-cell; f>1800MHz: waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z* frequency_response (see Frequency Response Chart). This
 linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the
 frequency response is included in the stated uncertainty of ConvF.
- DCPx, y,z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- Ax, y, z; Bx, y, z; Cx, y, z; VRx, y, z: A, B, C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f≤800MHz) and inside waveguide using analytical field distributions based on power measurements for f >800MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty valued are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from±50MHz to±100MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the
 probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: Z18-60226

Page 2 of 11





 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2512
 Fax: +86-10-62304633-2504

 E-mail: ettl@chinatil.com
 Http://www.chinattl.cn

Probe EX3DV4

SN: 3924

Calibrated: July 19, 2018

Calibrated for DASY/EASY Systems (Note: non-compatible with DASY2 system!)

Certificate No: Z18-60226

Page 3 of 11





 Figure 1
 Figure 2
 Figure 2

DASY/EASY – Parameters of Probe: EX3DV4 – SN: 3924

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm(µV/(V/m)2) ^A	0.50	0.42	0.68	±10.0%
DCP(mV) ⁸	101.1	100.2	99.9	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dBõV	C	D dB	VR mV	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	172.2	±2.2%
		Y	0.0	0.0	1.0		153.7	C SA DA SERSE
		Z	0.0	0.0	1.0		202.8	

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X, Y, Z do not affect the E²-field uncertainty inside TSL (see Page 5 and Page 6).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainly is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Page 4 of 11





DASY/EASY - Parameters of Probe: EX3DV4 - SN: 3924

f [MHz] ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
750	41.9	0.89	10.06	10.06	10.06	0.40	0.80	±12.1%
835	41.5	0.90	9.66	9.66	9.66	0.17	1.33	±12.1%
900	41.5	0.97	9.63	9.63	9.63	0.16	1.37	±12.1%
1750	40.1	1.37	8.30	8.30	8.30	0.17	1.26	±12.1%
1900	40.0	1.40	8.03	8.03	8.03	0.24	1.05	±12.1%
2300	39.5	1.67	7.86	7.86	7.86	0.52	0.73	±12.1%
2450	39.2	1.80	7.51	7.51	7.51	0.55	0.73	±12.1%
2600	39.0	1.96	7.27	7.27	7.27	0.65	0.69	±12.1%

Calibration Parameter Determined in Head Tissue Simulating Media

^c Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequency below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters. ^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies

between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Page 5 of 11





DASY/EASY – Parameters of Probe: EX3DV4 – SN: 3924

f [MHz] ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
750	55.5	0.96	10.23	10.23	10.23	0.40	0.80	±12.1%
835	55.2	0.97	9.86	9.86	9.86	0.17	1.44	±12.1%
900	55.0	1.05	9.83	9.83	9.83	0.24	1.18	±12.1%
1750	53.4	1.49	8.02	8.02	8.02	0.21	1.13	±12.1%
1900	53.3	1.52	7.72	7.72	7.72	0.21	1.15	±12.1%
2300	52.9	1.81	7.75	7.75	7.75	0.55	0.81	±12.1%
2450	52.7	1.95	7.49	7.49	7.49	0.50	0.89	±12.1%
2600	52.5	2.16	7.12	7.12	7.12	0.60	0.74	±12.1%

Calibration Parameter Determined in Body Tissue Simulating Media

^c Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


[#] At frequency below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: Z18-60226

Page 6 of 11



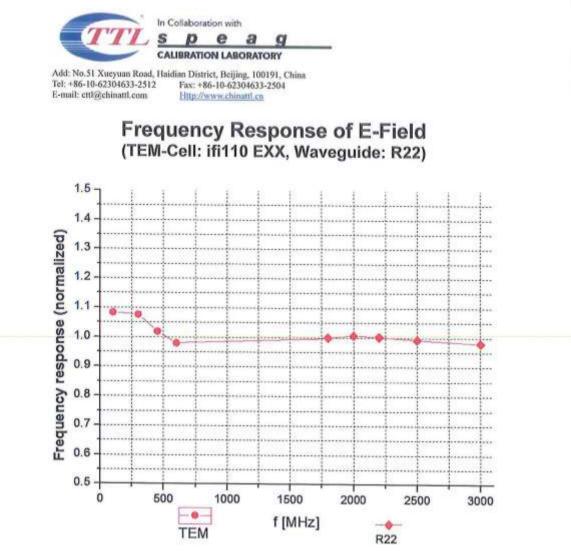

Uncertainty of Frequency Response of E-field: ±7.4% (k=2)

Certificate No: Z18-60226

Page 7 of 11






Littp://www.chinattl.co

Receiving Pattern (Φ), θ=0°

f=600 MHz, TEM


f=1800 MHz, R22

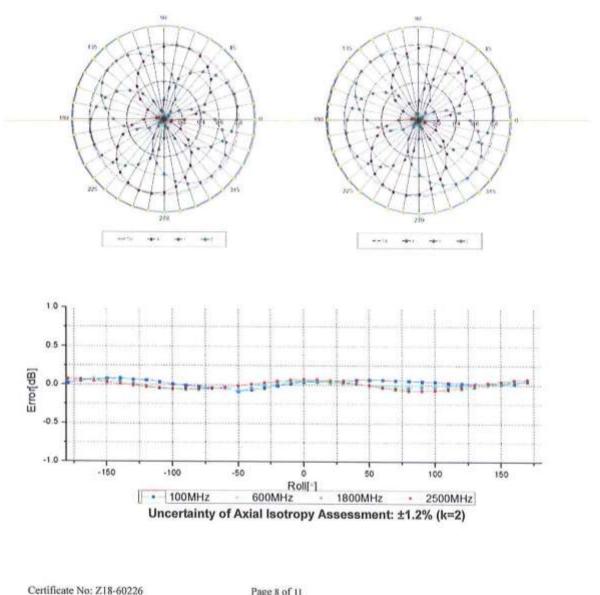


Page 8 of 11


23



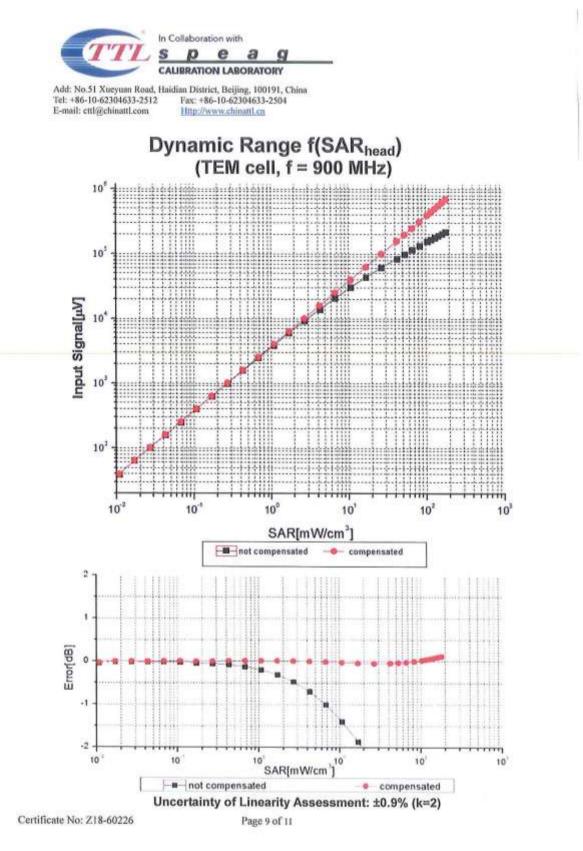



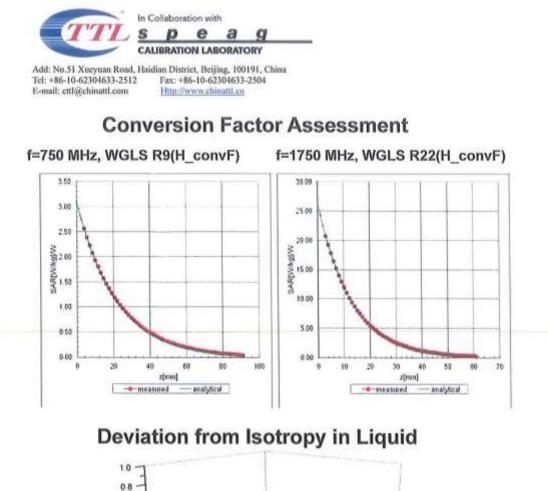

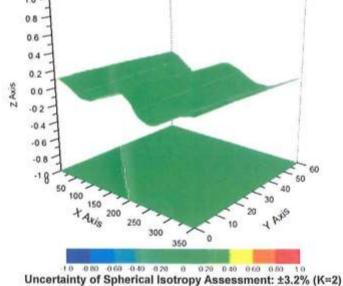

Certificate No: Z18-60226

Page 10 of 11





DASY/EASY - Parameters of Probe: EX3DV4 - SN: 3924

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	159.7
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disable
Probe Overall Length	337mm
Probe Body Diameter	10mm
Tip Length	9mm
Tip Diameter	2.5mm
Probe Tip to Sensor X Calibration Point	1mm
Probe Tip to Sensor Y Calibration Point	1mm
Probe Tip to Sensor Z Calibration Point	1mm
Recommended Measurement Distance from Surface	1.4mm

Certificate No: Z18-60226

Page 11 of 11



	Calib	ration information for Dipole	
		pration with	中国认可
	- Contract of the second secon	<u>eag</u>	国际石山
	CALIBRA	TION LABORATORY	NAS 校准
		trict, Beijing, 100191, China	CALIBRATION
Tel: +86-10-623046. E-mail: cttl@chinatt		86-10-62304633-2504	CNAS L0570
Client CCIS	S	Certificate No: Z1	16-97091
CALIBRATION CE	RTIFICAT	E	
Object	D2450	/2 - SN: 910	1.15
Collibration Dragodura(a)			
Calibration Procedure(s)	FD-Z11	-2-003-01	
	Calibra	tion Procedures for dipole validation kits	
Calibration date:	Jun 15,	2016	
	Contract of Land		
This calibration Certificate of	documents the	traceability to national standards, which rea	alize the physical units of
measurements(SI). The mea	asurements and	the uncertainties with confidence probability	are given on the following
pages and are part of the ce	rtificate.		
All calibrations have been humidity<70%.	conducted in	the closed laboratory facility: environment	temperature(22±3) $^\circ\!$
			t temperature(22±3)℃ and
humidity<70%.			t temperature(22±3)℃ and Scheduled Calibration
humidity<70%. Calibration Equipment used	(M&TE critical fo	or calibration)	
humidity<70%. Calibration Equipment used Primary Standards	(M&TE critical fo	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2	(M&TE critical fo	Cal Date(Calibrated by, Certificate No.) 01-Jul-15 (CTTL, No.J15X04256)	Scheduled Calibration Jun-16
humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91	(M&TE critical fo ID # 101919 101547	Cal Date(Calibrated by, Certificate No.) 01-Jul-15 (CTTL, No.J15X04256) 01-Jul-15 (CTTL, No.J15X04256)	Scheduled Calibration Jun-16 Jun-16
humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Reference Probe EX3DV4 DAE4	(M&TE critical fo ID # 101919 101547 SN 7307 SN 771	Cal Date(Calibrated by, Certificate No.) 01-Jul-15 (CTTL, No.J15X04256) 01-Jul-15 (CTTL, No.J15X04256) 19-Feb-16(SPEAG,No.EX3-7307_Feb16) 02-Feb-16(CTTL-SPEAG,No.Z16-97011)	Scheduled Calibration Jun-16 Jun-16 Feb-17 Feb-17
humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Reference Probe EX3DV4 DAE4 Secondary Standards	(M&TE critical fo ID # 101919 101547 SN 7307 SN 771 ID #	Cal Date(Calibrated by, Certificate No.) 01-Jul-15 (CTTL, No.J15X04256) 01-Jul-15 (CTTL, No.J15X04256) 19-Feb-16(SPEAG,No.EX3-7307_Feb16) 02-Feb-16(CTTL-SPEAG,No.Z16-97011) Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration Jun-16 Jun-16 Feb-17 Feb-17 Scheduled Calibration
humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Reference Probe EX3DV4 DAE4	(M&TE critical fo ID # 101919 101547 SN 7307 SN 771	Cal Date(Calibrated by, Certificate No.) 01-Jul-15 (CTTL, No.J15X04256) 01-Jul-15 (CTTL, No.J15X04256) 19-Feb-16(SPEAG,No.EX3-7307_Feb16) 02-Feb-16(CTTL-SPEAG,No.Z16-97011)	Scheduled Calibration Jun-16 Jun-16 Feb-17 Feb-17
humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	(M&TE critical fo ID # 101919 101547 SN 7307 SN 771 ID # MY49071430 MY46110673	Cal Date(Calibrated by, Certificate No.) 01-Jul-15 (CTTL, No.J15X04256) 01-Jul-15 (CTTL, No.J15X04256) 19-Feb-16(SPEAG,No.EX3-7307_Feb16) 02-Feb-16(CTTL-SPEAG,No.Z16-97011) Cal Date(Calibrated by, Certificate No.) 01-Feb-16 (CTTL, No.J16X00893) 26-Jan-16 (CTTL, No.J16X00894)	Scheduled Calibration Jun-16 Jun-16 Feb-17 Feb-17 Scheduled Calibration Jan-17 Jan-17
humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C Network Analyzer E5071C	(M&TE critical fo ID # 101919 101547 SN 7307 SN 771 ID # MY49071430 MY46110673 Name	Cal Date(Calibrated by, Certificate No.) 01-Jul-15 (CTTL, No.J15X04256) 01-Jul-15 (CTTL, No.J15X04256) 19-Feb-16(SPEAG,No.EX3-7307_Feb16) 02-Feb-16(CTTL-SPEAG,No.Z16-97011) Cal Date(Calibrated by, Certificate No.) 01-Feb-16 (CTTL, No.J16X00893) 26-Jan-16 (CTTL, No.J16X00894) Function	Scheduled Calibration Jun-16 Jun-16 Feb-17 Feb-17 Scheduled Calibration Jan-17
humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	(M&TE critical fo ID # 101919 101547 SN 7307 SN 771 ID # MY49071430 MY46110673	Cal Date(Calibrated by, Certificate No.) 01-Jul-15 (CTTL, No.J15X04256) 01-Jul-15 (CTTL, No.J15X04256) 19-Feb-16(SPEAG,No.EX3-7307_Feb16) 02-Feb-16(CTTL-SPEAG,No.Z16-97011) Cal Date(Calibrated by, Certificate No.) 01-Feb-16 (CTTL, No.J16X00893) 26-Jan-16 (CTTL, No.J16X00894)	Scheduled Calibration Jun-16 Jun-16 Feb-17 Feb-17 Scheduled Calibration Jan-17 Jan-17
humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C Network Analyzer E5071C	(M&TE critical fo ID # 101919 101547 SN 7307 SN 771 ID # MY49071430 MY46110673 Name	Cal Date(Calibrated by, Certificate No.) 01-Jul-15 (CTTL, No.J15X04256) 01-Jul-15 (CTTL, No.J15X04256) 19-Feb-16(SPEAG,No.EX3-7307_Feb16) 02-Feb-16(CTTL-SPEAG,No.Z16-97011) Cal Date(Calibrated by, Certificate No.) 01-Feb-16 (CTTL, No.J16X00893) 26-Jan-16 (CTTL, No.J16X00894) Function	Scheduled Calibration Jun-16 Jun-16 Feb-17 Feb-17 Scheduled Calibration Jan-17 Jan-17
humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C Network Analyzer E5071C Calibrated by: Reviewed by:	(M&TE critical fo ID # 101919 101547 SN 7307 SN 771 ID # MY49071430 MY46110673 Name Zhao Jing	Cal Date(Calibrated by, Certificate No.) 01-Jul-15 (CTTL, No.J15X04256) 01-Jul-15 (CTTL, No.J15X04256) 19-Feb-16(SPEAG,No.EX3-7307_Feb16) 02-Feb-16(CTTL-SPEAG,No.Z16-97011) Cal Date(Calibrated by, Certificate No.) 01-Feb-16 (CTTL, No.J16X00893) 26-Jan-16 (CTTL, No.J16X00894) Function SAR Test Engineer	Scheduled Calibration Jun-16 Jun-16 Feb-17 Feb-17 Scheduled Calibration Jan-17 Jan-17
humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C Network Analyzer E5071C	(M&TE critical fo ID # 101919 101547 SN 7307 SN 771 ID # MY49071430 MY46110673 Name Zhao Jing	Cal Date(Calibrated by, Certificate No.) 01-Jul-15 (CTTL, No.J15X04256) 01-Jul-15 (CTTL, No.J15X04256) 19-Feb-16(SPEAG,No.EX3-7307_Feb16) 02-Feb-16(CTTL-SPEAG,No.Z16-97011) Cal Date(Calibrated by, Certificate No.) 01-Feb-16 (CTTL, No.J16X00893) 26-Jan-16 (CTTL, No.J16X00894) Function SAR Test Engineer	Scheduled Calibration Jun-16 Jun-16 Feb-17 Feb-17 Scheduled Calibration Jan-17 Jan-17
humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C Network Analyzer E5071C Calibrated by: Reviewed by:	(M&TE critical fo ID # 101919 101547 SN 7307 SN 771 ID # MY49071430 MY46110673 Name Zhao Jing Qi Dianyuan	Cal Date(Calibrated by, Certificate No.) 01-Jul-15 (CTTL, No.J15X04256) 01-Jul-15 (CTTL, No.J15X04256) 19-Feb-16(SPEAG,No.EX3-7307_Feb16) 02-Feb-16(CTTL-SPEAG,No.Z16-97011) Cal Date(Calibrated by, Certificate No.) 01-Feb-16 (CTTL, No.J16X00893) 26-Jan-16 (CTTL, No.J16X00894) Function SAR Test Engineer	Scheduled Calibration Jun-16 Jun-16 Feb-17 Feb-17 Scheduled Calibration Jan-17 Jan-17 Signature

Certificate No: Z16-97091





 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2079
 Fax: +86-10-62304633-2504

 E-mail: ettl@chinattl.com
 Http://www.chinattl.cn

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORMx,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) For hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005
- c) IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
- d) KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

Additional Documentation:

e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z16-97091

Page 2 of 8







 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2079
 Fax: +86-10-62304633-2504

 E-mail: cttl@chinattl.com
 Http://www.chinattl.cn

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.8.8.1258
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.0 ± 6 %	1.77 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.0 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	52.4 mW /g ± 20.8 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	6.06 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	24.3 mW /g ± 20.4 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.9 ± 6 %	1.97 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C		

SAR result with Body TSL

SAR averaged over 1 cm^3 (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.0 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	51.8 mW /g ± 20.8 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	6.18 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	24.7 mW /g ± 20.4 % (k=2)

Certificate No: Z16-97091

Page 3 of 8

	In Co	ollabora	tion wit	'n	
TTL	S	P	е	а	g
	CAL	BRATI	ON LAB	ORATO	DRY

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	54.6Ω+ 2.77jΩ	
Return Loss	- 25.8dB	

Antenna Parameters with Body TSL

Impedance, transformed to feed point	50.7Ω+ 4.28jΩ	
Return Loss	- 27.3dB	

General Antenna Parameters and Design

Electrical Delay (one direction)	1.263 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.


The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: Z16-97091


Page 4 of 8

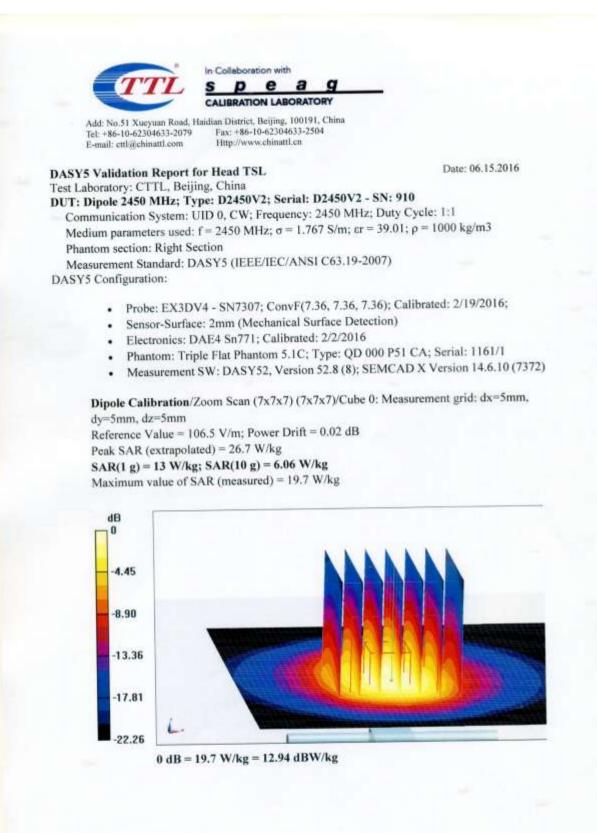


Certificate No: Z16-97091


Page 5 of 8

Shenzhen Zhongjian Nanfang Testing Co., Ltd. No. B-C, 1/F., Building 2, Laodong No.2 Industrial Park, Xixiang Road, Bao'an District, Shenzhen, Guangdong, China Telephone: +86 (0) 755 23118282 Fax: +86 (0) 755 23116366, E-mail: info@ccis-cb.com

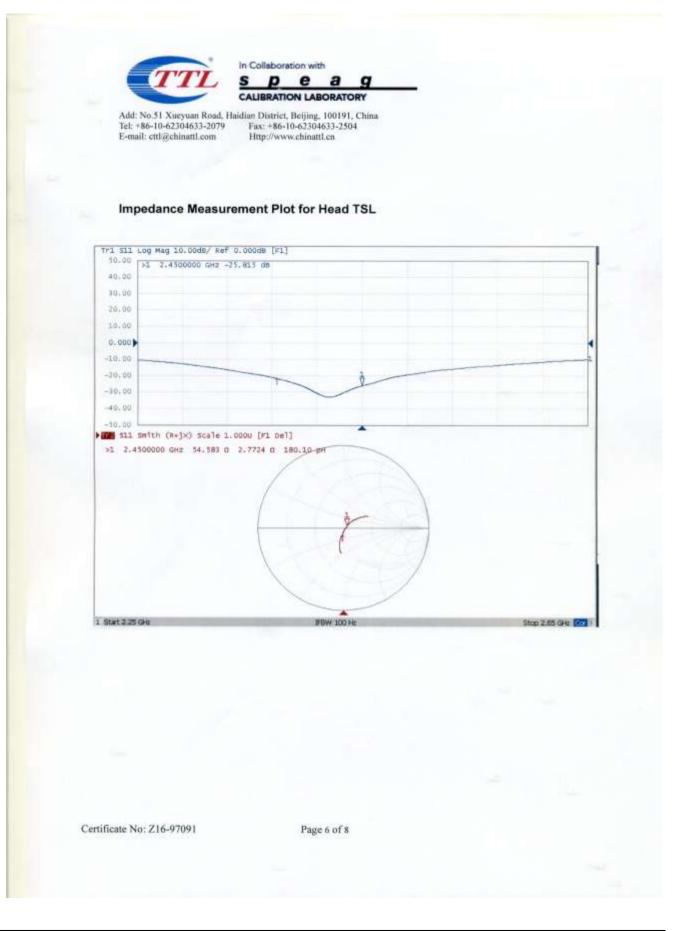

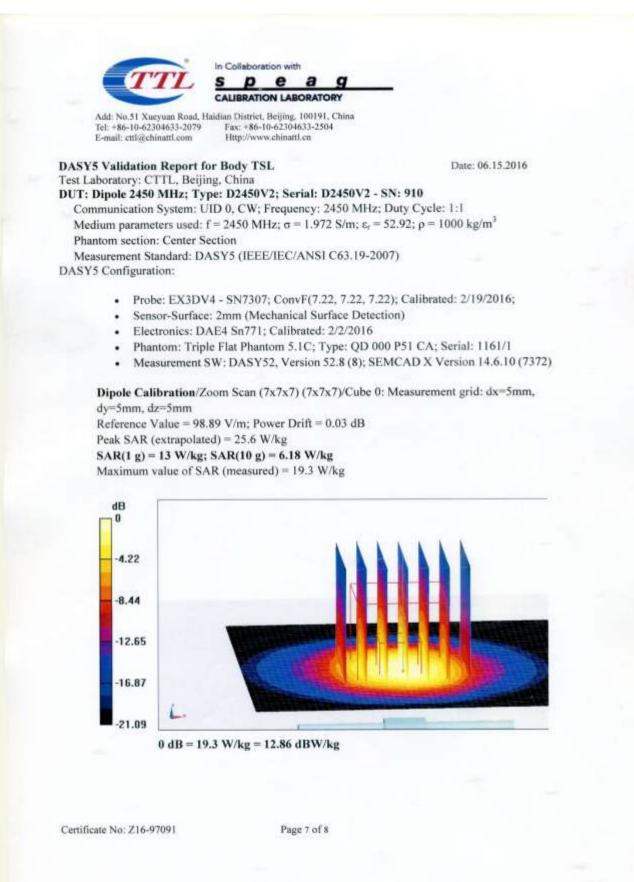

<u>CCIS</u>

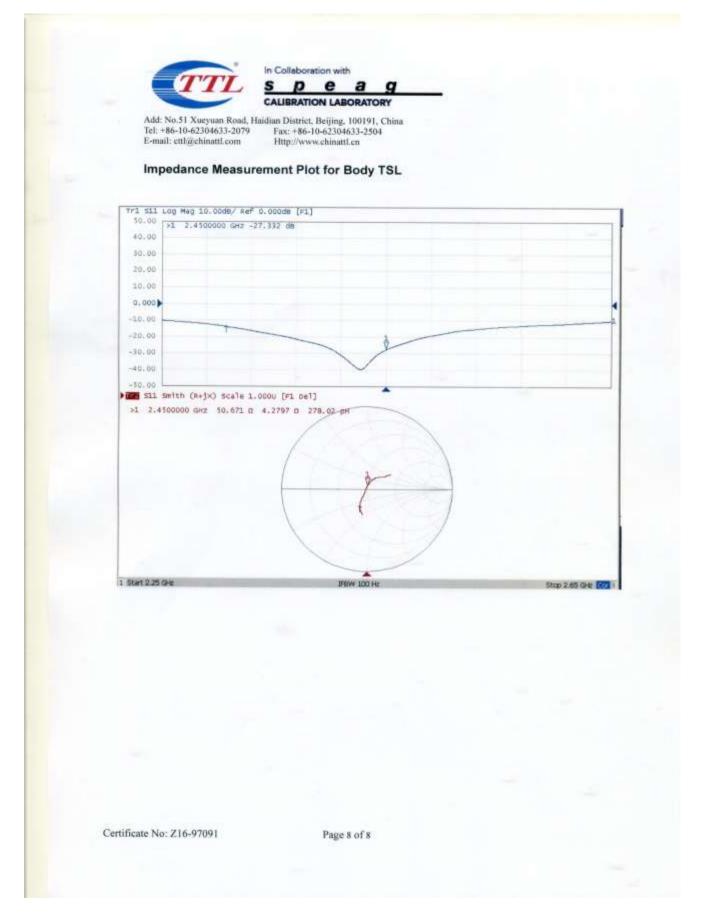



Dipole Impedance and Return Loss calibration Report

Object:	D2450V2 - SN: 910
Calibration Date:	June 10, 2018
Calibration reference:	IEEE Std 1528:2013, IEC 62209-1:2006, FCC KDB 865664 D01
Calibrated By:	Janet Wei (Janet Wei, SAR project engineer)
Reviewed By:	(Bruce Zhang, Technical manager)

Environment of Test Site

Temperature:	18 ~ 25°C
Humidity:	50~60% RH
Atmospheric Pressure:	1011 mbar


CH15

Price I

Cen Del Arp 16

Test Data

Measurement Plot for Head TSL In 2017

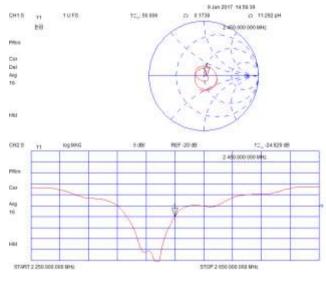



11 1078 T0_49329 D 2469 D 159342H



Measurement Plot for Body TSL In 2017



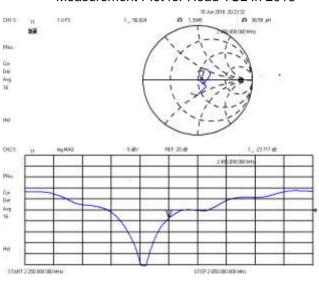

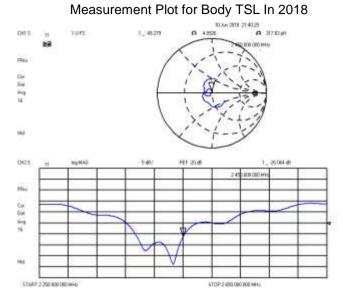

Measurement Plot for Head TSL In 2018

Comparison with Original report

Items	Calibrated By CCIS In 2017	Calibrated By CCIS In 2018	Deviation	Limit
Impendence for Head TSL	56.0Ω+0.17jΩ	56.82Ω+1.39jΩ	0.82Ω-1.22 jΩ	±5Ω
Return Loss for Head TSL	-24.9dB	-23.7dB	-4.8%	±20%(No less than 20 dB)
Impendence for Body TSL	49.63Ω+2.46jΩ	49.28Ω+4.89jΩ	-0.35Ω+2.43 jΩ	±5Ω
Return Loss for Body TSL	-25.6dB	-26.1dB	1.95%	±20%(No less than 20 dB)

Result

Compliance



Calibration information for DAE

the second s	TL s p	e a g	ころ ころ 日本
Add: No.51 Xuey Tel: +86-10-6230 E-mail: ettl@chir	yuan Road, Haidian Di 14633-2512 Fax:	strict, Beijing, 100191, China *86-10-62304633-2504 //www.chinattl.en	CALIBRATIO CNAS L0570
Client : CCI	Contraction Contraction		No: Z18-97054
CALIBRATION	ERTIFICA	ТЕ	
Dbject	DAE4	- SN: 1373	
Calibration Procedure(s)		1-002-01 ration Procedure for the Data Acquis x)	sition Electronics
Calibration date:	March	n 22, 2018	
measurements(SI). The r pages and are part of the	certificate.		
pages and are part of the	e certificate.	n the closed laboratory facility: enviro	onment temperature(22±3)℃ and
pages and are part of the All calibrations have be humidity<70%.	e certificate.		onment temperature(22±3)℃ and Scheduled Calibration
pages and are part of the All calibrations have be humidity<70%. Calibration Equipment us	e certificate.	I for calibration)	
bages and are part of the All calibrations have be numidity<70%. Calibration Equipment us Primary Standards	e certificate. een conducted ir sed (M&TE critica ID # C	I for calibration) Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
bages and are part of the All calibrations have be numidity<70%. Calibration Equipment us Primary Standards	e certificate. een conducted in sed (M&TE critica ID # C 1971018	I for calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-17 (CTTL, No.J17X05859) Function	Scheduled Calibration June-18
ages and are part of the All calibrations have be numidity<70%. Calibration Equipment us Primary Standards Process Calibrator 753	e certificate. een conducted in sed (M&TE critica ID # C 1971018 Name	I for calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-17 (CTTL, No.J17X05859) Function	Scheduled Calibration June-18
ages and are part of the All calibrations have be numidity<70%. Calibration Equipment us Primary Standards Process Calibrator 753 Calibrated by:	e certificate. een conducted in sed (M&TE critica ID # C 1971018 Name Yu Zongying	I for calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-17 (CTTL, No.J17X05859) Function SAR Test Engineer SAR Test Engineer	Scheduled Calibration June-18

Certificate No: Z18-97054

Page 1 of 3





Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504 E-mnil: ettl@chinattl.com Http://www.chinattl.cn

Glossary:

DAE Connector angle data acquisition electronics information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters:

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The report provide only calibration results for DAE, it does not contain other performance test results.

Certificate No: Z18-97054

Page 2 of 3





 Add: No.51 Xueyunn Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2512
 Fax: +86-10-62304633-2504

 E-mail: ettl@chinuttl.com
 Http://www.chinattl.cn

DC Voltage Measurement

A/D - Converter Re	solution nomin	nat		
High Range:	1LSB =	6.1µV,	full range =	-100+300 mV
Low Range:	1LSB =	61nV .	full range =	-1+3mV
DASY measuremen	t parameters	Auto Zero	Time: 3 sec; Meas	uring time: 3 sec

Calibration Factors	x	Y	z
High Range	403.902 ± 0.15% (k=2)	403.864 ± 0.15% (k=2)	404.160 ± 0.15% (k=2)
Low Range	3.98605 ± 0.7% (k=2)	4.00729 ± 0.7% (k=2)	4.01146 ± 0.7% (k=2)

Connector Angle

Connector Angle to be used in DASY system	219.5°±1°

Certificate No: Z18-97054

Page 3 of 3

-----End of Report-----