		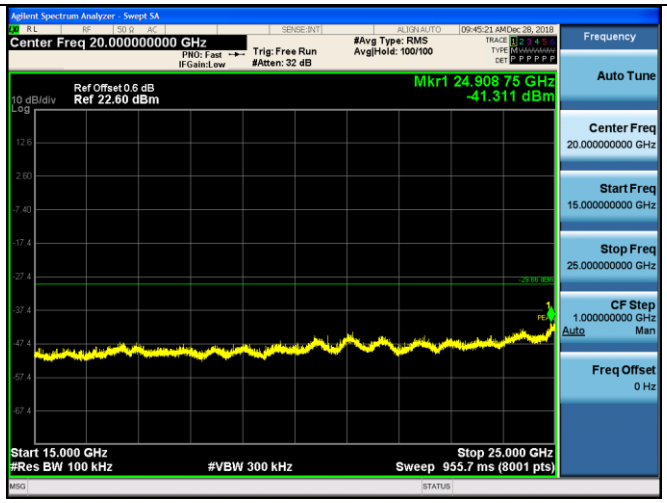

11B_HCH_Graphs		
Pref/11B/HCH		
Puw/11B/HCH		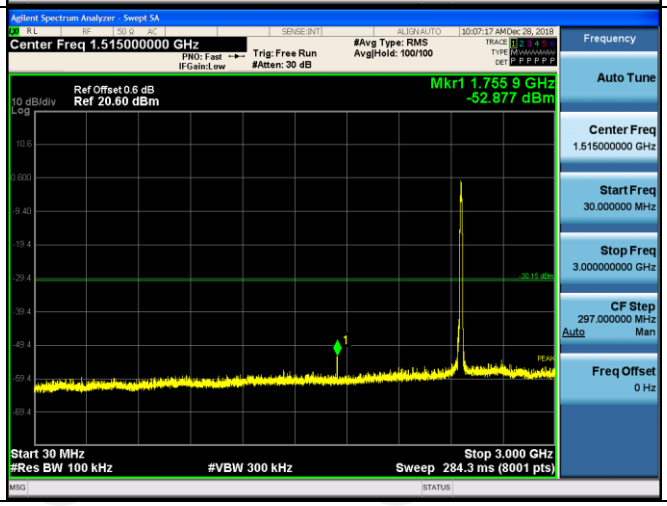

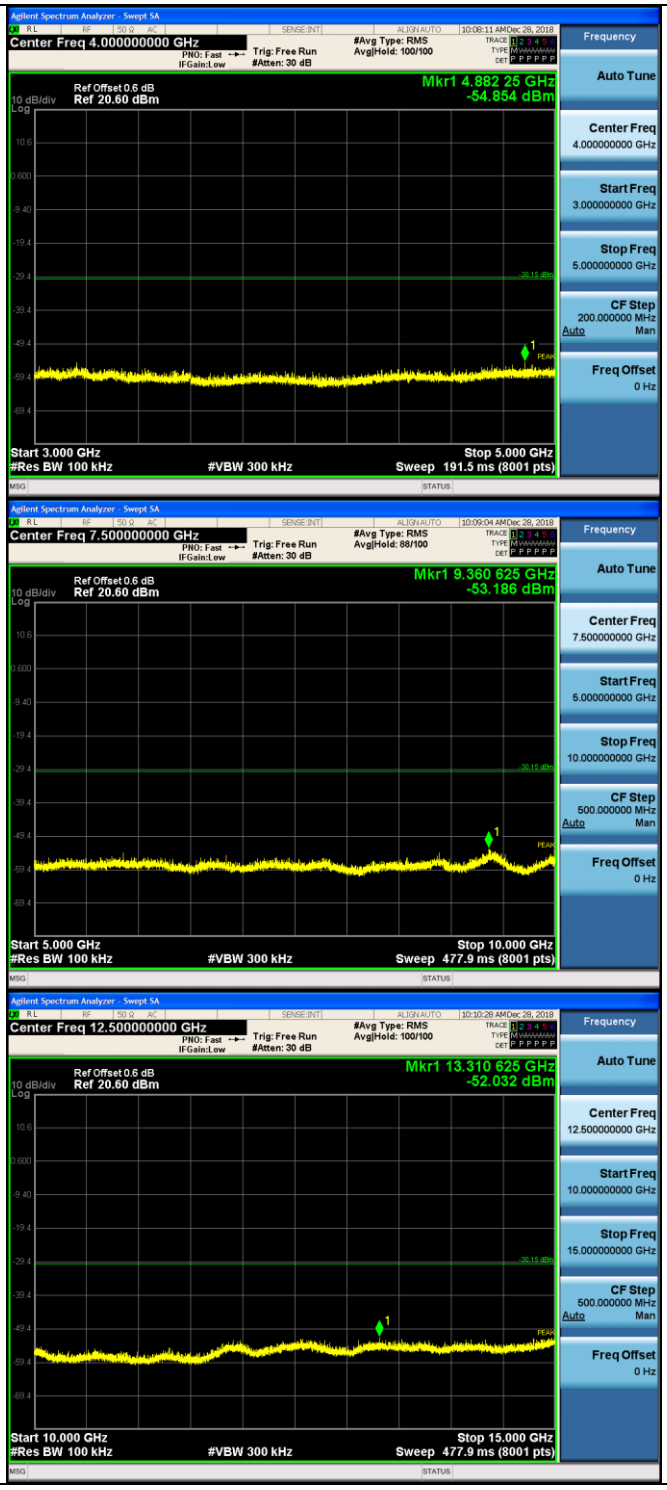
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Ref Offset 0.6 dB
10 dB/div
Ref 20.60 dBm
Mkr1 4.882 25 GHz
-54.854 dBm
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)
Frequency
Auto Tune
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz
Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 88/100
Ref Offset 0.6 dB
10 dB/div
Ref 20.60 dBm
Mkr1 9.360 625 GHz
-53.186 dBm
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)
Frequency
Auto Tune
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Ref Offset 0.6 dB
10 dB/div
Ref 20.60 dBm
Mkr1 13.310 625 GHz
-52.032 dBm
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)
Frequency
Auto Tune
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz

		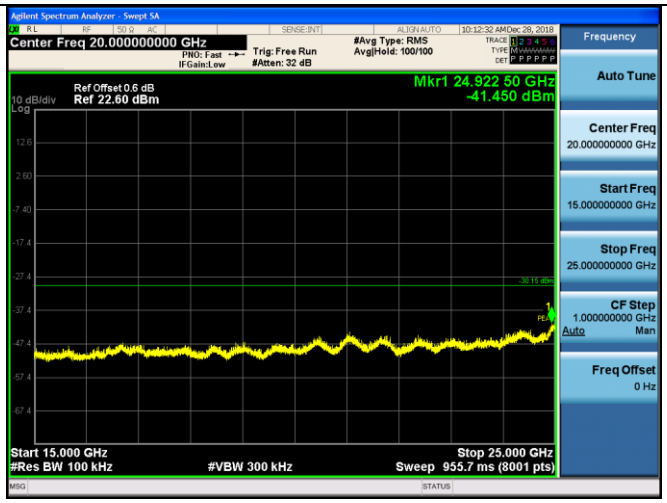

11G_LCH_Graphs		
Pref/11G/LCH		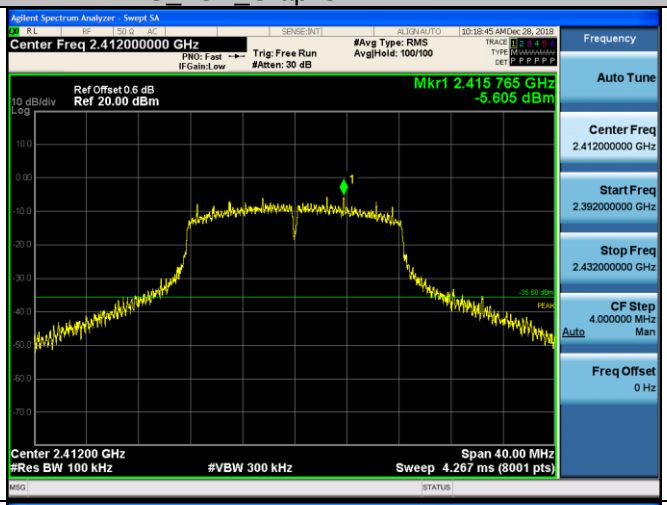
Puw/11G/LCH		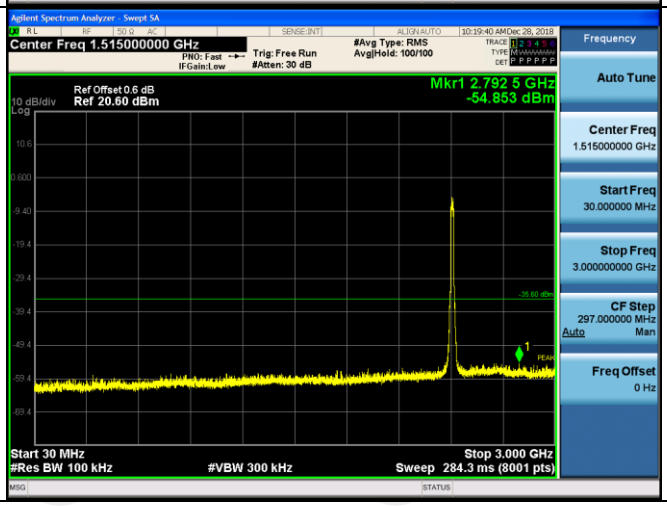

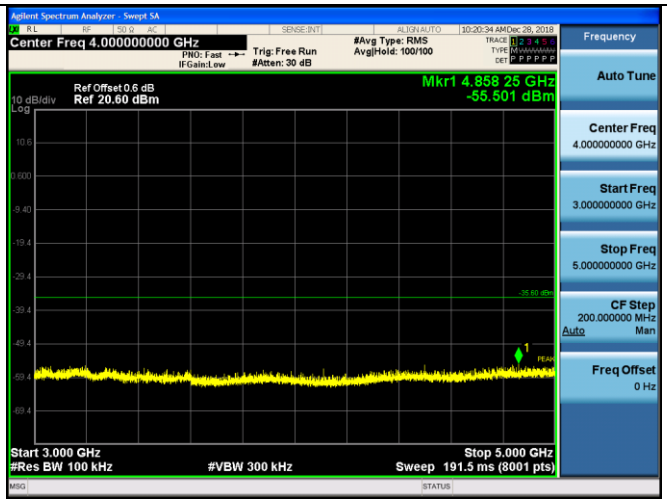
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
10:20:34 AM Dec 28, 2018
Frequency
Auto Tune
Ref Offset 0.6 dB
10 dB/div
Ref 20.60 dBm
Mkr1 4.858 25 GHz
-55.501 dBm
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)

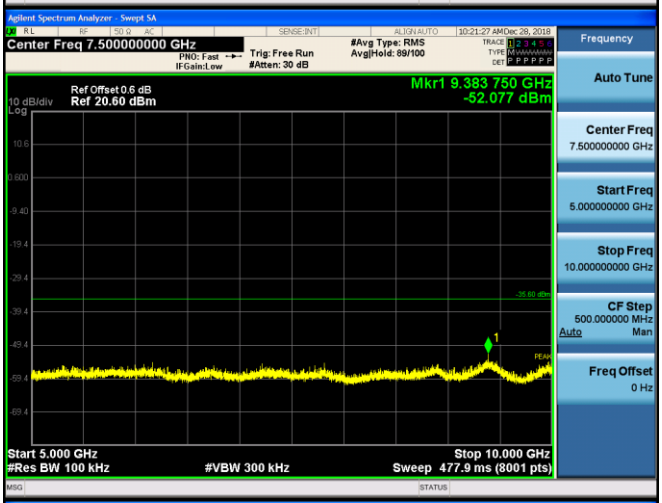
Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 89/100
10:21:27 AM Dec 28, 2018
Frequency
Auto Tune
Ref Offset 0.6 dB
10 dB/div
Ref 20.60 dBm
Mkr1 9.383 750 GHz
-52.077 dBm
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)

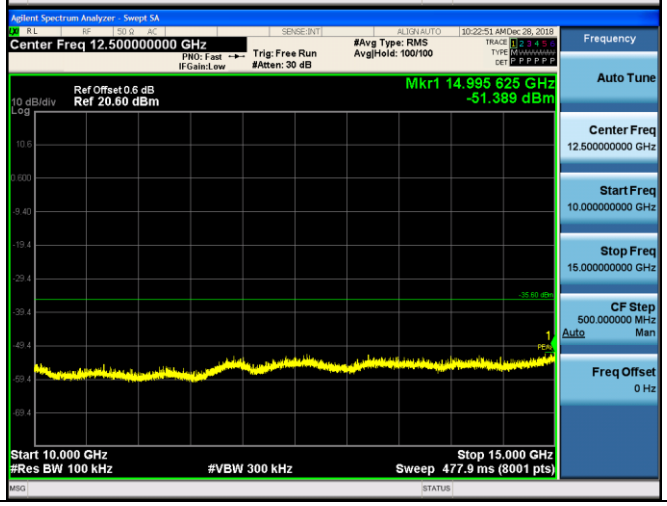
Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
10:22:51 AM Dec 28, 2018
Frequency
Auto Tune
Ref Offset 0.6 dB
10 dB/div
Ref 20.60 dBm
Mkr1 14.995 625 GHz
-51.389 dBm
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)

		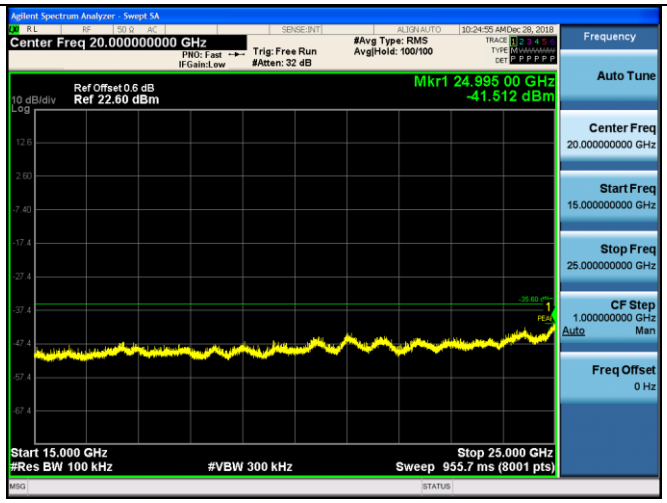

11G_MCH_Graphs		
Pref/11G/MCH		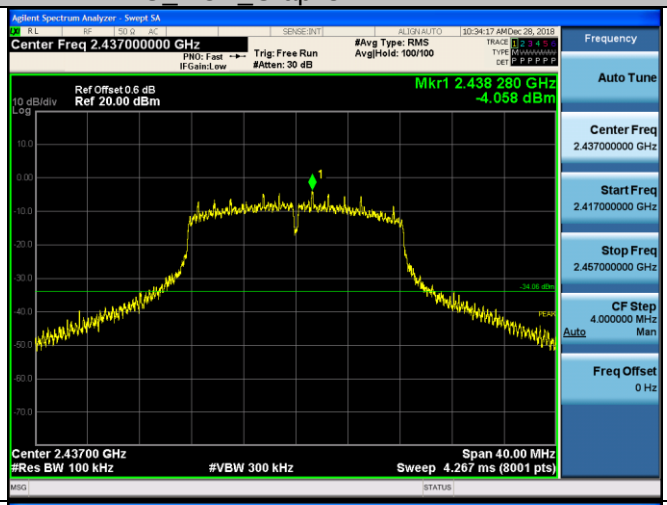
Puw/11G/MCH		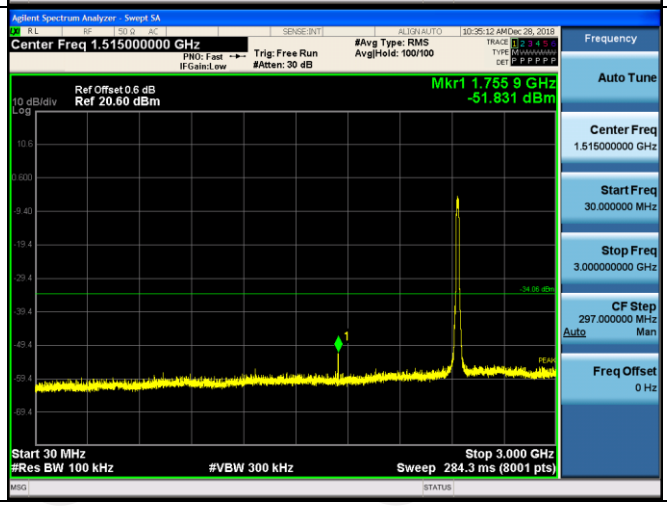

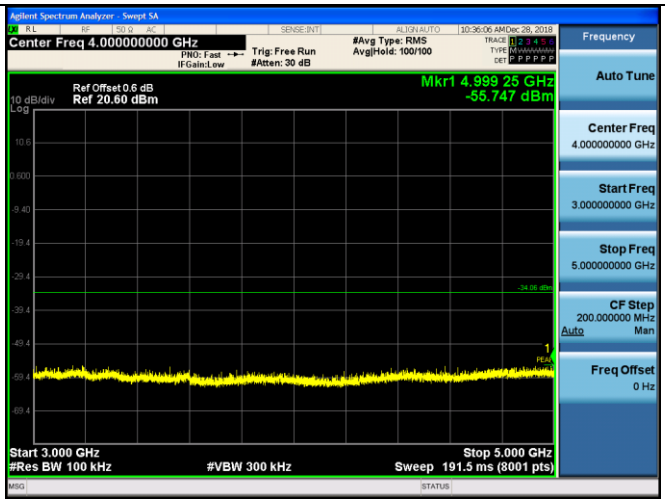
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
10:36:06 AM Dec 28, 2018
Frequency
Ref Offset 0.6 dB
10 dB/div
Ref 20.60 dBm
Mkr1 4.999 25 GHz
-55.747 dBm
Auto Tune
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)

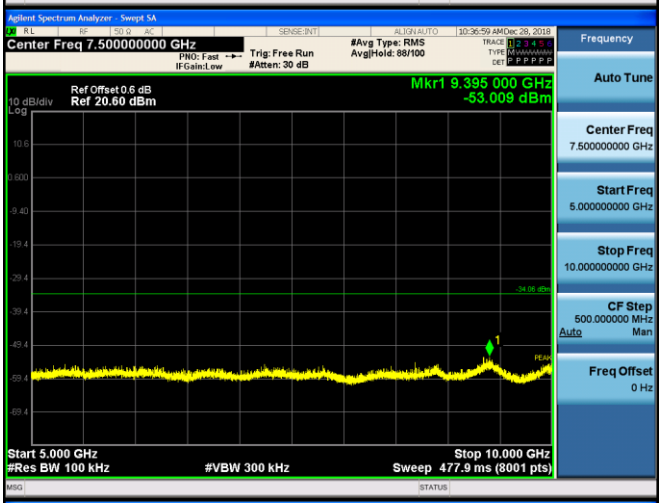
Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 88/100
10:36:59 AM Dec 28, 2018
Frequency
Ref Offset 0.6 dB
10 dB/div
Ref 20.60 dBm
Mkr1 9.395 000 GHz
-53.009 dBm
Auto Tune
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)


Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
10:38:23 AM Dec 28, 2018
Frequency
Ref Offset 0.6 dB
10 dB/div
Ref 20.60 dBm
Mkr1 14.890 625 GHz
-51.047 dBm
Auto Tune
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)

		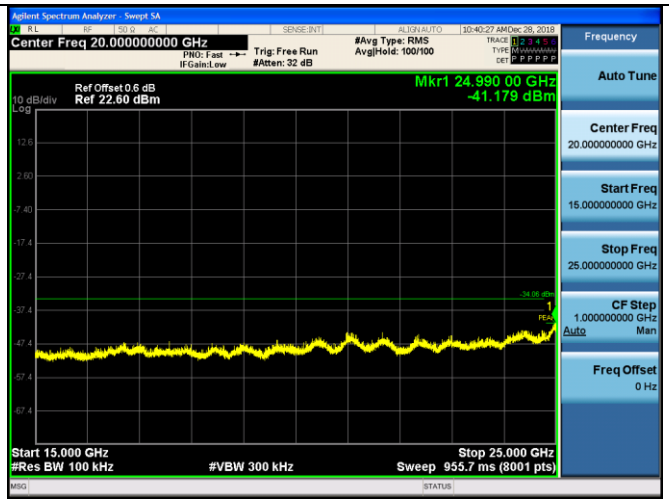

11G_HCH_Graphs		
Pref/11G/HCH		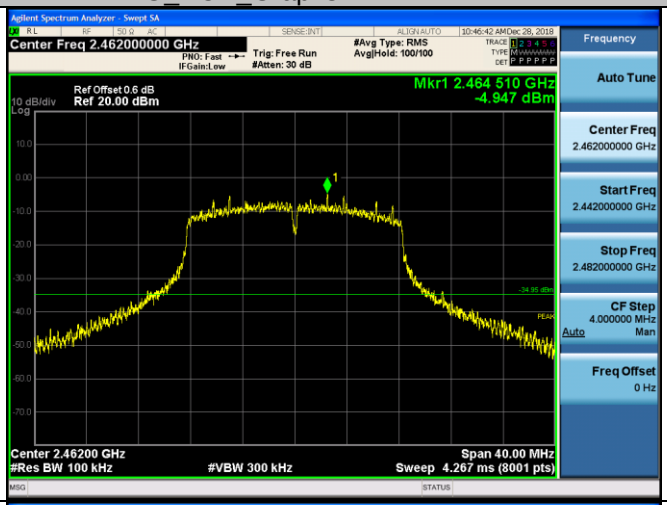
Puw/11G/HCH		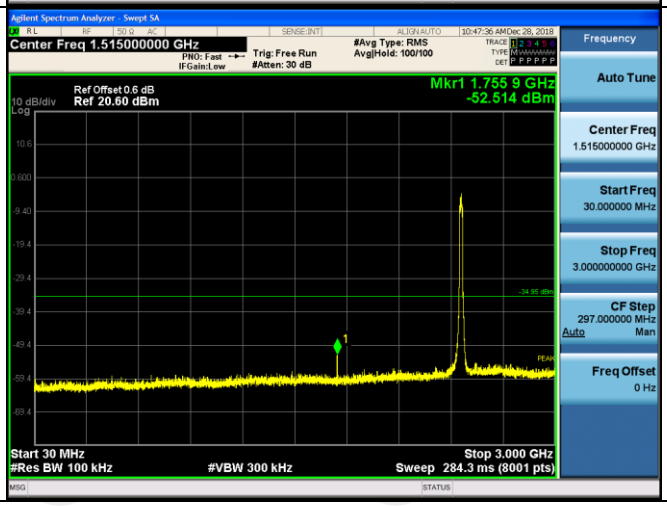

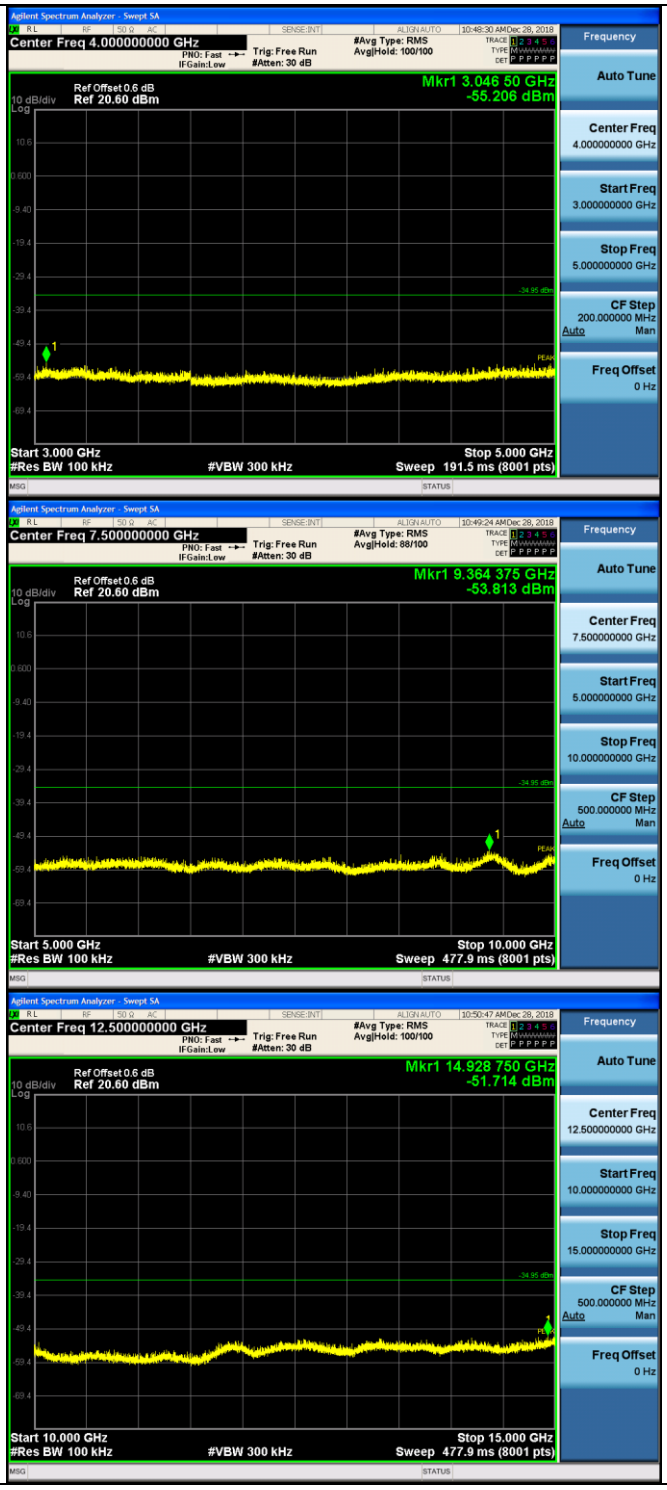
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Ref Offset 0.6 dB
10 dB/div
Ref 20.60 dBm
Mkr1 3.046 50 GHz
-55.206 dBm
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)
Frequency
Auto Tune
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz
Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 88/100
Ref Offset 0.6 dB
10 dB/div
Ref 20.60 dBm
Mkr1 9.364 375 GHz
-53.813 dBm
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)
Frequency
Auto Tune
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
Ref Offset 0.6 dB
10 dB/div
Ref 20.60 dBm
Mkr1 14.928 750 GHz
-51.714 dBm
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)
Frequency
Auto Tune
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz

		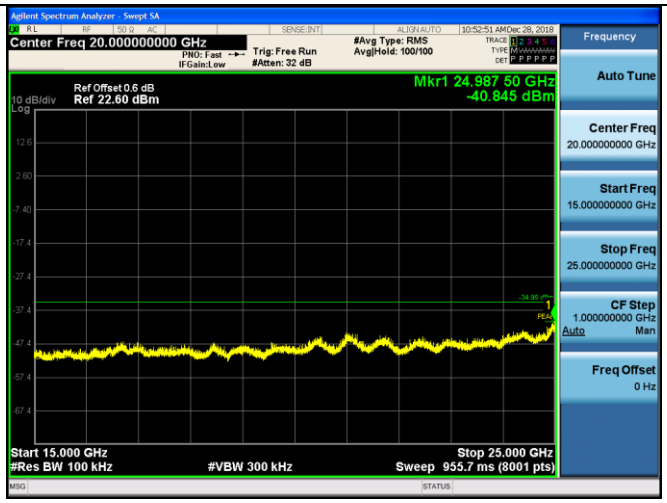

11N20SISO_LCH_Graphs		
Pref/11N20SISO/LCH		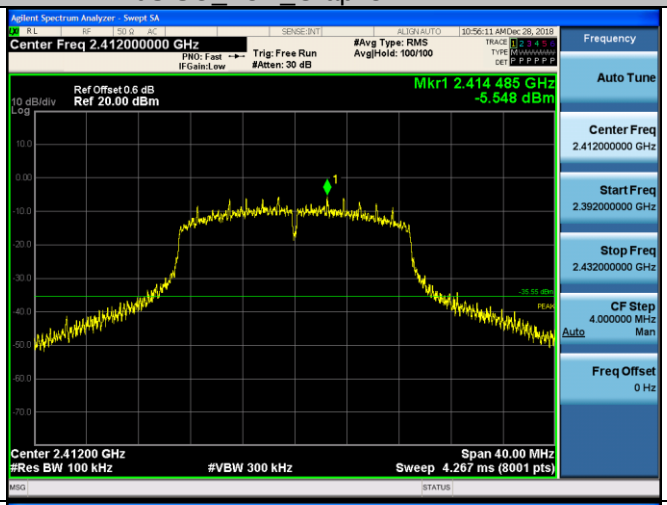
/11N20SISO/LCH		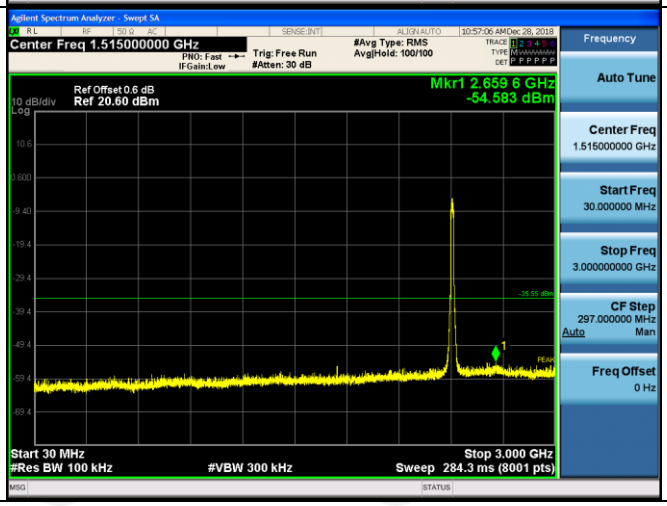

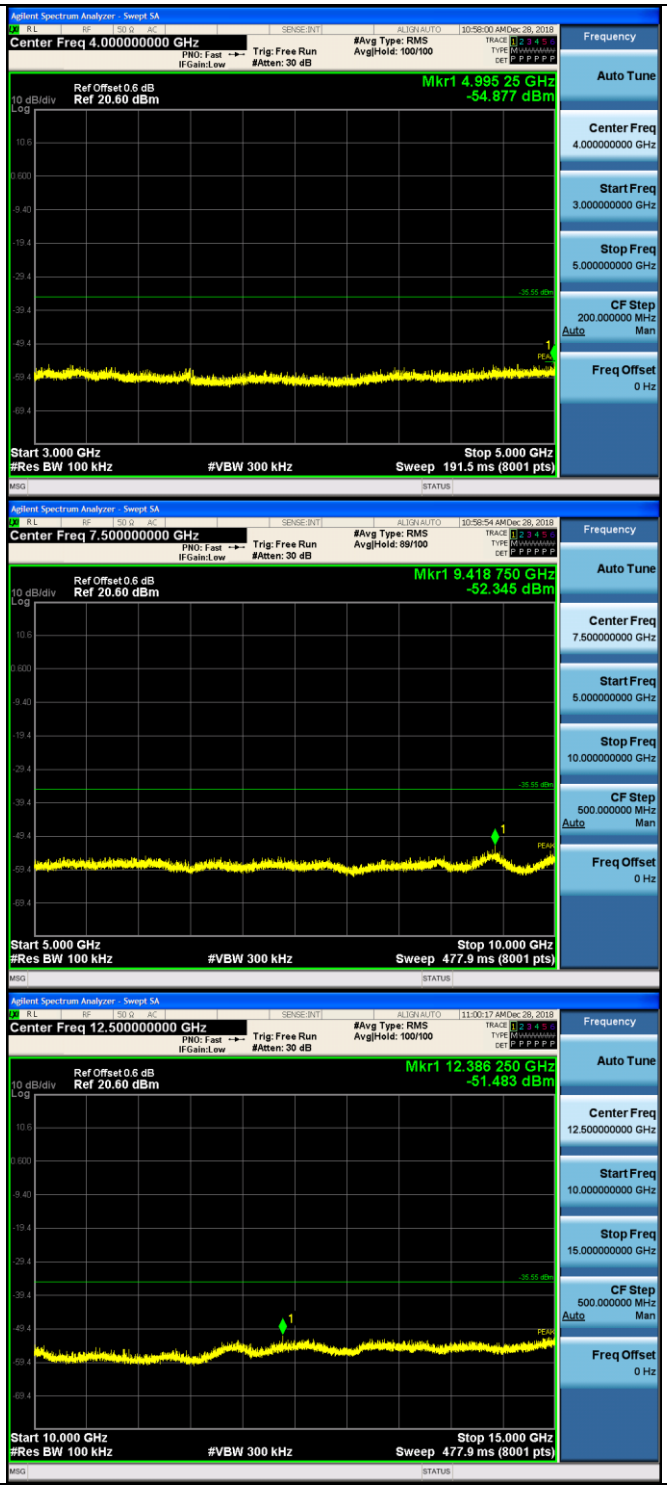
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
10:58:00 AM Dec 28, 2018
Frequency
Auto Tune
Ref Offset 0.6 dB
10 dB/div
Ref 20.60 dBm
Log
Mkr1 4.995 25 GHz
-54.877 dBm
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)
Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 89/100
10:58:54 AM Dec 28, 2018
Frequency
Auto Tune
Ref Offset 0.6 dB
10 dB/div
Ref 20.60 dBm
Log
Mkr1 9.418 750 GHz
-52.345 dBm
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)
Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
11:00:17 AM Dec 28, 2018
Frequency
Auto Tune
Ref Offset 0.6 dB
10 dB/div
Ref 20.60 dBm
Log
Mkr1 12.386 250 GHz
-51.483 dBm
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)

		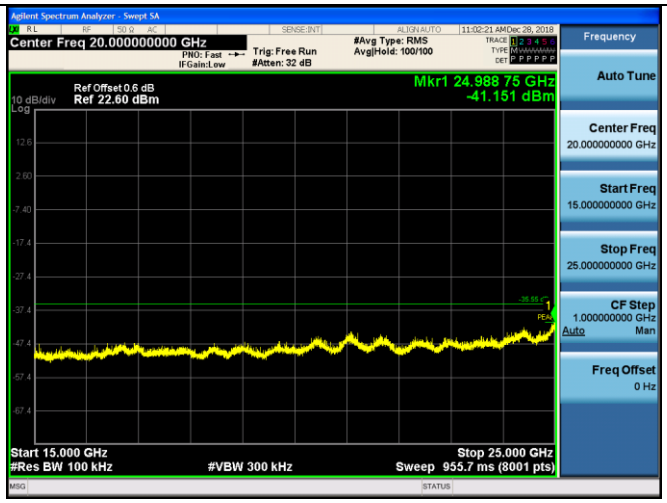

11N20SISO_MCH_Graphs		
Pref/11N20SISO/MCH		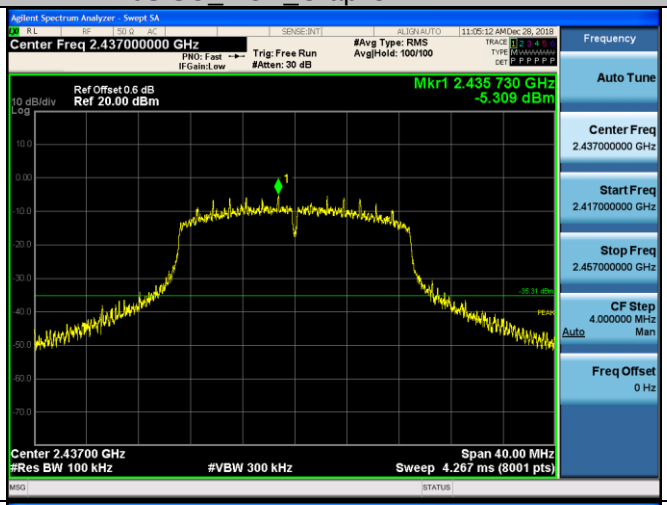
Puw/11N20SISO/MCH		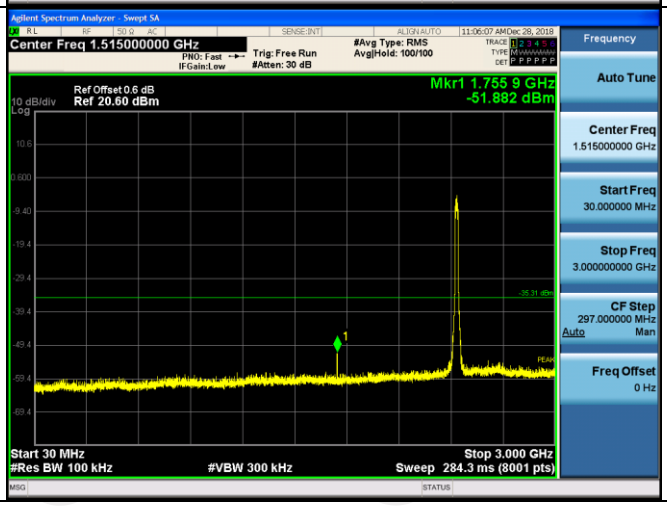

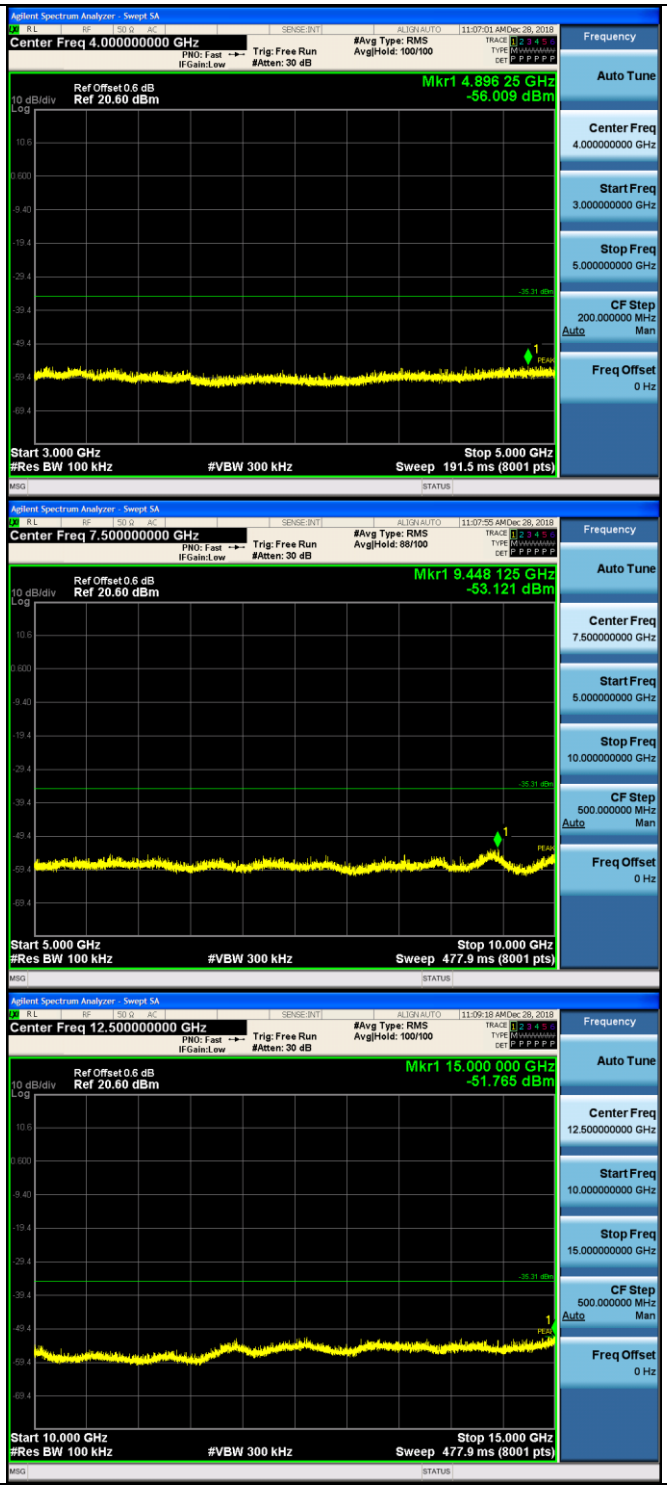
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
11:07:01 AM Dec 28, 2018
Frequency
Mkr1 4.896 25 GHz
-56.009 dBm
Ref Offset 0.6 dB
10 dB/div
Ref 20.60 dBm
Log
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)
Auto Tune
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz
MSG
STATUS
Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 88/100
11:07:55 AM Dec 28, 2018
Frequency
Mkr1 9.448 125 GHz
-53.121 dBm
Ref Offset 0.6 dB
10 dB/div
Ref 20.60 dBm
Log
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)
Auto Tune
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
MSG
STATUS
Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
11:09:18 AM Dec 28, 2018
Frequency
Mkr1 15.000 000 GHz
-51.765 dBm
Ref Offset 0.6 dB
10 dB/div
Ref 20.60 dBm
Log
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)
Auto Tune
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
MSG
STATUS

		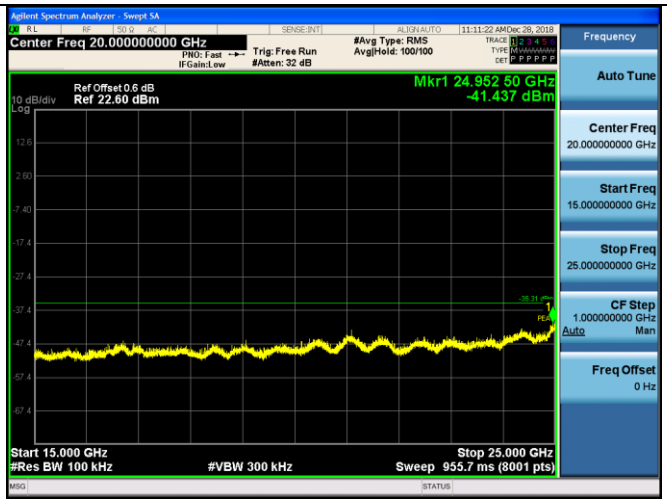

11N20SISO_HCH_Graphs		
Pref/11N20SISO/HCH		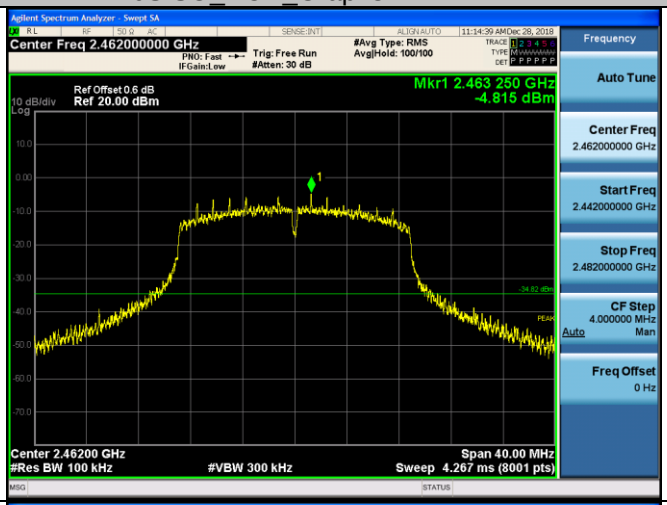
Puw/11N20SISO/HCH		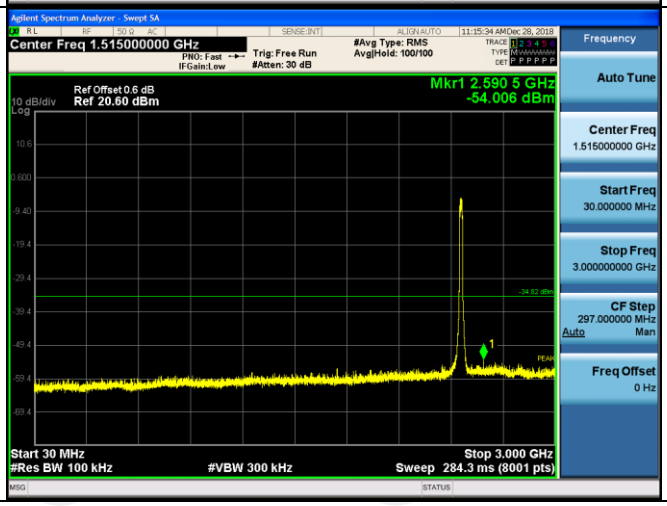

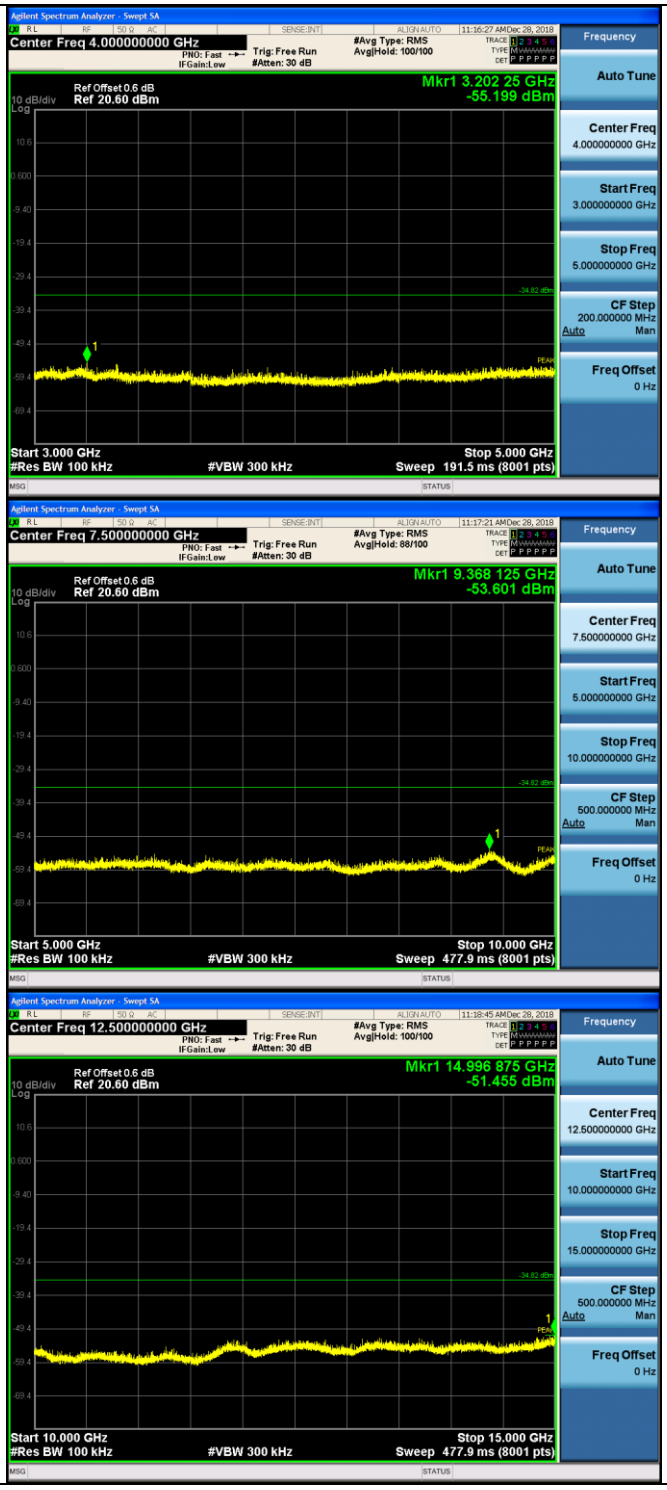
Agilent Spectrum Analyzer - Swept SA
Center Freq 4.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
11:16:27 AM Dec 28, 2018
Frequency
Auto Tune
Ref Offset 0.6 dB
10 dB/div
Log
Ref 20.60 dBm
Mkr1 3.202 25 GHz
-55.199 dBm
Center Freq
4.000000000 GHz
Start Freq
3.000000000 GHz
Stop Freq
5.000000000 GHz
CF Step
200.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 3.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 5.000 GHz
Sweep 191.5 ms (8001 pts)
Agilent Spectrum Analyzer - Swept SA
Center Freq 7.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 88/100
11:17:21 AM Dec 28, 2018
Frequency
Auto Tune
Ref Offset 0.6 dB
10 dB/div
Log
Ref 20.60 dBm
Mkr1 9.368 125 GHz
-53.601 dBm
Center Freq
7.500000000 GHz
Start Freq
5.000000000 GHz
Stop Freq
10.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 5.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 10.000 GHz
Sweep 477.9 ms (8001 pts)
Agilent Spectrum Analyzer - Swept SA
Center Freq 12.500000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 30 dB
#Avg Type: RMS
Avg|Hold: 100/100
11:18:45 AM Dec 28, 2018
Frequency
Auto Tune
Ref Offset 0.6 dB
10 dB/div
Log
Ref 20.60 dBm
Mkr1 14.996 875 GHz
-51.455 dBm
Center Freq
12.500000000 GHz
Start Freq
10.000000000 GHz
Stop Freq
15.000000000 GHz
CF Step
500.000000 MHz
Auto
Man
Freq Offset
0 Hz
Start 10.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 15.000 GHz
Sweep 477.9 ms (8001 pts)

		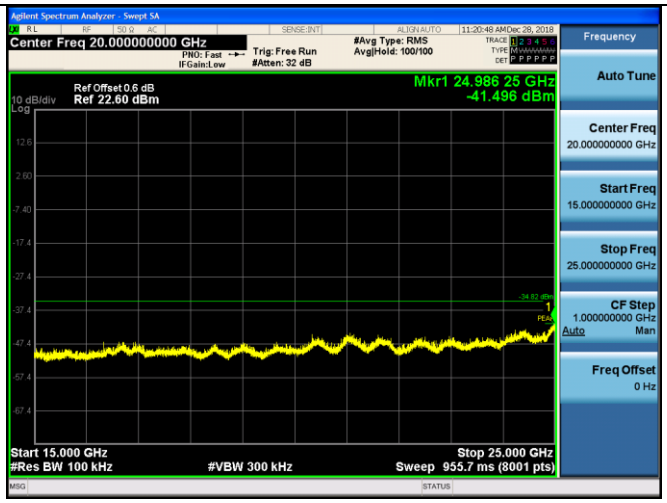

Agilent Spectrum Analyzer - Swept SA
Center Freq 20.000000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 32 dB
#Avg Type: RMS
Avg|Hold: 100/100
11:20:48 AM Dec 28, 2018
Ref Offset 0.6 dB
10 dB/div
Log
Ref 22.60 dBm
Mkr1 24.986 25 GHz
-41.496 dBm
Start 15.000 GHz
#Res BW 100 kHz
#VBW 300 kHz
Stop 25.000 GHz
Sweep 955.7 ms (8001 pts)
Frequency
Auto Tune
Center Freq
20.000000000 GHz
Start Freq
15.000000000 GHz
Stop Freq
25.000000000 GHz
CF Step
1.000000000 GHz
Auto
Man
Freq Offset
0 Hz

Power Spectral Density

Result Table

Mode	Channel	Meas.Level [dBm]	Verdict
11B	LCH	-15.828	PASS
11B	MCH	-14.292	PASS
11B	HCH	-16.206	PASS
11G	LCH	-20.708	PASS
11G	MCH	-20.105	PASS
11G	HCH	-21.545	PASS
11N20SISO	LCH	-21.779	PASS
11N20SISO	MCH	-21.541	PASS
11N20SISO	HCH	-20.990	PASS

Test Graph

Graphs			
11B/LCH			
11B/MCH			

11B/HCH			
11G/LCH			
11G/MCH			

11G/HCH			
11N20SISO/LCH			
11N20SISO/MCH			

11N20SISO/HCH			

Appendix B: Photographs of Test Setup

Refer to test report TCT181226E037

Appendix C: Photographs of EUT

Refer to test report TCT181226E037

*****END OF REPORT*****