

展开尺寸: 254x304.8 mm, R角: 6.35 mm

成品尺寸: 254x152.4 mm, R角: 6.35 mm

C 52.7,M 0, Y 34.52, K 0

C 38.67,M 31.25,Y 32.03,K 0.39

C 0,M 0,Y 0,K 80

254mm

Let's get started.



152.4mm

152.4mm



CAUTION

The manufacturer is not responsible for any interference or damage caused by unauthorized modifications to this equipment. UV light can be irritating to the eyes and skin. This device has been designed to contain UV exposure. Do not attempt to look directly at the UV lamp while it is on.

FCC STATEMENT

WARNING: CHANGES OR MODIFICATIONS TO THIS UNIT NOT EXPRESSLY APPROVED BY THE PARTY RESPONSIBLE FOR COMPLIANCE COULD VOID THE USER'S AUTHORITY TO OPERATE THE EQUIPMENT.

NOTE: THIS EQUIPMENT HAS BEEN TESTED AND FOUND TO COMPLY WITH THE LIMITS FOR A CLASS B DIGITAL DEVICE, PURSUANT TO PART 15 AND PART 18 OF THE FCC RULES. THESE LIMITS ARE DESIGNED TO PROVIDE REASONABLE PROTECTION AGAINST HARMFUL INTERFERENCE IN A RESIDENTIAL INSTALLATION. THIS EQUIPMENT GENERATES, USES AND CAN RADIATE RADIO FREQUENCY ENERGY AND, IF NOT INSTALLED AND USED IN ACCORDANCE WITH THE INSTRUCTIONS, MAY CAUSE HARMFUL INTERFERENCE TO RADIO COMMUNICATIONS.

HOWEVER, THERE IS NO GUARANTEE THAT INTERFERENCE WILL NOT OCCUR IN A PARTICULAR INSTALLATION. IF THIS EQUIPMENT DOES CAUSE HARMFUL INTERFERENCE TO RADIO OR TELEVISION RECEPTION, WHICH CAN BE DETERMINED BY TURNING THE EQUIPMENT OFF AND ON, THE USER IS ENCOURAGED TO TRY TO CORRECT THE INTERFERENCE BY ONE OR MORE OF THE FOLLOWING MEASURES: REORIENT OR RELOCATE THE RECEIVING ANTENNA.; INCREASE THE SEPARATION BETWEEN THE EQUIPMENT AND RECEIVER.; CONNECT THE EQUIPMENT INTO AN OUTLET ON A CIRCUIT DIFFERENT FROM THAT TO WHICH THE RECEIVER IS CONNECTED.; CONSULT THE DEALER OR AN EXPERIENCED RADIO/TV TECHNICIAN FOR HELP.

THIS PRODUCT MAY CAUSE INTERFERENCE TO RADIO EQUIPMENT AND SHOULD NOT BE INSTALLED NEAR MARITIME SAFETY COMMUNICATIONS EQUIPMENT OR OTHER CRITICAL NAVIGATION OR COMMUNICATIONS EQUIPMENT OPERATING BETWEEN 0.45-30 MHZ.

FCC RADIATION EXPOSURE STATEMENT

THIS EQUIPMENT COMPLIES WITH THE FCC RF RADIATION EXPOSURE LIMITS SET FORTH FOR AN UNCONTROLLED ENVIRONMENT. THIS EQUIPMENT SHOULD BE INSTALLED AND OPERATED WITH A MINIMUM DISTANCE OF 20 CENTIMETERS BETWEEN THE RADIATOR AND YOUR BODY. THIS EQUIPMENT COMPLIES WITH PART 15 AND PART 18 OF THE FCC RULES. OPERATION IS SUBJECT TO THE FOLLOWING TWO CONDITIONS: (1) THIS DEVICE MAY NOT CAUSE HARMFUL INTERFERENCE. (2) THIS DEVICE MUST ACCEPT ANY INTERFERENCE RECEIVED INCLUDING INTERFERENCE THAT MAY CAUSE UNDESIRABLE OPERATION.



PhoneSoap LLC
3400 N 1200 W Suite 204
Lehi, UT 84043
medsales@phonesoap.com
(866) 432-0525


We stand behind the quality of our product. We offer a 1-year limited warranty on every PhoneSoap product as well as a lifetime warranty on the UV-C bulbs. Exclusions and limitations may apply.

To view the full warranty and return policy visit:
phonesoap.com/warranty


By using this product, you agree to the Legal and Privacy Policies as stated on our website at:
phonesoap.com/legal

Please contact us with any questions or concerns.
www.phonesoap.com/contact


Ready to sanitize, right out of the box.

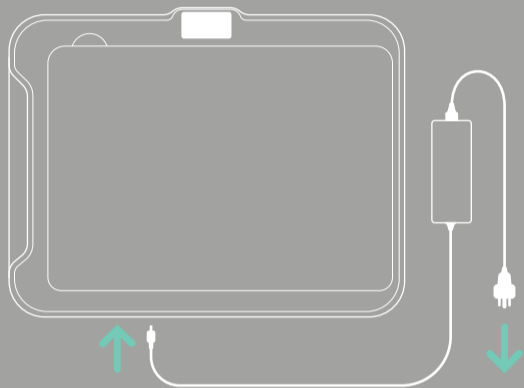

Plug Med Pro into power with provided cord.

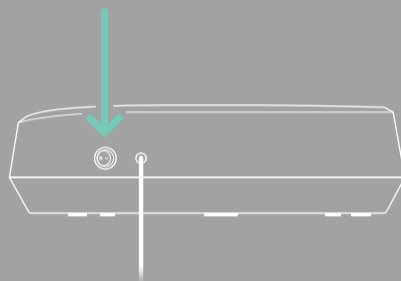

Flip switch to start Med Pro unit.

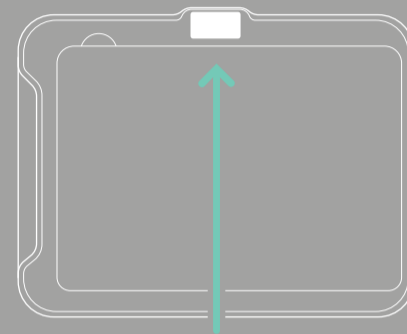


Follow on-screen instructions to complete set-up and begin sanitizing.

Power cables with magnetic ring must be used with this unit to ensure compliance with the Class B FCC limits.




For an instructional video and language-specific instructions, scan the QR code or visit the following link:

phonesoap.com/med_pro_setup

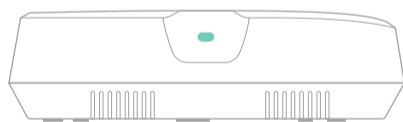

Motion Sensor

- Your primary form of device input. Waving your hand over this sensor will activate disinfection sequence, open sanitizing bay, and confirm settings.

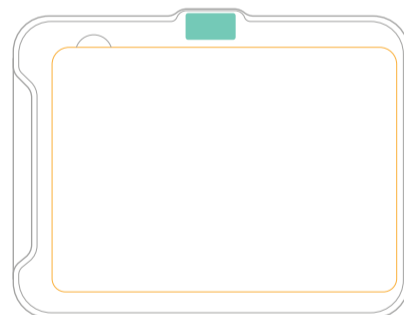


OLED Display

- Instructions and notifications will display here.
- **Motorized Door**
Provides a completely touchless experience.



On/Off Switch

- Use this switch to power on and off the unit.
- **Power Adapter**
Plug in provided power adapter to power unit.

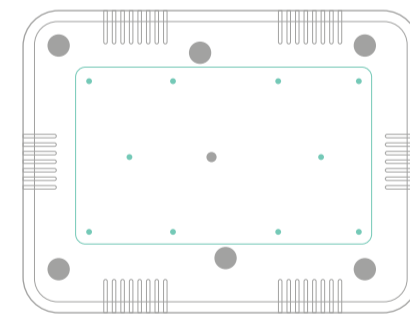

Mounting Plate

- Location for optional mounting plate for use with wall mount, desk stand, and roller stands.

Need help?

If you are experiencing trouble, please contact us:
medsales@phonesoap.com (866) 432-0525