


# Compuray Scan

REF

SN



Manufactured

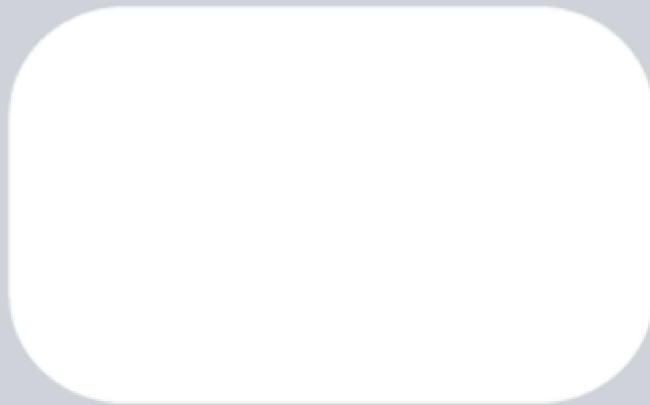

Product Name Intraoral Imaging Plate System

Model Name Compuray Scan

24V  2A

CLASS 1 LASER PRODUCT  
APPAREIL A LASER DE CLASSE 1


COMPLIES WITH 21 CFR 1040.10  
AND 1040.11 EXCEPT FOR  
DEVIATIONS PURSUANT TO LASER  
NOTICE NO. 50, DATED JUNE 24, 2007.



Carestream Dental LLC  
3625 Cumberland Boulevard, Suite 700  
Atlanta GA USA 30339  
Made in China



AREA	REV	DATE	DESCRIPTION	SIGNATURE
	A	2019-04-02	RELEASE TO PRODUCTION.	HATA GAO

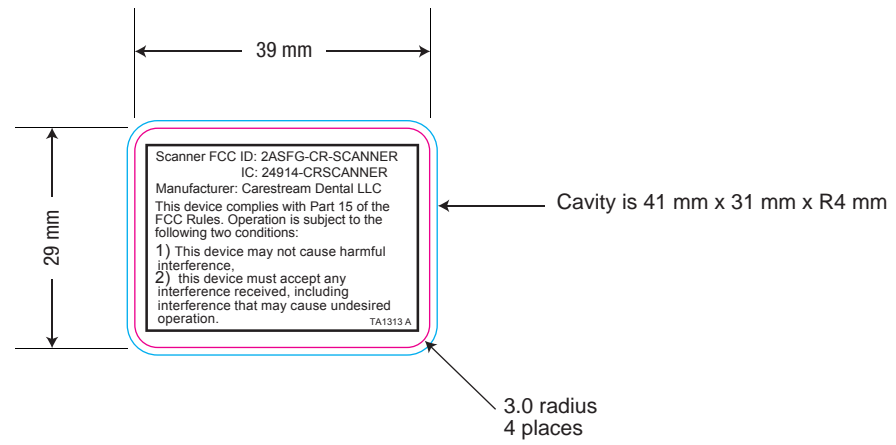

- PMS White
- PMS Black
- DIE LINE

NOTES:

1. MATERIAL: GENERAL ELECTRIC LEXAN 8010, 0.254mm HIGH GLOSS, POLYCARBONATE WITH 3M 468MP ADHESIVE OR 3M #9505 ADHESIVE.
2. LABEL TO BE MADE PER ELECTRONIC ARTWORK SUPPLIED BY CARESTREAM DENTAL LLC.
3. OVERLAY MATERIAL MUST MEET THE REQUIREMENTS OF UL STANDARD 969 (MARKING AND LABELING SYSTEMS [PGDQ2]).
4. SUPPLIER ARTWORK TO BE APPROVED BY CUSTOMER PRIOR TO PRINTING.
5. INSPECTION REQUIREMENTS, IF SHOWN ON DRAWING:
  - A. INDICATES PRIMARY INSPECTION DIMENSION.
  - B. GEOMETRIC TOLERANCES ARE PRIMARY INSPECTION ATTRIBUTES.
  - C. REFERENCE DIMENSIONS ARE ENCLOSED IN PARENTHESES ( ). DO NOT INSPECT REFERENCE DIMENSIONS.

SUPPLIER REQUIREMENTS:

1. SUPPLIER MUST USE UL RECOGNIZED PRINTING PROCESS PER UL STANDARD 969 (MARKING AND LABELING SYSTEMS [PGDQ2]).
2. UL RECOGNIZED SUPPLIERS MUST INDICATE COMPLIANCE TO UL STANDARD 969 BY MARKING THE SMALLEST LOT SIZE WITH THE FOLLOWING:
  - A. UL FILE NUMBER
  - B. SUPPLIER'S NAME AND/OR TRADEMARK
  - C. CARESTREAM HEALTH INC. PART NUMBER AND REVISION
  - D. DATE OF PRODUCTION.

CARESTREAM DENTAL LLC GLOBAL R&D CENTER (SHANGHAI)		TRACE FILE :		MATERIAL			
		DESIGN SW:					
DATUM PLANE PRIORITY A, B, C UNLESS SPECIFIED		CONTRACT NO:		NAME PRODUCT LABEL-LABEL FCC STATEMENT, CS 7600 CSD			
		DESIGN HATA GAO	DATE 2019-04-02				
UNIT : mm	METER	AUDITING	DATE	BUY LEV	SIZE	PART NUMBER TA1313	REV A
UNSPECIFIED TOL.		APPROVE	DATE	SCALE: 1: 1	PROJECT: CS 7600	SHEET 1 OF 1	
ANGLE ±1		0 ±0.5					
0.0 ±0.13		0.00 ±NA					