





CS 3800 Laser Label

AREA	REV	DATE	DESCRIPTION	SIGNATURE
	A	2020-03-27	INITIAL RELEASE	HATA GAO
	B	2020-10-27	UPDATE MODEL	HATA GAO
	C	2020-12-31	COMBINE UDI CODE	HATA GAO

Intraoral Scanner
Model : CS 3800 Wireless


SN



MD   



(01) 60192155943065
(21)EDLA0011

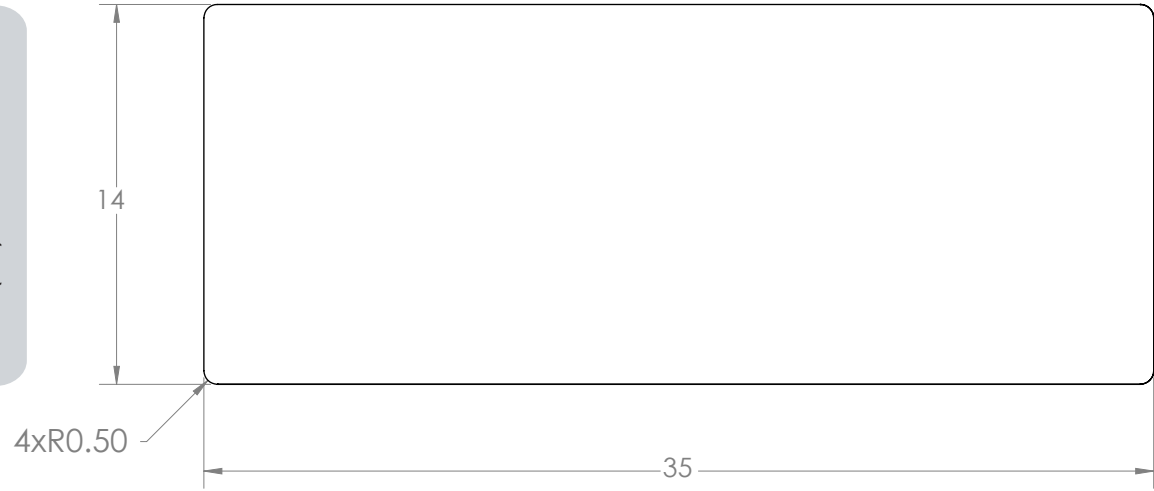

Example



- Barcode Specification:
- 1) Bar code format: GS1 DataMatrix ECC 200
 - 2) Height of bar code: 12 mm
 - 3) Printing density: 300 DPI

NOTES:


- 1) MATERIAL: 5 MIL 8B35 + 3M 467
- 2) PARTS SHALL BE SUPPLIED DIE-CUT TO SHAPE WITH PEEL-OFF LINER.
- 3) COLORS: BACKGROUND TO BE SILER LINING (PANTONE 428), TEXT AND SYMBOLS TO BE ECLIPSE EXCEPT WHERE INDICATED.
- 4) SHALL MEET THE DURABILITY REQUIREMENTS OF UL 60601-1.
- 5) PLACE WRITE-ON OVERLAMINATE OVER ENTIRE SURFACE.
- 6) SERIAL NUMBER AND MANUFACTURE DATA:
THE SERIAL NUMBER SHOULD BE PROVIDED BY CARESTREAM. MANUFACTURE DATE FORMAT: YYYY-MM-DD
- 7) SEE PACKAGING GROUP FOR ARTWORK. ENVIRONMENTAL SPECIFICATIONS:
- 8) SUPPLIER MUST PROVIDE IPC-1752A DECLARATION THAT ALL COMPONENT MATERIALS ARE CERTIFIED RoHS-RESTRICTED MATERIALS COMPLIANT.

CARESTREAM DENTAL LLC GLOBAL R&D CENTER (SHANGHAI)		TRACE FILE :		MATERIAL			
		DESIGN SW:					
DATUM PLANE PRIORITY A, B, C UNLESS SPECIFIED		CONTRACT NO:		NAME DATA PLATE-HANDPIECE, CS 3800			
		DESIGN HATA GAO	DATE 2020-03-27				
UNIT : mm	METER	AUDITING	DATE	BUY LEV	SIZE	PART NUMBER	REV
ANGLE ±1	0 ±0.5	APPROVE	DATE			TA2970	C
0.0 ±0.13	0.00 ±NA			SCALE: 1: 1	PROJECT: CS 3800	SHEET 1 OF 1	

Intraoral Scanner

Model : Trophy 3800 Wireless

SN




MD





Carestream Dental LLC
3625 Cumberland Boulevard, Suite 700
Atlanta, GA USA 30339

FCC ID: 2ASFG-CS3800
IC ID: 24914-CS3800

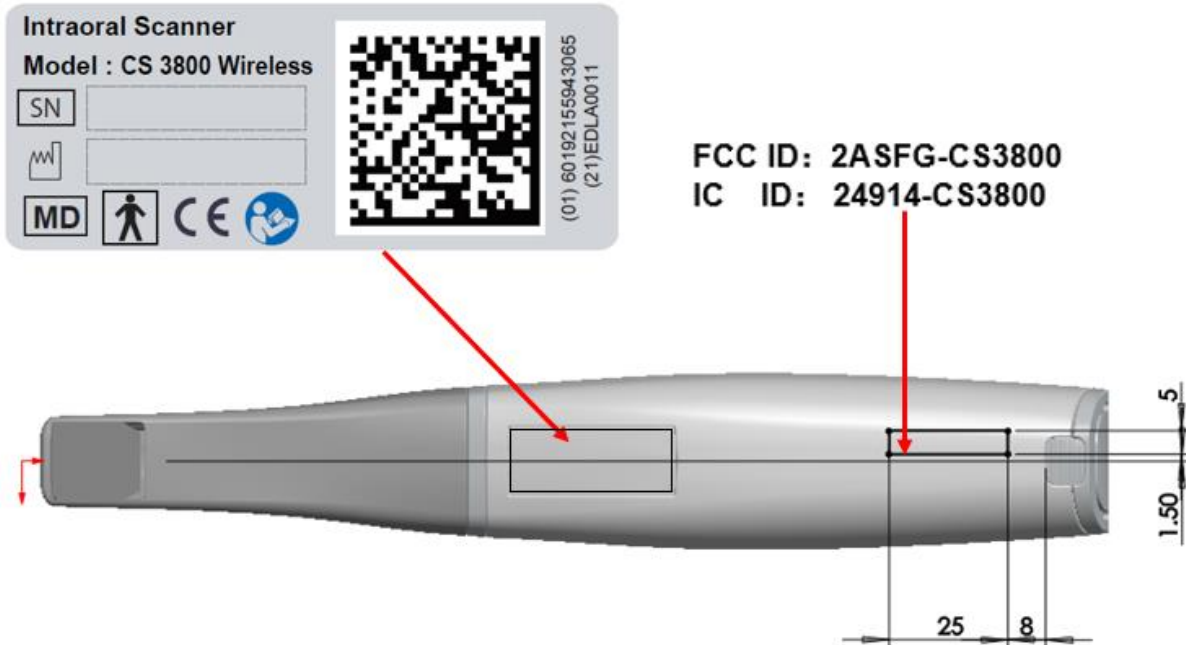

Product label will be adhered on the side enclosure of the scanner handpiece.

FCC ID "2ASFG-CS3800" and IC ID "24914-CS3800" will be also engraved on this side enclosure.


The statement according to FCC part 15 §15.19(a)(3) has been added in CS 3800 Safety & Regulatory Guide, page 26.



Carestream Dental LLC
3625 Cumberland Boulevard, Suite 700
Atlanta, GA USA 30339

FCC ID: 2ASFG-CS3800
IC ID: 24914-CS3800

For Trophy 3800 Wireless:

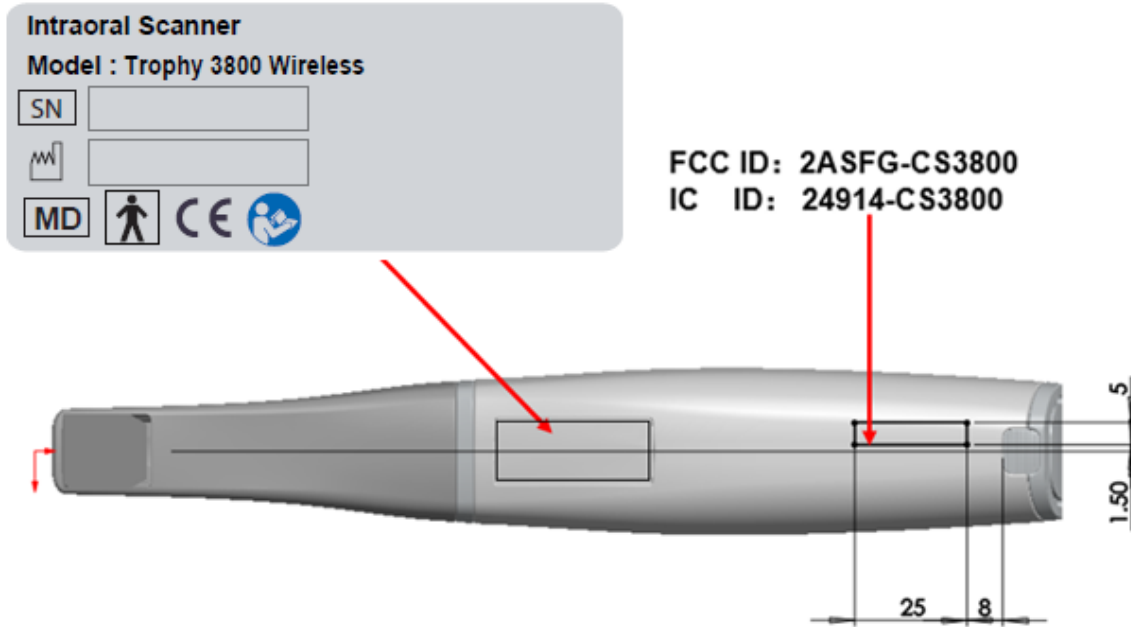

Product label will be adhered on the side enclosure of the scanner handpiece.

FCC ID "2ASFG-CS3800" and IC ID "24914-CS3800" will be also engraved on this side enclosure.

The statement according to FCC part 15 §15.19(a)(3) has been added in CS 3800 Safety & Regulatory Guide, page 26.