


Label photo

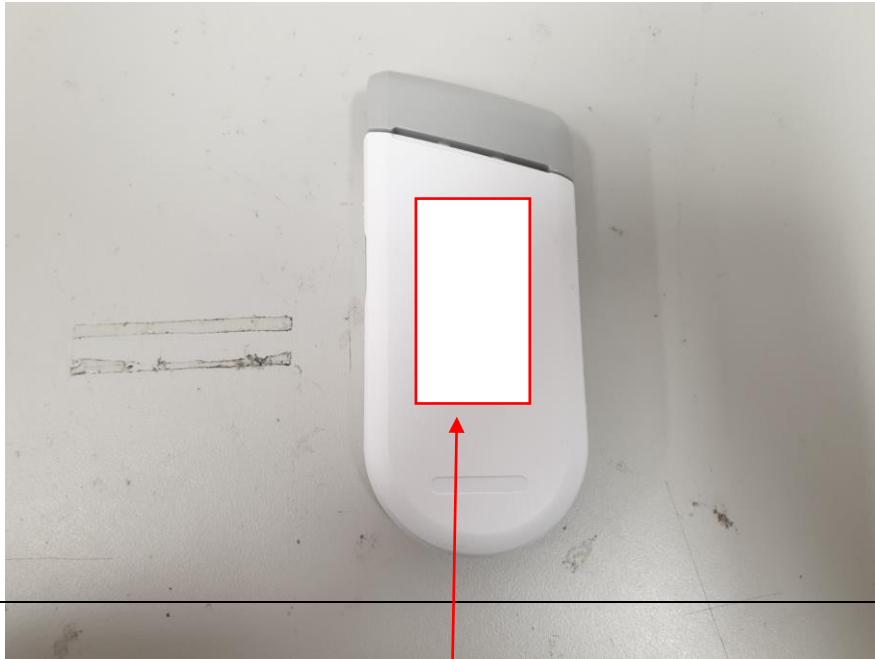

Multi Use Breath Analyzer
Model: KETOSCAN SMART
FCC ID : 2ASFRKETOSCANSMA
This device complies with part 15 of the FCC Rules.
Operation is subject to the following two conditions :
(1) This device may not cause harmful interference, and
(2) This device must accept any interference received, including
interference that may cause undesired operation.

SENTECH GMI Corp.