

APPENDIX B EUT TEST POSITION PHOTOS

Liquid depth $\geq 15\text{cm}$


Phantom: SAM (30deg probe tilt) with CRP v5.0_20150321; Type: QD000P40CD; Serial: TP:1874



Body Back Setup Photo (10mm)

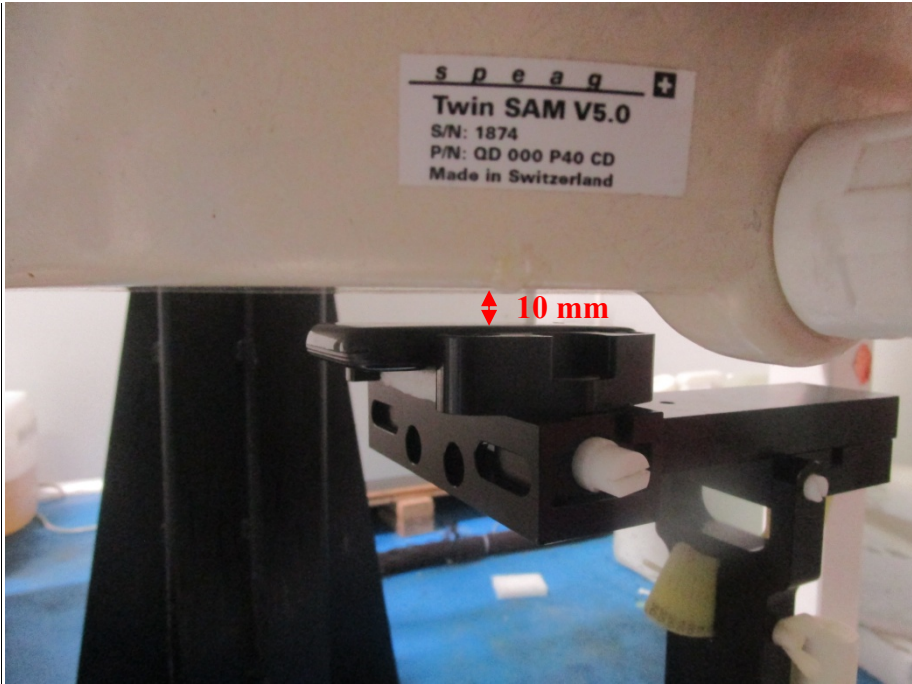


Body Front Setup Photo (10mm)

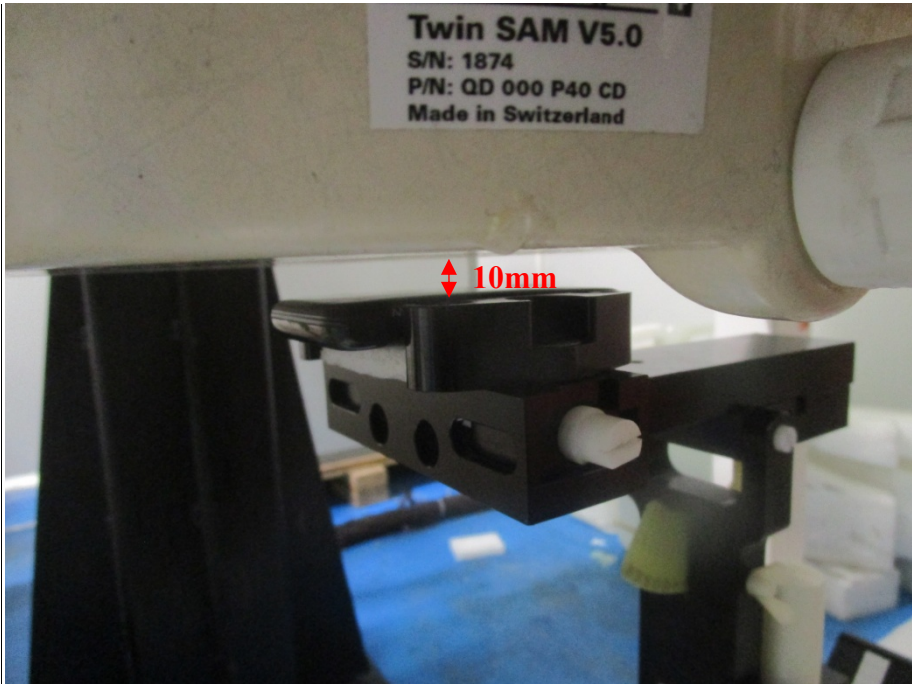


Body Left Setup Photo (10mm)



Body Right Setup Photo (10mm)

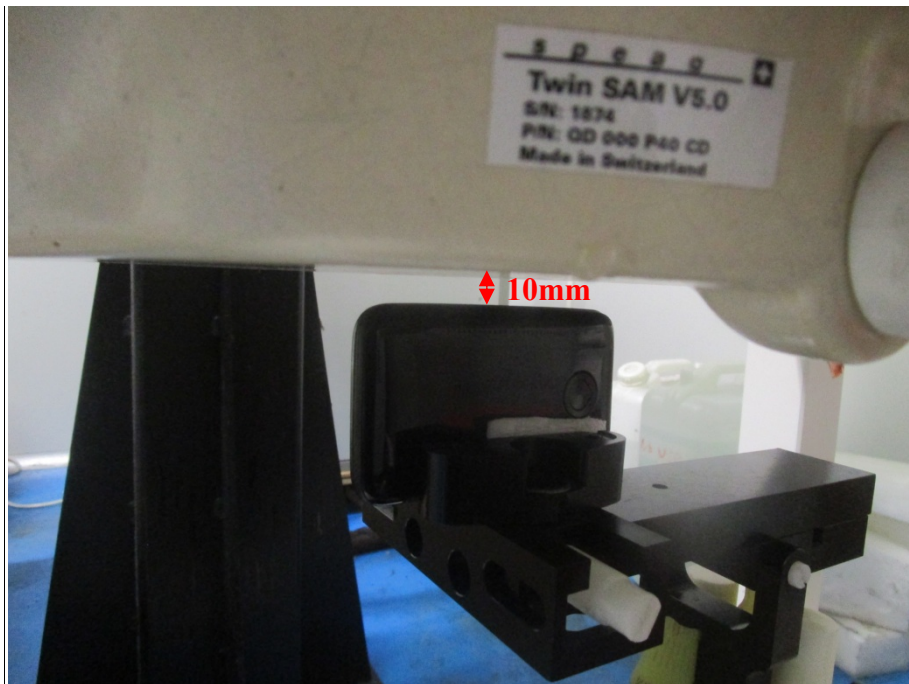

Body Bottom Setup Photo (10mm)

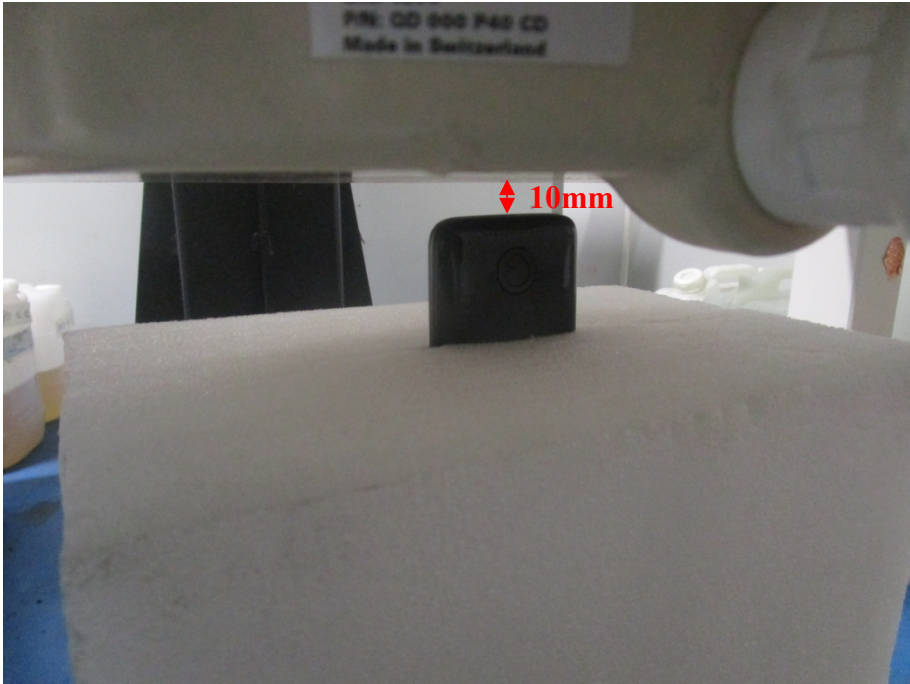

Body Top Setup Photo (10mm)

