



Canada

Exhibit: External Photos

Report File #: 7169006356RA-000

© TÜV SÜD Canada Inc. This test report shall not be reproduced except in full, without written approval of TÜV SÜD Canada Inc

Client	Innovere Medical Inc.	 Canada
Product	WMODHP	
Standard(s)	RSS 247 Issue 1:2017 FCC Part 15 Subpart 15.247:2018	

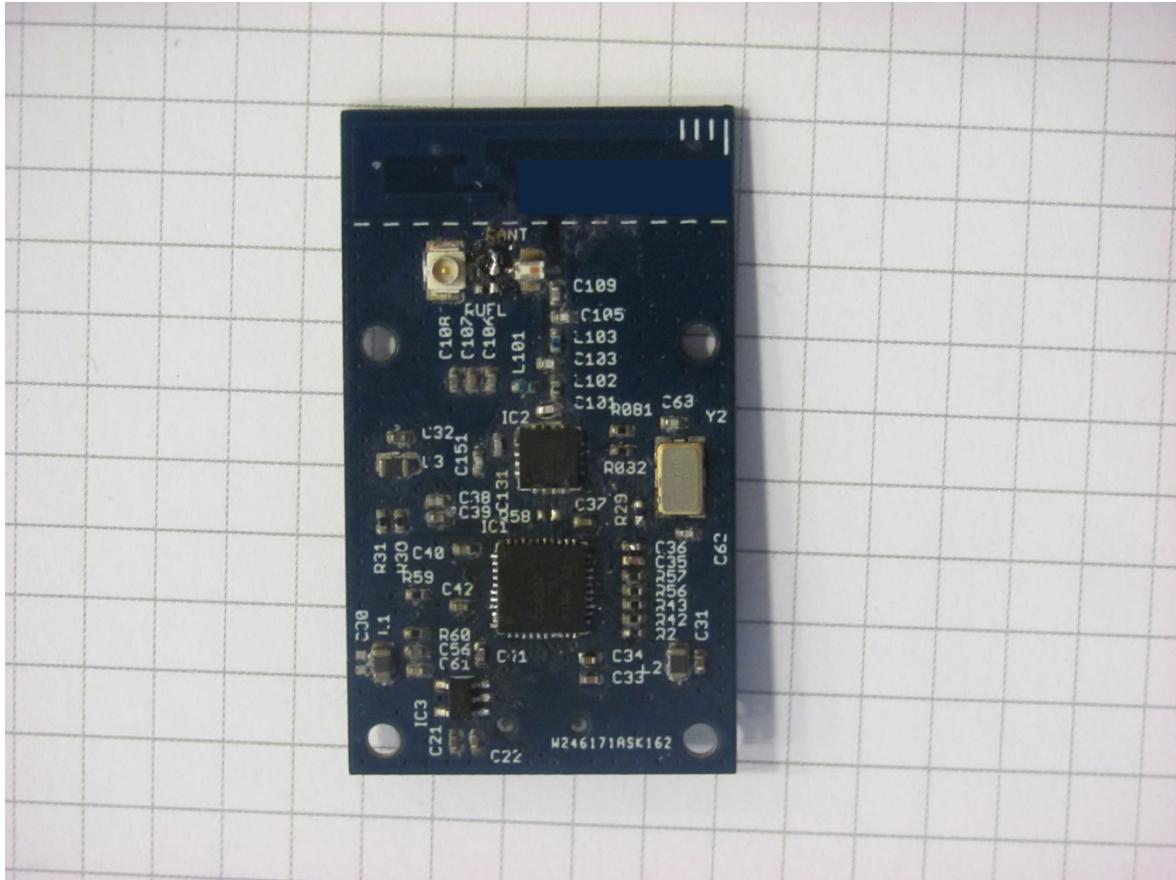


Figure 1 – EUT External Photo Front

Client	Innovere Medical Inc.	 Canada
Product	WMODHP	
Standard(s)	RSS 247 Issue 1:2017 FCC Part 15 Subpart 15.247:2018	

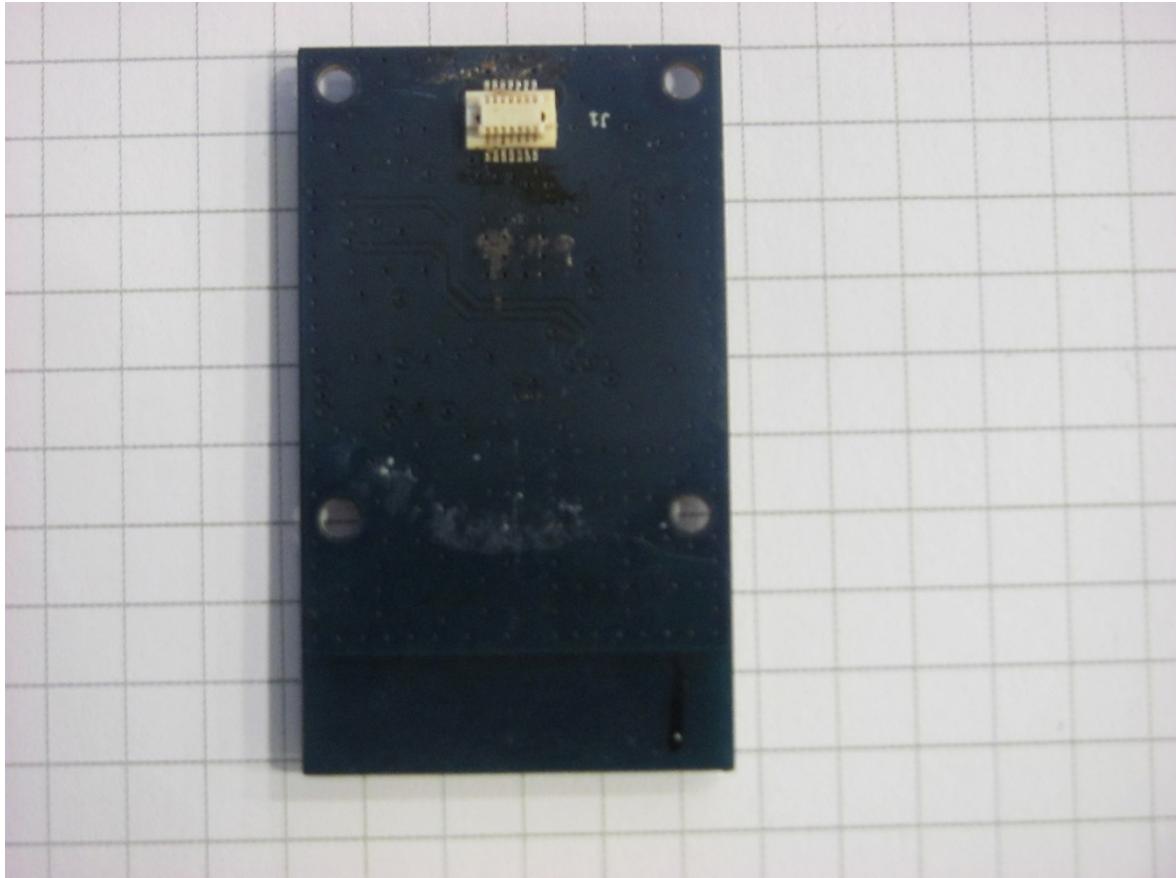


Figure 2 – EUT External Photo Back

Client	Innovere Medical Inc.	 Canada
Product	WMODHP	
Standard(s)	RSS 247 Issue 1:2017 FCC Part 15 Subpart 15.247:2018	

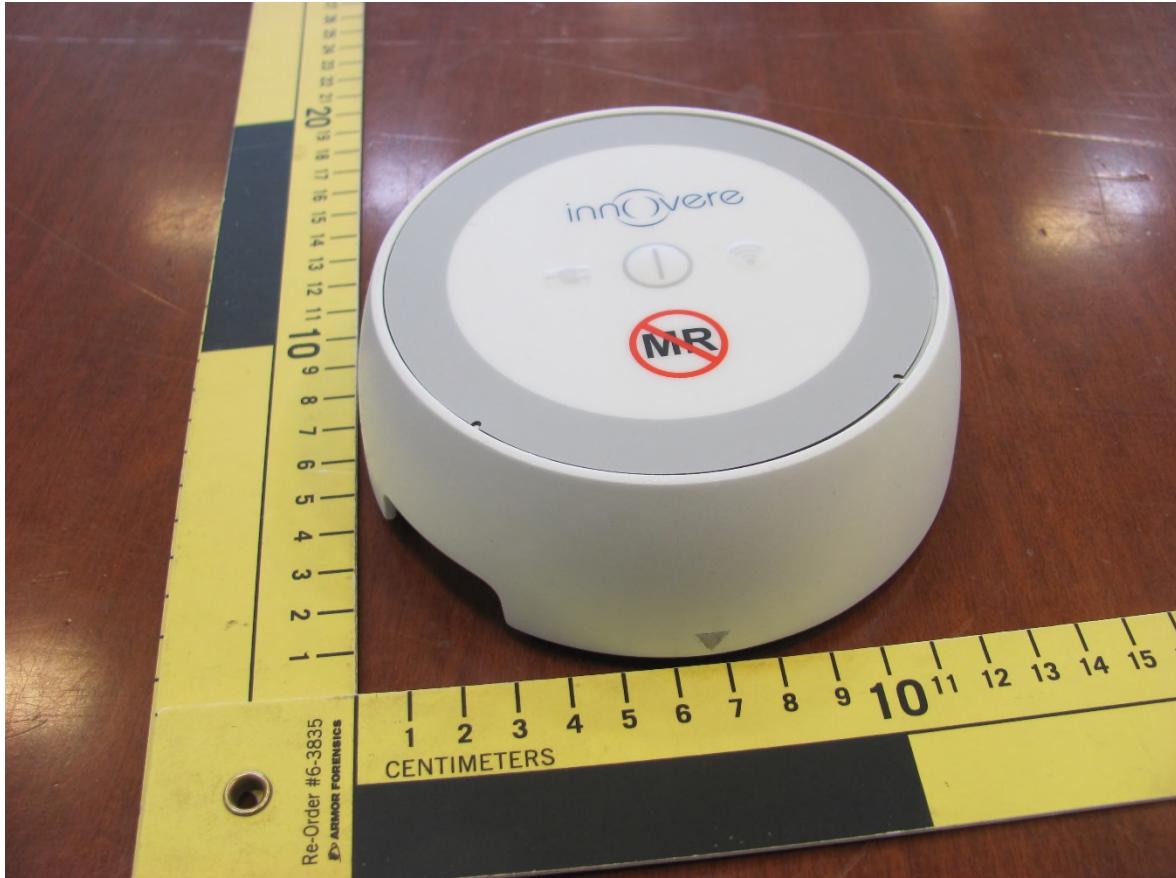


Figure 3 – Sample Host