



Canada

Exhibit: Test Setup Photos

Report File #: 7169006356RA-000

© TÜV SÜD Canada Inc. This test report shall not be reproduced except in full, without written approval of TÜV SÜD Canada Inc

Client	Innovere Medical Inc.	
Product	WMODHP	
Standard(s)	RSS 247 Issue 2:2017 FCC Part 15 Subpart 15.247:2018	



Figure 1 – Radiated Emissions Setup – Photo 1

Client	Innovere Medical Inc.	
Product	WMODHP	
Standard(s)	RSS 247 Issue 2:2017 FCC Part 15 Subpart 15.247:2018	



Figure 2 – Radiated Emissions Setup – Photo 2

Note: As per ANSI C63.10-2013 Clause 6.3.1, below 1GHz, the height of the EUT was set to 80cm. Above 1GHz, the height was raised to 1.5m.

Client	Innovere Medical Inc.	
Product	WMODHP	
Standard(s)	RSS 247 Issue 2:2017 FCC Part 15 Subpart 15.247:2018	



Figure 3 – Radiated Emissions Setup – Photo 3

Note: As per ANSI C63.10-2013 Clause 6.3.1, above 1GHz, the height of the EUT was set to 1.5m.

Client	Innovere Medical Inc.	
Product	WMODHP	
Standard(s)	RSS 247 Issue 2:2017 FCC Part 15 Subpart 15.247:2018	

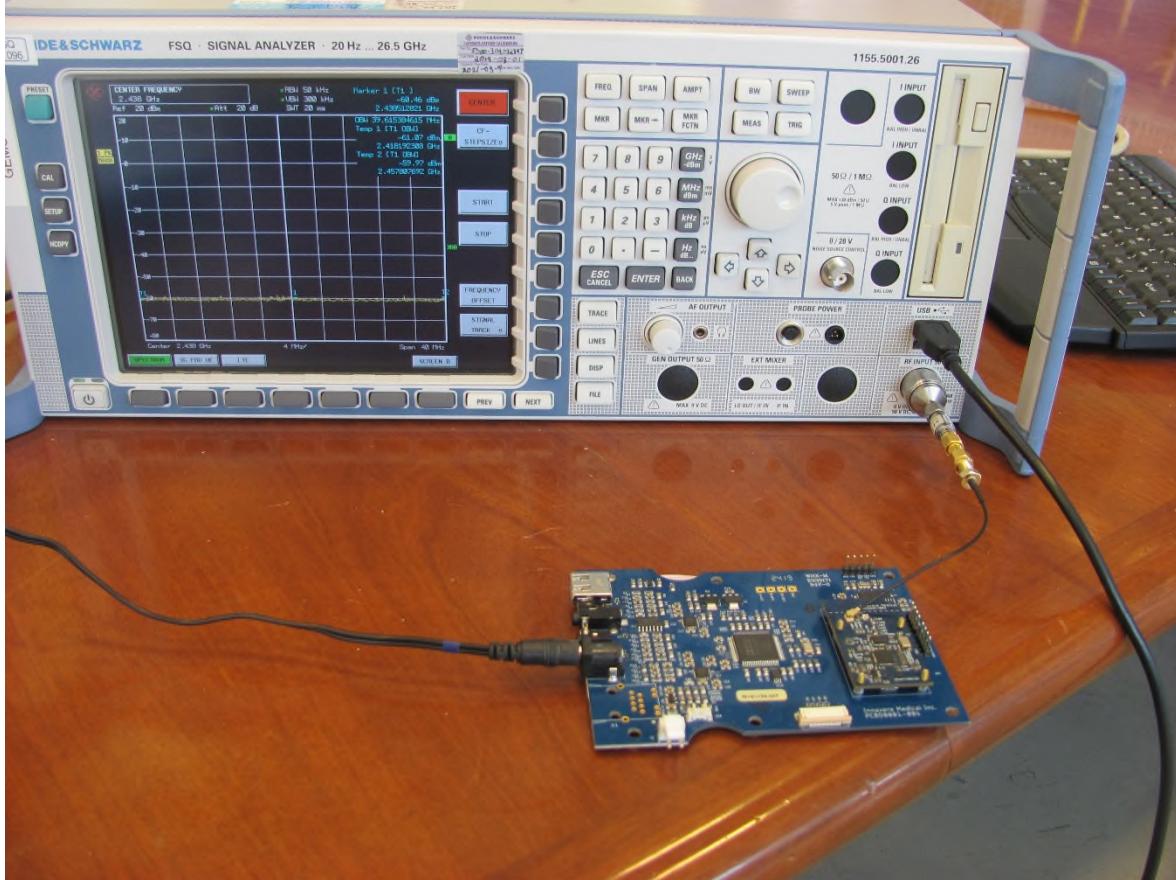


Figure 4 – Antenna Port Conducted Emissions Setup