


Appendix D

Photographs


1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

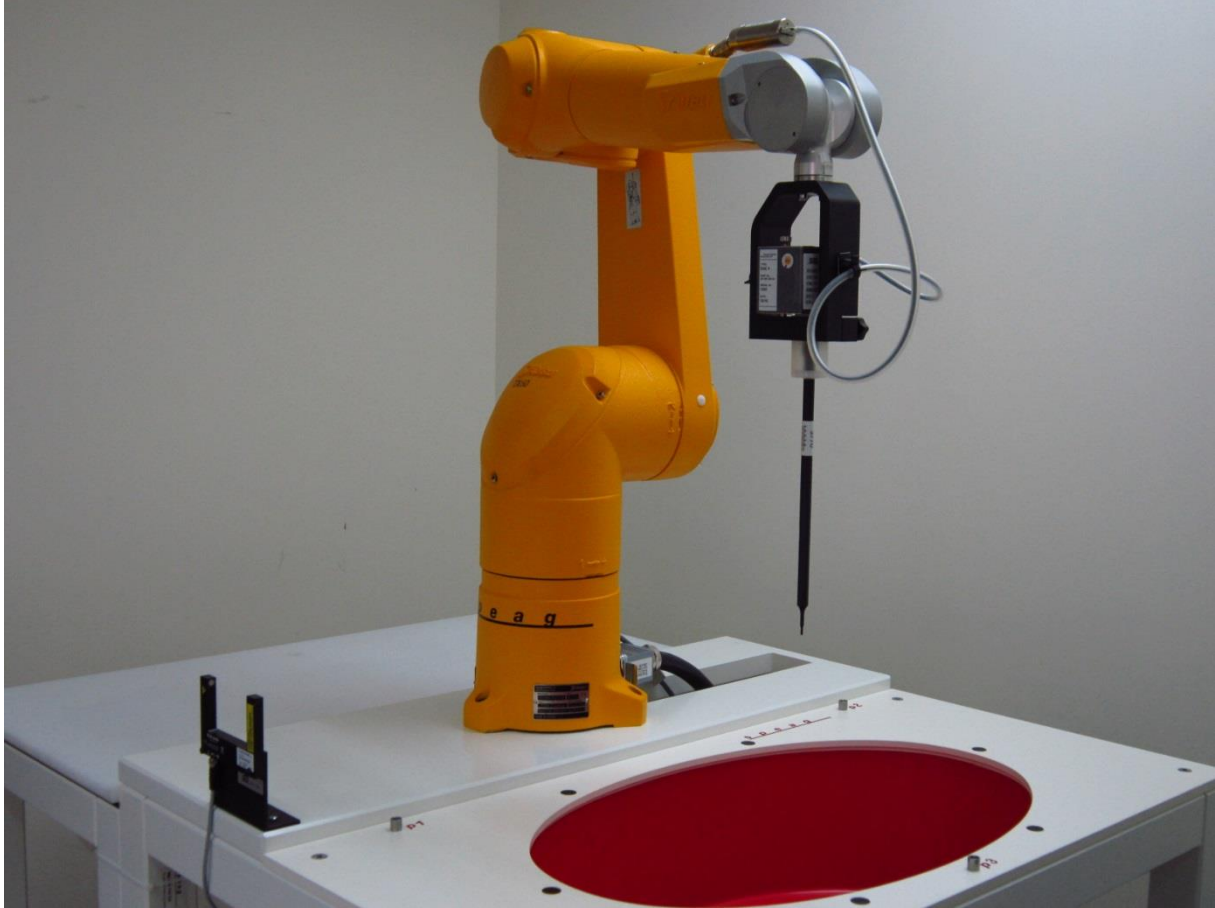

2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 2450

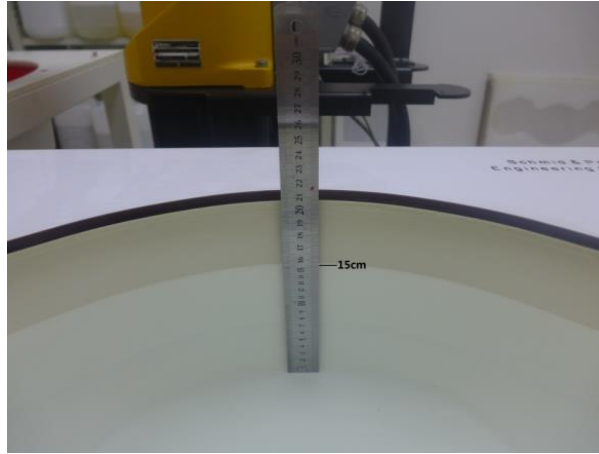

3. Photographs of EUT test position








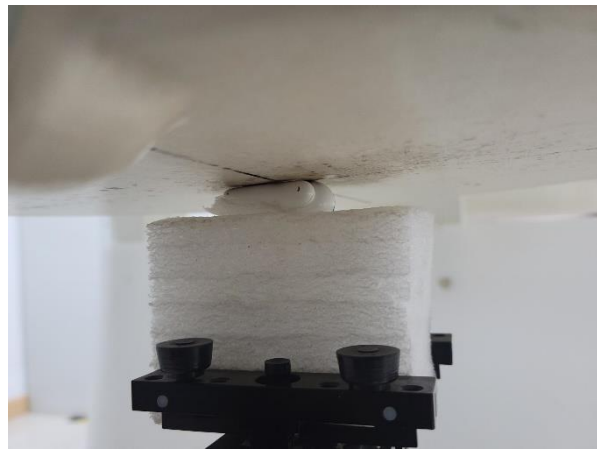
<p>Photo 1: Side 1 0mm</p>	<p>Photo 2: Side 2 0mm</p>
	
<p>Photo 3: Side 3 0mm</p>	<p>Photo 4: Side 4 0mm</p>
	
<p>Photo 5: Side 5 0mm</p>	<p>Photo 6: Side 6 0mm</p>
	

Photo 7: Side 7 0mm	Photo 8: Side 8 0mm
 A microscopic image showing a white, cylindrical object mounted on a black base. The object has a textured, fibrous surface. The view is from the side, showing the top edge of the cylinder and the base. The background is a light, neutral color.	 A microscopic image showing a white, cylindrical object mounted on a black base, similar to Photo 7. The view is from the side, showing the top edge of the cylinder and the base. The background is a light, neutral color.

4. EUT Constructional Details

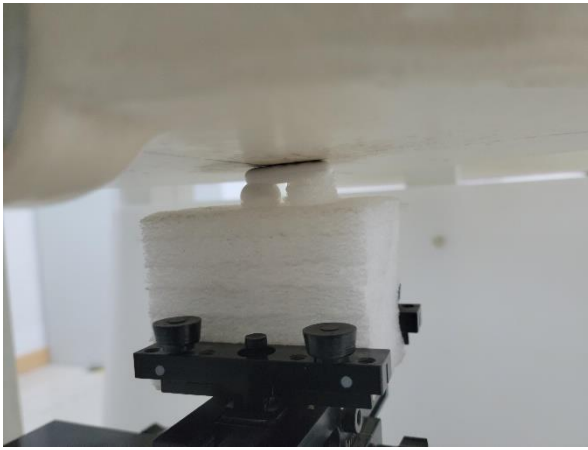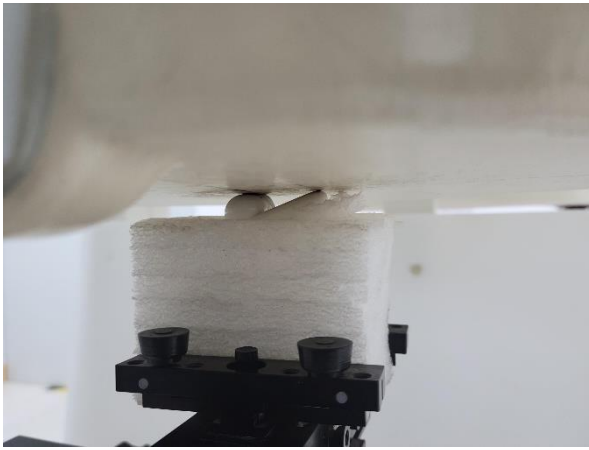Details please Refer to the <External Photos>&<Internal Photos>.