


## EXHIBIT 1 - PRODUCT LABELING

### Proposed IC Label

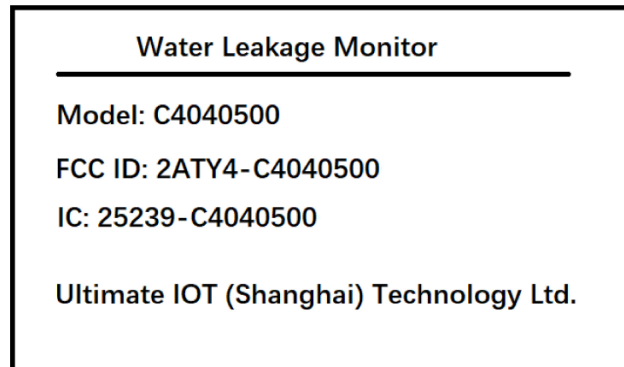

Specifications: Text is black in color and justified. The label shall be securely affixed to a permanently attached part of the device, in a location where it is visible or easily accessible to the user, and shall not be readily detachable. The label shall be sufficiently durable to remain fully legible and intact on the device in all normal conditions of use throughout the device’s expected lifetime. These requirements may be met either by a separate label or nameplate permanently attached to the device or by permanently imprinting or impressing the label directly onto the device. The label text shall be legible without the aid of magnification, but is not required to be larger than 8- point font size. If the device is too small to meet this condition, the label information may be included in the user manual upon agreement with Industry Canada. The label for medical implants designed to be used within the human body shall be placed on the package and in the user manual.

### Proposed Label Location on EUT

IC Label Location

