

Report No. : TESA2205000105ES Rev: Page: 1 of 7

# Appendix C

# **Phantom Description**

Schmid & Partner Engineering AG



Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 9700, Fax +41 44 245 9779 info@speag.com, http://www.speag.com

## Certificate of Conformity / First Article Inspection

Item	Oval Flat Phantom ELI 5.0
Type No	QD OVA 002 A
Series No	1108 and higher
Manufacturer	Untersee Composites
	Knebelstrasse 8, CH-8268 Mannenbach, Switzerland

### Tests

Complete tests were made on the prototype units QD OVA 001 A, pre-series units QD OVA 001 B as well as on some series units QD OVA 001 B. Some tests are made on all series units QD OVA 002 A.

Test	Requirement	Details	Units tested
Shape	Internal dimensions, depth and sagging are compatible with standards	Bottom elliptical 600 x 400 mm, Depth 190 mm, dimension compliant with [1] for f > 375 MHz	Prototypes
Material thickness	Bottom: 2.0mm +/- 0.2mm	dimension compliant with [3] for f > 800 MHz	all
Material parameters	rel. permittivity 2 – 5, loss tangent ≤ 0.05, at f ≤ 6 GHz	rel. permittivity 3.5 +/- 0.5 loss tangent ≤ 0.05	Material samples
Material resistivity	Compatibility with tissue simulating liquids .	Compatible with SPEAG liquids. **	Phantoms, Material sample
Sagging	Sagging of the flat section in tolerance when filled with tissue simulating liquid.	within tolerance for filling height up to 155 mm	Prototypes, samples

Note: Compatibility restrictions apply certain liquid components mentioned in the standard, containing e.g. DGBE, DGMHE or Triton X-100. Observe technical note on material compatibility.

### Standards

- [1] OET Bulletin 65, Supplement C, "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields<sup>®</sup>, Edition 01-01 IEEE 1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific
- [2] Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques, December 2003
- [3] IEC 62209-1 ed1.0. "Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices - Human models, instrumentation, and procedures - Part 1: Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", 2005-02-18
- [4] IEC 62209-2 ed 10, "Human exposure to radio frequency fields from hard-held and body-mounted wireless communication devices Human models, instrumentation, and procedures Part 2: Procedure to determine the specific absorption rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", 2010-03-30

## Conformity

Based on the sample tests above, we certify that this item is in compliance with the uncertainty requirements of body-worn SAR measurements and system performance checks as specified in [1 - 4] and further standards.

Date

реад

Signature / Stamp

Schmid & Partner-Engineering/AG Zeugba-estrasse 43, 8004 Zeich, Sciumpand Phone/441 44/35 9708, Fext+44 64485 9779

Doc No 881 - QD OVA 002 A - A

25.7.2011

1 (1) Page

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction form exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號 SGS Taiwan Ltd.

f (886-2) 2298-0488



Report No. : TESA2205000105ES Rev: Page: 2 of 7

# System Validation from Original Equipment Supplier

	tion Service (SAS)		ccreditation No.: SCS 0108
he Swiss Accreditation Service			
Iultilateral Agreement for the re			
Client SGS-TW (Aude	n)	Certificate N	o: D2450V2-727_Apr22
CALIBRATION C	ERTIFICAT		
	LITTITIOAT	-	
Object	D2450V2 - SN:7	27	
Calibration procedure(s)	QA CAL-05.v11	edure for SAR Validation Sources	hotusen 0.7.0 CLis
	Galibration Froce	sources	s between 0.7-3 GHz
2010 - 10 - 10 - 10 - 10 - 10 - 10 - 10			
Calibration date:	April 25, 2022		
This calibration certificate docume	ents the traceability to nat	ional standards, which realize the physical un	nits of measurements (SI)
This calibration certificate docume The measurements and the uncer	ents the traceability to nat tainties with confidence p	ional standards, which realize the physical un probability are given on the following pages a	nits of measurements (SI).
This calibration certificate docume The measurements and the uncer	ents the traceability to nat tainties with confidence p	ional standards, which realize the physical un probability are given on the following pages a	nits of measurements (SI). nd are part of the certificate.
The measurements and the uncer	tainties with confidence p	probability are given on the following pages a	nd are part of the certificate.
The measurements and the uncer	tainties with confidence p	ional standards, which realize the physical un robability are given on the following pages a ry facility: environment temperature $(22 \pm 3)^{\circ}$	nd are part of the certificate.
The measurements and the uncer All calibrations have been conduc	tainties with confidence p ted in the closed laborato	probability are given on the following pages a	nd are part of the certificate.
The measurements and the uncert All calibrations have been conduc Calibration Equipment used (M&T	tainties with confidence p ted in the closed laborato E critical for calibration)	robability are given on the following pages a ry facility: environment temperature $(22\pm3)^{\circ}$	nd are part of the certificate.
The measurements and the uncert All calibrations have been conduc Calibration Equipment used (M&T Primary Standards	tainties with confidence p ted in the closed laborato E critical for calibration)	robability are given on the following pages a ry facility: environment temperature $(22 \pm 3)^{\circ}$ Cal Date (Certificate No.)	nd are part of the certificate. 'C and humidity < 70%. Scheduled Calibration
The measurements and the uncert All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter NRP	tainties with confidence p ted in the closed laborato E critical for calibration) ID # SN: 104778	robability are given on the following pages a ry facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 04-Apr-22 (No. 217-03525/03524)	nd are part of the certificate. 'C and humidity < 70%. Scheduled Calibration Apr-23
The measurements and the uncer All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter NRP Power sensor NRP-291	tainties with confidence p ted in the closed laborato E critical for calibration) ID # SN: 104778 SN: 103244	robability are given on the following pages a ry facility: environment temperature (22 ± 3) <sup>4</sup> Cal Date (Certificata No.) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03524)	nd are part of the certificate. 'C and humidity < 70%. Scheduled Calibration Apr-23 Apr-23
The measurements and the uncer All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power sensor NRP-291 Power sensor NRP-291 Power sensor NRP-291	tainties with confidence p ted in the closed laborato E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245	robability are given on the following pages a ry facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525)	nd are part of the certificate. 'C and humidity < 70%. Scheduled Cellbration Apr-23 Apr-23 Apr-23
The measurements and the uncer All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter NRP Power sensor NRP-291 Reference 20 d8 Attenuator	tainlies with confidence p ted in the closed laborato E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 8H:9394 (20k)	robability are given on the following pages a ry facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03527)	nd are part of the certificate. *C and humidity < 70% Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23
The measurements and the uncer All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power Sansor NRP-Z91 Power sansor NRP-Z91 Power sansor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination	tainlies with confidence p ted in the closed laborato E critical for calibration) ID # SN: 103245 SN: 103245 SN: 103245 SN: 103245 SN: 103245 SN: 30394 (20k) SN: 30982 / 06327	robability are given on the following pages a ry facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 04-Apr-22 (No. 217-0352/30324) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03527)	nd are part of the certificate. C and humidity < 70%. Scheduled Cellbration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23
The measurements and the uncert All calibrations have been conduc Calibration Equipment used (M&T Primury Standards Power mater NRP Power sensor NRP-291 Power sensor NRP-291 Reference robe 20 dB Attenuator Type-N mismatch combination Reference Probe EXSDV4	ID #   ID # SN: 104778   SN: 103244 SN: 103244   SN: 103245 SN: 310324 (20k)   SN: 310982 (06327 SN: 310982 (06327	Cal Date (Certificate No.)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03526)   04-Apr-22 (No. 217-03528)   04-Apr-22 (No. 217-03528)   04-Apr-22 (No. 217-03528)   04-Dar-22 (No. 217-03528)   04-Dar-22 (No. 217-03528)	nd are part of the certificate. 'C and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Doc-22
The measurements and the uncer All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4	tainlies with confidence p ted in the closed laborato E critical for calibration) ID # SN: 103245 SN: 103245 SN: 103245 SN: 103245 SN: 103245 SN: 30394 (20k) SN: 30982 / 06327	robability are given on the following pages a ry facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 04-Apr-22 (No. 217-0352/30324) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03527)	nd are part of the certificate. C and humidity < 70%. Scheduled Cellbration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23
The measurements and the uncer All calibrations have been concluc Calibration Equipment used (M&T Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismark comtinuation Reference Probe EX3DV4 DAE4	ID #   ID # SN: 104778   SN: 103244 SN: 103244   SN: 103245 SN: 310324 (20k)   SN: 310982 (06327 SN: 310982 (06327	Cal Date (Certificate No.)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03526)   04-Apr-22 (No. 217-03528)   04-Apr-22 (No. 217-03528)   04-Apr-22 (No. 217-03528)   04-Dar-22 (No. 217-03528)   04-Dar-22 (No. 217-03528)	nd are part of the certificate. 'C and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Doc-22
The measurements and the uncer All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards	tainlies with confidence p ted in the closed laborato E critical for calibration) ID # SN: 103244 SN: 103245 SN: 303245 SN: 3193245 SN: 319324 SN: 319324 SN: 319324 SN: 319324 SN: 319324 SN: 319324 SN: 501	Cal Date (Certificate No.)   04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525)   04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525)   04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03526)   04-Apr-22 (No. 217-03526) 31-Dec-21 (No. 217-03528)   31-Dec-21 (No. EX3-7349_Dec21) 01-Nov/21 (No. DAE-4-601_Nov21)	nd are part of the certificate. 'C and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Doc-22 Nov-22
The measurements and the uncer All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B	tainlies with confidence p   ted in the closed laborato   E critical for calibration)   ID #   SN: 104778   SN: 103245   SN: 103245   SN: 310822 / 06327   SN: 31082 / 06327   SN: 5H-9394 (20k)   SN: 5H-934 (20k)   SN: 601   ID #	robability are given on the following pages a ry facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03528) 31-Dec-21 (No. ZK3-7349 (Dec21)) 01-Nov-21 (No. ZK3-7349 (Dec21)) Check Date (in house)	nd are part of the certificate. *C and humidity < 70% Scheduled Calibration Apr-23 Apr-24 Apr-2
The measurements and the uncer All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power mere NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EXSDV4 DAE4 Secondary Standards Power meter E41198 Power meter E41198	tainlies with confidence p   ted in the closed laborato   E critical for calibration)   ID #   SN: 104778   SN: 103244   SN: 103245   SN: 310862 / 06327   SN: 7349   SN: 708   SN: 501   ID #	Cal Date (Cartificata No.)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03525)   04-Apr-22 (No. 217-03525)   04-Apr-22 (No. 217-03525)   04-Apr-22 (No. 217-03526)   04-Apr-22 (No. 217-03527)   04-Apr-22 (No. 217-03528)   31-Dec-21 (No. 217-03528)   31-Dec-21 (No. 217-03528)   31-Dec-21 (No. 217-03528)   31-Dec-21 (No. Apr-24 (No. 217-03528)   31-Dec-21 (No. Apr-24 (No. 217-03528)   33-Dec-14 (In house head No.21)   Check Date (In house head No.2-20)	nd are part of the certificate. 'C and humidity < 70%. Scheduled Calibration Apr/23 Apr/24 Apr/24 Apr/25 Apr/25 Apr/25 Apr/25 Apr/26
The measurements and the uncer All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power sensor NRP-Z91 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E44198 Power sensor HP 8481A Power sensor HP 8481A	tainlies with confidence p   ted in the closed laborato   E critical for calibration)   ID #   SN: 104778   SN: 103244   SN: 103245   SN: 103245   SN: 103245   SN: 310862 (20k)   SN: 310862 (30k)   SN: 601   ID #   SN: 0339512475   SN: US37282783	Cal Date (Certificate No.)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03526)   04-Apr-22 (No. 217-03527)   04-Apr-22 (No. 217-03528)   31-Dac-21 (No. 217-03528)   30-Oct-14 (in house check Oct-20)   07-Oct-15 (in house check Oct-20)   07-Oct-15 (in house check Oct-20)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Nov-22 Scheduled Check In house check: Oct-22 In house check: Oct-22
The measurements and the uncer All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe 2304 Secondary Standards Power meter E44198 Power sensor HP 8481A Power sensor HP 8481A Power sensor HP 8481A	tainlies with confidence p   ted in the closed laborato   E critical for calibration)   ID #   SN: 104778   SN: 103244   SN: 103245   SN: 8H9394 (20k)   SN: 601   ID #   SN: 603   SN: 603   SN: 8H9394 (20k)   SN: 601   ID #   SN: 00512475   SN: W41093315   SN: W141093315   SN: W141093215   SN: 100972	Cal Date (Certificata No.)   Cal Date (Certificata No.)   04-Apr-62 (No. 217-03625/03524)   04-Apr-62 (No. 217-03625/03524)   04-Apr-62 (No. 217-03625/03524)   04-Apr-62 (No. 217-03525)   04-Apr-62 (No. 217-03525)   04-Apr-62 (No. 217-03525)   04-Apr-62 (No. 217-03525)   04-Apr-62 (No. 217-03527)   04-Apr-62 (No. 217-03528)   31-Dac-21 (No. 217-03528)   31-Dac-21 (No. 217-03528)   30-Odt-14 (in house)   Check Date (in house)   00-Odt-15 (in house check Oct-20)   07-Odt-15 (in house check Oct-20)   07-Odt-15 (in house check Oct-20)	nd are part of the certificate. 'C and humidity < 70%. Scheduled Calibration Apr/23 Apr/24 Apr/24 Apr/25 Apr/25 Apr/25 Apr/25 Apr/26
The measurements and the uncer All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power sensor NRP-291 Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe 2500/4 DAE4 Secondary Standards Power sensor HP 8481A Power sensor HP 8481A Power sensor HP 8481A Power sensor HP 8481A	ID #   ID #   SN: 104778   SN: 104778   SN: 103244   SN: 103245   SN: 3108270620327   SN: 7349   SN: 503512475   SN: US37262783   SN: 109272   SN: 109272   SN: 109272   SN: US3702773	Cal Date (Certificate No.)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03525)   04-Apr-22 (No. 217-03525)   04-Apr-22 (No. 217-03525)   04-Apr-22 (No. 217-03525)   04-Apr-22 (No. 217-03526)   31-Dec-21 (No. 217-03528)   31-Dec-21 (No. 217-03528)   30-Oct +4 (n house hteck Cct-20)   07-Oct +5 (in house check Cct-20)   07-Oct +5 (in house check Cct-20)   15-Jun-15 (in house check Cct-20)   31-Mar-14 (in house check Cct-20)	nd are part of the certificate. 'C and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Dec-22 Nov-22 Scheduled Check In house check: Oct-22 In house check: Oct-22 In house check: Oct-22 In house check: Oct-22
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&T Primury Standards Power sensor NRP-291 Power sensor NRP-291 Reference Probe EX3DV4 DAE4 Secondary Standards Power metre E4198 Power sensor HP 8481A Power Sensor HP 8	tainlies with confidence p   ted in the closed laborato   ID #   SN: 104778   SN: 103244   SN: 103245   SN: 103245   SN: 103245   SN: 103245   SN: 103245   SN: 103245   SN: 51082 (06)27   SN: 601   ID #   SN: 06327   SN: US37292783   SN: W141093315   SN: W141090477   Name	Cal Date (Certificate No.)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03526)   04-Apr-22 (No. 217-03527)   04-Apr-22 (No. 217-03528)   31-0a-21 (No. 217-03528)   31-0a-21 (No. 217-03528)   31-0a-21 (No. 217-03528)   30-Oct-14 (in house)   30-Oct-15 (in house check Oct-20)   07-Odt-15 (in house check Oct-20)   07-Odt-15 (in house check Oct-20)   31-Mar-14 (in house check Oct-20)   31-Mar-14 (in house check Oct-20)	nd are part of the certificate. 'C and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Dec-22 Nov-22 Scheduled Check In house check: Oct-22 In house check: Oct-22 In house check: Oct-22 In house check: Oct-22
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&T Primury Standards Power sensor NRP-291 Power sensor NRP-291 Reference Probe EX3DV4 DAE4 Secondary Standards Power metre E4198 Power sensor HP 8481A Power Sensor HP 8	ID #   ID #   SN: 104778   SN: 104778   SN: 103244   SN: 103245   SN: 3108270620327   SN: 7349   SN: 503512475   SN: US37262783   SN: 109272   SN: 109272   SN: 109272   SN: US3702773	Cal Date (Certificate No.)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03525)   04-Apr-22 (No. 217-03525)   04-Apr-22 (No. 217-03525)   04-Apr-22 (No. 217-03525)   04-Apr-22 (No. 217-03526)   31-Dec-21 (No. 217-03528)   31-Dec-21 (No. 217-03528)   30-Oct +4 (n house hteck Cct-20)   07-Oct +5 (in house check Cct-20)   07-Oct +5 (in house check Cct-20)   15-Jun-15 (in house check Cct-20)   31-Mar-14 (in house check Cct-20)	nd are part of the certificate. 'C and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Dec-22 Nov-22 Scheduled Check In house check: Oct-22 In house check: Oct-22
The measurements and the uncer	tainlies with confidence p   ted in the closed laborato   ID #   SN: 104778   SN: 103244   SN: 103245   SN: 103245   SN: 103245   SN: 103245   SN: 103245   SN: 103245   SN: 51082 (06)27   SN: 601   ID #   SN: 06327   SN: US37292783   SN: W141093315   SN: W141090477   Name	Cal Date (Certificate No.)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03525/03524)   04-Apr-22 (No. 217-03526)   04-Apr-22 (No. 217-03527)   04-Apr-22 (No. 217-03528)   31-0a-21 (No. 217-03528)   31-0a-21 (No. 217-03528)   31-0a-21 (No. 217-03528)   30-Oct-14 (in house)   30-Oct-15 (in house check Oct-20)   07-Odt-15 (in house check Oct-20)   07-Odt-15 (in house check Oct-20)   31-Mar-14 (in house check Oct-20)   31-Mar-14 (in house check Oct-20)	nd are part of the certificate. 'C and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Dec-22 Nov-22 Scheduled Check In house check: Oct-22 In house check: Oct-22

Certificate No: D2450V2-727\_Apr22

Page 1 of 6

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sqs.com.tw/Terms-and-Conditions. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document dear and the contract and company's mining all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.


SGS Taiwan Ltd. No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



## Report No. : TESA2205000105ES Rev:

Page: 3 of 7

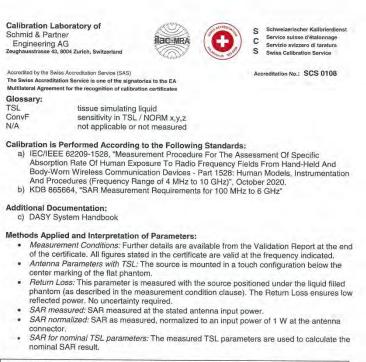

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D2450V2-727\_Apr22

Page 2 of 6

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

t (886-2) 2299-3279

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction form exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

f (886-2) 2298-0488



## Report No. : TESA2205000105ES Rev: Page: 4 of 7

Measurement Conditions

DASY Version	DASY52	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	37.8 ± 6 %	1.87 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.6 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	52.8 W/kg ± 17.0 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL. SAR measured	condition 250 mW input power	6.34 W/kg

Certificate No: D2450V2-727 Apr22

Page 3 of 6

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <u>http://www.sgs.com.tw/Terms-and-Conditions</u> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's not reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

SGS Taiwan Ltd. No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



## Report No. : TESA2205000105ES Rev: Page: 5 of 7

Appendix (Additional assessments outside the scope of SCS 0108)

## Antenna Parameters with Head TSL

Impedance, transformed to feed point	55.7 Ω + 3.0 jΩ	
Return Loss	- 24.4 dB	

## General Antenna Parameters and Design

Electrical Delay (one direction) 1.149 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. according to the Standard. No excessive force must b sive force must be applied to the dipole arms, because they might bend or the soldered connections near the

feedpoint may be damaged.

### Additional EUT Data

Manufactured by	SPEAG

Certificate No: D2450V2-727 Apr22

Page 4 of 6

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sqs.com.tw/Terms-and-Conditions. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號 SGS Taiwan Ltd.



## Report No. : TESA2205000105ES Rev: Page: 6 of 7

## **DASY5 Validation Report for Head TSL**

Test Laboratory: SPEAG, Zurich, Switzerland

Date: 25.04.2022


DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 727 Communication System: UID 0 - CW; Frequency: 2450 MHz Medium parameters used: f = 2450 MHz;  $\sigma$  = 1.87 S/m;  $\epsilon_r$  = 37.8;  $\rho$  = 1000 kg/m<sup>3</sup> Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN7349; ConvF(7.96, 7.96, 7.96) @ 2450 MHz; Calibrated: 31.12.2021
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 01.11.2021
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 115.6 V/m; Power Drift = 0.09 dB

Reference value = 11.5.0 v/m, rower D/m = 0.09 uB Peak SAR (extrapolated) = 26.5 W/kg SAR(1 g) = 13.6 W/kg; SAR(10 g) = 6.34 W/kg Smallest distance from peaks to all points 3 dB below = 9 mm Ratio of SAR at M2 to SAR at M1 = 51% Maximum value of SAR (measured) = 22.1 W/kg

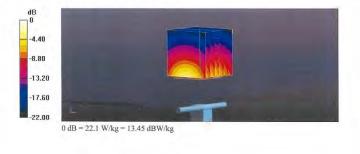

Certificate No: D2450V2-727 Apr22

Page 5 of 6

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.


除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction form exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號 SGS Taiwan Ltd.



Report No. : TESA2205000105ES Rev: Page: 7 of 7

Impedance Measurement Plot for Head TSI

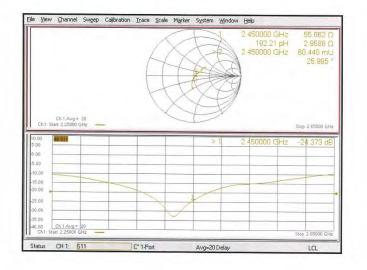

Certificate No: D2450V2-727\_Apr22 Page 6 of 6

# - End of report -

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's not reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號 SGS Taiwan Ltd.

f (886-2) 2298-0488