




# **Appendix D**







## **Photographs**

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details



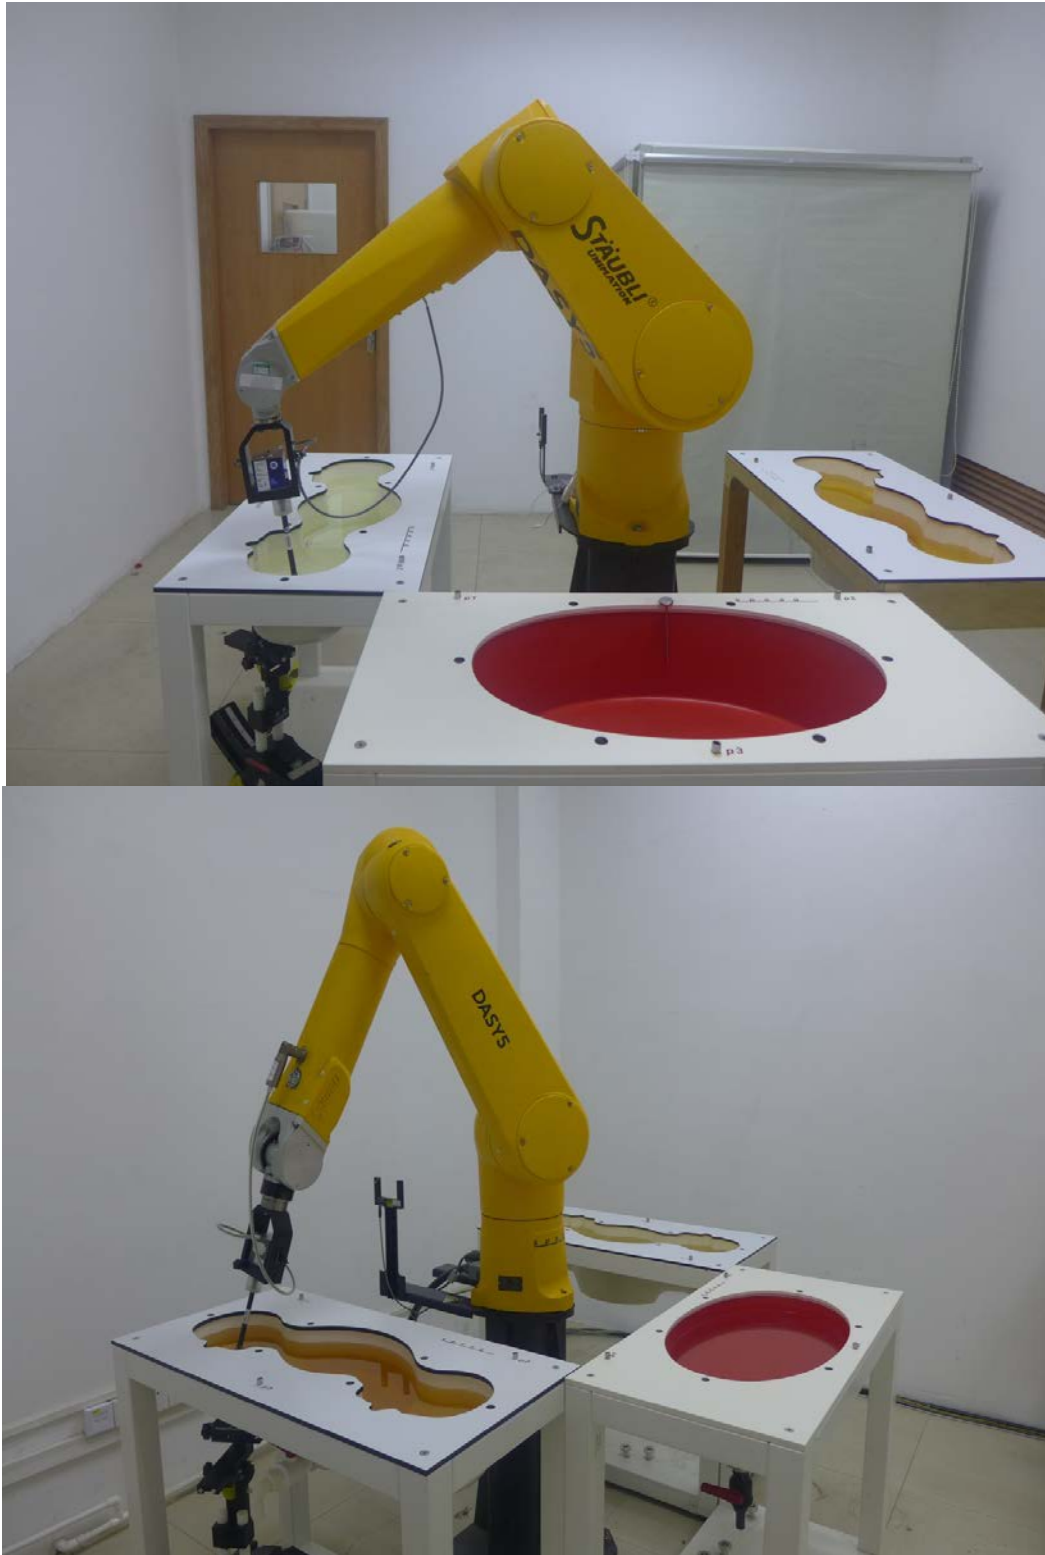



## 1. SAR measurement System

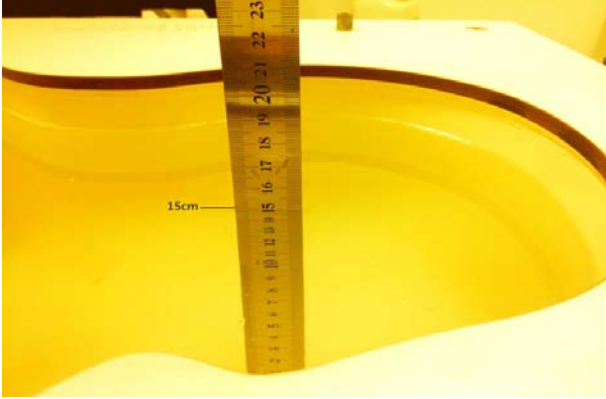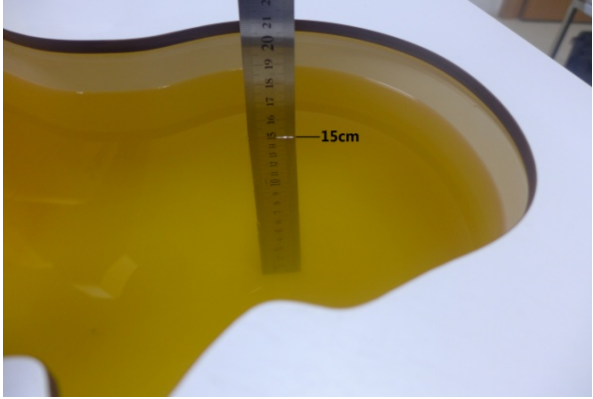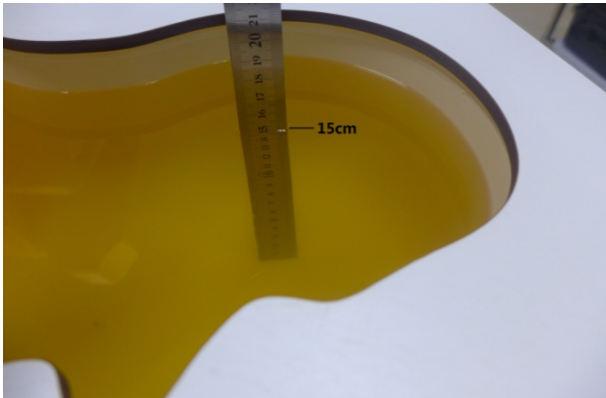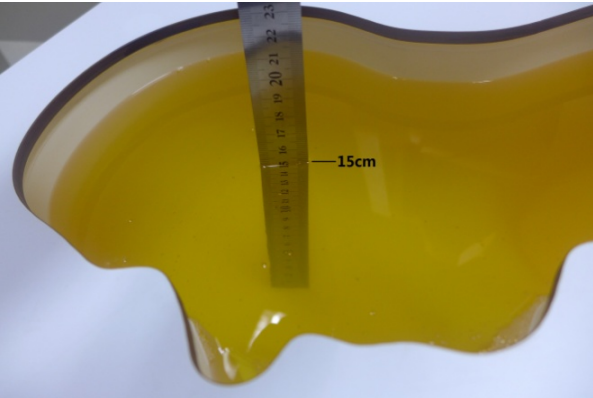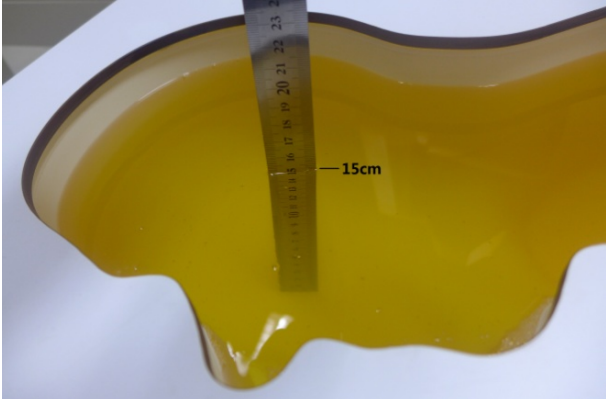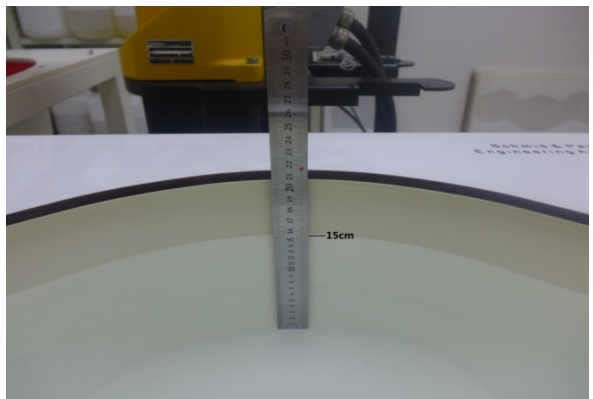





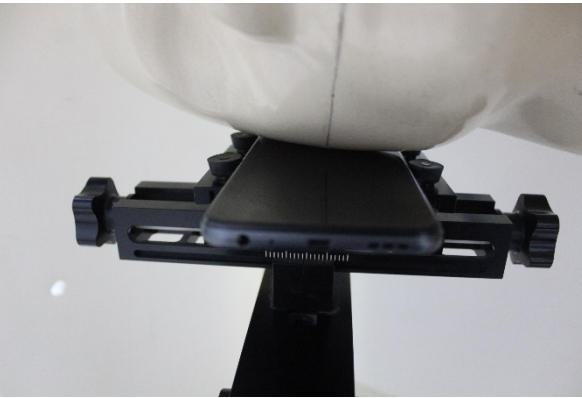


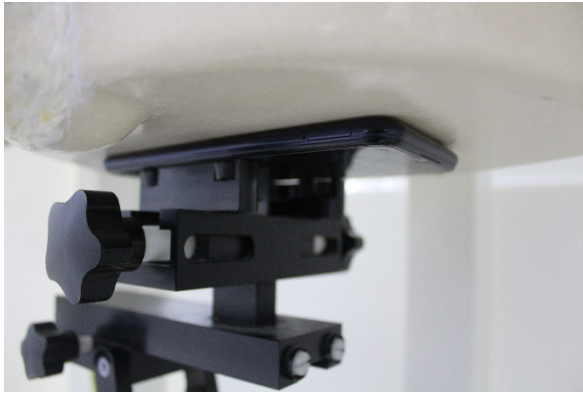




## 2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Head 835</p>	<p>Photo 2: Tissue Simulant Liquid for Head 1750</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 1900</p>	<p>Photo 4: Tissue Simulant Liquid for Head 2450</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 2600</p>	<p>Photo 6: Tissue Simulant Liquid for Head 5G</p>
	

### 3. Photographs of EUT test position

<p>Photo 7: Left cheek</p>	<p>Photo 8: Left tilted</p>
	
<p>Photo 9: Right cheek</p>	<p>Photo 10: Right tilted</p>
	
<p>Photo 11: Front side 10mm</p>	<p>Photo 12: Back side 10mm</p>
	

<p><b>Photo 13: Left side 10mm</b></p>	<p><b>Photo 14: Right side 10mm</b></p>
	
<p><b>Photo 15: Top side 10mm</b></p>	<p><b>Photo 16: Bottom side 10mm</b></p>
	
<p><b>Photo 17: Front side 15mm</b></p>	<p><b>Photo 18: Back side 15mm</b></p>
	

<p><b>Photo 19: Front side 0mm</b></p>	<p><b>Photo 20: Back side 0mm</b></p>
	
<p><b>Photo 21: Right side 0mm</b></p>	<p><b>Photo 22: Top side 0mm</b></p>
	
<p><b>Photo 23: Front side 4mm</b></p>	<p><b>Photo 24: Back side 8mm</b></p>
	

#### 4. EUT Constructional Details

Photo 25: Front View	Photo 26: Back View
