

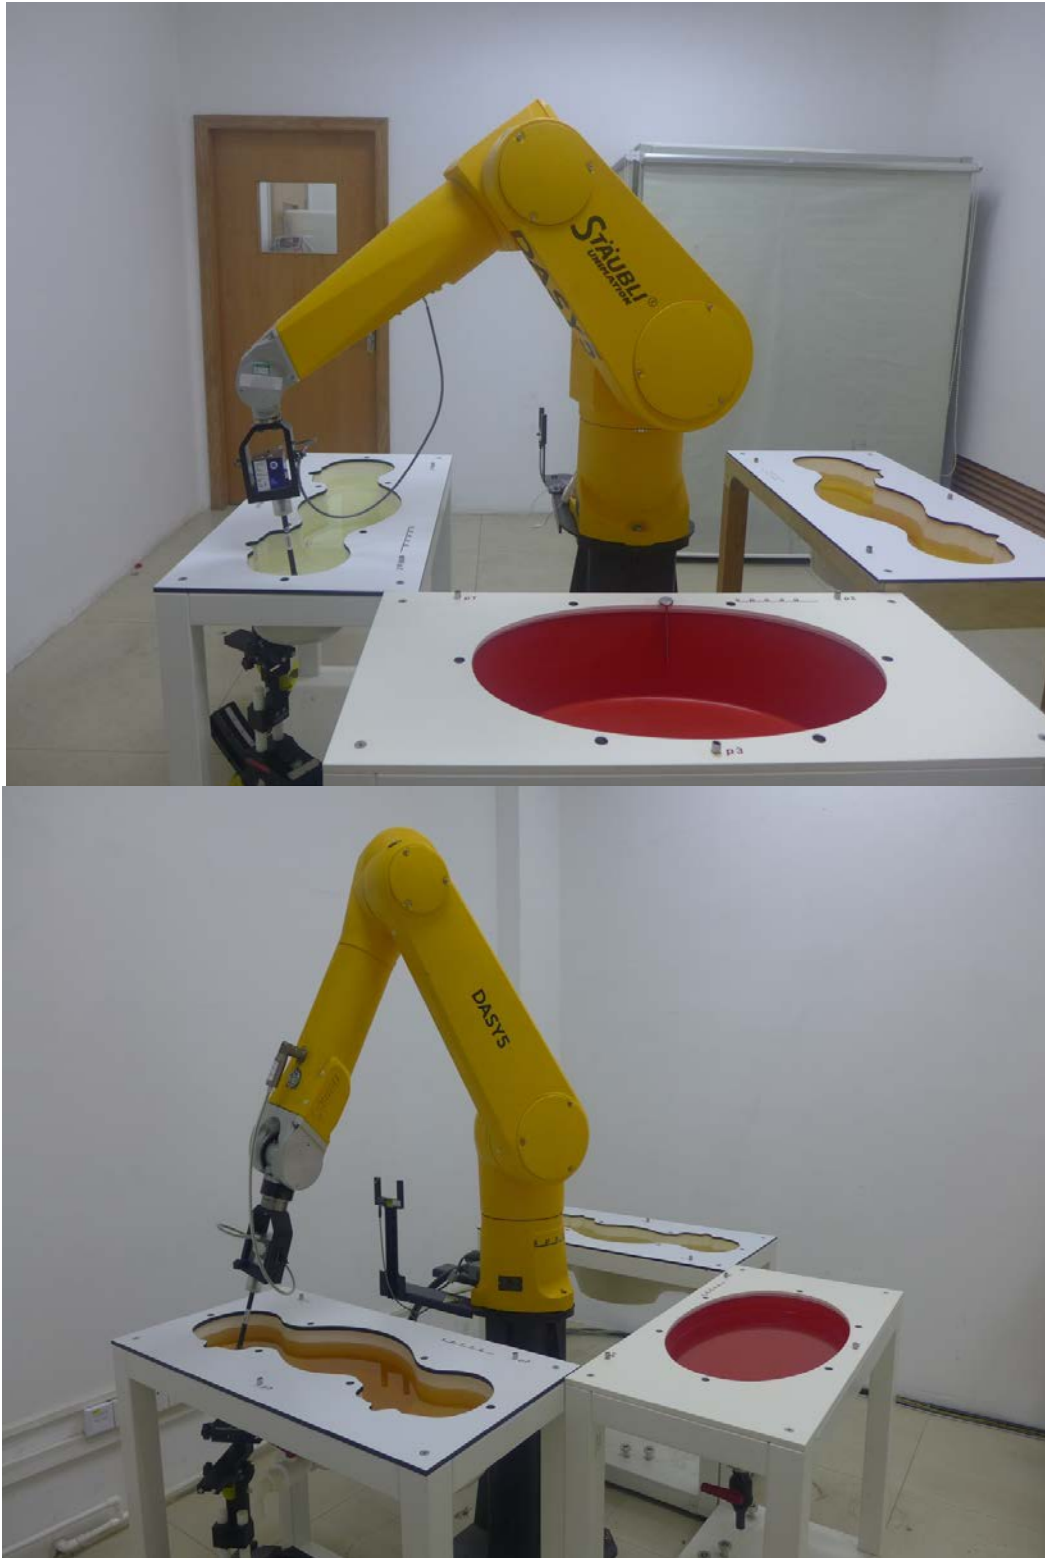


Appendix D

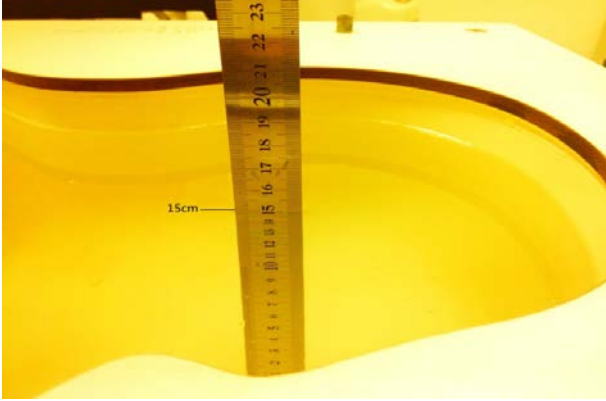
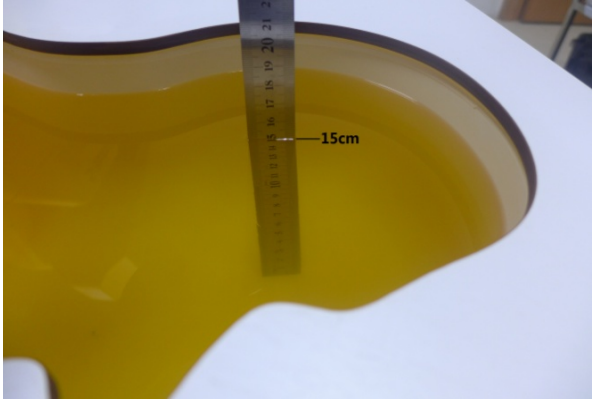
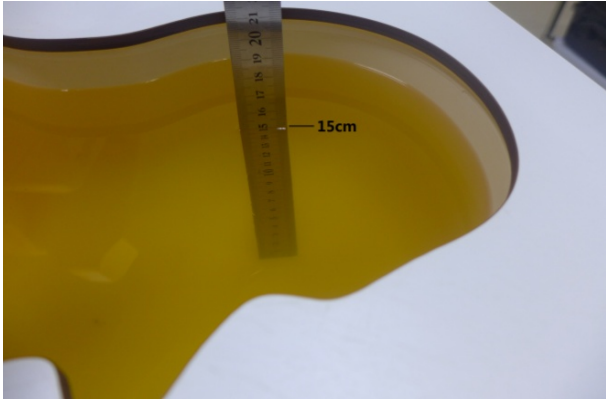
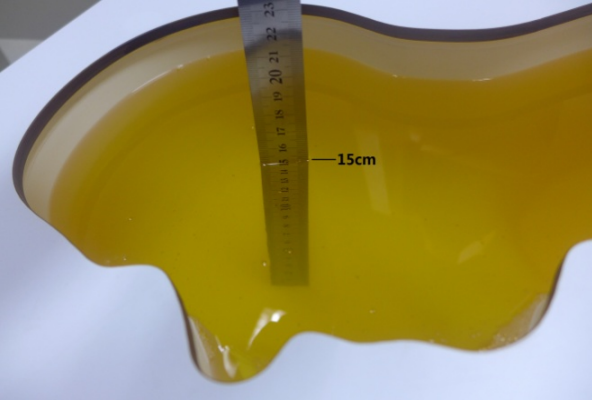
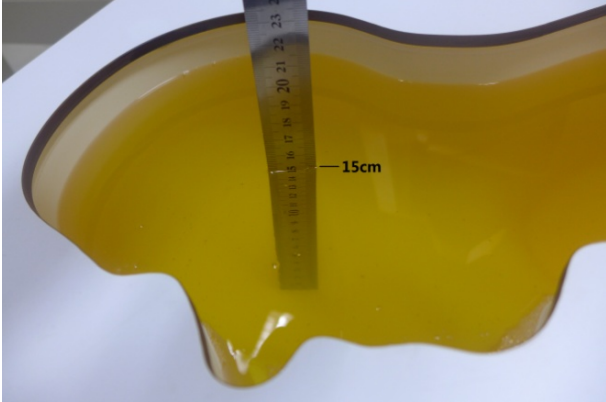
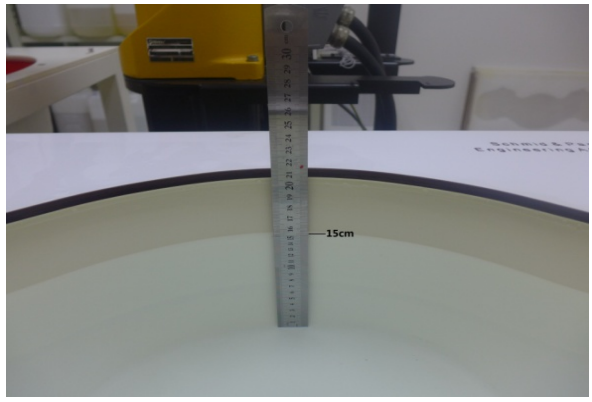
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Head 835</p>	<p>Photo 2: Tissue Simulant Liquid for Head 1750</p>
	
<p>Photo 3: issue Simulant Liquid for Head 1900</p>	<p>Photo 4: Tissue Simulant Liquid for Head 2450</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 2600</p>	<p>Photo 6: Tissue Simulant Liquid for Head 5G</p>
	

3. Photographs of EUT test position


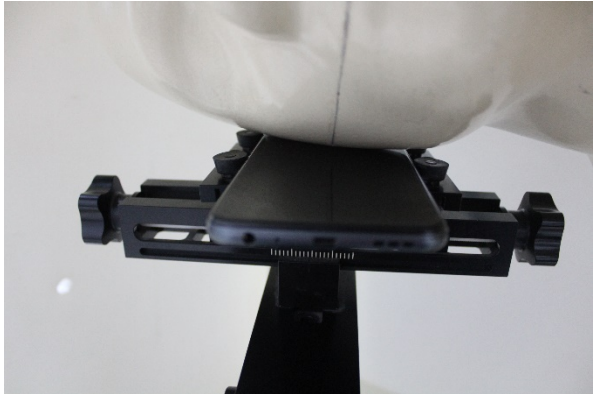
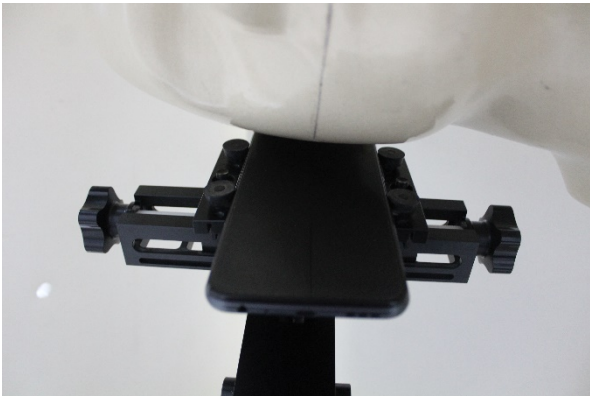





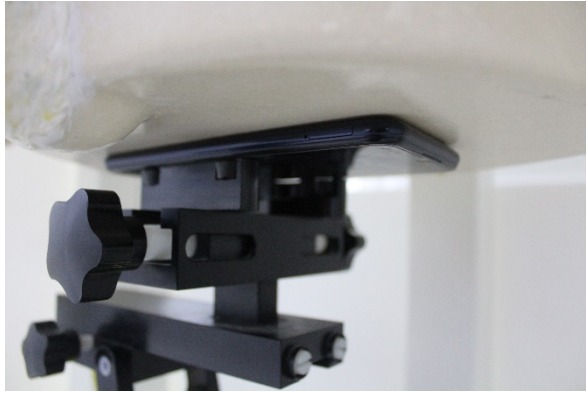

<p>Photo 7: Left cheek</p>	<p>Photo 8: Right cheek</p>
	
<p>Photo 9: Right tilted</p>	<p>Photo 10: Back side 10mm</p>
	
<p>Photo 11: Right side 10mm</p>	<p>Photo 12: Top side 10mm</p>
	

Photo 13: Bottom side 10mm	Photo 14: Back side 15mm
	
Photo 15: Back side 0mm	Photo 16: Top side 0mm
	

4. EUT Constructional Details

Photo 17: Front View	Photo 18: Back View
