


Weight-Sensing Floor Mats

Step on the floor mat. The alert tone will sound. Press the **Reset** button to reset the monitor.

Repeat steps 1–4 if system is not working properly.

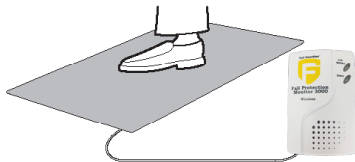


Floor Mat Placement

- Place the floor mat in the desired location such as a critical doorway or next to a bed.
- Place the monitor out of reach of resident. Suitable mounting locations include the back of the headboard, wall or under the bed so the resident cannot tamper with the monitor.

Test the System

- Step on Floor Mat to set off the alert. The monitor is now active. The alert will sound whenever weight is on the floor mat.
- When the alert is activated, press the “Reset” button on the side of the monitor to silence the alarm.

NOTE: The Status Light does not blink when using floor mats.

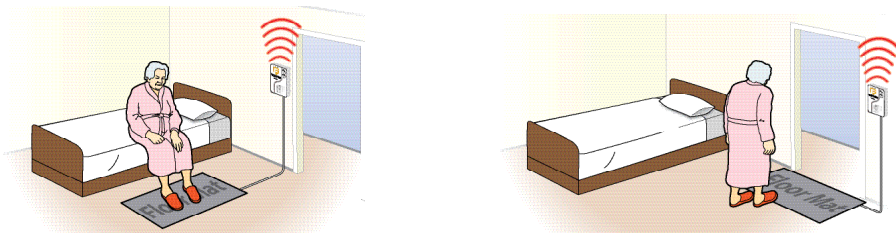

Wireless Fall Protection Monitor

The SCG devices are designed to be installed by the end user. As such, it is the entire responsibility of the buyer to insure that the system is properly installed and tested. Further, the system is not designed to replace good caregiving practices including, but not limited to:

- A.) Direct patient supervision
- B.) Adequate training for staff personnel for fall prevention and elopement
- C.) Testing of the system before each use

Read the instructions and Legal Disclaimer.

Limited Warranty: Seller warrants that the goods sold will be free from defects of workmanship and manufacturing, for a warranty period from the date of sale. Other than this limited warranty, seller makes no express or implied warranties. Except for this limited warranty. No express or implied warranties are given and no affirmation of seller, by words or action will constitute a warranty. The goods being purchased are being sold on a “with all faults” basis. The entire risk as to the quality and performance of the goods is with the buyer. Should the goods prove defective following their purchase, the buyer, and not the manufacturer, distributor or retailer, assumes the entire cost of all necessary installation, servicing or repairs.

WARNING: The manufacturer does not claim that this device will stop elopement and/or stop falls. This device is designed to augment caregivers’ comprehensive resident mobility management program. Failure to comply with the warning may result in injury or death. This device is not suitable for all individuals. Other devices may be required. This device is not a substitute for visual monitoring by a caregiver.

Where permissible, it is the seller’s intent to limit any liability for special, consequential or incidental economic damages to refund of the purchase price or replacement of the goods. Seller disclaims any liability for compensatory or other damages arising out of the use of the goods.

IMPORTANT INFORMATION: Cordless and Wireless Systems rely on wireless technology which is subject to physical and environmental considerations. Please be aware that the transmitter will not be 100% accurate if it is out of range at any time. It is the end-user’s responsibility to make sure that the product is used correctly and within range of each other. Cordless and wireless systems and devices are intended as an adjunct to good caregiving practices and are not a substitute for proper staffing and patient management practices. We recommend that all caregivers receive periodic training in the operation of these systems and that the devices are tested daily. It is important to read and follow the directions.



Installation and Use Instructions



Fall Guardian Fall Protection Monitor 3000

- Reduces in room alert noise
- Monitor can be set to silent
- Works with corded weight-sensing pads and floor mats

1 Install 9 Volt Battery


- Using a small Phillips screwdriver, unscrew battery cover.
- Insert 1 new 9 Volt battery as shown.
- Optional:
 - Monitor can be used with AC Adapter (AC-02)
 - AC Adapter port is located on side of monitor.



2 Adjust Tone, Volume, and Delay Options to the Desired Level

- Set tone switch to Tone 1 (1 beep), Tone 2 (2 beeps), or Tone 3 (3 beeps).
- Set the alarm volume high or low.
- A one second delay can usually allow the resident to reposition in bed without triggering the alarm.

*To silence the monitor, move volume dial to “Silent”. Warning: In silent position, you **MUST** use a pager.

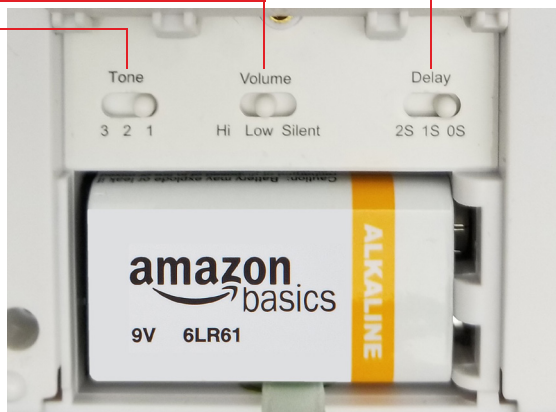

3 Connect Sensor Device

- Plug sensor device cord into monitor.
- Lace cord through the T-shaped strain relief to guard against accidentally unplugging the device and cord damage.
- Make sure the cord is placed so it is well out of resident's reach and is not a tripping hazard.




4 Test the System

Bed and Chair Weight-Sensing Pads



Apply pressure.

After two beeps, release pressure. Press the Reset button to reset the monitor.

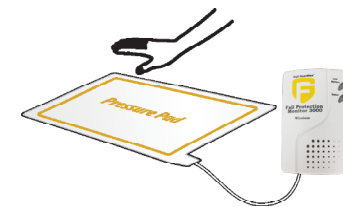


Bed Placement

- Place the pad under shoulders to be alerted when the patient sits up in bed.
- Place pad under lower back/buttocks to be alerted when the resident vacates the bed.
- Place the monitor out of reach of patient. Suitable mounting locations include: back of headboard, wall or under bed. Make sure the resident cannot tamper with monitor. (It is the caregiver's responsibility to route the cord under the sheet so the resident cannot tamper with it).

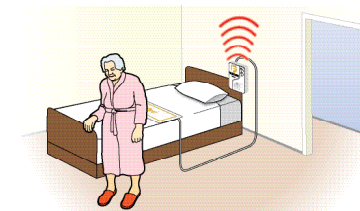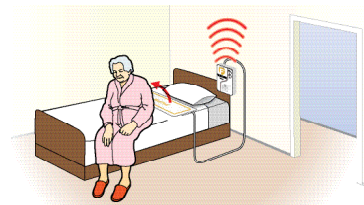

Wheelchair/Chair Placement

- Center pad on the chair seat under buttocks.
- Place the monitor out of reach of the resident. Suitable mounting location is the back of wheelchair, so that the resident cannot tamper with monitor.

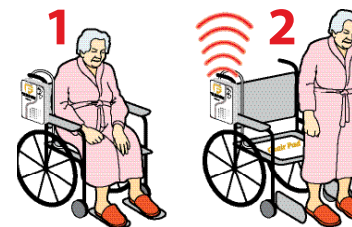

Important: Test the System

- Plug the pad into the monitor and apply weight to the pad to activate the system. The monitor will beep twice when activated.
- The alert tone will sound when weight is removed from pad. Press the “Reset” button on side of monitor to silence the alert. The status light on the front of monitor will blink when pad is plugged into the monitor and pressure is on pad.

This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Note: This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

Note: The Grantee is not responsible for any changes or modifications not expressly approved by the party responsible for compliance. such modifications could void the user's authority to operate the equipment.