



Exhibit: Test Setup Photos

Report File #: 7169006883R-000

Client	Flosonic Medical	
Product	FloPatch FP120	
Standard(s)	RSS 247 Issue 2:2017 FCC Part 15 Subpart 15.247:2018	

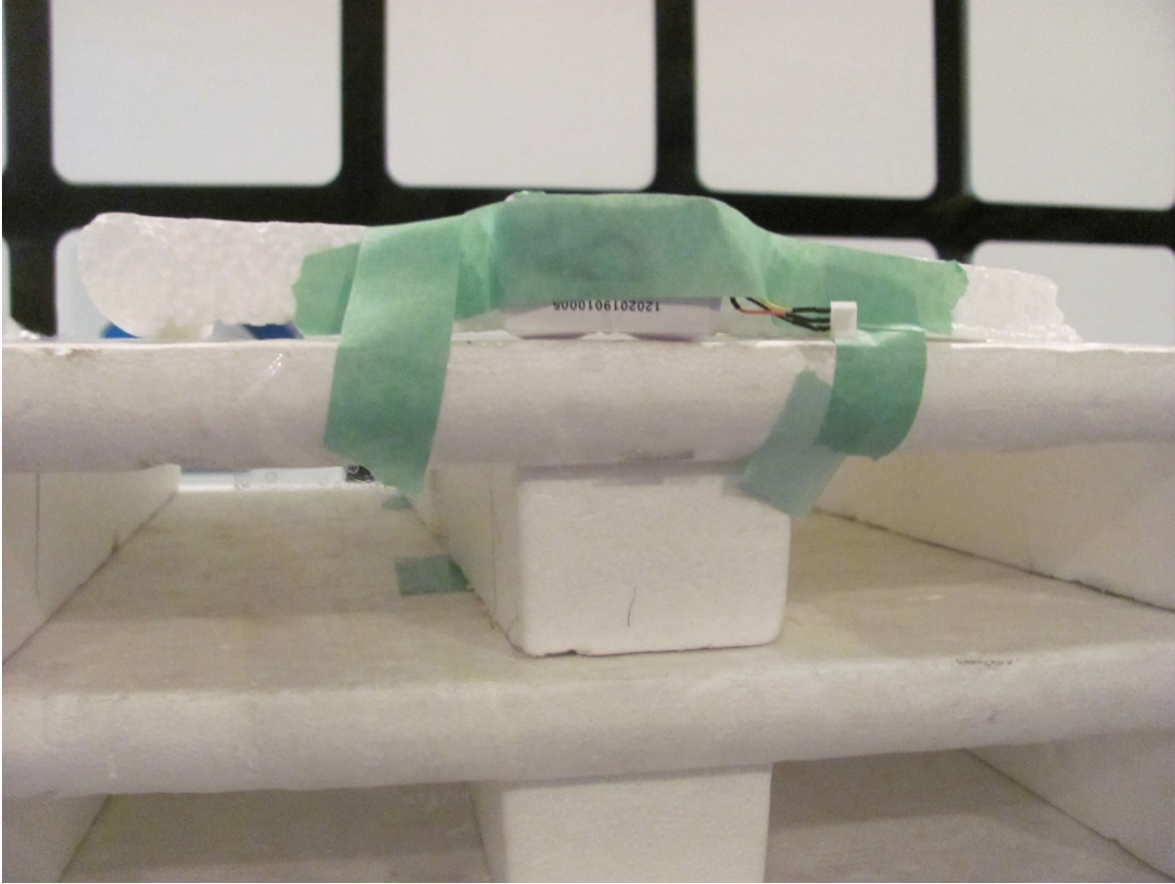


Figure 1 – EUT Close Up

Client	Flosonic Medical	
Product	FloPatch FP120	
Standard(s)	RSS 247 Issue 2:2017 FCC Part 15 Subpart 15.247:2018	



Figure 2 – Radiated Emissions Setup – Photo 1

Client	Flosonic Medical	
Product	FloPatch FP120	
Standard(s)	RSS 247 Issue 2:2017 FCC Part 15 Subpart 15.247:2018	



Figure 3 – Radiated Emissions Setup – Photo 2

Note: As per ANSI C63.10-2013 Clause 6.3.1, below 1GHz, the height of the EUT was set to 80cm. Above 1GHz, the height was raised to 1.5m.

Client	Flosonic Medical	
Product	FloPatch FP120	
Standard(s)	RSS 247 Issue 2:2017 FCC Part 15 Subpart 15.247:2018	

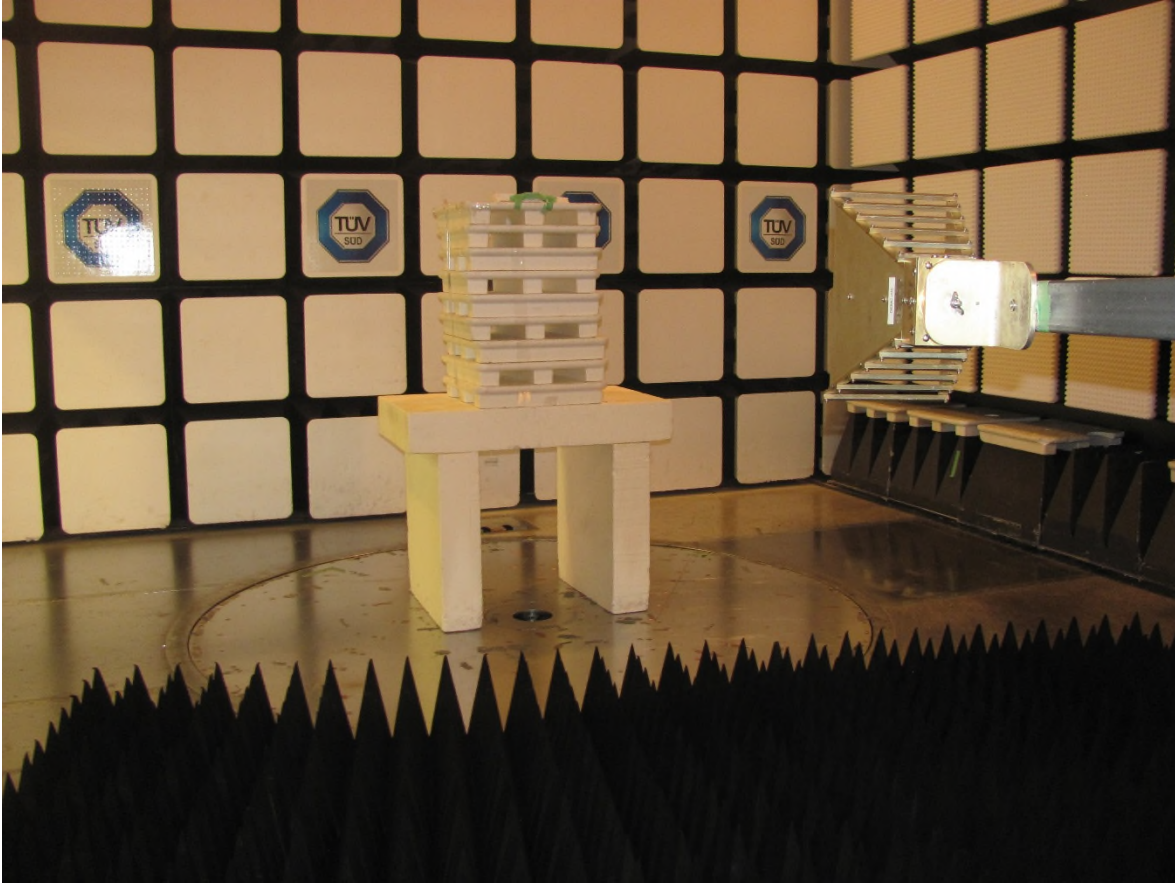


Figure 4 – Radiated Emissions Setup – Photo 3

Note: As per ANSI C63.10-2013 Clause 6.3.1, above 1GHz, the height of the EUT was set to 1.5m.

Client	Flosonic Medical	
Product	FloPatch FP120	
Standard(s)	RSS 247 Issue 2:2017 FCC Part 15 Subpart 15.247:2018	

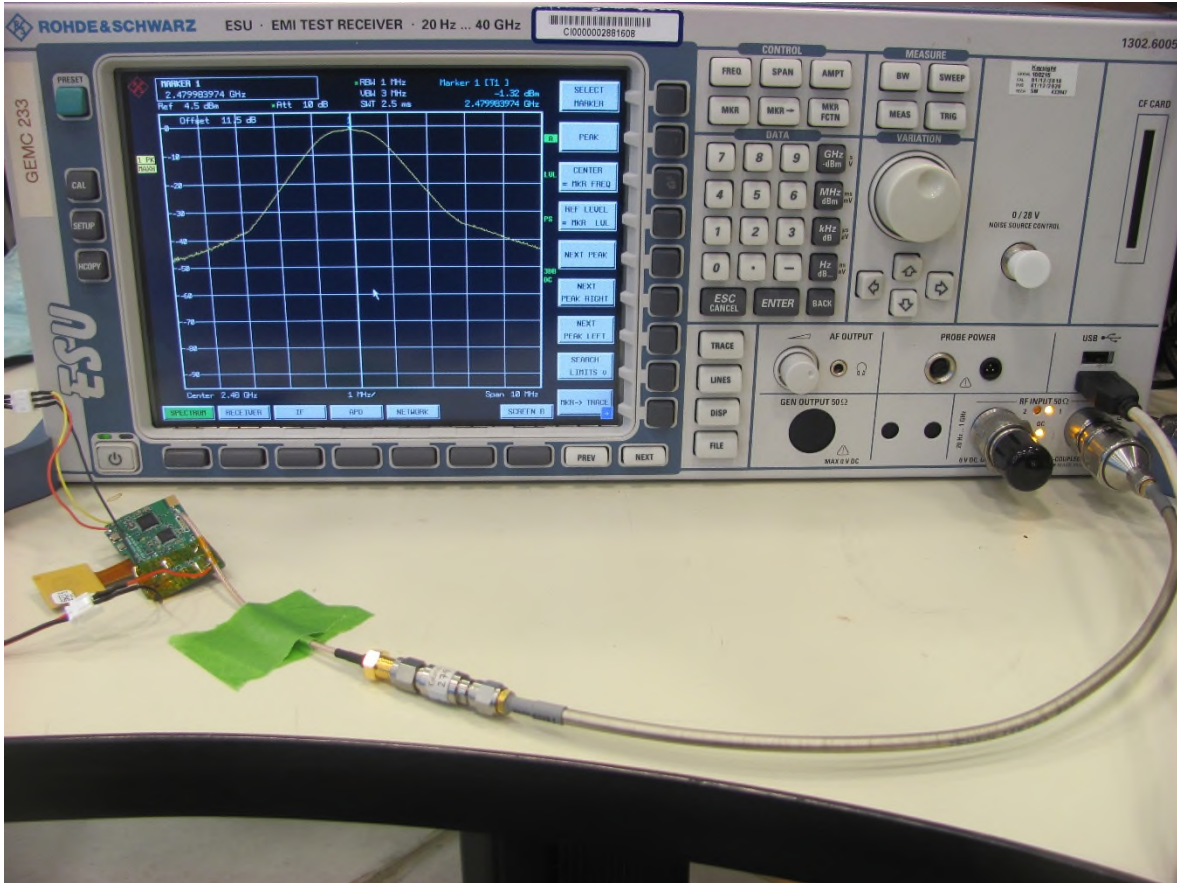


Figure 5 – Antenna Port Conducted Emissions Setup